

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092525\
 Data File : VN087950.D
 Acq On : 25 Sep 2025 12:59
 Operator : JC\MD
 Sample : VN0925WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0925WBL01

Quant Time: Sep 26 07:29:41 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N092325W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 24 05:05:30 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.206	168	168763	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.082	114	367239	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.847	117	361992	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.770	152	171513	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.559	65	165738	58.355	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	116.720%
35) Dibromofluoromethane	8.153	113	142300	53.369	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	106.740%
50) Toluene-d8	10.547	98	470183	50.145	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	100.280%
62) 4-Bromofluorobenzene	12.829	95	153124	45.687	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	91.380%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092525\
Data File : VN087950.D
Acq On : 25 Sep 2025 12:59
Operator : JC\MD
Sample : VN0925WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0925WBL01

Quant Time: Sep 26 07:29:41 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N092325W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 24 05:05:30 2025
Response via : Initial Calibration




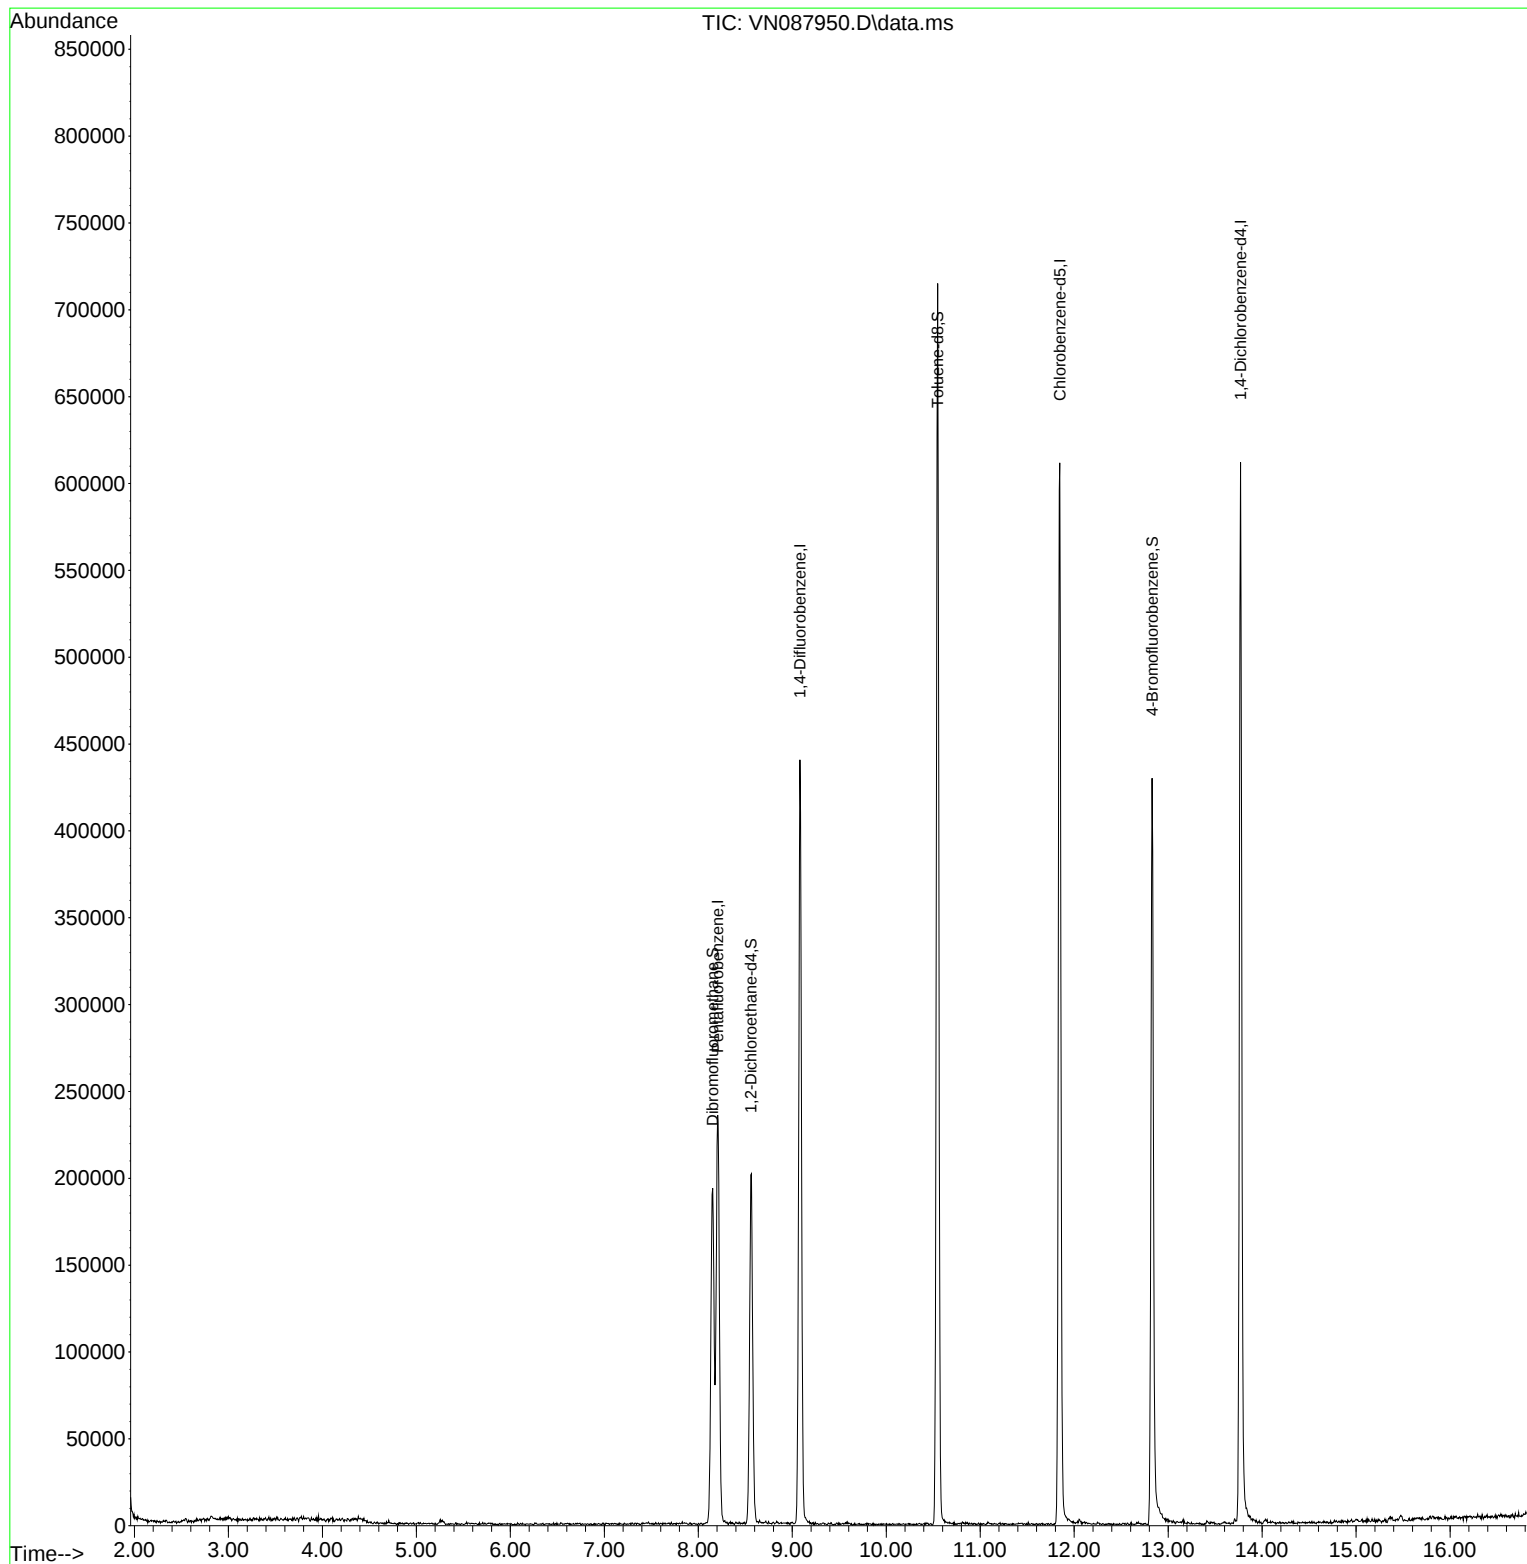


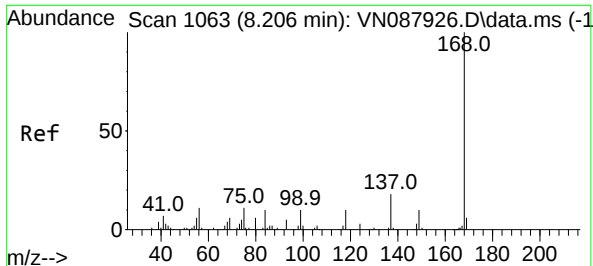

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.206 min Scan# 1063
Delta R.T. -0.000 min
Lab File: VN087950.D
Acq: 25 Sep 2025 12:59




Instrument :
MSVOA_N
ClientSampleId :
VN0925WBL01


Tgt Ion:168 Resp: 168763
Ion Ratio Lower Upper
168 100
99 59.7 52.2 78.2

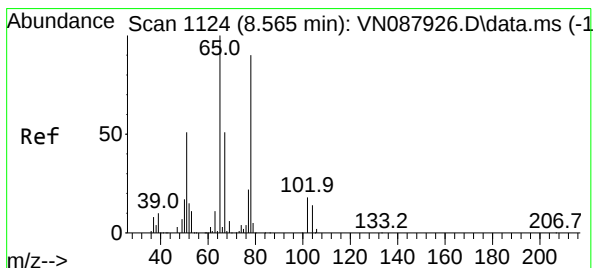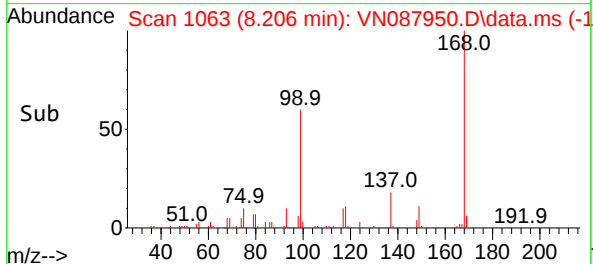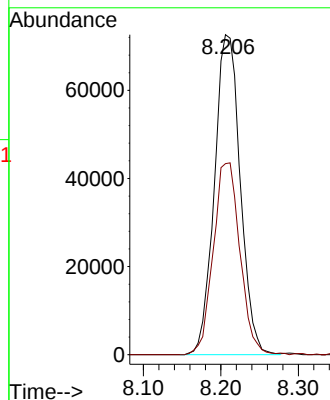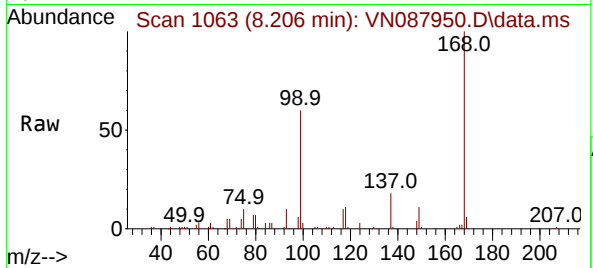

#33
1,2-Dichloroethane-d4
Concen: 58.355 ug/l
RT: 8.559 min Scan# 1123
Delta R.T. -0.006 min
Lab File: VN087950.D
Acq: 25 Sep 2025 12:59

Tgt Ion: 65 Resp: 165738
Ion Ratio Lower Upper
65 100
67 50.9 0.0 103.4

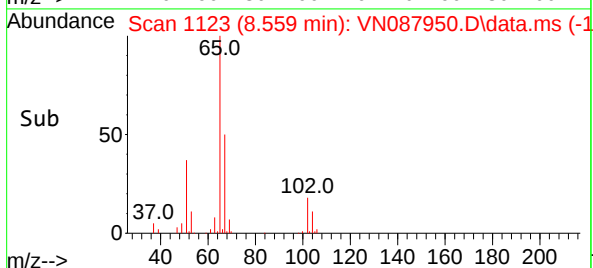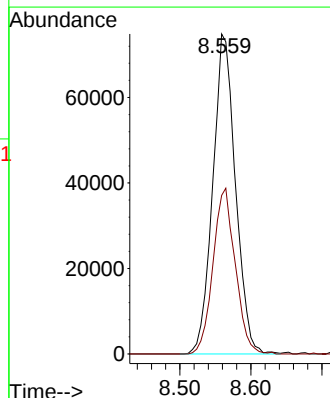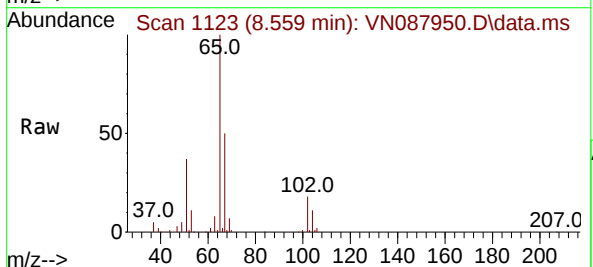

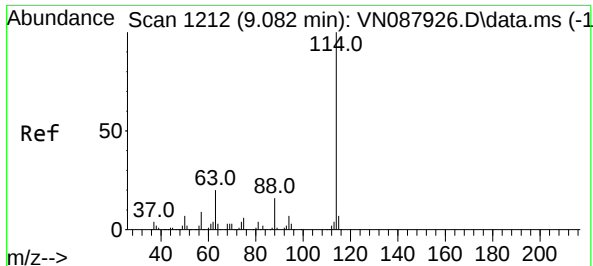

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.082 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN087950.D

Acq: 25 Sep 2025 12:59

Instrument :

MSVOA_N

ClientSampleId :

VN0925WBL01





Tgt Ion:114 Resp: 367239

Ion Ratio Lower Upper

114 100

63 18.6 0.0 40.0

88 13.7 0.0 31.8

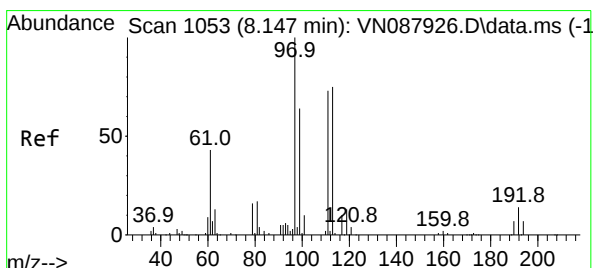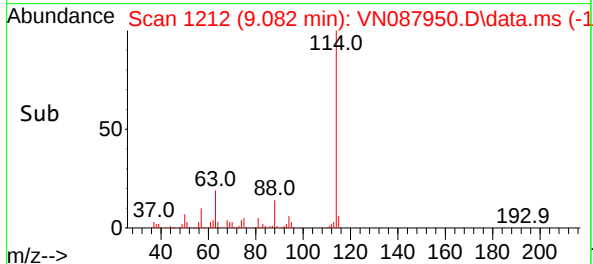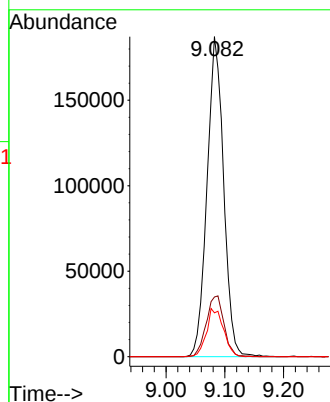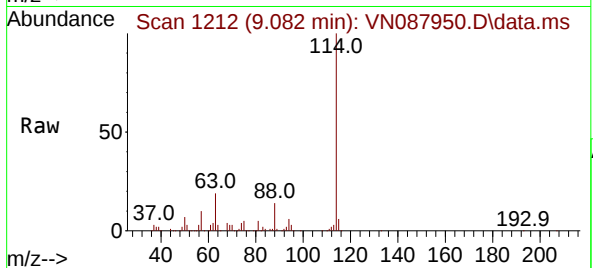

#35

Dibromofluoromethane

Concen: 53.369 ug/l

RT: 8.153 min Scan# 1054

Delta R.T. 0.006 min

Lab File: VN087950.D

Acq: 25 Sep 2025 12:59




Tgt Ion:113 Resp: 142300


Ion Ratio Lower Upper

113 100

111 102.6 82.2 123.2

192 17.2 14.2 21.2


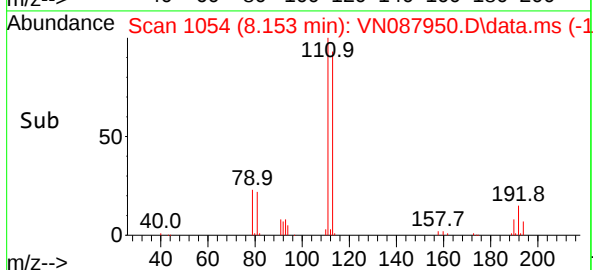
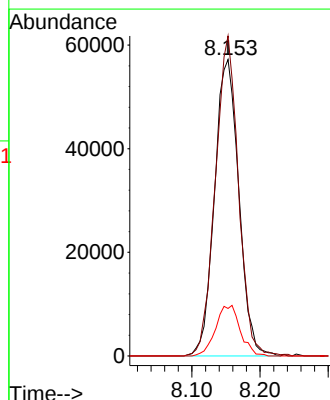
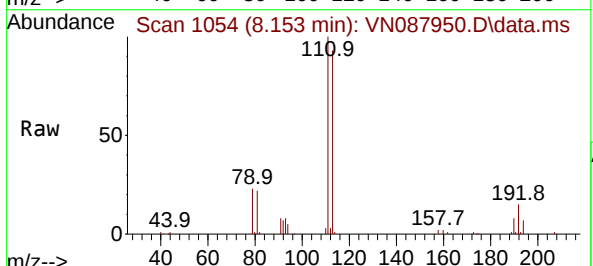


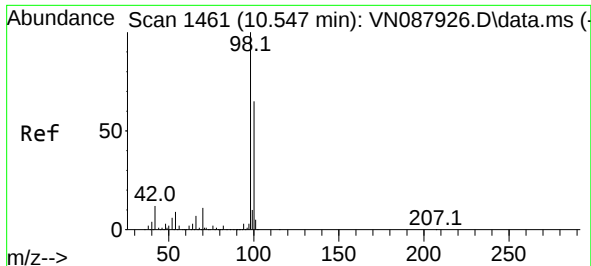

#50
Toluene-d8
Concen: 50.145 ug/l
RT: 10.547 min Scan# 1461
Delta R.T. -0.000 min
Lab File: VN087950.D
Acq: 25 Sep 2025 12:59




Instrument :
MSVOA_N
ClientSampleId :
VN0925WBL01


Tgt Ion: 98 Resp: 470183
Ion Ratio Lower Upper
98 100
100 63.8 51.7 77.5

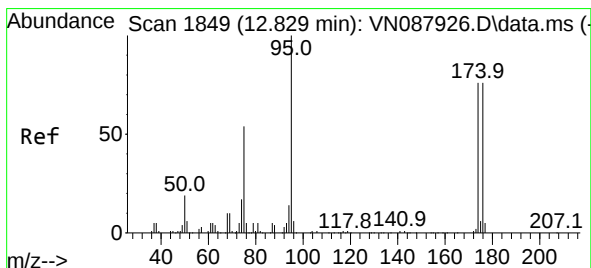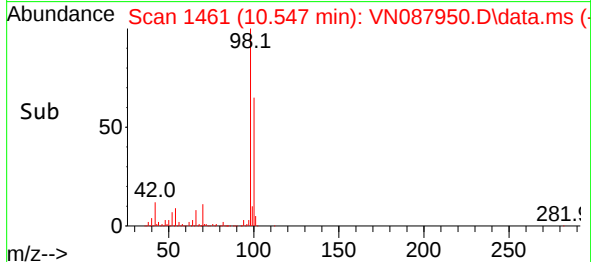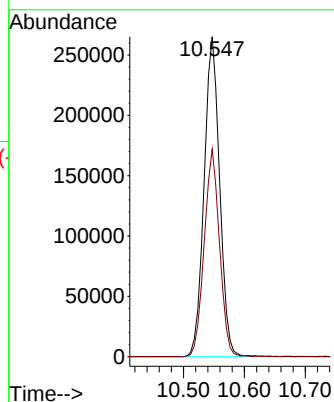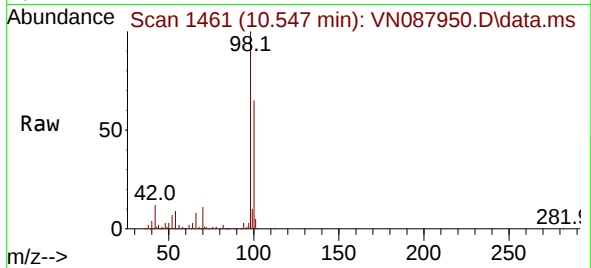

#62
4-Bromofluorobenzene
Concen: 45.687 ug/l
RT: 12.829 min Scan# 1849
Delta R.T. -0.000 min
Lab File: VN087950.D
Acq: 25 Sep 2025 12:59

Tgt Ion: 95 Resp: 153124
Ion Ratio Lower Upper
95 100
174 80.3 0.0 159.2
176 74.3 0.0 152.6


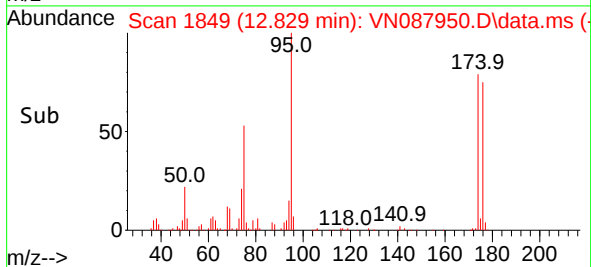
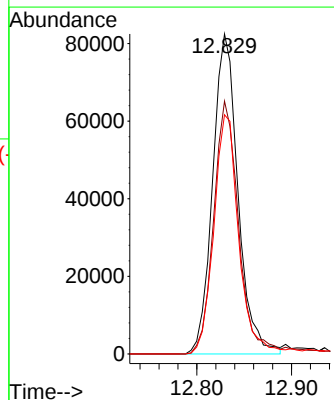
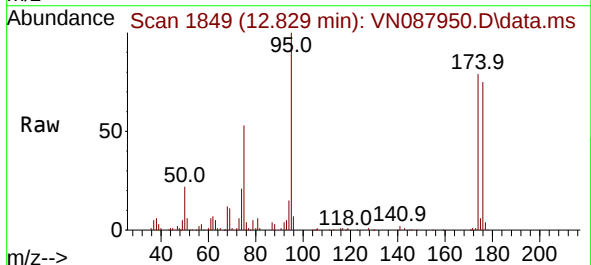


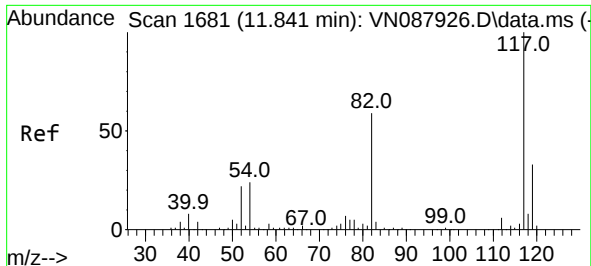

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.847 min Scan# 1184
Delta R.T. 0.006 min
Lab File: VN087950.D
Acq: 25 Sep 2025 12:59

Instrument :
MSVOA_N
ClientSampleId :
VN0925WBL01

Tgt Ion:117 Resp: 361992
Ion Ratio Lower Upper
117 100
82 56.4 47.0 70.4
119 30.9 26.1 39.1

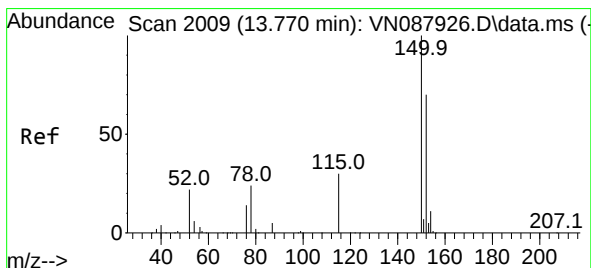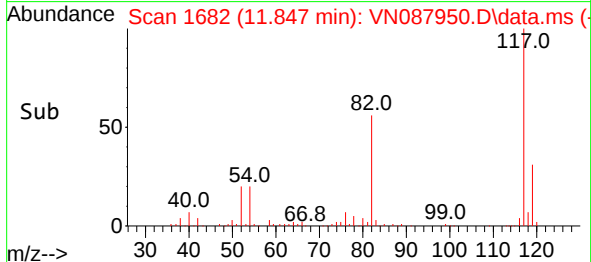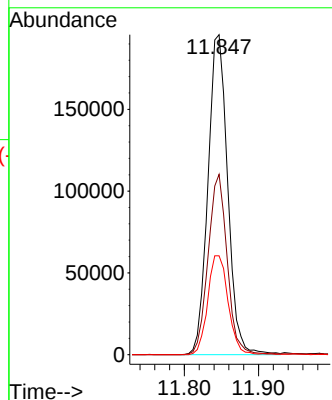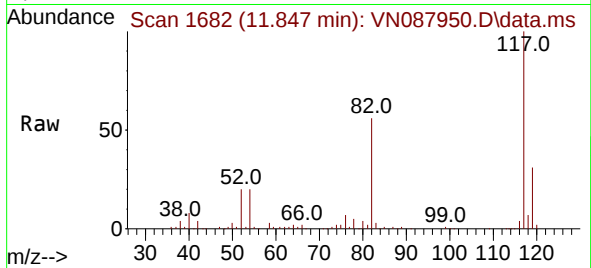

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.770 min Scan# 2009
Delta R.T. -0.000 min
Lab File: VN087950.D
Acq: 25 Sep 2025 12:59

Tgt Ion:152 Resp: 171513
Ion Ratio Lower Upper
152 100
115 60.5 29.9 89.7
150 154.5 0.0 335.0

