


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092618\
Data File : VN051514.D
Acq On : 26 Sep 2018 4:35
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092318W.M
Title : SW846 8260
Last Update : Mon Sep 24 06:41:32 2018

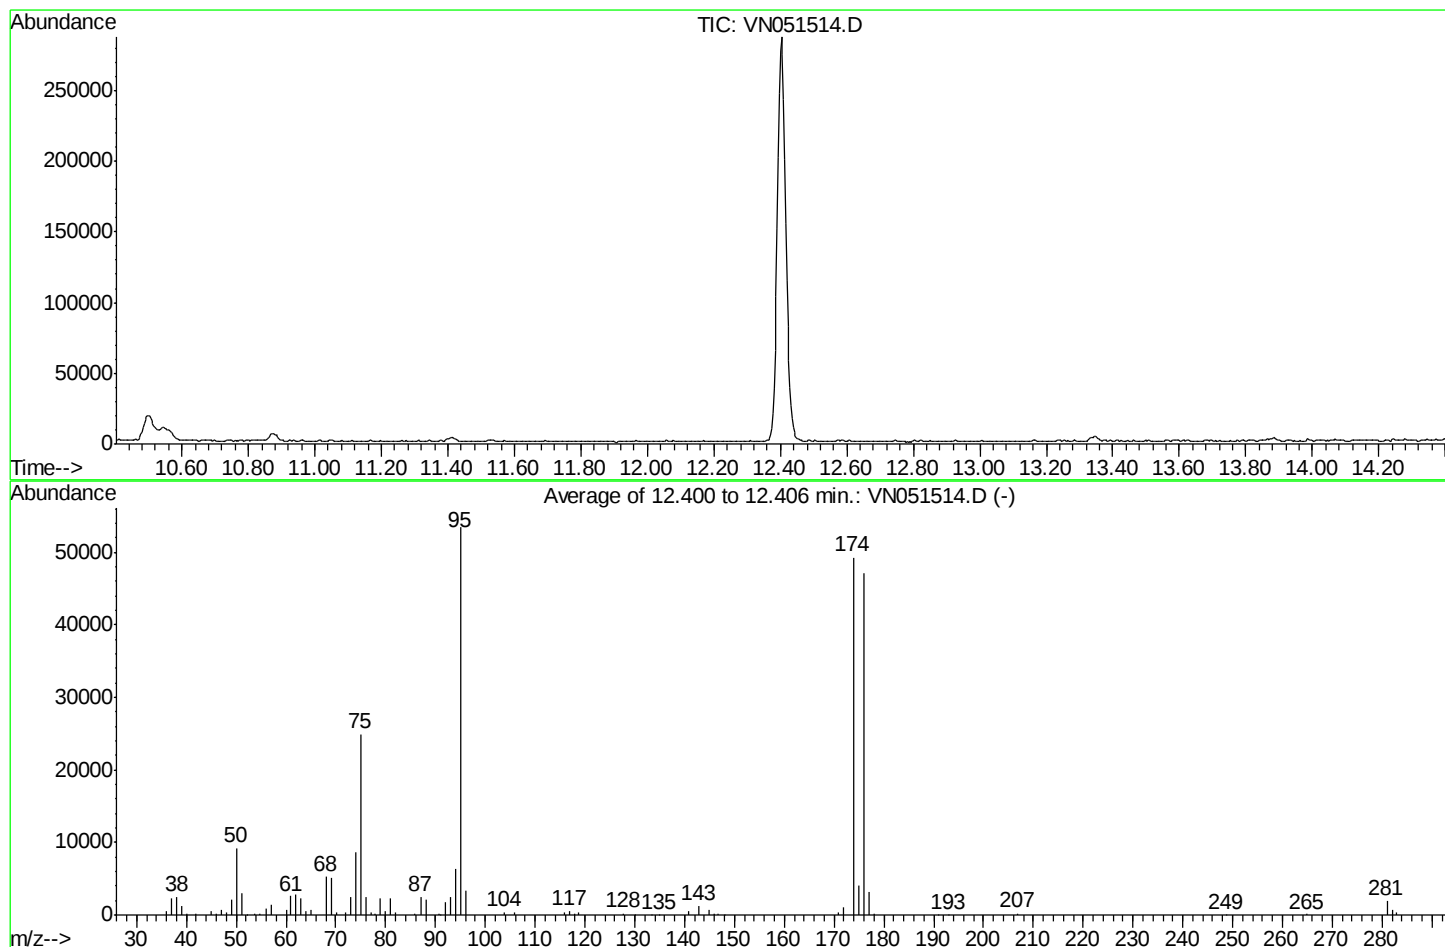

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	9219	PASS
75	95	30	60	46.7	24968	PASS
95	95	100	100	100.0	53461	PASS
96	95	5	9	6.4	3437	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	92.2	49304	PASS
175	174	5	9	8.3	4077	PASS
176	174	95	101	95.5	47106	PASS
177	176	5	9	6.9	3233	PASS