

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092623\
 Data File : VN079346.D
 Acq On : 26 Sep 2023 10:31
 Operator : JC\MD
 Sample : VN0926WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Sep 27 06:23:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091123W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 12 05:05:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	154173	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	283276	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	246237	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	71953	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	130060	62.493	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 124.980%	
35) Dibromofluoromethane	8.171	113	103813	55.094	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 110.180%	
50) Toluene-d8	10.571	98	341663	49.381	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 98.760%	
62) 4-Bromofluorobenzene	12.853	95	105162	47.650	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 95.300%	
Target Compounds						
					Qvalue	
3) Chloromethane	2.371	50	409	0.204	ug/l #	42
5) Bromomethane	2.959	94	740	0.590	ug/l	99
6) Chloroethane	3.095	64	161	Below Cal	#	43
13) Acrolein	4.189	56	274	0.748	ug/l #	49
15) Acrylonitrile	5.736	53	373	0.374	ug/l #	62
17) Carbon Disulfide	4.718	76	2189	0.426	ug/l #	75
25) 2-Butanone	7.500	43	388	0.303	ug/l #	37
31) Cyclohexane	8.230	56	4155	1.367	ug/l #	47
36) 1,1-Dichloropropene	8.230	75	14459	4.978	ug/l #	46
38) Carbon Tetrachloride	8.224	117	16949	5.639	ug/l #	16
43) Isopropyl Acetate	8.741	43	1398	0.296	ug/l #	49
51) 4-Methyl-2-Pentanone	10.453	43	1504	0.548	ug/l #	82
59) 2-Hexanone	11.200	43	2365	1.190	ug/l	75
68) m/p-Xylenes	12.076	106	793	0.223	ug/l	80
71) Bromoform	12.853	173	956	0.619	ug/l #	1
74) N-amyl acetate	12.506	43	1106	0.445	ug/l #	60
75) 1,1,2,2-Tetrachloroethane	12.953	83	514	0.211	ug/l #	95
76) 1,2,3-Trichloropropane	12.853	75	59963	30.921	ug/l #	1
77) Bromobenzene	12.976	156	423	0.255	ug/l	61
81) trans-1,4-Dichloro-2-b...	12.853	75	59963	85.009	ug/l #	15
82) 4-Chlorotoluene	13.223	91	1482	0.328	ug/l	93
86) p-Isopropyltoluene	13.735	119	1212	0.244	ug/l #	68
87) 1,3-Dichlorobenzene	13.741	146	1193	0.439	ug/l	97
88) 1,4-Dichlorobenzene	13.741	146	1193	0.434	ug/l	99
89) n-Butylbenzene	14.059	91	1930	0.494	ug/l	85
91) 1,2-Dichlorobenzene	14.106	146	1492	0.556	ug/l	90
92) 1,2-Dibromo-3-Chloropr...	14.723	75	134	0.362	ug/l	86
93) 1,2,4-Trichlorobenzene	15.388	180	1292	1.340	ug/l	91
94) Hexachlorobutadiene	15.500	225	756	0.996	ug/l	72
95) Naphthalene	15.641	128	5223	1.823	ug/l	100
96) 1,2,3-Trichlorobenzene	15.841	180	1938	1.703	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092623\
Data File : VN079346.D
Acq On : 26 Sep 2023 10:31
Operator : JC\MD
Sample : VN0926WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :


Quant Time: Sep 27 06:23:10 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091123W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 12 05:05:24 2023
Response via : Initial Calibration

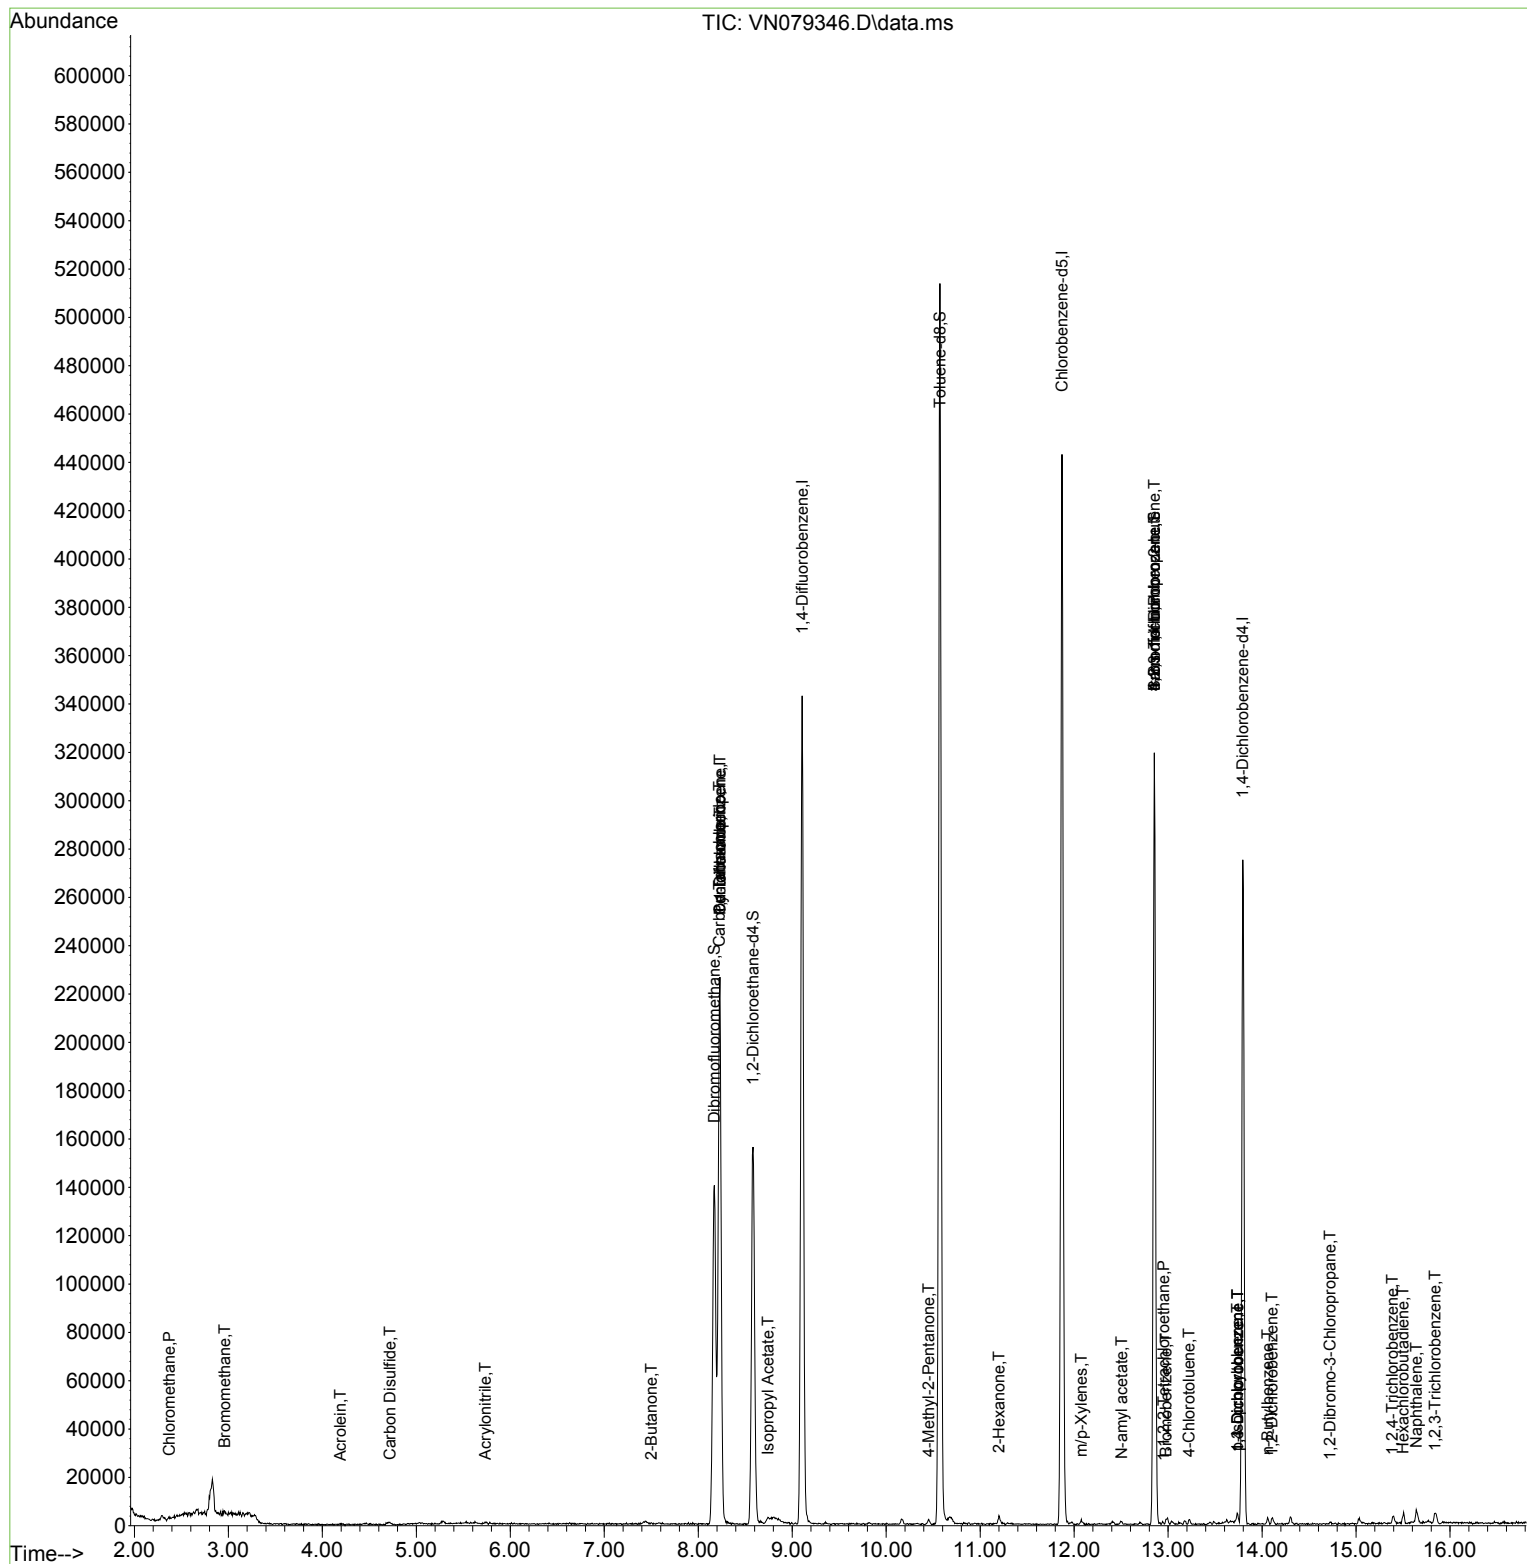






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 10
Delta R.T. -0.000 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31

Instrument :
MSVOA_N
ClientSampleId :



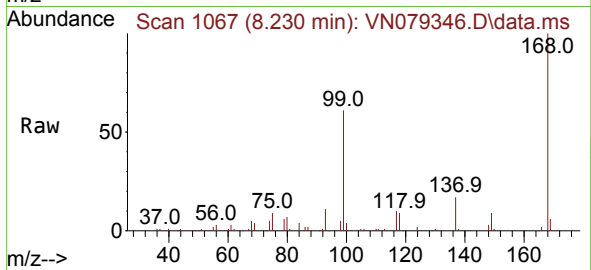



Tgt Ion:168 Resp: 154173
Ion Ratio Lower Upper
168 100
99 61.0 53.0 79.6

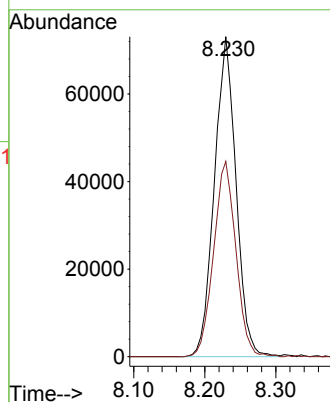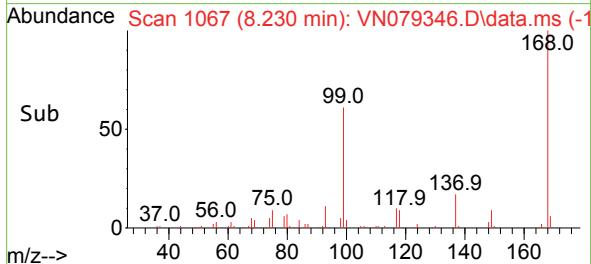

#3
Chloromethane
Concen: 0.204 ug/l
RT: 2.371 min Scan# 71
Delta R.T. 0.000 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31

Tgt Ion: 50 Resp: 409
Ion Ratio Lower Upper
50 100
52 0.0 26.5 39.7#



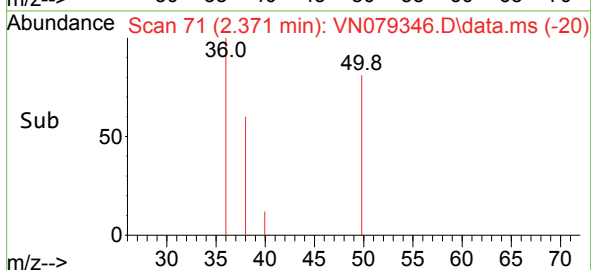



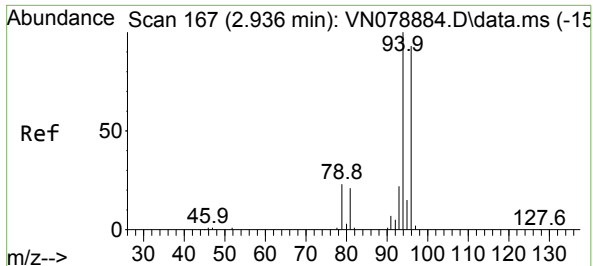

#5
Bromomethane
Concen: 0.590 ug/l
RT: 2.959 min Scan# 11
Delta R.T. 0.011 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 94 Resp: 740
Ion Ratio Lower Upper
94 100
96 92.2 73.1 109.7

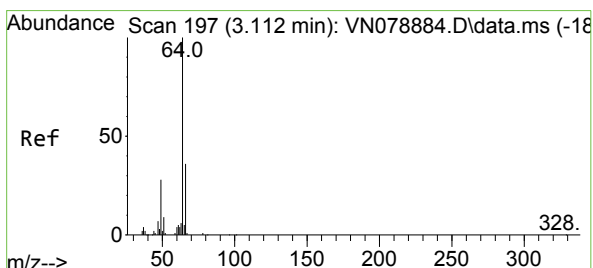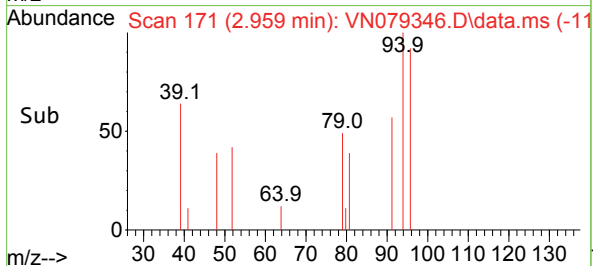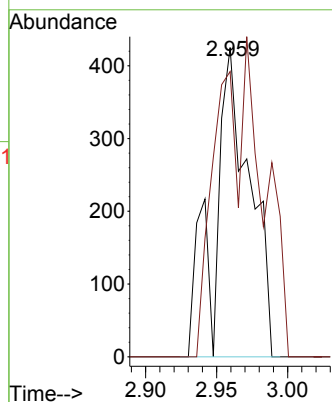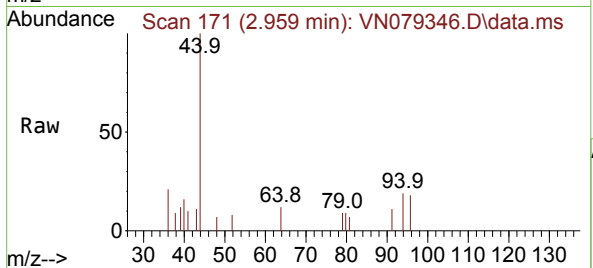

#6
Chloroethane
Concen: Below Cal
RT: 3.095 min Scan# 194
Delta R.T. -0.023 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31


Tgt Ion: 64 Resp: 161
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.2#

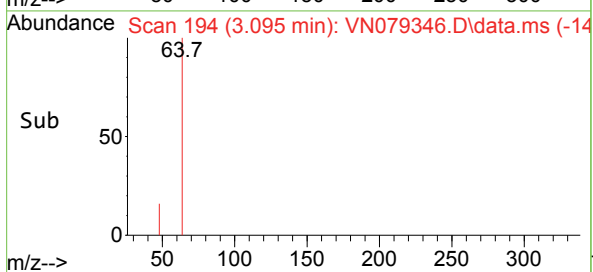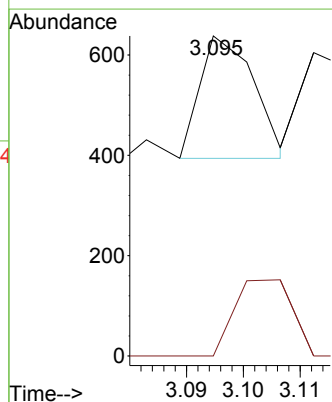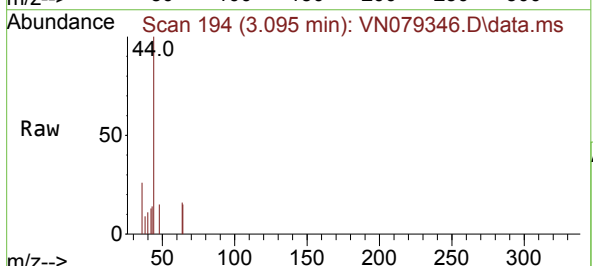





#13
Acrolein
Concen: 0.748 ug/l
RT: 4.189 min Scan# 31
Delta R.T. -0.006 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion: 56 Resp: 274
Ion Ratio Lower Upper
56 100
55 26.6 54.5 81.7#

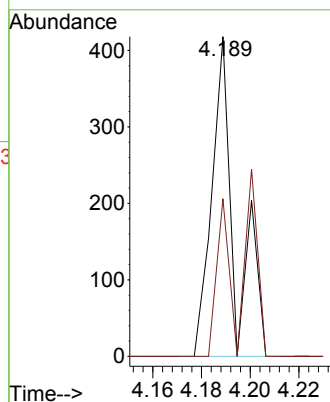


#15
Acrylonitrile
Concen: 0.374 ug/l
RT: 5.736 min Scan# 643
Delta R.T. 0.006 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31




Tgt Ion: 53 Resp: 373
Ion Ratio Lower Upper
53 100
52 106.4 65.3 97.9#
51 0.0 28.9 43.3#

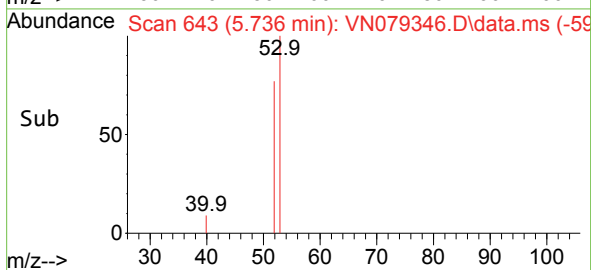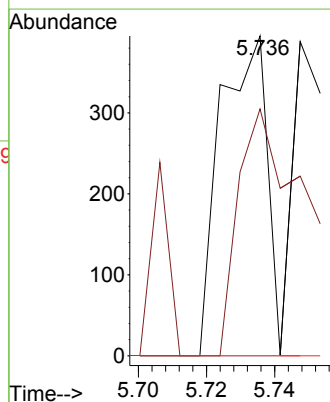






#17
Carbon Disulfide
Concen: 0.426 ug/l
RT: 4.718 min Scan# 41
Delta R.T. -0.006 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 76 Resp: 2189
Ion Ratio Lower Upper
76 100
78 0.0 7.4 11.0#

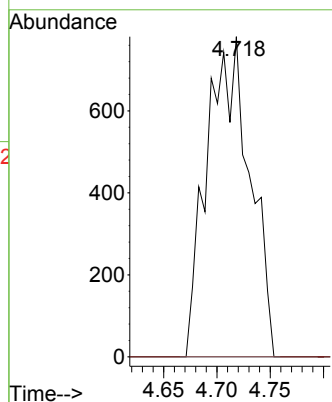

#25
2-Butanone
Concen: 0.303 ug/l
RT: 7.500 min Scan# 943
Delta R.T. 0.006 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31


Tgt Ion: 43 Resp: 388
Ion Ratio Lower Upper
43 100
72 0.0 30.2 45.2#

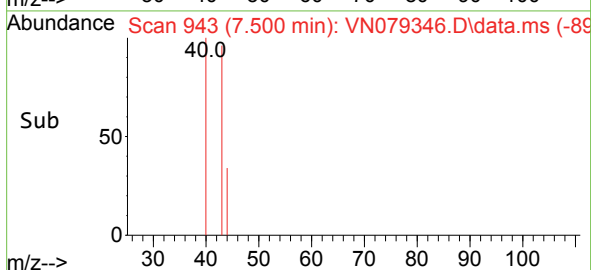






#31
Cyclohexane
Concen: 1.367 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.035 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 56 Resp: 4155
Ion Ratio Lower Upper
56 100
69 128.9 26.8 40.2#
84 117.8 81.8 122.6

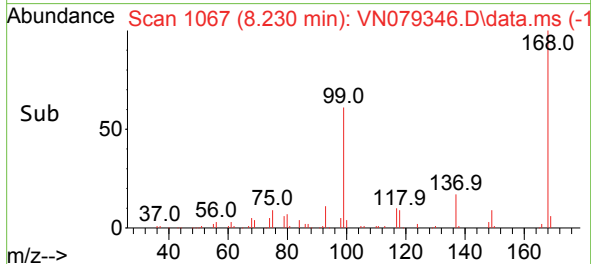

#33
1,2-Dichloroethane-d4
Concen: 62.493 ug/l
RT: 8.583 min Scan# 1127
Delta R.T. -0.000 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31

Tgt Ion: 65 Resp: 130060
Ion Ratio Lower Upper
65 100
67 53.0 0.0 106.6


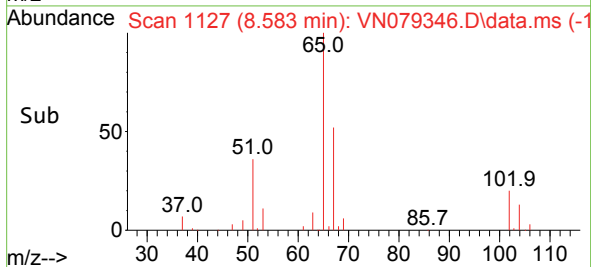

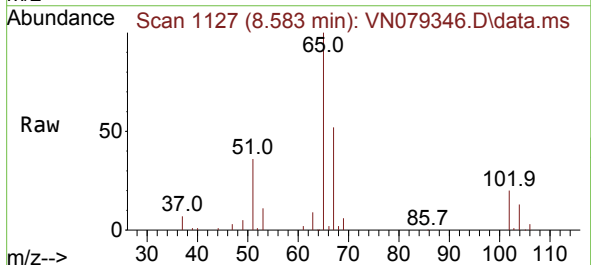




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:114 Resp: 283276
Ion Ratio Lower Upper
114 100
63 23.2 0.0 36.4
88 14.9 0.0 30.6

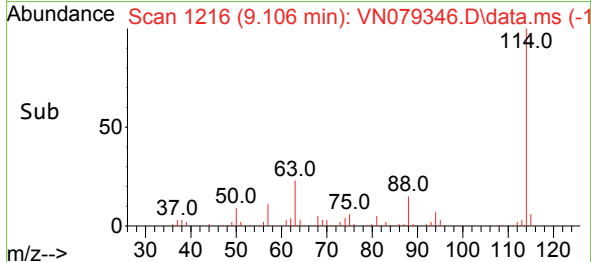

#35
Dibromofluoromethane
Concen: 55.094 ug/l
RT: 8.171 min Scan# 1057
Delta R.T. -0.000 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31

Tgt Ion:113 Resp: 103813
Ion Ratio Lower Upper
113 100
111 100.3 82.6 123.8
192 16.9 12.7 19.1


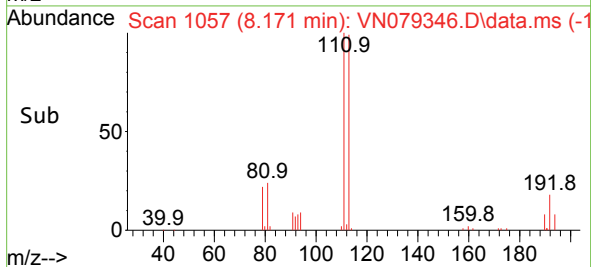

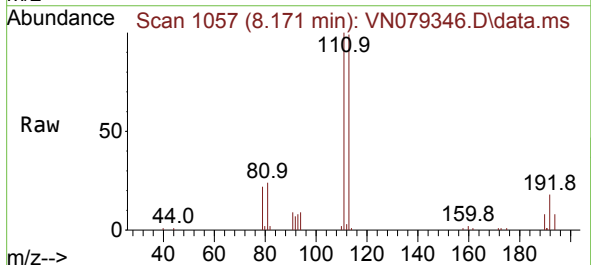




#36
1,1-Dichloropropene
Concen: 4.978 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.147 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 14459
Ion Ratio Lower Upper
75 100
110 7.0 19.1 57.3#
77 0.0 25.0 37.4#

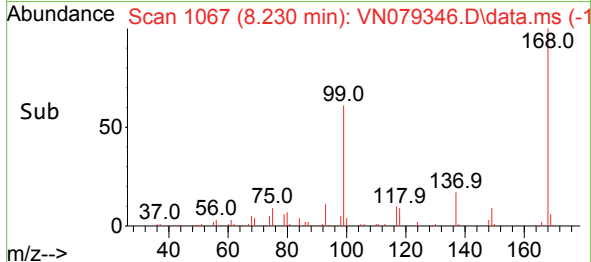

#38
Carbon Tetrachloride
Concen: 5.639 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.147 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31


Tgt Ion: 117 Resp: 16949
Ion Ratio Lower Upper
117 100
119 5.8 77.3 115.9#
121 0.0 23.3 34.9#

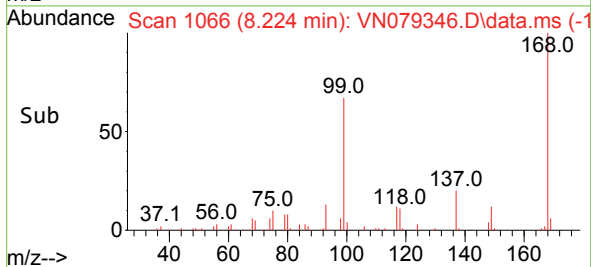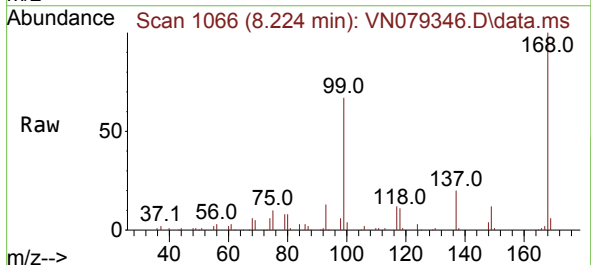






#43
Isopropyl Acetate
Concen: 0.296 ug/l
RT: 8.741 min Scan# 1146
Delta R.T. 0.047 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 43 Resp: 1398
Ion Ratio Lower Upper
43 100
61 0.0 24.7 37.1#
87 0.0 14.6 21.8#

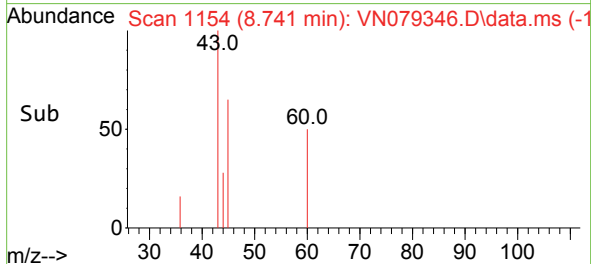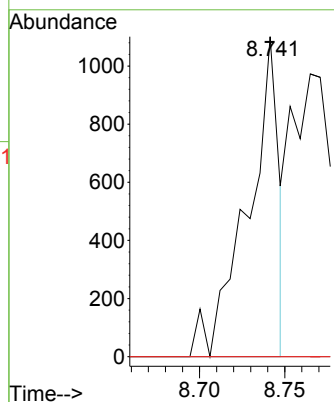

#50
Toluene-d8
Concen: 49.381 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31

Tgt Ion: 98 Resp: 341663
Ion Ratio Lower Upper
98 100
100 63.3 52.0 78.0


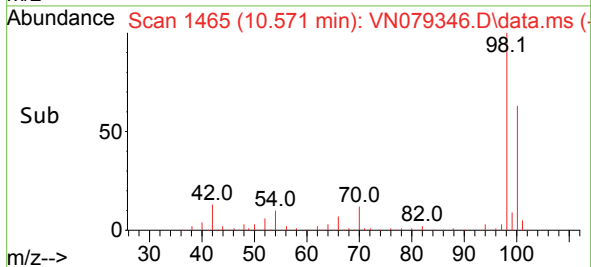
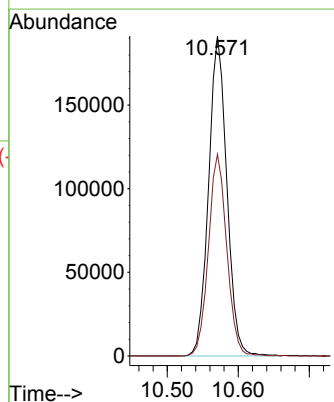
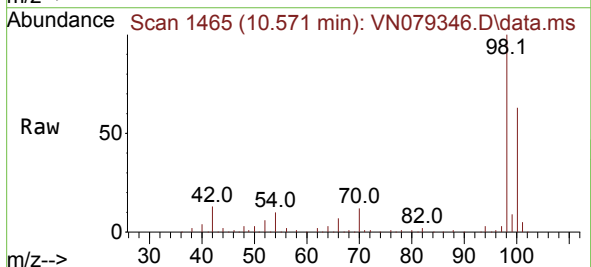




#51
4-Methyl-2-Pentanone
Concen: 0.548 ug/l
RT: 10.453 min Scan# 1445
Delta R.T. 0.000 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 1504
Ion Ratio Lower Upper
43 100
58 33.8 36.6 54.8#

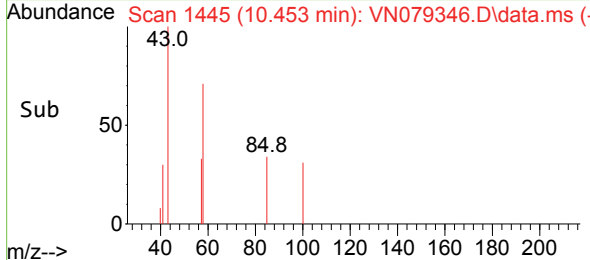

#59
2-Hexanone
Concen: 1.190 ug/l
RT: 11.200 min Scan# 1572
Delta R.T. 0.000 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31


Tgt Ion: 43 Resp: 2365
Ion Ratio Lower Upper
43 100
58 44.3 31.7 95.1

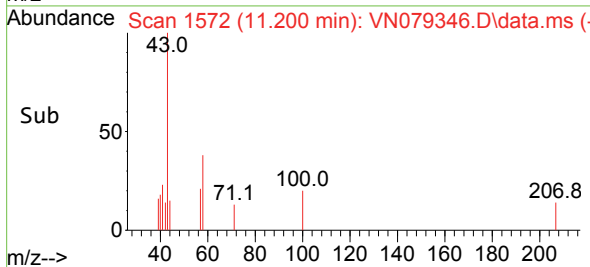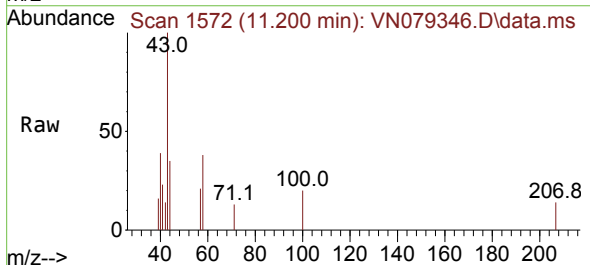






#62
4-Bromofluorobenzene
Concen: 47.650 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 95 Resp: 105162
Ion Ratio Lower Upper
95 100
174 75.9 0.0 143.8
176 73.2 0.0 135.8

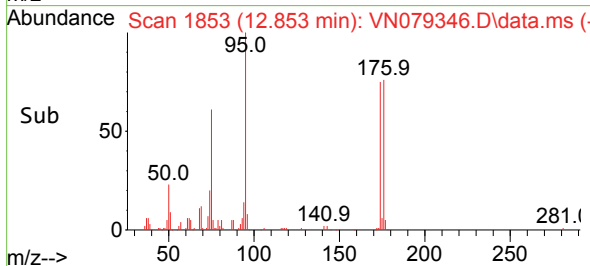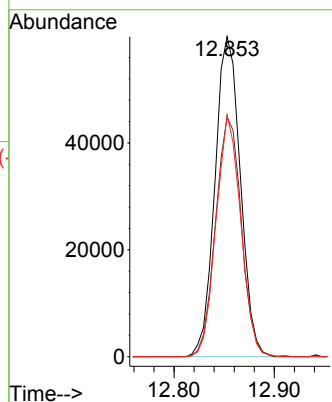

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1686
Delta R.T. -0.000 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31

Tgt Ion: 117 Resp: 246237
Ion Ratio Lower Upper
117 100
82 55.7 44.0 66.0
119 33.1 25.6 38.4


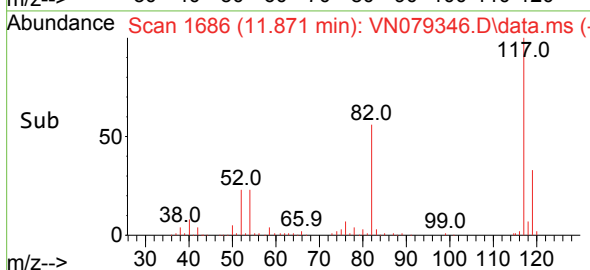

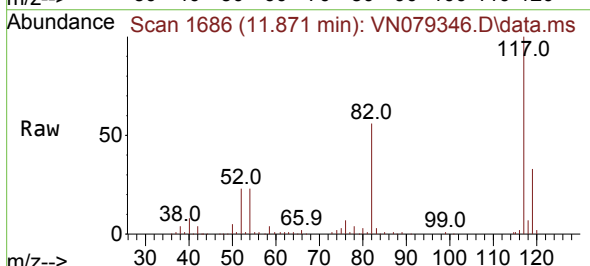




#68
m/p-Xylenes
Concen: 0.223 ug/l
RT: 12.076 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:106 Resp: 793
Ion Ratio Lower Upper
106 100
91 169.4 159.6 239.4

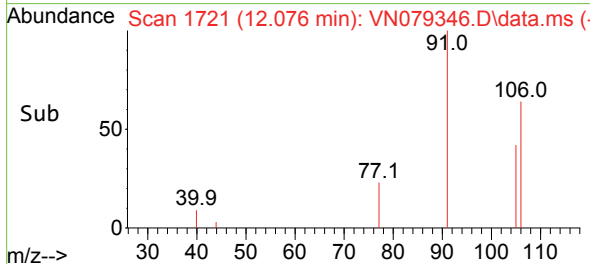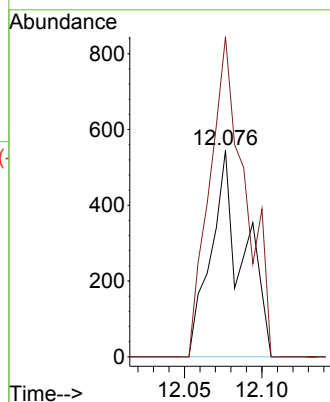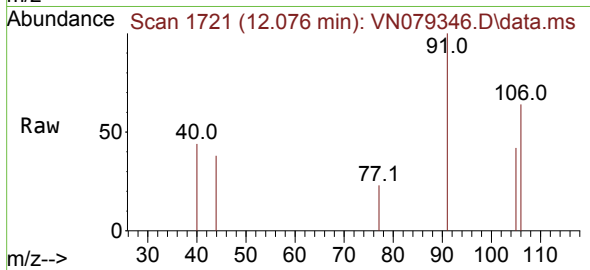

#71
Bromoform
Concen: 0.619 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.271 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31

Tgt Ion:173 Resp: 956
Ion Ratio Lower Upper
173 100
175 501.6 24.3 73.0#
254 0.0 0.0 0.0

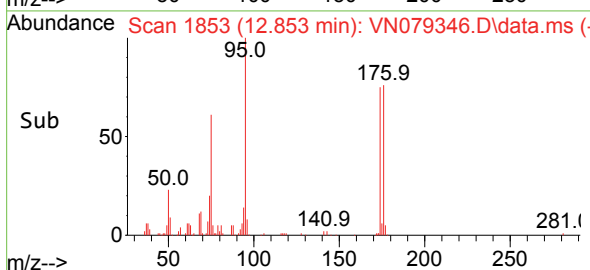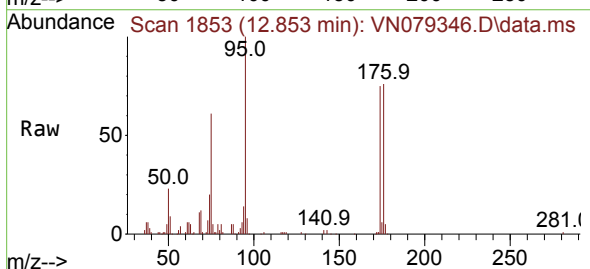

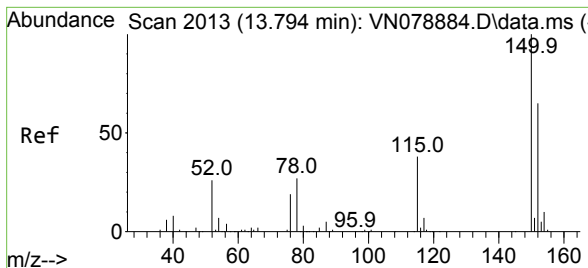

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 20

Delta R.T. 0.000 min


Lab File: VN079346.D

Acq: 26 Sep 2023 10:31

Instrument :

MSVOA_N

ClientSampleId :

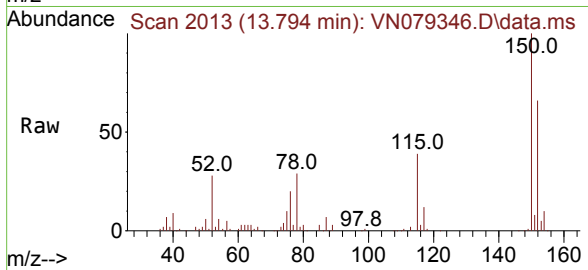




Tgt Ion:152 Resp: 71953

Ion Ratio Lower Upper

152 100

115 58.9 32.3 96.8

150 154.1 0.0 355.8

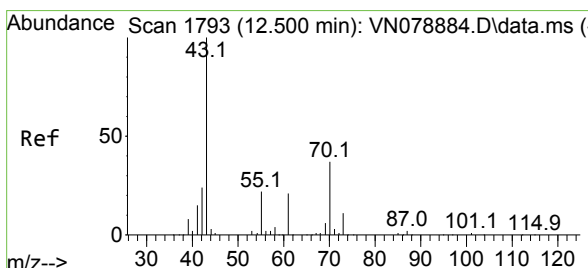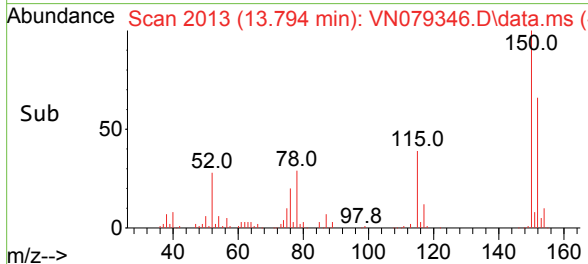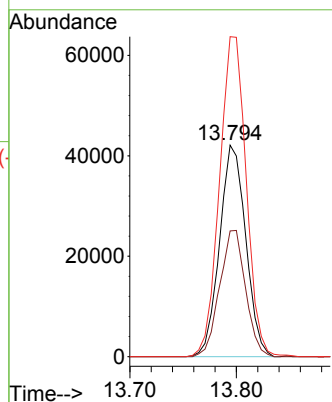

#74

N-ethyl acetate

Concen: 0.445 ug/l

RT: 12.506 min Scan# 1794

Delta R.T. 0.006 min

Lab File: VN079346.D

Acq: 26 Sep 2023 10:31

Tgt Ion: 43 Resp: 1106




Ion Ratio Lower Upper


43 100

70 19.7 43.4 65.2#

55 17.5 21.4 32.0#

61 4.8 22.8 34.2#


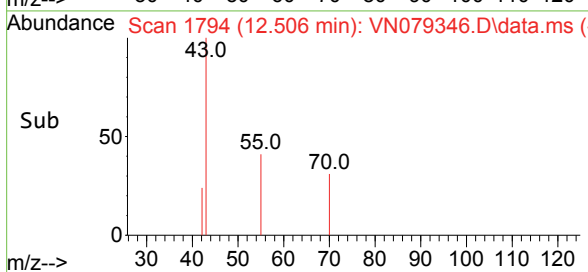
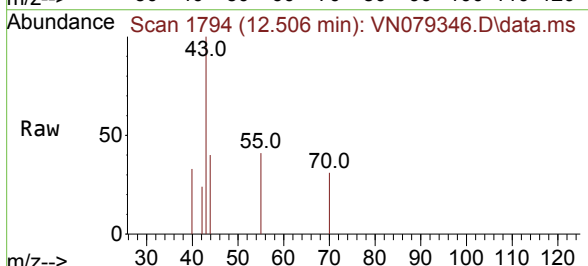



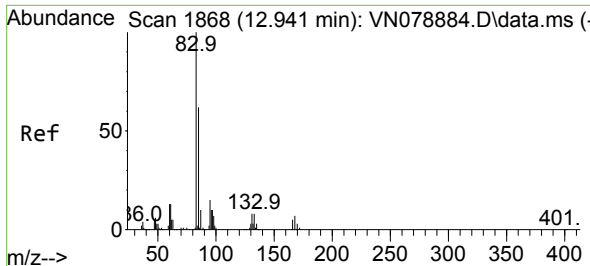

#75
 1,1,2,2-Tetrachloroethane
 Concen: 0.211 ug/l
 RT: 12.953 min Scan# 1853
 Delta R.T. 0.012 min
 Lab File: VN079346.D
 Acq: 26 Sep 2023 10:31




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 83 Resp: 514
 Ion Ratio Lower Upper
 83 100
 131 0.0 5.0 15.0#
 85 62.5 31.9 95.7

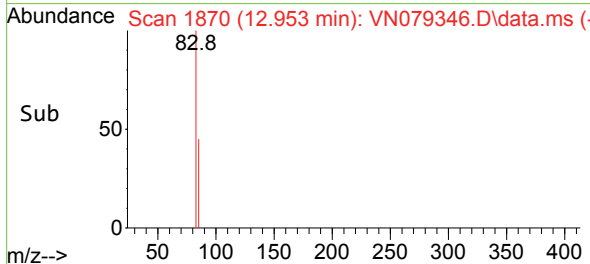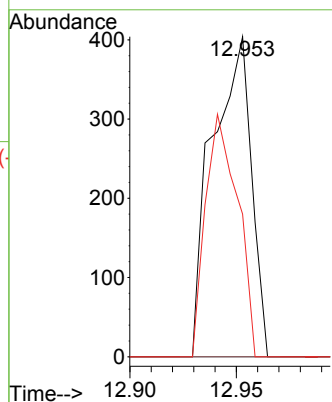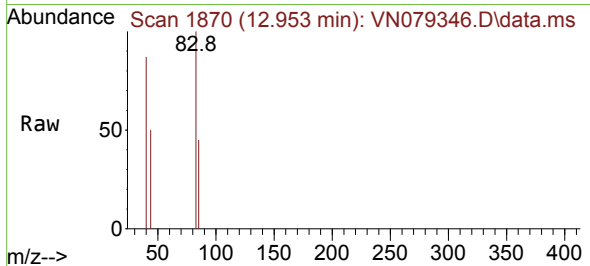

#76
 1,2,3-Trichloropropane
 Concen: 30.921 ug/l
 RT: 12.853 min Scan# 1853
 Delta R.T. -0.147 min
 Lab File: VN079346.D
 Acq: 26 Sep 2023 10:31


Tgt Ion: 75 Resp: 59963
 Ion Ratio Lower Upper
 75 100
 77 1.3 84.5 253.5#

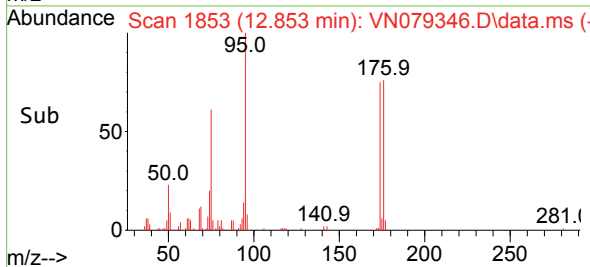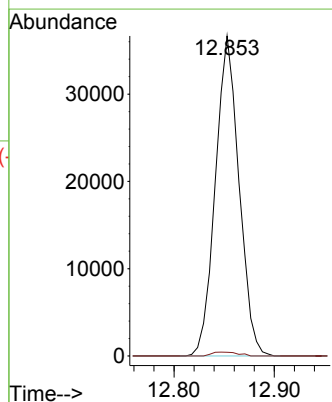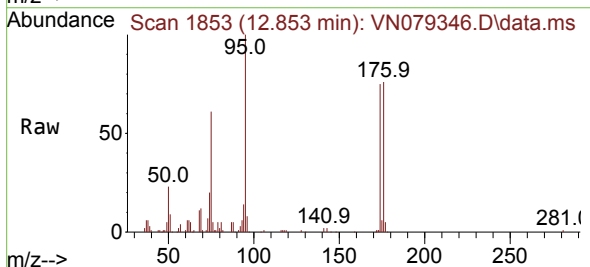






#77
Bromobenzene
Concen: 0.255 ug/l
RT: 12.976 min Scan# 1874
Delta R.T. -0.006 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:156 Resp: 423
Ion Ratio Lower Upper
156 100
77 300.2 107.7 323.3
158 102.8 48.4 145.3

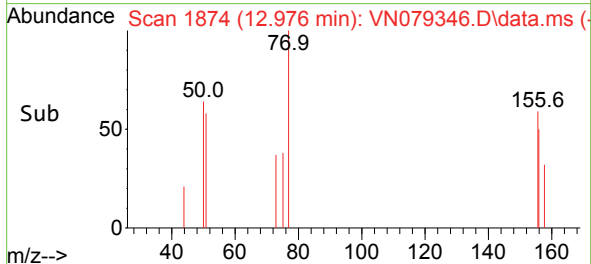


#81
trans-1,4-Dichloro-2-butene
Concen: 85.009 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.112 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31



Tgt Ion: 75 Resp: 59963
Ion Ratio Lower Upper
75 100
53 0.0 67.4 101.2#
89 0.1 38.8 58.2#




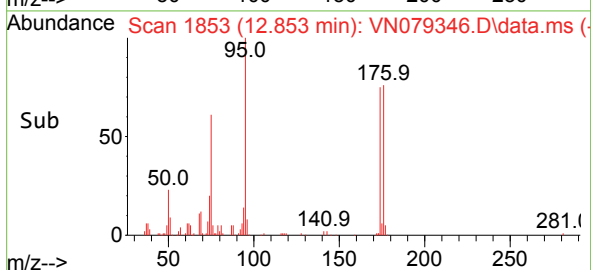




#82
4-Chlorotoluene
Concen: 0.328 ug/l
RT: 13.223 min Scan# 1916
Delta R.T. -0.006 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 1482
Ion Ratio Lower Upper
91 100
126 29.6 16.7 50.0

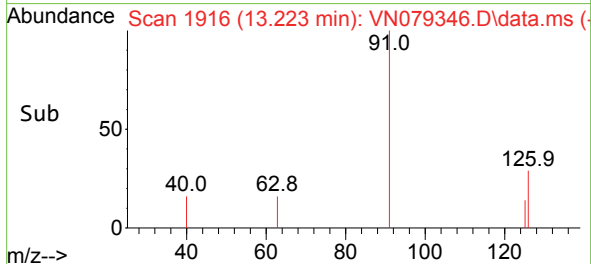

#86
p-Isopropyltoluene
Concen: 0.244 ug/l
RT: 13.735 min Scan# 2003
Delta R.T. 0.000 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31

Tgt Ion: 119 Resp: 1212
Ion Ratio Lower Upper
119 100
134 4.6 12.6 37.8#
91 13.0 12.4 37.2

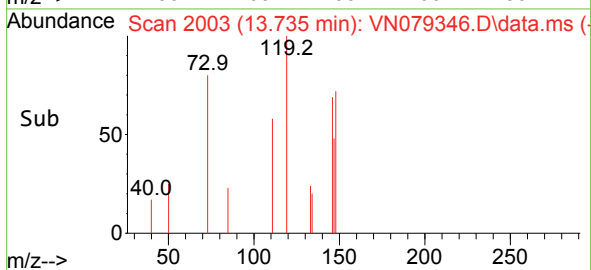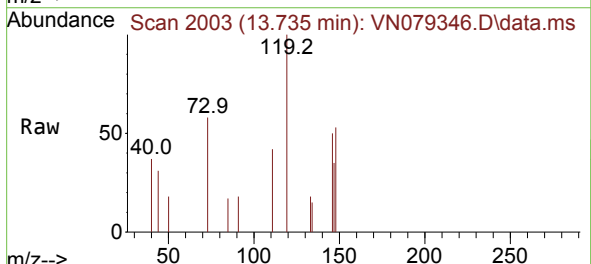

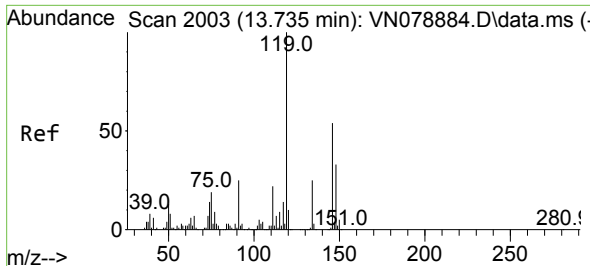

#87

1,3-Dichlorobenzene

Concen: 0.439 ug/l

RT: 13.741 min Scan# 2004

Delta R.T. 0.000 min


Lab File: VN079346.D

Acq: 26 Sep 2023 10:31

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion:146 Resp: 1193

Ion Ratio Lower Upper

146 100

111 41.6 22.1 66.3

148 62.1 32.0 96.0

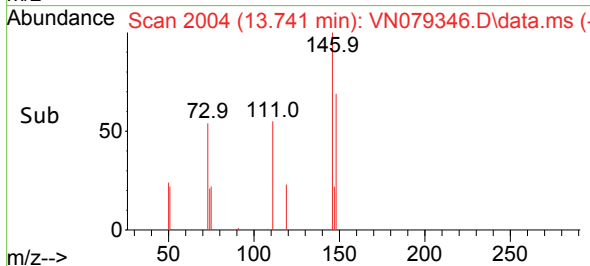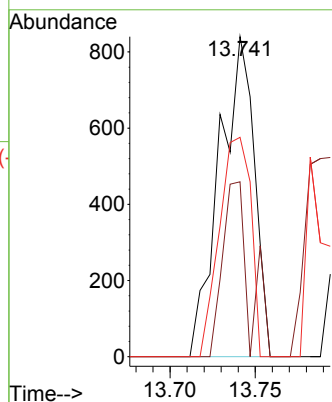

#88

1,4-Dichlorobenzene

Concen: 0.434 ug/l

RT: 13.741 min Scan# 2004

Delta R.T. -0.077 min

Lab File: VN079346.D

Acq: 26 Sep 2023 10:31




Tgt Ion:146 Resp: 1193


Ion Ratio Lower Upper

146 100

111 41.6 20.6 61.8

148 62.1 31.6 94.8


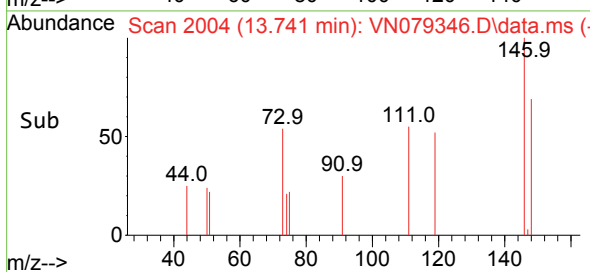
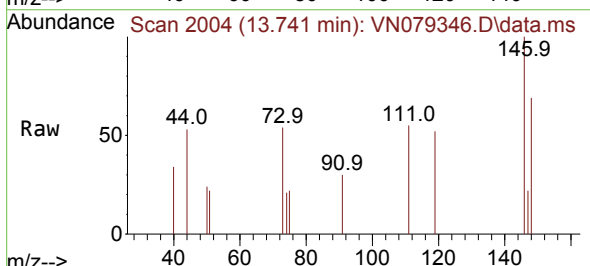
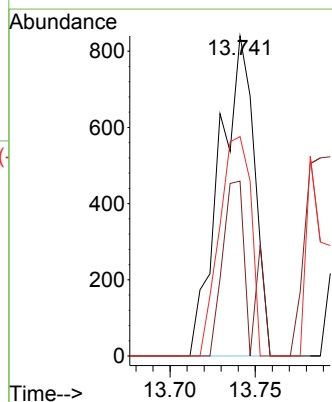




#89
n-Butylbenzene
Concen: 0.494 ug/l
RT: 14.059 min Scan# 2058
Delta R.T. -0.000 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:	91	Resp:	1930
Ion	Ratio	Lower	Upper
91	100		
92	45.3	26.4	79.0
134	13.3	12.6	37.6

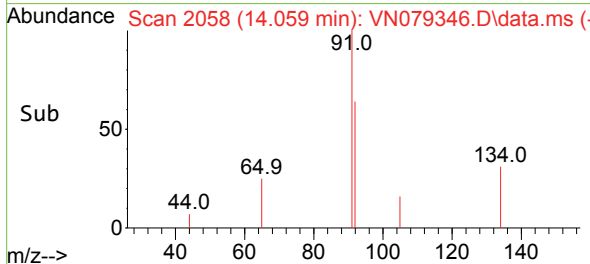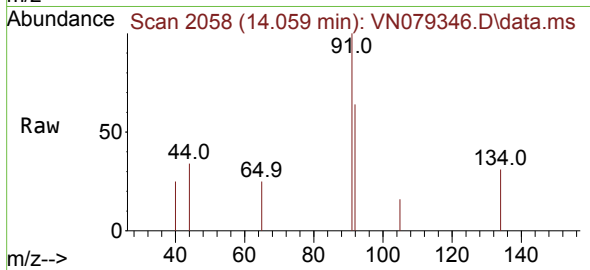

#91
1,2-Dichlorobenzene
Concen: 0.556 ug/l
RT: 14.106 min Scan# 2066
Delta R.T. -0.006 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31


Tgt Ion:	146	Resp:	1492
Ion	Ratio	Lower	Upper
146	100		
111	41.8	22.0	66.0
148	52.3	31.8	95.3

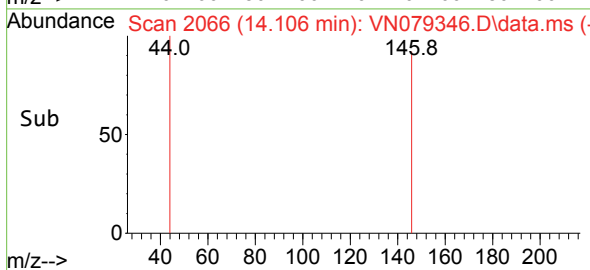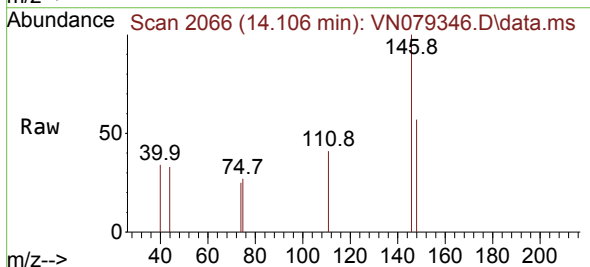






#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.362 ug/l
 RT: 14.723 min Scan# 2171
 Delta R.T. 0.000 min
 Lab File: VN079346.D
 Acq: 26 Sep 2023 10:31


Instrument :
 MSVOA_N
 ClientSampleId :





Tgt Ion: 75 Resp: 134
 Ion Ratio Lower Upper
 75 100
 155 97.8 39.1 117.2
 157 92.5 50.3 150.9

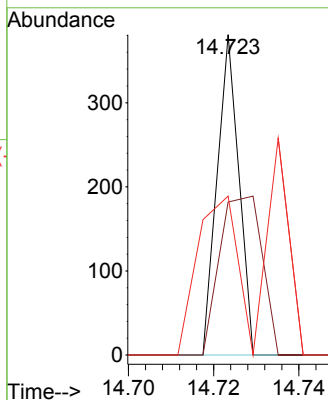


#93
 1,2,4-Trichlorobenzene
 Concen: 1.340 ug/l
 RT: 15.388 min Scan# 2284
 Delta R.T. -0.012 min
 Lab File: VN079346.D
 Acq: 26 Sep 2023 10:31



Tgt Ion: 180 Resp: 1292
 Ion Ratio Lower Upper
 180 100
 182 99.7 46.1 138.2
 145 25.4 16.6 49.8



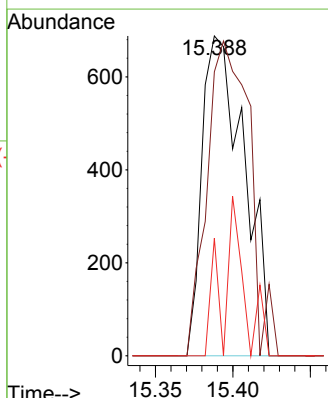





#94
Hexachlorobutadiene
Concen: 0.996 ug/l
RT: 15.500 min Scan# 21
Delta R.T. -0.006 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:	225	Resp:	756
Ion	Ratio	Lower	Upper
225	100		
223	92.7	31.3	93.8
227	77.9	31.9	95.9

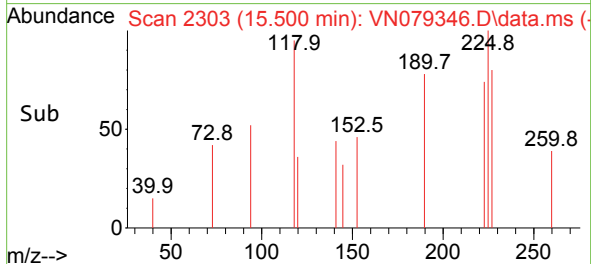

#95
Naphthalene
Concen: 1.823 ug/l
RT: 15.641 min Scan# 2327
Delta R.T. -0.006 min
Lab File: VN079346.D
Acq: 26 Sep 2023 10:31


Tgt Ion:	128	Resp:	5223
Ion	Ratio	Lower	Upper
128	100		
127	12.3	10.0	15.0
129	10.8	8.7	13.1

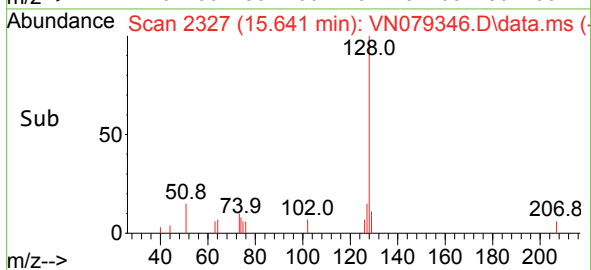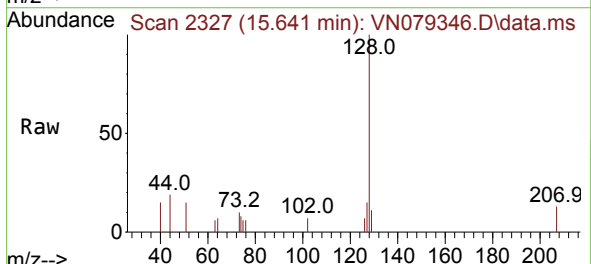



#96
 1,2,3-Trichlorobenzene
 Concen: 1.703 ug/l
 RT: 15.841 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: VN079346.D
 Acq: 26 Sep 2023 10:31

Instrument :
 MSVOA_N
 ClientSampleId :

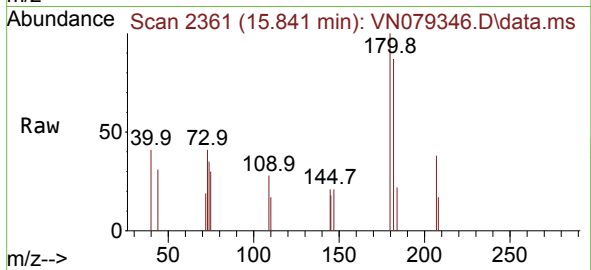

Tgt Ion:	180	Resp:	1938
Ion	Ratio	Lower	Upper
180	100		
182	93.8	46.2	138.6
145	30.0	17.5	52.6

