
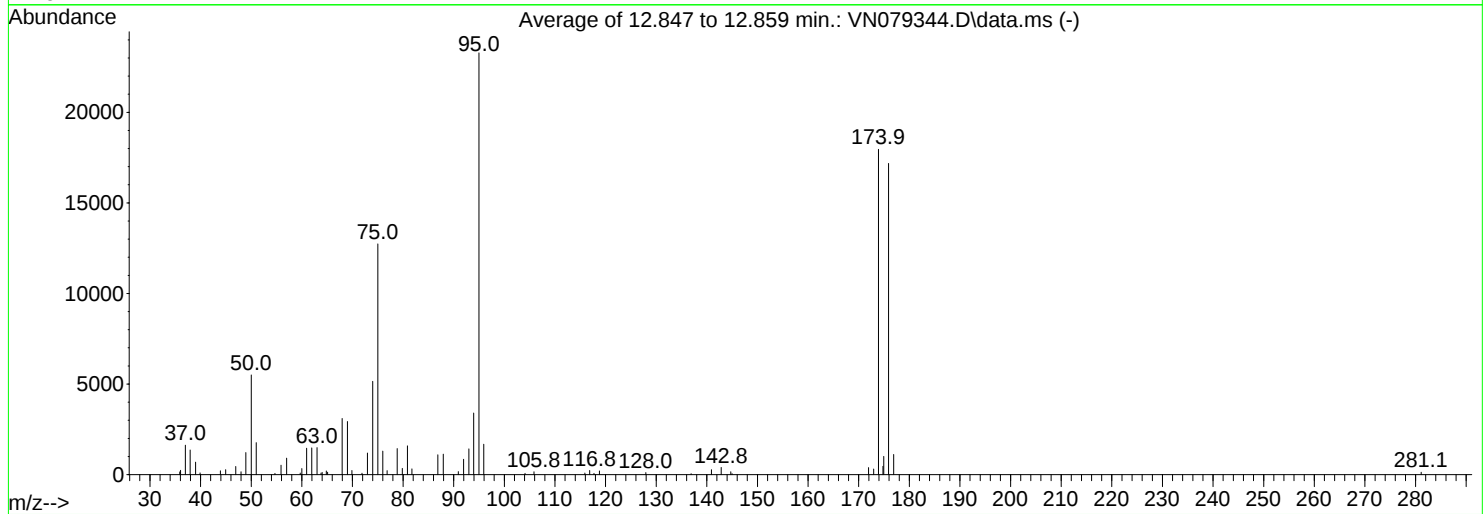


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092623\
 Data File : VN079344.D
 Acq On : 26 Sep 2023 08:25
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091123W.M
 Title : SW846 8260
 Last Update : Tue Sep 12 05:05:24 2023

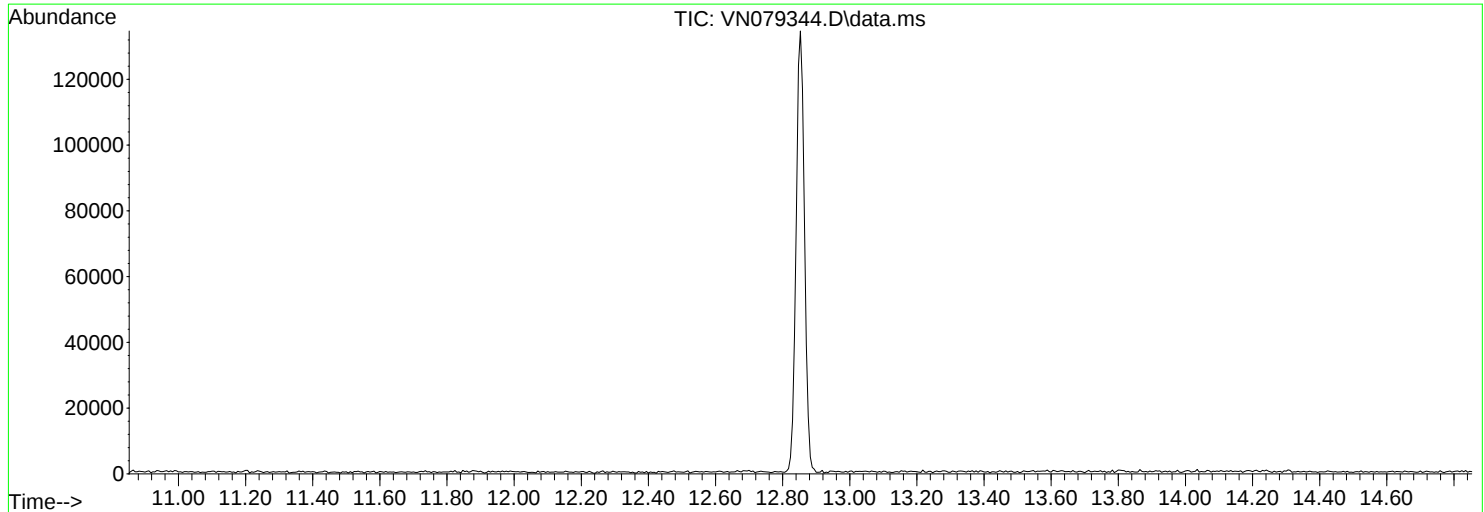

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.6	5504	PASS
75	95	30	60	54.7	12734	PASS
95	95	100	100	100.0	23283	PASS
96	95	5	9	7.2	1680	PASS
173	174	0.00	2	1.7	308	PASS
174	95	50	100	77.1	17957	PASS
175	174	5	9	5.6	1006	PASS
176	174	95	101	95.7	17181	PASS
177	176	5	9	6.5	1117	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	147	50.00	5504	64.00	121	76.85	221
36.05	237	51.00	1768	64.85	199	78.85	143
37.00	1627	54.70	67	65.10	129	79.85	34
37.95	1364	55.90	521	67.95	3097	80.85	158
39.00	687	57.00	912	69.00	2930	81.75	315
39.90	94	59.70	93	69.90	231	86.85	1098
43.90	209	60.00	334	71.90	84	87.95	1133
44.95	277	60.95	1461	72.95	1189	90.90	167
46.95	451	61.95	1477	74.00	5149	91.95	849
48.00	161	63.00	1496	75.00	12734	93.00	1420
48.95	1217	63.80	87	76.00	1296	93.95	3405

Average of 12.847 to 12.859 min.: VN079344.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.00	23283	142.85	395				
95.95	1680	144.75	161				
104.10	72	145.00	57				
105.85	158	171.95	391				
115.90	92	172.95	308				
116.85	231	173.90	17957				
117.70	70	174.80	463				
118.80	201	174.95	1006				
127.95	119	175.90	17181				
136.90	51	176.90	1117				
140.90	278	281.10	134				

Instrument :

MSVOA_N

ClientSampleId :

BFB