

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092624\
 Data File : VN084178.D
 Acq On : 26 Sep 2024 15:52
 Operator : JC\MD
 Sample : P4176-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 FB-NC-SYS2

Quant Time: Sep 27 01:10:40 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N090624W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Fri Sep 06 23:42:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	7.812	128	28263	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	9.100	114	138817	30.000	ug/l	0.00
57) Chlorobenzene-d5	11.865	117	127236	30.000	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.577	65	69719	26.987	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	89.967%#
60) 4-Bromofluorobenzene	12.853	95	54543	24.873	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	82.900%
63) Toluene-d8	10.571	98	173326	29.420	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	98.067%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092624\
Data File : VN084178.D
Acq On : 26 Sep 2024 15:52
Operator : JC\MD
Sample : P4176-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FB-NC-SYS2

Quant Time: Sep 27 01:10:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N090624W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Fri Sep 06 23:42:47 2024
Response via : Initial Calibration




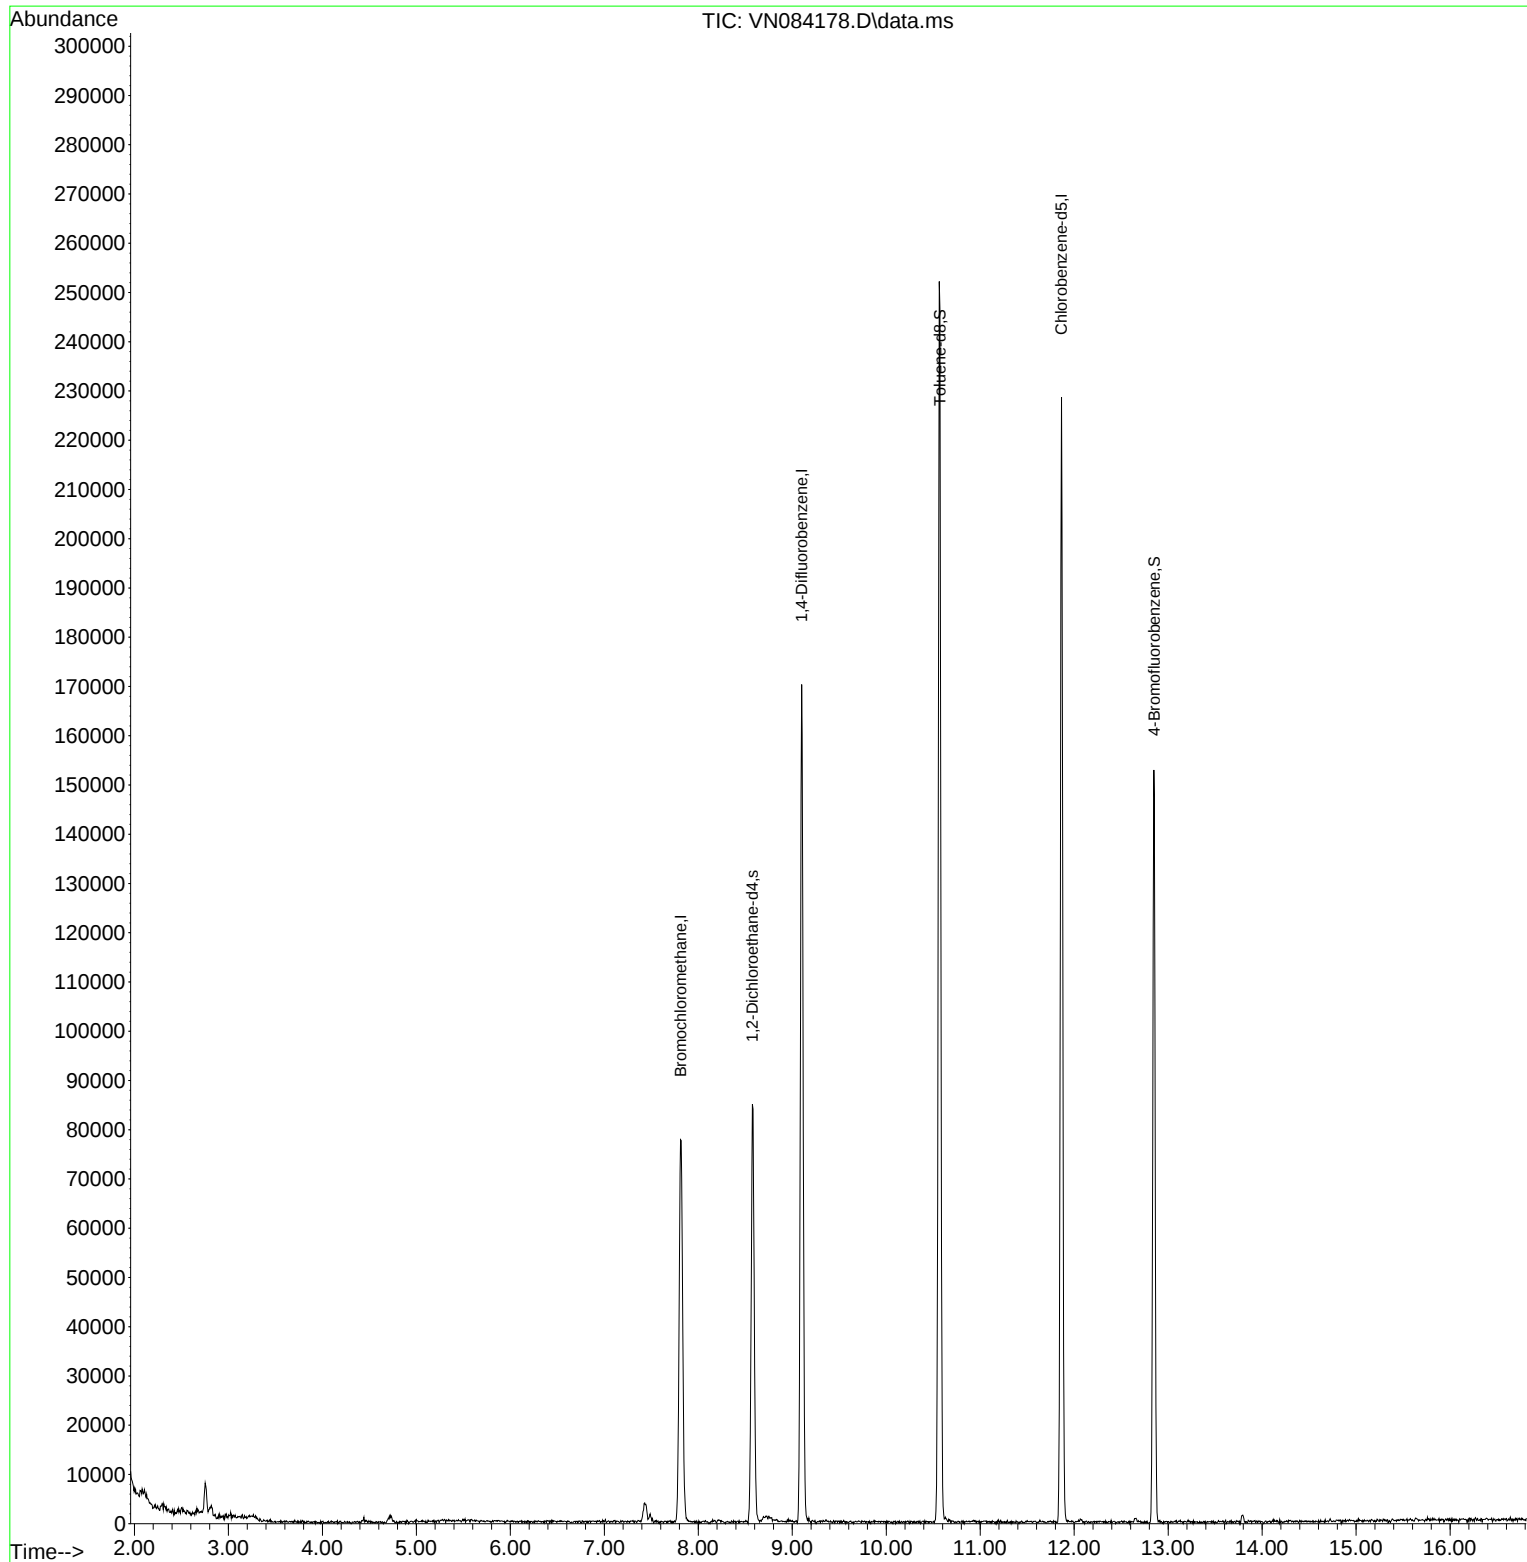




#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 7.812 min Scan# 996
Delta R.T. -0.000 min
Lab File: VN084178.D
Acq: 26 Sep 2024 15:52




Instrument :
MSVOA_N
ClientSampleId :
FB-NC-SYS2


Tgt Ion:128 Resp: 28263
Ion Ratio Lower Upper
128 100
49 171.8 0.0 403.7
130 126.4 0.0 323.3

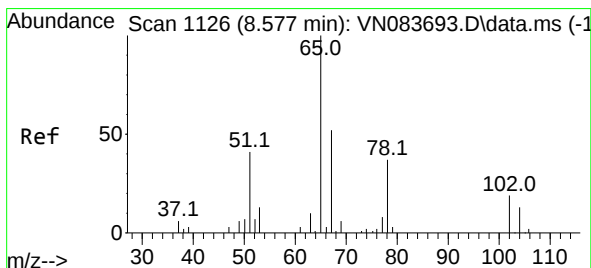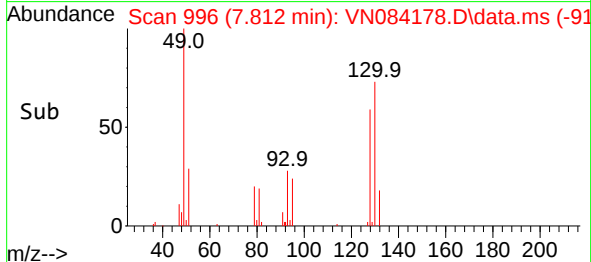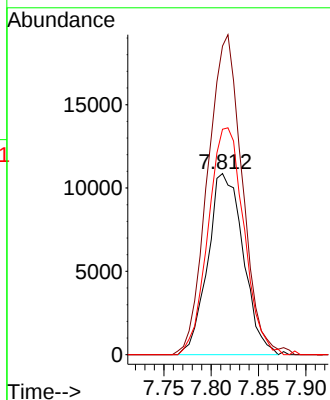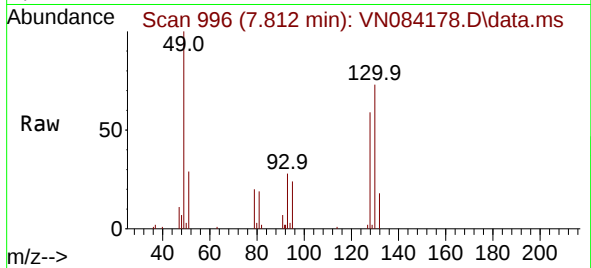

#27
1,2-Dichloroethane-d4
Concen: 26.987 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. -0.000 min
Lab File: VN084178.D
Acq: 26 Sep 2024 15:52

Tgt Ion: 65 Resp: 69719
Ion Ratio Lower Upper
65 100
67 53.4 43.2 64.8


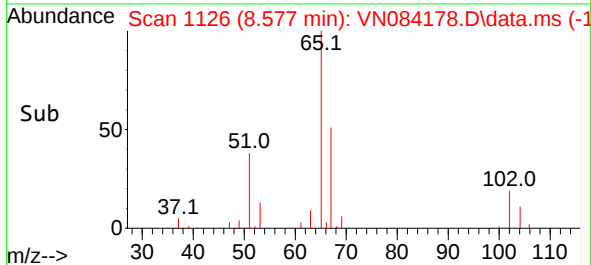
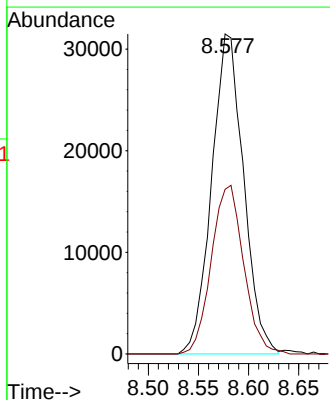
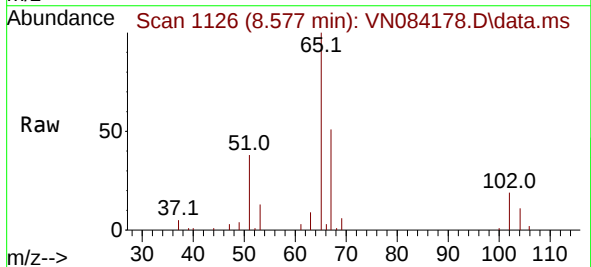


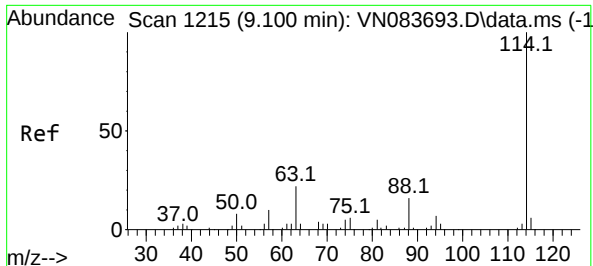

#28
1,4-Difluorobenzene
Concen: 30.000 ug/l
RT: 9.100 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN084178.D
Acq: 26 Sep 2024 15:52




Instrument :
MSVOA_N
ClientSampleId :
FB-NC-SYS2


Tgt Ion:114 Resp: 138817
Ion Ratio Lower Upper
114 100
63 22.8 15.9 23.9
88 16.6 12.7 19.1

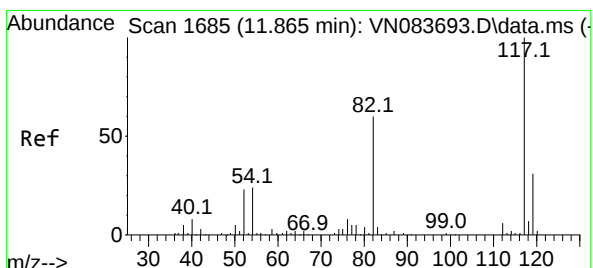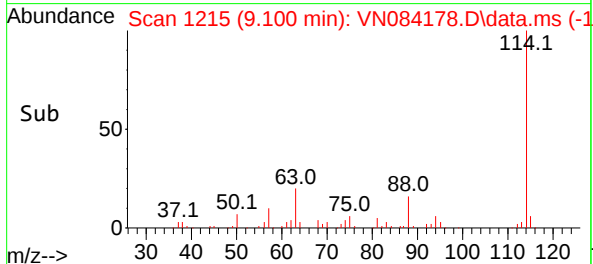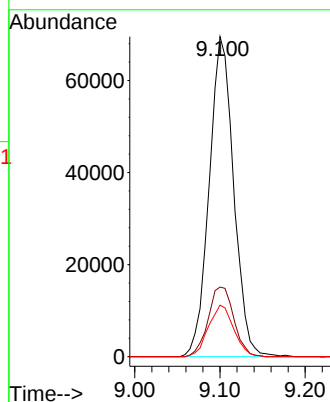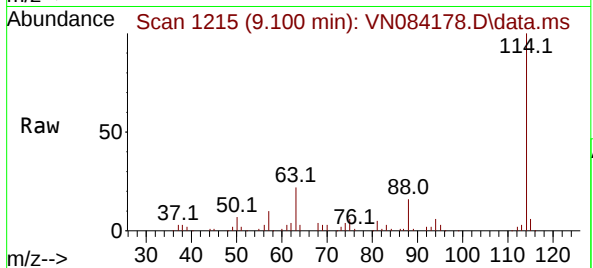

#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 11.865 min Scan# 1685
Delta R.T. -0.000 min
Lab File: VN084178.D
Acq: 26 Sep 2024 15:52

Tgt Ion:117 Resp: 127236
Ion Ratio Lower Upper
117 100
82 58.1 46.6 69.8
119 31.8 25.4 38.2


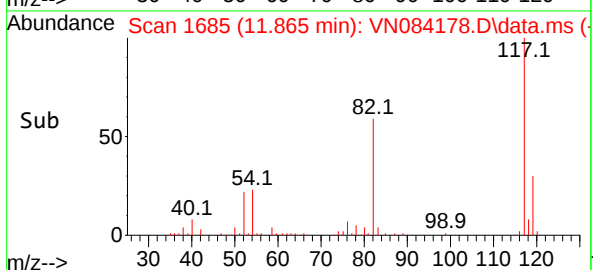
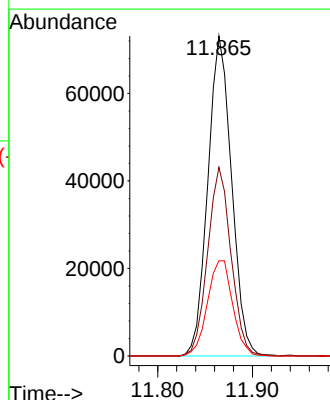
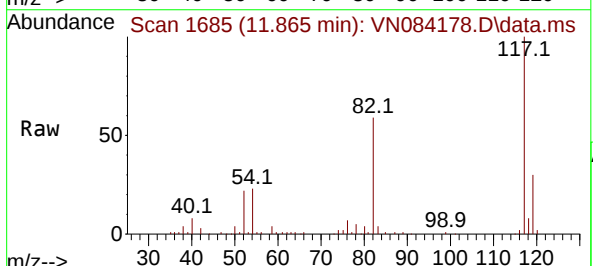


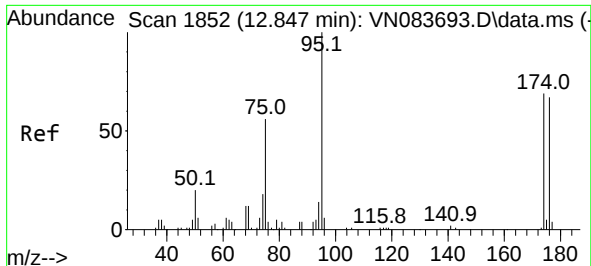

#60
4-Bromofluorobenzene
Concen: 24.873 ug/l
RT: 12.853 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN084178.D
Acq: 26 Sep 2024 15:52

Instrument :
MSVOA_N
ClientSampleId :
FB-NC-SYS2

Tgt Ion: 95 Resp: 54543
Ion Ratio Lower Upper
95 100
174 72.3 60.5 90.7
176 66.1 57.8 86.6

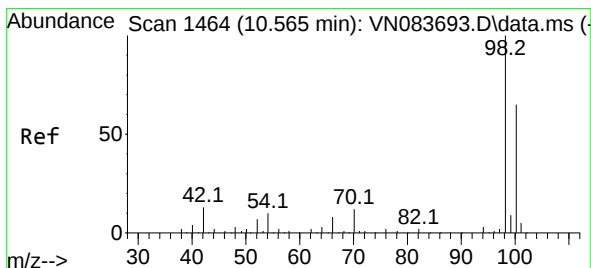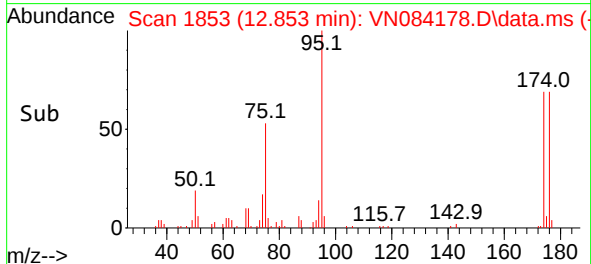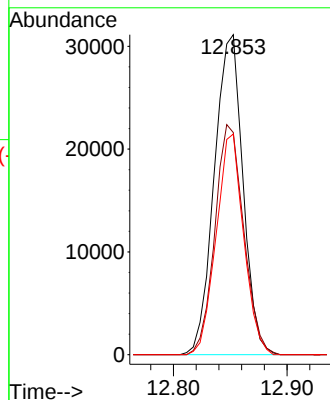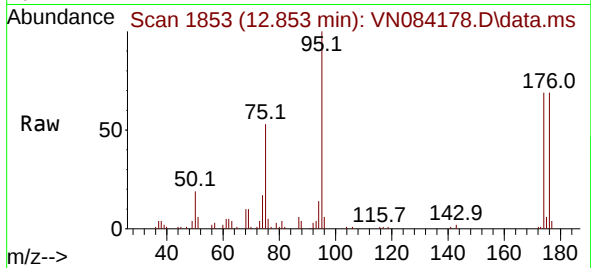

#63
Toluene-d8
Concen: 29.420 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.006 min
Lab File: VN084178.D
Acq: 26 Sep 2024 15:52

Tgt Ion: 98 Resp: 173326
Ion Ratio Lower Upper
98 100
100 64.7 52.7 79.1

