
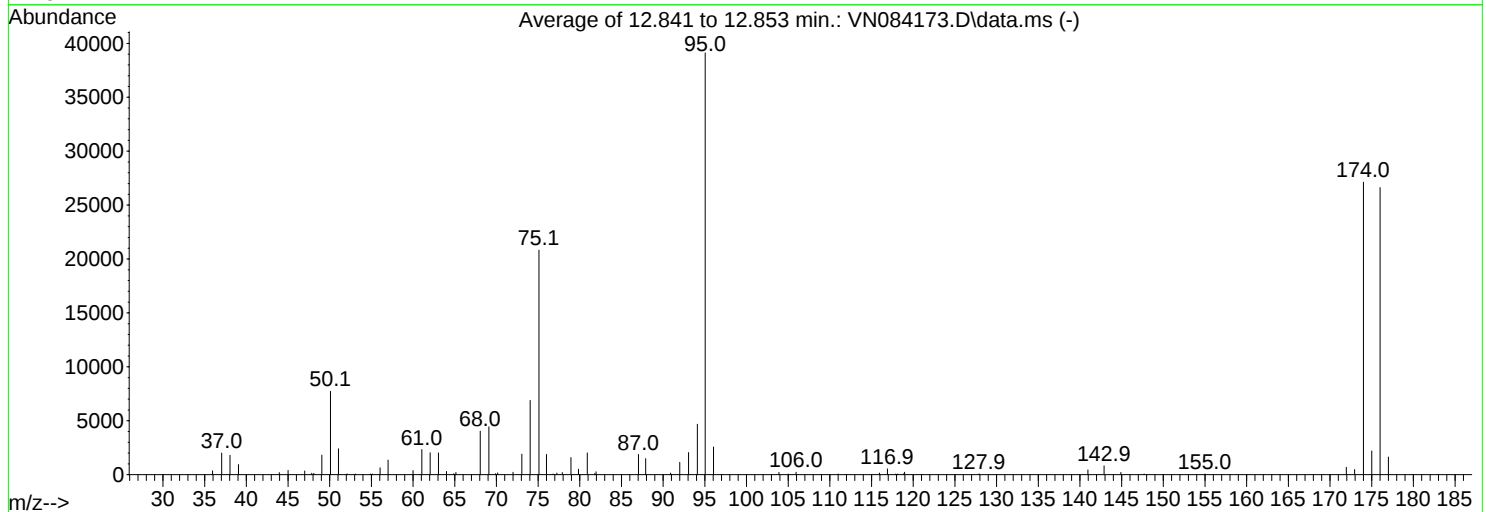


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092624\
Data File : VN084173.D
Acq On : 26 Sep 2024 11:55
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N090624W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Sep 06 23:42:47 2024

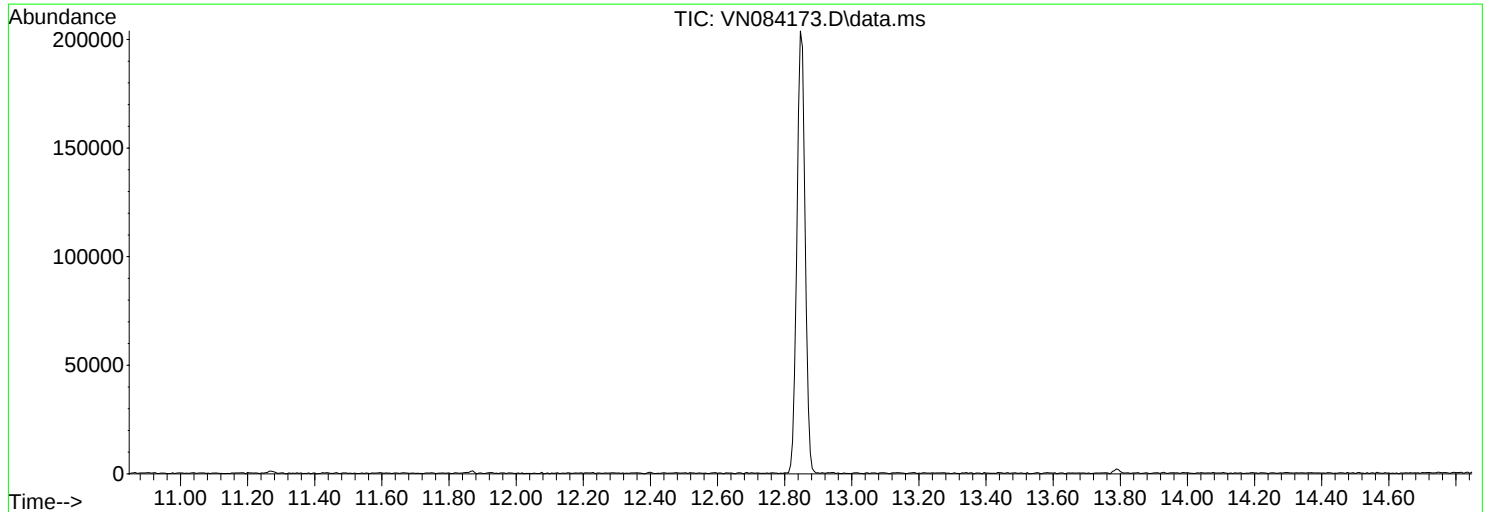

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	7731	PASS
75	95	30	60	53.2	20819	PASS
95	95	100	100	100.0	39120	PASS
96	95	5	9	6.6	2563	PASS
173	174	0.00	2	1.7	470	PASS
174	95	50	100	69.3	27128	PASS
175	174	5	9	8.1	2193	PASS
176	174	95	101	98.1	26624	PASS
177	176	5	9	6.1	1633	PASS