


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092625\
Data File : VN087960.D
Acq On : 26 Sep 2025 12:11
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N092325W.M
Title : SW846 8260
Last Update : Wed Sep 24 05:05:30 2025

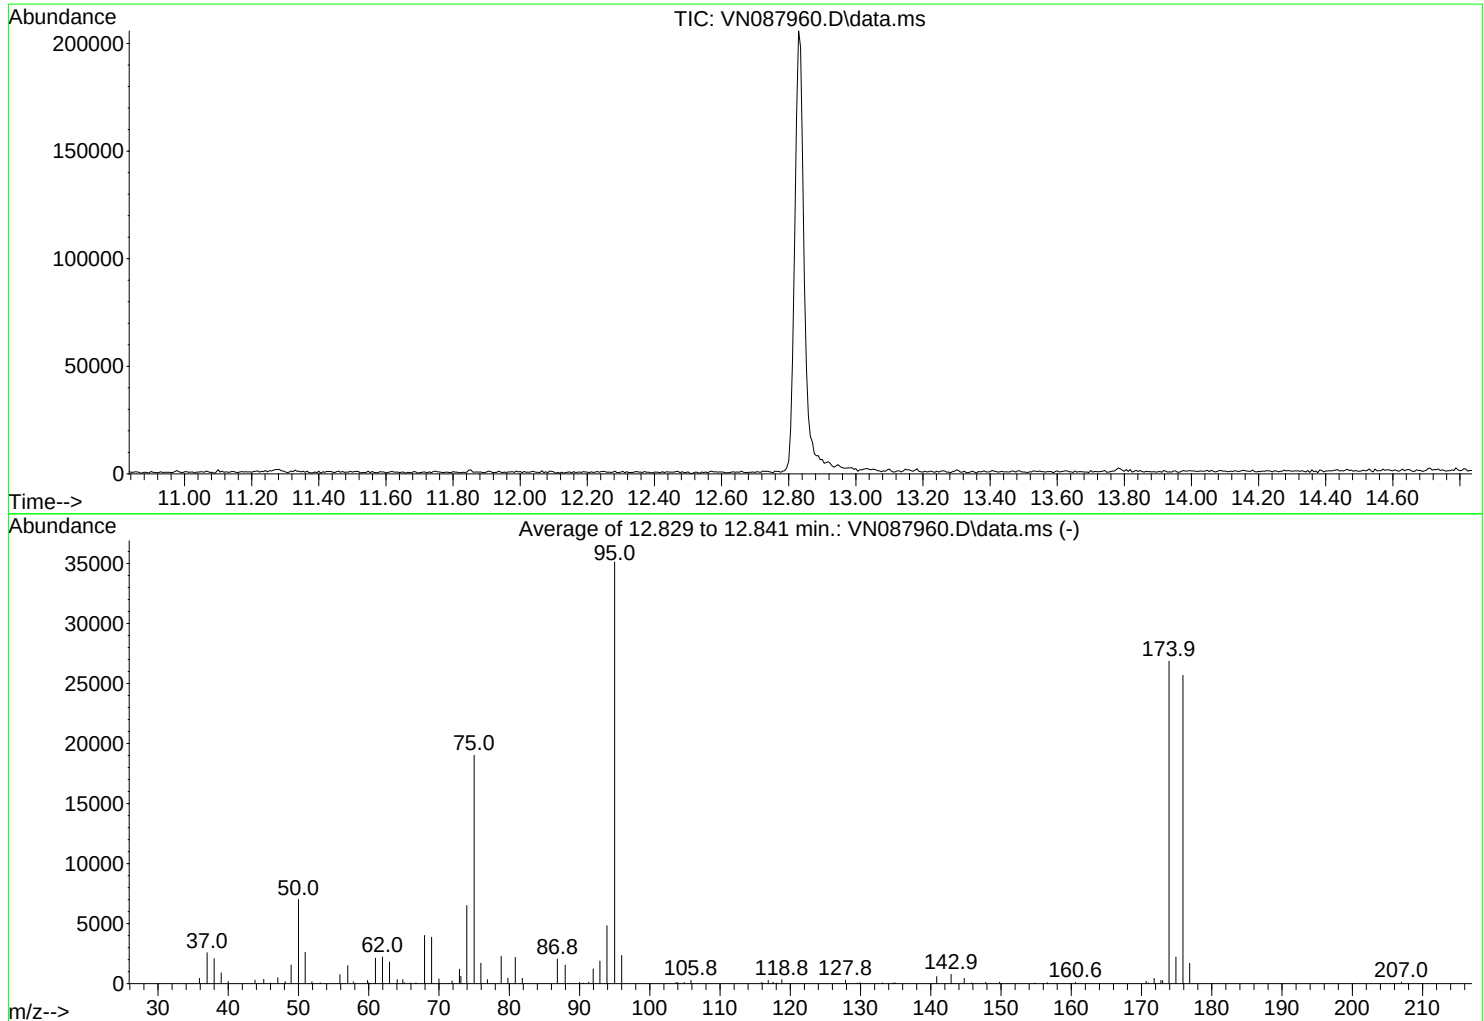

AutoFind: Scans 1849, 1850, 1851; Background Corrected with Scan 1840

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.9	6994	PASS
75	95	30	60	54.2	19030	PASS
95	95	100	100	100.0	35133	PASS
96	95	5	9	6.7	2347	PASS
173	174	0.00	2	1.0	269	PASS
174	95	50	100	76.4	26859	PASS
175	174	5	9	8.3	2218	PASS
176	174	95	101	95.6	25677	PASS
177	176	5	9	6.6	1703	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	446	50.00	6994	62.95	1803	73.10	611
37.00	2568	50.95	2609	64.05	338	73.95	651
38.00	2098	51.90	166	64.85	329	75.00	1903
39.00	897	53.10	66	65.10	64	75.95	170
40.00	171	55.90	751	65.90	56	76.90	329
43.80	290	57.00	1498	66.70	62	78.85	2272
45.05	354	57.80	151	67.95	4015	79.80	452
46.00	59	59.80	271	68.95	3869	80.85	2191
47.05	494	60.00	87	70.00	400	81.85	446
48.10	175	60.95	2116	71.85	222	86.85	2037
48.95	1550	61.95	2219	72.90	1198	87.95	1546

Average of 12.829 to 12.841 min.: VN087960.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.00	105	105.85	283	134.60	52	170.65	205
90.50	53	115.90	100	134.90	80	171.00	66
91.30	122	116.10	54	140.85	584	171.80	439
91.95	1232	116.85	263	142.90	776	172.75	269
92.90	1883	117.55	133	144.75	444	173.00	258
93.90	4830	118.10	51	145.80	68	173.90	26859
95.00	35133	118.80	331	147.80	121	174.90	2218
96.00	2347	127.85	284	149.80	115	175.90	25677
103.75	109	129.60	59	154.80	54	176.85	1703
104.00	99	129.90	78	156.60	76	207.00	136
104.90	104	133.10	66	160.60	126		

Instrument :

MSVOA_N

ClientSampleId :

BFB