


Naphthalene

Response Ratio

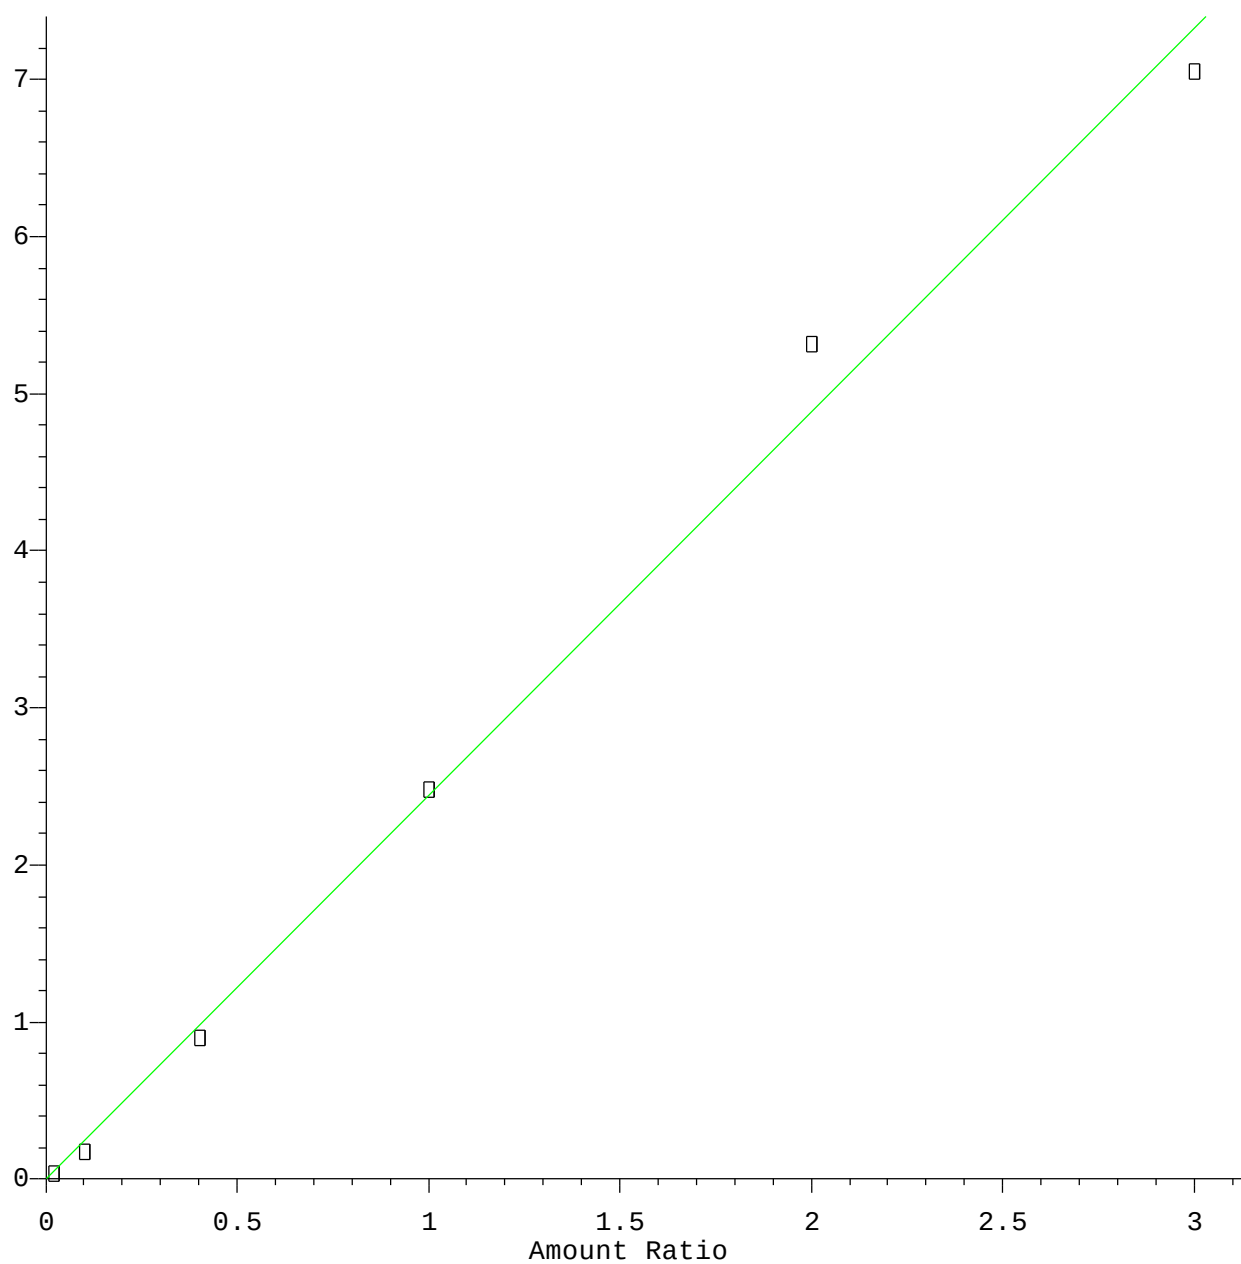


Resp Ratio = 2.44e+000 * Amt + 1.43e-003
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092719W.M
Calibration Table Last Updated: Mon Sep 30 08:07:38 2019


1,2,3-Trichlorobenzene

Response Ratio

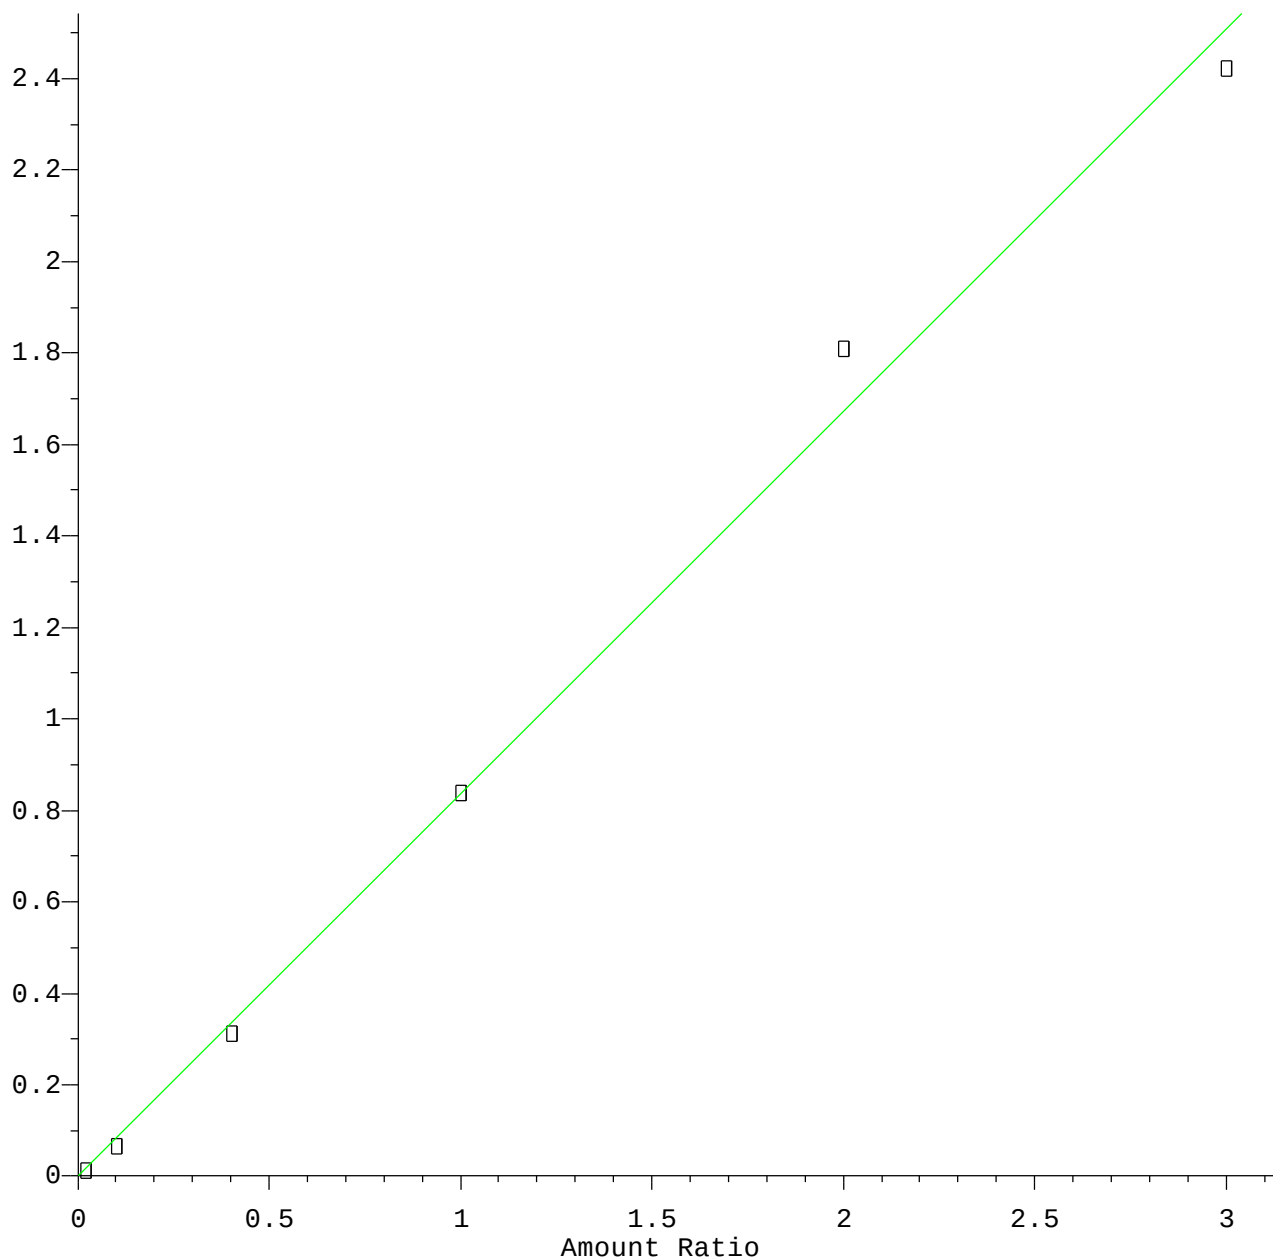


Resp Ratio = $8.36 \times 10^{-1} \times \text{Amt} + 4.23 \times 10^{-4}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092719W.M
Calibration Table Last Updated: Mon Sep 30 08:07:38 2019

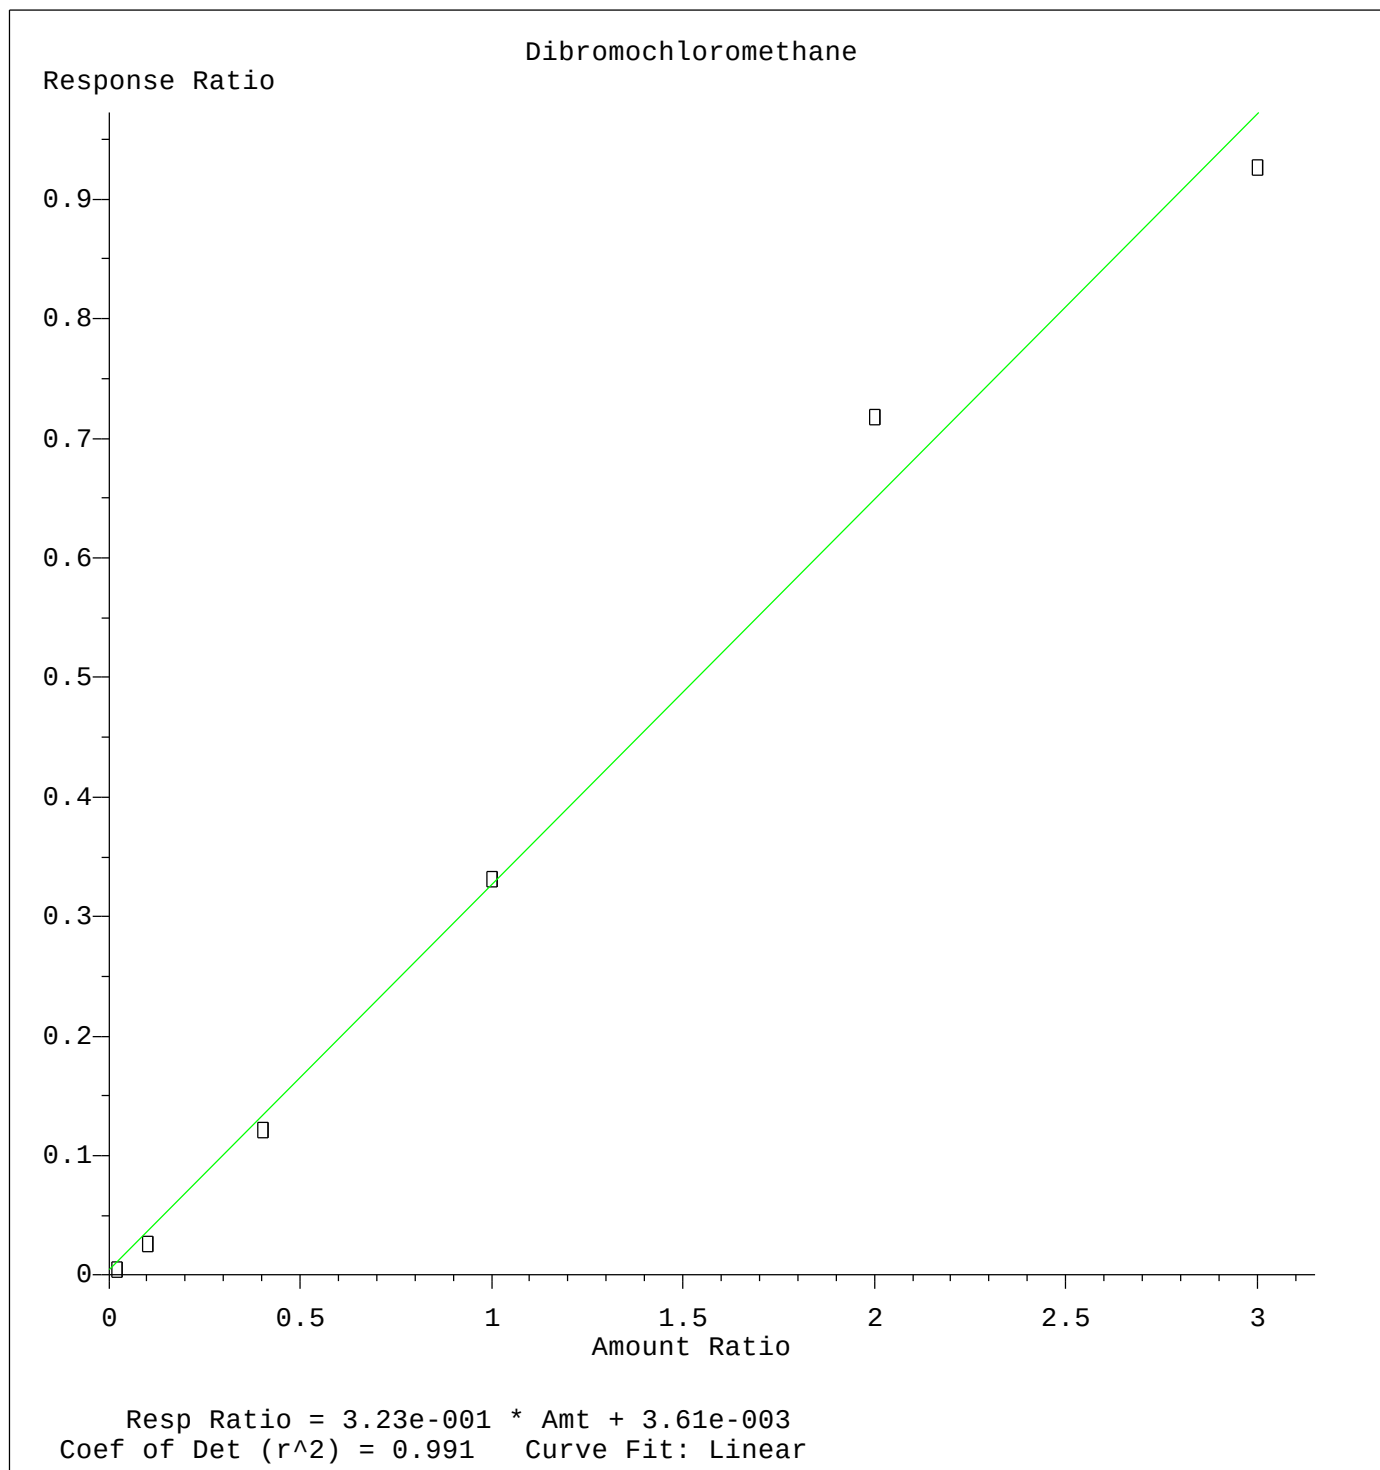

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092719W.M
Calibration Table Last Updated: Mon Sep 30 08:07:38 2019

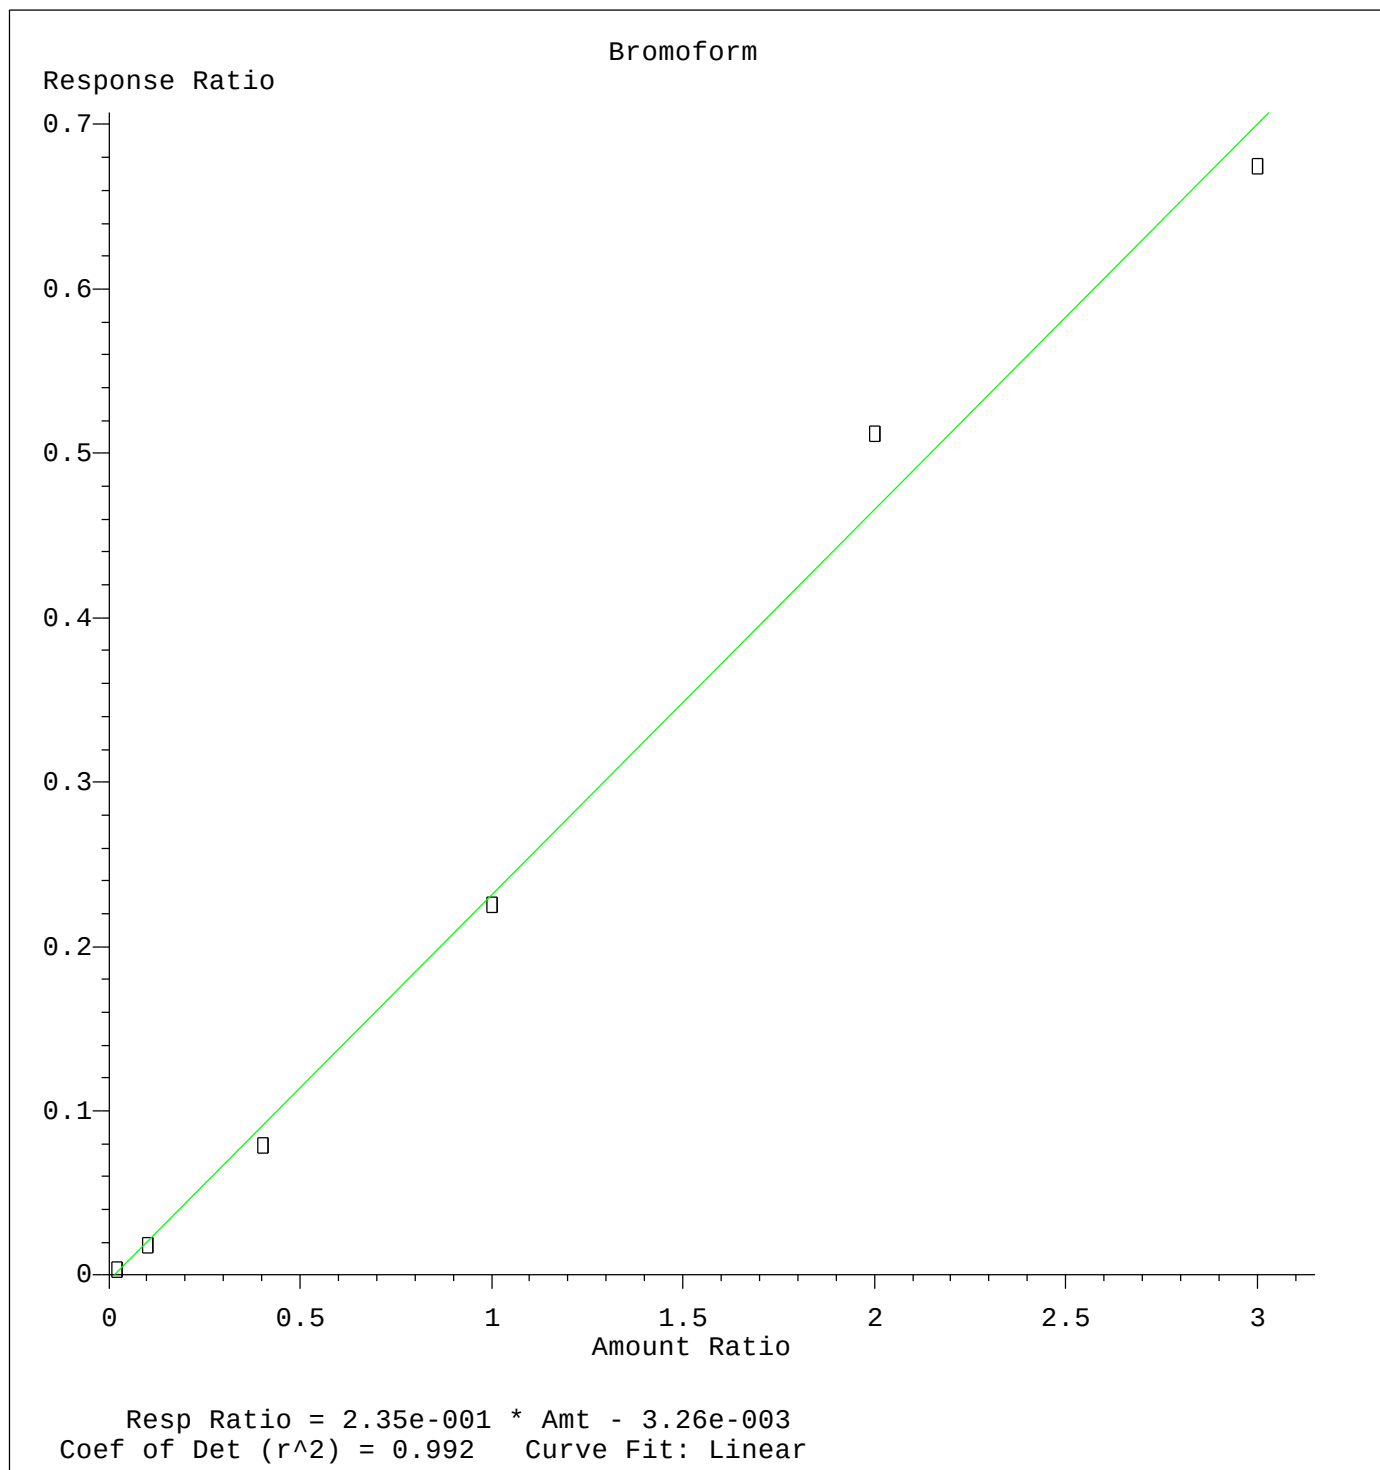

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092719W.M
Calibration Table Last Updated: Mon Sep 30 08:07:38 2019