


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN092719\
 Data File : VN058398.D
 Acq On : 27 Sep 2019 10:50
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092719W.M
 Title : SW846 8260
 Last Update : Mon Sep 30 08:07:38 2019

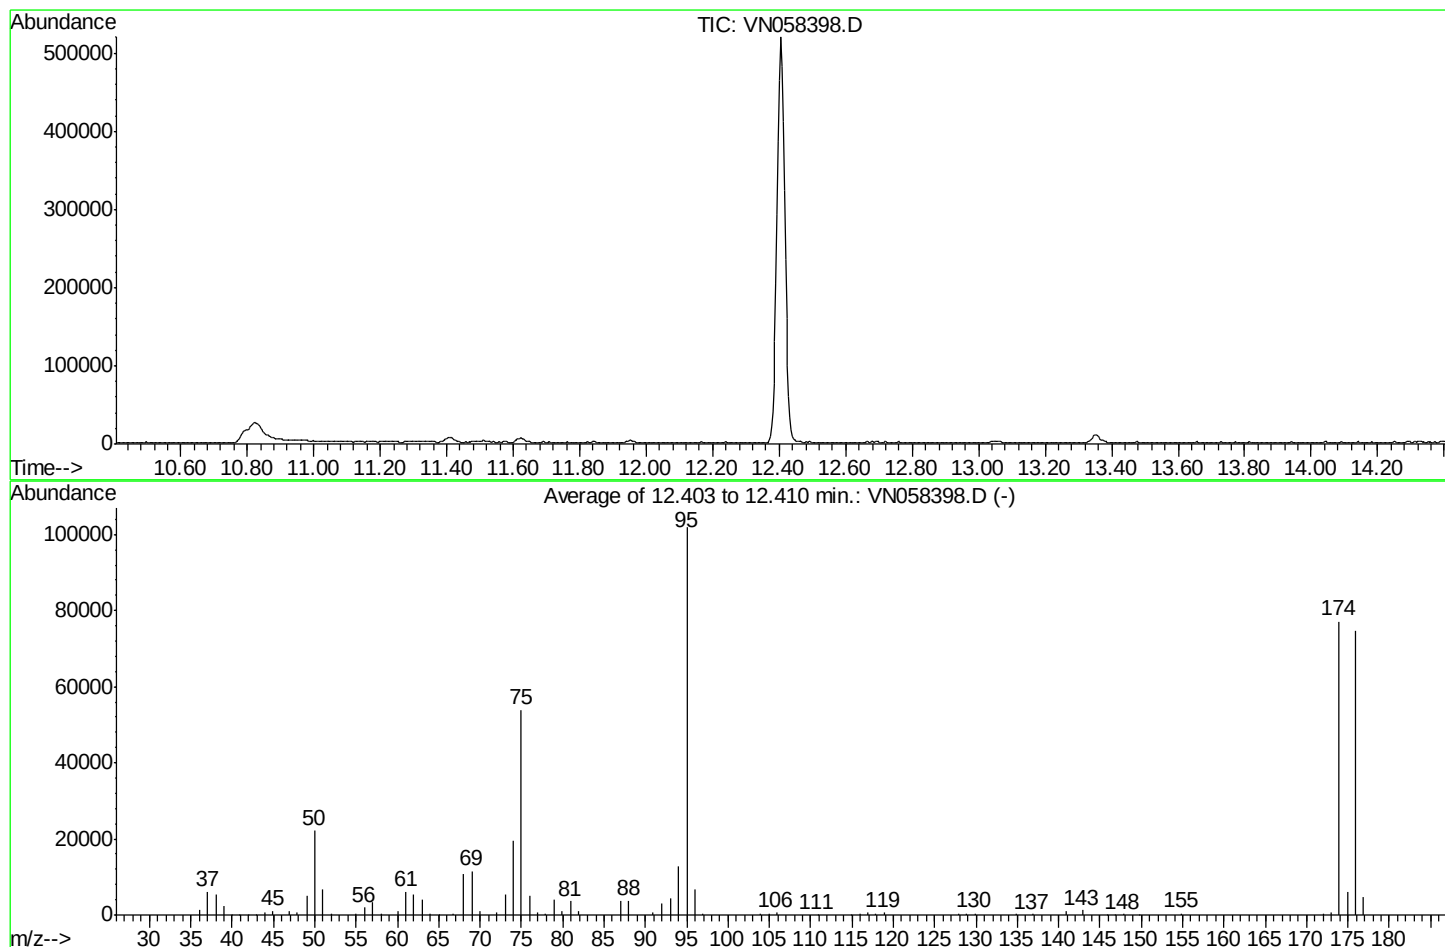

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	22157	PASS
75	95	30	60	53.0	53949	PASS
95	95	100	100	100.0	101877	PASS
96	95	5	9	6.5	6572	PASS
173	174	0.00	2	1.1	812	PASS
174	95	50	100	75.7	77109	PASS
175	174	5	9	8.1	6213	PASS
176	174	95	101	96.7	74576	PASS
177	176	5	9	6.3	4683	PASS