
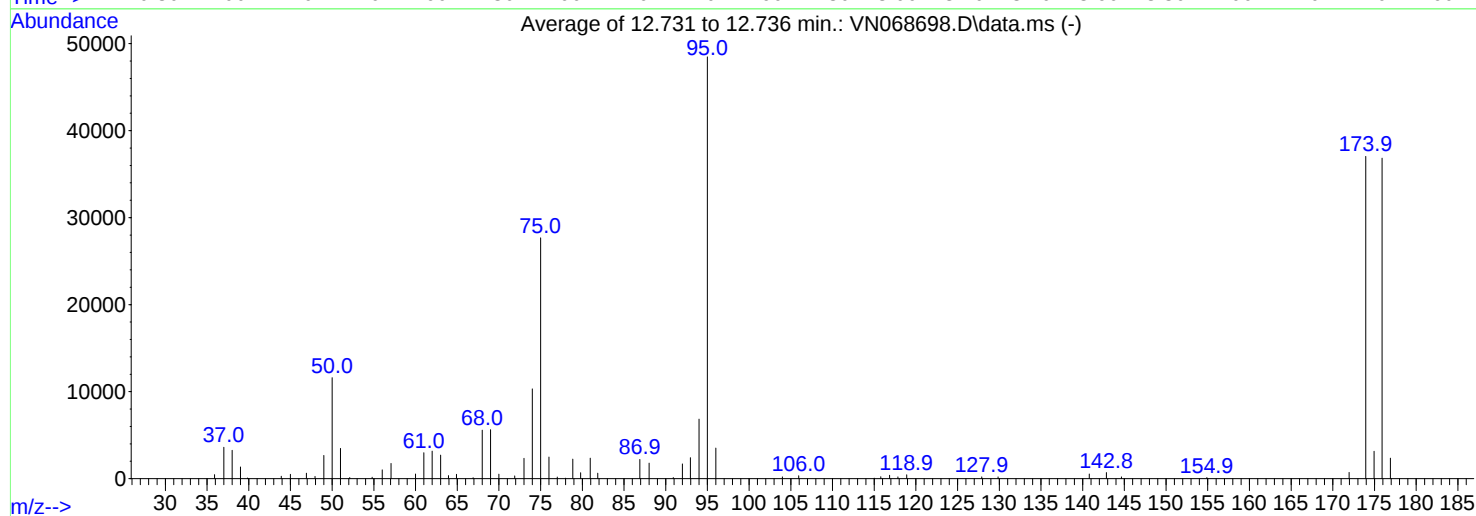


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092721\
 Data File : VN068698.D
 Acq On : 27 Sep 2021 11:28
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N092721W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Mon Sep 27 14:37:57 2021

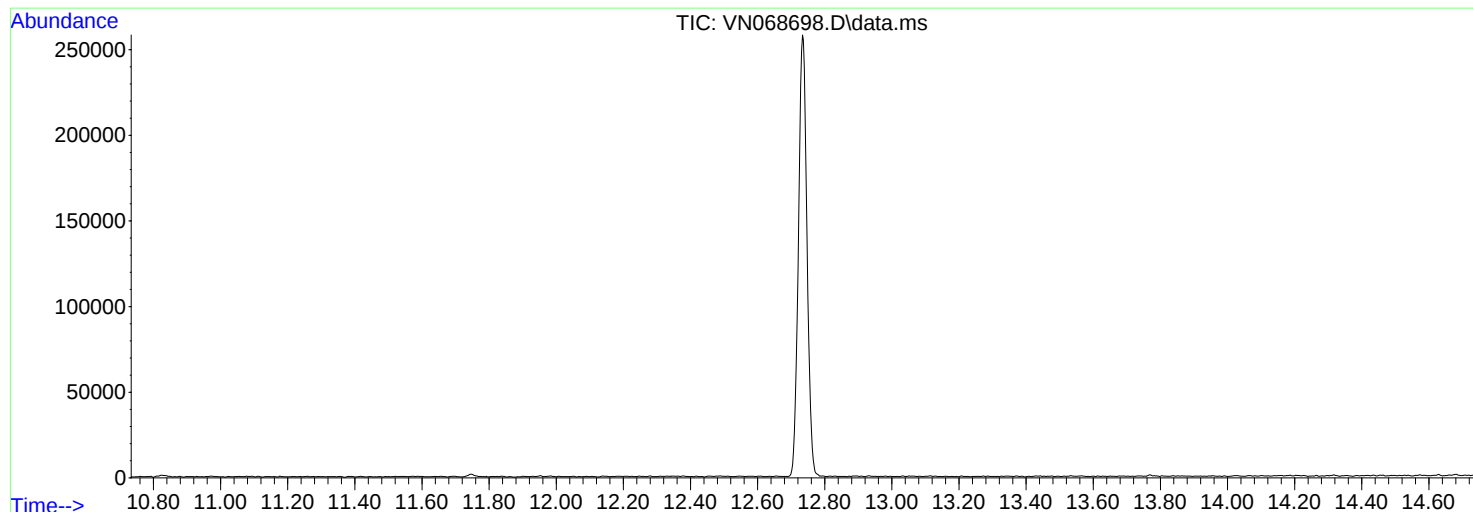

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3991

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.0	11612	PASS
75	95	30	60	57.1	27680	PASS
95	95	100	100	100.0	48483	PASS
96	95	5	9	7.3	3516	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	76.4	37048	PASS
175	174	5	9	8.5	3139	PASS
176	174	95	101	99.4	36832	PASS
177	176	5	9	6.4	2360	PASS