

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092722\
 Data File : VN074636.D
 Acq On : 27 Sep 2022 18:53
 Operator : JC\MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VIBLK

Quant Time: Sep 28 08:07:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N092722W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Wed Sep 28 07:48:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	7.498	128	95476	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	8.827	114	496927	30.000	ug/l	0.00
57) Chlorobenzene-d5	11.621	117	428373	30.000	ug/l	0.00
System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.286	65	278938	30.985	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	103.267%
60) 4-Bromofluorobenzene	12.604	95	194012	23.316	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	77.733%
63) Toluene-d8	10.310	98	750754	31.071	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	103.567%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092722\
Data File : VN074636.D
Acq On : 27 Sep 2022 18:53
Operator : JC\MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VIBLK

Quant Time: Sep 28 08:07:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N092722W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Wed Sep 28 07:48:31 2022
Response via : Initial Calibration

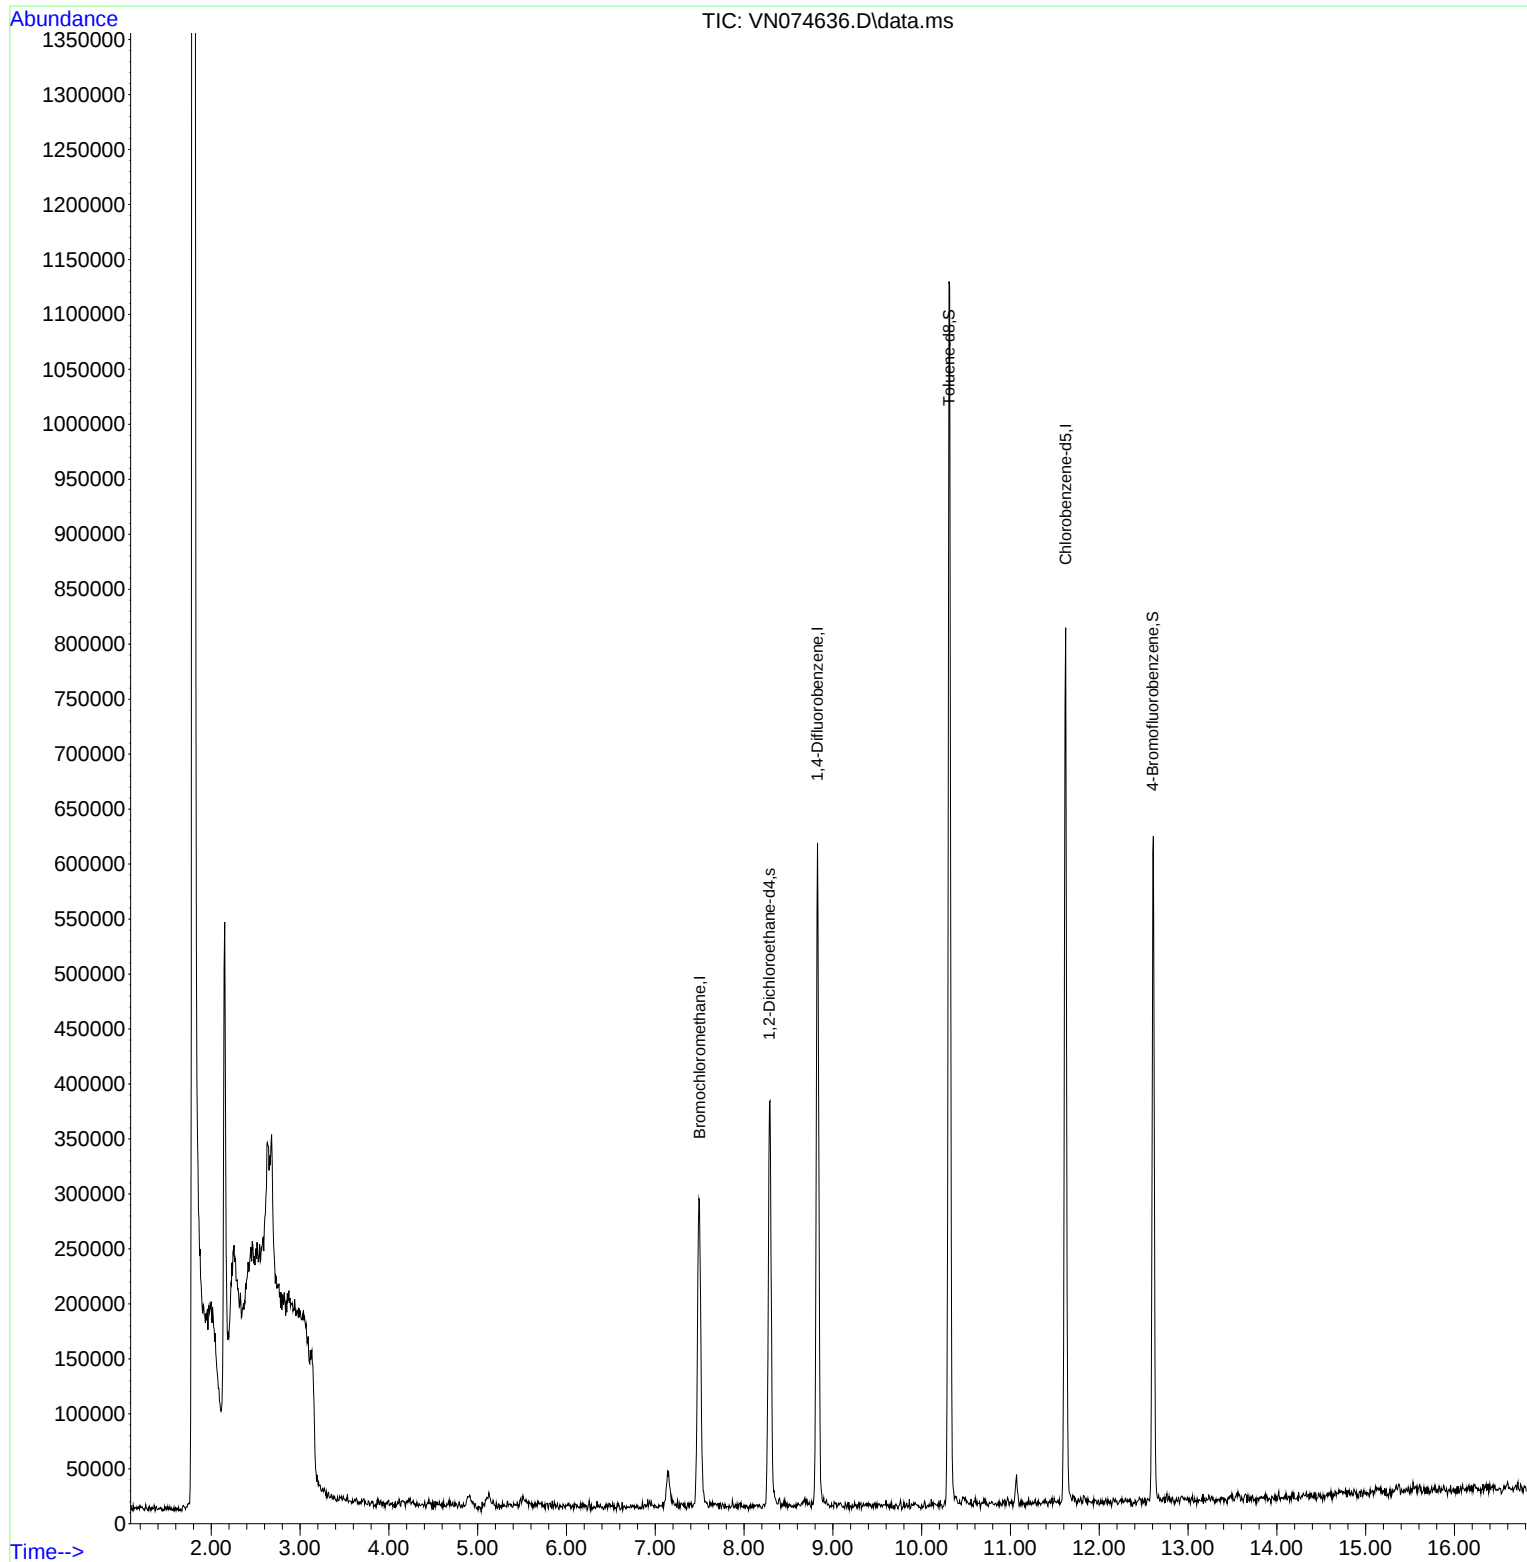

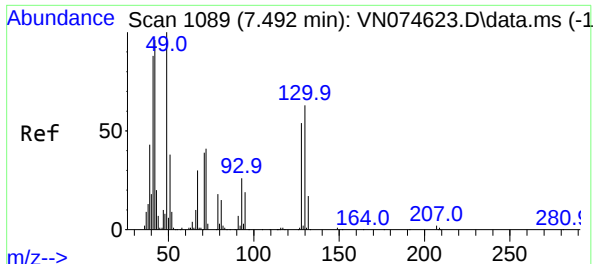

#1

Bromochloromethane

Concen: 30.000 ug/l

RT: 7.498 min Scan# 1089

Delta R.T. 0.006 min

Lab File: VN074636.D

Acq: 27 Sep 2022 18:53

Instrument :

MSVOA_N

ClientSampleId :

VIBLK





Tgt Ion:128 Resp: 95476

Ion Ratio Lower Upper

128 100

49 203.6 0.0 492.0

130 124.2 0.0 313.3

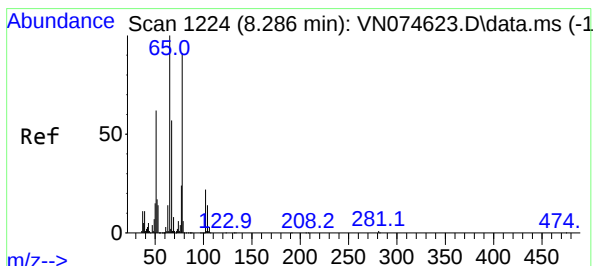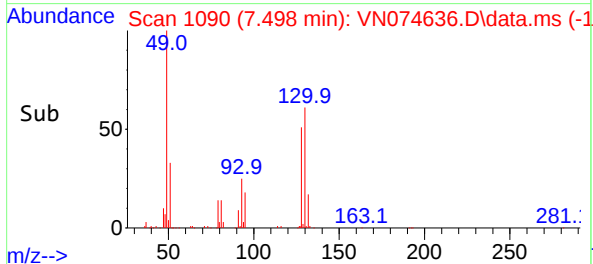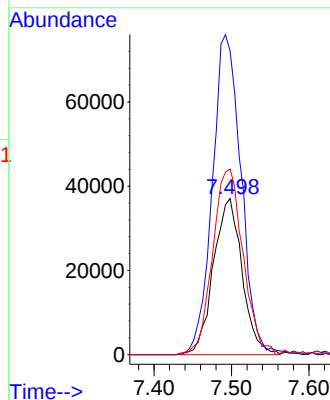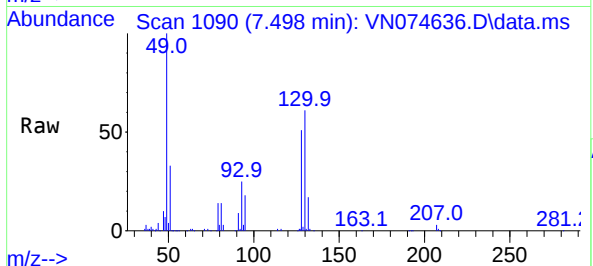

#27

1,2-Dichloroethane-d4

Concen: 30.985 ug/l

RT: 8.286 min Scan# 1224

Delta R.T. -0.000 min

Lab File: VN074636.D




Acq: 27 Sep 2022 18:53


Tgt Ion: 65 Resp: 278938

Ion Ratio Lower Upper

65 100

67 53.4 45.2 67.8


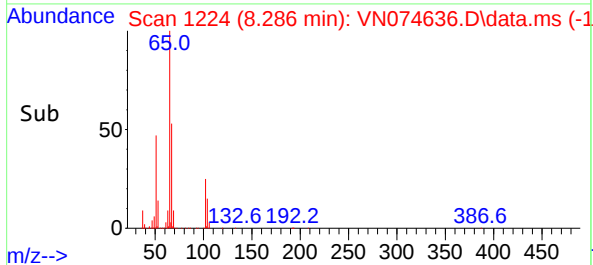
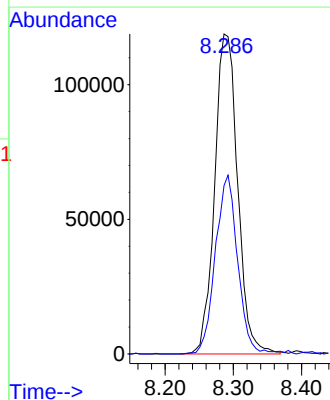
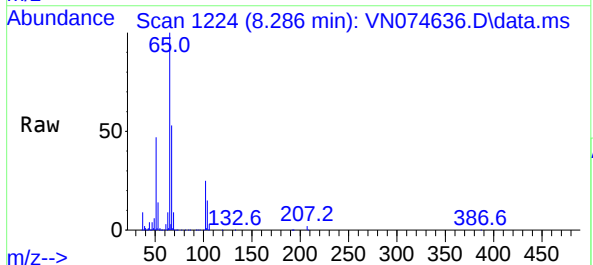


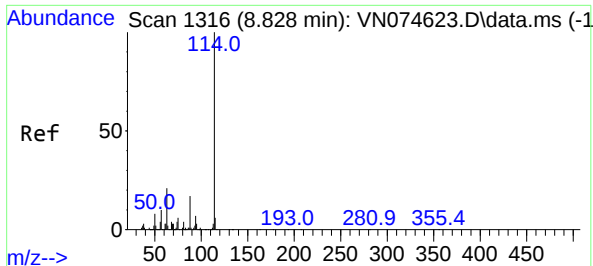

#28
1,4-Difluorobenzene
Concen: 30.000 ug/l
RT: 8.827 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN074636.D
Acq: 27 Sep 2022 18:53




Instrument :
MSVOA_N
ClientSampleId :
VIBLK


Tgt Ion:114 Resp: 496927
Ion Ratio Lower Upper
114 100
63 22.1 16.6 25.0
88 15.0 12.2 18.4

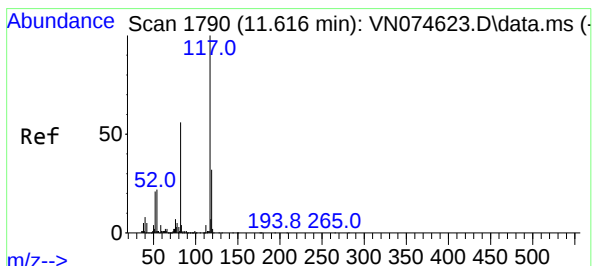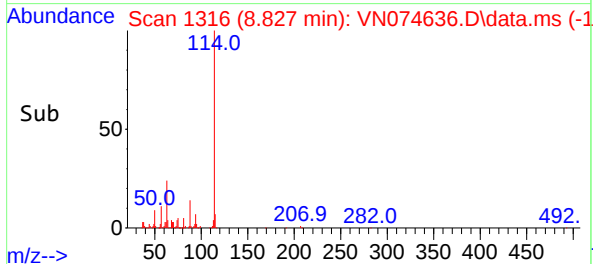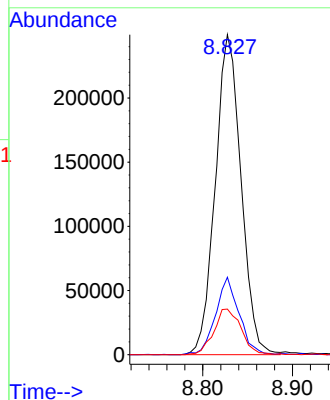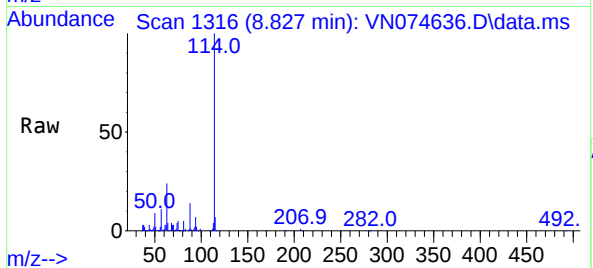

#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 11.621 min Scan# 1791
Delta R.T. 0.006 min
Lab File: VN074636.D
Acq: 27 Sep 2022 18:53

Tgt Ion:117 Resp: 428373
Ion Ratio Lower Upper
117 100
82 56.2 44.6 67.0
119 32.3 25.6 38.4


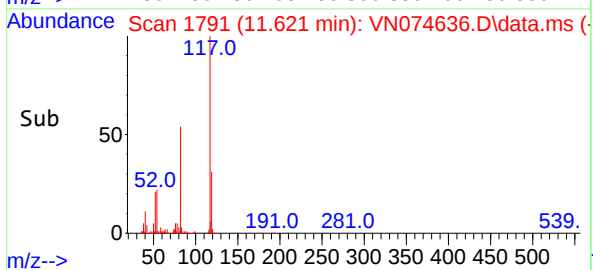
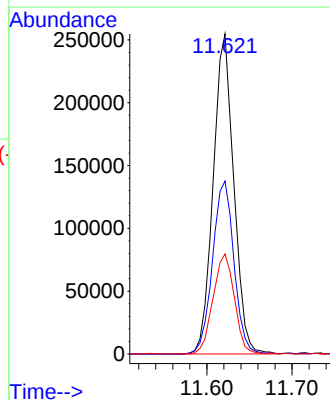
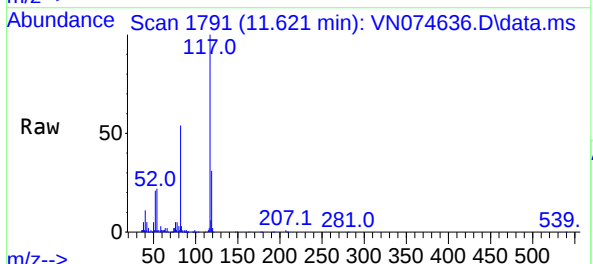


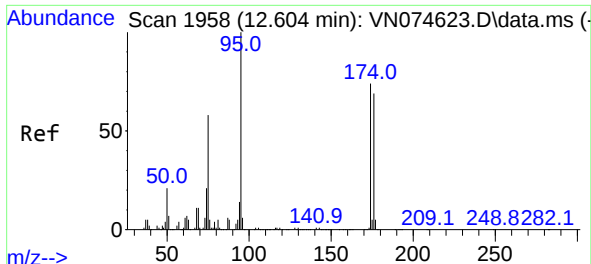

#60
4-Bromofluorobenzene
Concen: 23.316 ug/l
RT: 12.604 min Scan# 1958
Delta R.T. -0.000 min
Lab File: VN074636.D
Acq: 27 Sep 2022 18:53

Instrument :
MSVOA_N
ClientSampleId :
VIBLK

Tgt Ion: 95 Resp: 194012
Ion Ratio Lower Upper
95 100
174 74.1 57.8 86.8
176 72.6 57.0 85.4

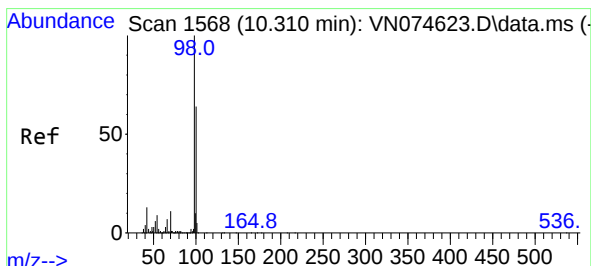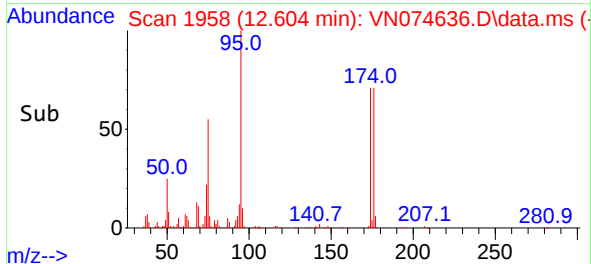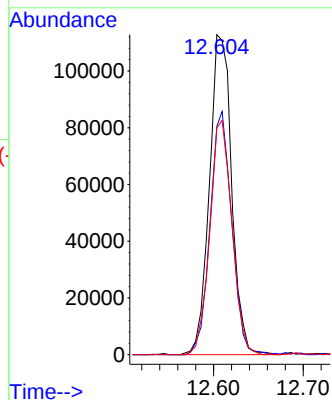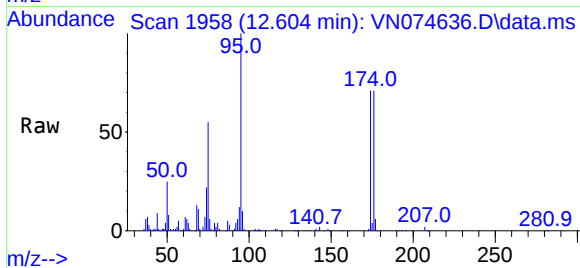

#63
Toluene-d8
Concen: 31.071 ug/l
RT: 10.310 min Scan# 1568
Delta R.T. -0.000 min
Lab File: VN074636.D
Acq: 27 Sep 2022 18:53

Tgt Ion: 98 Resp: 750754
Ion Ratio Lower Upper
98 100
100 64.0 52.7 79.1

