


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092722\
 Data File : VN074621.D
 Acq On : 27 Sep 2022 10:13
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090622W.M
 Title : SW846 8260
 Last Update : Wed Sep 07 04:58:13 2022

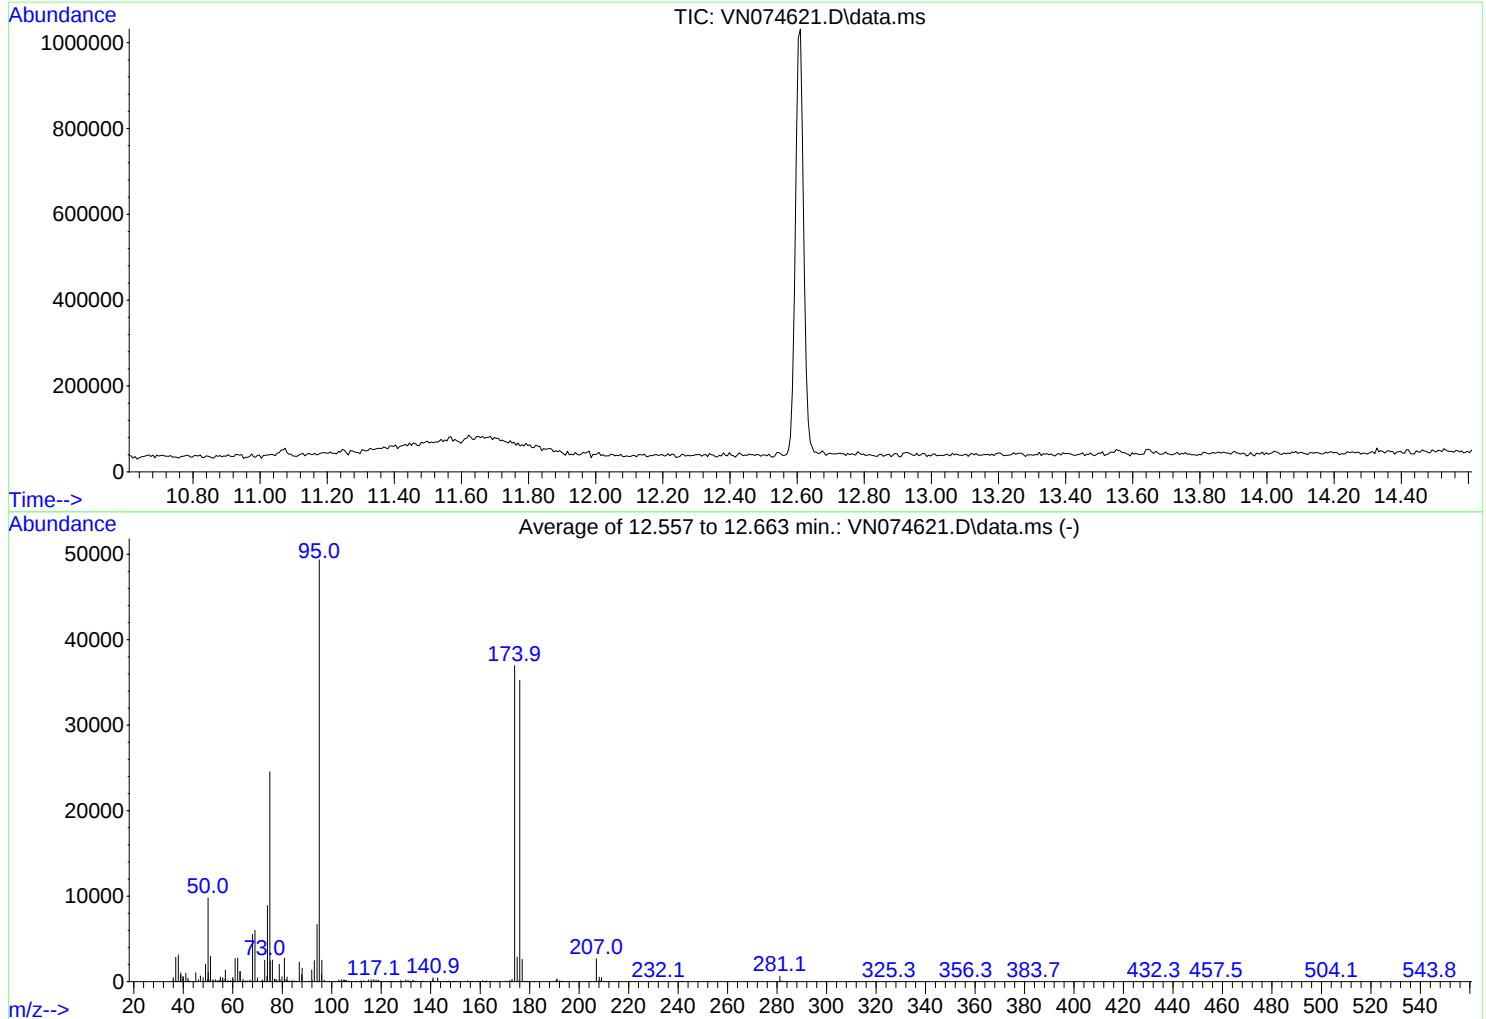

AutoFind: Averaged scan 1814 to 1832; Bkg corrected with scan 1813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	9791	PASS
75	95	30	60	49.7	24548	PASS
95	95	100	100	100.0	49349	PASS
96	95	5	9	5.1	2506	PASS
173	174	0.00	2	0.7	256	PASS
174	95	50	100	74.9	36961	PASS
175	174	5	9	7.8	2873	PASS
176	174	95	101	95.4	35248	PASS
177	176	5	9	7.4	2607	PASS