
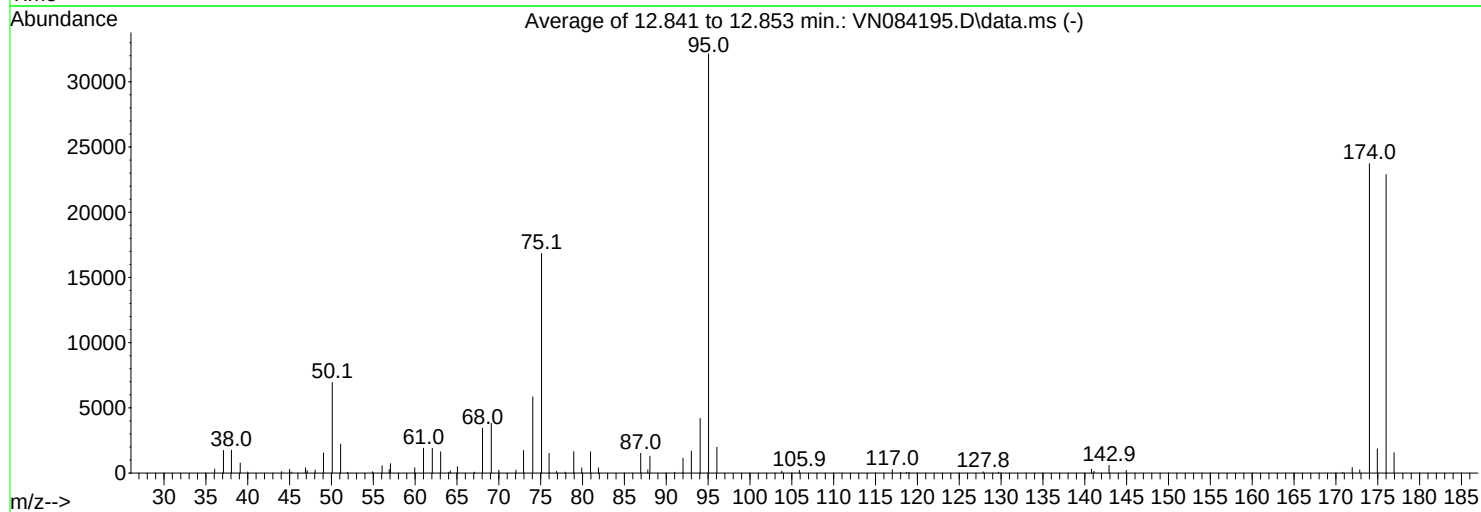


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092724\
Data File : VN084195.D
Acq On : 27 Sep 2024 09:21
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091024W.M
Title : SW846 8260
Last Update : Wed Sep 11 15:18:56 2024

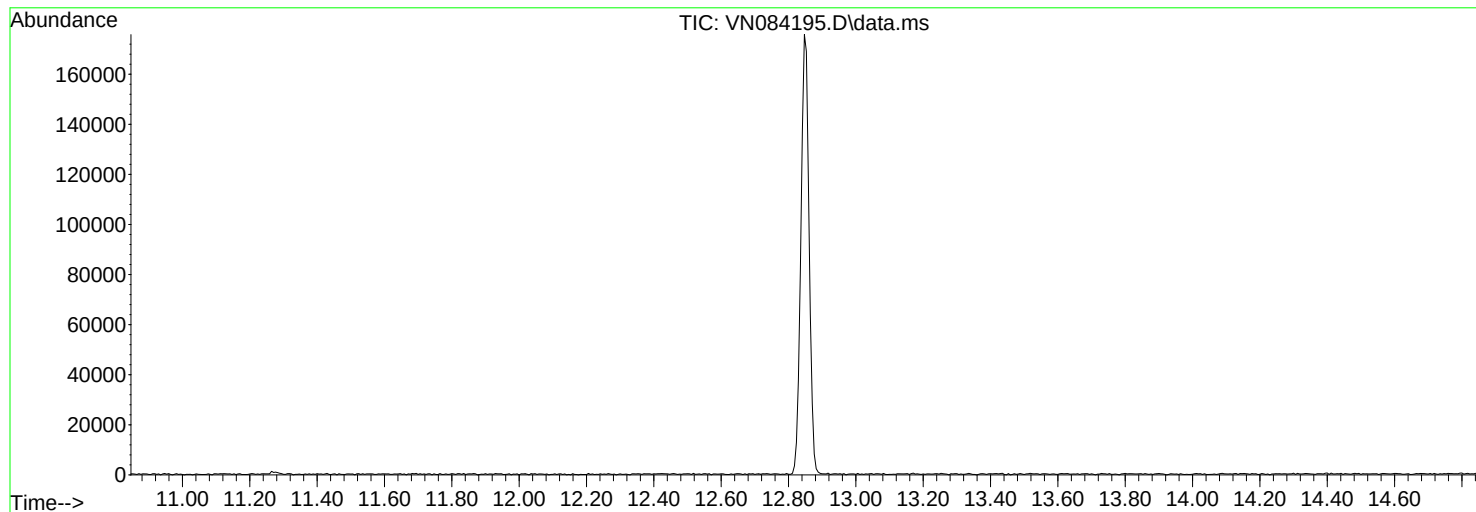

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	6941	PASS
75	95	30	60	52.4	16843	PASS
95	95	100	100	100.0	32152	PASS
96	95	5	9	6.2	1978	PASS
173	174	0.00	2	1.0	242	PASS
174	95	50	100	73.8	23720	PASS
175	174	5	9	7.9	1867	PASS
176	174	95	101	96.5	22893	PASS
177	176	5	9	6.8	1560	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	305	49.05	1552	63.05	1632	75.10	16843
37.10	1737	50.10	6941	64.00	61	76.00	1509
38.05	1765	51.10	2224	64.20	167	76.90	131
39.10	774	51.90	60	65.05	484	77.90	78
40.00	84	54.90	105	67.10	72	78.95	1650
44.05	113	56.05	559	68.05	3444	79.90	398
45.00	289	56.90	274	69.10	3804	80.95	1629
45.20	76	57.05	720	70.00	233	81.90	396
46.90	406	59.95	411	72.05	230	86.95	1519
47.10	203	61.00	1904	72.95	1735	87.80	251
48.05	234	62.05	1897	74.05	5847	88.05	1296

Average of 12.841 to 12.853 min.: VN084195.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
91.00	59	119.00	59	174.95	1867		
92.00	1145	127.85	105	176.00	22893		
93.00	1687	129.70	70	176.95	1560		
94.05	4191	140.80	294				
95.05	32152	141.10	142				
96.05	1978	142.90	595				
103.80	156	144.95	212				
105.90	212	170.80	55				
117.00	266	171.95	427				
118.00	58	172.85	242				
118.70	54	174.00	23720				

Instrument :

MSVOA_N

ClientSampleId :

BFB