


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN092818\
Data File : VN051606.D
Acq On : 28 Sep 2018 7:42
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N092818W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Sat Sep 29 01:07:29 2018

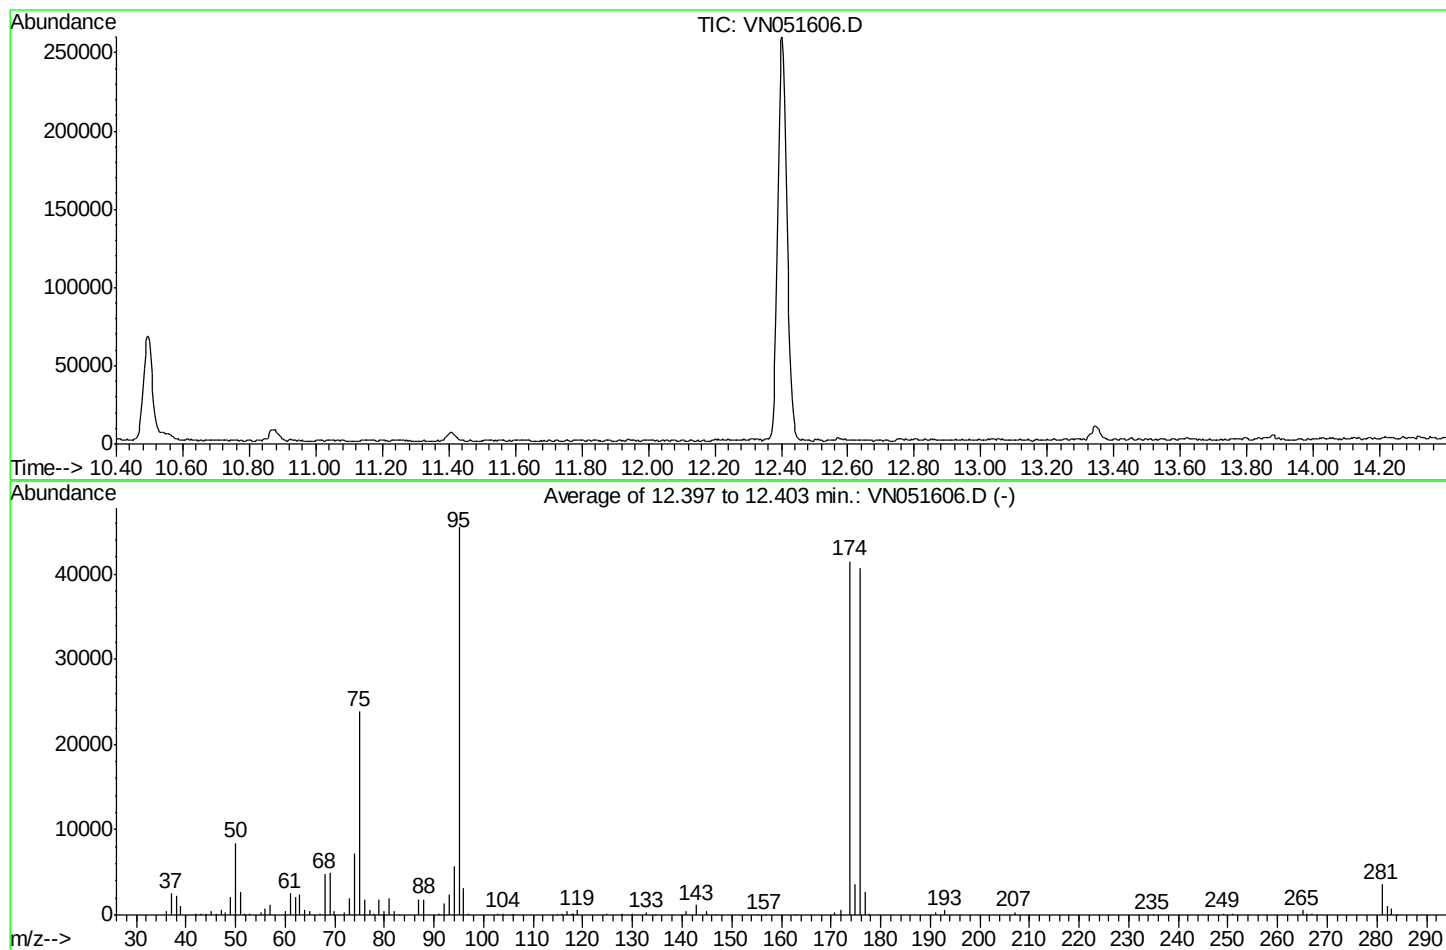

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	8424	PASS
75	95	30	60	52.5	23853	PASS
95	95	100	100	100.0	45477	PASS
96	95	5	9	6.9	3117	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	91.2	41461	PASS
175	174	5	9	8.5	3537	PASS
176	174	95	101	98.3	40754	PASS
177	176	5	9	6.8	2769	PASS