

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN092820\
 Data File : VN063700.D
 Acq On : 28 Sep 2020 13:04
 Operator : JC/MD
 Sample : VN0928WBL01
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0928WBL01

Quant Time: Sep 29 00:38:50 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN092820\
Data File : VN063700.D
Acq On : 28 Sep 2020 13:04
Operator : JC/MD
Sample : VN0928WBL01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0928WBL01


Quant Time: Sep 29 00:38:50 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82




#1

Pentafluorobenzene

Concen: 50.000 ug/l

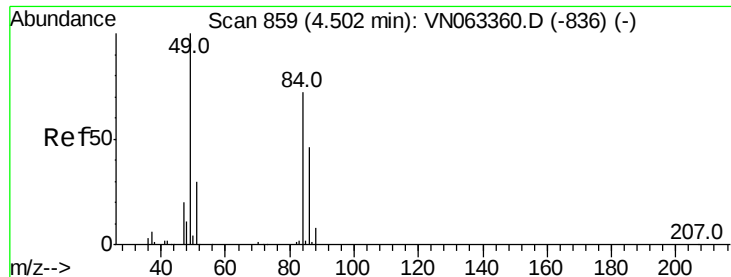


#20
Methylene Chloride
Concen: 0.273 ug/l
RT: 4.51 min Scan# 860
Delta R.T. 0.00 min
Lab File: VN063700.D
Acq: 28 Sep 2020 13:04

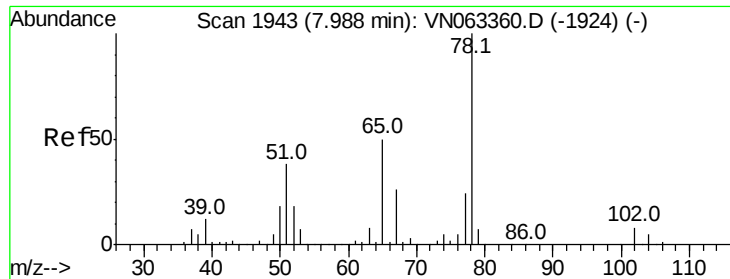

#33
 1,2-Dichloroethane-d4
 Concen: 51.239 ug/l
 RT: 7.99 min Scan# 1943
 Delta R.T. -0.00 min
 Lab File: VN063700.D
 Acq: 28 Sep 2020 13:04


Instrument

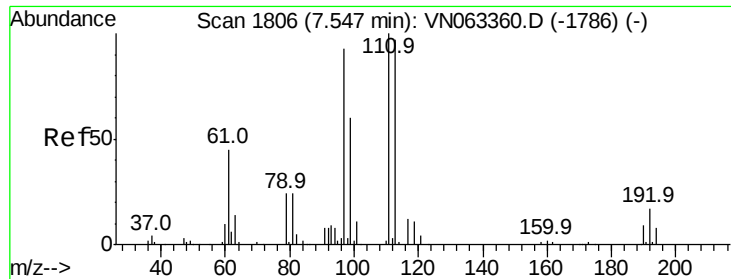

#35

Dibromofluoromethane

Concen: 49

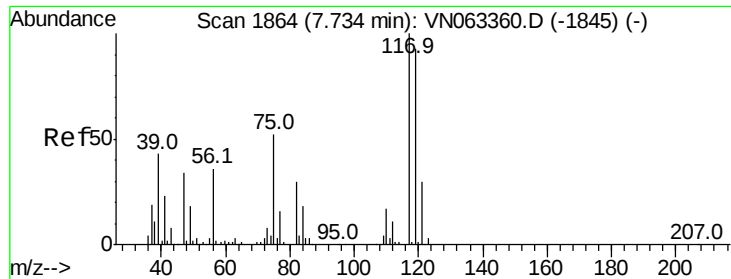


#38

Carbon Tetrachloride

Concen: 5.568 ug/l

RT: 7.63 min Scan

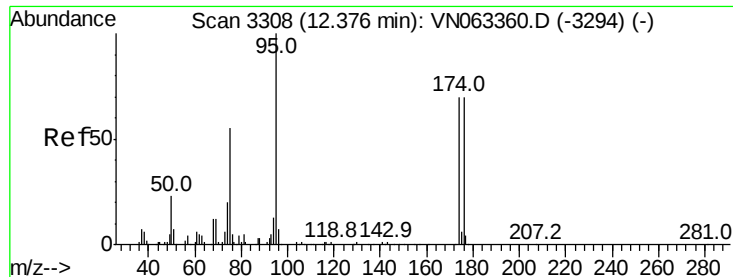


#62

4-Bromofluorobenzene

Concen: 52.477 ug/l

RT: 12.38 min Scan# 3308

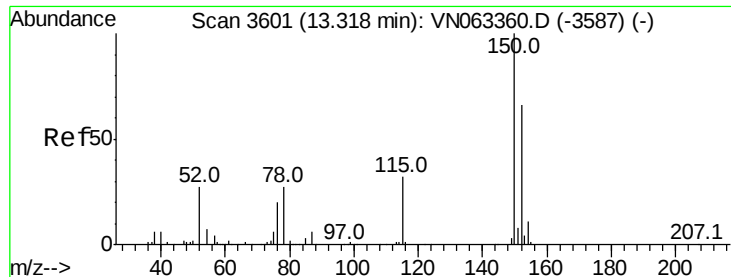


#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 1

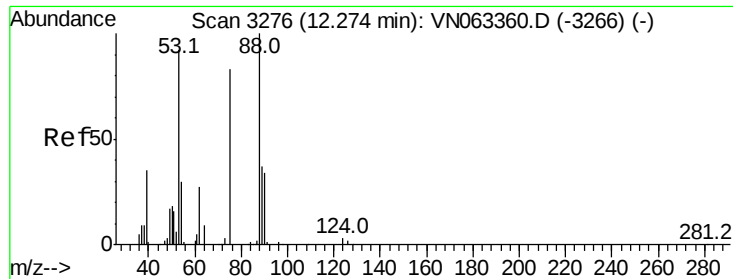

#81

trans-1,4-Dichloro-2-butene

Concen: 74.663 ug/l