


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN092820\
Data File : VN063697.D
Acq On : 28 Sep 2020 10:56
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091620W.M
Title : SW846 8260
Last Update : Wed Sep 16 13:05:20 2020

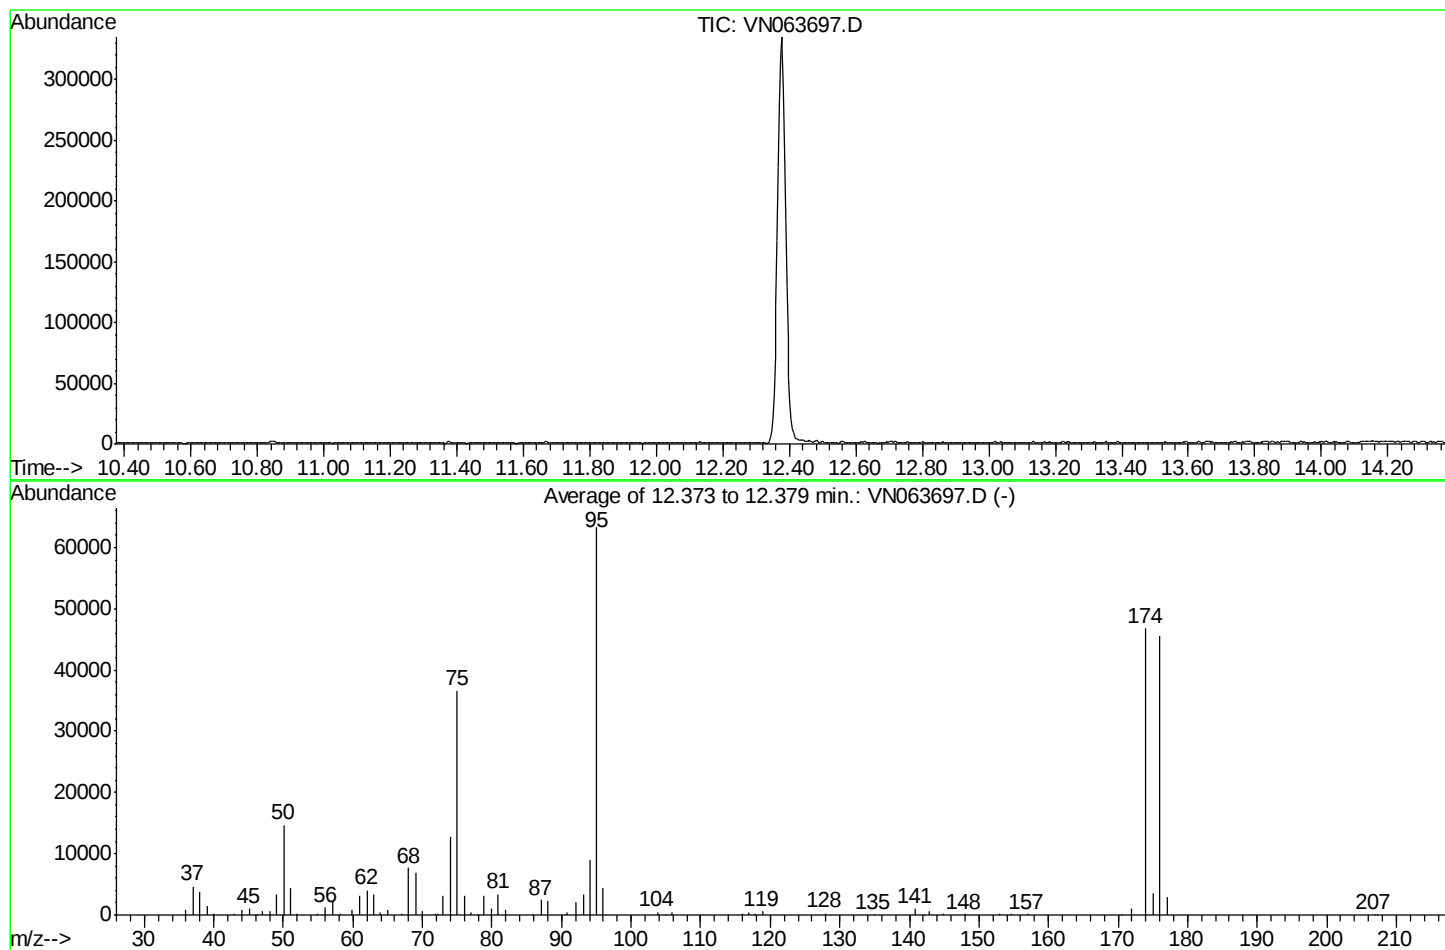

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	14660	PASS
75	95	30	60	57.9	36624	PASS
95	95	100	100	100.0	63301	PASS
96	95	5	9	7.0	4423	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	73.9	46789	PASS
175	174	5	9	7.7	3589	PASS
176	174	95	101	97.2	45482	PASS
177	176	5	9	6.4	2891	PASS