
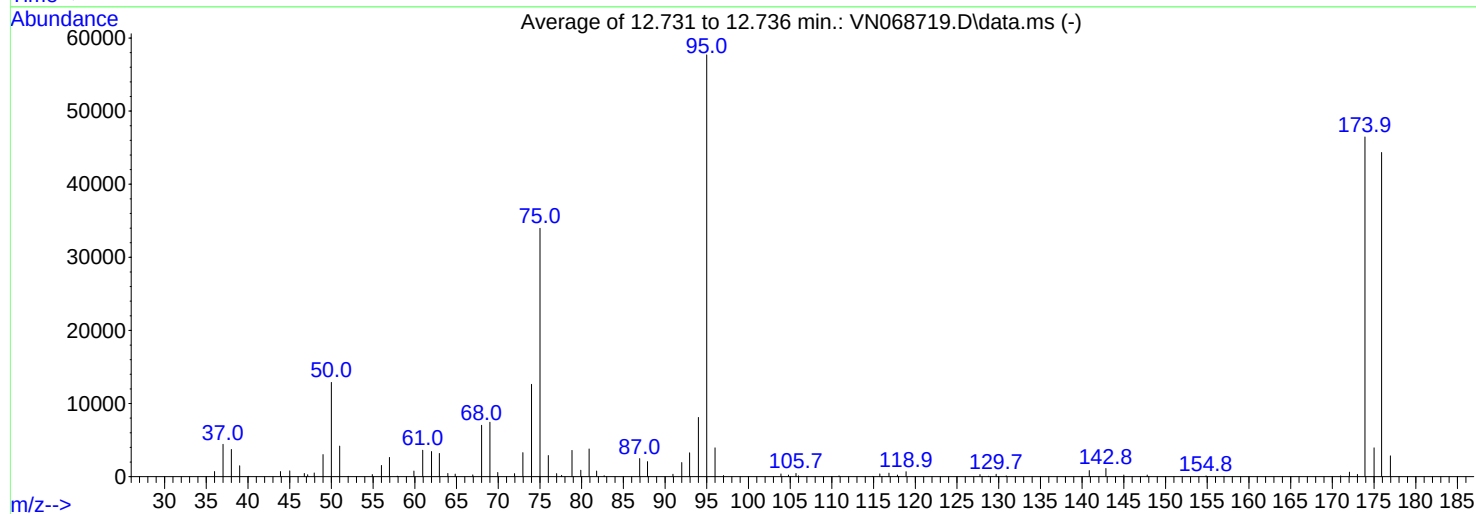


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092821\
 Data File : VN068719.D
 Acq On : 28 Sep 2021 14:13
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N092821W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Wed Sep 29 08:56:32 2021

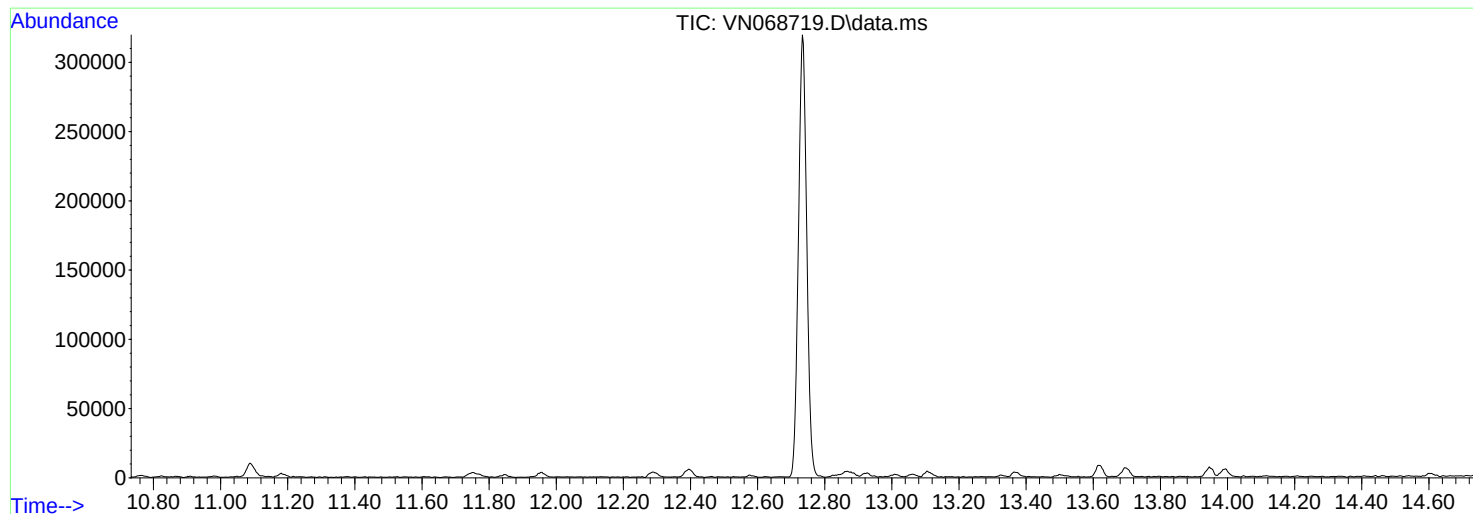

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3990

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	12892	PASS
75	95	30	60	58.9	33968	PASS
95	95	100	100	100.0	57696	PASS
96	95	5	9	6.8	3939	PASS
173	174	0.00	2	0.7	303	PASS
174	95	50	100	80.5	46456	PASS
175	174	5	9	8.5	3934	PASS
176	174	95	101	95.5	44352	PASS
177	176	5	9	6.4	2840	PASS