
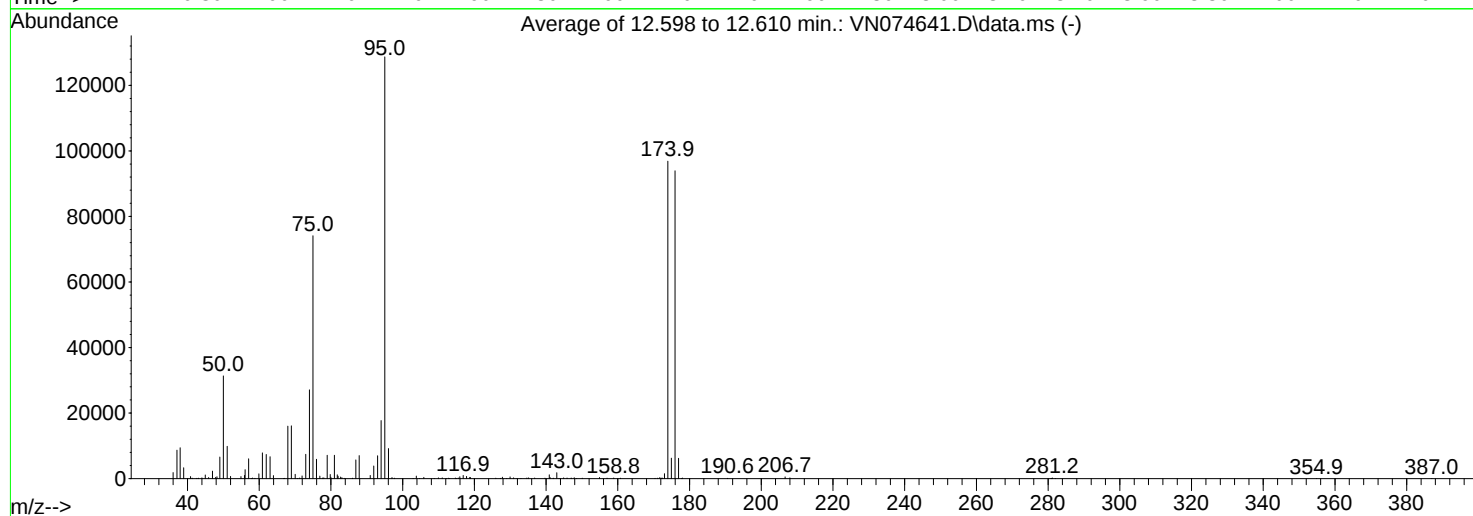


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092822\
 Data File : VN074641.D
 Acq On : 28 Sep 2022 09:58
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N092722W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Wed Sep 28 07:48:31 2022

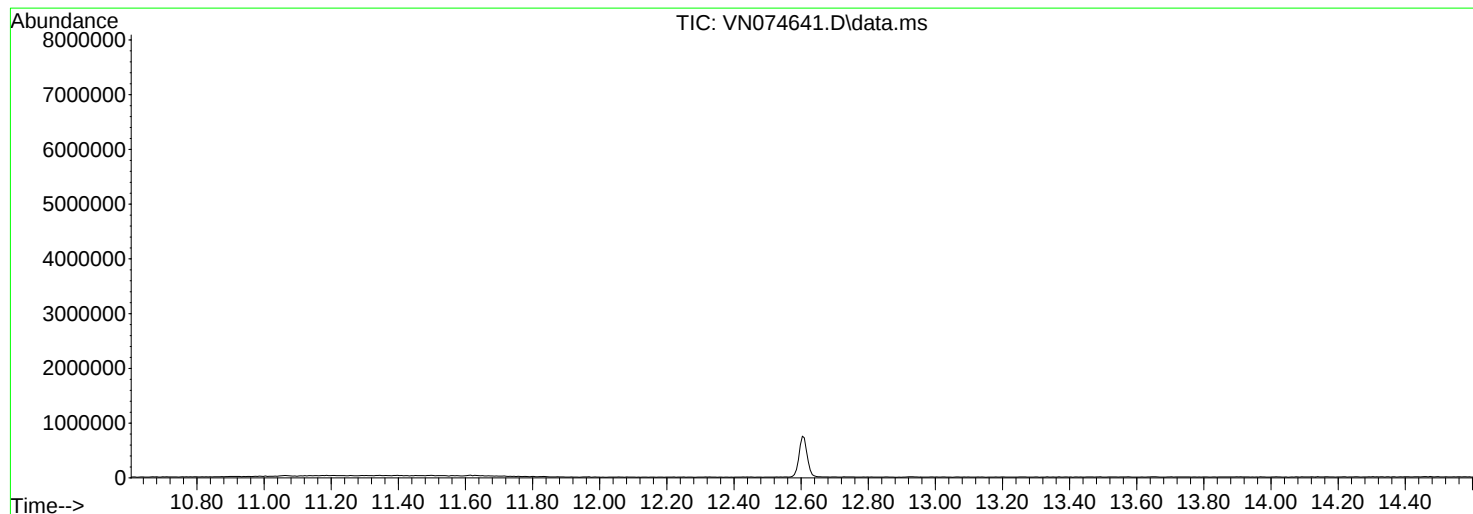

AutoFind: Scans 1957, 1958, 1959; Background Corrected with Scan 1949

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.3	31333	PASS
75	95	30	60	57.6	74128	PASS
95	95	100	100	100.0	128693	PASS
96	95	5	9	7.1	9178	PASS
173	174	0.00	2	1.6	1532	PASS
174	95	50	100	75.3	96861	PASS
175	174	5	9	6.5	6253	PASS
176	174	95	101	96.9	93904	PASS
177	176	5	9	6.6	6229	PASS