

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092823\
 Data File : VN079364.D
 Acq On : 28 Sep 2023 10:30
 Operator : JC\MD
 Sample : VN0928WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Sep 29 04:31:51 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091123W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 12 05:05:24 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	8.229	168	151459	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	277525	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	237336	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	69475	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	122294	59.815	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 119.620%	
35) Dibromofluoromethane	8.171	113	96122	52.069	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 104.140%	
50) Toluene-d8	10.570	98	308580	45.524	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 91.040%	
62) 4-Bromofluorobenzene	12.853	95	96929	44.829	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 89.660%	
Target Compounds						Qvalue
5) Bromomethane	2.965	94	743	0.603	ug/l #	51
6) Chloroethane	3.142	64	348	Below Cal	#	43
11) Tert butyl alcohol	5.500	59	924	2.448	ug/l #	72
15) Acrylonitrile	5.724	53	412	0.421	ug/l #	39
16) Acetone	4.441	43	681	0.784	ug/l #	40
17) Carbon Disulfide	4.706	76	1597	0.316	ug/l #	75
20) Methylene Chloride	5.283	84	860	0.407	ug/l #	51
25) 2-Butanone	7.494	43	429	0.341	ug/l #	37
31) Cyclohexane	8.229	56	4250	1.424	ug/l #	58
36) 1,1-Dichloropropene	8.224	75	13206	4.641	ug/l #	47
38) Carbon Tetrachloride	8.224	117	16166	5.490	ug/l #	16
43) Isopropyl Acetate	8.759	43	1438	0.311	ug/l #	49
51) 4-Methyl-2-Pentanone	10.447	43	1043	0.388	ug/l #	76
58) 2-Chloroethyl Vinyl ether	10.165	63	156	Below Cal	#	42
59) 2-Hexanone	11.212	43	2144	1.101	ug/l	76
74) N-amyl acetate	12.494	43	908	0.379	ug/l #	56
75) 1,1,2,2-Tetrachloroethane	12.947	83	644	0.274	ug/l #	63
76) 1,2,3-Trichloropropane	12.853	75	54362	29.033	ug/l #	1
79) 2-Chlorotoluene	13.229	91	1334	0.287	ug/l	76
81) trans-1,4-Dichloro-2-b...	12.853	75	54362	79.817	ug/l #	15
82) 4-Chlorotoluene	13.229	91	1334	0.306	ug/l	75
87) 1,3-Dichlorobenzene	13.735	146	1059	0.403	ug/l	85
88) 1,4-Dichlorobenzene	13.735	146	1059	0.399	ug/l	87
89) n-Butylbenzene	14.059	91	1874	0.497	ug/l #	87
91) 1,2-Dichlorobenzene	14.117	146	1171	0.452	ug/l	78
92) 1,2-Dibromo-3-Chloropr...	14.711	75	157	0.439	ug/l	69
93) 1,2,4-Trichlorobenzene	15.400	180	1134	1.218	ug/l #	79
94) Hexachlorobutadiene	15.511	225	591	0.807	ug/l	75
95) Naphthalene	15.658	128	3834	1.386	ug/l #	94
96) 1,2,3-Trichlorobenzene	15.852	180	1635	1.488	ug/l	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092823\
Data File : VN079364.D
Acq On : 28 Sep 2023 10:30
Operator : JC\MD
Sample : VN0928WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :


Quant Time: Sep 29 04:31:51 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091123W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 12 05:05:24 2023
Response via : Initial Calibration

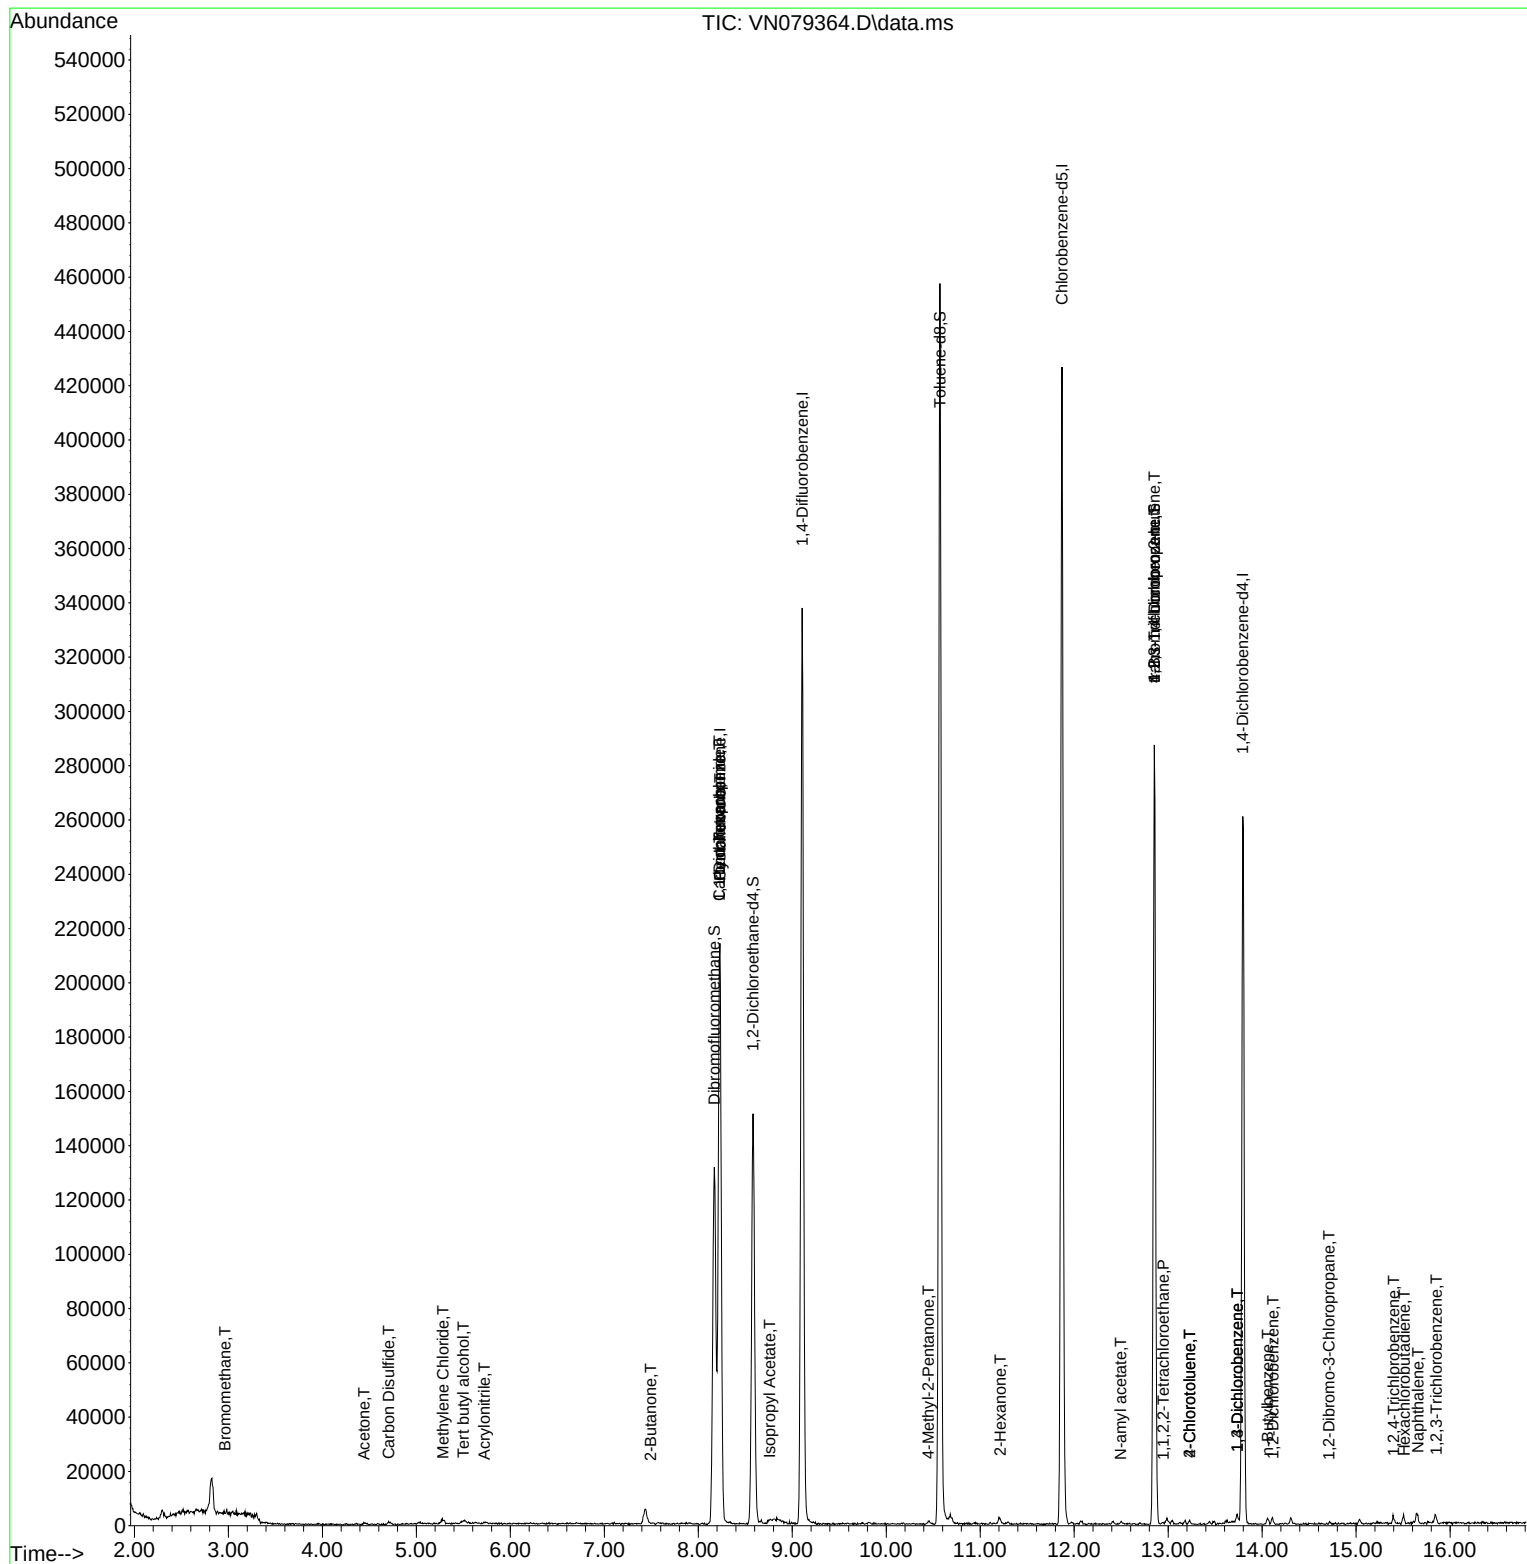



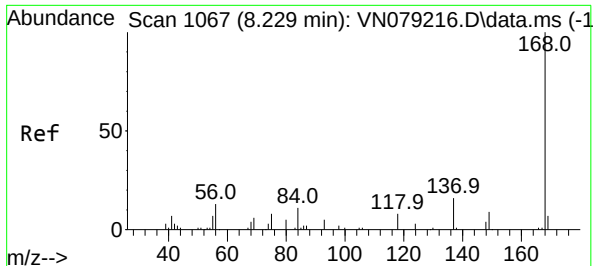


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.229 min Scan# 1067
Delta R.T. -0.001 min
Lab File: VN079364.D
Acq: 28 Sep 2023 10:30

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:168 Resp: 151459
Ion Ratio Lower Upper
168 100
99 60.3 53.0 79.6

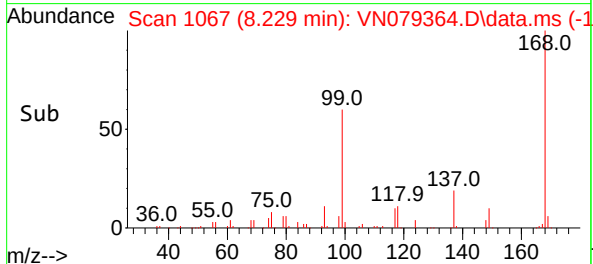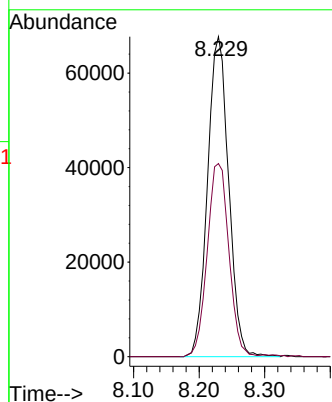

#5
Bromomethane
Concen: 0.603 ug/l
RT: 2.965 min Scan# 172
Delta R.T. 0.017 min
Lab File: VN079364.D
Acq: 28 Sep 2023 10:30

Tgt Ion: 94 Resp: 743
Ion Ratio Lower Upper
94 100
96 44.8 73.1 109.7#


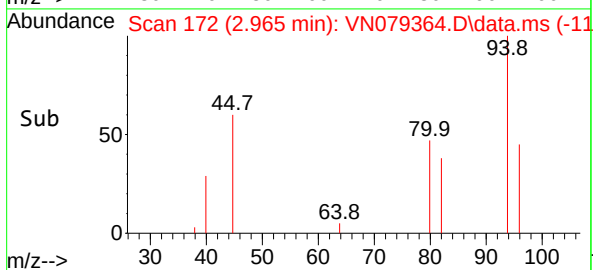
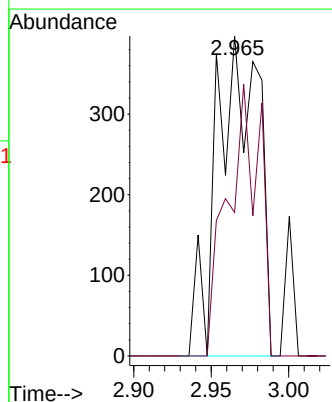
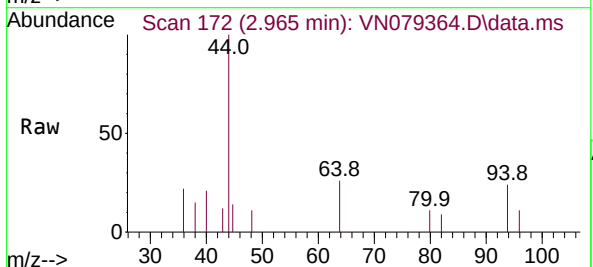




#6
Chloroethane
Concen: Below Cal
RT: 3.142 min Scan# 20
Delta R.T. 0.024 min
Lab File: VN079364.D
Acq: 28 Sep 2023 10:30




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 64 Resp: 348
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.2#

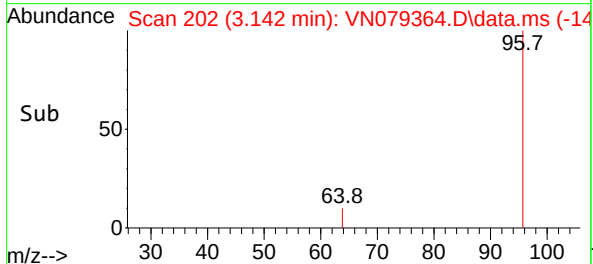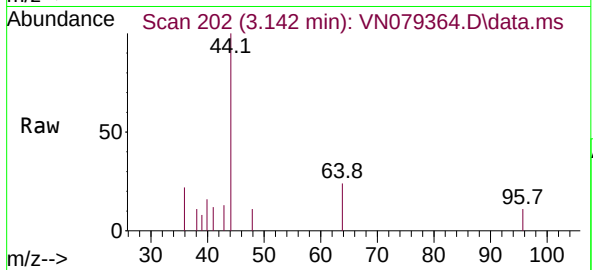

#11
Tert butyl alcohol
Concen: 2.448 ug/l
RT: 5.500 min Scan# 603
Delta R.T. -0.042 min
Lab File: VN079364.D
Acq: 28 Sep 2023 10:30


Tgt Ion: 59 Resp: 924
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#

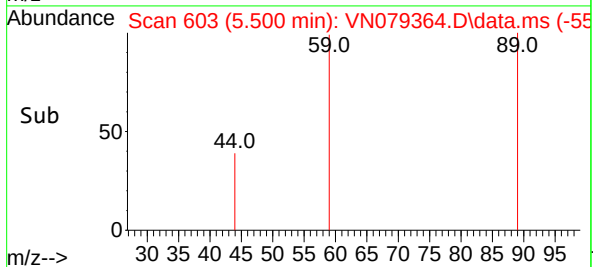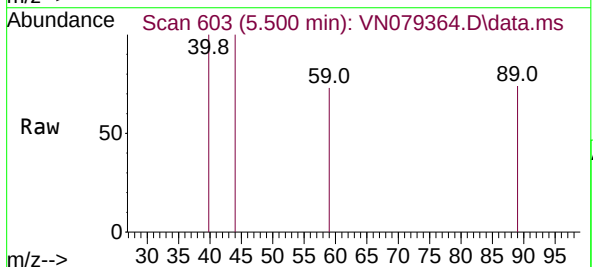






#15
Acrylonitrile
Concen: 0.421 ug/l
RT: 5.724 min Scan# 641
Delta R.T. -0.006 min
Lab File: VN079364.D
Acq: 28 Sep 2023 10:30

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 53 Resp: 412
Ion Ratio Lower Upper
53 100
52 27.7 65.3 97.9#
51 0.0 28.9 43.3#

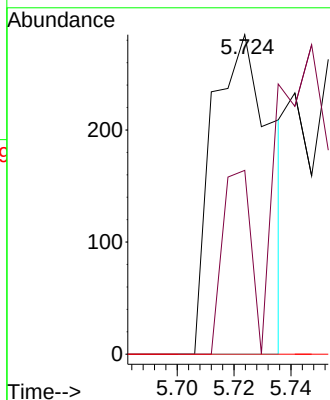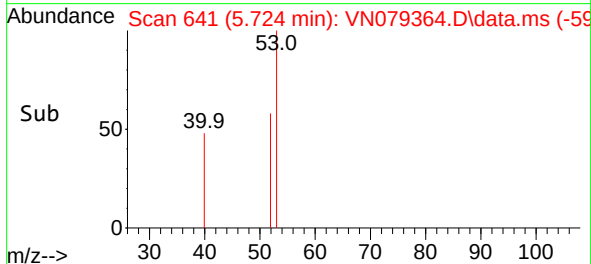

#16
Acetone
Concen: 0.784 ug/l
RT: 4.441 min Scan# 423
Delta R.T. -0.001 min
Lab File: VN079364.D
Acq: 28 Sep 2023 10:30

Tgt Ion: 43 Resp: 681
Ion Ratio Lower Upper
43 100
58 0.0 28.0 42.0#


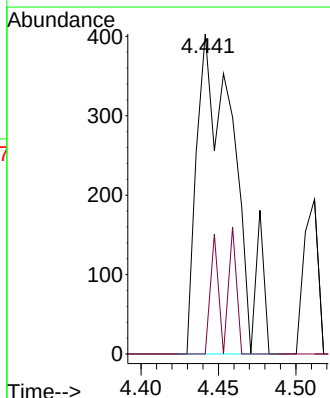
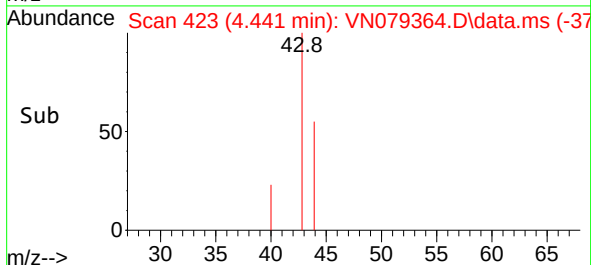
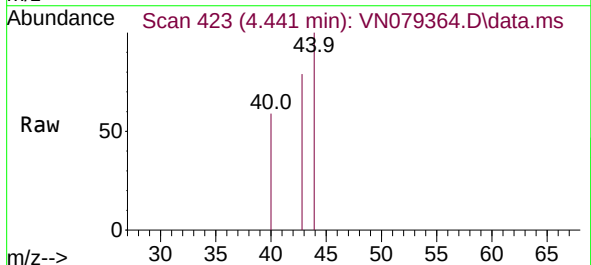




#17
Carbon Disulfide
Concen: 0.316 ug/l
RT: 4.706 min Scan# 41
Delta R.T. -0.018 min
Lab File: VN079364.D
Acq: 28 Sep 2023 10:30




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 76 Resp: 1597
Ion Ratio Lower Upper
76 100
78 0.0 7.4 11.0#

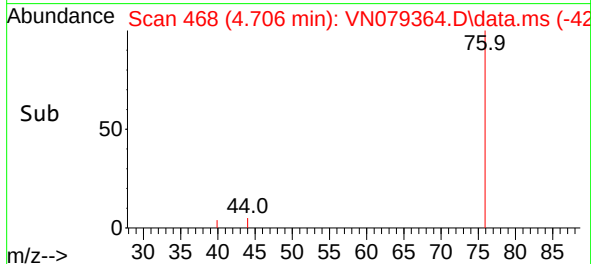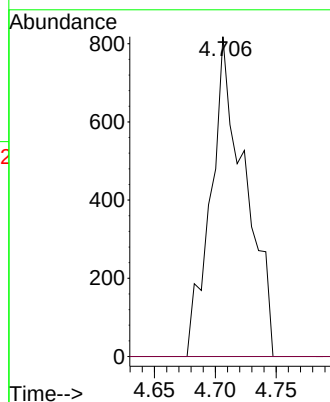

#20
Methylene Chloride
Concen: 0.407 ug/l
RT: 5.283 min Scan# 566
Delta R.T. -0.000 min
Lab File: VN079364.D
Acq: 28 Sep 2023 10:30

Tgt Ion: 84 Resp: 860
Ion Ratio Lower Upper
84 100
49 123.8 79.7 119.5#
51 0.0 25.2 37.8#
86 0.0 53.3 79.9#


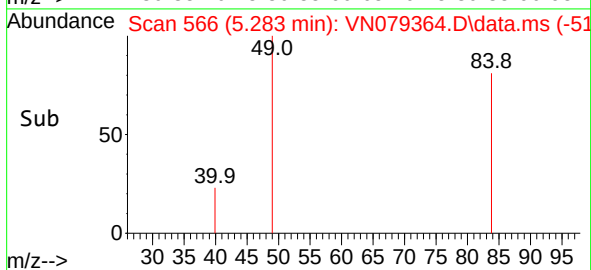
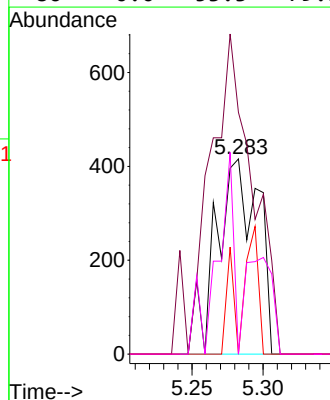
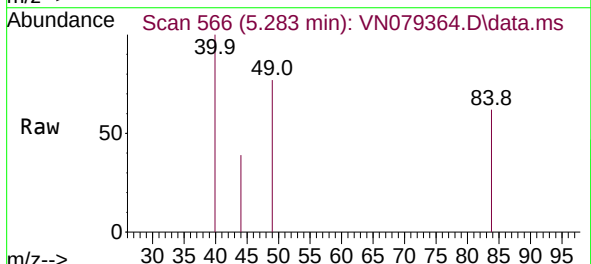




#25
2-Butanone
Concen: 0.341 ug/l
RT: 7.494 min Scan# 941
Delta R.T. 0.000 min
Lab File: VN079364.D
Acq: 28 Sep 2023 10:30




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 429
Ion Ratio Lower Upper
43 100
72 0.0 30.2 45.2#

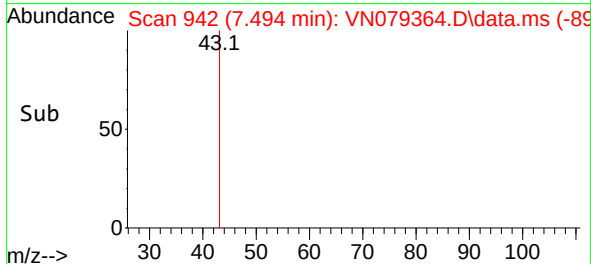

#31
Cyclohexane
Concen: 1.424 ug/l
RT: 8.229 min Scan# 1067
Delta R.T. -0.036 min
Lab File: VN079364.D
Acq: 28 Sep 2023 10:30

Tgt Ion: 56 Resp: 4250
Ion Ratio Lower Upper
56 100
69 119.6 26.8 40.2#
84 108.7 81.8 122.6

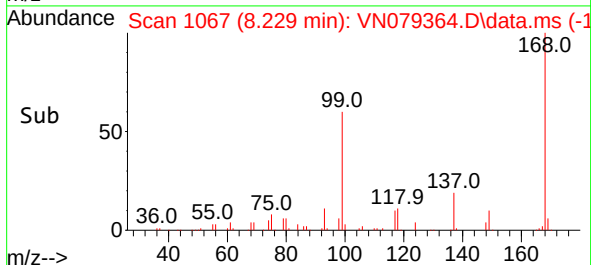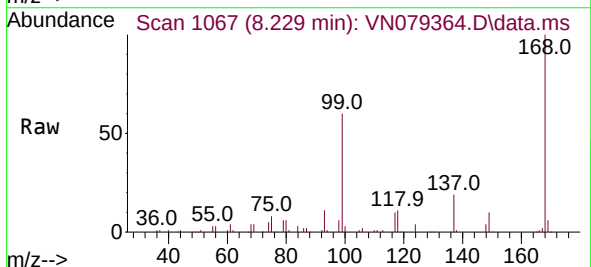

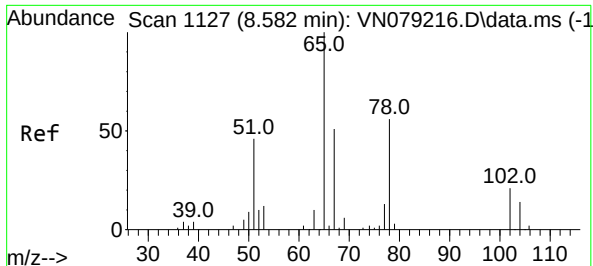

#33

1,2-Dichloroethane-d4

Concen: 59.815 ug/l

RT: 8.582 min Scan# 1127

Delta R.T. -0.001 min

Lab File: VN079364.D

Acq: 28 Sep 2023 10:30

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 65 Resp: 122294

Ion Ratio Lower Upper

65 100

67 51.1 0.0 106.6

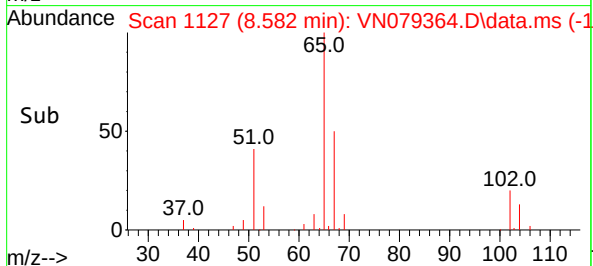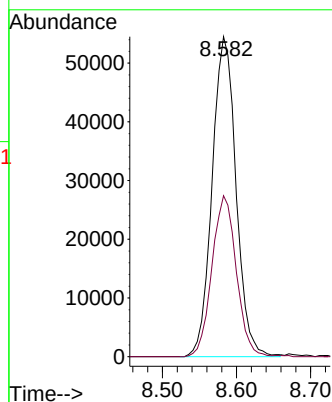

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1216

Delta R.T. -0.006 min

Lab File: VN079364.D

Acq: 28 Sep 2023 10:30




Tgt Ion: 114 Resp: 277525


Ion Ratio Lower Upper

114 100

63 20.7 0.0 36.4

88 14.9 0.0 30.6

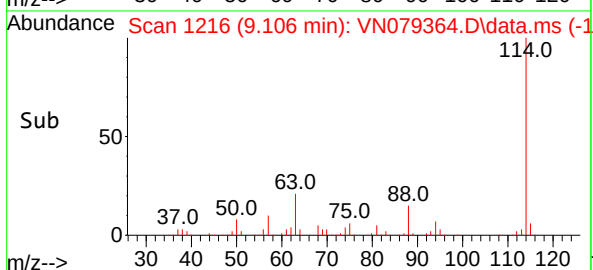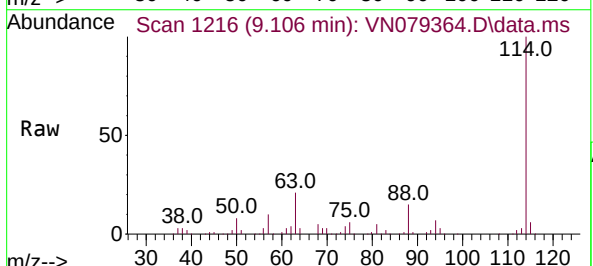

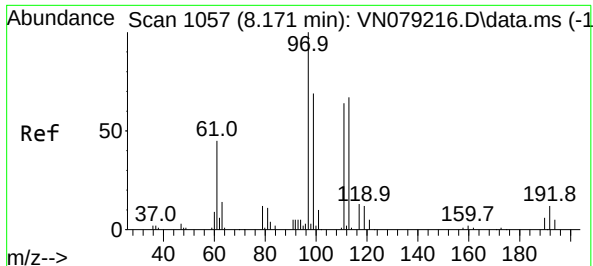

#35

Dibromofluoromethane

Concen: 52.069 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. -0.000 min

Lab File: VN079364.D





Acq: 28 Sep 2023 10:30

Instrument :

MSVOA_N

ClientSampleId :

Tgt Ion:	113	Resp:	96122
Ion	Ratio	Lower	Upper
113	100		
111	103.5	82.6	123.8
192	16.6	12.7	19.1

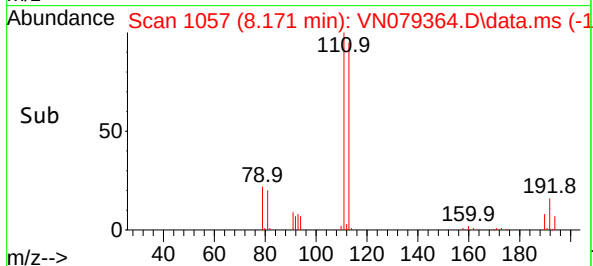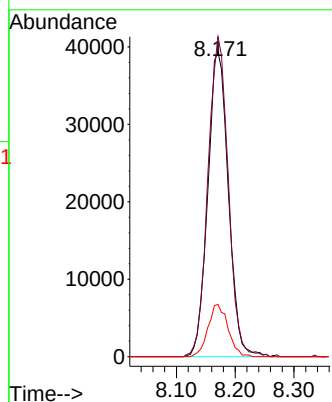

#36

1,1-Dichloropropene

Concen: 4.641 ug/l




RT: 8.224 min Scan# 1066


Delta R.T. -0.153 min

Lab File: VN079364.D

Acq: 28 Sep 2023 10:30


Tgt Ion:	75	Resp:	13206
Ion	Ratio	Lower	Upper
75	100		
110	8.2	19.1	57.3#
77	0.0	25.0	37.4#

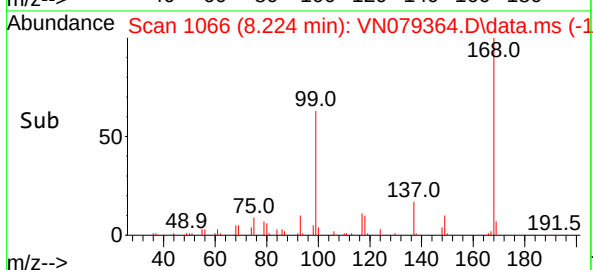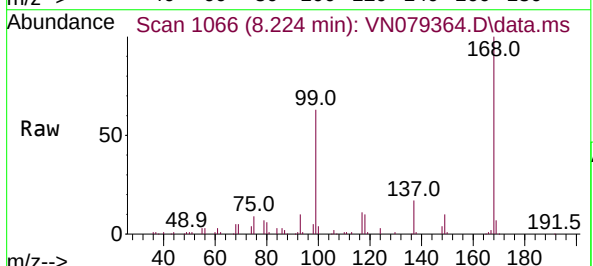






#38
Carbon Tetrachloride
Concen: 5.490 ug/l
RT: 8.224 min Scan# 1157
Delta R.T. -0.147 min
Lab File: VN079364.D
Acq: 28 Sep 2023 10:30

Instrument :
MSVOA_N
ClientSampleId :



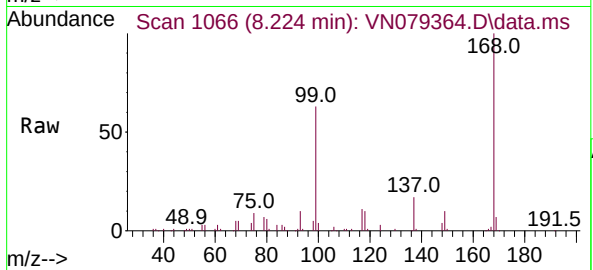



Tgt Ion:117 Resp: 16166
Ion Ratio Lower Upper
117 100
119 5.1 77.3 115.9#
121 0.0 23.3 34.9#

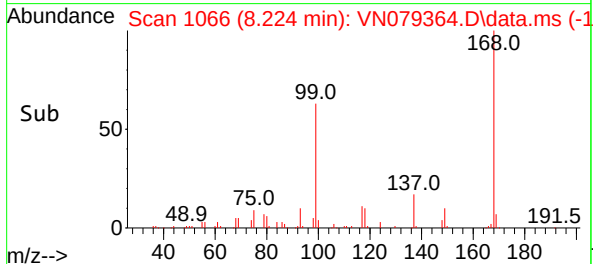

#43
Isopropyl Acetate
Concen: 0.311 ug/l
RT: 8.759 min Scan# 1157
Delta R.T. 0.065 min
Lab File: VN079364.D
Acq: 28 Sep 2023 10:30

Tgt Ion: 43 Resp: 1438
Ion Ratio Lower Upper
43 100
61 0.0 24.7 37.1#
87 0.0 14.6 21.8#


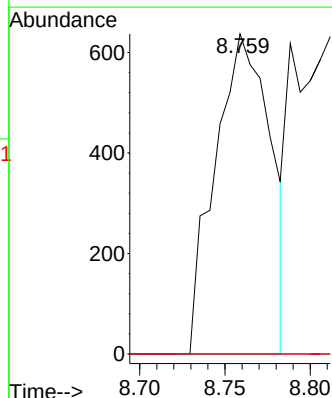

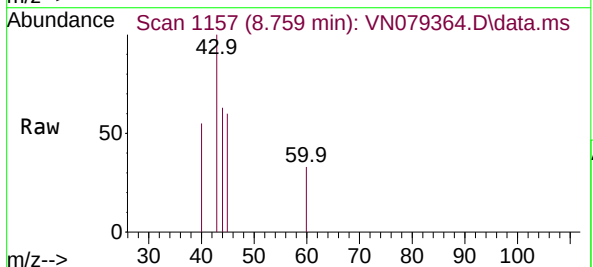




#50
Toluene-d8
Concen: 45.524 ug/l
RT: 10.570 min Scan# 1465
Delta R.T. -0.001 min
Lab File: VN079364.D
Acq: 28 Sep 2023 10:30




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 98 Resp: 308580
Ion Ratio Lower Upper
98 100
100 63.4 52.0 78.0

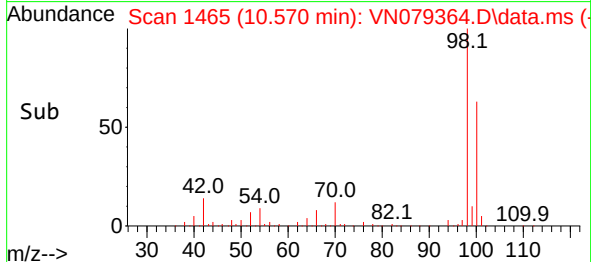

#51
4-Methyl-2-Pentanone
Concen: 0.388 ug/l
RT: 10.447 min Scan# 1444
Delta R.T. -0.006 min
Lab File: VN079364.D
Acq: 28 Sep 2023 10:30

Tgt Ion: 43 Resp: 1043
Ion Ratio Lower Upper
43 100
58 29.6 36.6 54.8#


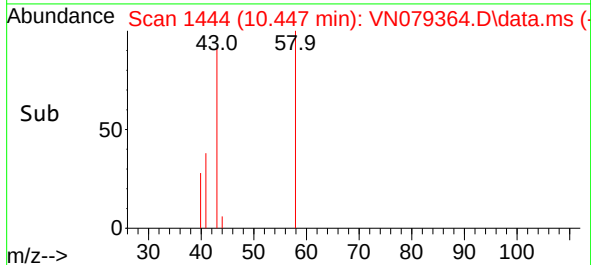

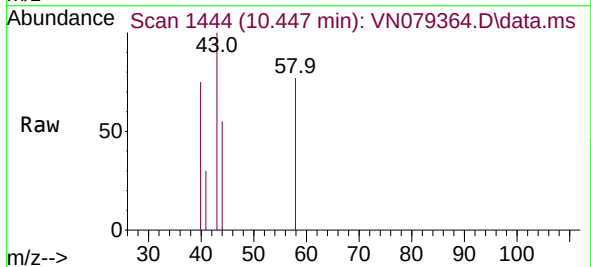




#58
2-Chloroethyl Vinyl ether
Concen: Below Cal
RT: 10.165 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN079364.D
Acq: 28 Sep 2023 10:30




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 63 Resp: 156
Ion Ratio Lower Upper
63 100
106 0.0 26.2 39.4#

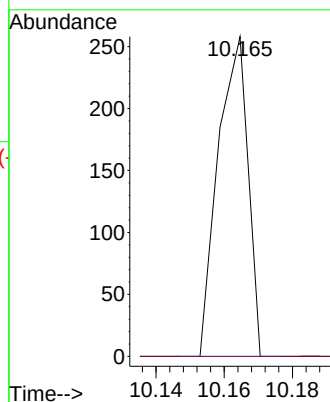

#59
2-Hexanone
Concen: 1.101 ug/l
RT: 11.212 min Scan# 1574
Delta R.T. 0.012 min
Lab File: VN079364.D
Acq: 28 Sep 2023 10:30

Tgt Ion: 43 Resp: 2144
Ion Ratio Lower Upper
43 100
58 44.6 31.7 95.1


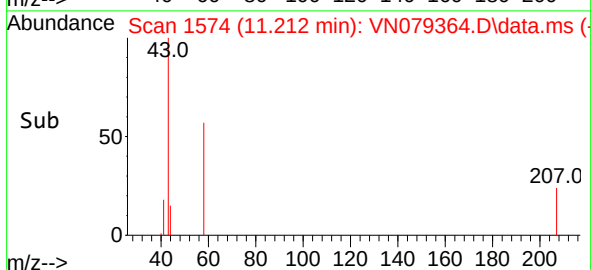
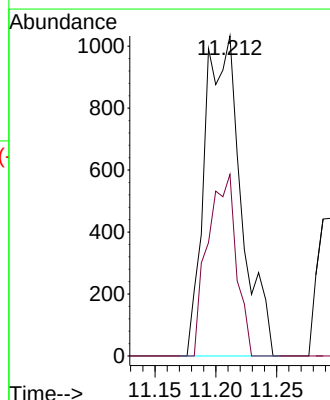
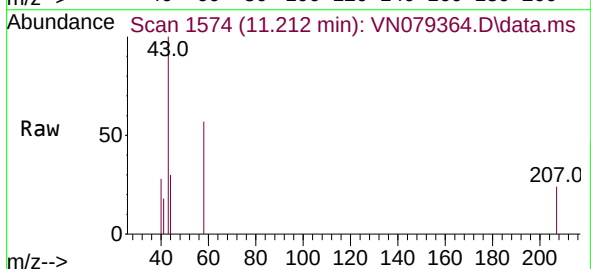




#62
4-Bromofluorobenzene
Concen: 44.829 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN079364.D
Acq: 28 Sep 2023 10:30




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 96929
Ion Ratio Lower Upper
95 100
174 75.0 0.0 143.8
176 72.2 0.0 135.8

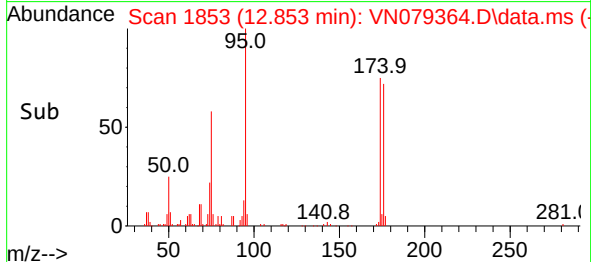

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 1686
Delta R.T. -0.001 min
Lab File: VN079364.D
Acq: 28 Sep 2023 10:30

Tgt Ion: 117 Resp: 237336
Ion Ratio Lower Upper
117 100
82 59.6 44.0 66.0
119 33.4 25.6 38.4


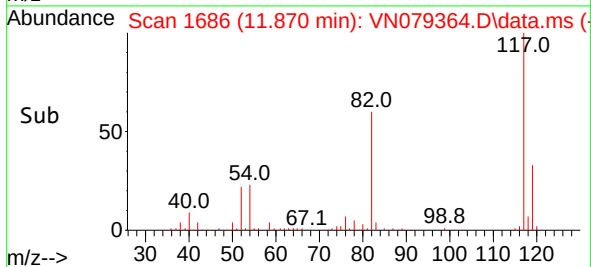

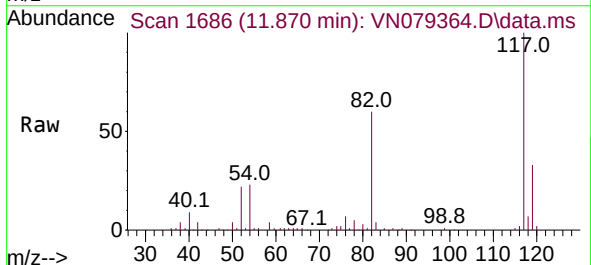


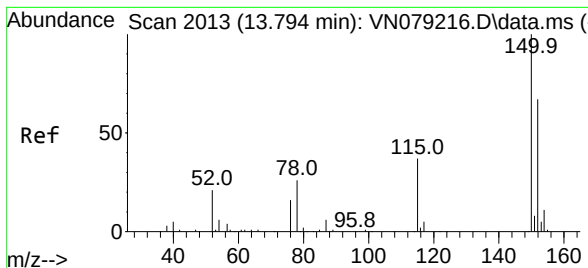

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.794 min Scan# 20
 Delta R.T. -0.000 min
 Lab File: VN079364.D
 Acq: 28 Sep 2023 10:30




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion:152 Resp: 69475
 Ion Ratio Lower Upper
 152 100
 115 61.9 32.3 96.8
 150 154.6 0.0 355.8

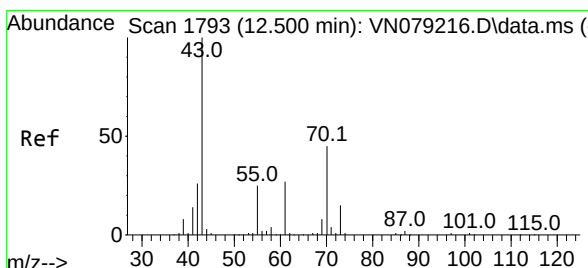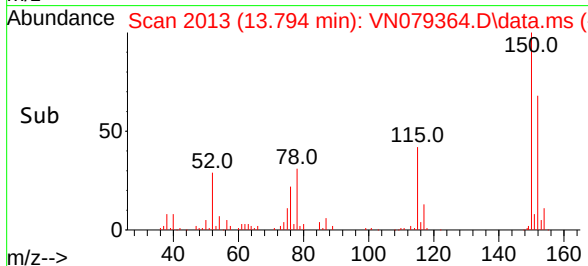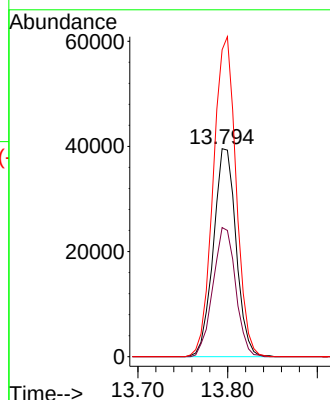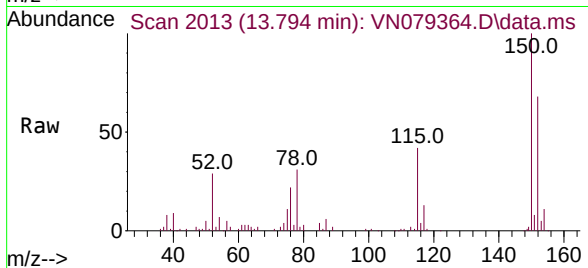

#74
 N-ethyl acetate
 Concen: 0.379 ug/l
 RT: 12.494 min Scan# 1792
 Delta R.T. -0.006 min
 Lab File: VN079364.D
 Acq: 28 Sep 2023 10:30

Tgt Ion: 43 Resp: 908
 Ion Ratio Lower Upper
 43 100
 70 29.8 43.4 65.2#
 55 0.0 21.4 32.0#
 61 0.0 22.8 34.2#

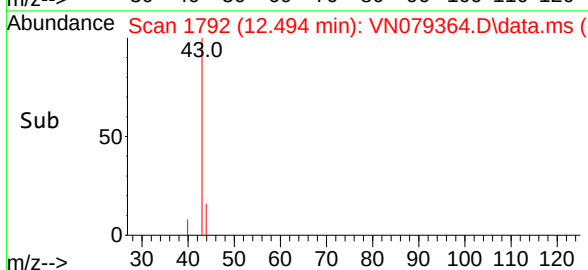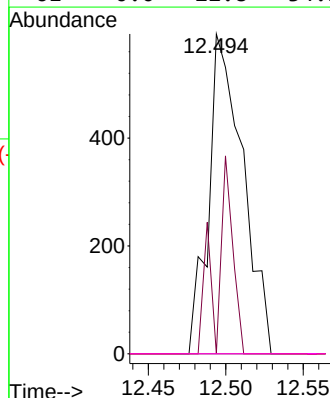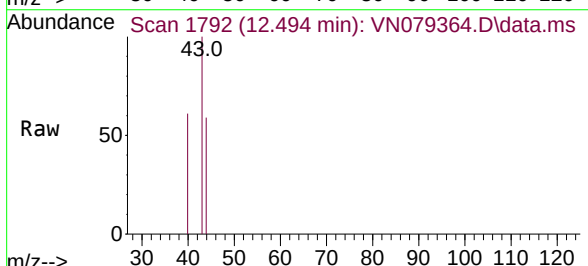



#75

1,1,2,2-Tetrachloroethane

Concen: 0.274 ug/l

RT: 12.947 min Scan# 1868

Delta R.T. 0.006 min

Lab File: VN079364.D

Acq: 28 Sep 2023 10:30

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion: 83 Resp: 644

Ion Ratio Lower Upper

83 100

131 0.0 5.0 15.0#

85 33.4 31.9 95.7

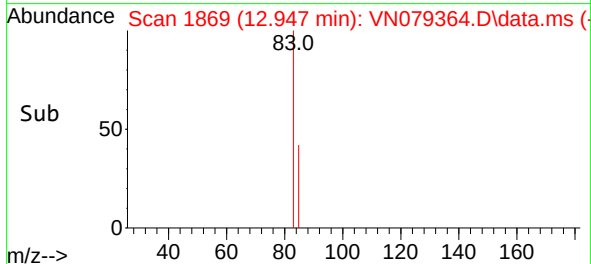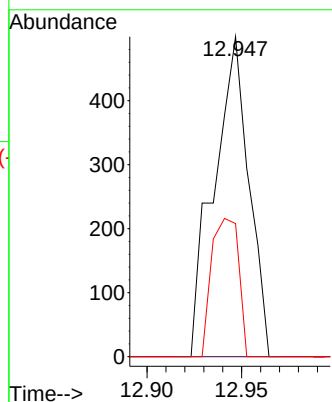

#76

1,2,3-Trichloropropane

Concen: 29.033 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. -0.147 min

Lab File: VN079364.D




Acq: 28 Sep 2023 10:30


Tgt Ion: 75 Resp: 54362

Ion Ratio Lower Upper

75 100


77 0.6 84.5 253.5#

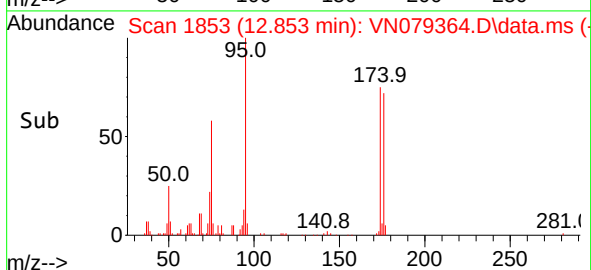






#79
2-Chlorotoluene
Concen: 0.287 ug/l
RT: 13.229 min Scan# 1900
Delta R.T. 0.100 min
Lab File: VN079364.D
Acq: 28 Sep 2023 10:30


Instrument :
MSVOA_N
ClientSampleId :

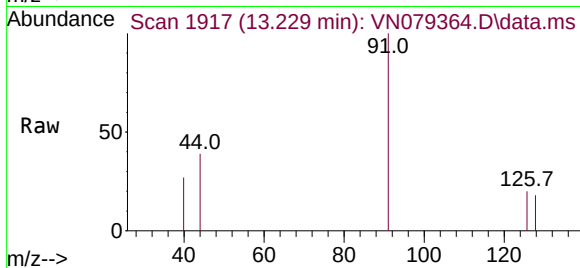



Tgt Ion: 91 Resp: 1334
Ion Ratio Lower Upper
91 100
126 19.1 16.3 48.8

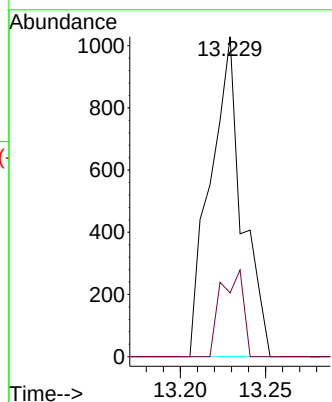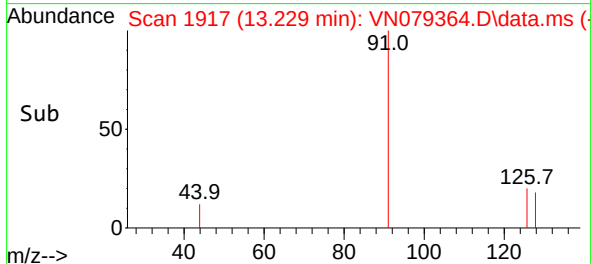


#81
trans-1,4-Dichloro-2-butene
Concen: 79.817 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.112 min
Lab File: VN079364.D
Acq: 28 Sep 2023 10:30

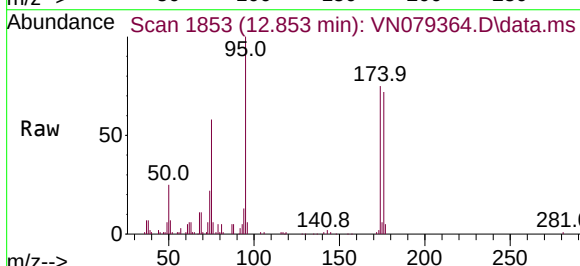

Tgt Ion: 75 Resp: 54362
Ion Ratio Lower Upper
75 100
53 0.0 67.4 101.2#
89 0.0 38.8 58.2#




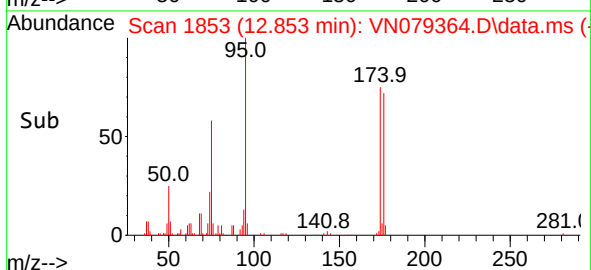




#82
4-Chlorotoluene
Concen: 0.306 ug/l
RT: 13.229 min Scan# 1916
Delta R.T. 0.000 min
Lab File: VN079364.D
Acq: 28 Sep 2023 10:30




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 1334
Ion Ratio Lower Upper
91 100
126 19.1 16.7 50.0

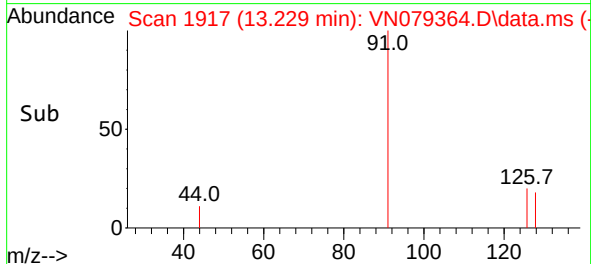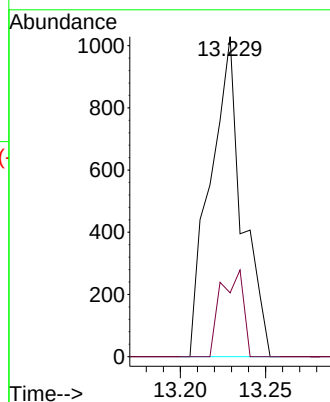

#87
1,3-Dichlorobenzene
Concen: 0.403 ug/l
RT: 13.735 min Scan# 2003
Delta R.T. -0.006 min
Lab File: VN079364.D
Acq: 28 Sep 2023 10:30


Tgt Ion: 146 Resp: 1059
Ion Ratio Lower Upper
146 100
111 34.5 22.1 66.3
148 52.0 32.0 96.0

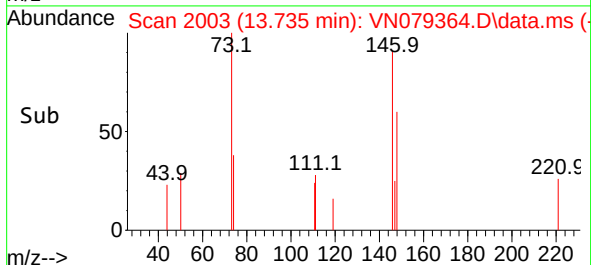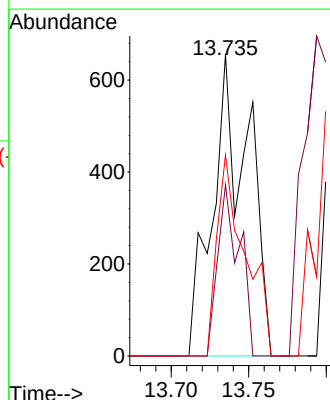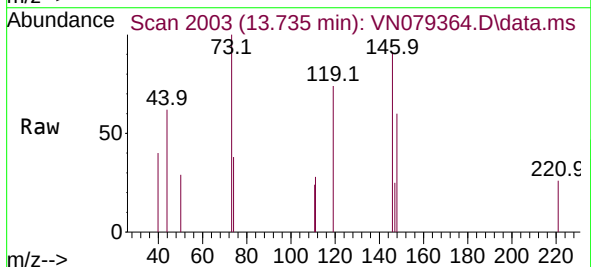






#88
1,4-Dichlorobenzene
Concen: 0.399 ug/l
RT: 13.735 min Scan# 2017
Delta R.T. -0.083 min
Lab File: VN079364.D
Acq: 28 Sep 2023 10:30

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:146 Resp: 1059
Ion Ratio Lower Upper
146 100
111 34.5 20.6 61.8
148 52.0 31.6 94.8

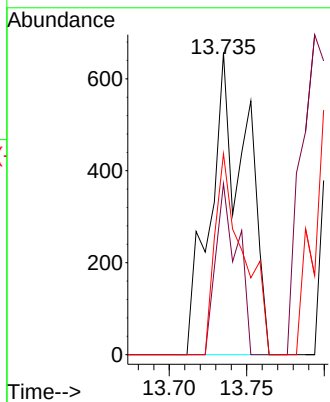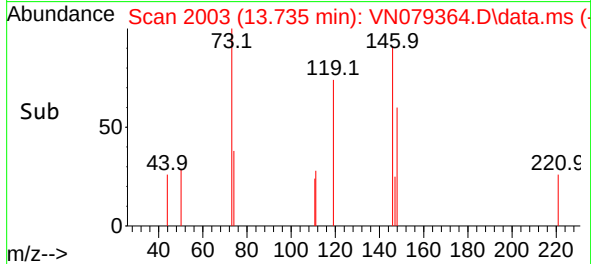

#89
n-Butylbenzene
Concen: 0.497 ug/l
RT: 14.059 min Scan# 2058
Delta R.T. -0.000 min
Lab File: VN079364.D
Acq: 28 Sep 2023 10:30

Tgt Ion: 91 Resp: 1874
Ion Ratio Lower Upper
91 100
92 47.4 26.4 79.0
134 12.3 12.6 37.6#

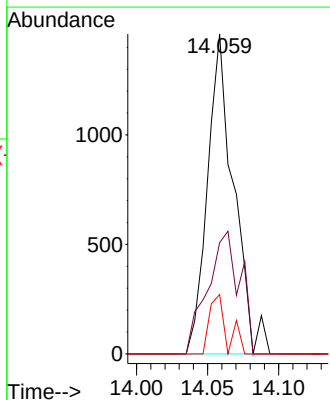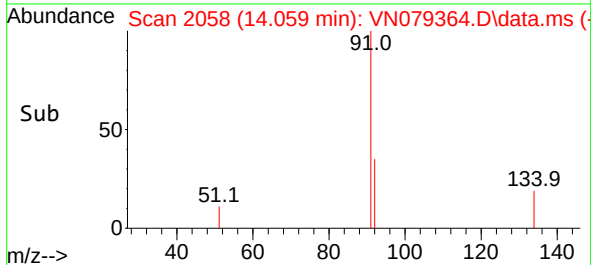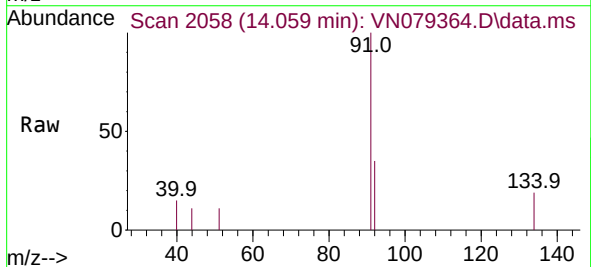

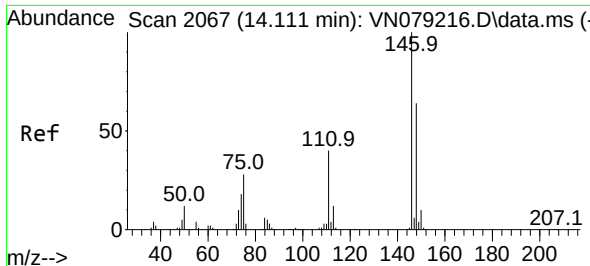

#91

1,2-Dichlorobenzene

Concen: 0.452 ug/l

RT: 14.117 min Scan# 2067

Delta R.T. 0.005 min


Lab File: VN079364.D

Acq: 28 Sep 2023 10:30

Instrument :

MSVOA_N

ClientSampleId :

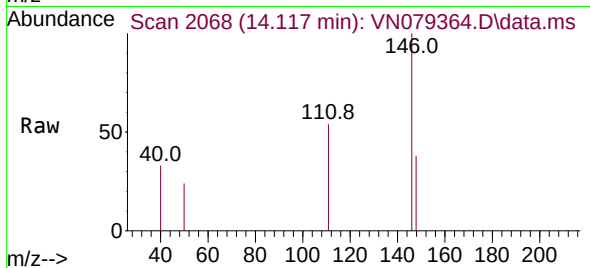




Tgt Ion:146 Resp: 1171

Ion Ratio Lower Upper

146 100

111 52.0 22.0 66.0

148 41.5 31.8 95.3

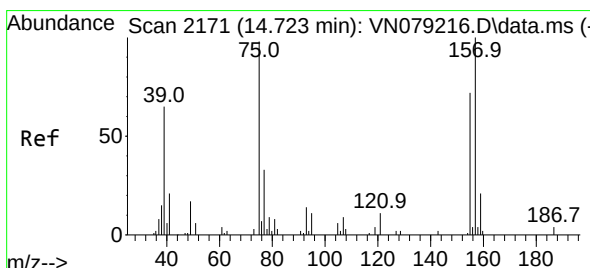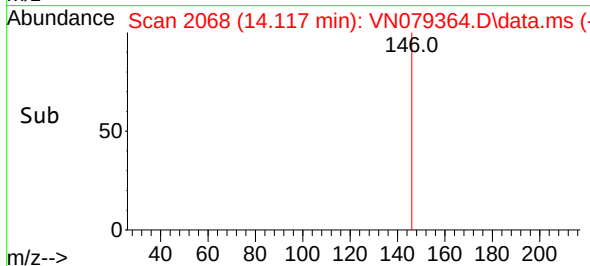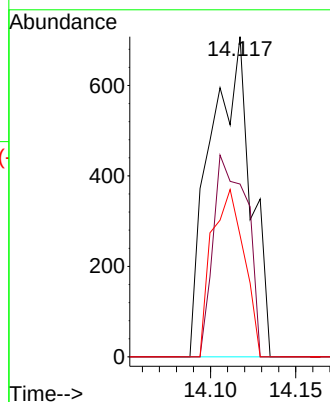

#92

1,2-Dibromo-3-Chloropropane

Concen: 0.439 ug/l

RT: 14.711 min Scan# 2169

Delta R.T. -0.012 min

Lab File: VN079364.D

Acq: 28 Sep 2023 10:30




Tgt Ion: 75 Resp: 157


Ion Ratio Lower Upper

75 100

155 43.3 39.1 117.2


157 75.8 50.3 150.9

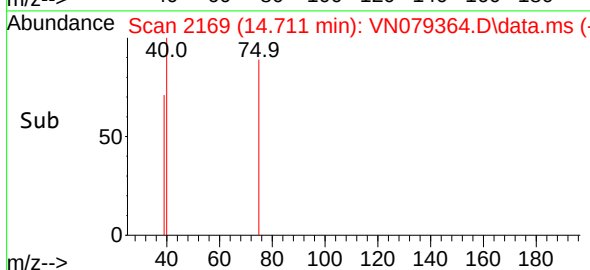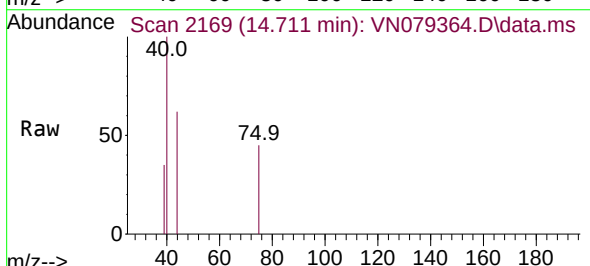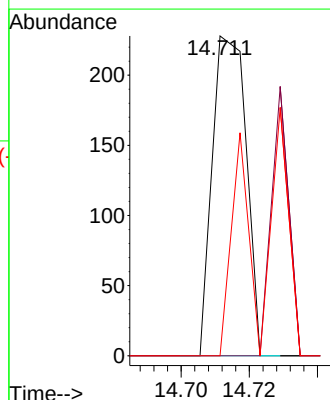



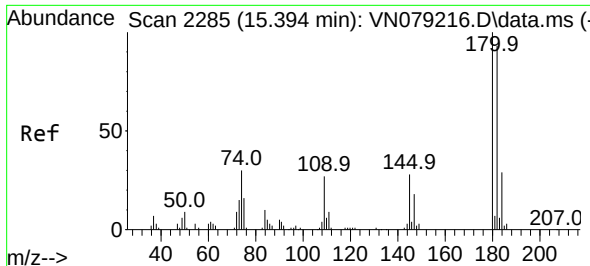


#93
 1,2,4-Trichlorobenzene
 Concen: 1.218 ug/l
 RT: 15.400 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VN079364.D
 Acq: 28 Sep 2023 10:30

Instrument :
 MSVOA_N
 ClientSampleId :



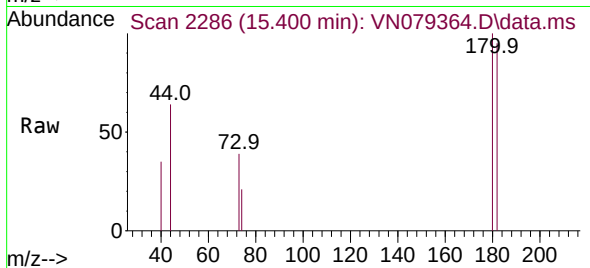



Tgt Ion:180 Resp: 1134
 Ion Ratio Lower Upper
 180 100
 182 81.4 46.1 138.2
 145 4.9 16.6 49.8#

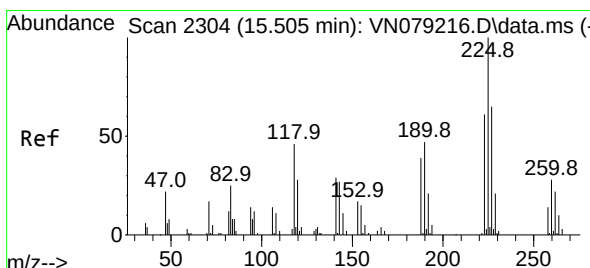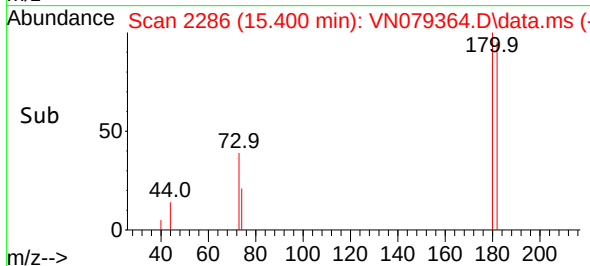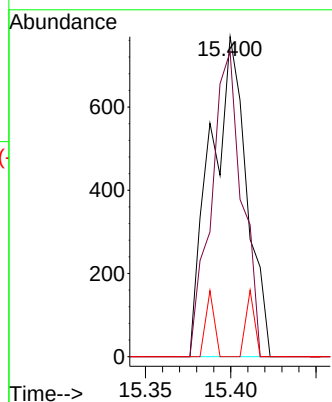

#94
 Hexachlorobutadiene
 Concen: 0.807 ug/l
 RT: 15.511 min Scan# 2305
 Delta R.T. 0.005 min
 Lab File: VN079364.D
 Acq: 28 Sep 2023 10:30

Tgt Ion:225 Resp: 591
 Ion Ratio Lower Upper
 225 100
 223 73.4 31.3 93.8
 227 91.7 31.9 95.9

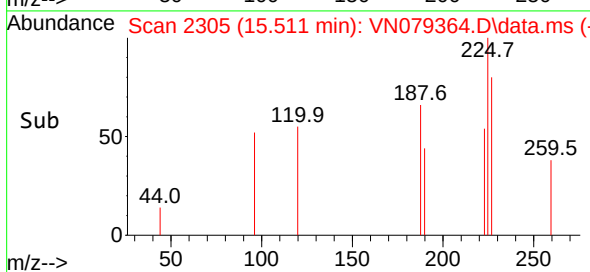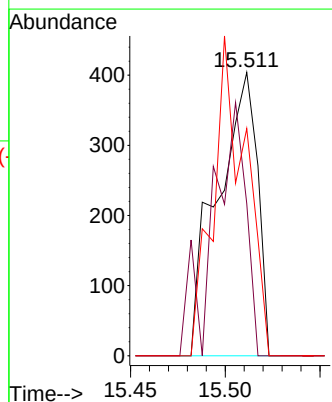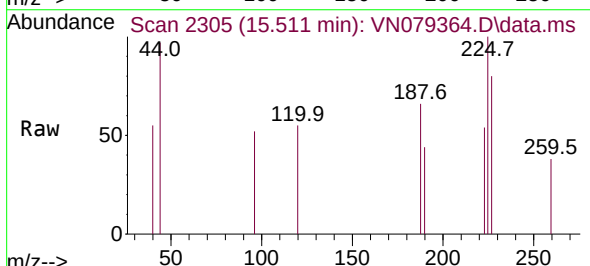



#95

Naphthalene

Concen: 1.386 ug/l

RT: 15.658 min Scan# 21

Delta R.T. 0.011 min


Lab File: VN079364.D

Acq: 28 Sep 2023 10:30




Instrument :

MSVOA_N

ClientSampleId :



Tgt Ion:128	Resp:	3834
Ion Ratio	Lower	Upper
128	100	
127	9.3	10.0 15.0#
129	11.9	8.7 13.1

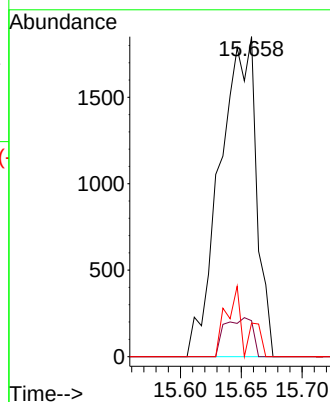

#96

1,2,3-Trichlorobenzene

Concen: 1.488 ug/l

RT: 15.852 min Scan# 2363

Delta R.T. 0.005 min

Lab File: VN079364.D

Acq: 28 Sep 2023 10:30

Tgt Ion:180	Resp:	1635
Ion Ratio	Lower	Upper
180	100	
182	91.4	46.2 138.6
145	20.3	17.5 52.6

