
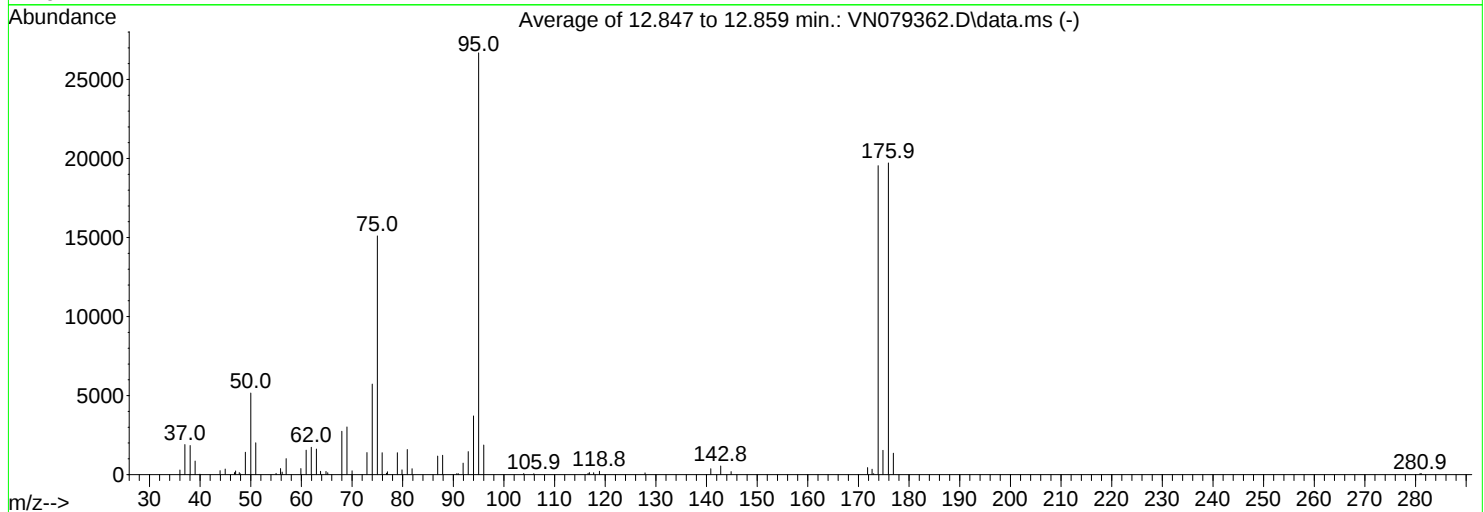


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN079362\
Data File : VN079362.D
Acq On : 28 Sep 2023 09:20
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091123W.M
Title : SW846 8260
Last Update : Tue Sep 12 05:05:24 2023

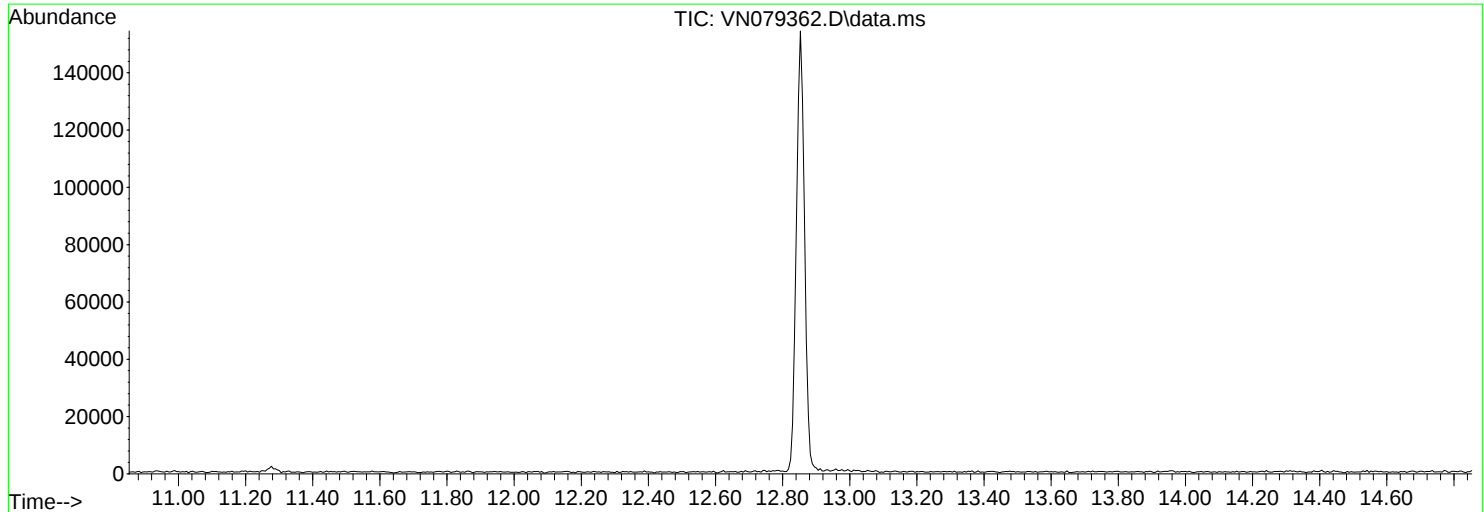

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	5164	PASS
75	95	30	60	56.6	15108	PASS
95	95	100	100	100.0	26685	PASS
96	95	5	9	7.0	1873	PASS
173	174	0.00	2	1.8	348	PASS
174	95	50	100	73.3	19547	PASS
175	174	5	9	7.9	1538	PASS
176	174	95	101	100.9	19717	PASS
177	176	5	9	6.9	1360	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	297	48.95	1416	63.80	214	77.00	181
37.00	1899	50.00	5164	64.85	206	78.95	139
38.05	1842	51.00	2013	65.20	120	79.85	30
39.00	856	55.00	79	68.00	2741	80.90	158
39.95	34	55.90	388	69.00	3020	81.85	374
43.95	254	56.20	158	70.00	239	86.90	1173
44.95	359	57.00	1012	72.95	1394	87.90	1222
46.80	132	59.90	385	74.00	5725	90.70	75
47.00	229	60.95	1545	75.00	15108	91.00	65
47.75	134	61.95	1733	75.95	1384	91.95	728
48.00	55	62.95	1619	76.80	90	92.95	1454

Average of 12.847 to 12.859 min.: VN079362.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.00	3717	142.80	550				
95.00	26685	144.85	194				
96.00	1873	171.80	449				
103.90	69	172.70	348				
105.90	65	173.00	66				
116.60	84	173.90	19547				
116.85	136	174.85	1538				
117.70	120	175.90	19717				
118.85	209	176.90	1360				
127.85	107	280.90	74				
140.85	374	281.10	72				

Instrument :

MSVOA_N

ClientSampleId :

BFB