


Chloromethane

Response Ratio

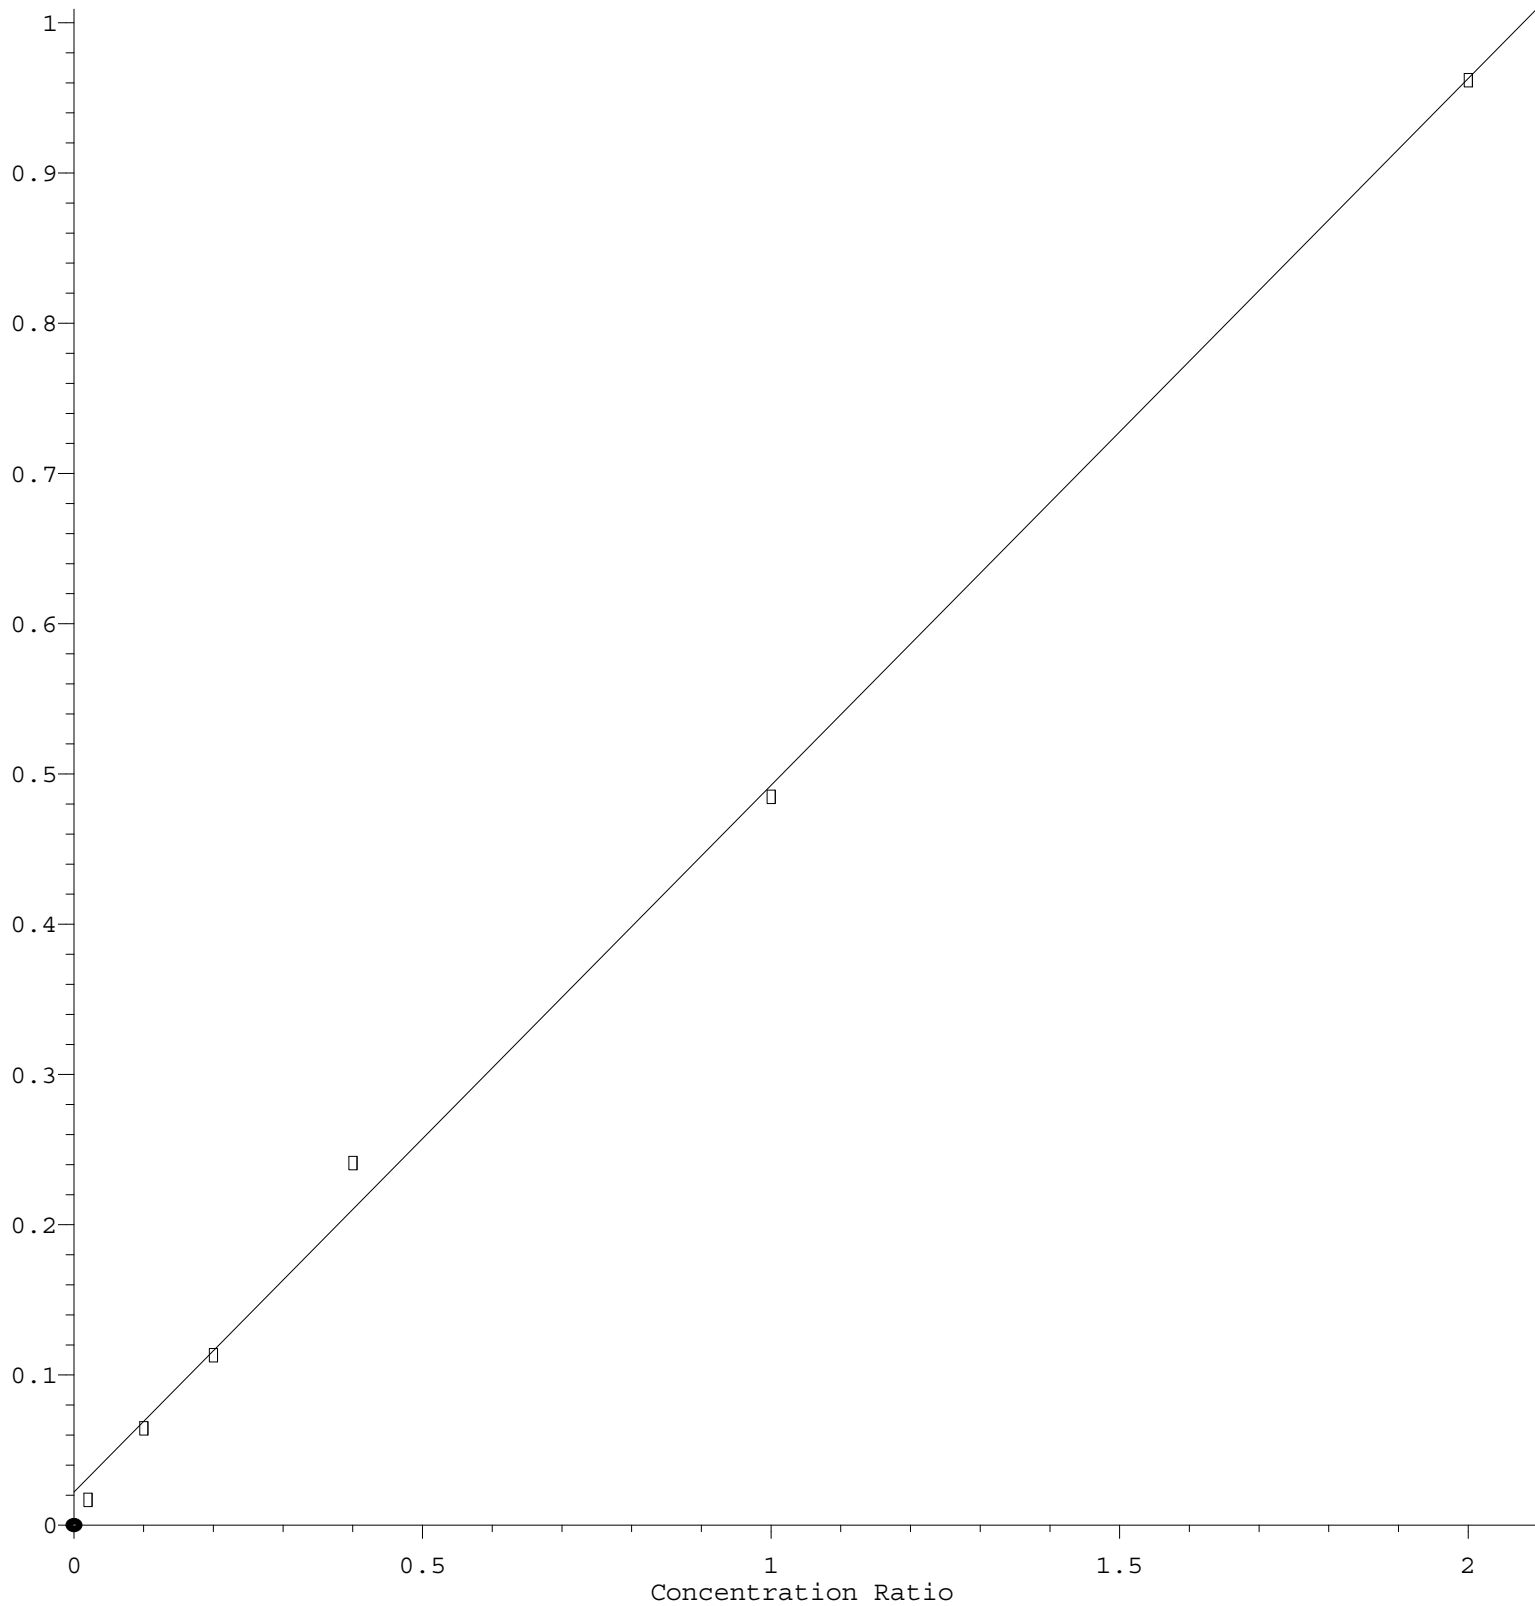

$$\text{Response} = 4.708\text{e-}001 * \text{Amt} + 2.171\text{e-}002$$


Coef of Det (r^2) = 0.998053 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N092921W.M

Calibration Table Last Updated: Wed Sep 29 23:31:35 2021

Methyl Iodide

Response Ratio

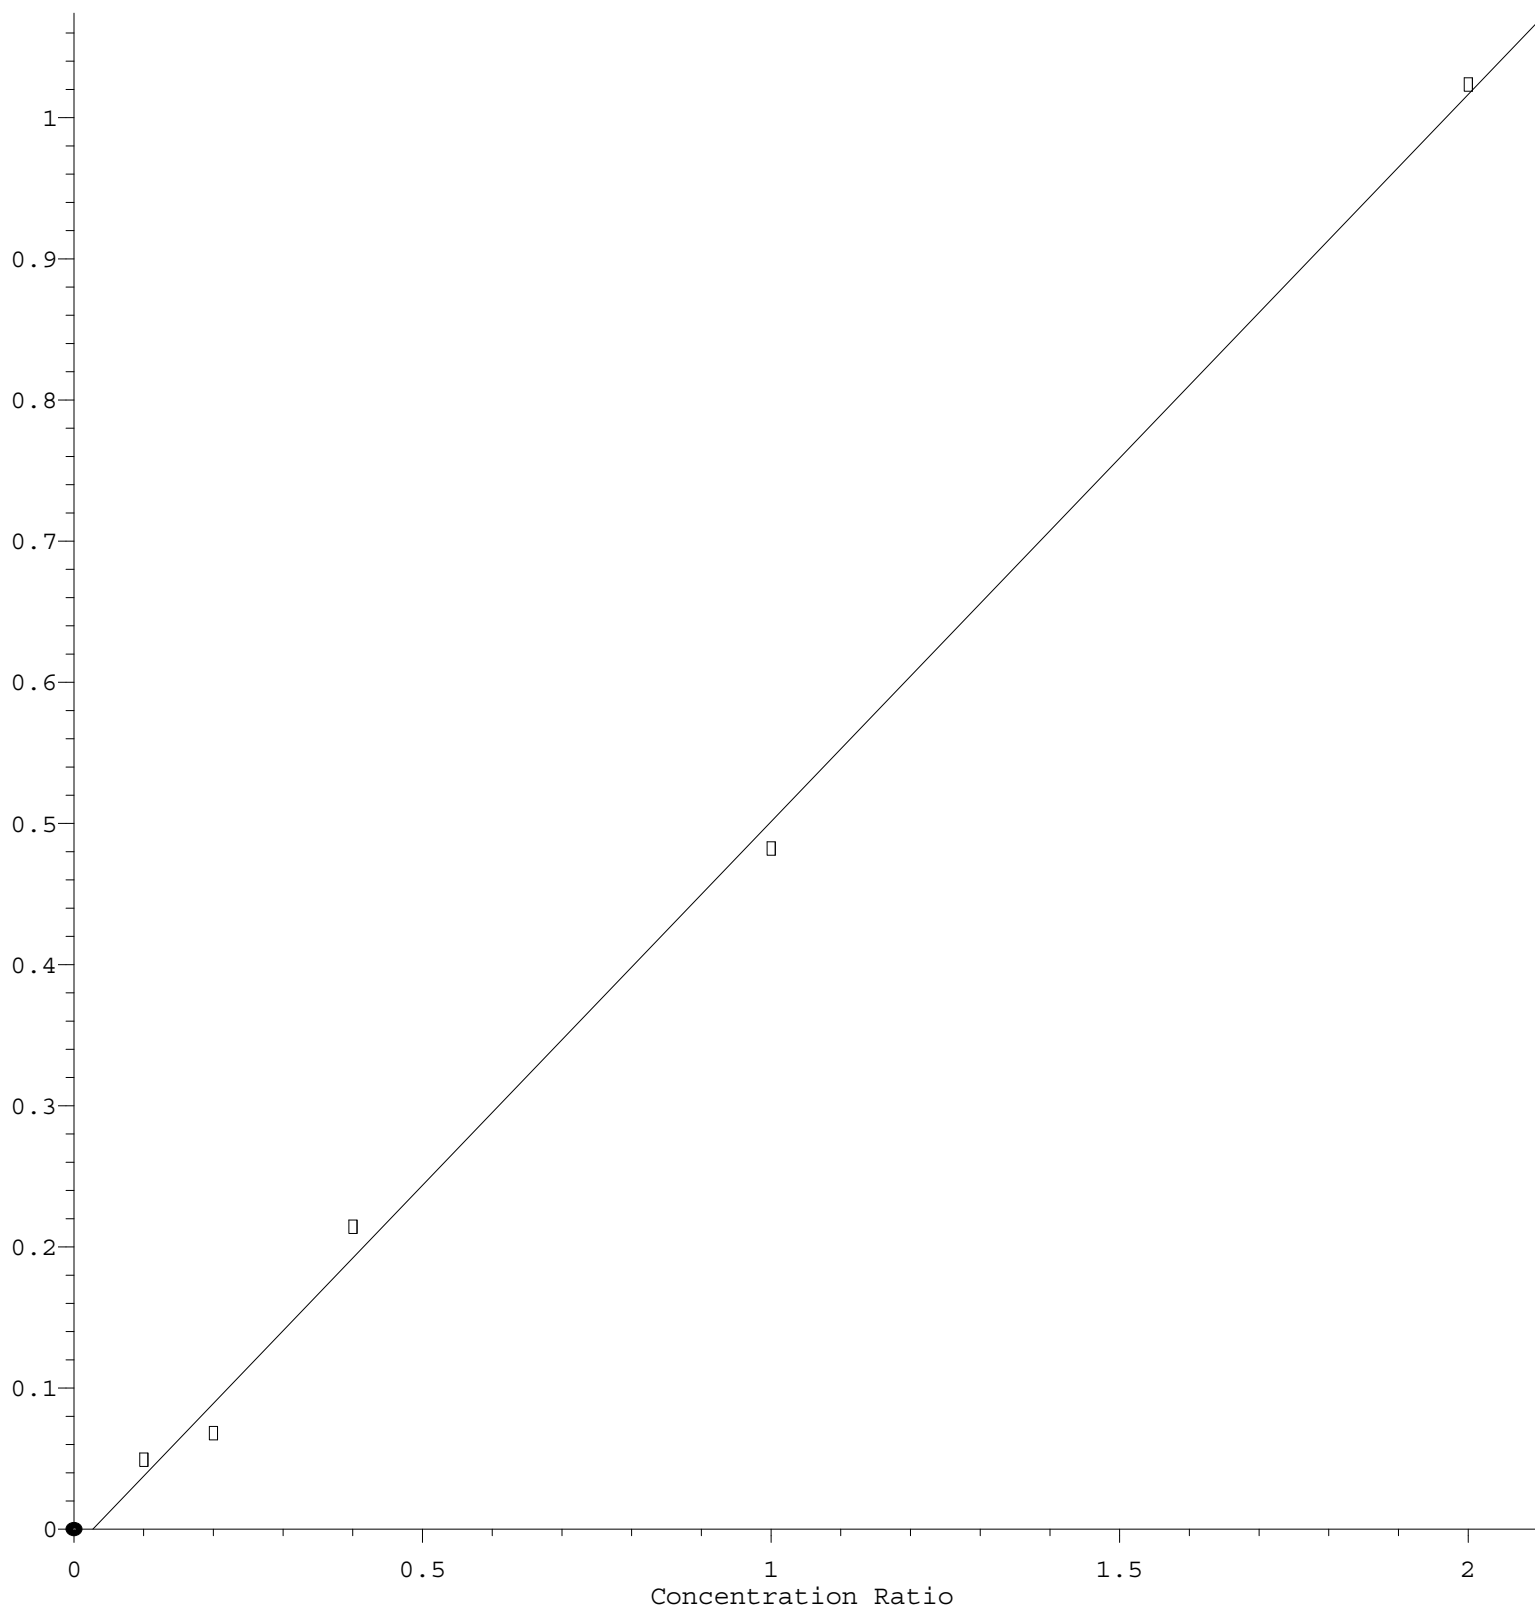

$$\text{Response} = 5.153\text{e-}001 * \text{Amt} - 1.392\text{e-}002$$


Coef of Det (r^2) = 0.997748 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N092921W.M

Calibration Table Last Updated: Wed Sep 29 23:31:35 2021

Trichlorofluoromethane

Response Ratio

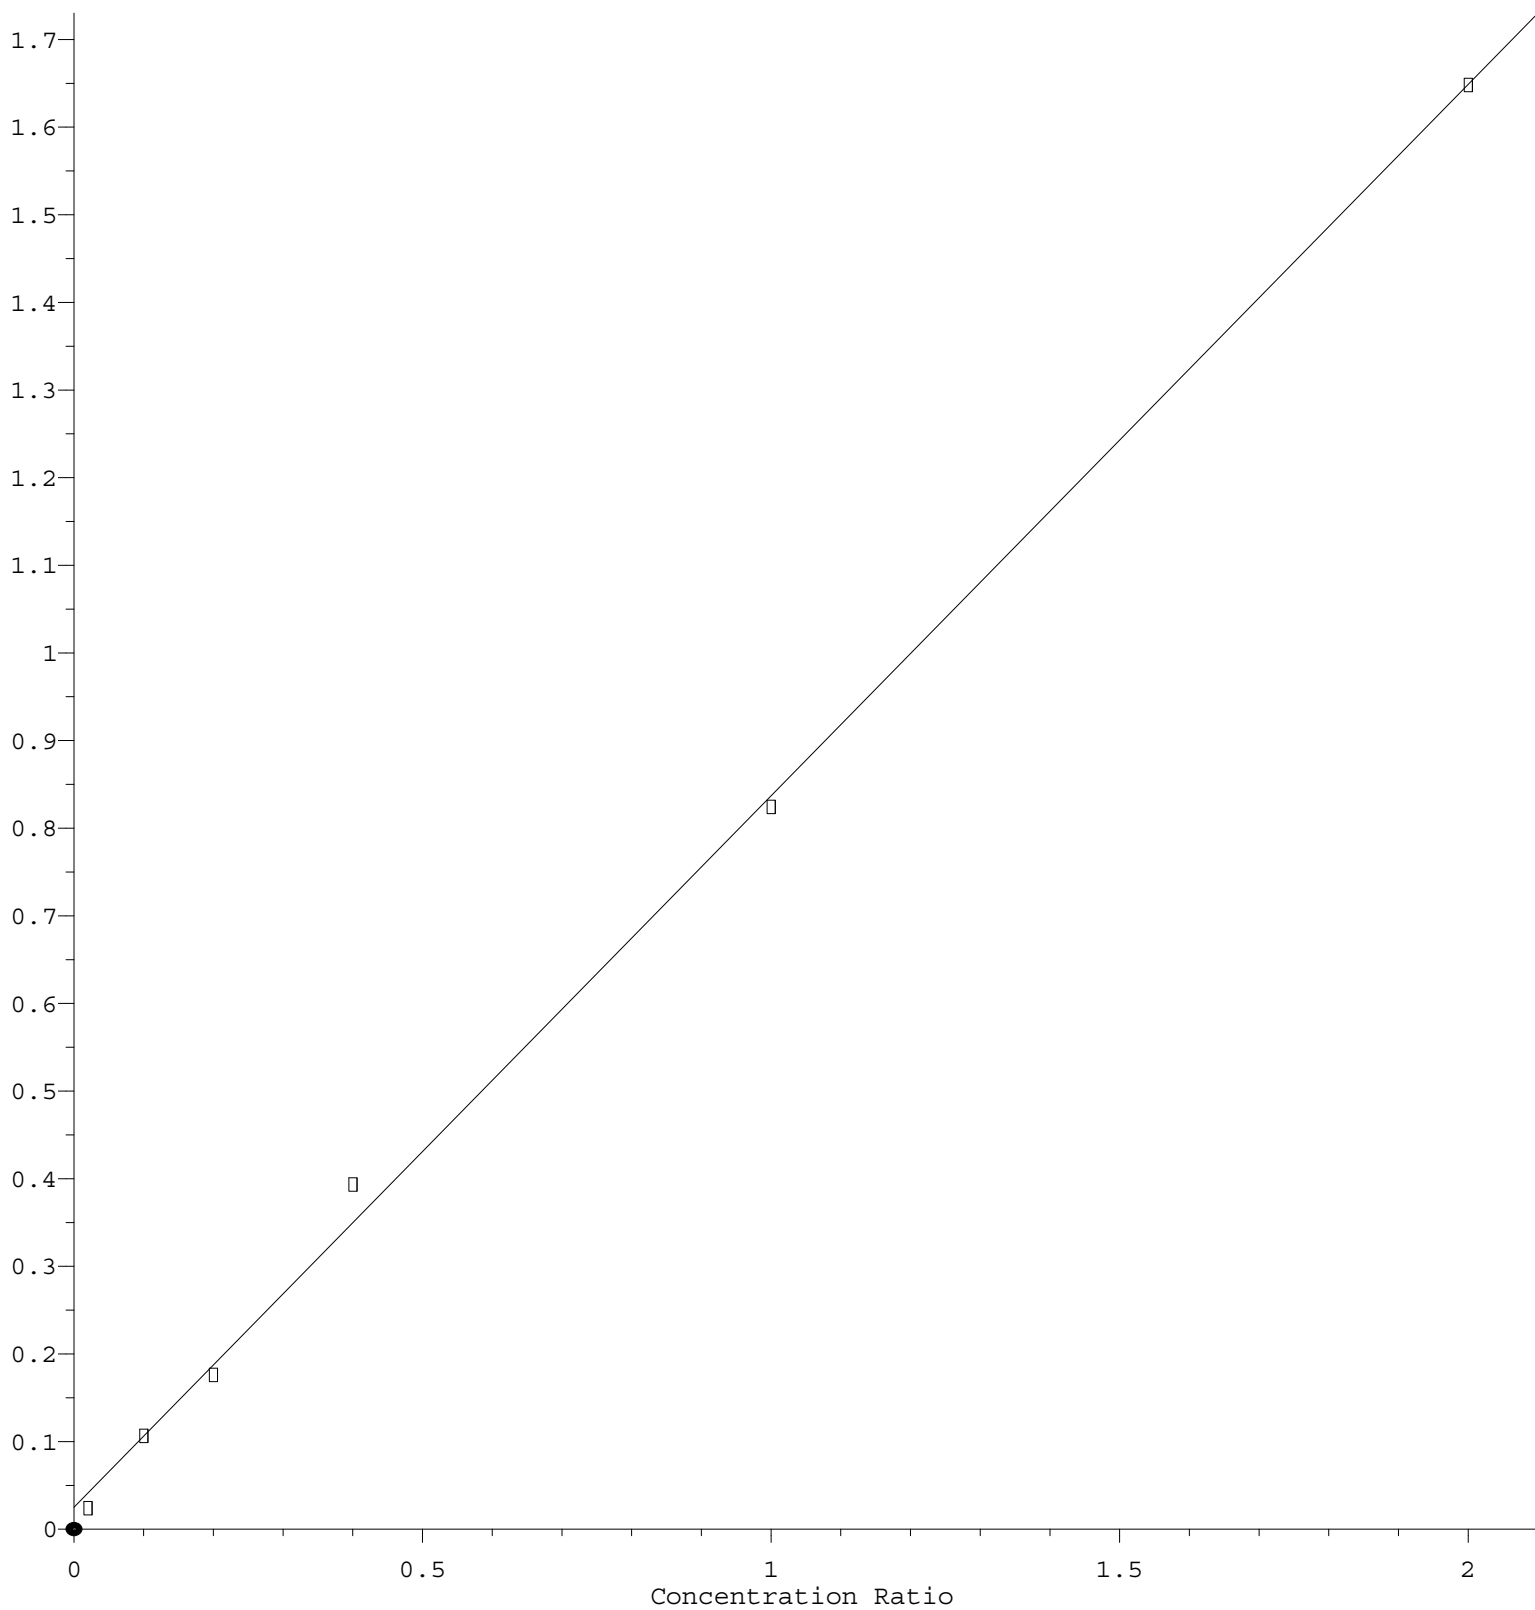

$$\text{Response} = 8.117\text{e-}001 * \text{Amt} + 2.540\text{e-}002$$


Coef of Det (r^2) = 0.998706 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N092921W.M

Calibration Table Last Updated: Wed Sep 29 23:31:35 2021

Chloroethane


Response Ratio

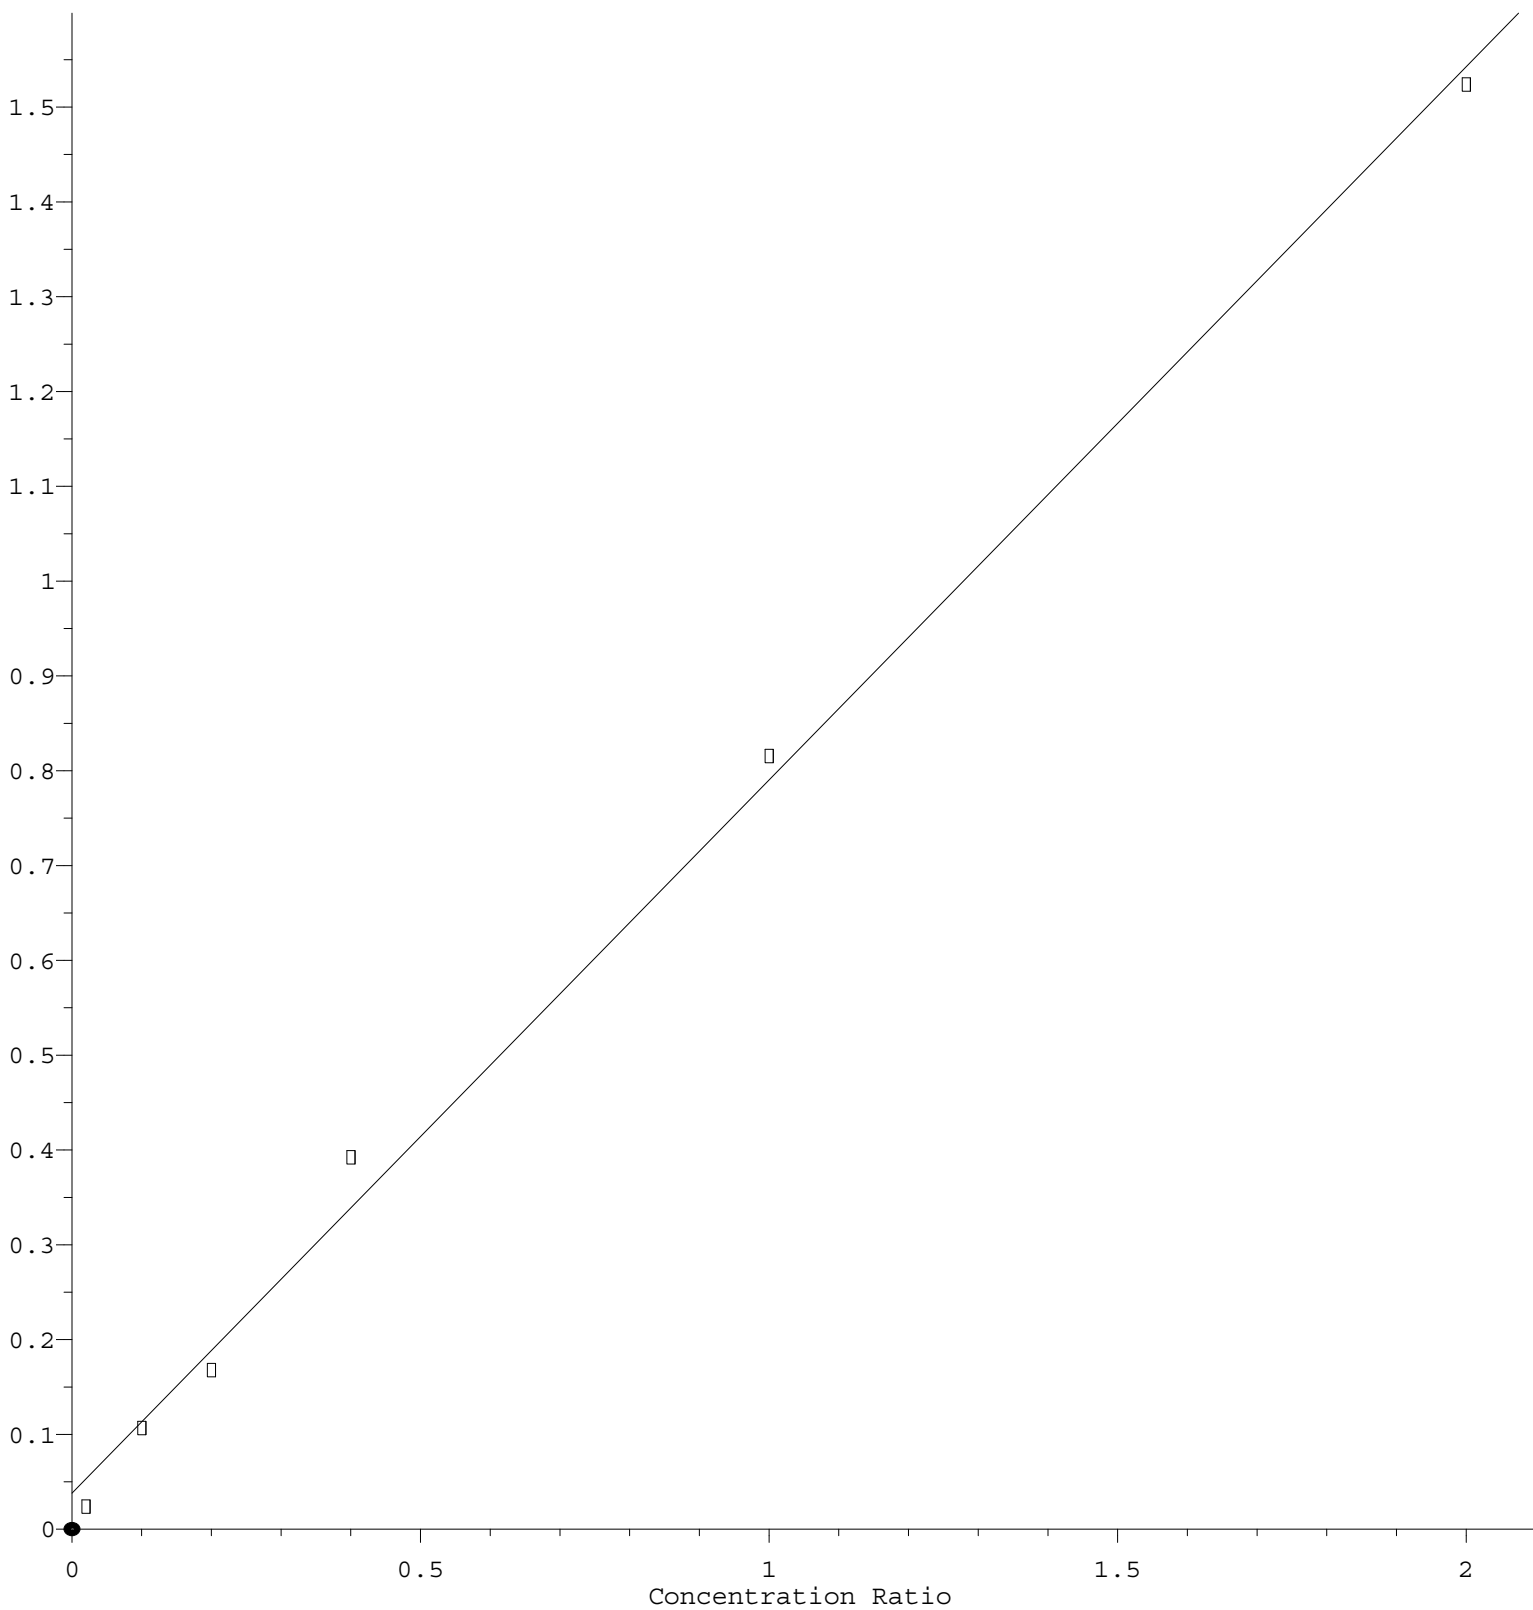

Response = 7.528e-001 * Amt + 3.815e-002
 Coef of Det (r^2) = 0.996884 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N092921W.M
 Calibration Table Last Updated: Wed Sep 29 23:31:35 2021

Bromomethane

Response Ratio

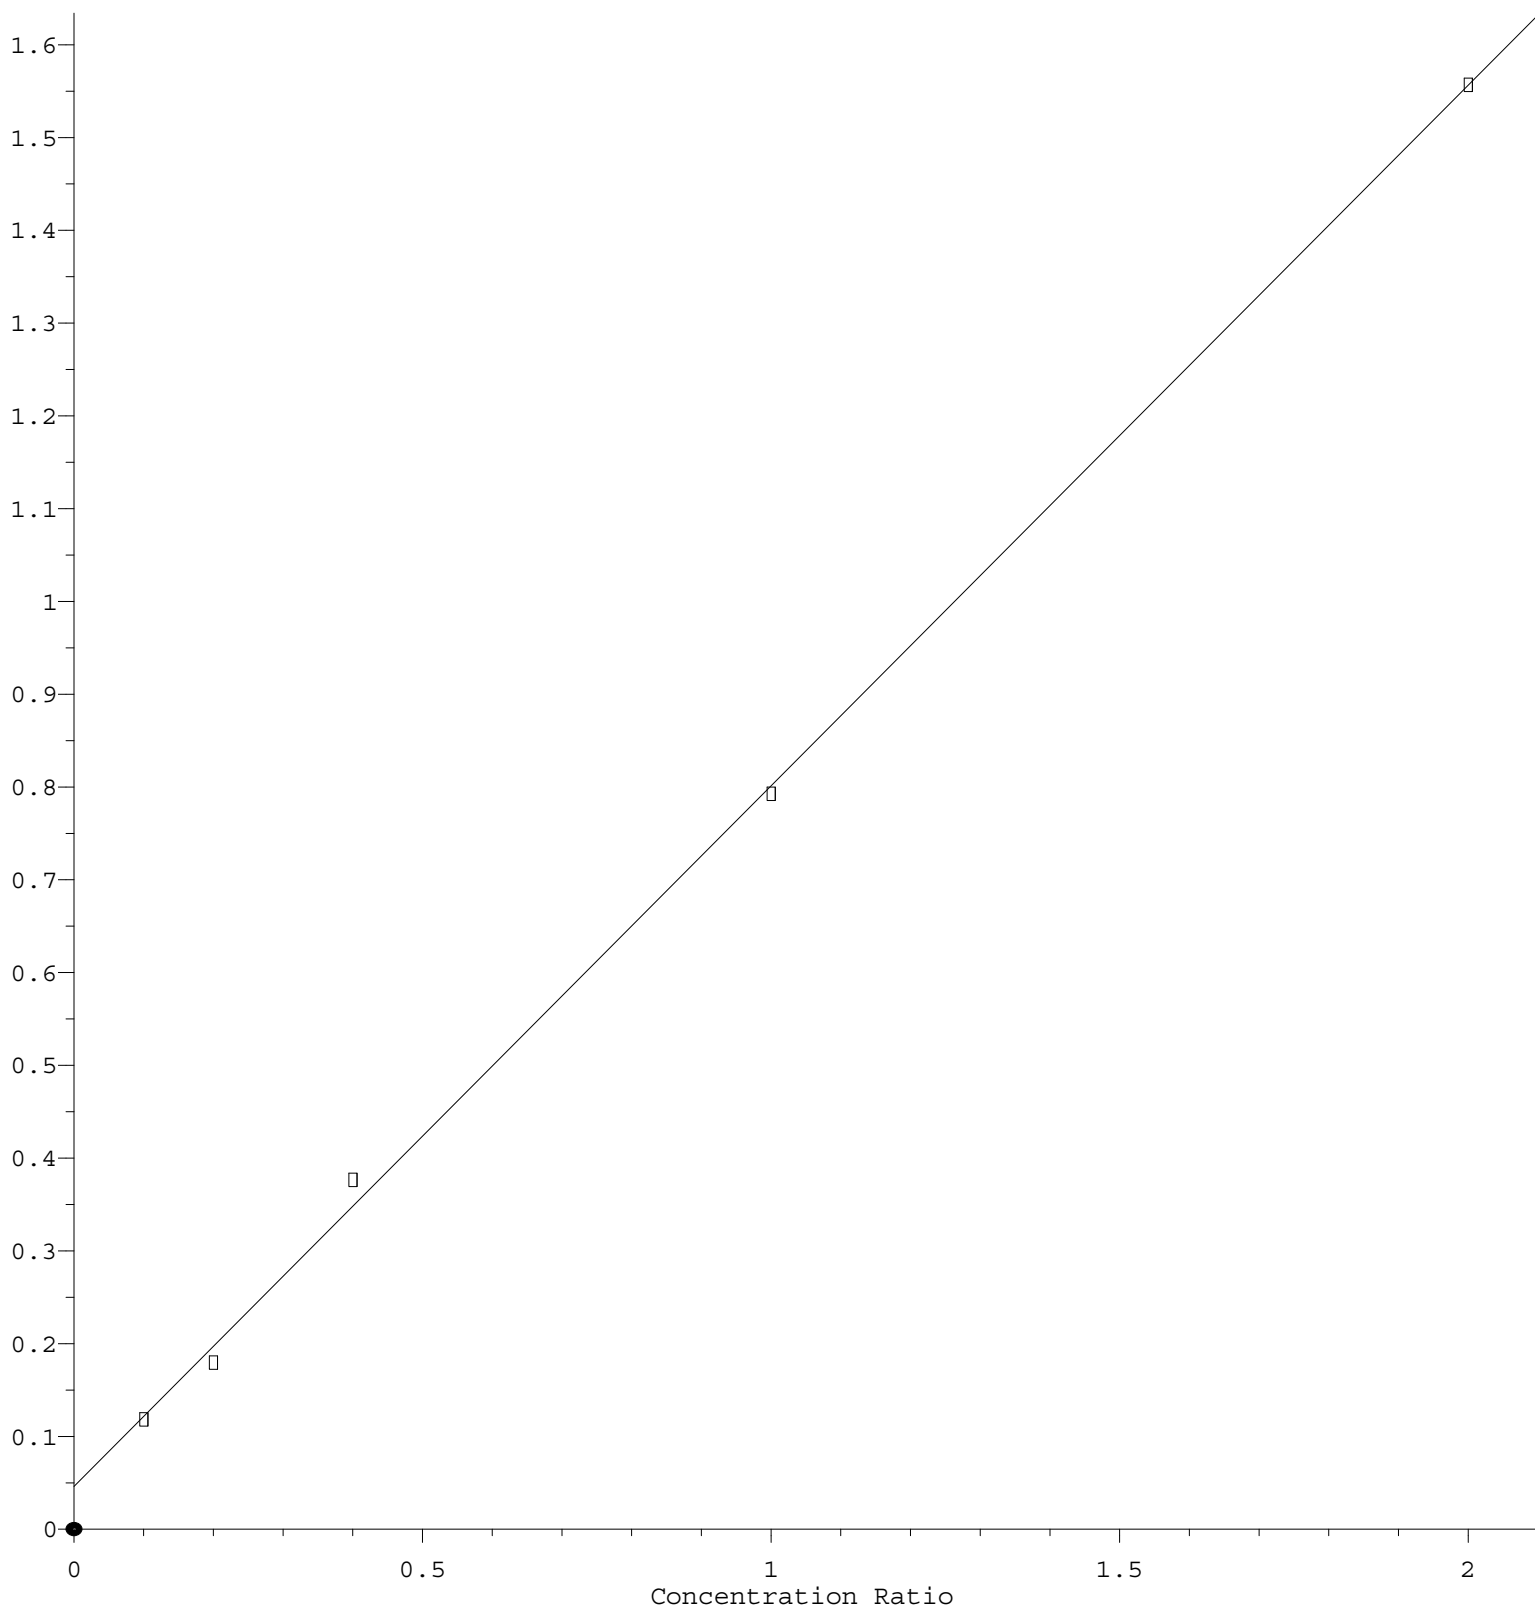

$$\text{Response} = 7.552\text{e-}001 * \text{Amt} + 4.591\text{e-}002$$


Coef of Det (r^2) = 0.999154 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N092921W.M

Calibration Table Last Updated: Wed Sep 29 23:31:35 2021

Naphthalene


Response Ratio

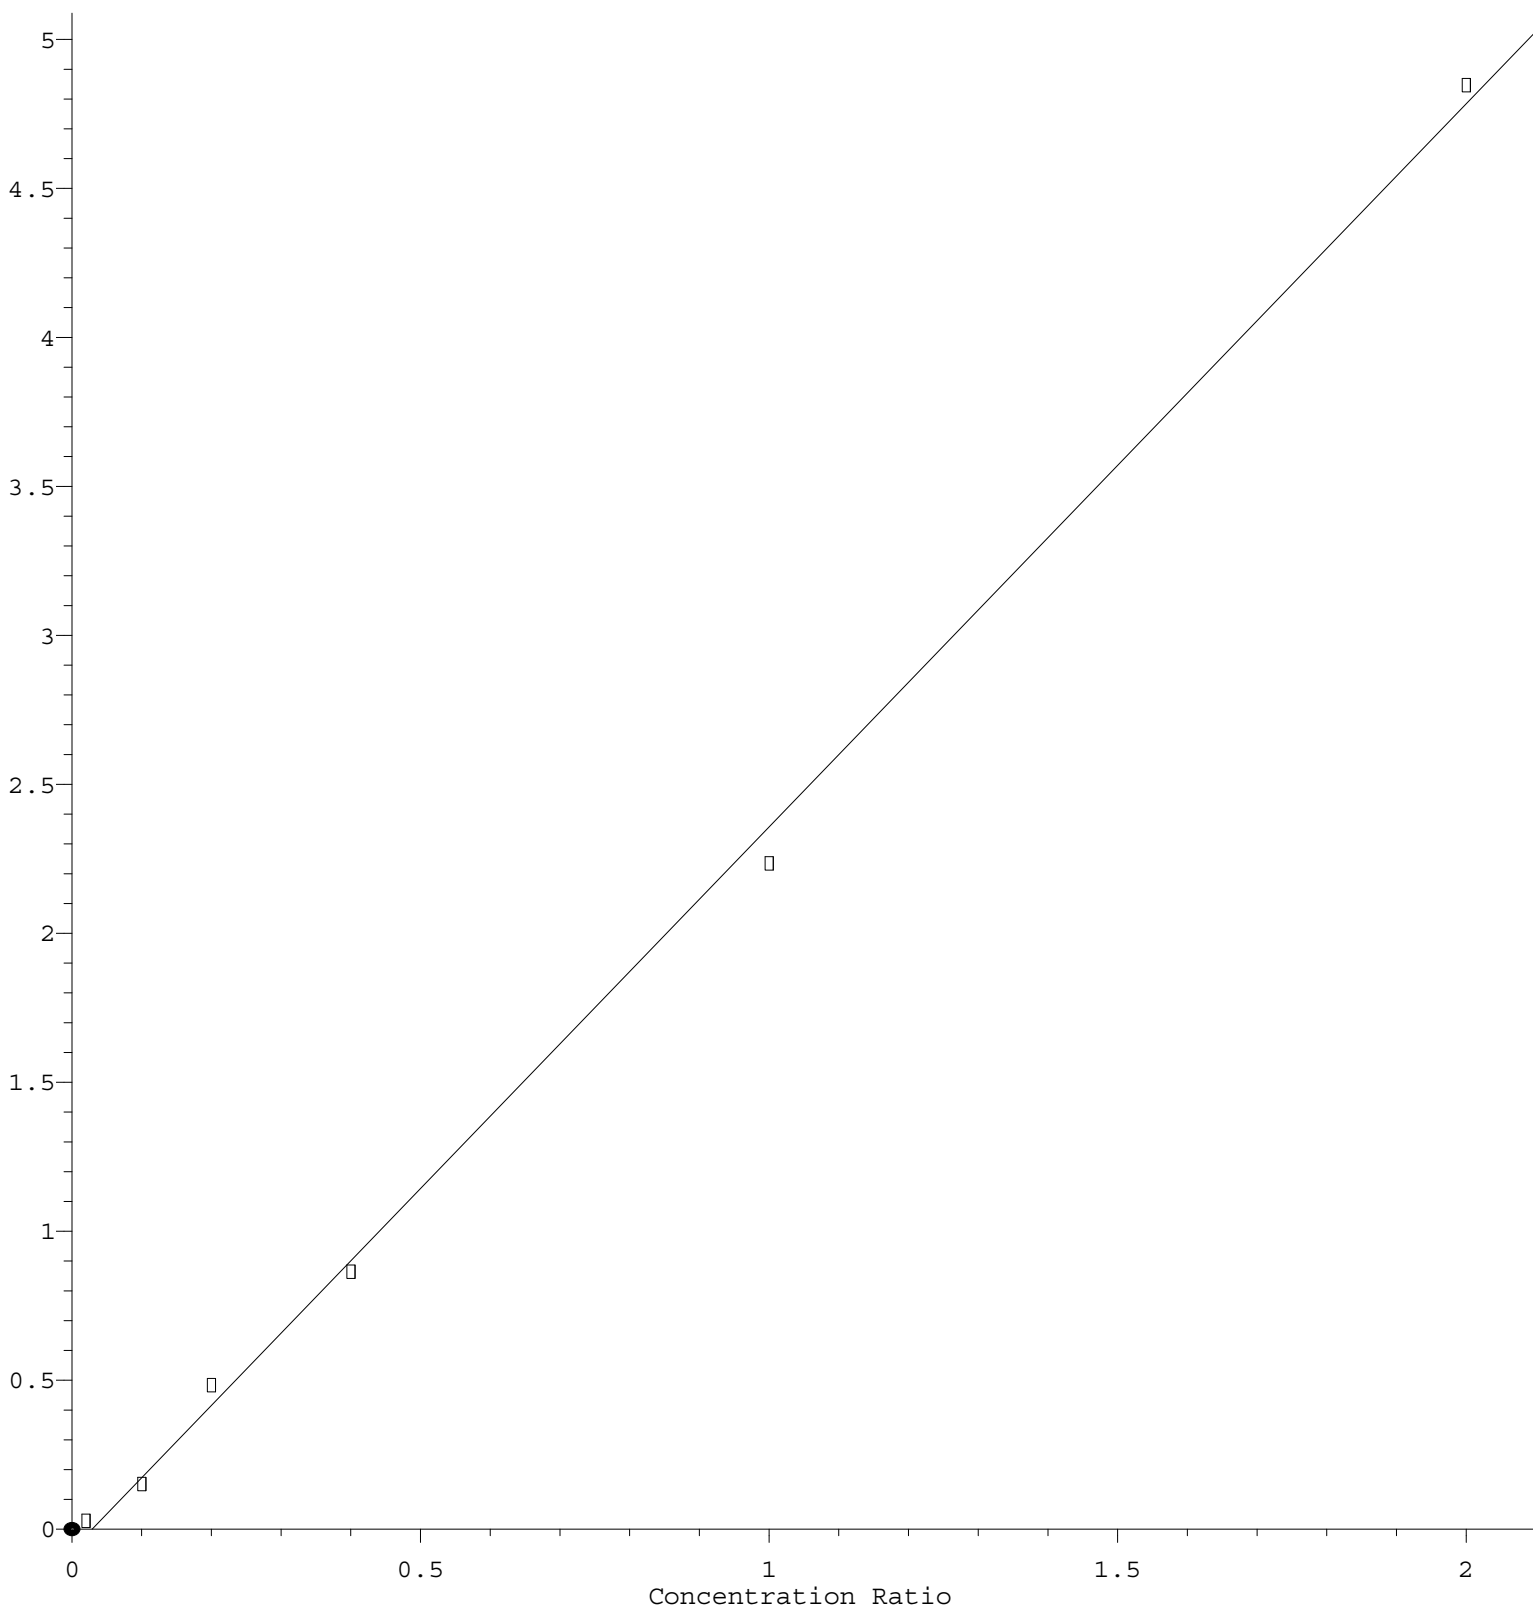

Response = 2.427e+000 * Amt - 7.024e-002
 Coef of Det (r^2) = 0.998377 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N092921W.M
 Calibration Table Last Updated: Wed Sep 29 23:31:35 2021

2-Chloroethyl Vinyl ether


Response Ratio

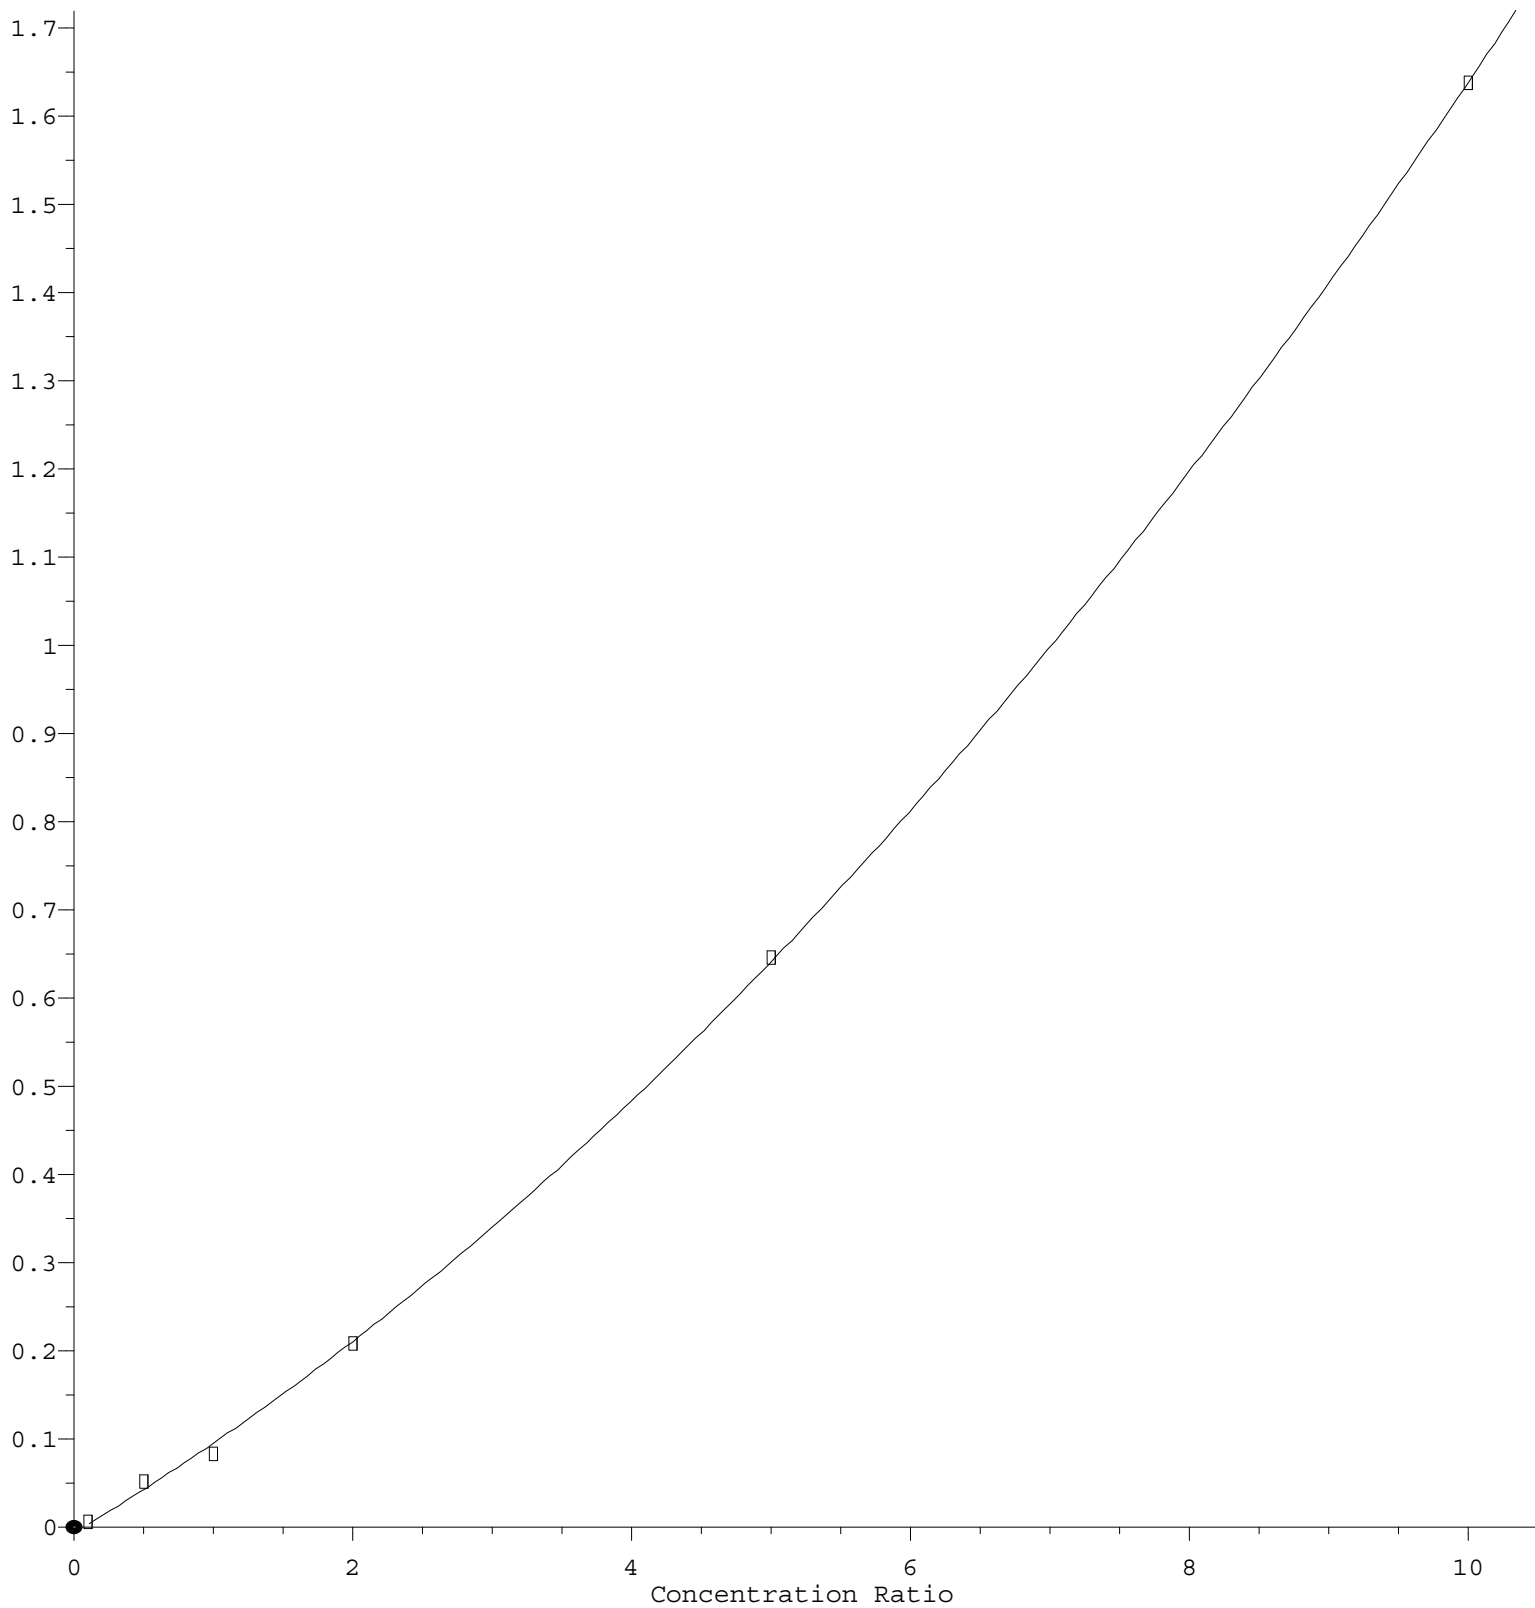

$R = 6.989e-003 A^2 + 9.458e-002 A - 6.154e-003$
 Coef of Det (r^2) = 0.999869 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N092921W.M
 Calibration Table Last Updated: Wed Sep 29 23:31:35 2021

Ethyl methacrylate

Response Ratio

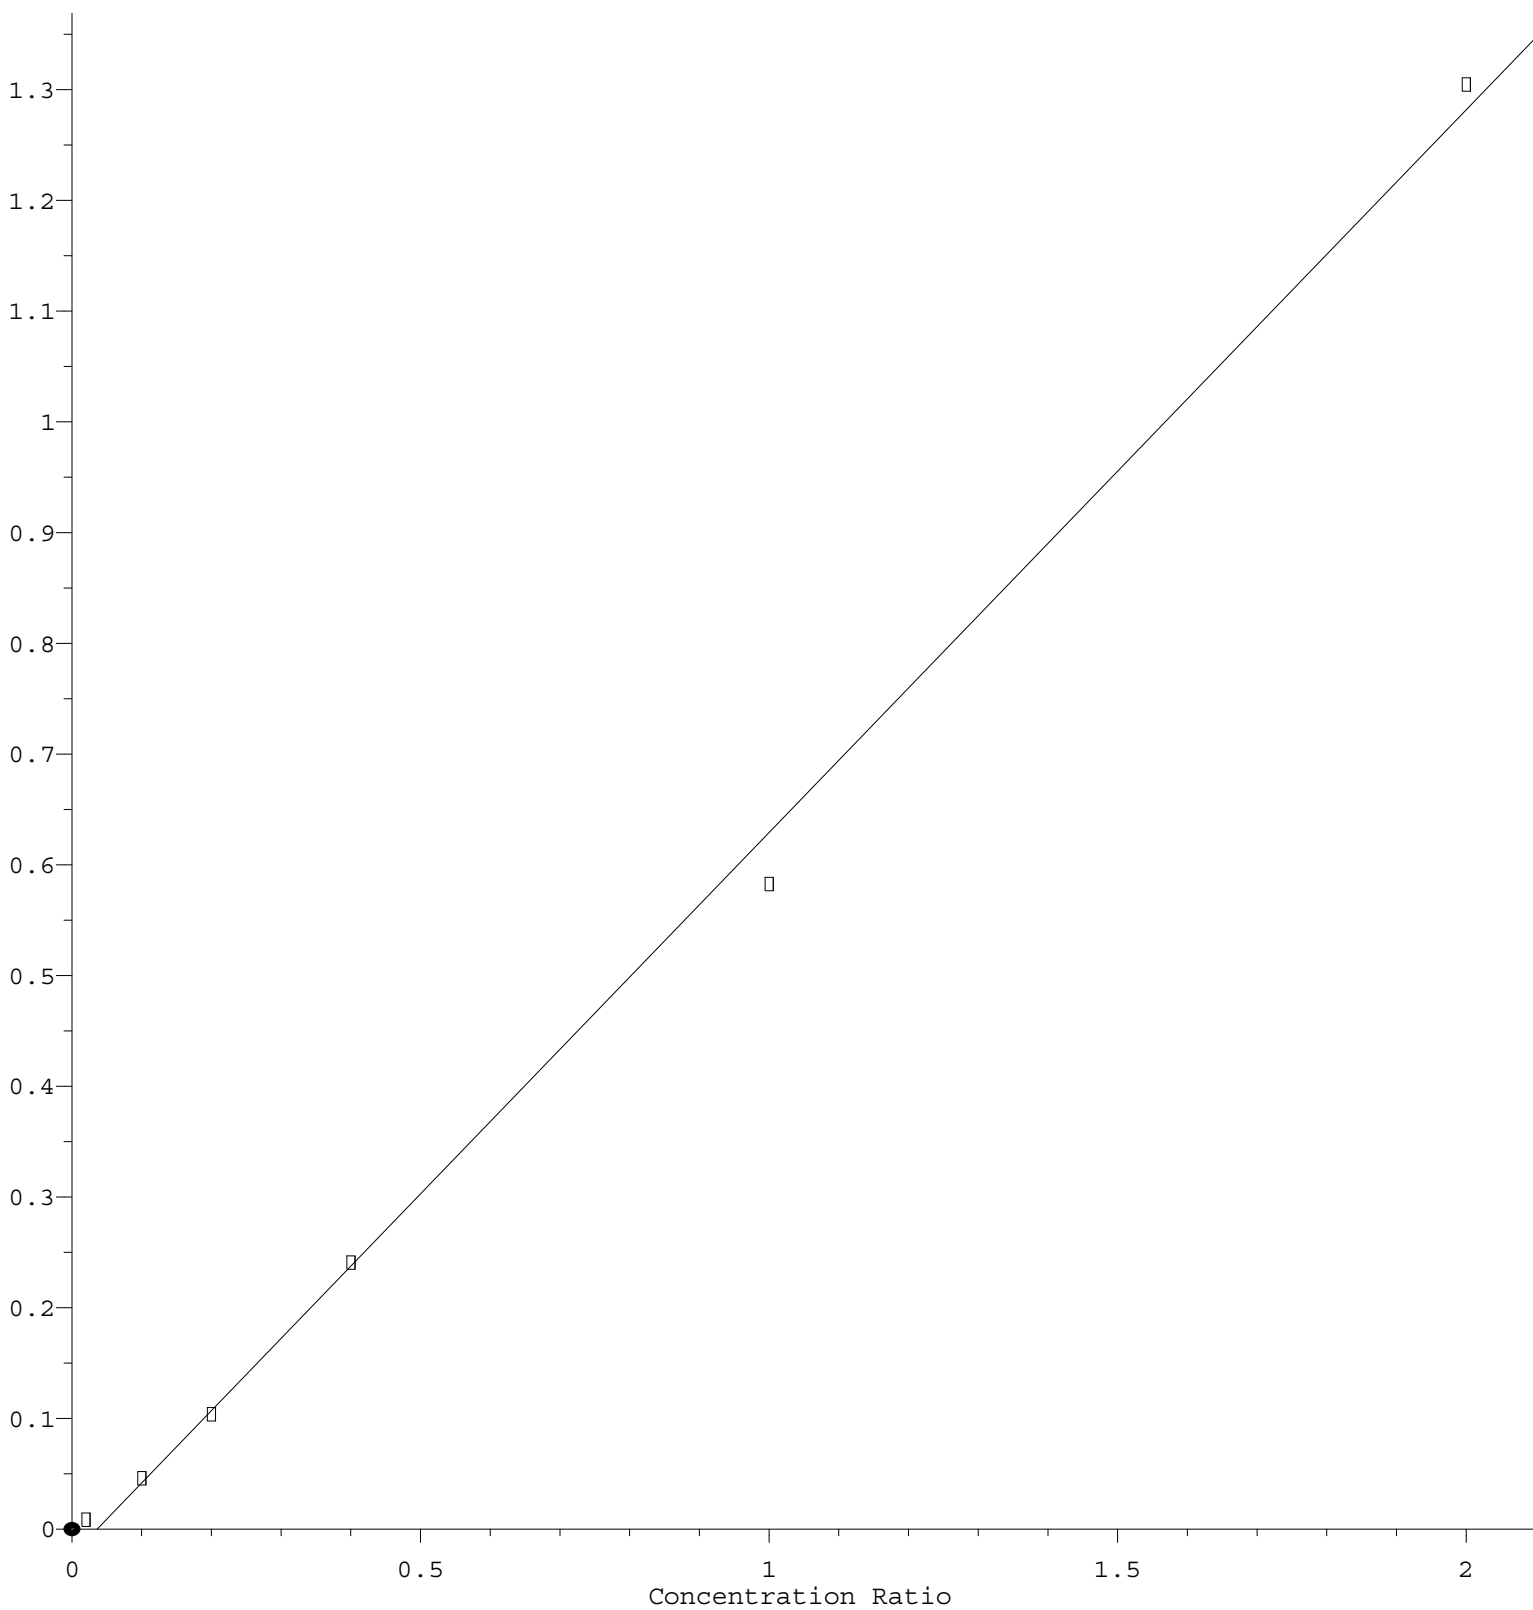

$$\text{Response} = 6.530\text{e-}001 * \text{Amt} - 2.383\text{e-}002$$


Coef of Det (r^2) = 0.997512 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N092921W.M

Calibration Table Last Updated: Wed Sep 29 23:31:35 2021

Cyclohexane

Response Ratio

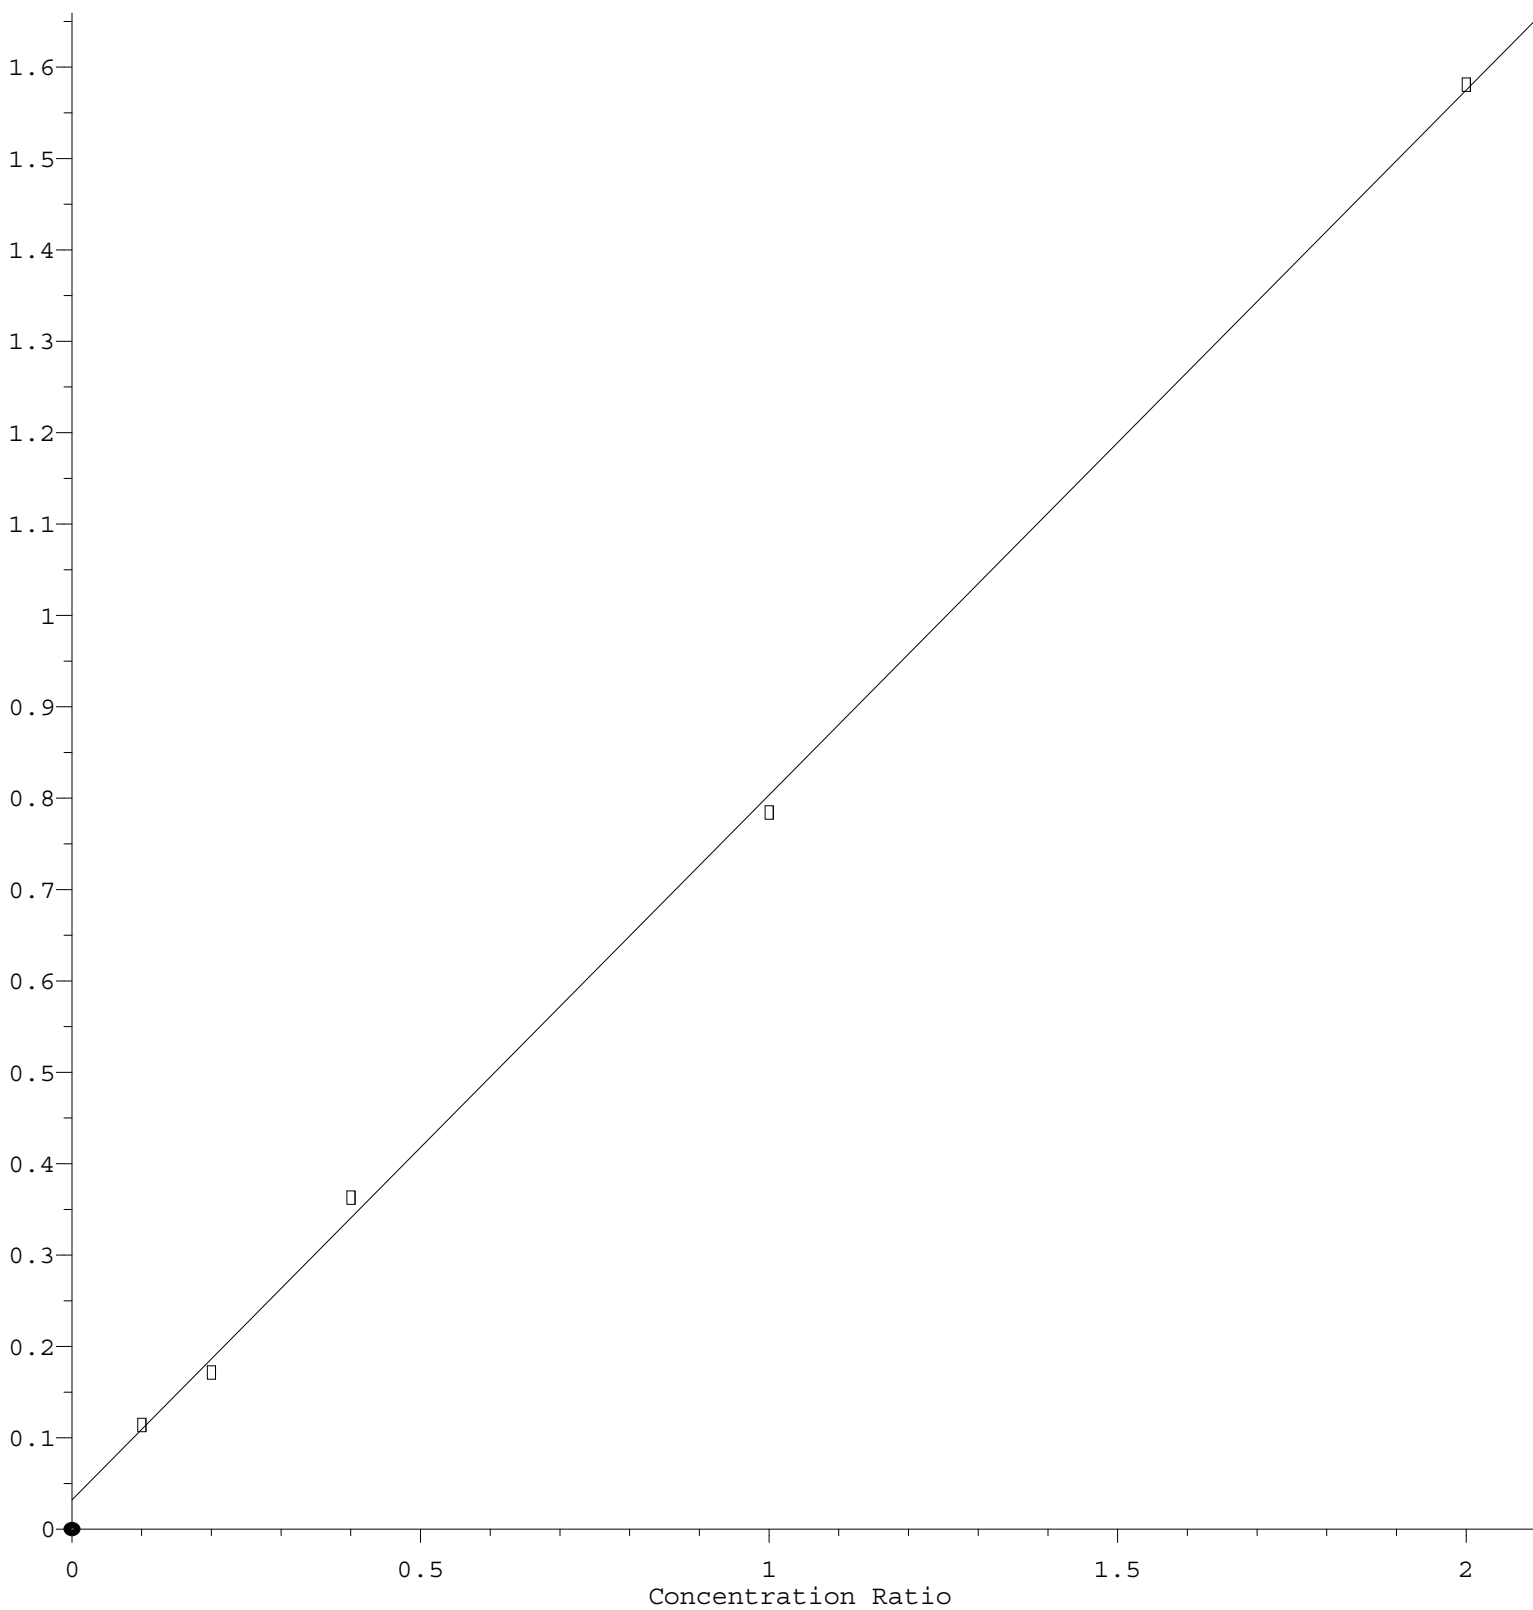

$$\text{Response} = 7.714\text{e-}001 * \text{Amt} + 3.182\text{e-}002$$


Coef of Det (r^2) = 0.999221 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N092921W.M

Calibration Table Last Updated: Wed Sep 29 23:31:35 2021

Carbon Disulfide

Response Ratio

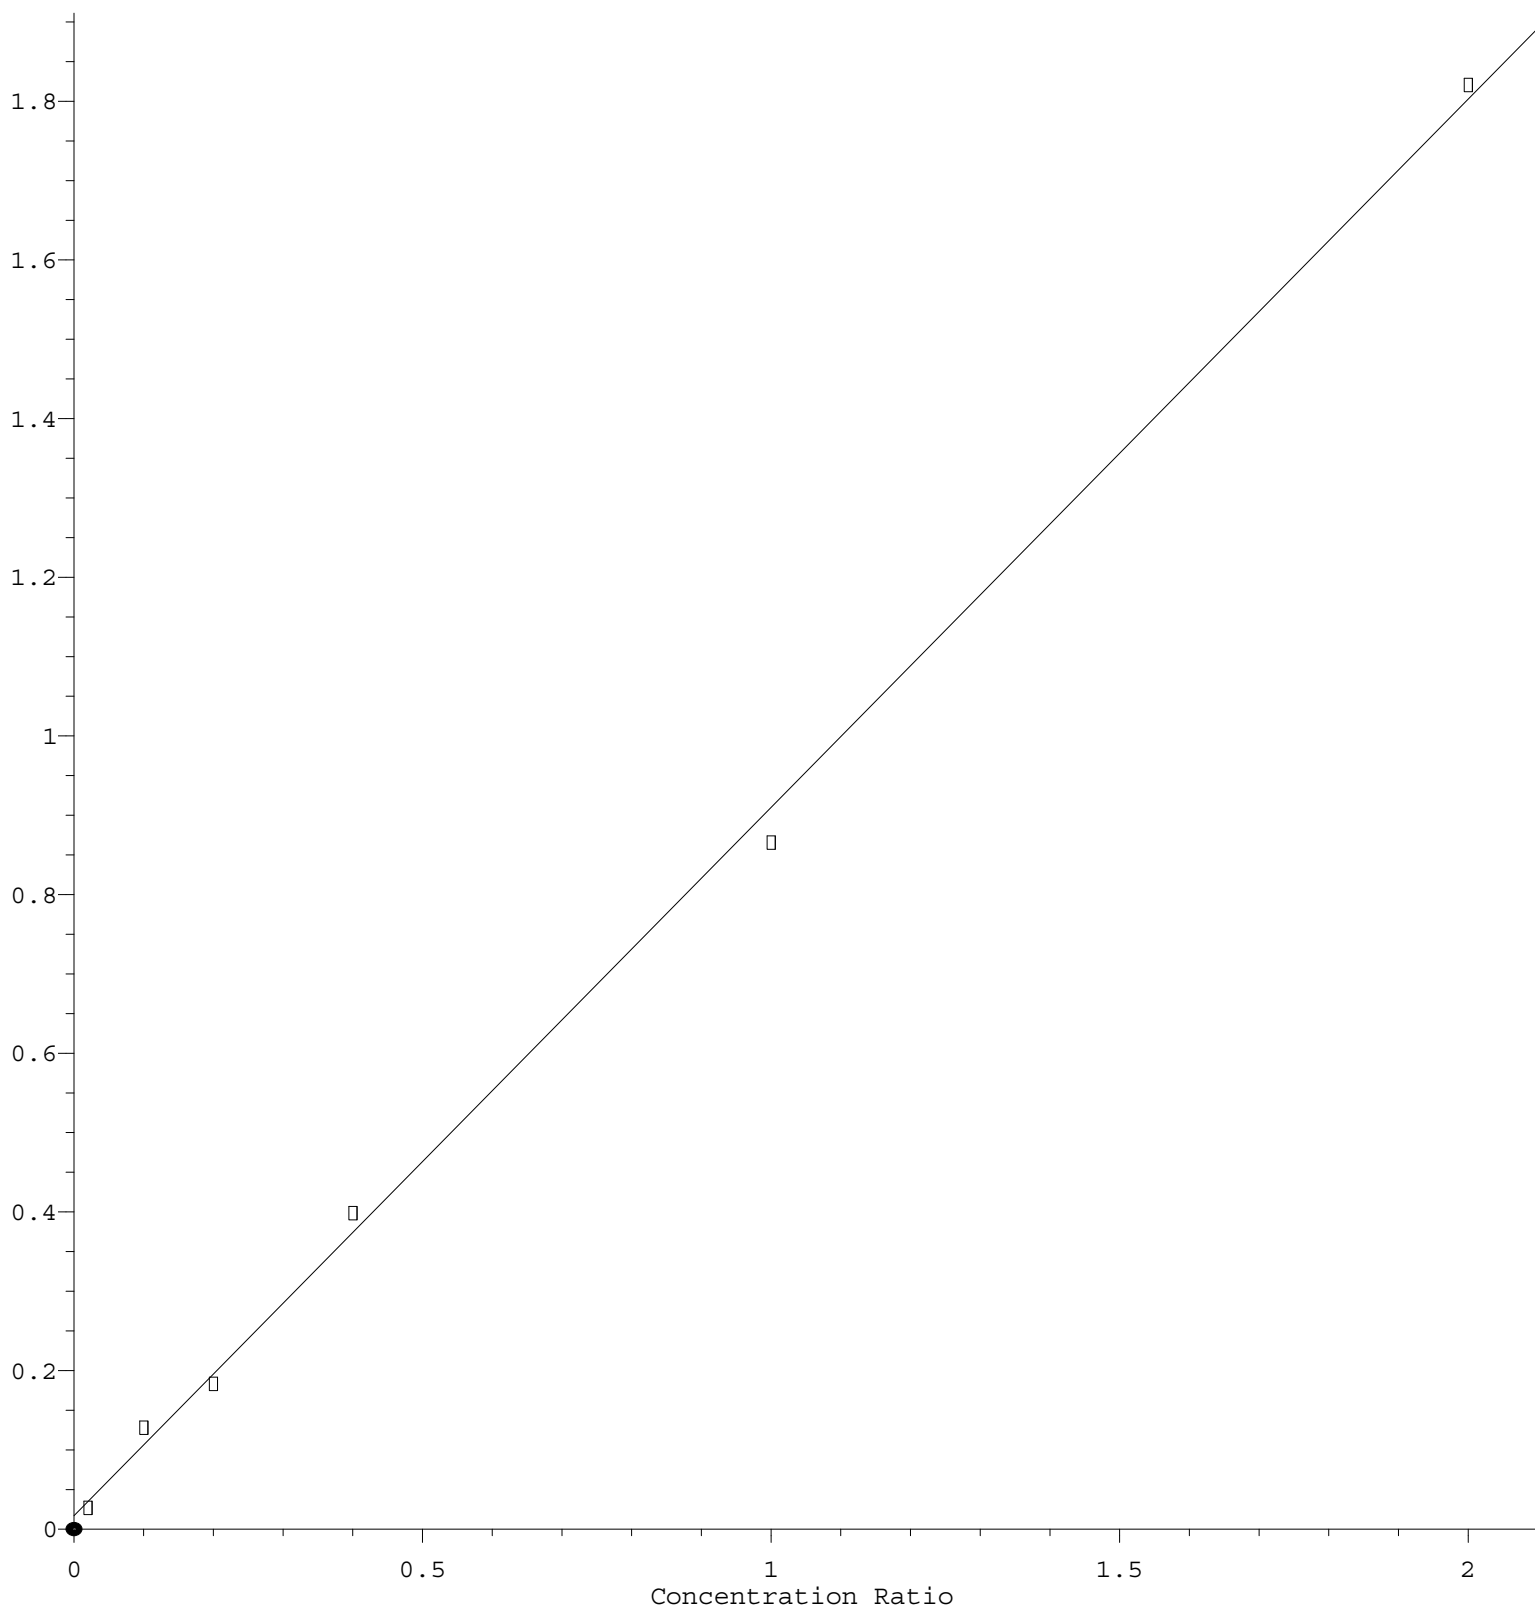

$$\text{Response} = 8.932\text{e-}001 * \text{Amt} + 1.659\text{e-}002$$


Coef of Det (r^2) = 0.998471 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N092921W.M

Calibration Table Last Updated: Wed Sep 29 23:31:35 2021


Acetone

Response Ratio

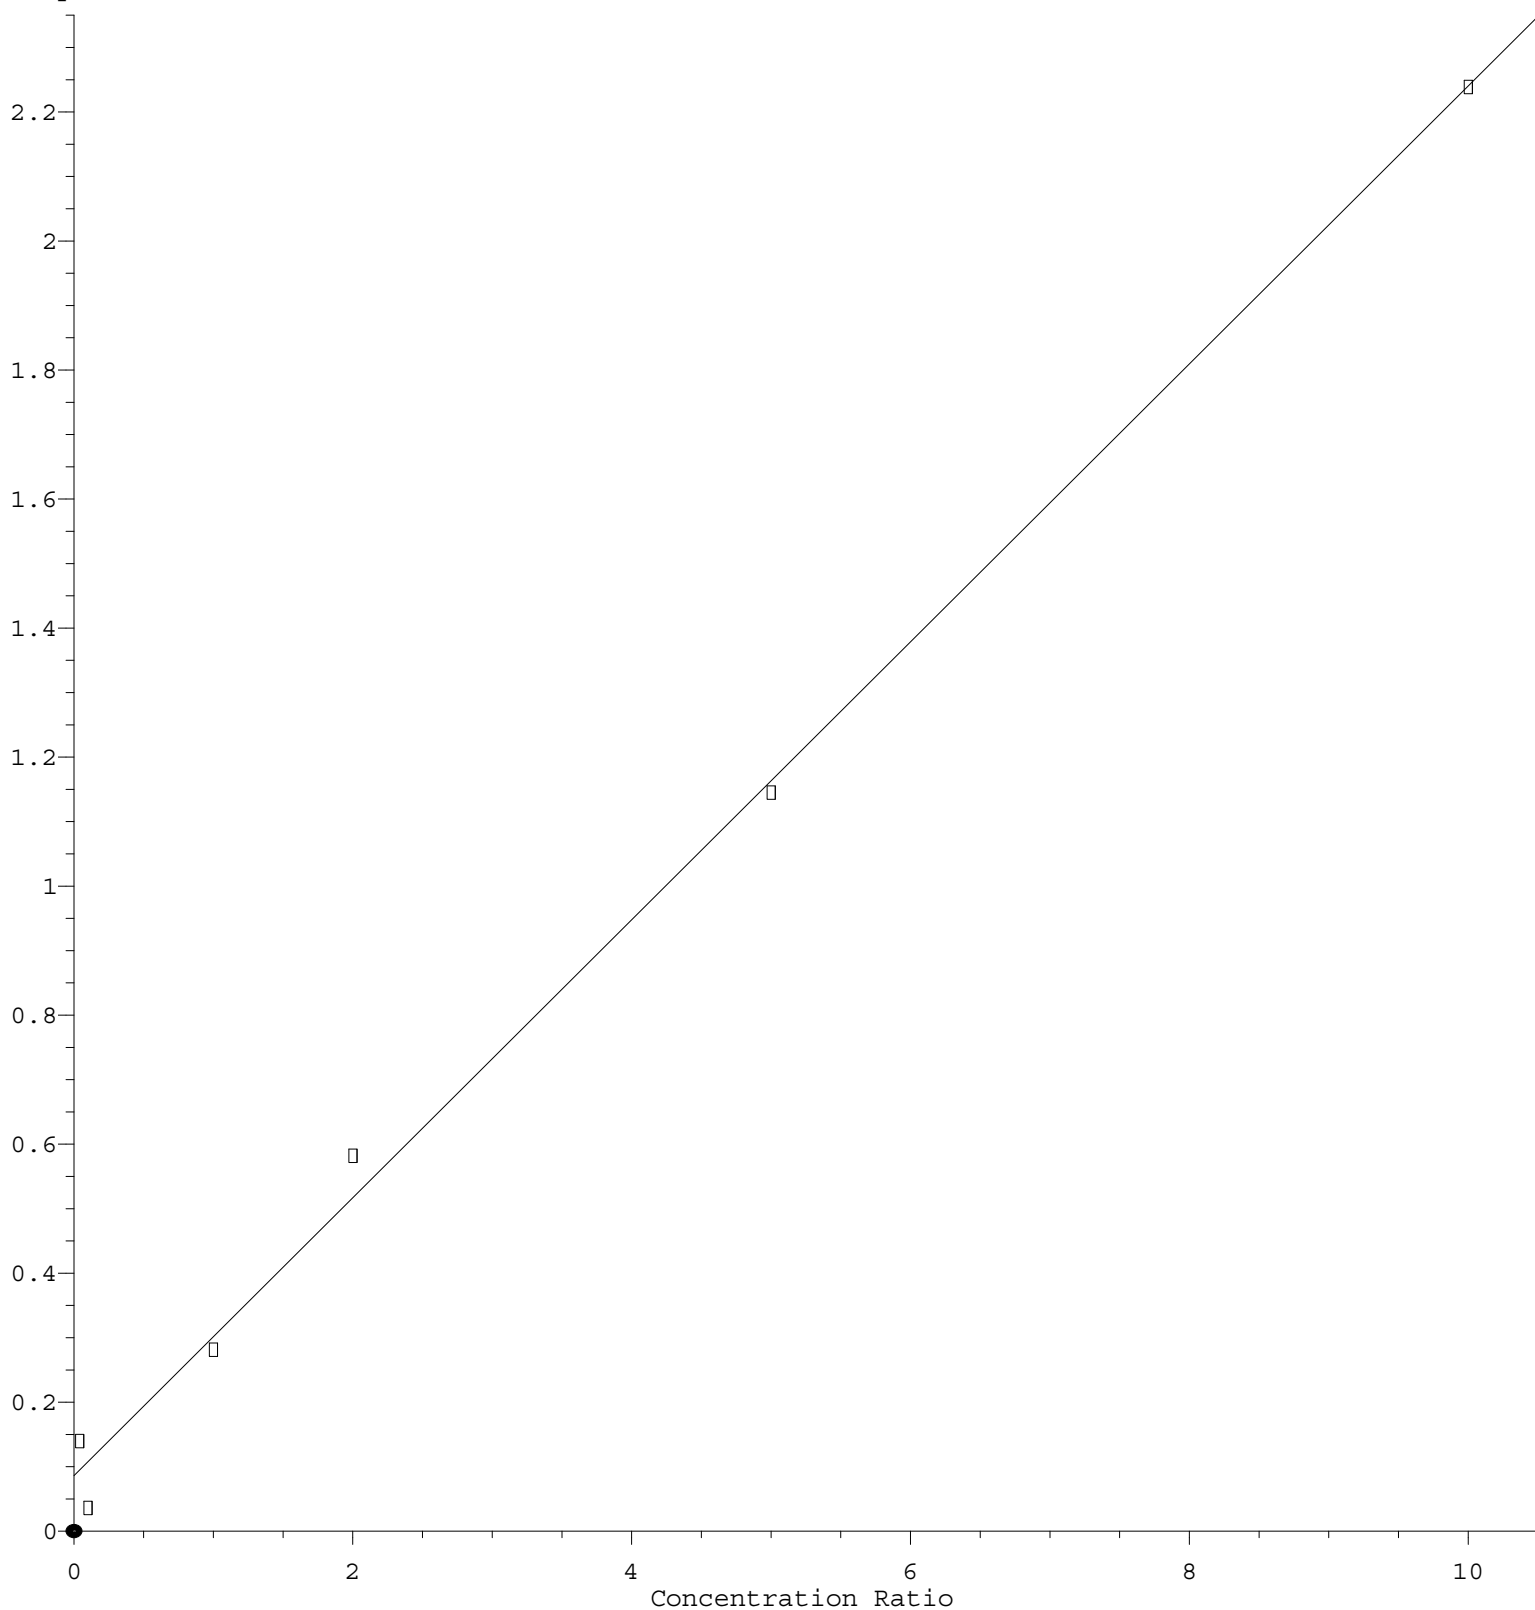

$\text{Response} = 2.154\text{e-}001 * \text{Amt} + 8.568\text{e-}002$
 Coef of Det (r^2) = 0.996530 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N092921W.M
 Calibration Table Last Updated: Wed Sep 29 23:31:35 2021

Acrolein

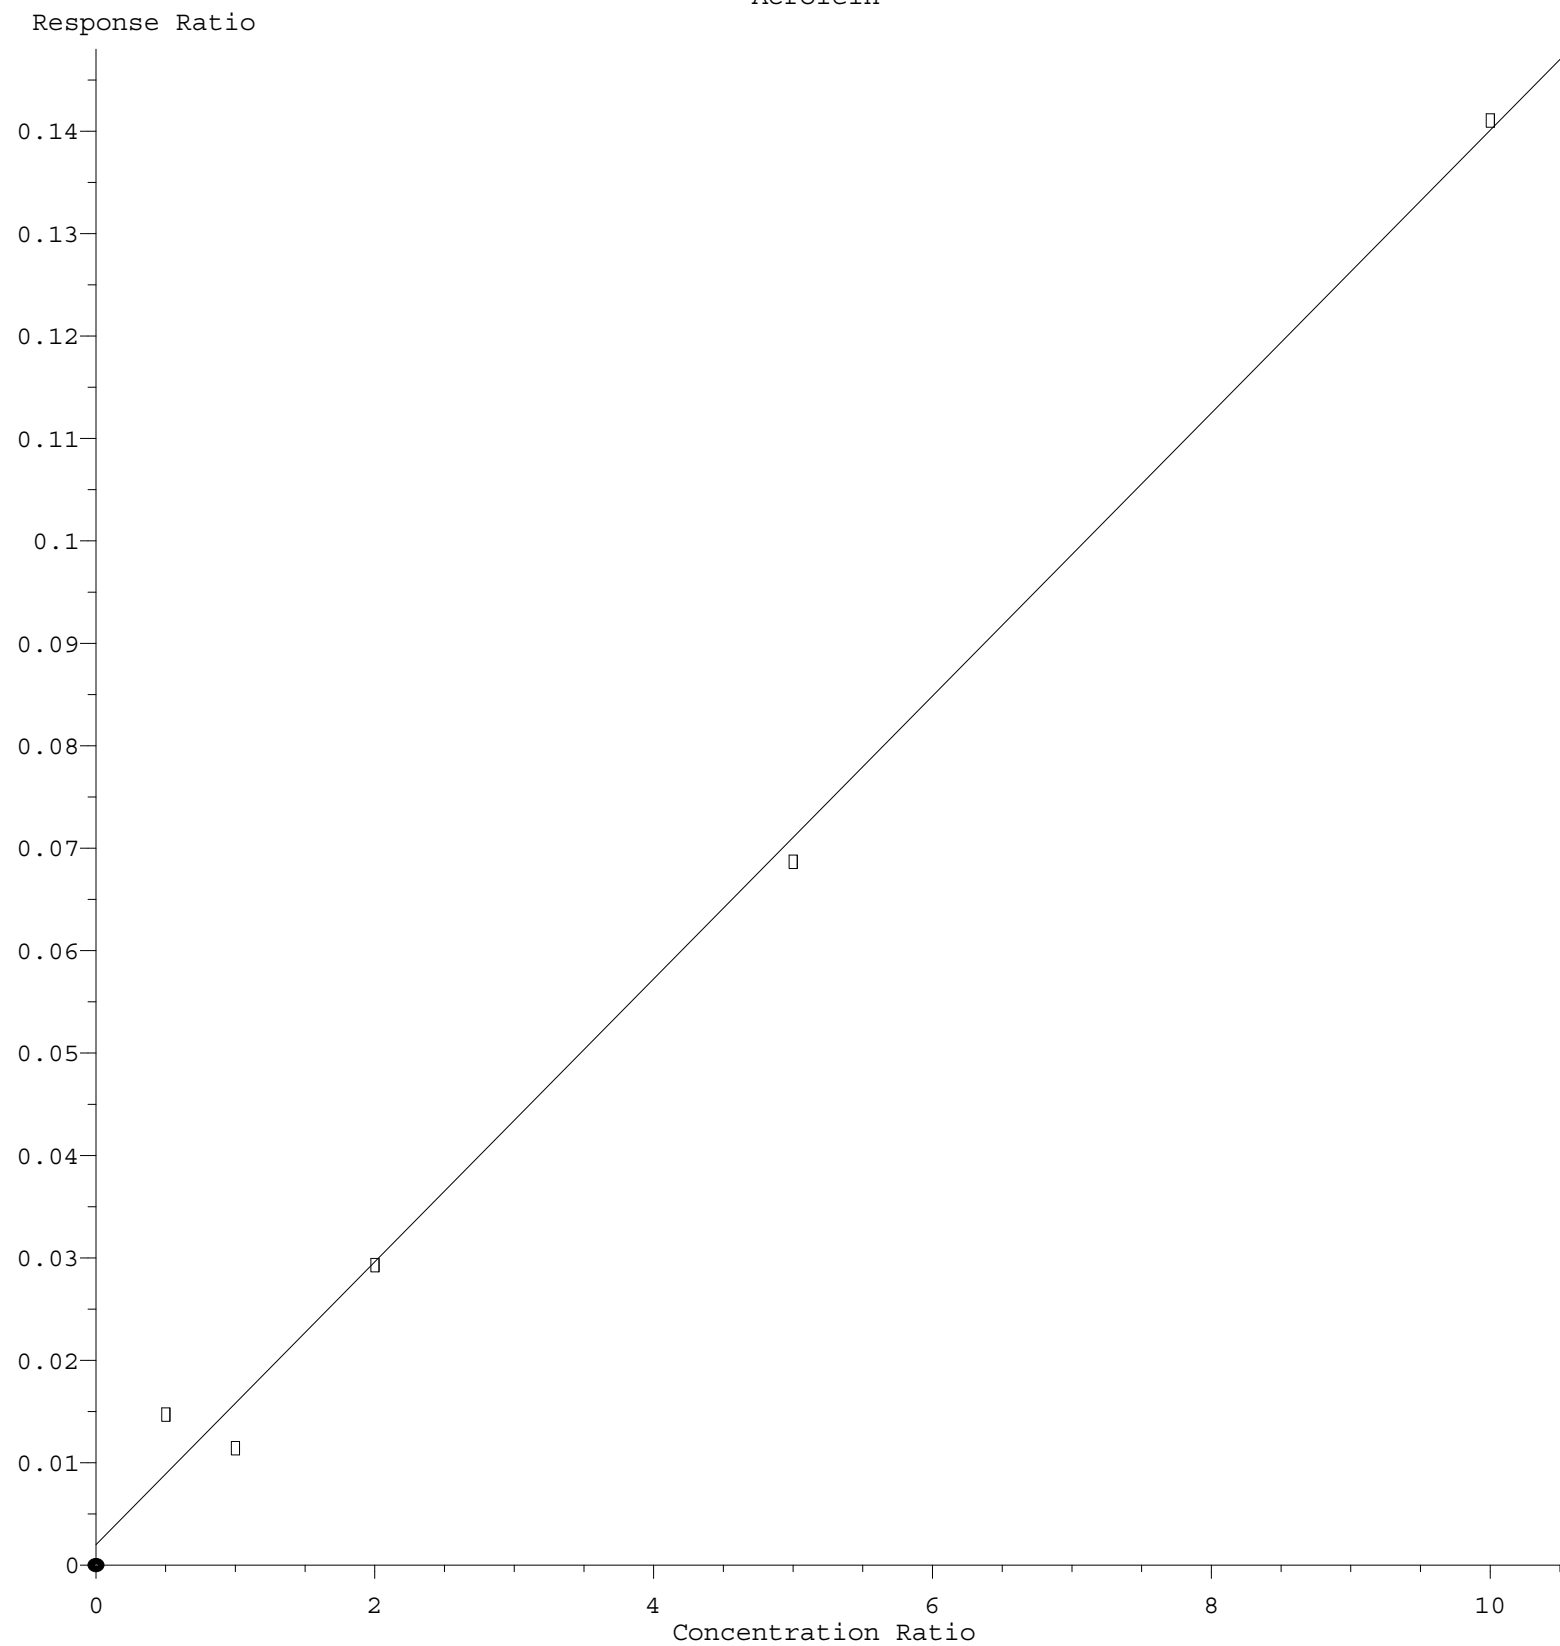

Response = 1.376e-002 * Amt + 2.130e-003
 Coef of Det (r^2) = 0.994953 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N092921W.M
 Calibration Table Last Updated: Wed Sep 29 23:31:35 2021