
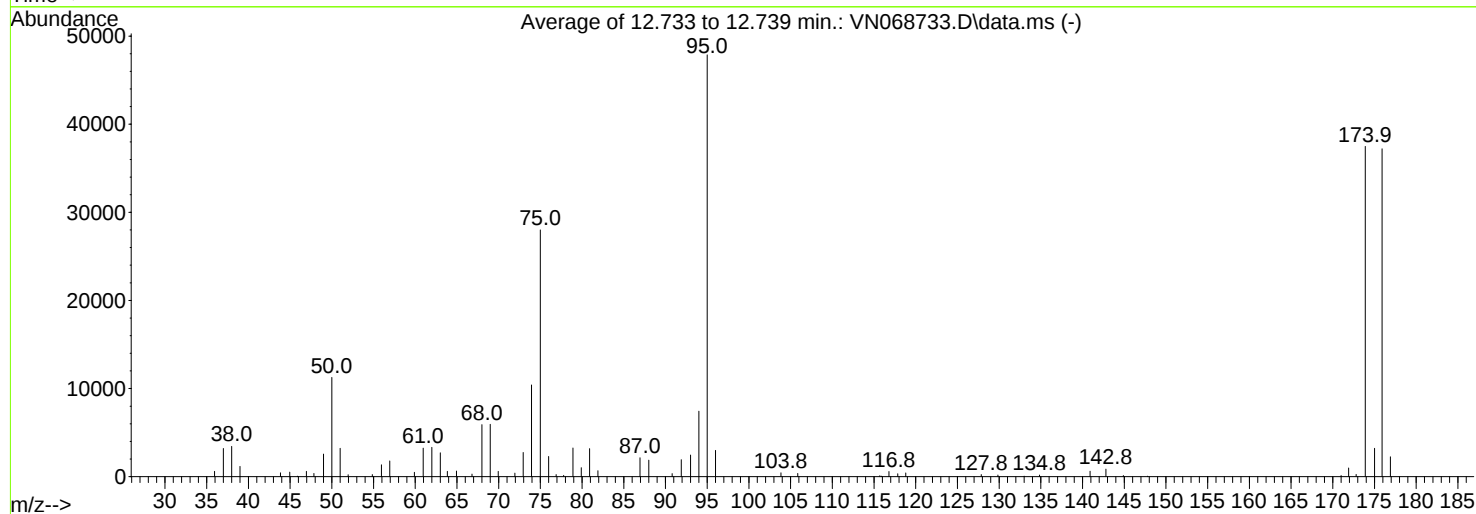


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092921\
 Data File : VN068733.D
 Acq On : 29 Sep 2021 11:07
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N092921W.M
 Title : SW846 8260
 Last Update : Wed Sep 29 23:31:35 2021

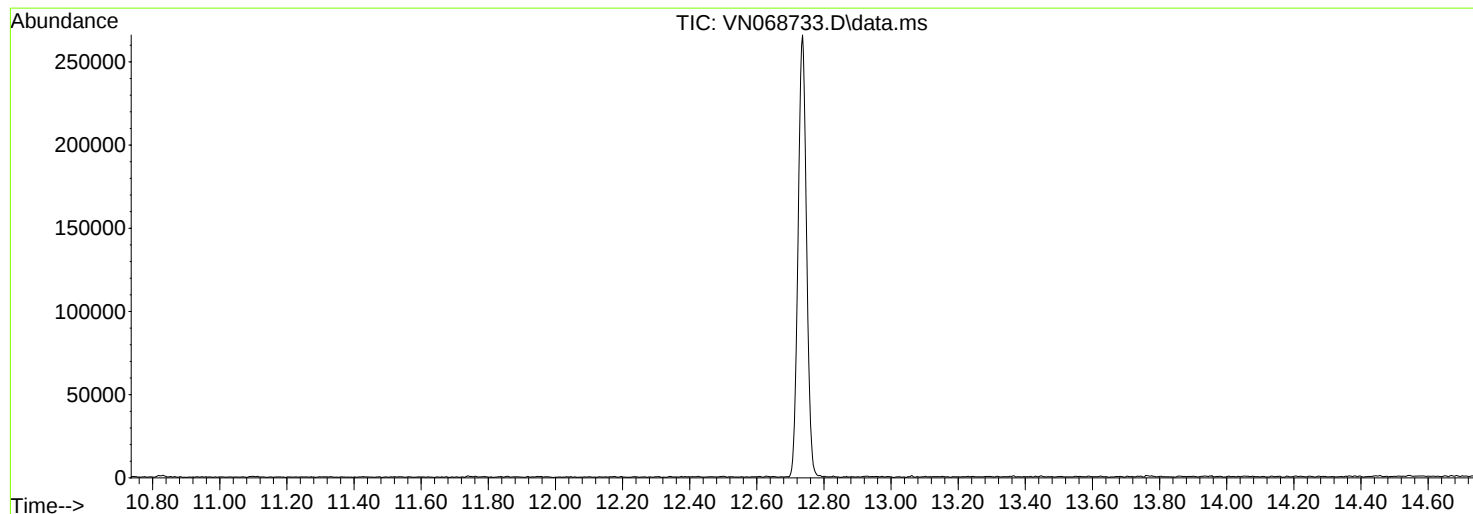

AutoFind: Scans 4006, 4007, 4008; Background Corrected with Scan 3990

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.5	11252	PASS
75	95	30	60	58.5	28008	PASS
95	95	100	100	100.0	47875	PASS
96	95	5	9	6.2	2980	PASS
173	174	0.00	2	0.7	258	PASS
174	95	50	100	78.3	37480	PASS
175	174	5	9	8.6	3208	PASS
176	174	95	101	99.3	37208	PASS
177	176	5	9	6.1	2259	PASS