


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092922\
Data File : VN074650.D
Acq On : 29 Sep 2022 08:45
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N092922W.M
Title : SW846 8260
Last Update : Fri Sep 30 07:44:59 2022

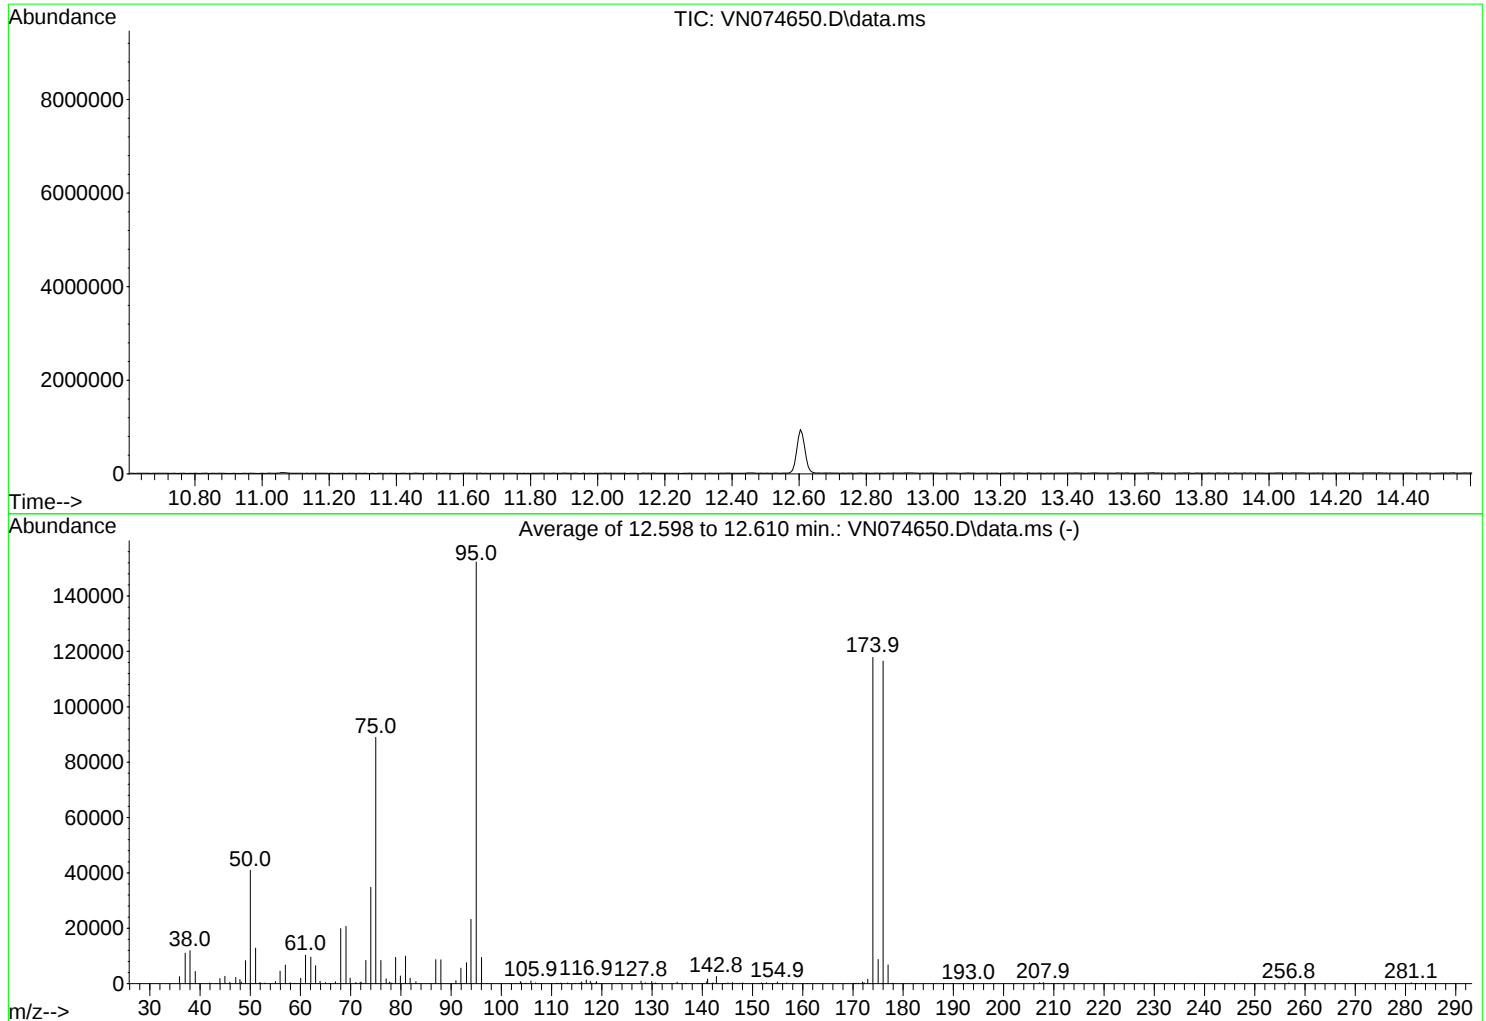

AutoFind: Scans 1957, 1958, 1959; Background Corrected with Scan 1948

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	26.9	40909	PASS
75	95	30	60	58.4	88928	PASS
95	95	100	100	100.0	152341	PASS
96	95	5	9	6.2	9484	PASS
173	174	0.00	2	1.4	1603	PASS
174	95	50	100	77.4	117840	PASS
175	174	5	9	7.4	8743	PASS
176	174	95	101	98.9	116515	PASS
177	176	5	9	5.8	6784	PASS