

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092925\
 Data File : VN087977.D
 Acq On : 29 Sep 2025 13:08
 Operator : JC\MD
 Sample : VN0929WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0929WBL01

Quant Time: Sep 30 03:52:56 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N092325W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 24 05:05:30 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.212	168	158754	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.088	114	351007	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.847	117	338452	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.770	152	154688	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.565	65	161783	60.554	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 121.100%			
35) Dibromofluoromethane	8.153	113	131718	51.684	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 103.360%			
50) Toluene-d8	10.547	98	448783	50.076	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 100.160%			
62) 4-Bromofluorobenzene	12.829	95	142869	44.598	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 89.200%			
Target Compounds						
					Qvalue	
5) Bromomethane	2.983	94	498	0.418	ug/l	87
10) Methyl Iodide	4.583	142	408	0.274	ug/l #	40
11) Tert butyl alcohol	5.494	59	78	0.203	ug/l #	71
13) Acrolein	4.183	56	543	1.100	ug/l #	12
15) Acrylonitrile	5.712	53	339	0.281	ug/l #	1
16) Acetone	4.424	43	2016	1.834	ug/l #	83
17) Carbon Disulfide	4.706	76	3672	0.705	ug/l #	76
18) Methyl Acetate	5.024	43	783	0.285	ug/l #	74
20) Methylene Chloride	5.259	84	1083	0.487	ug/l #	64
21) trans-1,2-Dichloroethene	5.765	96	1035	0.506	ug/l #	53
25) 2-Butanone	7.477	43	489	0.291	ug/l #	48
29) Tetrahydrofuran	7.841	42	399	0.371	ug/l #	58
31) Cyclohexane	8.206	56	4873	1.627	ug/l #	22
36) 1,1-Dichloropropene	8.206	75	14332	4.677	ug/l #	51
38) Carbon Tetrachloride	8.206	117	18144	5.160	ug/l #	19
42) 1,2-Dichloroethane	8.671	62	846	0.223	ug/l #	74
76) 1,2,3-Trichloropropane	12.829	75	81905	26.861	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.829	75	81905	74.588	ug/l #	9
83) tert-Butylbenzene	13.412	119	1565	0.223	ug/l #	87
85) sec-Butylbenzene	13.594	105	2456	0.239	ug/l	88
86) p-Isopropyltoluene	13.712	119	1752	0.201	ug/l #	84
87) 1,3-Dichlorobenzene	13.723	146	1326	0.266	ug/l	86
88) 1,4-Dichlorobenzene	13.723	146	1326	0.259	ug/l	85
89) n-Butylbenzene	14.041	91	1811	0.220	ug/l #	63
90) Hexachloroethane	14.306	117	668	0.367	ug/l	70
93) 1,2,4-Trichlorobenzene	15.376	180	1285	0.454	ug/l	95
94) Hexachlorobutadiene	15.470	225	213	0.204	ug/l #	1
95) Naphthalene	15.617	128	3347	0.368	ug/l #	76
96) 1,2,3-Trichlorobenzene	15.817	180	1567	0.569	ug/l	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092925\
Data File : VN087977.D
Acq On : 29 Sep 2025 13:08
Operator : JC\MD
Sample : VN0929WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0929WBL01

Quant Time: Sep 30 03:52:56 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N092325W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 24 05:05:30 2025
Response via : Initial Calibration




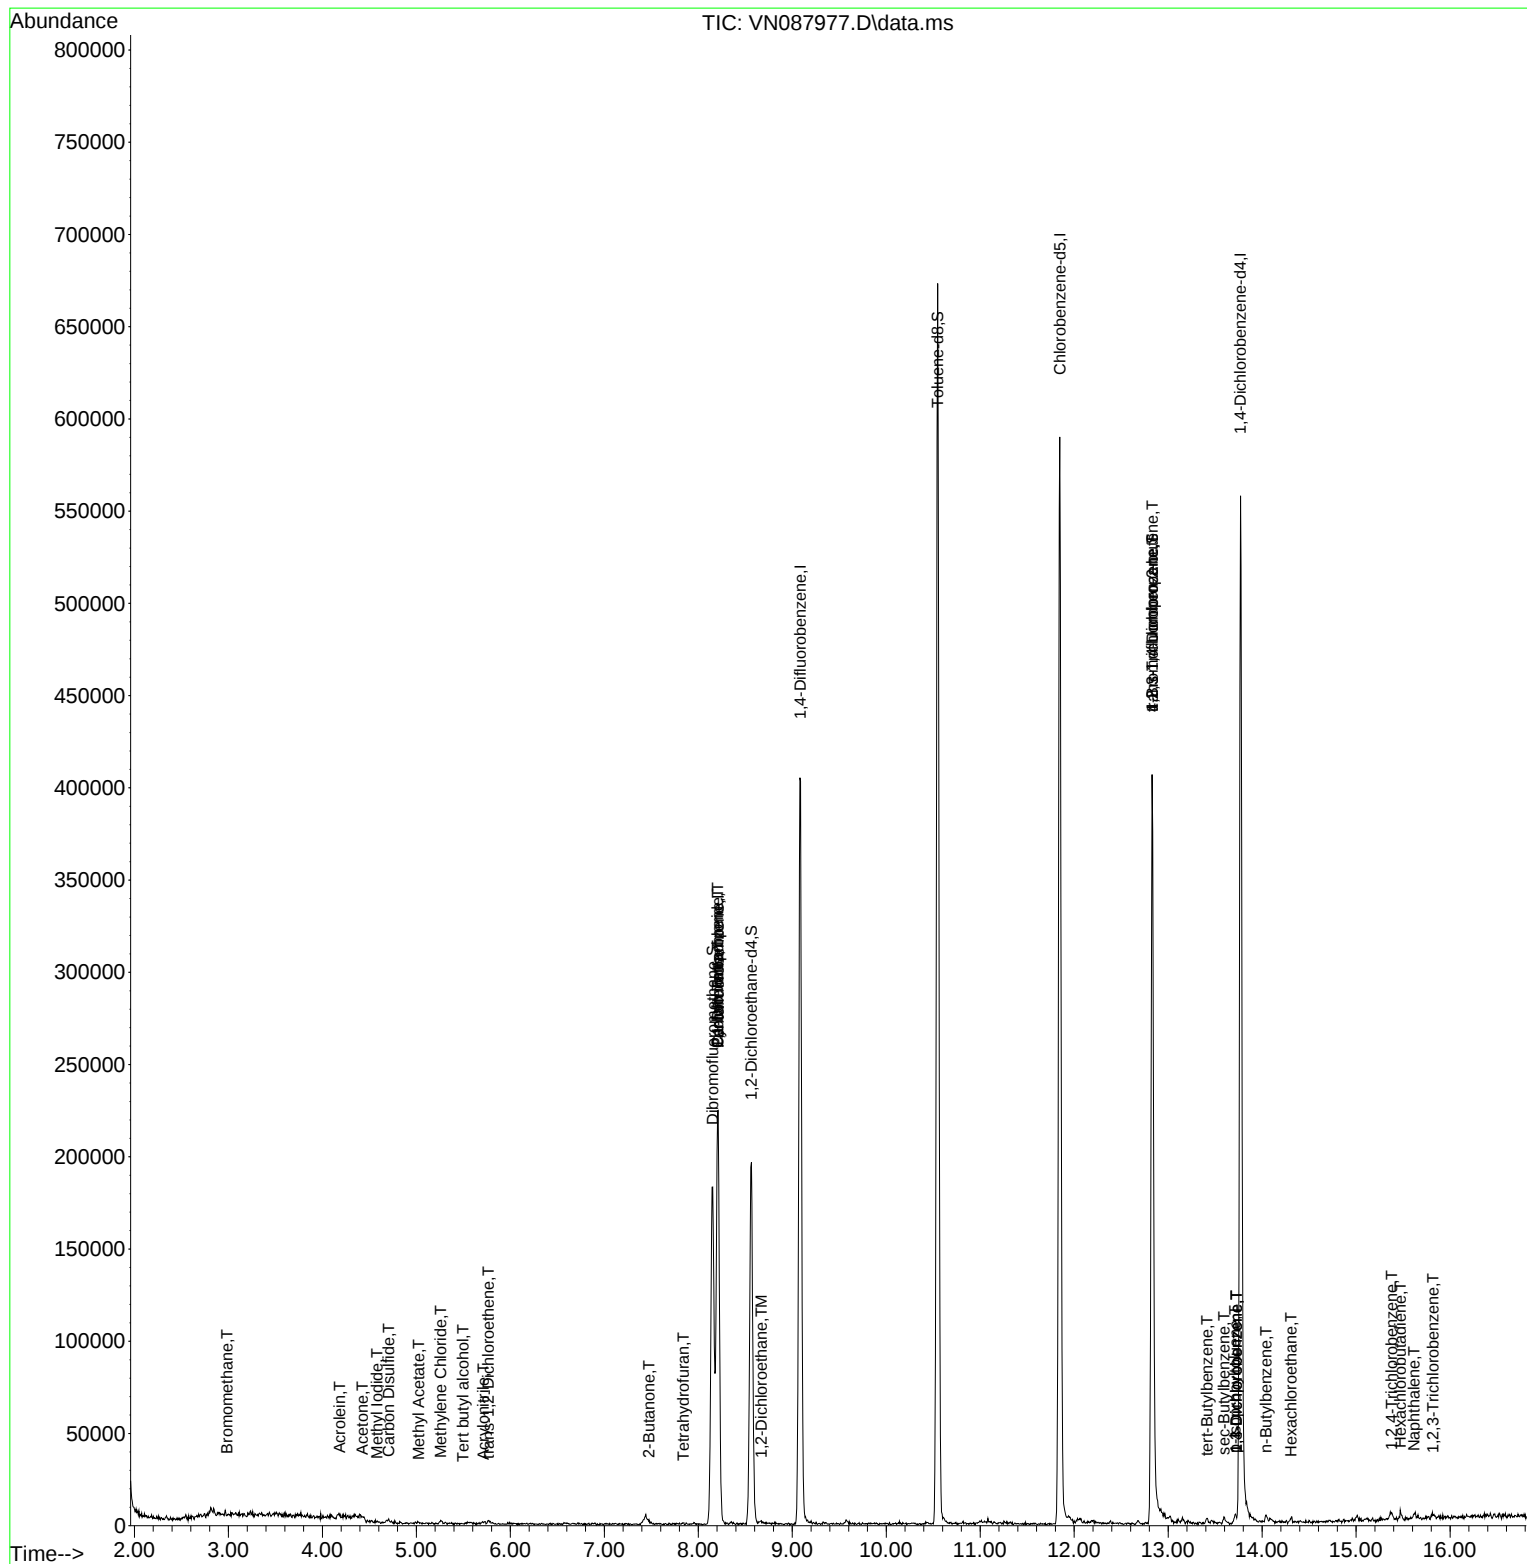


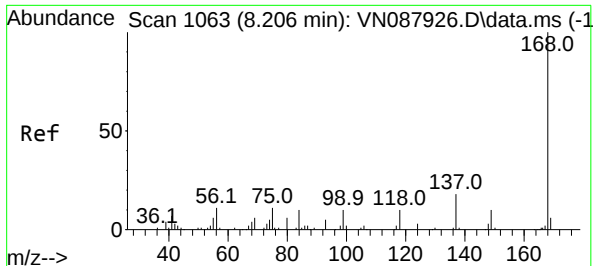

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.212 min Scan# 1064
Delta R.T. 0.006 min
Lab File: VN087977.D
Acq: 29 Sep 2025 13:08




Instrument :
MSVOA_N
ClientSampleId :
VN0929WBL01


Tgt Ion:168 Resp: 158754
Ion Ratio Lower Upper
168 100
99 58.7 52.2 78.2

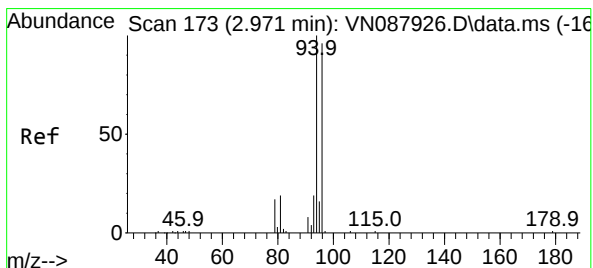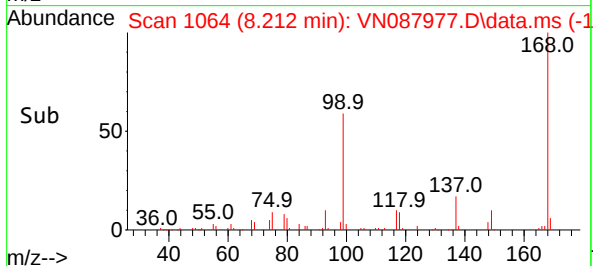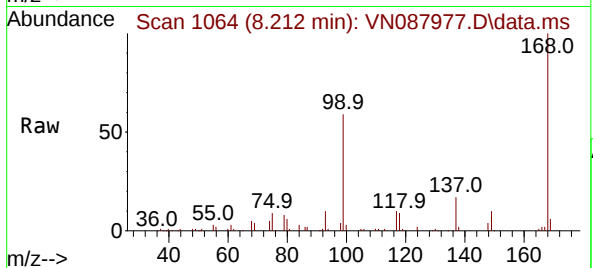

#5
Bromomethane
Concen: 0.418 ug/l
RT: 2.983 min Scan# 175
Delta R.T. 0.012 min
Lab File: VN087977.D
Acq: 29 Sep 2025 13:08

Tgt Ion: 94 Resp: 498
Ion Ratio Lower Upper
94 100
96 108.3 76.8 115.2


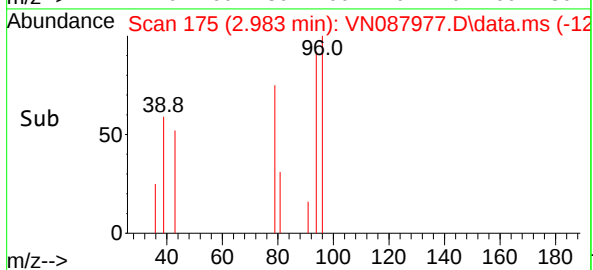

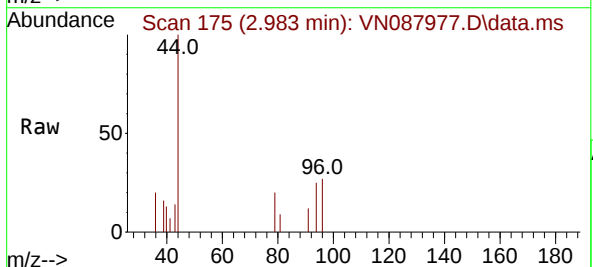




#10
Methyl Iodide
Concen: 0.274 ug/l
RT: 4.583 min Scan# 447
Delta R.T. -0.000 min
Lab File: VN087977.D
Acq: 29 Sep 2025 13:08




Instrument :
MSVOA_N
ClientSampleId :
VN0929WBL01


Tgt Ion:142 Resp: 408
Ion Ratio Lower Upper
142 100
127 0.0 35.3 52.9#
141 0.0 11.8 17.8#



#11
Tert butyl alcohol
Concen: 0.203 ug/l
RT: 5.494 min Scan# 602
Delta R.T. -0.024 min
Lab File: VN087977.D
Acq: 29 Sep 2025 13:08

Tgt Ion: 59 Resp: 78
Ion Ratio Lower Upper
59 100
57 0.0 8.8 13.2#

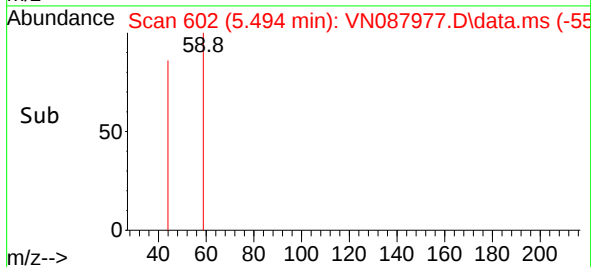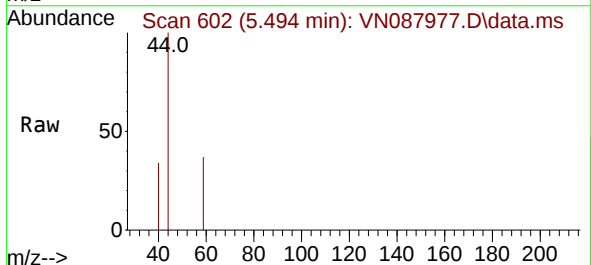



#13

Acrolein

Concen: 1.100 ug/l

RT: 4.183 min Scan# 31

Delta R.T. 0.006 min

Lab File: VN087977.D

Acq: 29 Sep 2025 13:08

Instrument :

MSVOA_N

ClientSampleId :





VN0929WBL01

Tgt Ion: 56 Resp: 543

Ion Ratio Lower Upper

56 100

55 0.0 59.3 88.9#

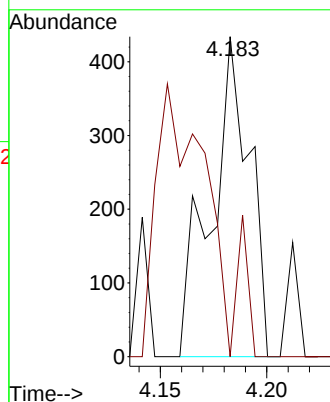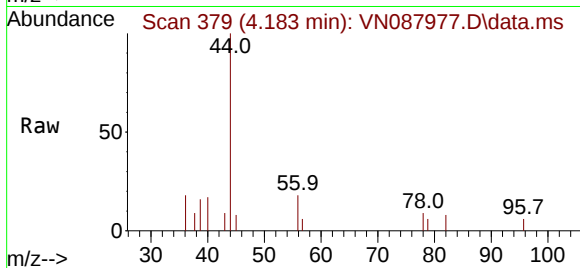

#15

Acrylonitrile

Concen: 0.281 ug/l

RT: 5.712 min Scan# 639

Delta R.T. 0.006 min

Lab File: VN087977.D

Acq: 29 Sep 2025 13:08




Tgt Ion: 53 Resp: 339


Ion Ratio Lower Upper

53 100

52 189.4 66.6 99.8#

51 0.0 29.0 43.4#

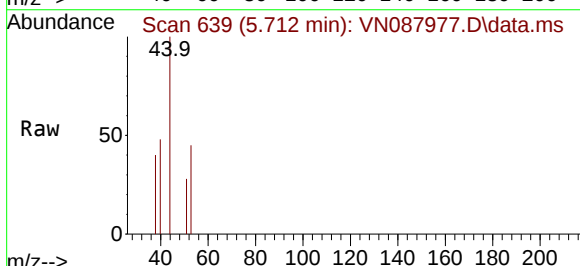



#16

Acetone

Concen: 1.834 ug/l

RT: 4.424 min Scan# 41

Delta R.T. -0.000 min

Lab File: VN087977.D

Acq: 29 Sep 2025 13:08

Instrument :

MSVOA_N

ClientSampleId :





VN0929WBL01

Tgt Ion: 43 Resp: 2016

Ion Ratio Lower Upper

43 100

58 20.9 24.1 36.1#

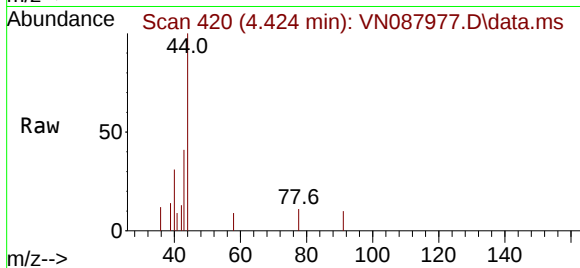

#17

Carbon Disulfide

Concen: 0.705 ug/l

RT: 4.706 min Scan# 468

Delta R.T. -0.000 min

Lab File: VN087977.D




Acq: 29 Sep 2025 13:08


Tgt Ion: 76 Resp: 3672

Ion Ratio Lower Upper

76 100

78 0.0 6.7 10.1#


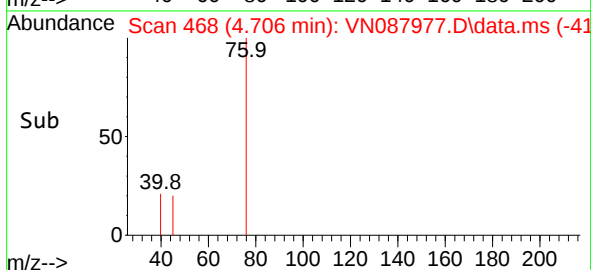
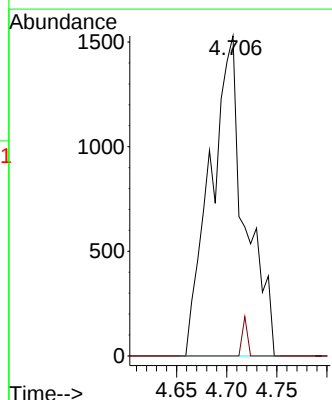
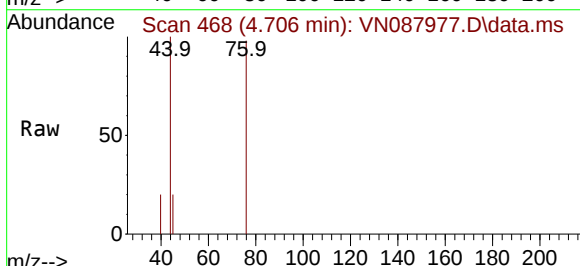




#18
Methyl Acetate
Concen: 0.285 ug/l
RT: 5.024 min Scan# 51
Delta R.T. 0.012 min
Lab File: VN087977.D
Acq: 29 Sep 2025 13:08




Instrument :
MSVOA_N
ClientSampleId :
VN0929WBL01


Tgt Ion: 43 Resp: 783
Ion Ratio Lower Upper
43 100
74 11.6 19.7 29.5#

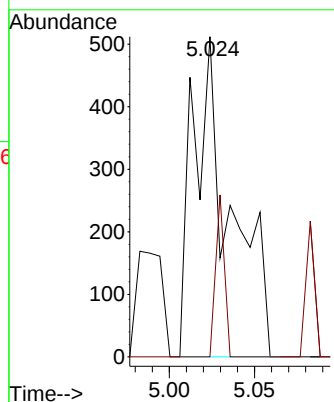

#20
Methylene Chloride
Concen: 0.487 ug/l
RT: 5.259 min Scan# 562
Delta R.T. -0.006 min
Lab File: VN087977.D
Acq: 29 Sep 2025 13:08

Tgt Ion: 84 Resp: 1083
Ion Ratio Lower Upper
84 100
49 59.9 92.1 138.1#
51 27.9 27.7 41.5
86 43.9 49.6 74.4#


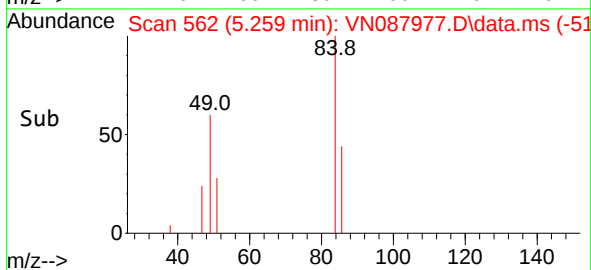
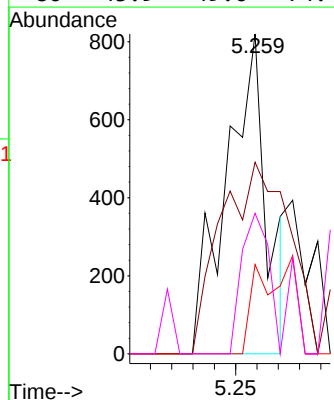





#21
trans-1,2-Dichloroethene
Concen: 0.506 ug/l
RT: 5.765 min Scan# 649
Delta R.T. -0.006 min
Lab File: VN087977.D
Acq: 29 Sep 2025 13:08




Instrument :
MSVOA_N
ClientSampleId :
VN0929WBL01


Tgt Ion: 96 Resp: 1035
Ion Ratio Lower Upper
96 100
61 70.6 114.4 171.6#
98 48.8 53.6 80.4#



#25
2-Butanone
Concen: 0.291 ug/l
RT: 7.477 min Scan# 939
Delta R.T. 0.006 min
Lab File: VN087977.D
Acq: 29 Sep 2025 13:08

Tgt Ion: 43 Resp: 489
Ion Ratio Lower Upper
43 100
72 0.0 21.5 32.3#

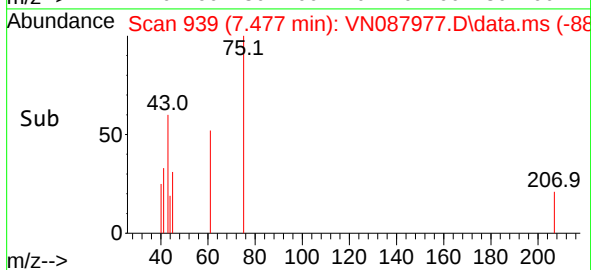



#29

Tetrahydrofuran

Concen: 0.371 ug/l

RT: 7.841 min Scan# 1001

Delta R.T. 0.018 min

Lab File: VN087977.D


Acq: 29 Sep 2025 13:08

Instrument :




MSVOA_N

ClientSampleId :

VN0929WBL01

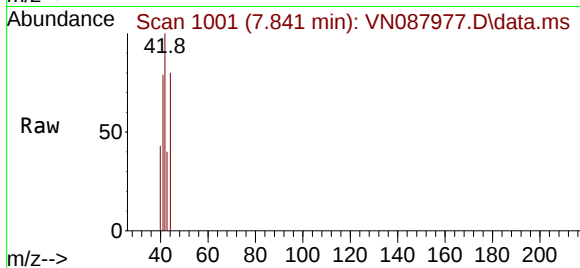

Tgt Ion:	42	Resp:	399
Ion	Ratio	Lower	Upper
42	100		
72	18.0	36.5	54.7#
71	15.0	33.8	50.8#

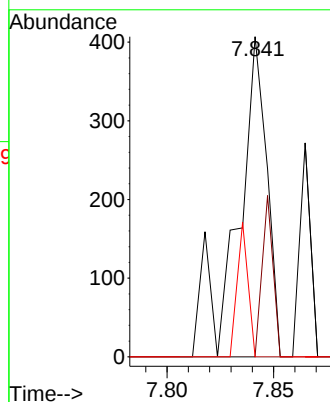

#31

Cyclohexane

Concen: 1.627 ug/l




RT: 8.206 min Scan# 1063


Delta R.T. -0.035 min

Lab File: VN087977.D

Acq: 29 Sep 2025 13:08

Tgt Ion:	56	Resp:	4873
Ion	Ratio	Lower	Upper
56	100		
69	168.2	23.4	35.0#
84	105.7	70.8	106.2


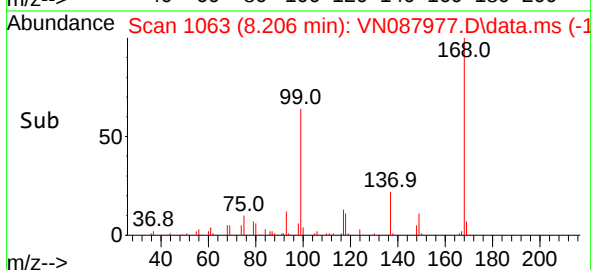
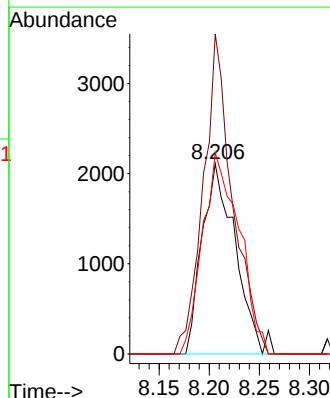
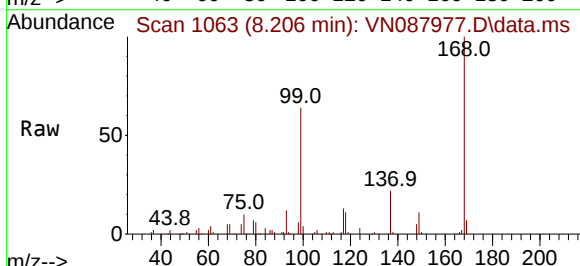


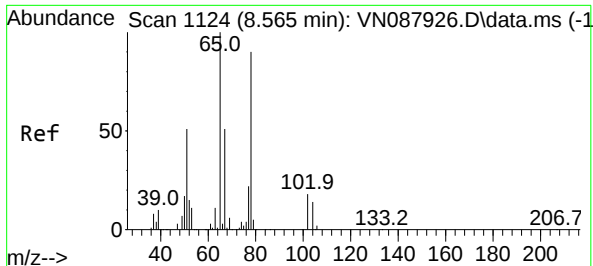

#33
 1,2-Dichloroethane-d4
 Concen: 60.554 ug/l
 RT: 8.565 min Scan# 1124
 Delta R.T. -0.000 min
 Lab File: VN087977.D
 Acq: 29 Sep 2025 13:08




Instrument :
 MSVOA_N
 ClientSampleId :
 VN0929WBL01


Tgt Ion: 65 Resp: 161783
 Ion Ratio Lower Upper
 65 100
 67 52.2 0.0 103.4

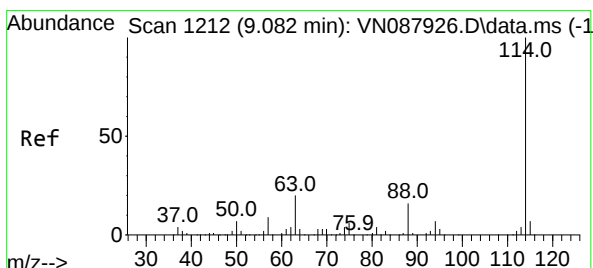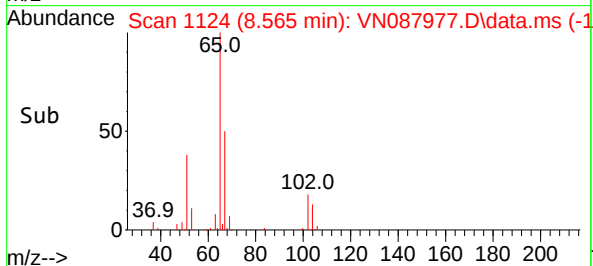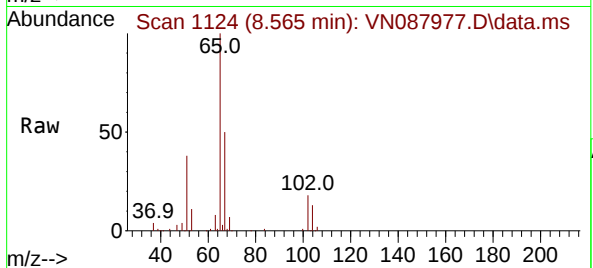

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 9.088 min Scan# 1213
 Delta R.T. 0.006 min
 Lab File: VN087977.D
 Acq: 29 Sep 2025 13:08

Tgt Ion: 114 Resp: 351007
 Ion Ratio Lower Upper
 114 100
 63 19.9 0.0 40.0
 88 15.4 0.0 31.8

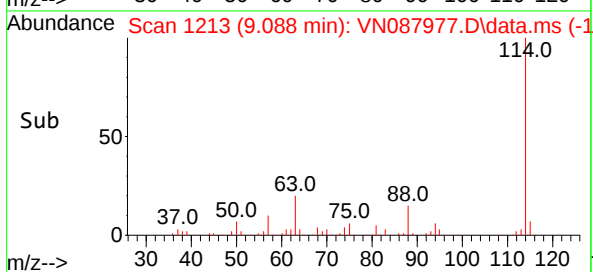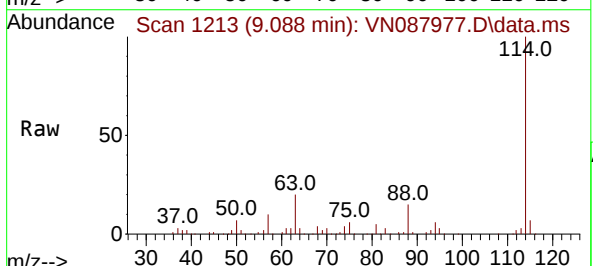

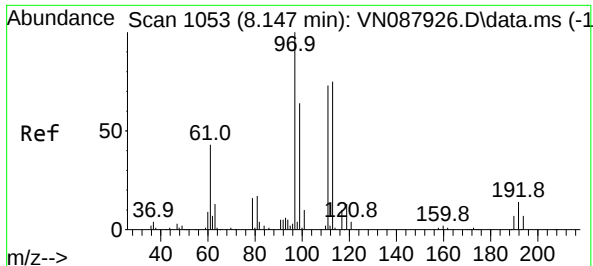

#35

Dibromofluoromethane

Concen: 51.684 ug/l

RT: 8.153 min Scan# 1054

Delta R.T. 0.006 min

Lab File: VN087977.D

Acq: 29 Sep 2025 13:08

Instrument :

MSVOA_N

ClientSampleId :

VN0929WBL01





Tgt Ion:113 Resp: 131718

Ion Ratio Lower Upper

113 100

111 103.6 82.2 123.2

192 17.7 14.2 21.2

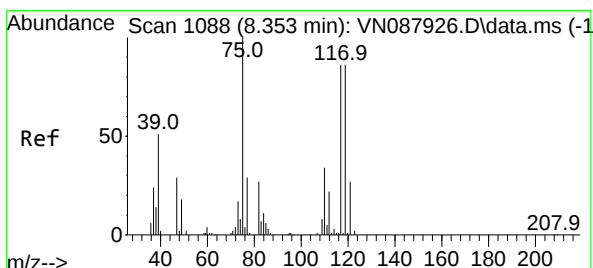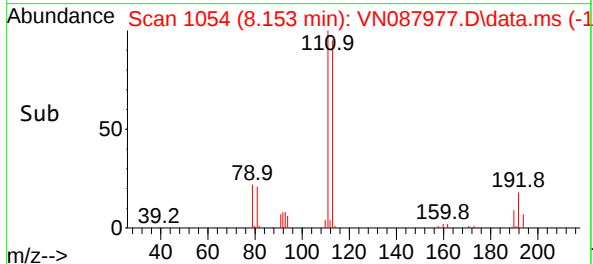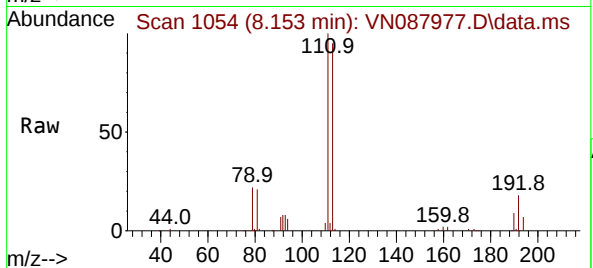

#36

1,1-Dichloropropene

Concen: 4.677 ug/l

RT: 8.206 min Scan# 1063

Delta R.T. -0.147 min

Lab File: VN087977.D

Acq: 29 Sep 2025 13:08




Tgt Ion: 75 Resp: 14332


Ion Ratio Lower Upper

75 100

110 9.5 17.1 51.3#


77 0.0 24.8 37.2#

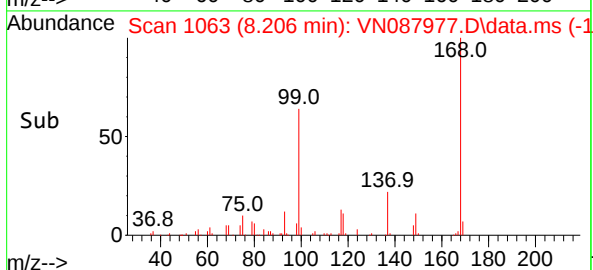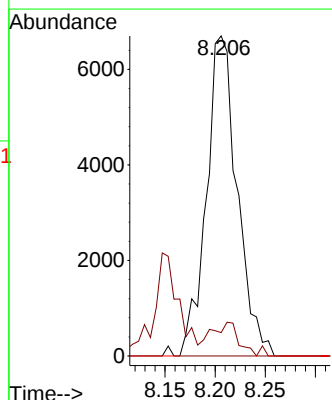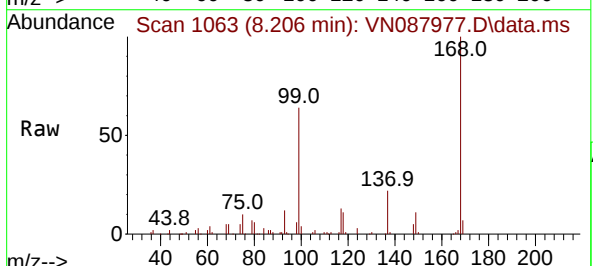



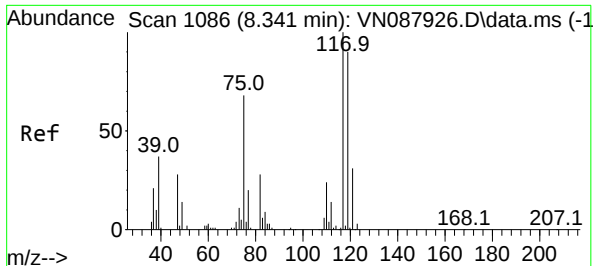


#38
Carbon Tetrachloride
Concen: 5.160 ug/l
RT: 8.206 min Scan# 110
Delta R.T. -0.135 min
Lab File: VN087977.D
Acq: 29 Sep 2025 13:08


Instrument :
MSVOA_N
ClientSampleId :
VN0929WBL01

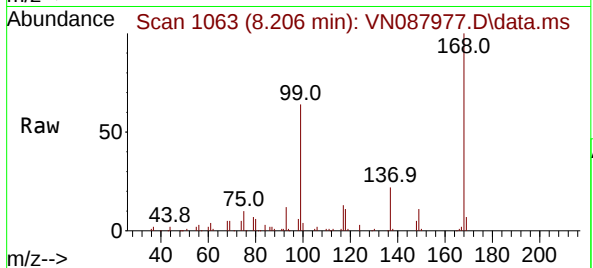



Tgt Ion: 117 Resp: 18144
Ion Ratio Lower Upper
117 100
119 6.1 72.1 108.1#
121 0.0 24.6 36.8#

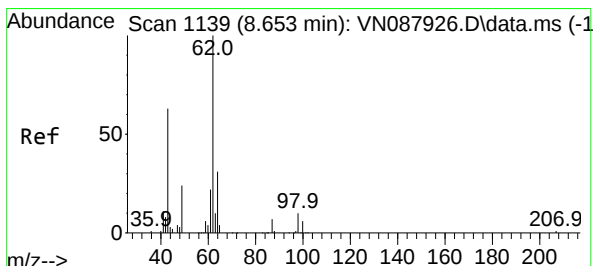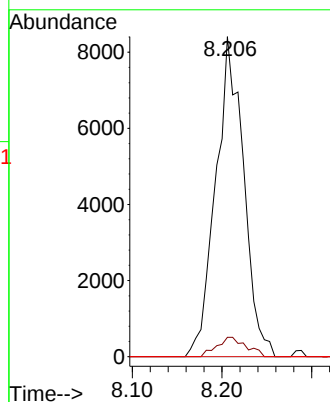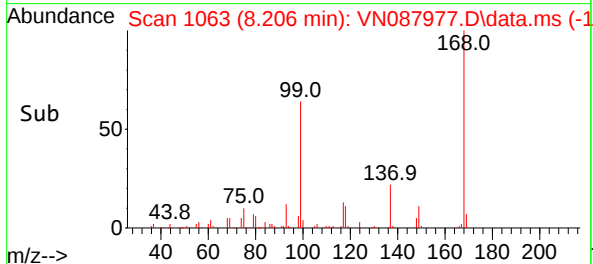


#42
1,2-Dichloroethane
Concen: 0.223 ug/l
RT: 8.671 min Scan# 1142
Delta R.T. 0.018 min
Lab File: VN087977.D
Acq: 29 Sep 2025 13:08

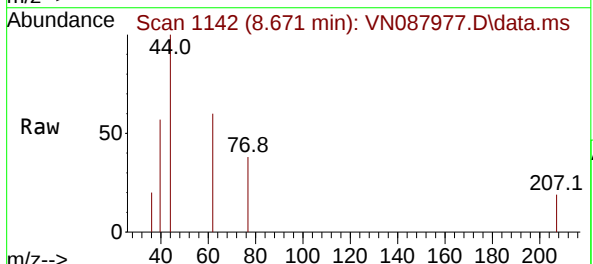

Tgt Ion: 62 Resp: 846
Ion Ratio Lower Upper
62 100
98 0.0 0.0 18.6




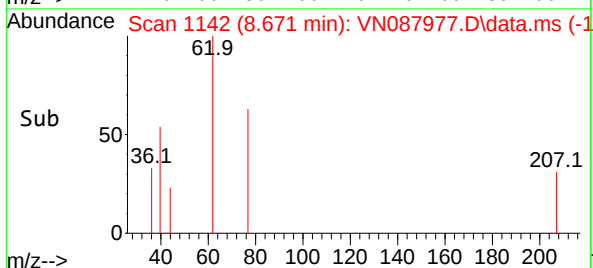


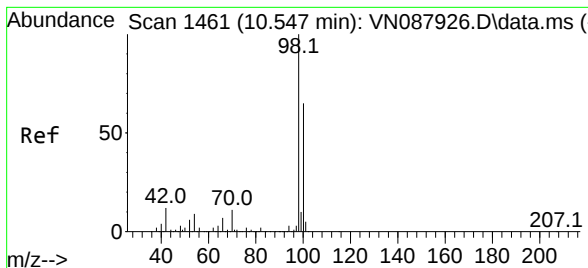

#50
Toluene-d8
Concen: 50.076 ug/l
RT: 10.547 min Scan# 1461
Delta R.T. -0.000 min
Lab File: VN087977.D
Acq: 29 Sep 2025 13:08




Instrument :
MSVOA_N
ClientSampleId :
VN0929WBL01


Tgt Ion: 98 Resp: 448783
Ion Ratio Lower Upper
98 100
100 63.5 51.7 77.5

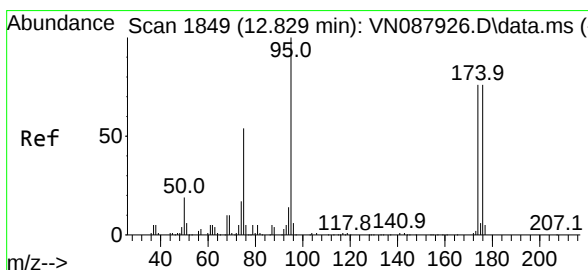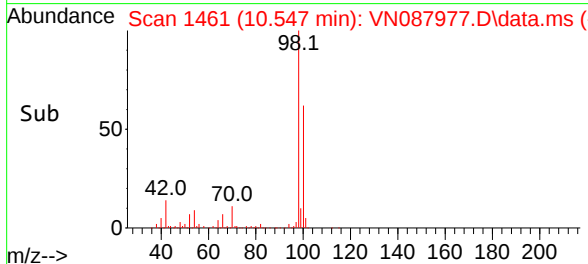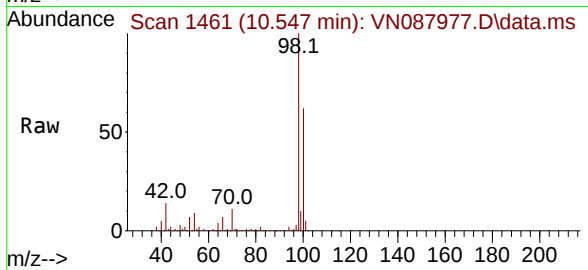

#62
4-Bromofluorobenzene
Concen: 44.598 ug/l
RT: 12.829 min Scan# 1849
Delta R.T. -0.000 min
Lab File: VN087977.D
Acq: 29 Sep 2025 13:08

Tgt Ion: 95 Resp: 142869
Ion Ratio Lower Upper
95 100
174 79.1 0.0 159.2
176 73.9 0.0 152.6


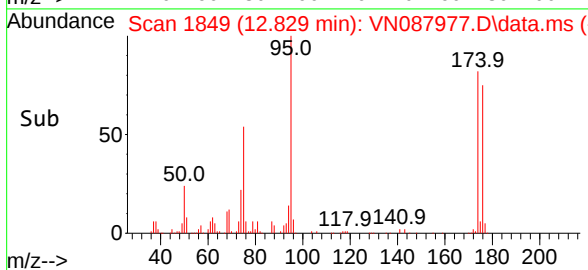

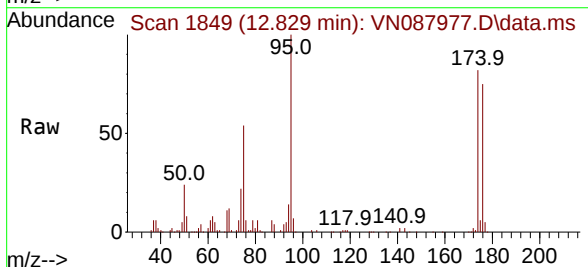




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.847 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN087977.D
Acq: 29 Sep 2025 13:08




Instrument :
MSVOA_N
ClientSampleId :
VN0929WBL01


Tgt Ion:117 Resp: 338452
Ion Ratio Lower Upper
117 100
82 55.1 47.0 70.4
119 32.6 26.1 39.1



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.770 min Scan# 2009
Delta R.T. -0.000 min
Lab File: VN087977.D
Acq: 29 Sep 2025 13:08

Tgt Ion:152 Resp: 154688
Ion Ratio Lower Upper
152 100
115 59.9 29.9 89.7
150 159.9 0.0 335.0



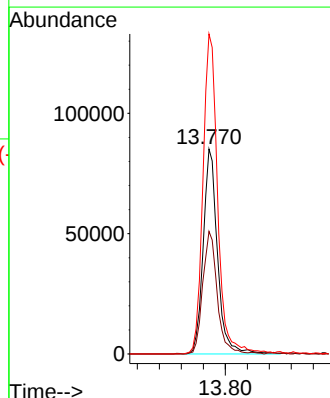
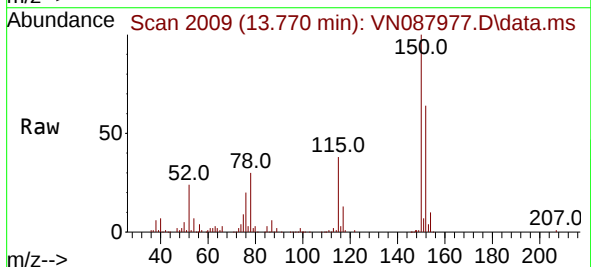


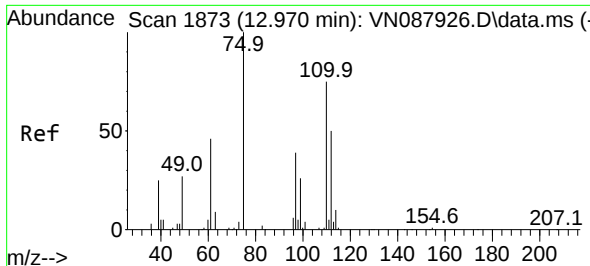

#76
1,2,3-Trichloropropane
Concen: 26.861 ug/l
RT: 12.829 min Scan# 1849
Delta R.T. -0.141 min
Lab File: VN087977.D
Acq: 29 Sep 2025 13:08




Instrument :
MSVOA_N
ClientSampleId :
VN0929WBL01


Tgt Ion: 75 Resp: 81905
Ion Ratio Lower Upper
75 100
77 1.6 89.5 268.5#

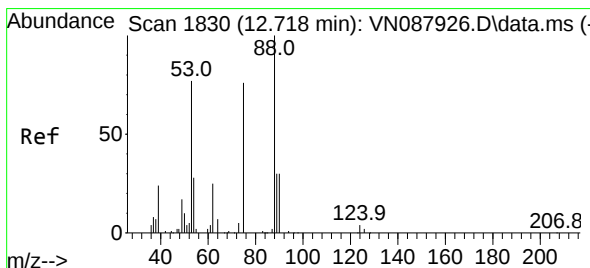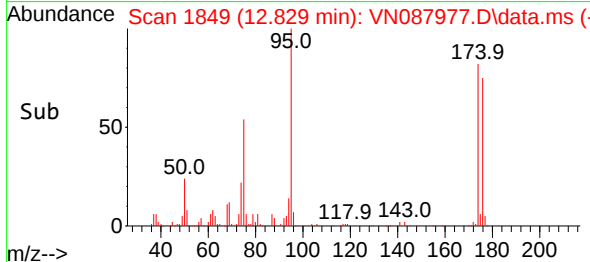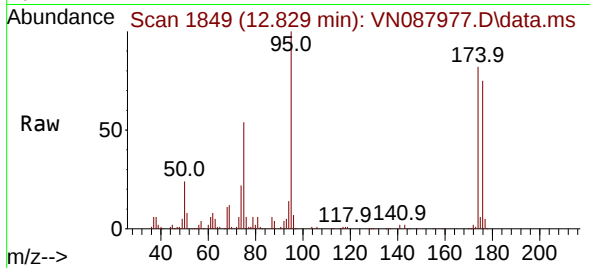

#81
trans-1,4-Dichloro-2-butene
Concen: 74.588 ug/l
RT: 12.829 min Scan# 1849
Delta R.T. 0.112 min
Lab File: VN087977.D
Acq: 29 Sep 2025 13:08

Tgt Ion: 75 Resp: 81905
Ion Ratio Lower Upper
75 100
53 0.3 82.0 123.0#
89 0.0 36.1 54.1#


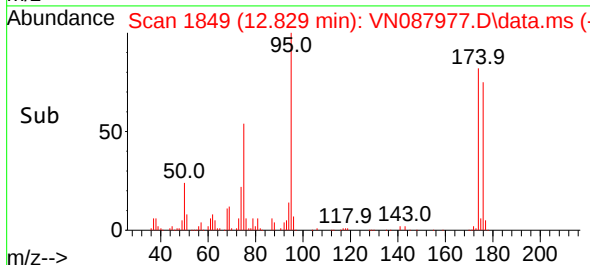
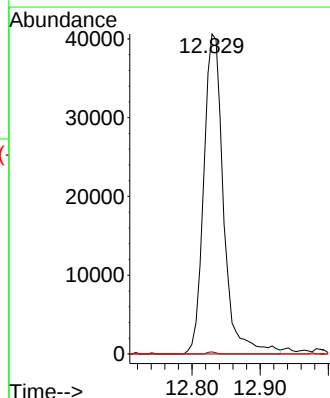
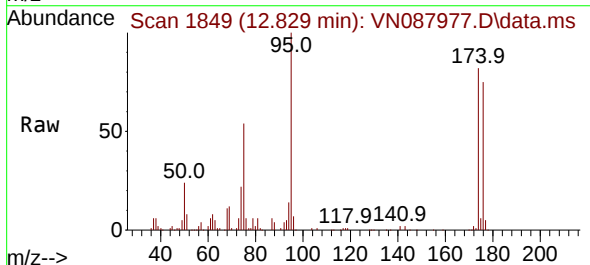




#83
tert-Butylbenzene
Concen: 0.223 ug/l
RT: 13.412 min Scan# 1948
Delta R.T. -0.000 min
Lab File: VN087977.D
Acq: 29 Sep 2025 13:08




Instrument :
MSVOA_N
ClientSampleId :
VN0929WBL01


Tgt Ion:119 Resp: 1565
Ion Ratio Lower Upper
119 100
91 70.0 32.1 96.3
134 10.0 12.3 36.8#

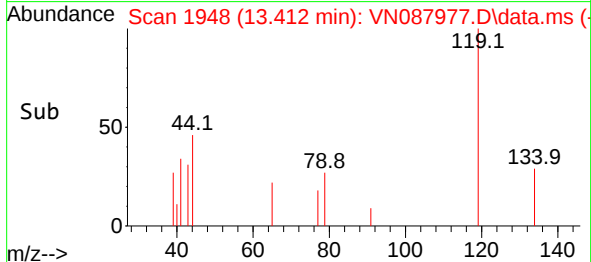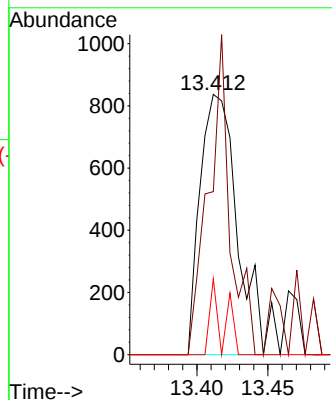

#85
sec-Butylbenzene
Concen: 0.239 ug/l
RT: 13.594 min Scan# 1979
Delta R.T. -0.000 min
Lab File: VN087977.D
Acq: 29 Sep 2025 13:08

Tgt Ion:105 Resp: 2456
Ion Ratio Lower Upper
105 100
134 24.8 9.6 28.8


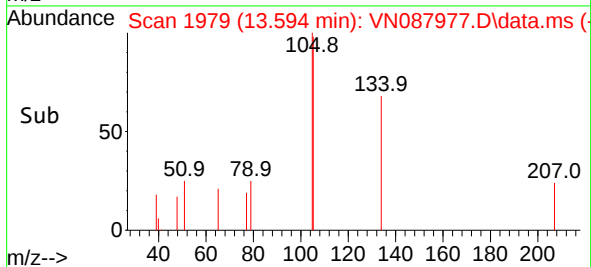
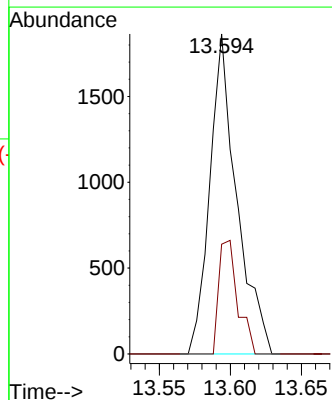
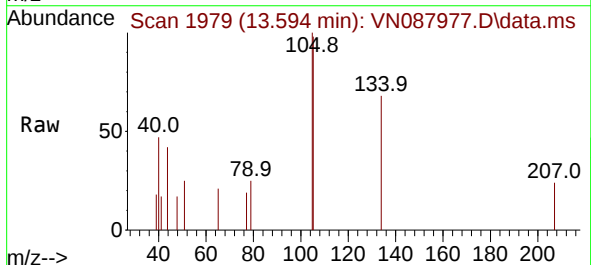




#86
p-Isopropyltoluene
Concen: 0.201 ug/l
RT: 13.712 min Scan# 1998
Delta R.T. 0.006 min
Lab File: VN087977.D
Acq: 29 Sep 2025 13:08




Instrument :
MSVOA_N
ClientSampleId :
VN0929WBL01


Tgt Ion:119 Resp: 1752
Ion Ratio Lower Upper
119 100
134 41.0 13.1 39.3#
91 23.1 11.9 35.5

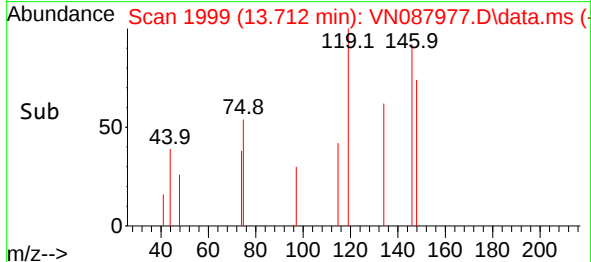

#87
1,3-Dichlorobenzene
Concen: 0.266 ug/l
RT: 13.723 min Scan# 2001
Delta R.T. 0.012 min
Lab File: VN087977.D
Acq: 29 Sep 2025 13:08

Tgt Ion:146 Resp: 1326
Ion Ratio Lower Upper
146 100
111 22.9 20.3 60.8
148 60.2 32.4 97.2


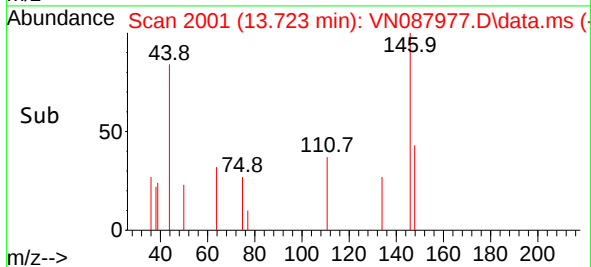

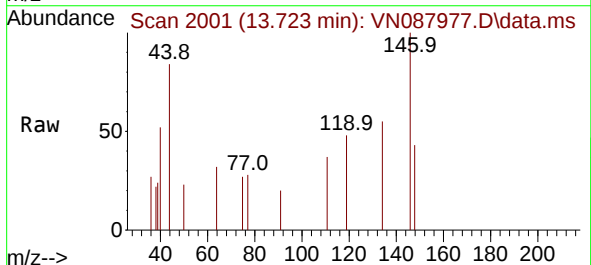




#88
1,4-Dichlorobenzene
Concen: 0.259 ug/l
RT: 13.723 min Scan# 2012
Delta R.T. -0.065 min
Lab File: VN087977.D
Acq: 29 Sep 2025 13:08




Instrument :
MSVOA_N
ClientSampleId :
VN0929WBL01


Tgt Ion:146 Resp: 1326
Ion Ratio Lower Upper
146 100
111 22.9 20.5 61.5
148 60.2 32.8 98.4

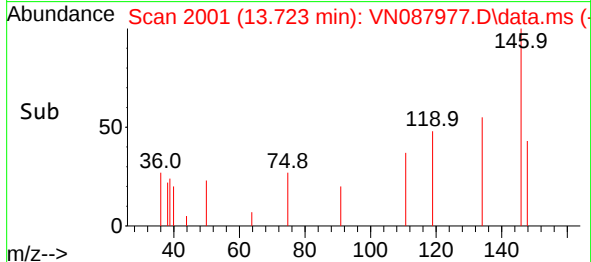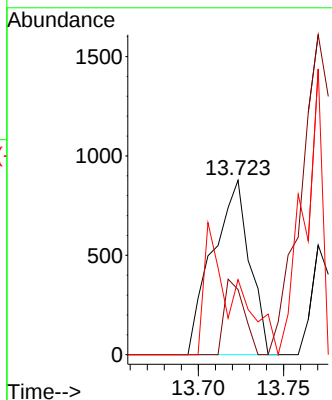

#89
n-Butylbenzene
Concen: 0.220 ug/l
RT: 14.041 min Scan# 2055
Delta R.T. 0.012 min
Lab File: VN087977.D
Acq: 29 Sep 2025 13:08

Tgt Ion: 91 Resp: 1811
Ion Ratio Lower Upper
91 100
92 87.0 25.9 77.8#
134 19.7 12.6 37.8


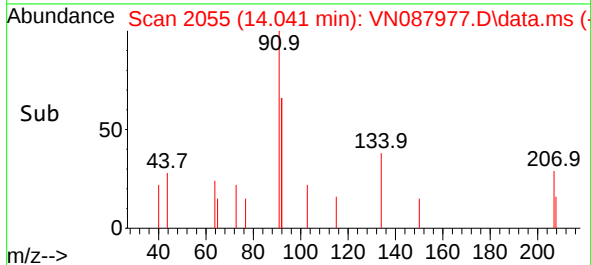
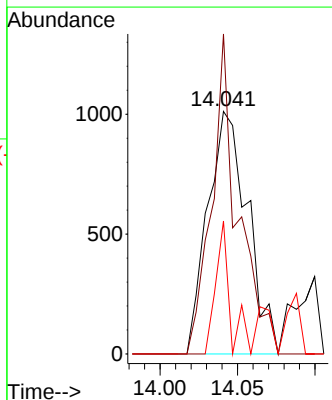
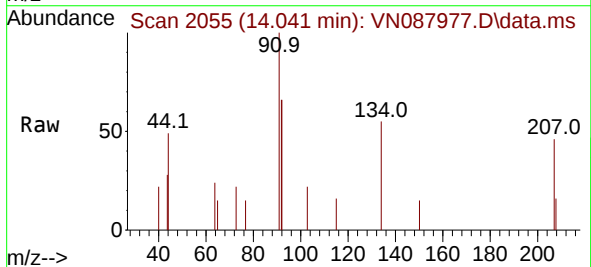




#90
Hexachloroethane
Concen: 0.367 ug/l
RT: 14.306 min Scan# 2101
Delta R.T. -0.006 min
Lab File: VN087977.D
Acq: 29 Sep 2025 13:08




Instrument :
MSVOA_N
ClientSampleId :
VN0929WBL01


Tgt Ion:117 Resp: 668
Ion Ratio Lower Upper
117 100
201 42.7 33.6 100.6

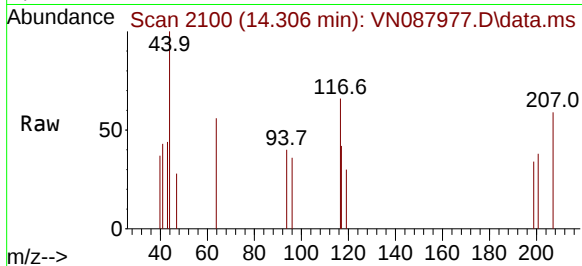

#93
1,2,4-Trichlorobenzene
Concen: 0.454 ug/l
RT: 15.376 min Scan# 2282
Delta R.T. 0.012 min
Lab File: VN087977.D
Acq: 29 Sep 2025 13:08

Tgt Ion:180 Resp: 1285
Ion Ratio Lower Upper
180 100
182 103.0 48.5 145.5
145 30.3 15.9 47.6


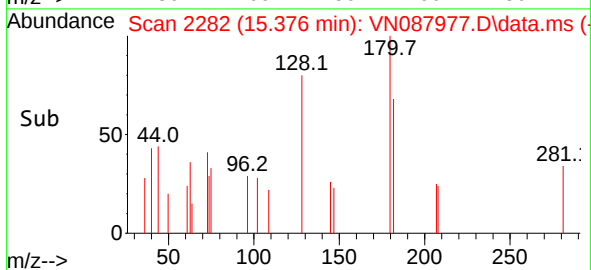
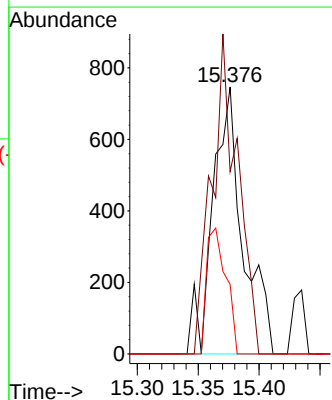
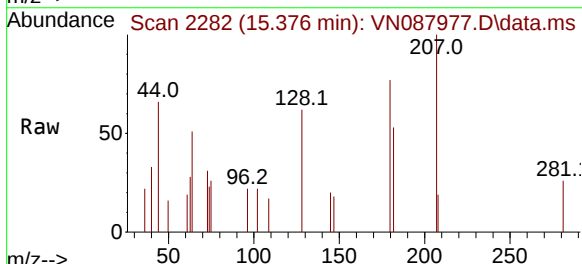




#94
Hexachlorobutadiene
Concen: 0.204 ug/l
RT: 15.470 min Scan# 213
Delta R.T. -0.000 min
Lab File: VN087977.D
Acq: 29 Sep 2025 13:08




Instrument :
MSVOA_N
ClientSampleId :
VN0929WBL01


Tgt Ion:	225	Resp:	213
Ion	Ratio	Lower	Upper
225	100		
223	328.2	31.8	95.4#
227	0.0	31.9	95.9#

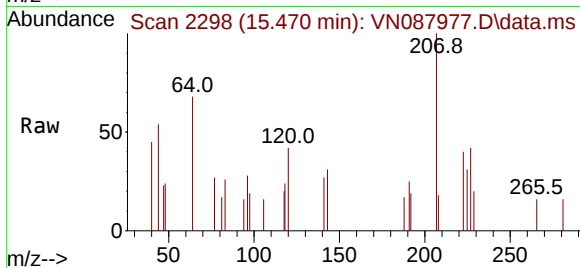

#95
Naphthalene
Concen: 0.368 ug/l
RT: 15.617 min Scan# 2323
Delta R.T. 0.006 min
Lab File: VN087977.D
Acq: 29 Sep 2025 13:08


Tgt Ion:	128	Resp:	3347
Ion	Ratio	Lower	Upper
128	100		
127	4.5	10.2	15.4#
129	0.0	8.6	13.0#

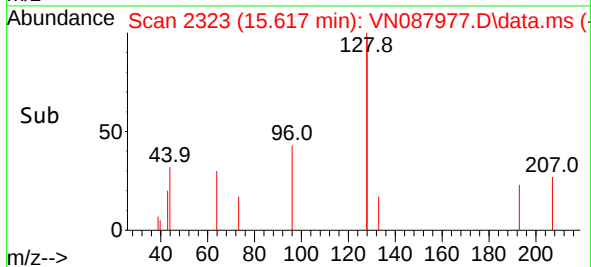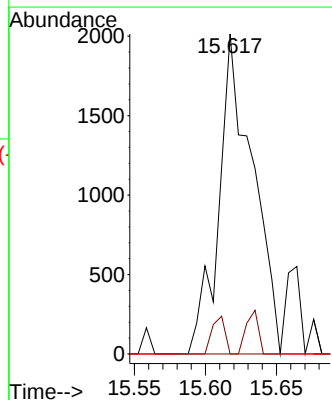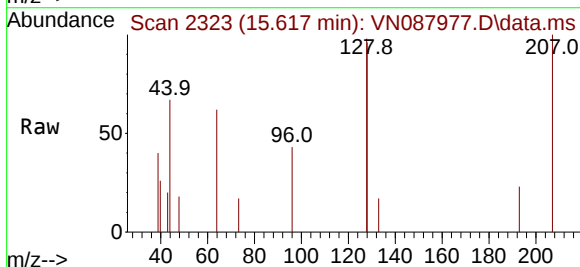



#96
 1,2,3-Trichlorobenzene
 Concen: 0.569 ug/l
 RT: 15.817 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VN087977.D
 Acq: 29 Sep 2025 13:08

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0929WBL01

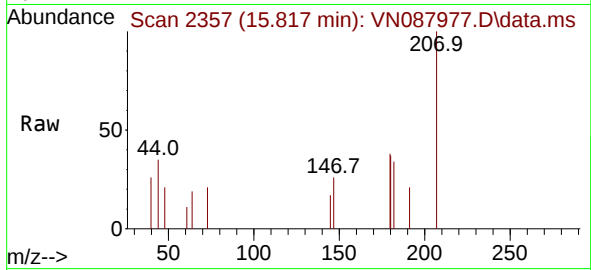

Tgt Ion:	180	Resp:	1567
Ion	Ratio	Lower	Upper
180	100		
182	75.4	47.3	142.0
145	26.7	16.1	48.3

