


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN093019\
Data File : VN058419.D
Acq On : 30 Sep 2019 8:56
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092719W.M
Title : SW846 8260
Last Update : Mon Sep 30 08:07:38 2019

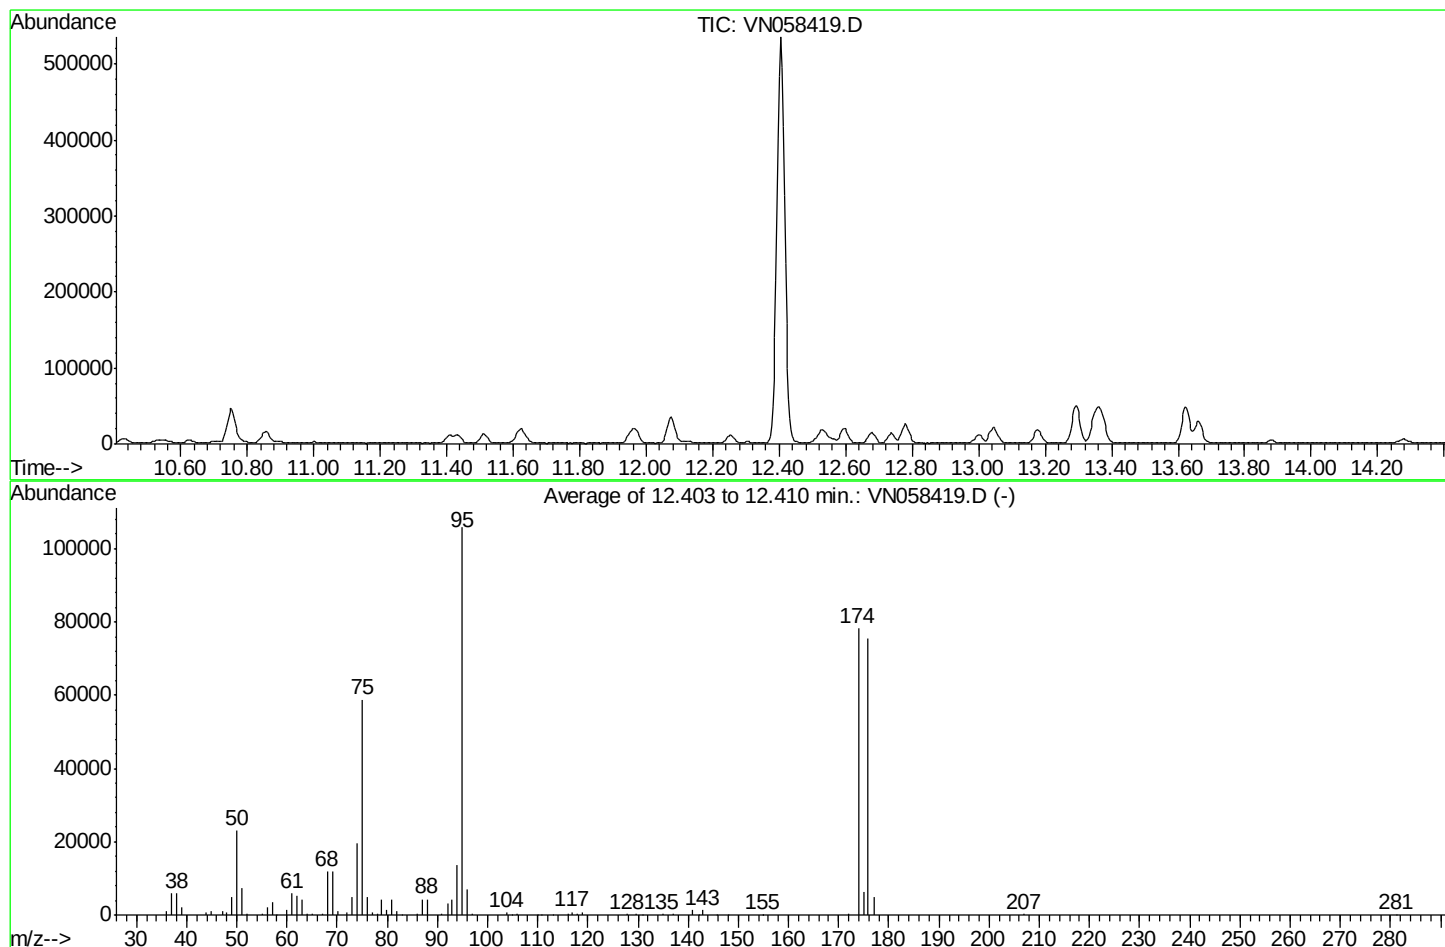

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	22986	PASS
75	95	30	60	55.5	58762	PASS
95	95	100	100	100.0	105848	PASS
96	95	5	9	6.5	6905	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	73.9	78250	PASS
175	174	5	9	7.9	6160	PASS
176	174	95	101	96.4	75418	PASS
177	176	5	9	6.3	4741	PASS