


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN093020\
 Data File : VN063736.D
 Acq On : 30 Sep 2020 8:31
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
 Title : SW846 8260
 Last Update : Wed Sep 30 11:29:11 2020

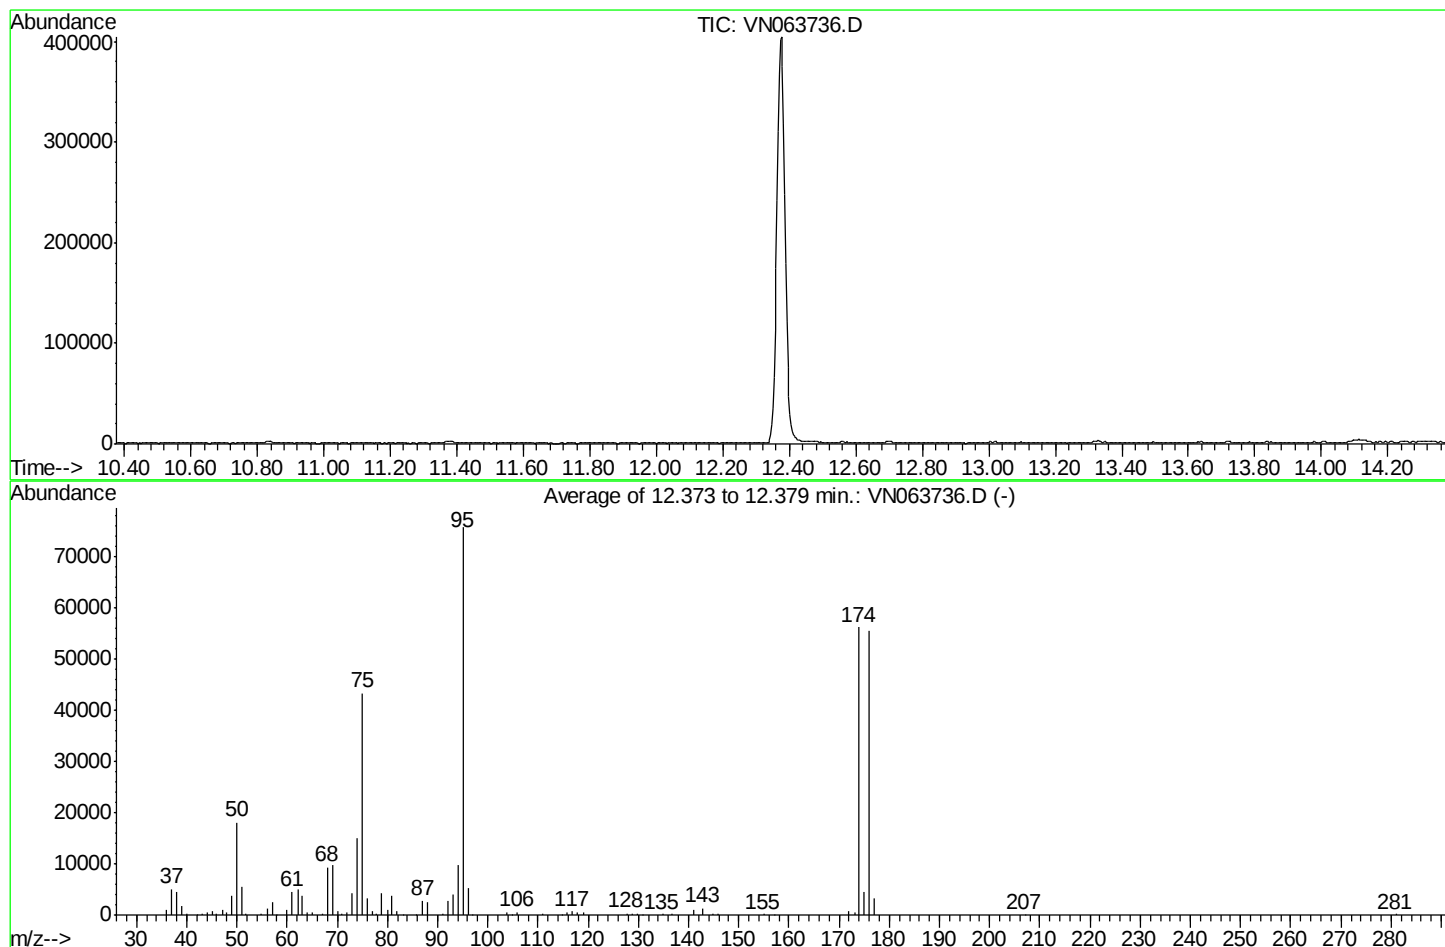

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.8	18008	PASS
75	95	30	60	57.3	43317	PASS
95	95	100	100	100.0	75600	PASS
96	95	5	9	7.0	5327	PASS
173	174	0.00	2	0.9	487	PASS
174	95	50	100	74.2	56114	PASS
175	174	5	9	8.0	4464	PASS
176	174	95	101	98.6	55317	PASS
177	176	5	9	5.9	3250	PASS