



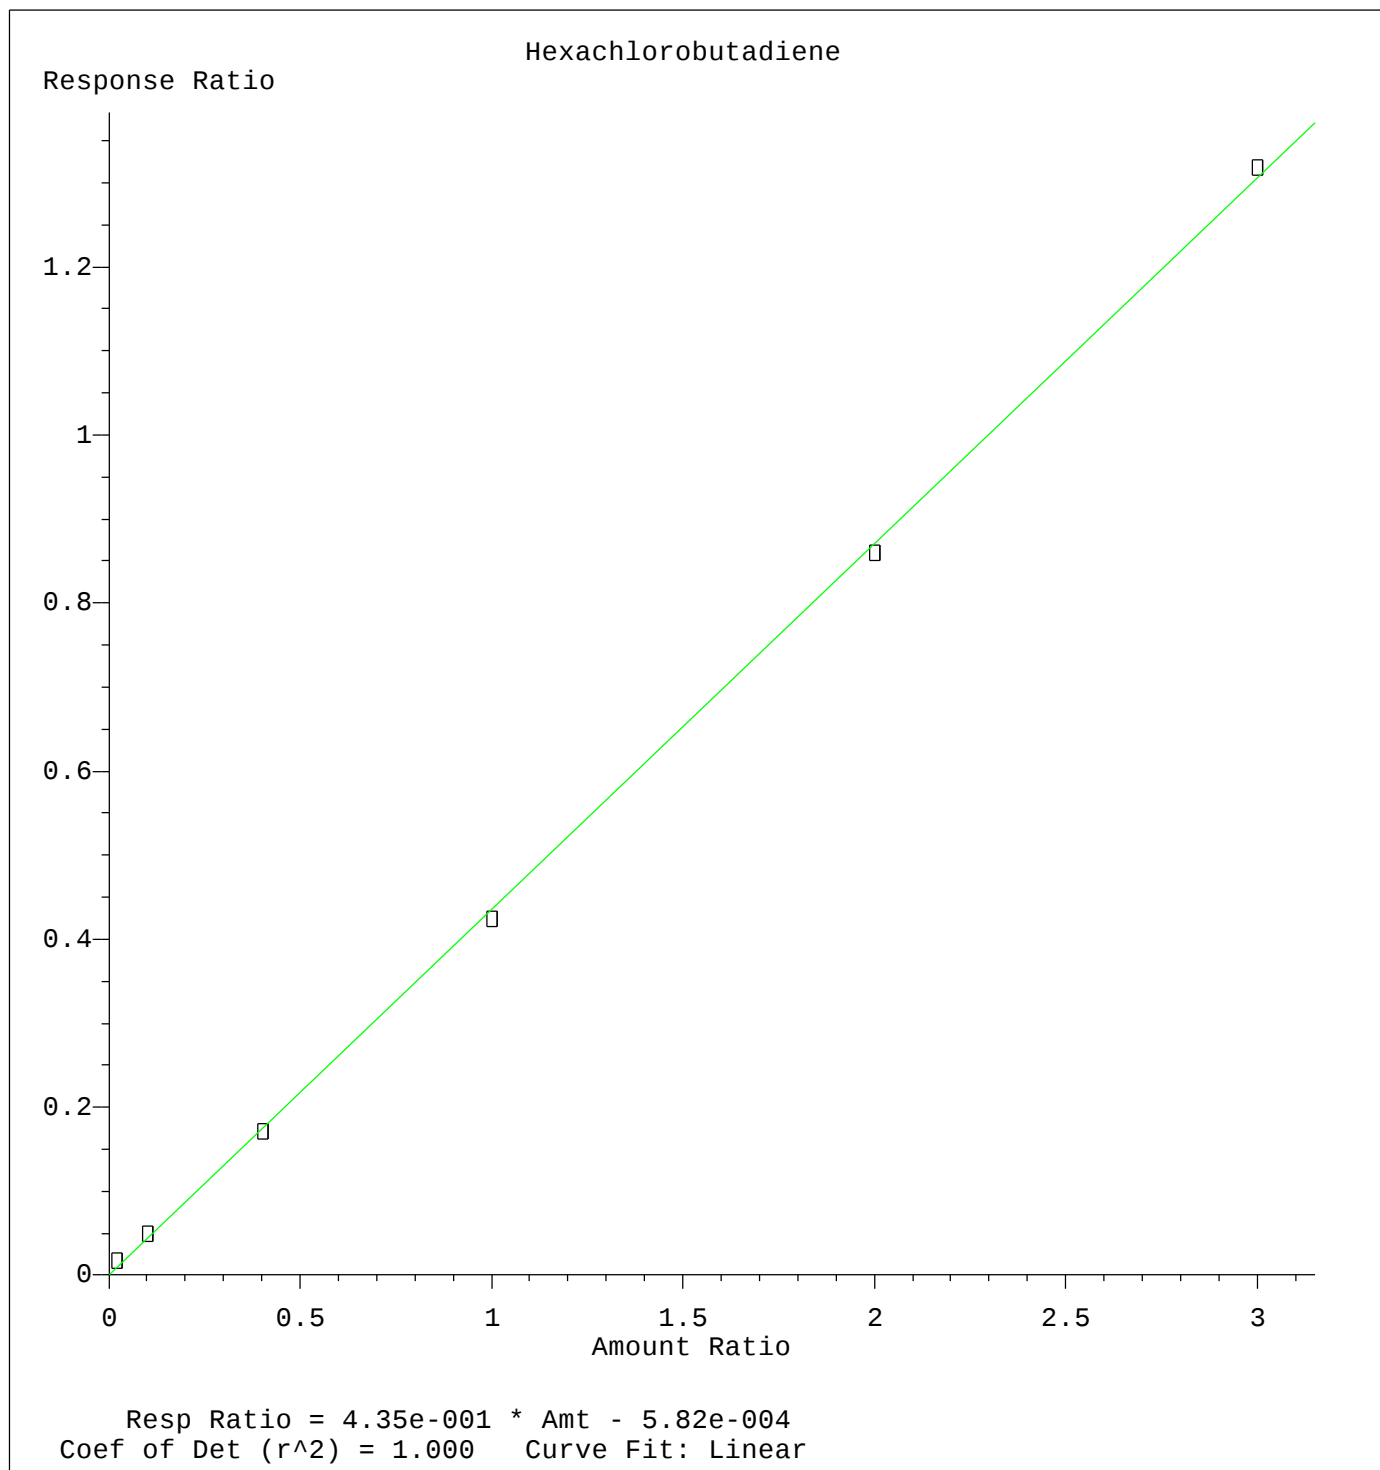

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
Calibration Table Last Updated: Thu Oct 01 01:46:38 2020

Naphthalene

Response Ratio

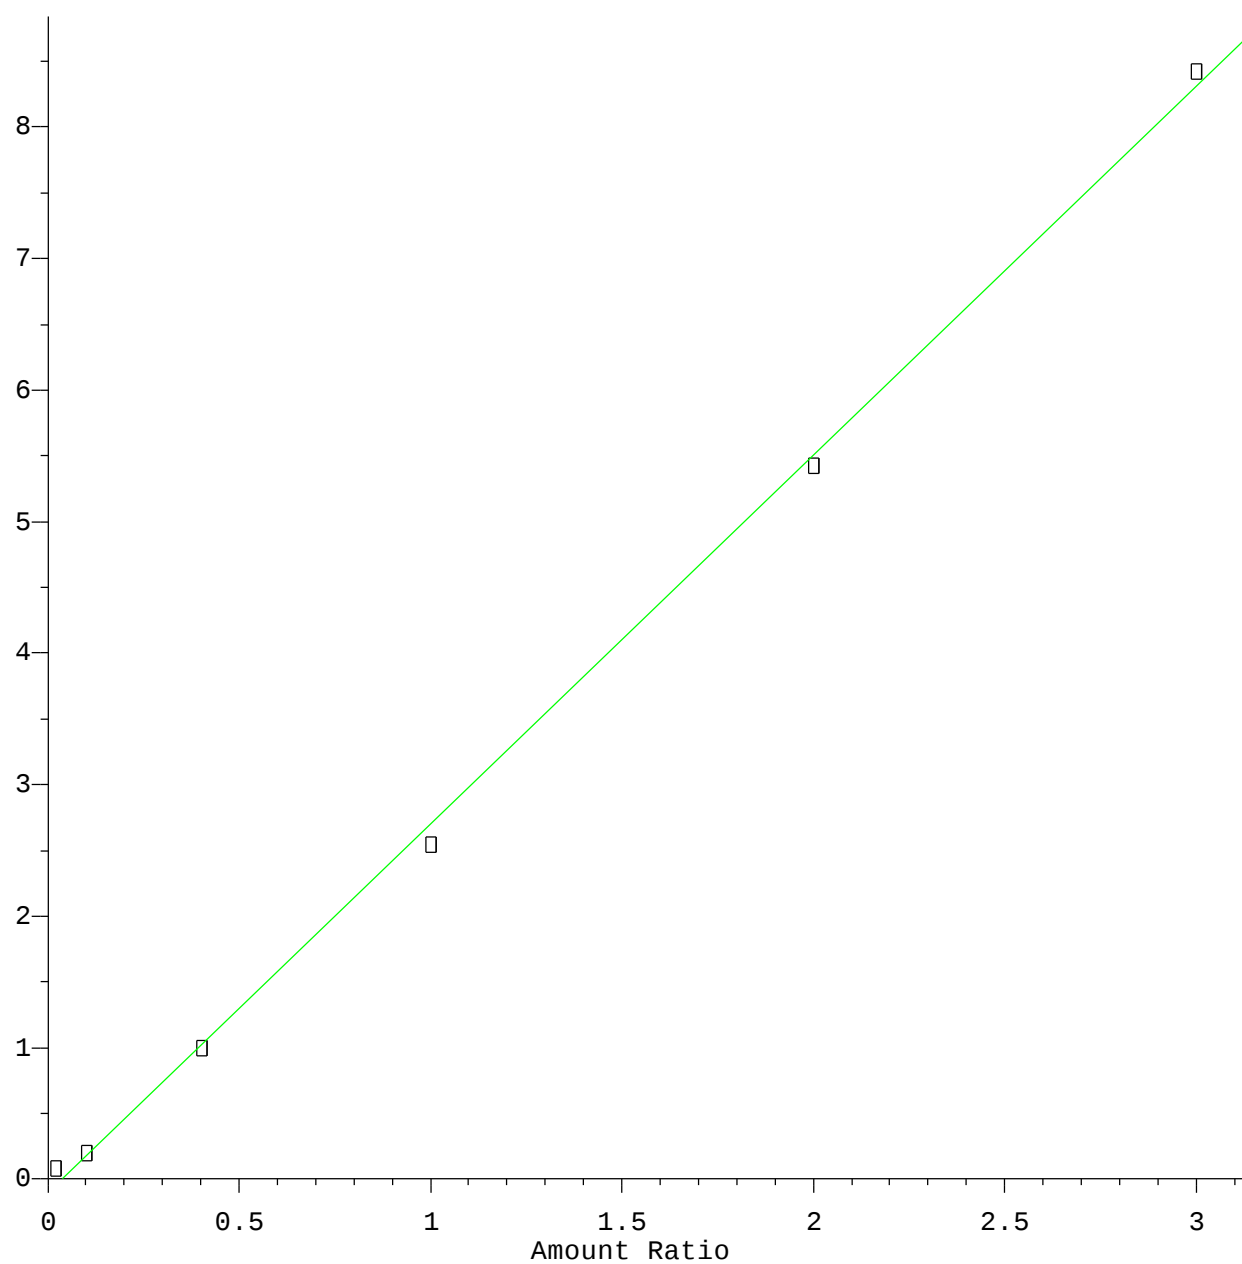


Resp Ratio = 2.81e+000 * Amt - 1.08e-001
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
Calibration Table Last Updated: Thu Oct 01 01:46:38 2020


1,2,3-Trichlorobenzene

Response Ratio

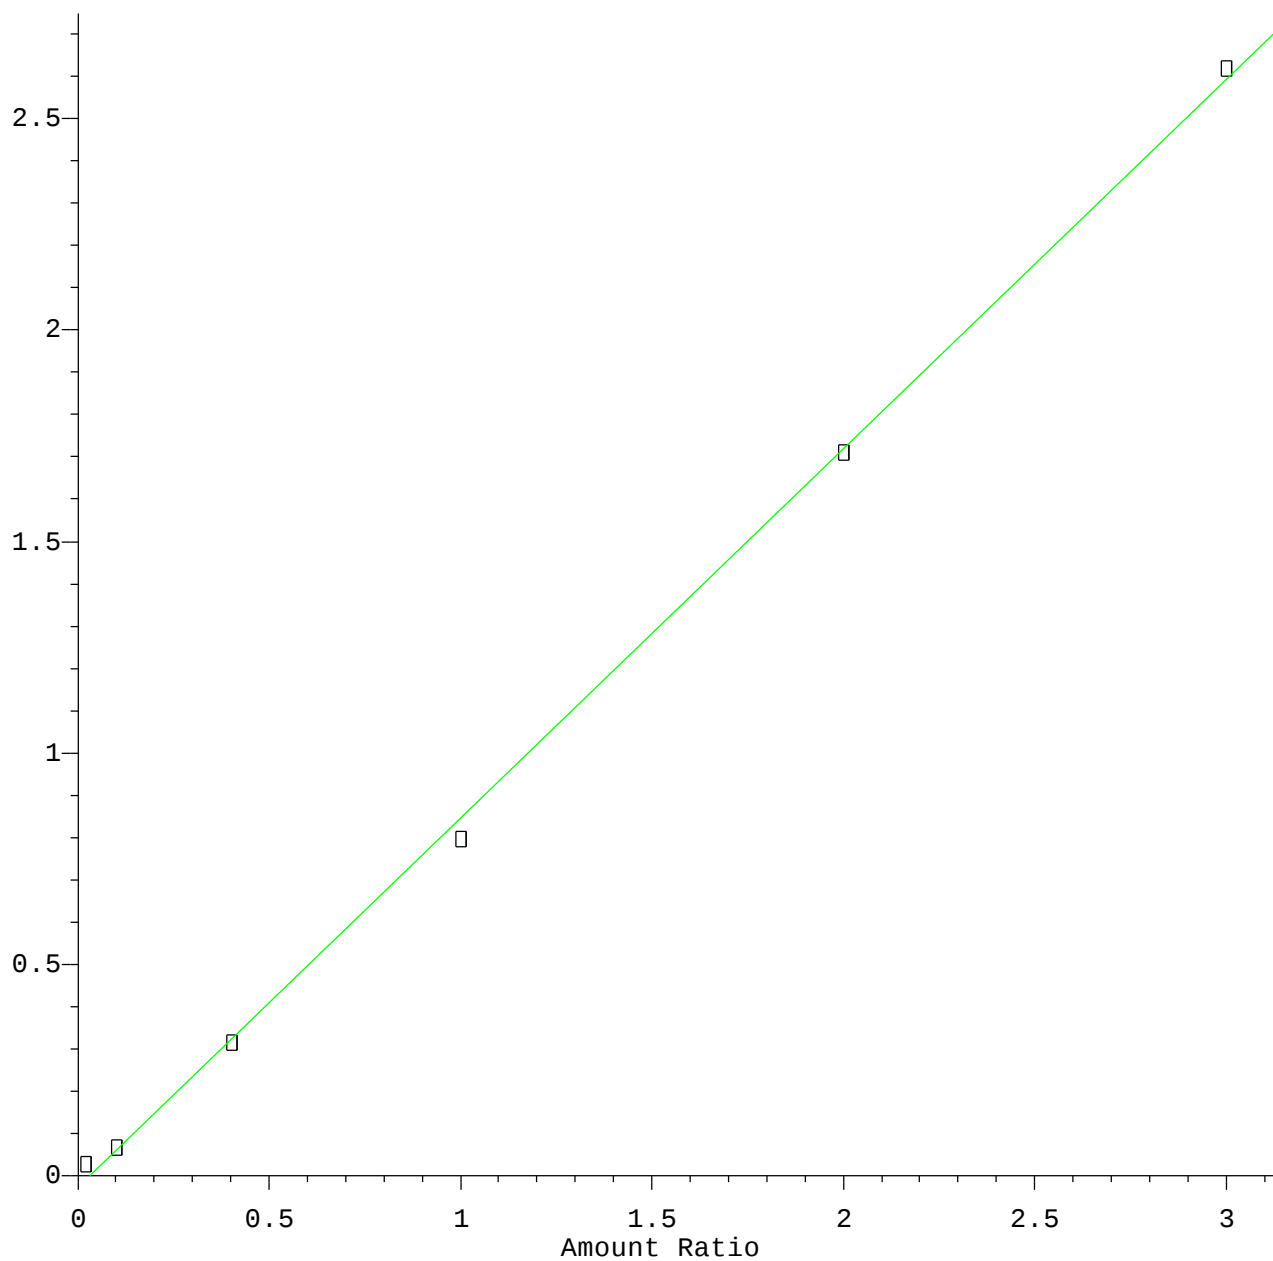

Resp Ratio = $8.73 \times 10^{-1} \times \text{Amt} - 2.74 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
Calibration Table Last Updated: Thu Oct 01 01:46:38 2020

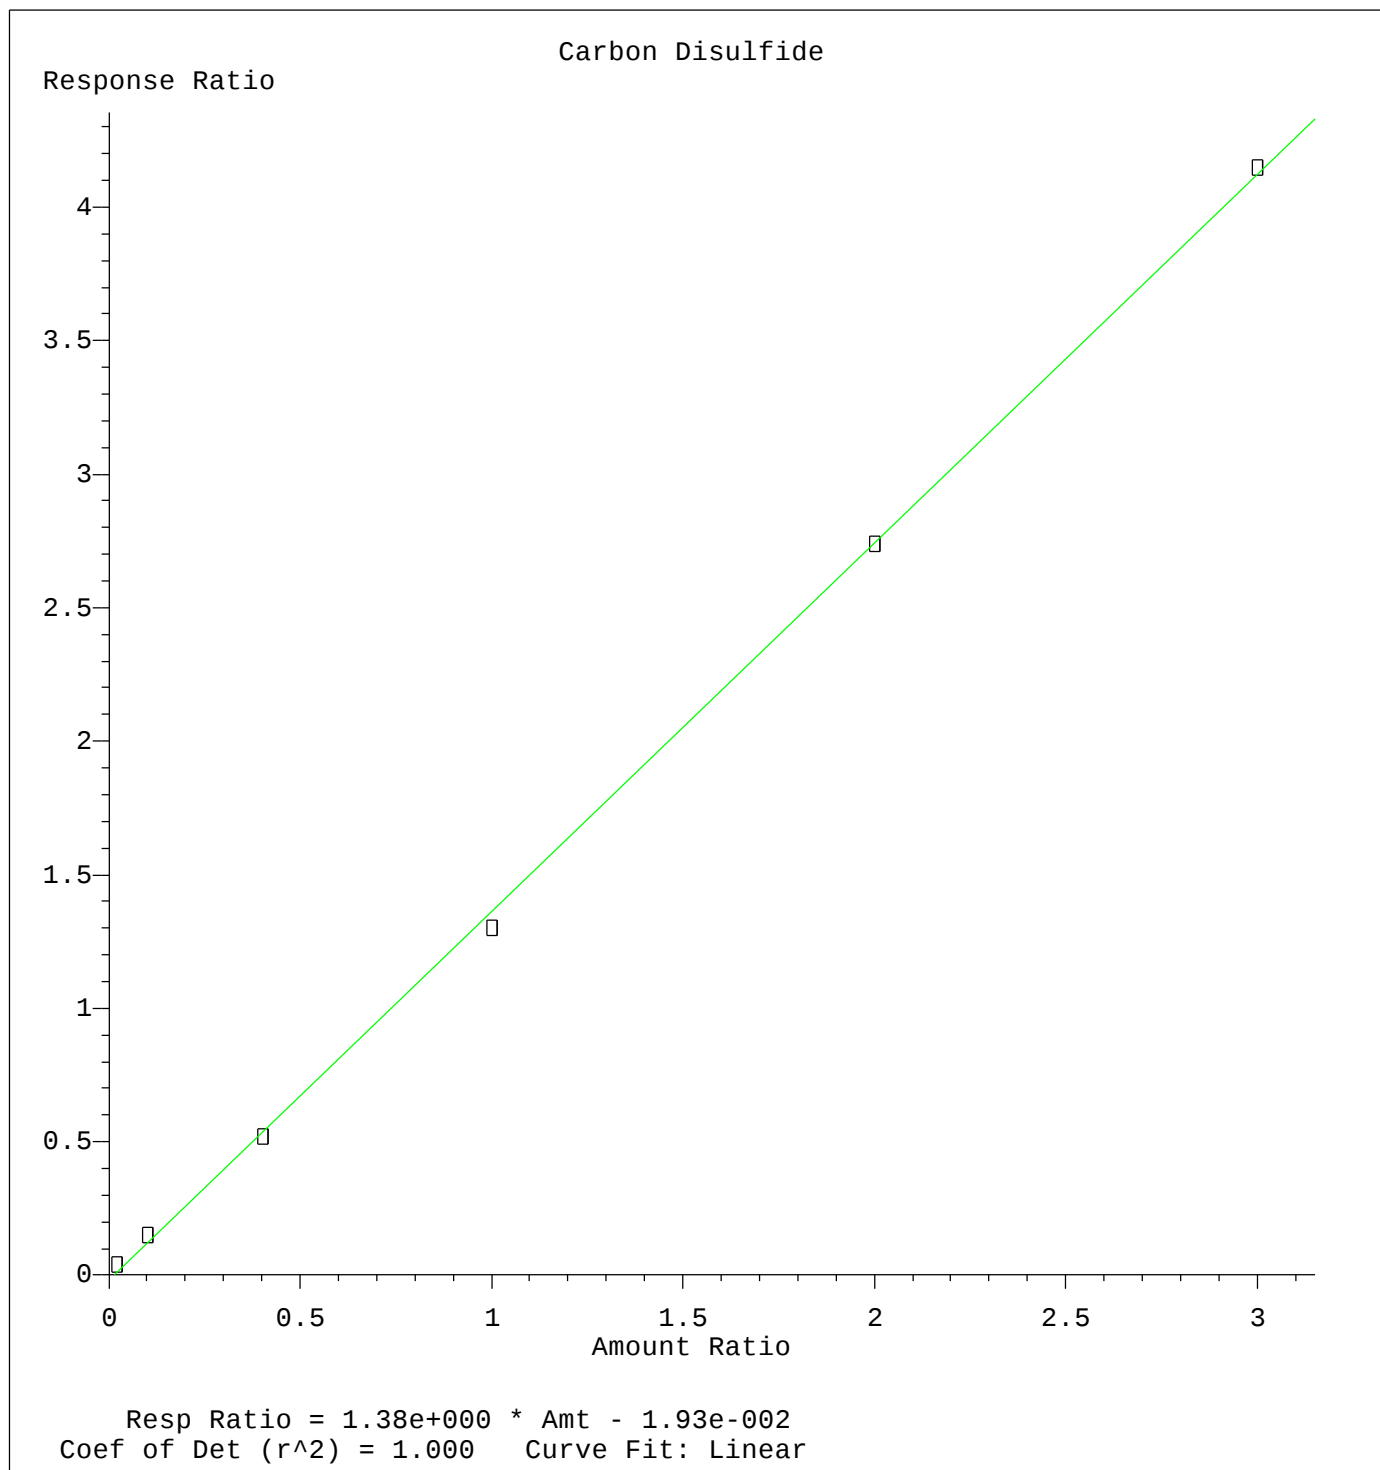

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
Calibration Table Last Updated: Thu Oct 01 01:46:38 2020


Methylene Chloride

Response Ratio

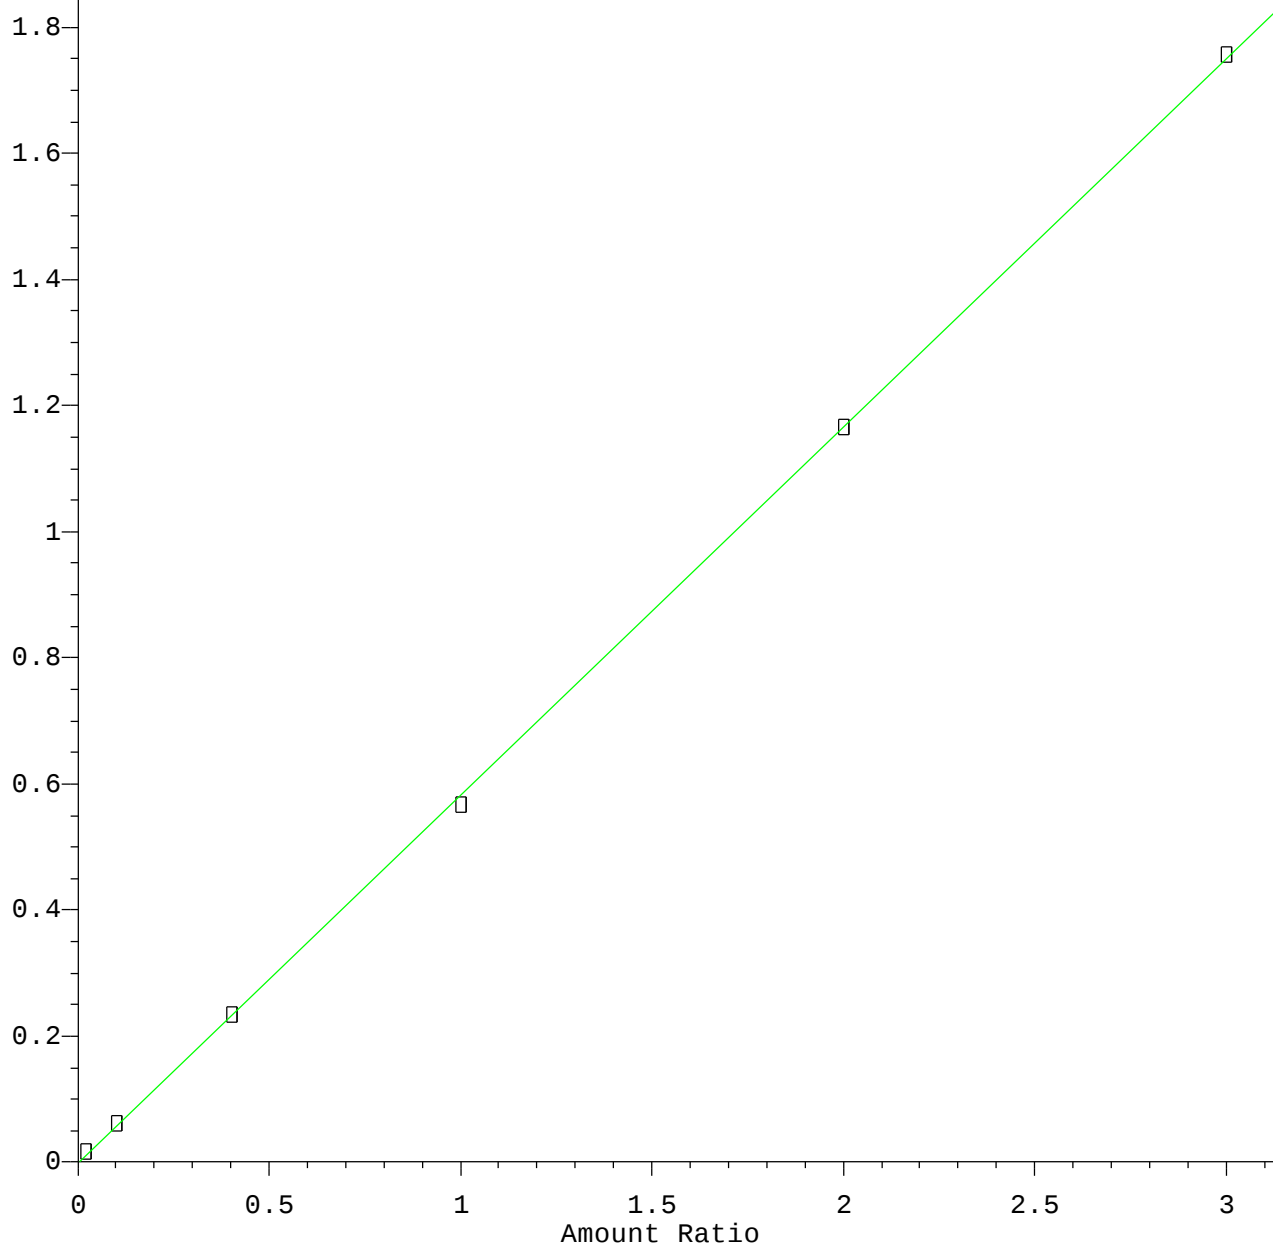

Resp Ratio = 5.84e-001 * Amt - 1.14e-003
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
Calibration Table Last Updated: Thu Oct 01 01:46:38 2020

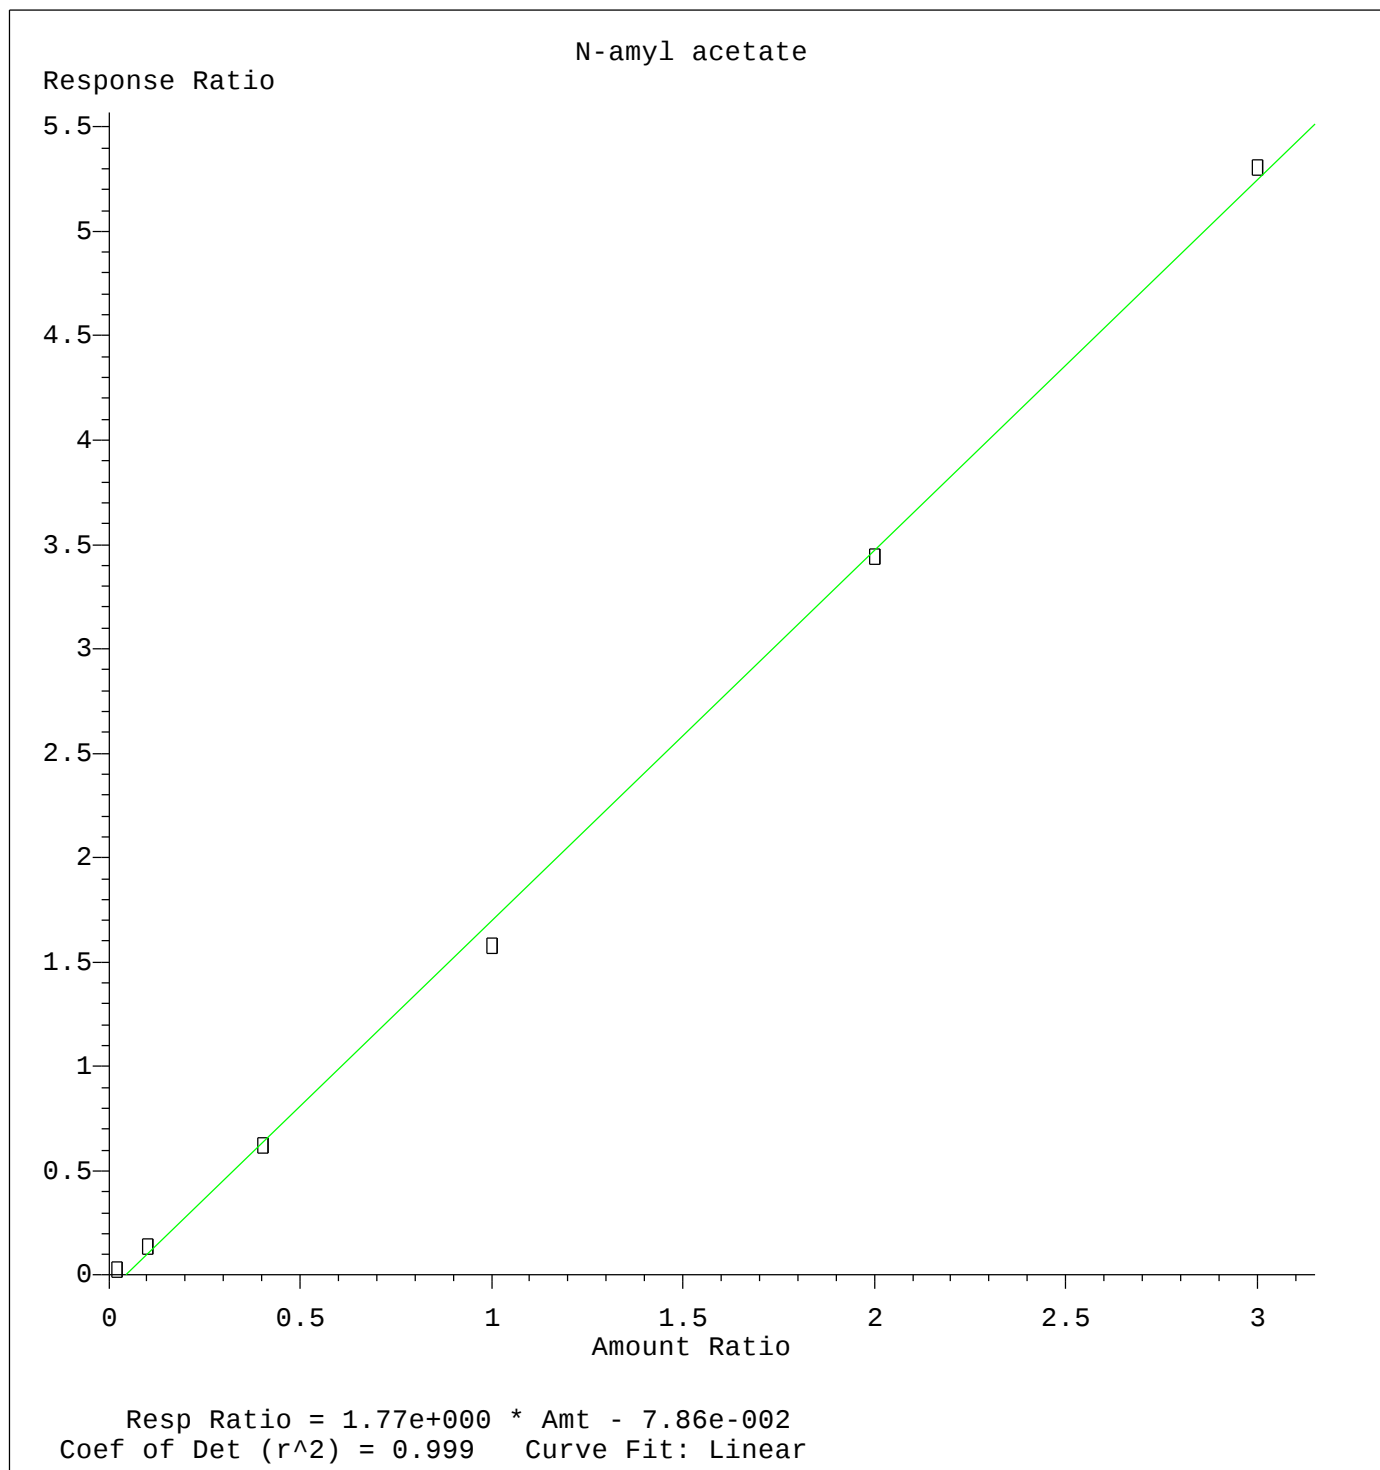

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
Calibration Table Last Updated: Thu Oct 01 01:46:38 2020

1,2,4-Trichlorobenzene

Response Ratio

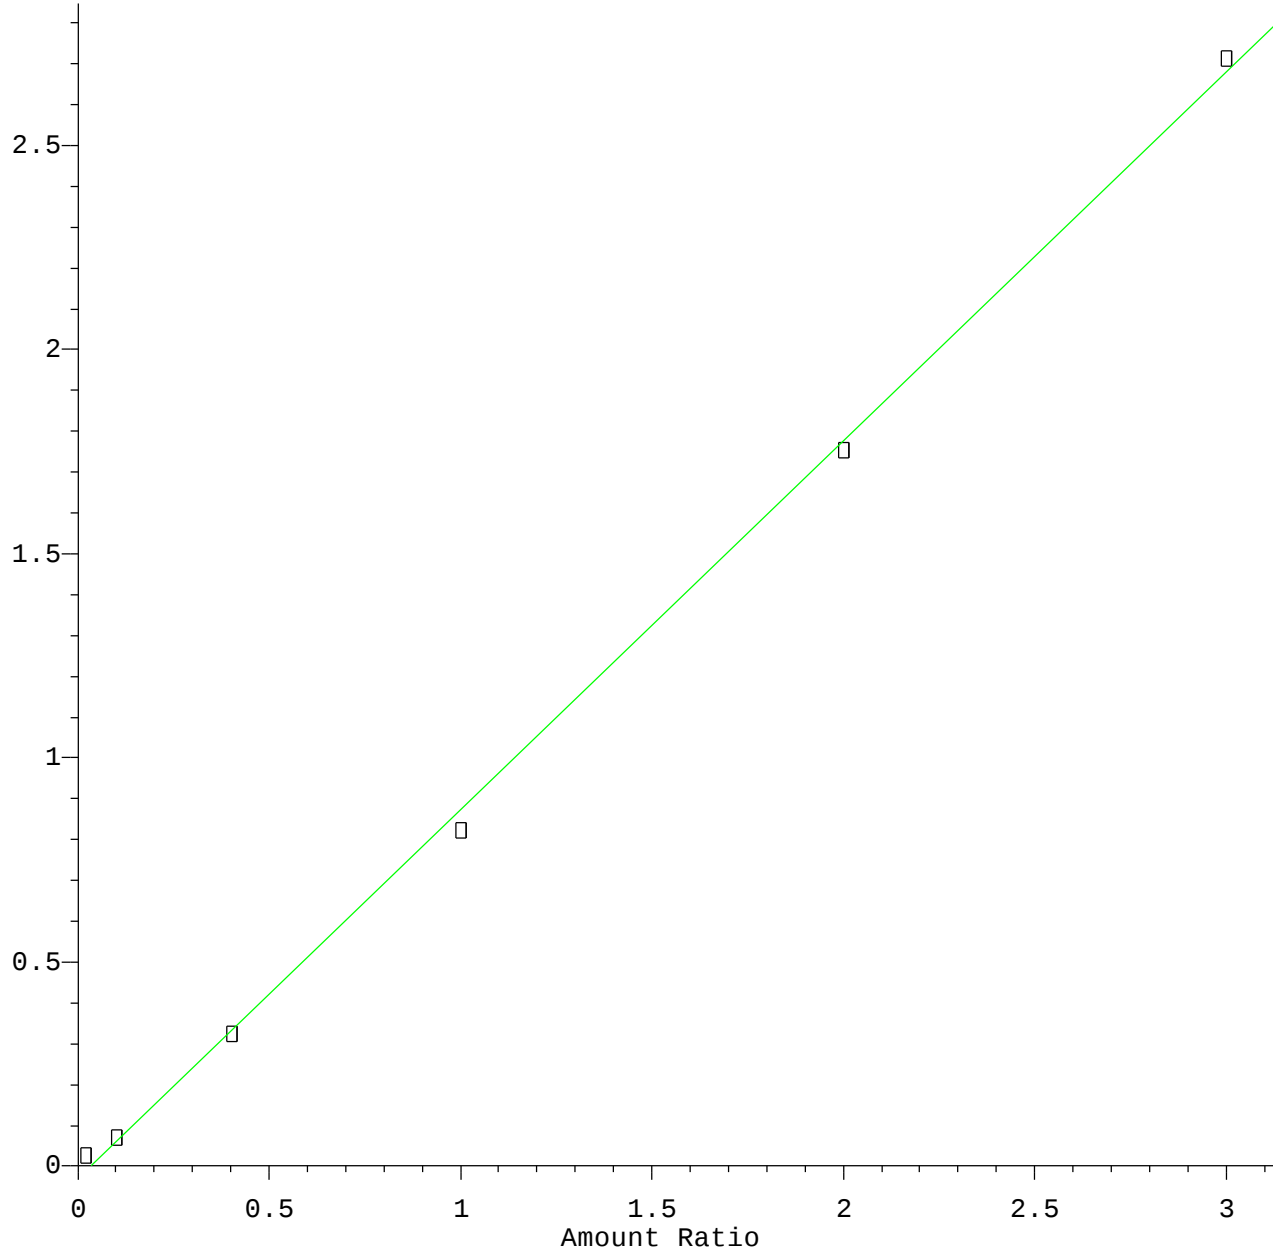

Resp Ratio = 9.03×10^{-1} * Amt - 3.14×10^{-2}
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
Calibration Table Last Updated: Thu Oct 01 01:46:38 2020