

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN093020\
 Data File : VN063745.D
 Acq On : 30 Sep 2020 13:27
 Operator : JC/MD
 Sample : VN0930MBL01
 Misc : 5.00µ/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0930MBL01

Quant Time: Oct 01 02:26:23 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 01 01:46:38 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.62	168	242180	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	435464	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	428666	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	183202	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.99	65	197072	49.26	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.52%	
35) Dibromofluoromethane	7.55	113	143233	47.40	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.80%	
50) Toluene-d8	10.06	98	550575	48.07	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.14%	
62) 4-Bromofluorobenzene	12.38	95	212012	49.24	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.48%	


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN093020\
Data File : VN063745.D
Acq On : 30 Sep 2020 13:27
Operator : JC/MD
Sample : VN0930MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0930MBL01

Quant Time: Oct 01 02:26:23 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 01 01:46:38 2020
Response via : Initial Calibration

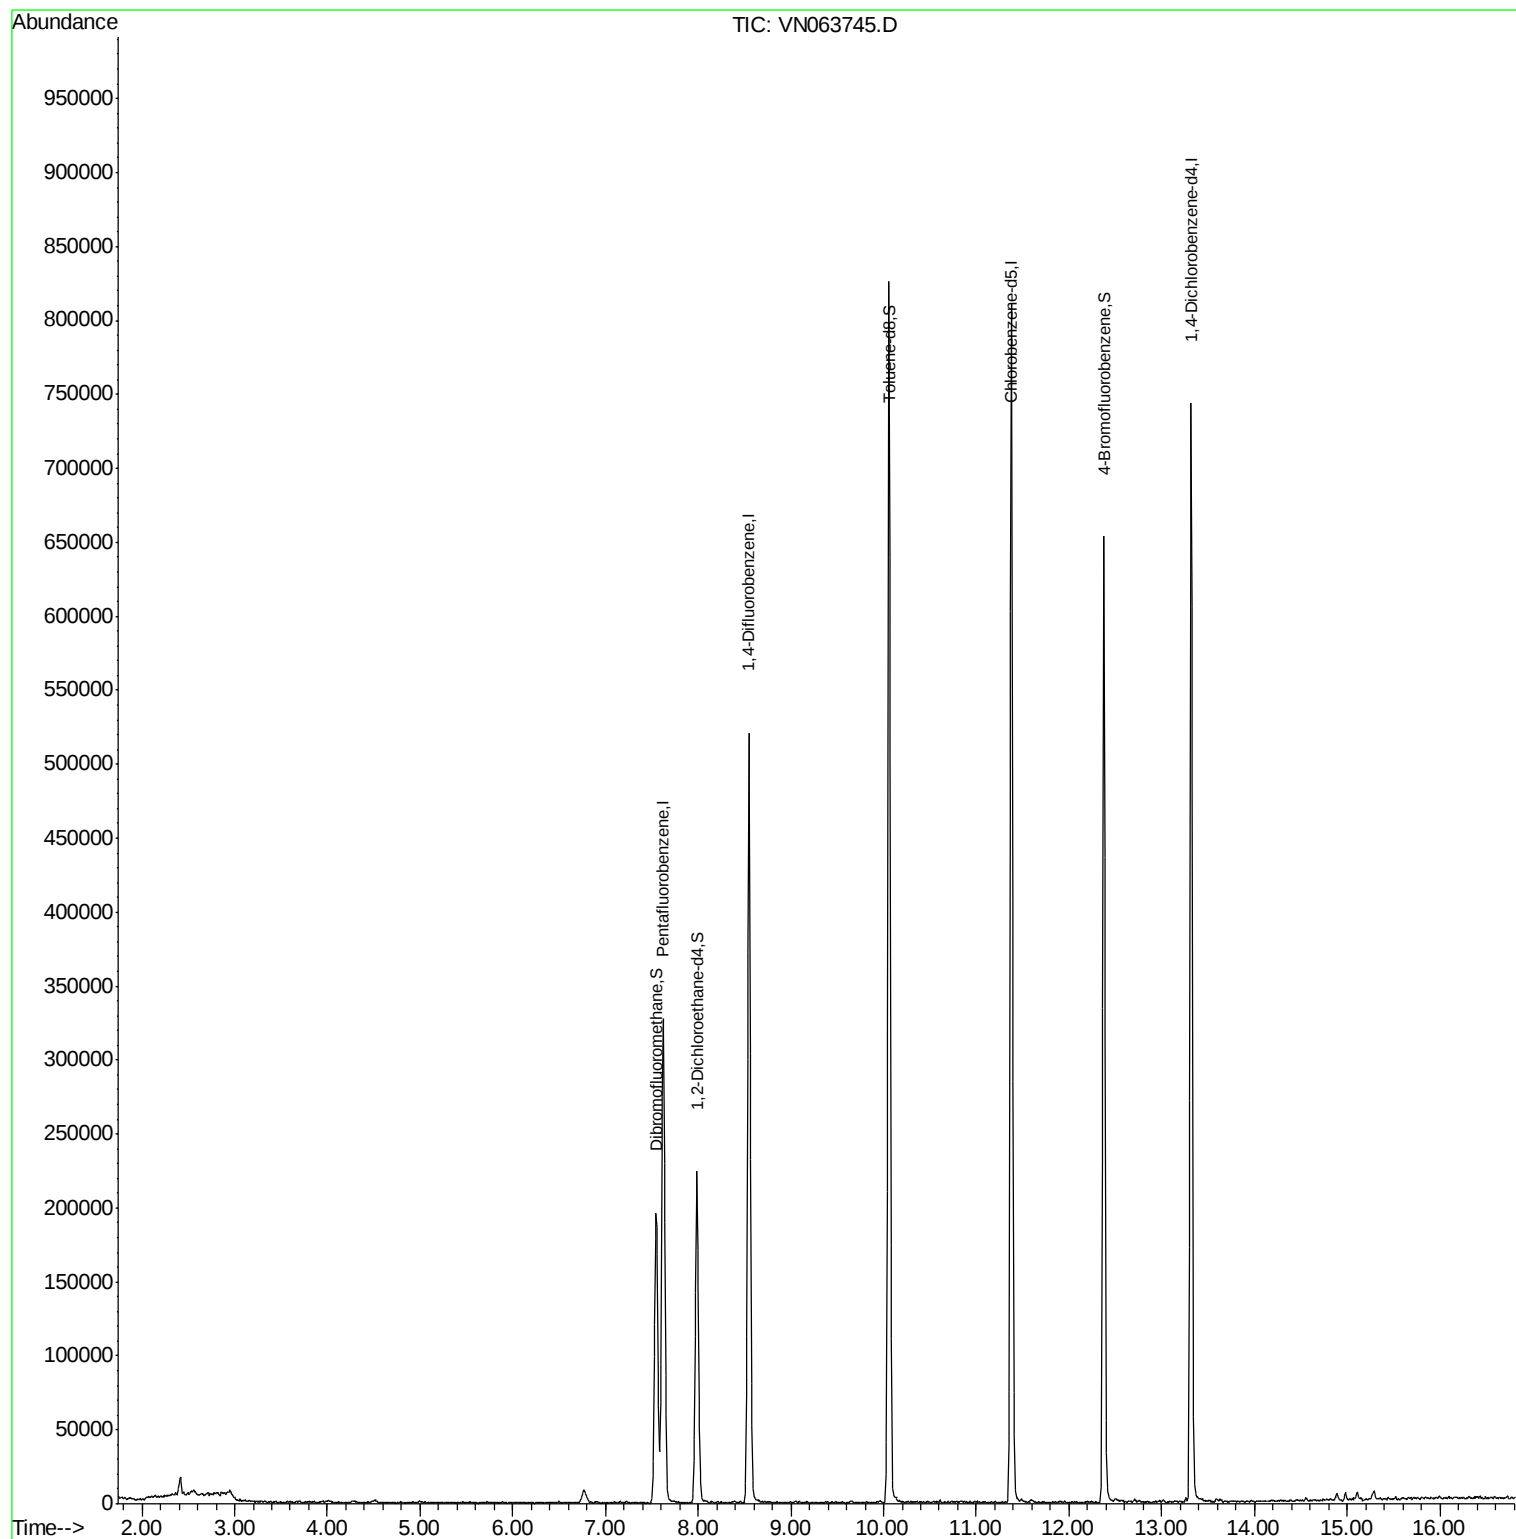



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.62 min Scan# 1830

Delta R.T. -0.00 min

Lab File: VN063745.D

Acq: 30 Sep 2020 13:27

Instrument :

MSVOA_N

ClientSampleId :


VN0930MBL01

Tot Ion:168 Resp: 242180

Ion Ratio Lower Upper

168 100

99 64.4 51.8 77.6

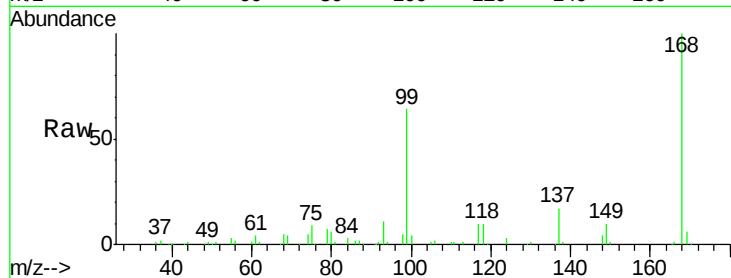

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

7.62

120000

100000

80000



60000

40000

20000

0

Time--> 7.50 7.60 7.70

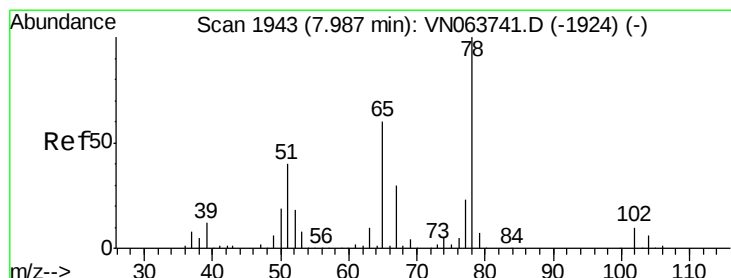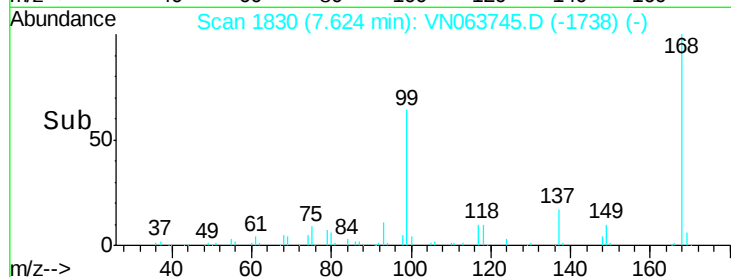

#33

1,2-Dichloroethane-d4

Concen: 49.256 ug/l

RT: 7.99 min Scan# 1943

Delta R.T. 0.00 min

Lab File: VN063745.D


Acq: 30 Sep 2020 13:27

Tgt Ion: 65 Resp: 197072

Ion Ratio Lower Upper

65 100

67 50.2 0.0 99.6

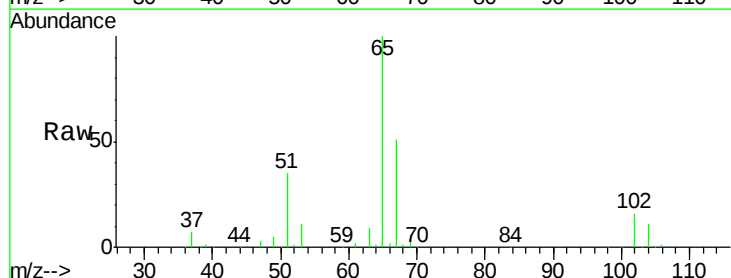

Abundance Ion 64.90 (64.60 to 65.60): VN0

Ion 66.90 (66.60 to 67.60): VN0

7.99

100000

80000


60000


40000

20000

0

Time--> 7.90 7.95 8.00 8.05 8.10

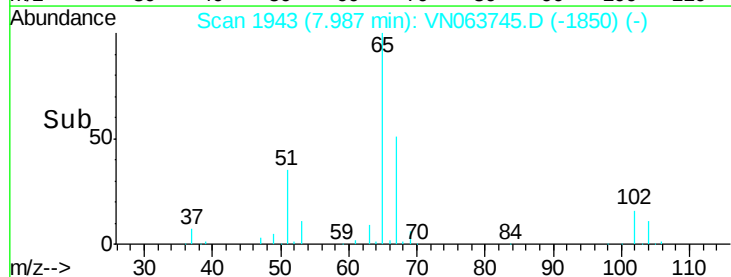

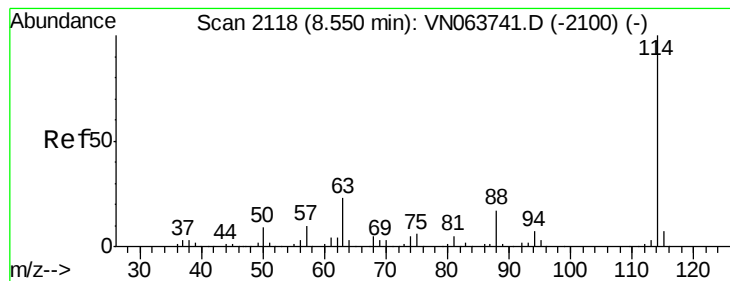

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.55 min Scan# 2118

Delta R.T. 0.00 min

Lab File: VN063745.D

Acq: 30 Sep 2020 13:27

Instrument :

MSVOA_N

ClientSampleId :

VN0930MBL01


Tot Ion:114 Resp: 435464

Ion Ratio Lower Upper

114 100

63 22.4 0.0 45.0




88 16.3 0.0 34.0

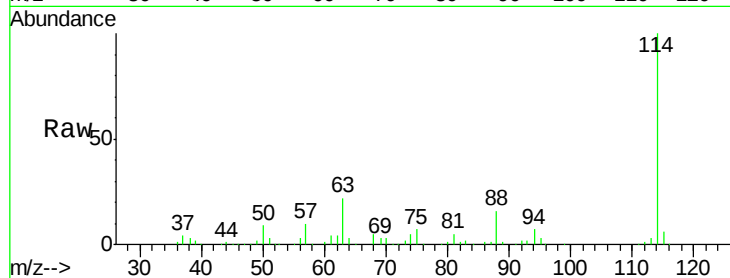

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN

Ion 87.90 (87.60 to 88.60): VN

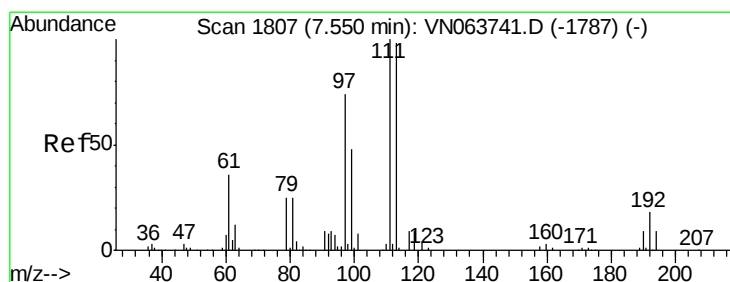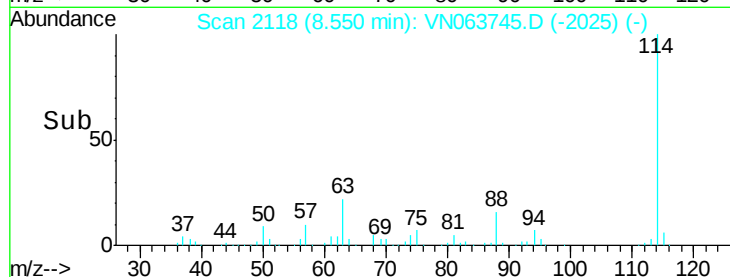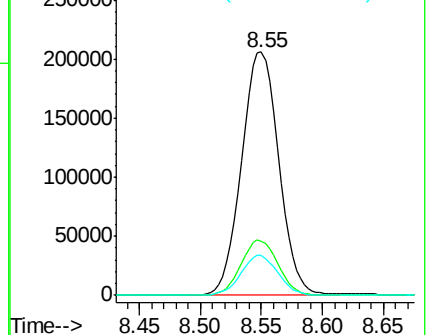

#35

Dibromofluoromethane

Concen: 47.403 ug/l

RT: 7.55 min Scan# 1807

Delta R.T. 0.00 min

Lab File: VN063745.D

Acq: 30 Sep 2020 13:27


Tgt Ion:113 Resp: 143233

Ion Ratio Lower Upper

113 100

111 103.0 81.8 122.8



192 18.8 14.2 21.2

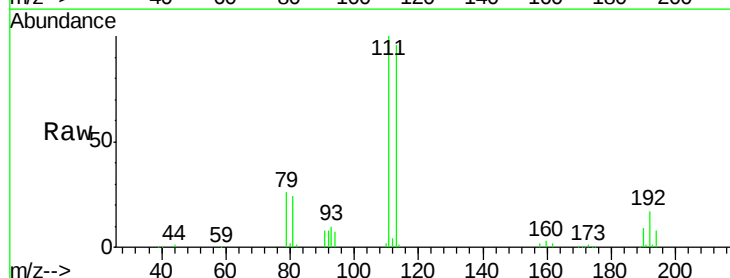


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

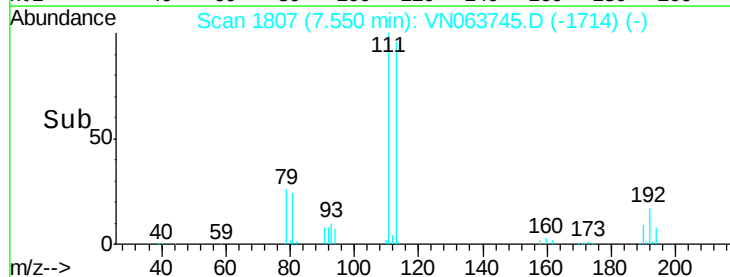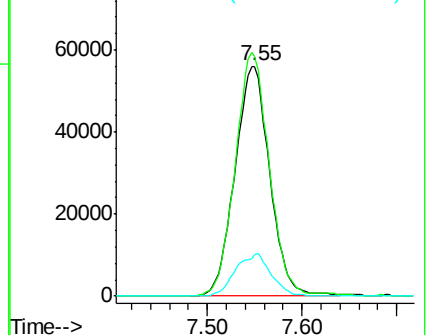

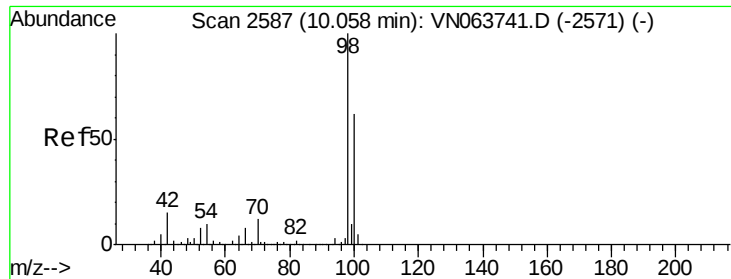

#50

Toluene-d8

Concen: 48.066 ug/l

RT: 10.06 min Scan# 2587

Delta R.T. 0.00 min

Lab File: VN063745.D

Acq: 30 Sep 2020 13:27

Instrument :

MSVOA_N

ClientSampleId :





VN0930MBL01

Tot Ion: 98 Resp: 550575

Ion Ratio Lower Upper

98 100

100 63.2 49.8 74.6

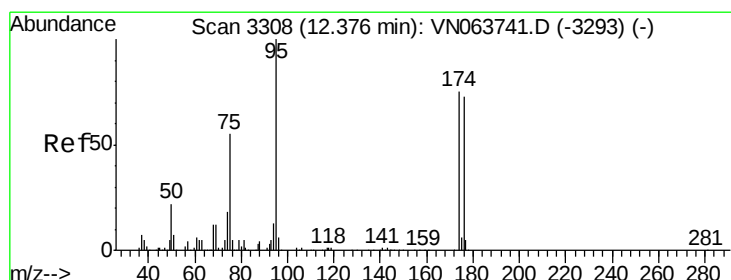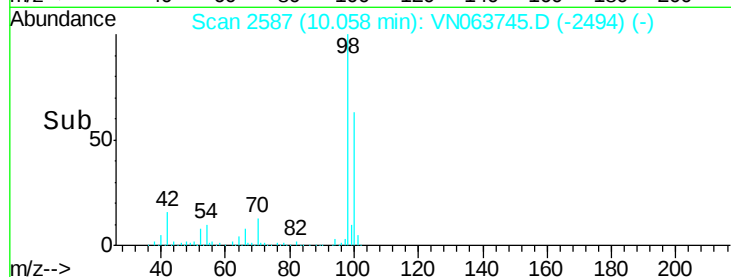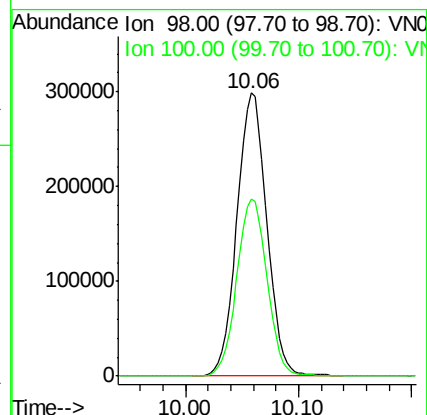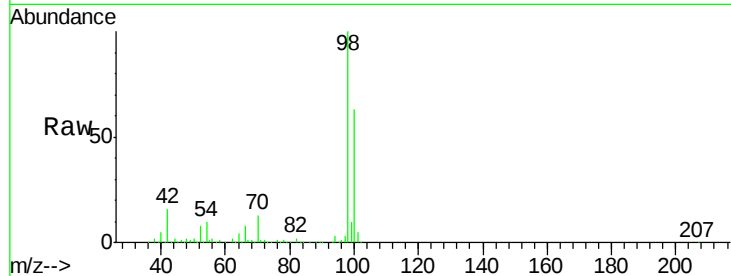

#62

4-Bromofluorobenzene

Concen: 49.238 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. 0.00 min

Lab File: VN063745.D

Acq: 30 Sep 2020 13:27




Tgt Ion: 95 Resp: 212012


Ion Ratio Lower Upper

95 100

174 75.7 0.0 150.6

176 72.8 0.0 145.4


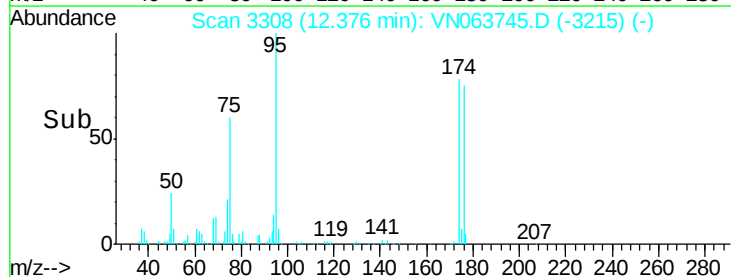
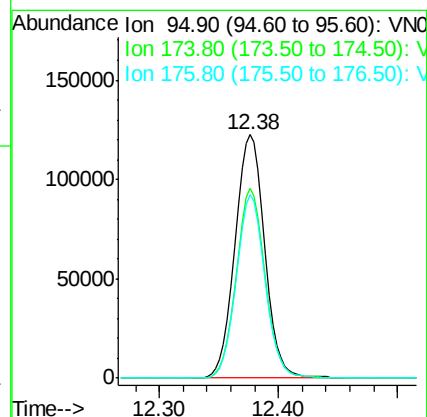
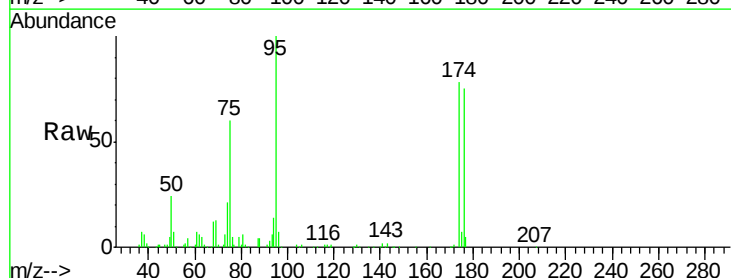


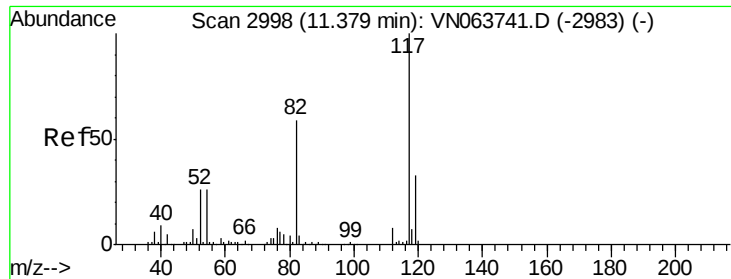

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2998
Delta R.T. 0.00 min
Lab File: VN063745.D
Acq: 30 Sep 2020 13:27

Instrument :
MSVOA_N
ClientSampleId :
VN0930MBL01

Tot Ion:117 Resp: 428666
Ion Ratio Lower Upper
117 100
82 59.7 47.4 71.2
119 31.9 26.4 39.6

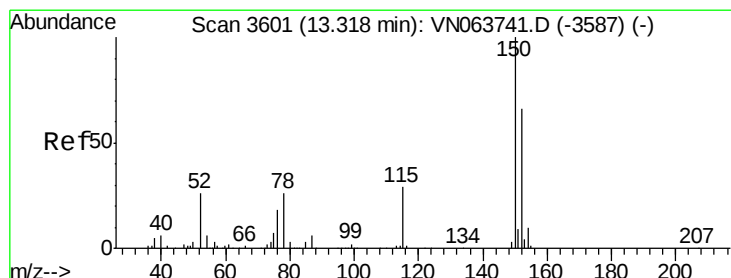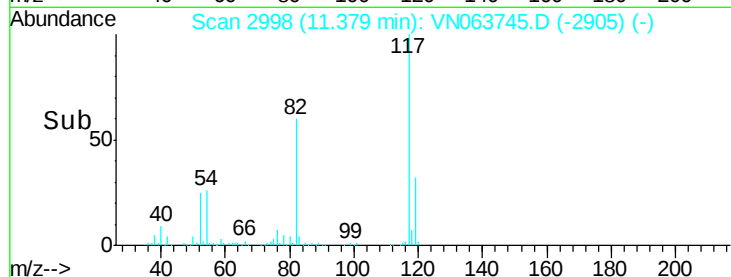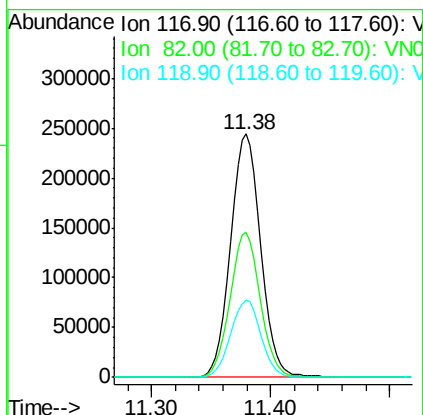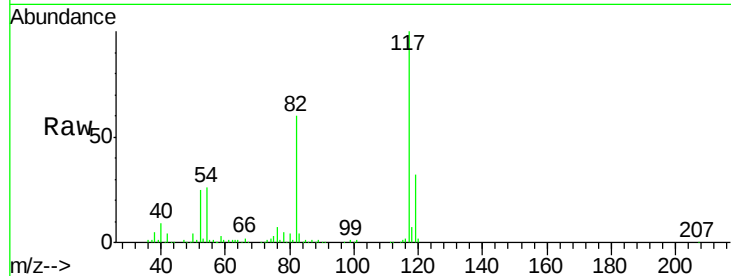

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.32 min Scan# 3601
Delta R.T. 0.00 min
Lab File: VN063745.D
Acq: 30 Sep 2020 13:27

Tgt Ion:152 Resp: 183202
Ion Ratio Lower Upper
152 100
115 62.7 31.3 93.8
150 156.6 0.0 341.8

