
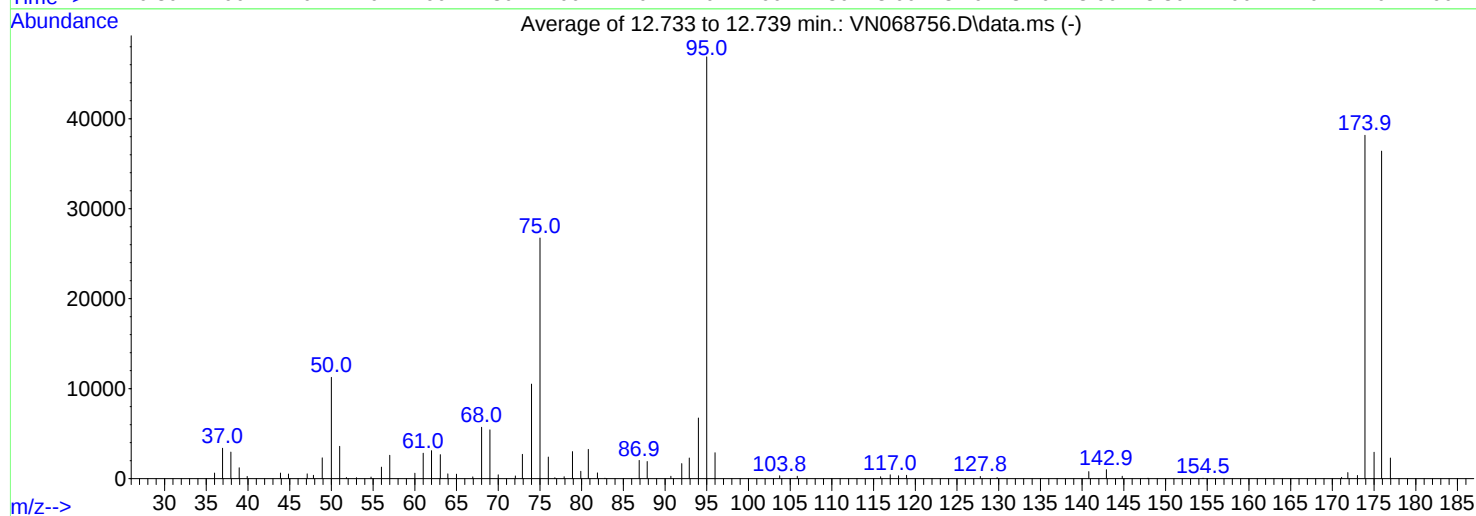


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN093021\
 Data File : VN068756.D
 Acq On : 30 Sep 2021 8:46
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N092921W.M
 Title : SW846 8260
 Last Update : Wed Sep 29 23:31:35 2021

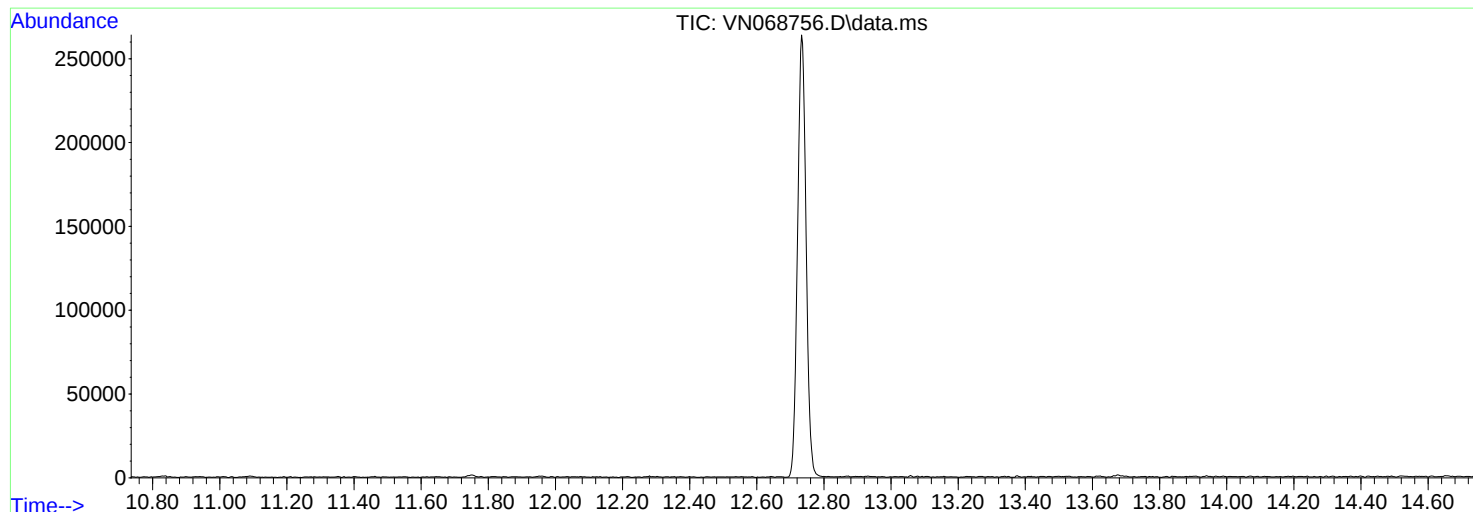

AutoFind: Scans 4006, 4007, 4008; Background Corrected with Scan 3989

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.0	11259	PASS
75	95	30	60	57.0	26744	PASS
95	95	100	100	100.0	46880	PASS
96	95	5	9	6.2	2889	PASS
173	174	0.00	2	0.9	353	PASS
174	95	50	100	81.4	38165	PASS
175	174	5	9	7.7	2938	PASS
176	174	95	101	95.4	36408	PASS
177	176	5	9	6.3	2299	PASS