


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN093022\
 Data File : VN074659.D
 Acq On : 30 Sep 2022 09:06
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N092922W.M
 Title : SW846 8260
 Last Update : Fri Sep 30 07:44:59 2022

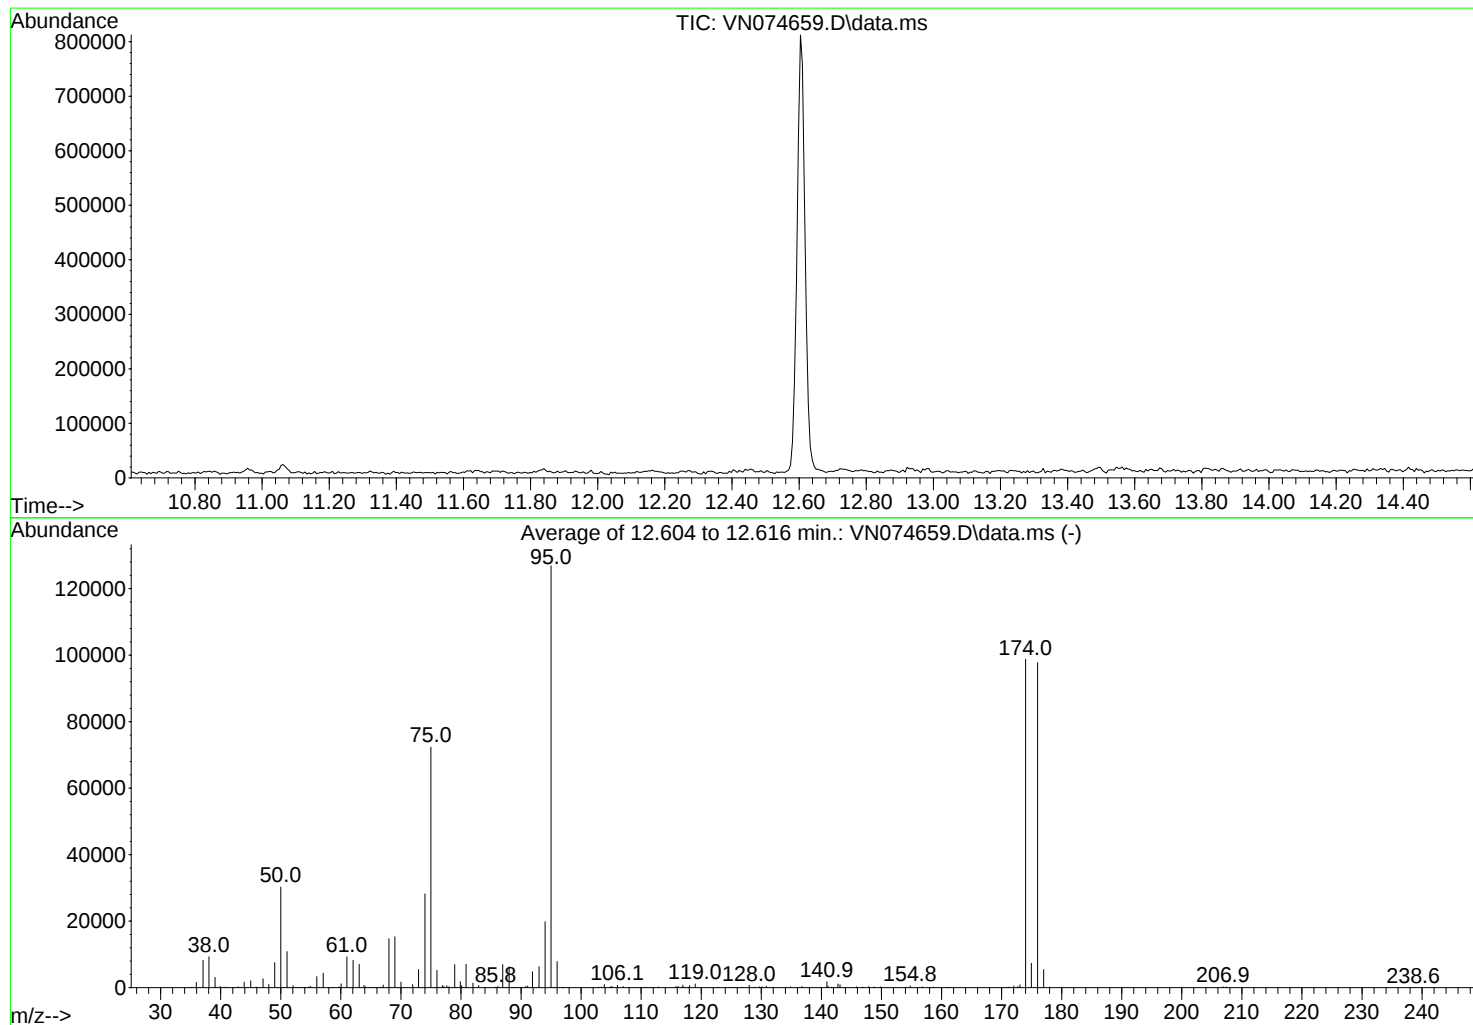

AutoFind: Scans 1822, 1823, 1824; Background Corrected with Scan 1813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.9	30288	PASS
75	95	30	60	57.0	72339	PASS
95	95	100	100	100.0	126869	PASS
96	95	5	9	6.2	7855	PASS
173	174	0.00	2	0.9	865	PASS
174	95	50	100	77.8	98741	PASS
175	174	5	9	7.4	7314	PASS
176	174	95	101	99.0	97749	PASS
177	176	5	9	5.6	5451	PASS