
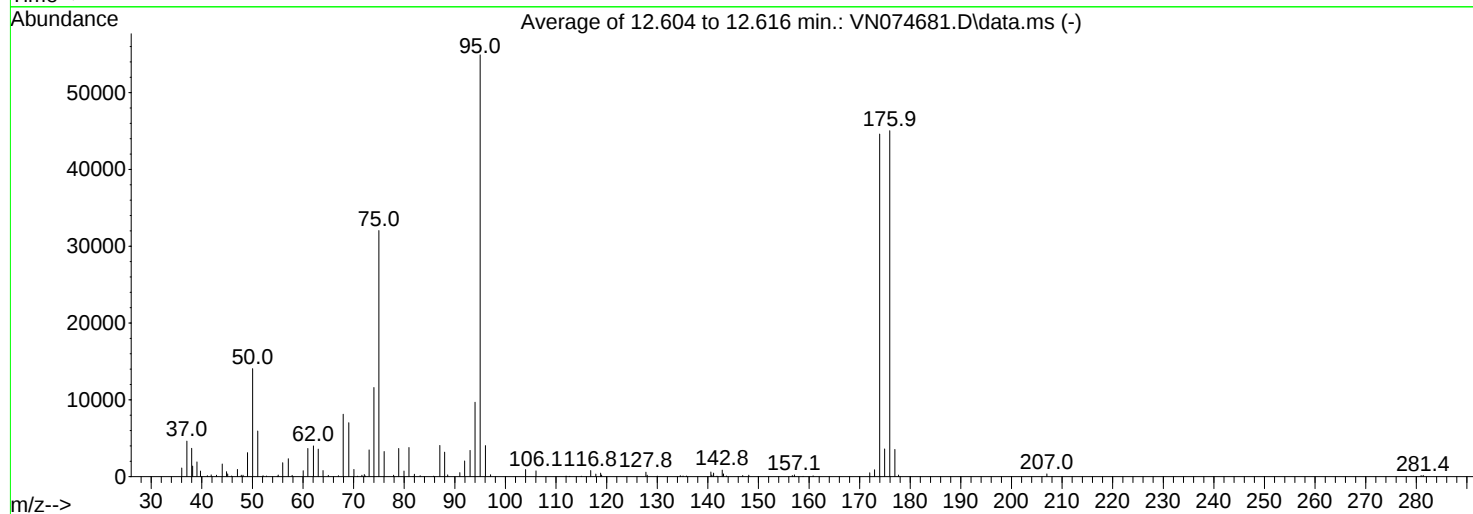


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN093022\
Data File : VN074681.D
Acq On : 01 Oct 2022 00:33
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N092922W.M
Title : SW846 8260
Last Update : Fri Sep 30 07:44:59 2022

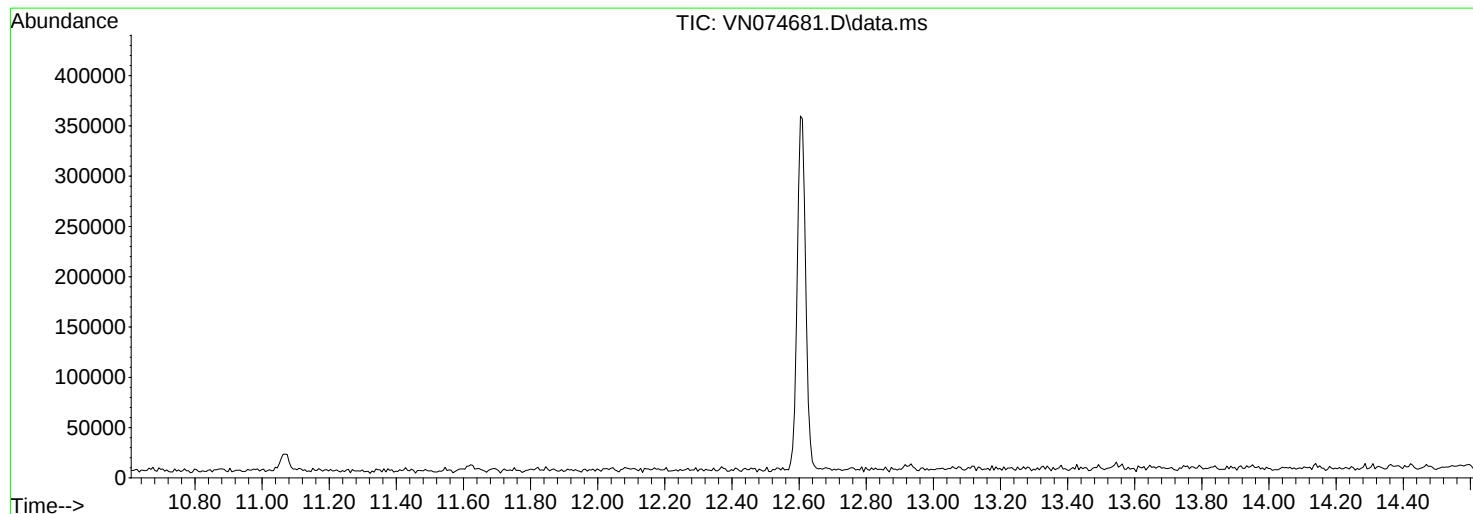

AutoFind: Scans 1822, 1823, 1824; Background Corrected with Scan 1814

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	25.6	14054	PASS
75	95	30	60	58.3	32043	PASS
95	95	100	100	100.0	54917	PASS
96	95	5	9	7.4	4051	PASS
173	174	0.00	2	2.0	900	PASS
174	95	50	100	81.2	44608	PASS
175	174	5	9	8.1	3613	PASS
176	174	95	101	101.0	45037	PASS
177	176	5	9	7.9	3541	PASS