
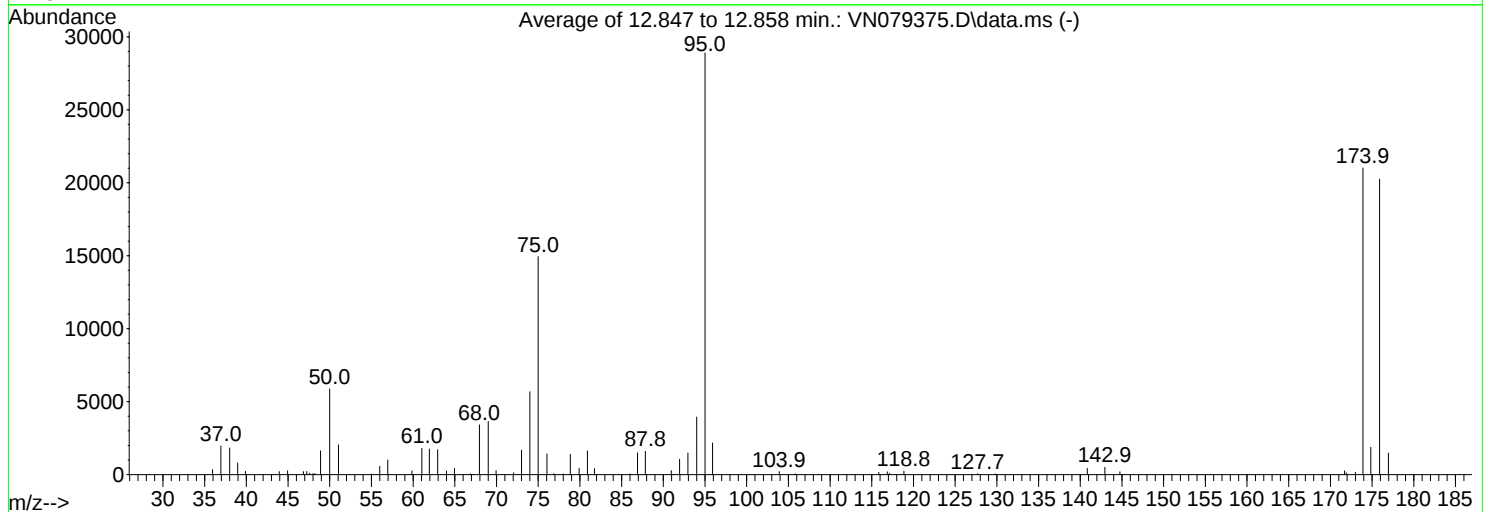


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN093023\
Data File : VN079375.D
Acq On : 30 Sep 2023 10:34
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091123W.M
Title : SW846 8260
Last Update : Tue Sep 12 05:05:24 2023

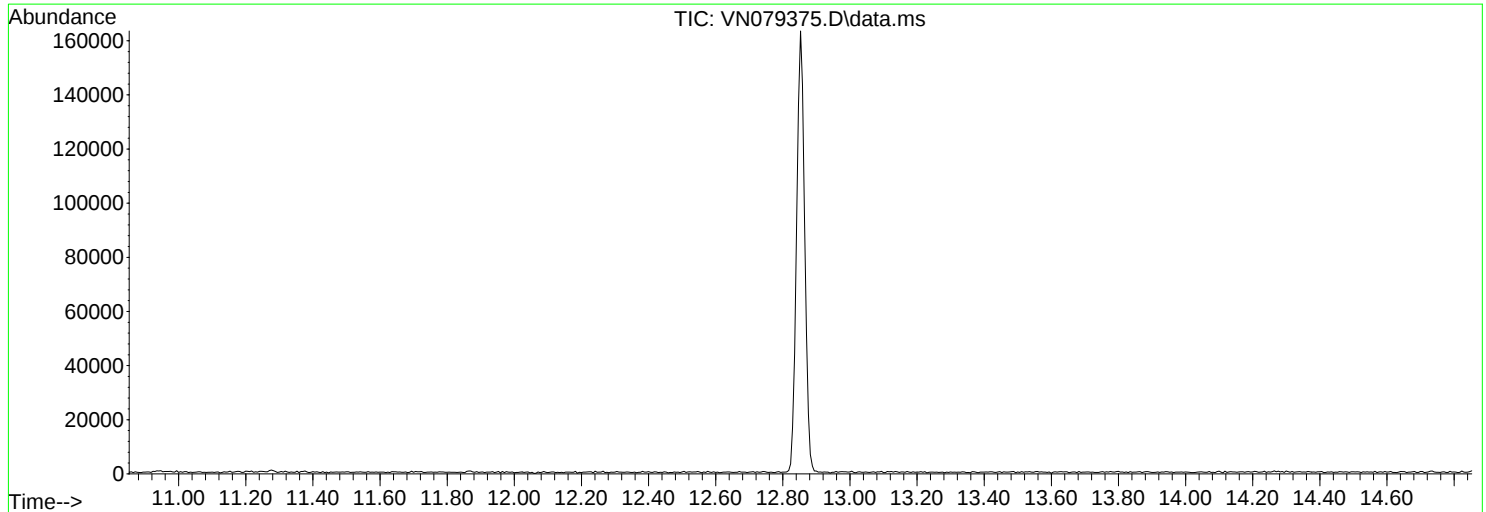

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	5880	PASS
75	95	30	60	51.7	14943	PASS
95	95	100	100	100.0	28904	PASS
96	95	5	9	7.5	2166	PASS
173	174	0.00	2	0.8	164	PASS
174	95	50	100	72.7	21019	PASS
175	174	5	9	8.9	1875	PASS
176	174	95	101	96.3	20248	PASS
177	176	5	9	7.3	1476	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	355	48.20	68	64.00	254	76.90	61
36.95	1960	48.90	1639	64.95	430	78.00	51
38.00	1835	50.00	5880	66.90	54	78.85	139
38.95	804	51.05	2039	67.95	3405	79.90	42
39.90	219	55.00	51	69.00	3639	80.90	1626
43.95	214	56.00	571	69.95	273	81.75	422
44.95	263	56.95	1008	72.05	128	86.00	50
46.85	206	59.85	268	73.00	1675	86.90	1489
47.25	215	61.05	1800	74.00	5684	87.85	1597
47.60	101	61.95	1751	75.00	14943	90.95	271
48.00	64	62.95	1708	76.05	1431	91.95	1050

Average of 12.847 to 12.858 min.: VN079375.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.95	1480	129.80	56				
94.00	3948	140.85	431				
95.00	28904	142.95	503				
95.90	2166	144.75	197				
103.90	214	171.70	266				
105.80	53	171.90	125				
115.85	151	173.00	164				
116.85	198	173.90	21019				
117.10	86	174.85	1875				
118.85	247	175.90	20248				
127.70	61	176.95	1476				

Instrument :
MSVOA_N
ClientSampleId :
BFB