
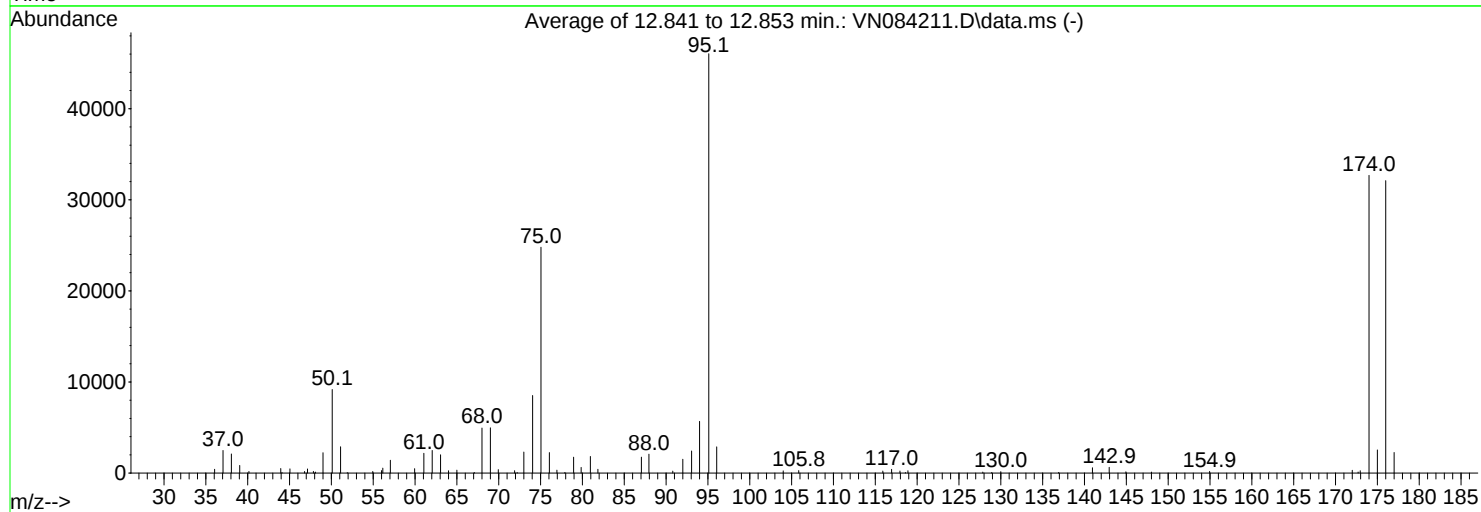


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN093024\
Data File : VN084211.D
Acq On : 30 Sep 2024 09:24
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N093024W.M
Title : SW846 8260
Last Update : Tue Oct 01 07:11:01 2024

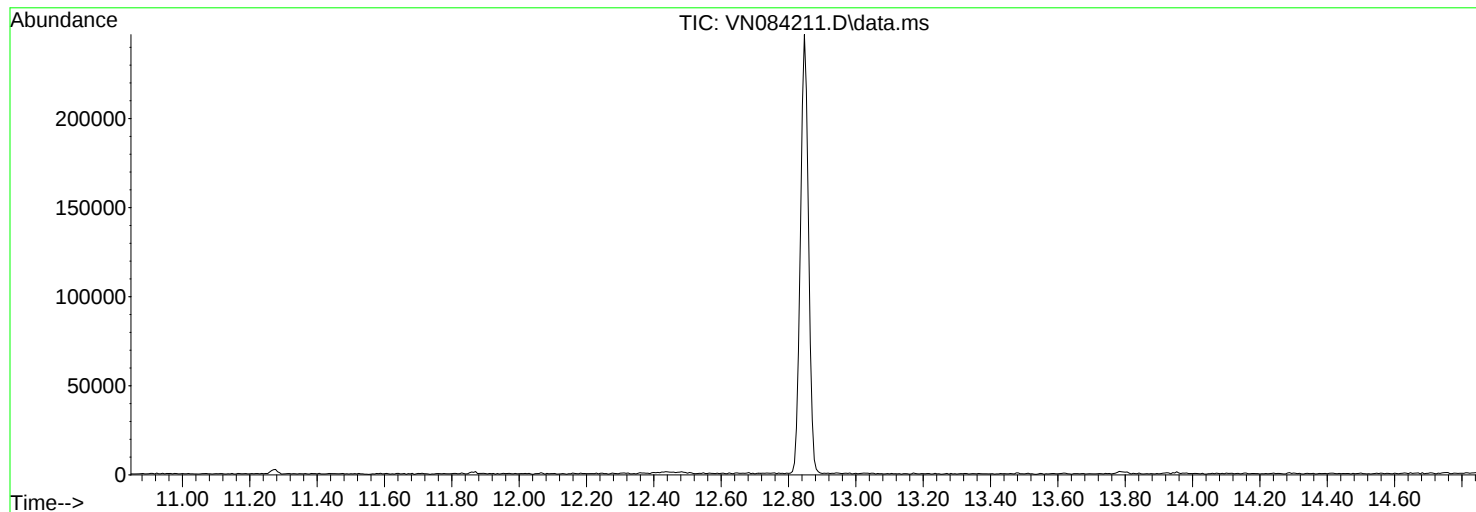

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	9177	PASS
75	95	30	60	53.9	24795	PASS
95	95	100	100	100.0	46040	PASS
96	95	5	9	6.3	2879	PASS
173	174	0.00	2	0.8	259	PASS
174	95	50	100	71.0	32685	PASS
175	174	5	9	7.8	2541	PASS
176	174	95	101	98.2	32104	PASS
177	176	5	9	7.0	2260	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	419	48.10	111	62.05	2483	74.05	8516
37.05	2481	49.00	2237	63.05	2007	75.05	24795
38.05	2101	50.10	9177	64.00	258	76.05	2253
39.05	836	51.10	2891	65.00	322	76.95	323
40.15	179	51.90	55	67.10	55	77.90	67
43.95	503	54.95	179	68.00	4945	78.95	1743
44.10	59	56.00	274	69.00	4971	79.85	625
45.05	462	56.15	545	69.95	382	80.95	1822
46.80	174	57.05	1406	71.90	264	81.85	418
47.15	455	59.95	485	72.20	67	87.05	1750
47.85	183	61.05	2172	73.00	2306	87.95	2078

Average of 12.841 to 12.853 min.: VN084211.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.80	219	118.60	60	172.00	305		
92.00	1521	118.90	261	172.70	115		
93.05	2424	127.85	111	172.95	259		
94.00	5677	128.90	54	174.00	32685		
95.10	46040	130.00	156	175.00	2541		
96.05	2879	136.90	63	176.00	32104		
104.00	245	140.95	584	177.00	2260		
105.85	277	142.95	633				
115.90	223	144.95	142				
116.95	410	148.00	113				
117.95	228	154.95	185				

Instrument :

MSVOA_N

ClientSampleId :

BFB