
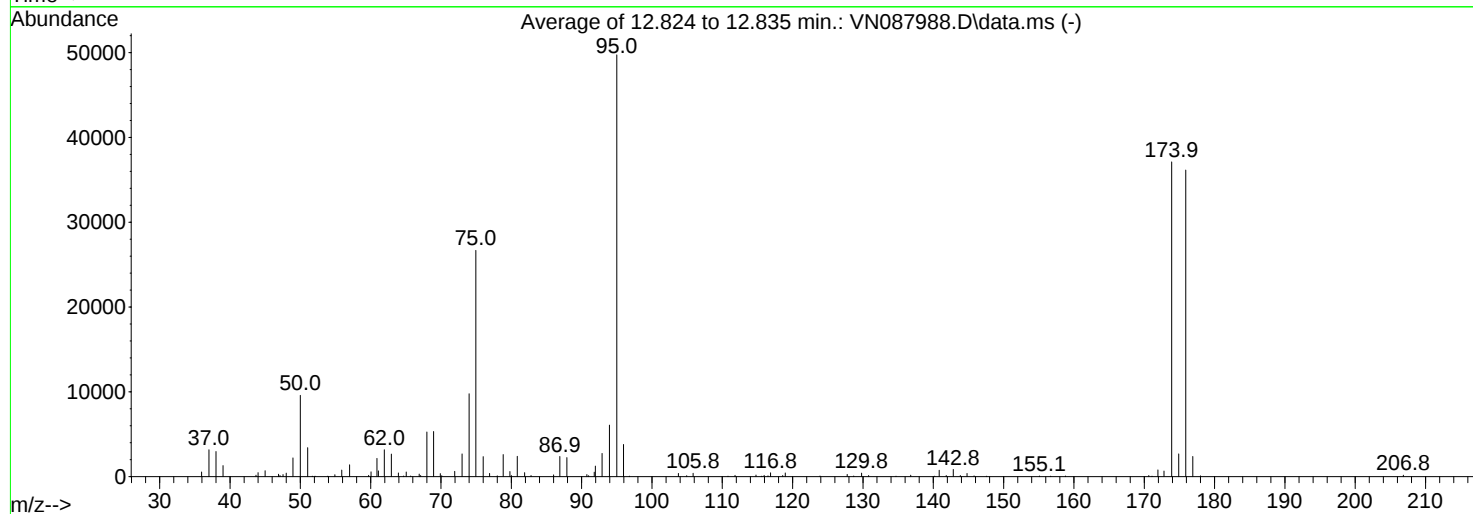


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN093025\
Data File : VN087988.D
Acq On : 30 Sep 2025 08:18
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N092325W.M
Title : SW846 8260
Last Update : Wed Sep 24 05:05:30 2025

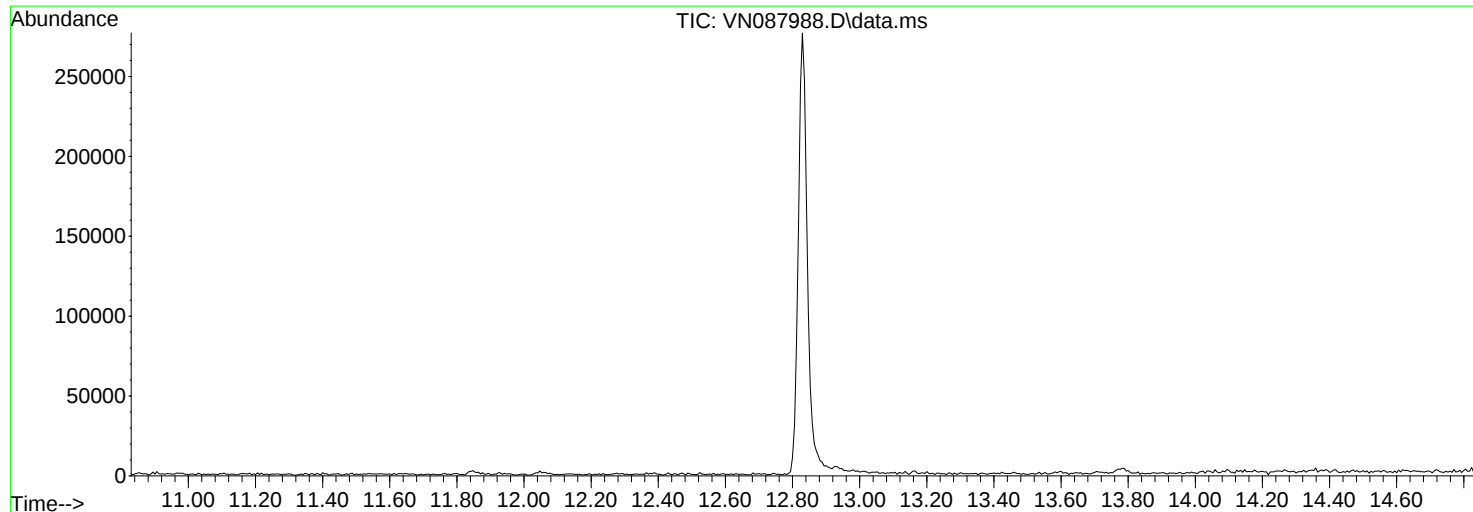

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1838

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	9594	PASS
75	95	30	60	53.7	26688	PASS
95	95	100	100	100.0	49744	PASS
96	95	5	9	7.6	3801	PASS
173	174	0.00	2	1.8	652	PASS
174	95	50	100	74.6	37115	PASS
175	174	5	9	7.2	2682	PASS
176	174	95	101	97.4	36152	PASS
177	176	5	9	6.6	2384	PASS

Average of 12.824 to 12.835 min.: VN087988.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	550	48.95	2204	60.90	2146	68.95	532
37.00	3180	50.00	9594	61.10	688	69.90	359
38.00	2960	51.05	3410	61.95	3168	70.10	11
39.00	1297	51.70	67	62.95	2659	71.95	62
43.70	169	52.10	54	63.95	435	73.00	2689
44.00	464	53.90	59	64.70	80	74.00	9782
45.00	703	54.90	231	65.05	547	74.95	26688
46.90	289	55.90	769	65.70	76	76.00	2369
47.10	139	57.00	1398	66.90	303	76.90	376
47.55	246	59.70	144	67.10	125	78.00	101
48.00	424	60.05	560	68.00	5257	78.85	2610

Average of 12.824 to 12.835 min.: VN087988.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.80	613	91.95	1239	114.80	193	130.80	138
80.00	125	92.90	2733	115.60	62	134.70	54
80.85	2396	93.95	6083	115.95	156	136.80	166
81.90	470	95.00	49744	116.50	101	140.20	52
82.80	139	95.95	3801	116.85	457	140.85	754
86.00	209	96.80	58	118.60	142	141.85	126
86.90	2380	103.75	386	118.95	438	142.85	849
87.90	2243	104.95	114	123.90	82	143.85	124
90.75	243	105.85	406	127.75	256	144.80	385
91.00	114	110.80	55	128.70	79	145.80	100
91.80	529	111.80	157	129.80	408	147.60	66

Average of 12.824 to 12.835 min.: VN087988.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
155.10	77	178.00	102				
156.70	67	206.85	168				
158.80	69						
170.65	134						
171.10	57						
171.95	789						
172.80	652						
173.90	37115						
174.90	2682						
175.90	36152						
176.90	2384						

Instrument :

MSVOA_N

ClientSampleId :

BFB