

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN100118\
 Data File : VN051635.D
 Acq On : 1 Oct 2018 14:04
 Operator : MD\SY
 Sample : J5166-01
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 11 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 001-WILLETS-PT-BLVD(AUG)

Quant Time: Oct 02 01:35:26 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA N\METHODS\624N092818W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Sat Sep 29 01:07:29 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	7.20	128	90228	30.00	ug/l	0.00
28) 1,4-Difluorobenzene	8.59	114	450424	30.00	ug/l	0.00
57) Chlorobenzene-d5	11.41	117	402812	30.00	ug/l	0.00

System Monitoring Compounds

27) 1,2-Dichloroethane-d4	8.03	65	193384	30.78	ug/l	0.00
Spiked Amount	30.000	Range	50 - 169	Recovery	=	102.60%
60) 4-Bromofluorobenzene	12.40	95	149439	24.13	ug/l	0.00
Spiked Amount	30.000	Range	56 - 143	Recovery	=	80.43%
63) Toluene-d8	10.09	98	528141	27.79	ug/l	0.00
Spiked Amount	30.000	Range	66 - 137	Recovery	=	92.63%

Target Compounds


					Ovalue
15) Acetone	3.82	58	926206	1834.500	ug/l 94
30) 2-Butanone	6.85	43	38236	18.291	ug/l # 91
58) 4-Methyl-2-Pentanone	9.99	43	14955	3.270	ug/l 99
62) Toluene	10.16	91	8234265	333.381	ug/l 99
66) Ethyl Benzene	11.51	91	9639	0.381	ug/l 93
82) p-Isopropyltoluene	13.29	119	165580	7.809	ug/l 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN100118\
Data File : VN051635.D
Acq On : 1 Oct 2018 14:04
Operator : MD\SY
Sample : J5166-01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 11 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
001-WILLETS-PT-BLVD(AUG)

Quant Time: Oct 02 01:35:26 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA N\METHODS\624N092818W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Sat Sep 29 01:07:29 2018
Response via : Initial Calibration

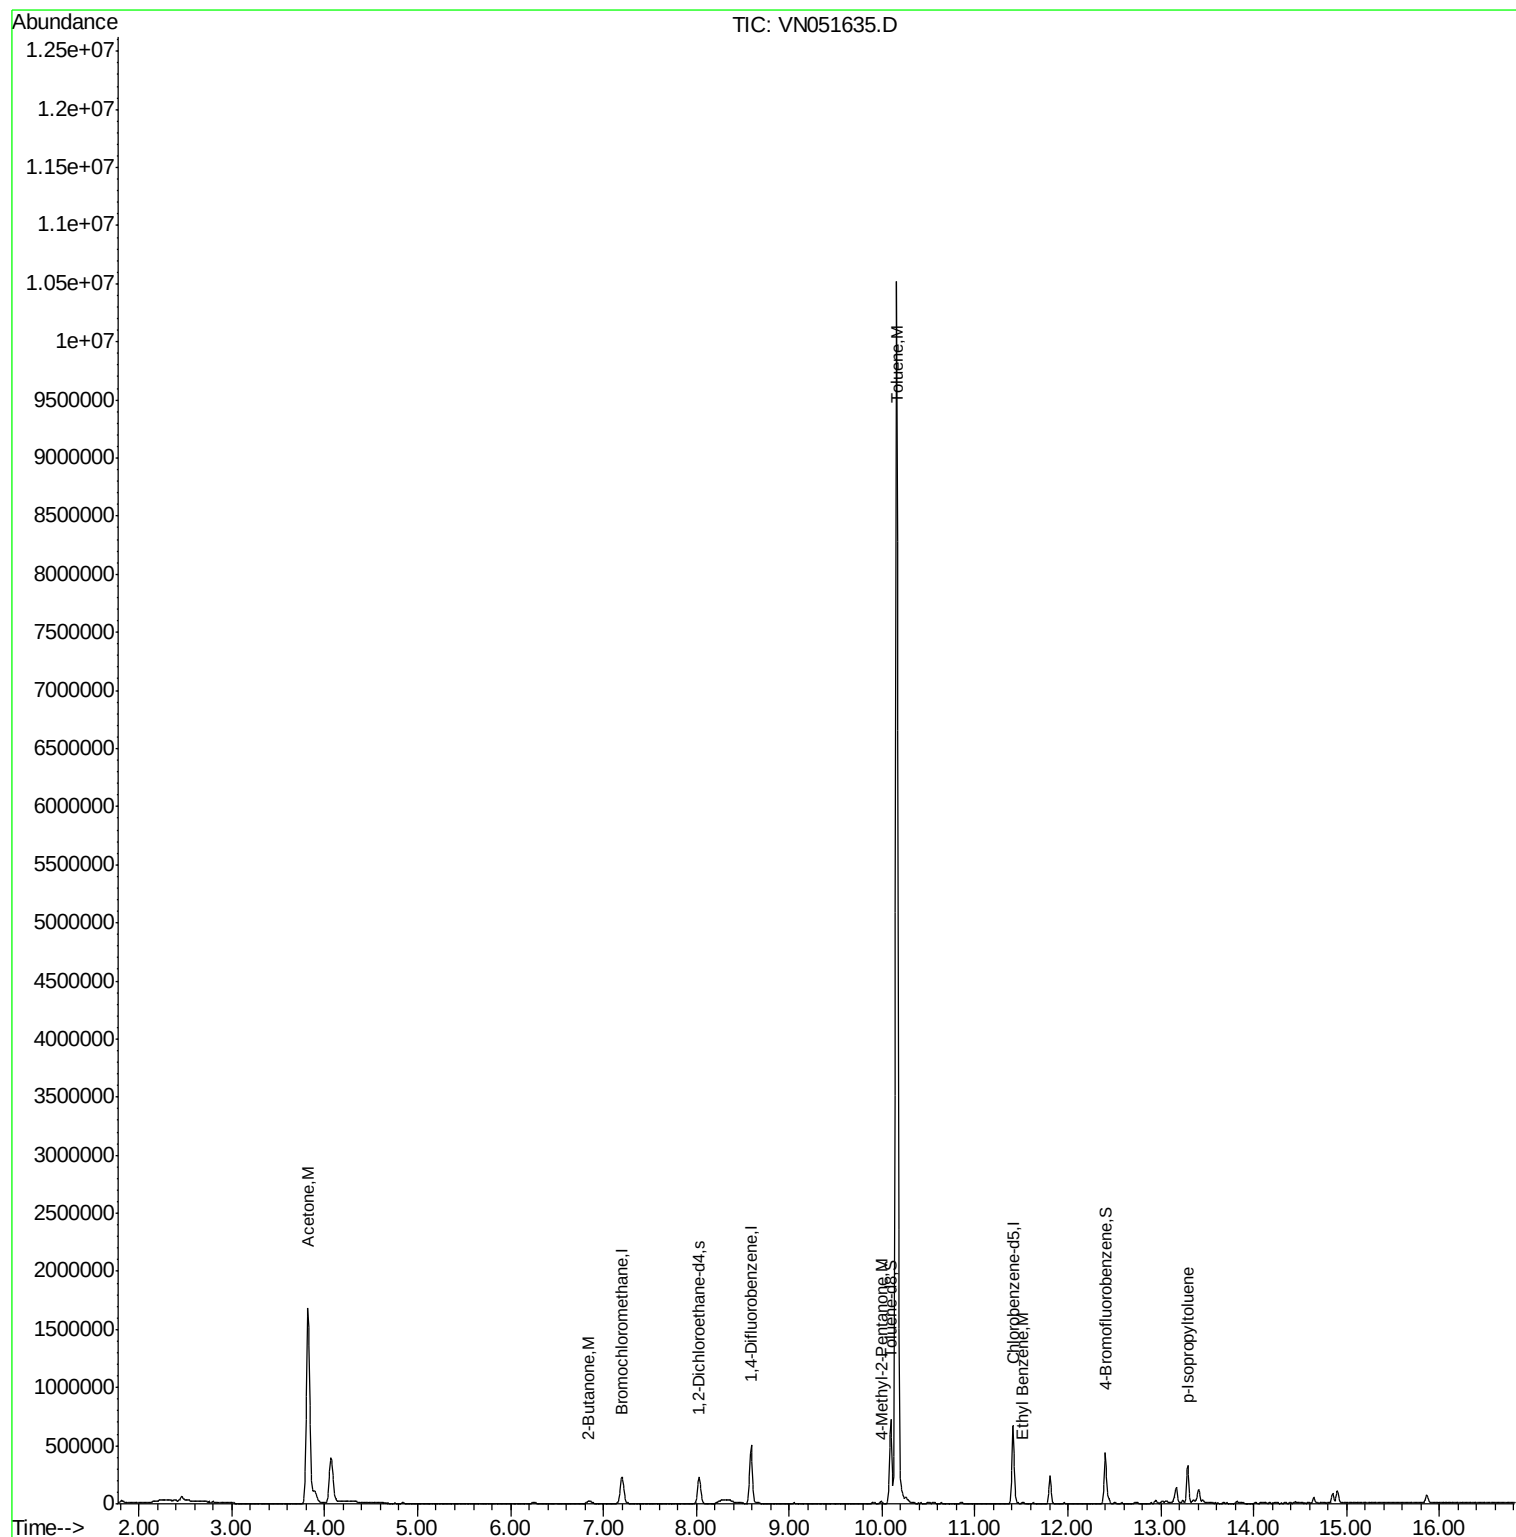


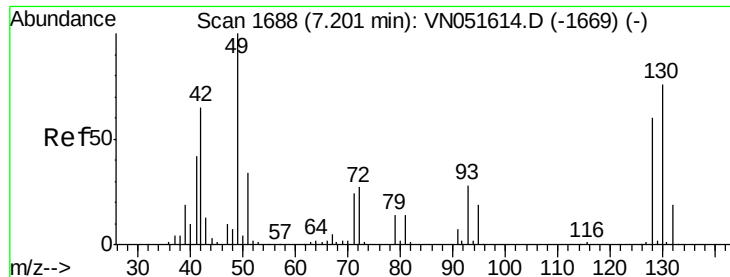




#1
 Bromochloromethane
 Concen: 30.000 ug/l
 RT: 7.20 min Scan# 1688
 Delta R.T. -0.00 min
 Lab File: VN051635.D
 Acq: 1 Oct 2018 14:04

Instrument :
 MSVOA_N
 ClientSampleId :
 001-WILLETS-PT-BLVD(AUG)

Tot Ion:128 Resp: 90228
 Ion Ratio Lower Upper
 128 100
 49 170.2 0.0 426.8
 130 131.0 0.0 326.3

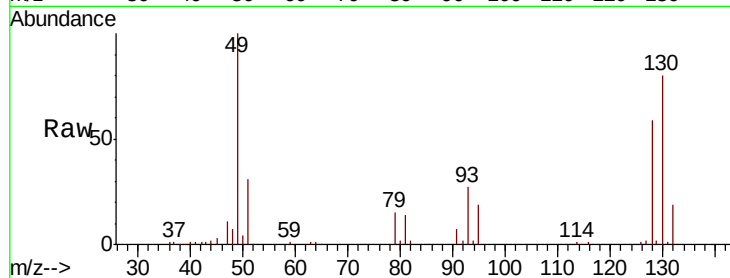


Abundance Ion 128.00 (127.70 to 128.70): V
 Ion 49.00 (48.70 to 49.70): VN
 Ion 130.00 (129.70 to 130.70): V

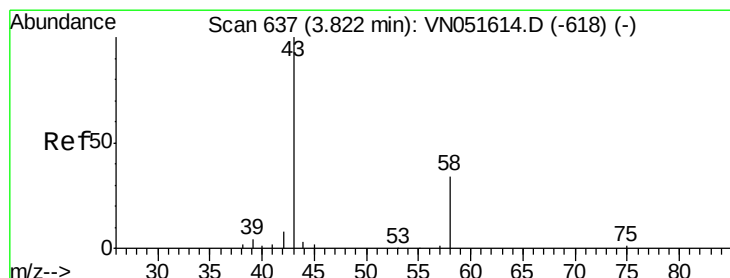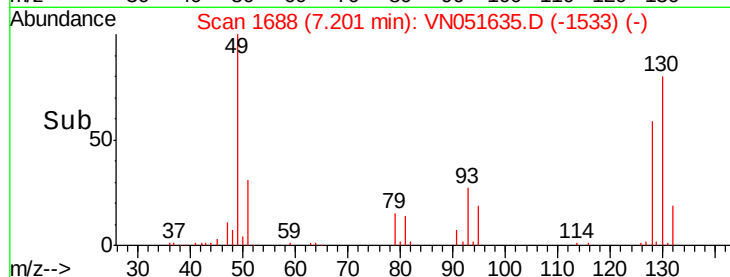
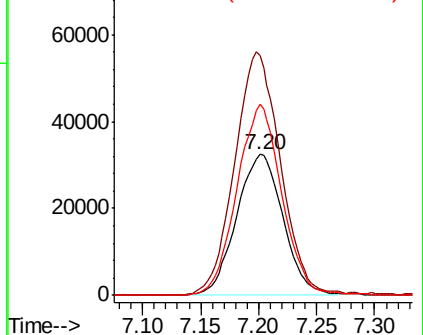



#15
 Acetone
 Concen: 1834.500 ug/l
 RT: 3.82 min Scan# 636
 Delta R.T. -0.00 min
 Lab File: VN051635.D
 Acq: 1 Oct 2018 14:04

Tgt Ion: 58 Resp: 926206
 Ion Ratio Lower Upper
 58 100
 43 308.9 238.0 357.0

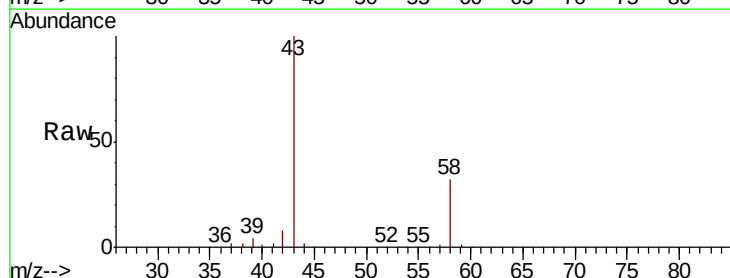

Abundance Ion 58.00 (57.70 to 58.70): VN
 Ion 43.00 (42.70 to 43.70): VN



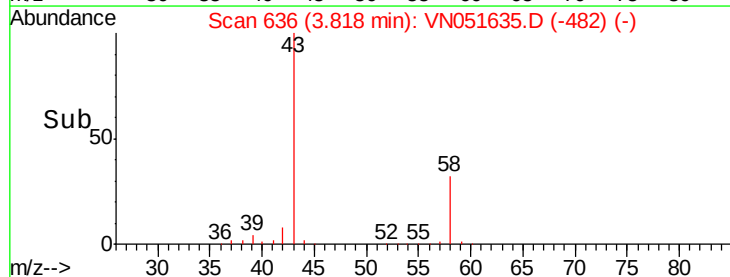
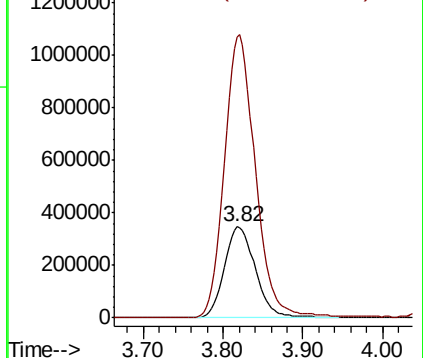


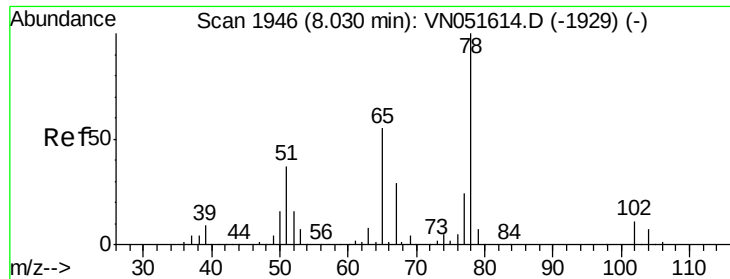

#27
 1,2-Dichloroethane-d4
 Concen: Below ug/l
 RT: 8.03 min Scan# 1945
 Delta R.T. -0.00 min
 Lab File: VN051635.D
 Acq: 1 Oct 2018 14:04




Instrument :
 MSVOA_N
 ClientSampleId :
 001-WILLETS-PT-BLVD(AUG)


Tot Ion: 65 Resp: 193384
 Ion Ratio Lower Upper
 65 100
 67 54.5 43.1 64.7

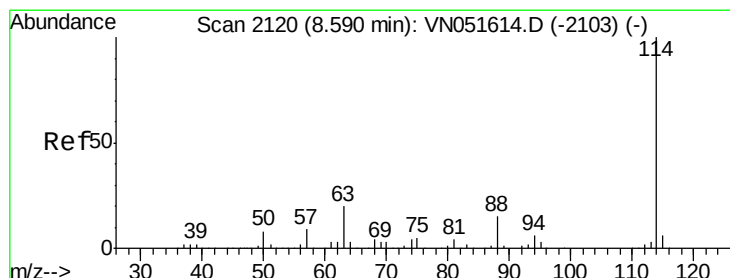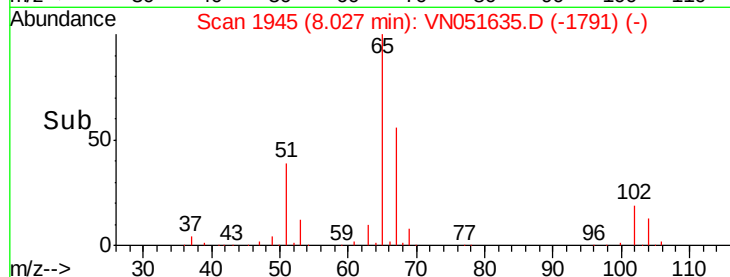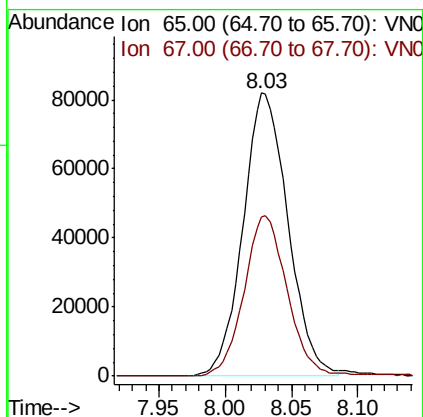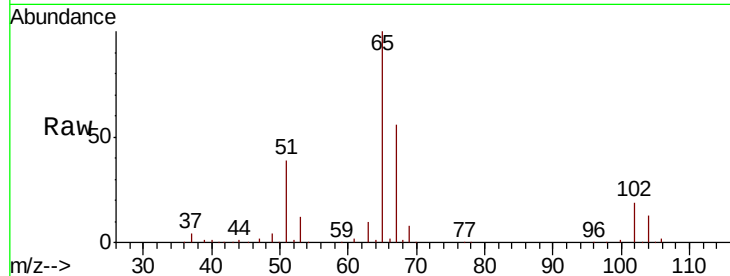

#28
 1,4-Difluorobenzene
 Concen: 30.000 ug/l
 RT: 8.59 min Scan# 2120
 Delta R.T. -0.00 min
 Lab File: VN051635.D
 Acq: 1 Oct 2018 14:04

Tgt Ion: 114 Resp: 450424
 Ion Ratio Lower Upper
 114 100
 63 20.4 16.4 24.6
 88 15.6 12.6 18.8


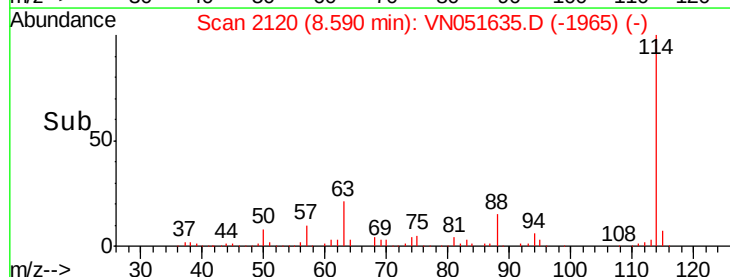
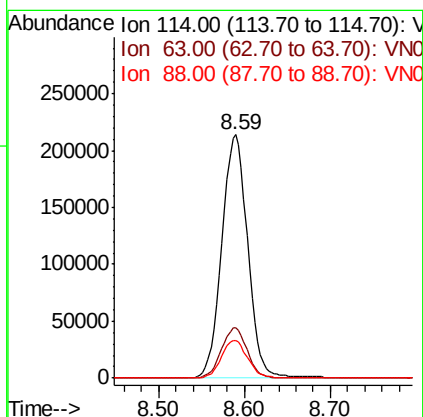
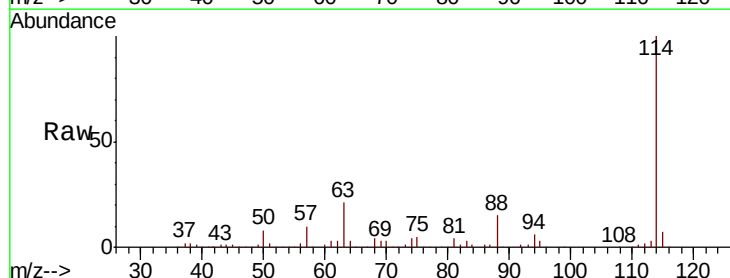


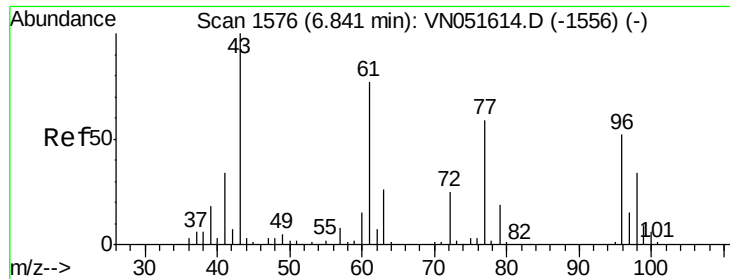

#30
2-Butanone
Concen: 18.291 ug/l
RT: 6.85 min Scan# 1579
Delta R.T. 0.01 min
Lab File: VN051635.D
Acq: 1 Oct 2018 14:04




Instrument :
MSVOA_N
ClientSampleId :
001-WILLETS-PT-BLVD(AUG)


Tot Ion: 43 Resp: 38236
Ion Ratio Lower Upper
43 100
57 2.4 6.6 10.0#
72 22.3 20.8 31.2

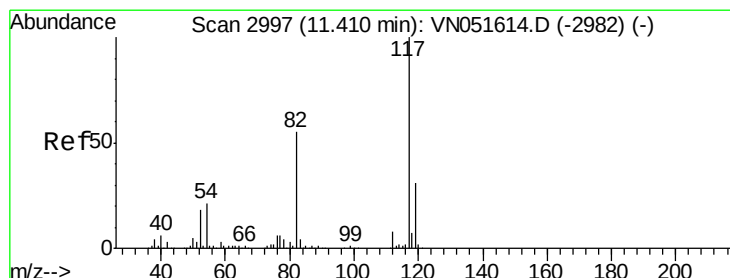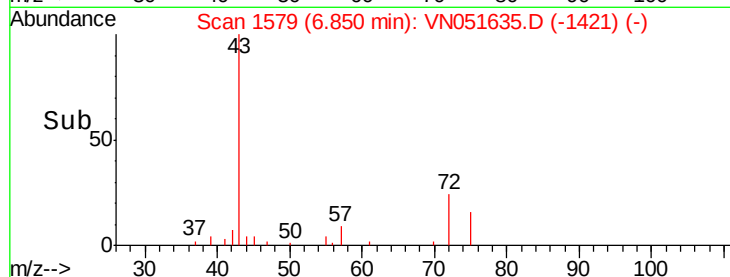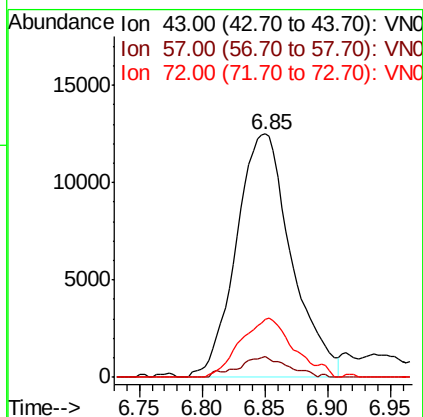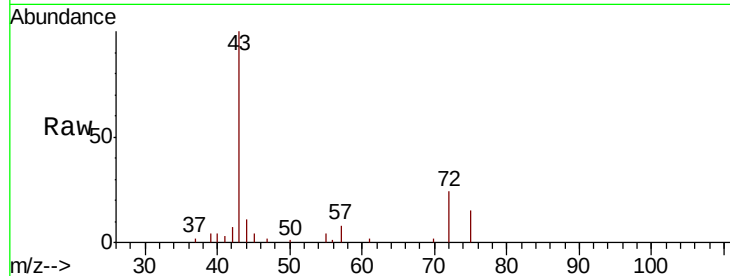

#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 11.41 min Scan# 2997
Delta R.T. -0.00 min
Lab File: VN051635.D
Acq: 1 Oct 2018 14:04

Tgt Ion:117 Resp: 402812
Ion Ratio Lower Upper
117 100
82 54.6 44.2 66.2
119 32.0 25.2 37.8


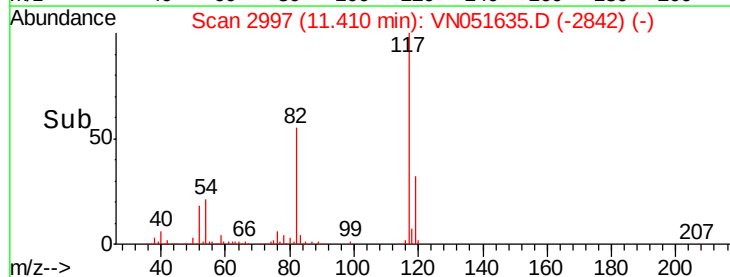
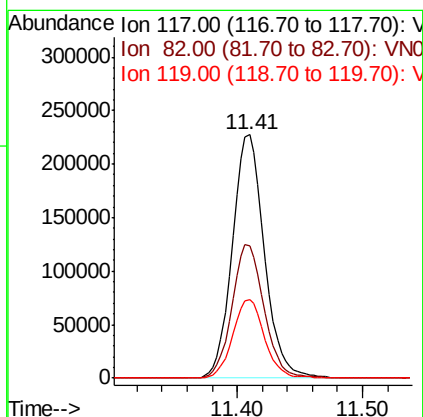
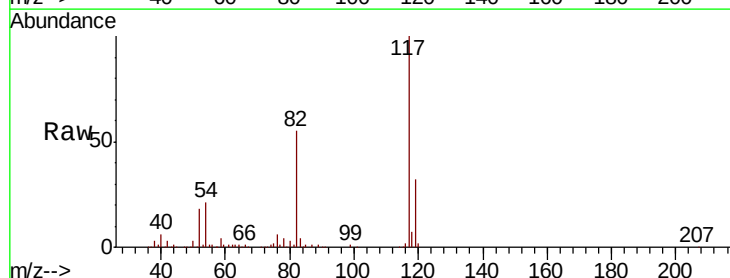


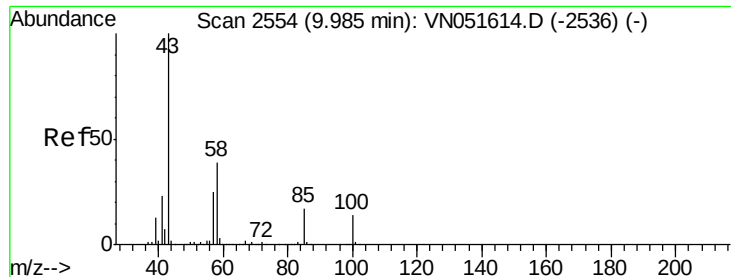

#58
4-Methyl-2-Pentanone
Concen: 3.270 ug/l
RT: 9.99 min Scan# 2554
Delta R.T. -0.00 min
Lab File: VN051635.D
Acq: 1 Oct 2018 14:04




Instrument :
MSVOA_N
ClientSampleId :
001-WILLETS-PT-BLVD(AUG)


Tot Ion: 43 Resp: 14955
Ion Ratio Lower Upper
43 100
58 38.1 31.0 46.4
85 15.8 13.4 20.2

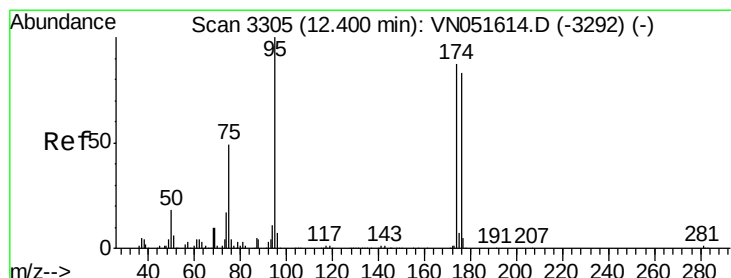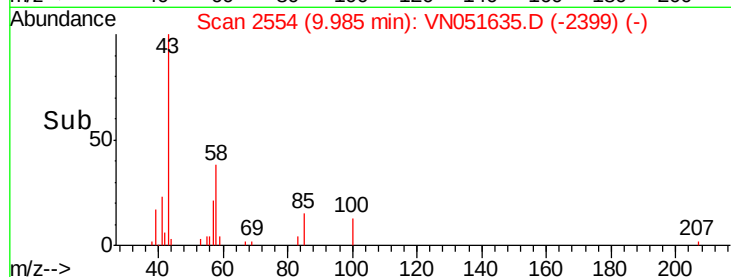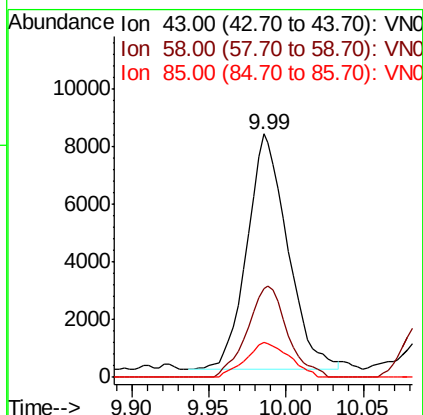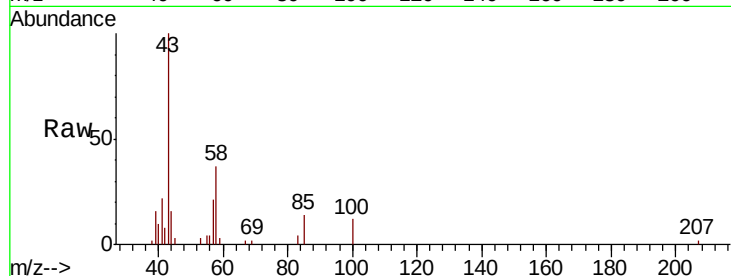

#60
4-Bromofluorobenzene
Concen: N.D. ug/l
RT: 12.40 min Scan# 3306
Delta R.T. 0.00 min
Lab File: VN051635.D
Acq: 1 Oct 2018 14:04

Tgt Ion: 95 Resp: 149439
Ion Ratio Lower Upper
95 100
174 88.5 71.2 106.8
176 87.0 67.8 101.8

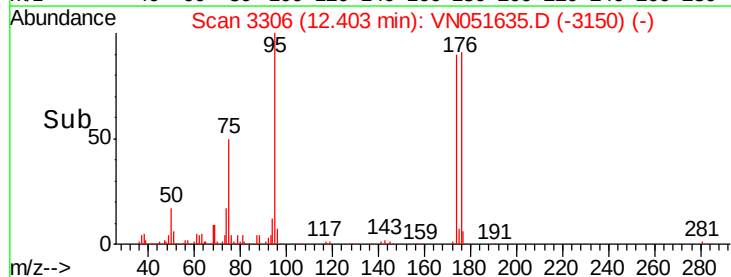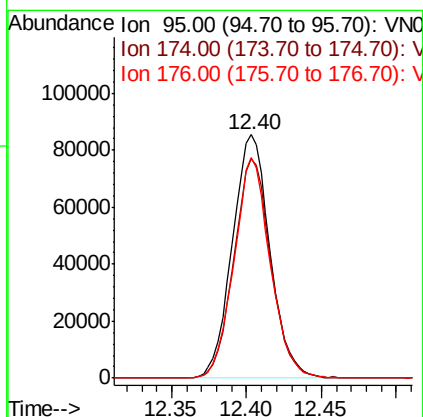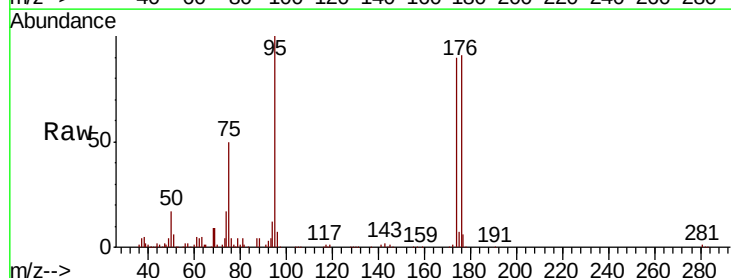

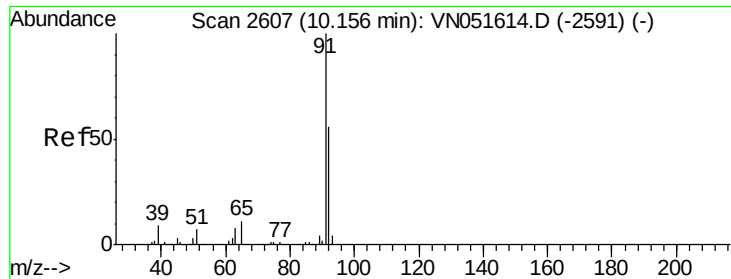

#62

Toluene

Concen: 333.381 ug/l

RT: 10.16 min Scan# 2607

Delta R.T. -0.00 min

Lab File: VN051635.D

Acq: 1 Oct 2018 14:04

Instrument :

MSVOA_N

ClientSampleId :





001-WILLETS-PT-BLVD(AUG)

Tot Ion: 91 Resp: 8234265

Ion Ratio Lower Upper

91 100

92 57.0 45.3 67.9

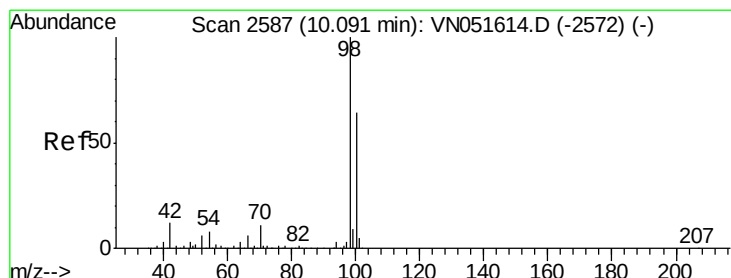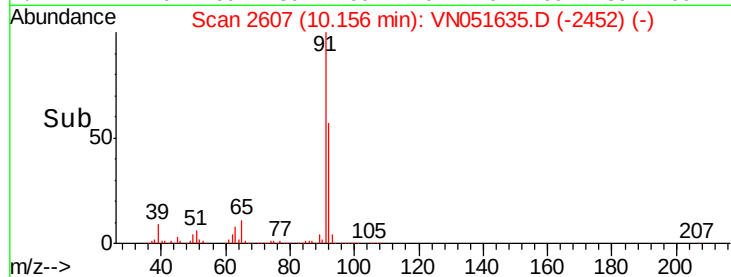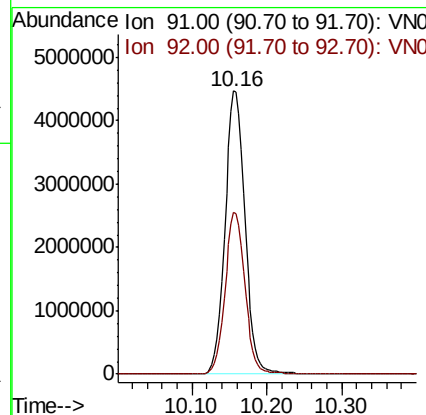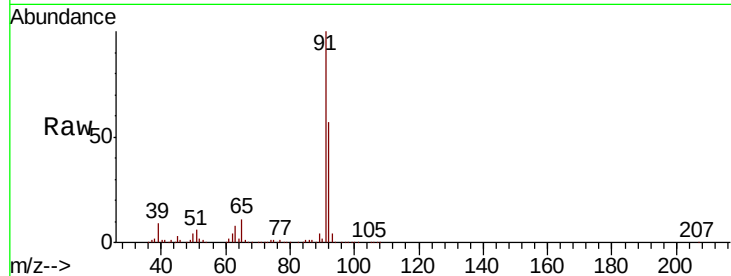

#63

Toluene-d8

Concen: 333.381 ug/l

RT: 10.09 min Scan# 2587

Delta R.T. -0.00 min

Lab File: VN051635.D




Acq: 1 Oct 2018 14:04


Tgt Ion: 98 Resp: 528141

Ion Ratio Lower Upper

98 100

100 60.9 51.4 77.0

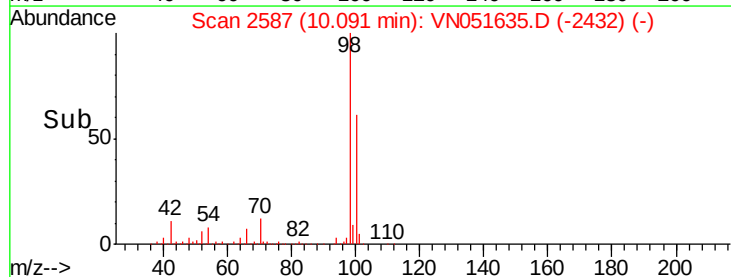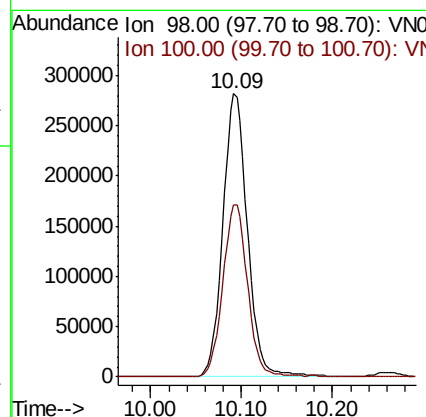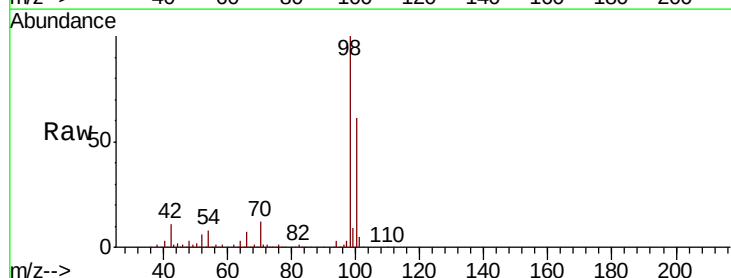

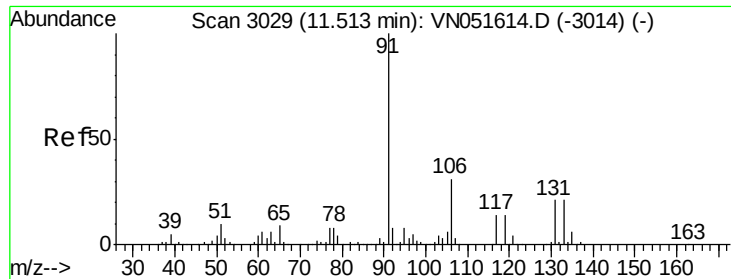

#66

Ethyl Benzene

Concen: 0.381 ug/l

RT: 11.51 min Scan# 3029

Delta R.T. -0.00 min

Lab File: VN051635.D

Acq: 1 Oct 2018 14:04

Instrument :

MSVOA_N

ClientSampleId :


001-WILLETS-PT-BLVD(AUG)

Tot Ion: 91 Resp: 9639

Ion Ratio Lower Upper

91 100

106 27.1 25.0 37.4

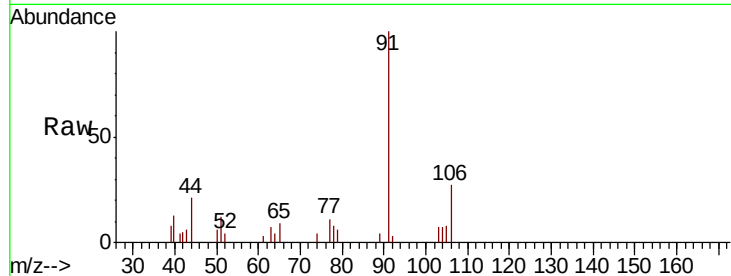

Abundance Ion 91.00 (90.70 to 91.70): VN051614.D (-3014) (-)

Ion 106.00 (105.70 to 106.70): VN051614.D (-3014) (-)

11.51

6000

5000

4000

3000



2000

1000

0

11.45 11.50 11.55

Time-->

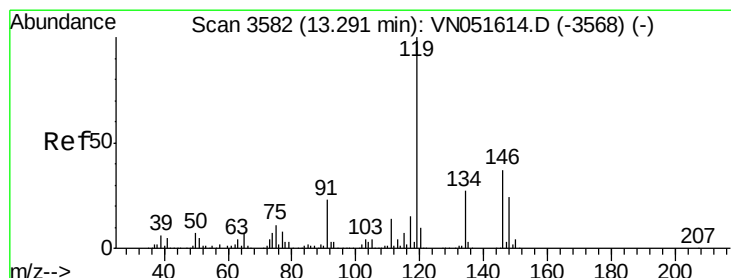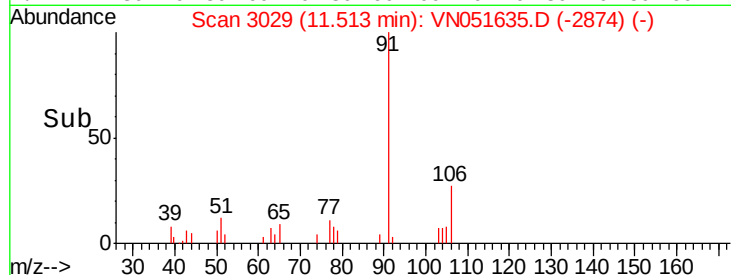

#82

p-Isopropyltoluene

Concen: 7.809 ug/l

RT: 13.29 min Scan# 3582

Delta R.T. -0.00 min

Lab File: VN051635.D

Acq: 1 Oct 2018 14:04


Tgt Ion: 119 Resp: 165580

Ion Ratio Lower Upper

119 100

134 25.9 0.0 52.0

91 25.2 0.0 46.0

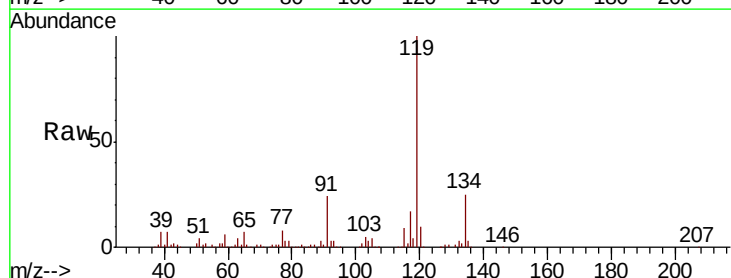

Abundance Ion 119.00 (118.70 to 119.70): VN051614.D (-3568) (-)

Ion 134.00 (133.70 to 134.70): VN051614.D (-3568) (-)

Ion 91.00 (90.70 to 91.70): VN051614.D (-3568) (-)

13.29

150000

100000

50000

0

13.25 13.30 13.35

Time-->

