


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN100118\
Data File : VN051625.D
Acq On : 1 Oct 2018 9:48
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N092818W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Sat Sep 29 01:07:29 2018

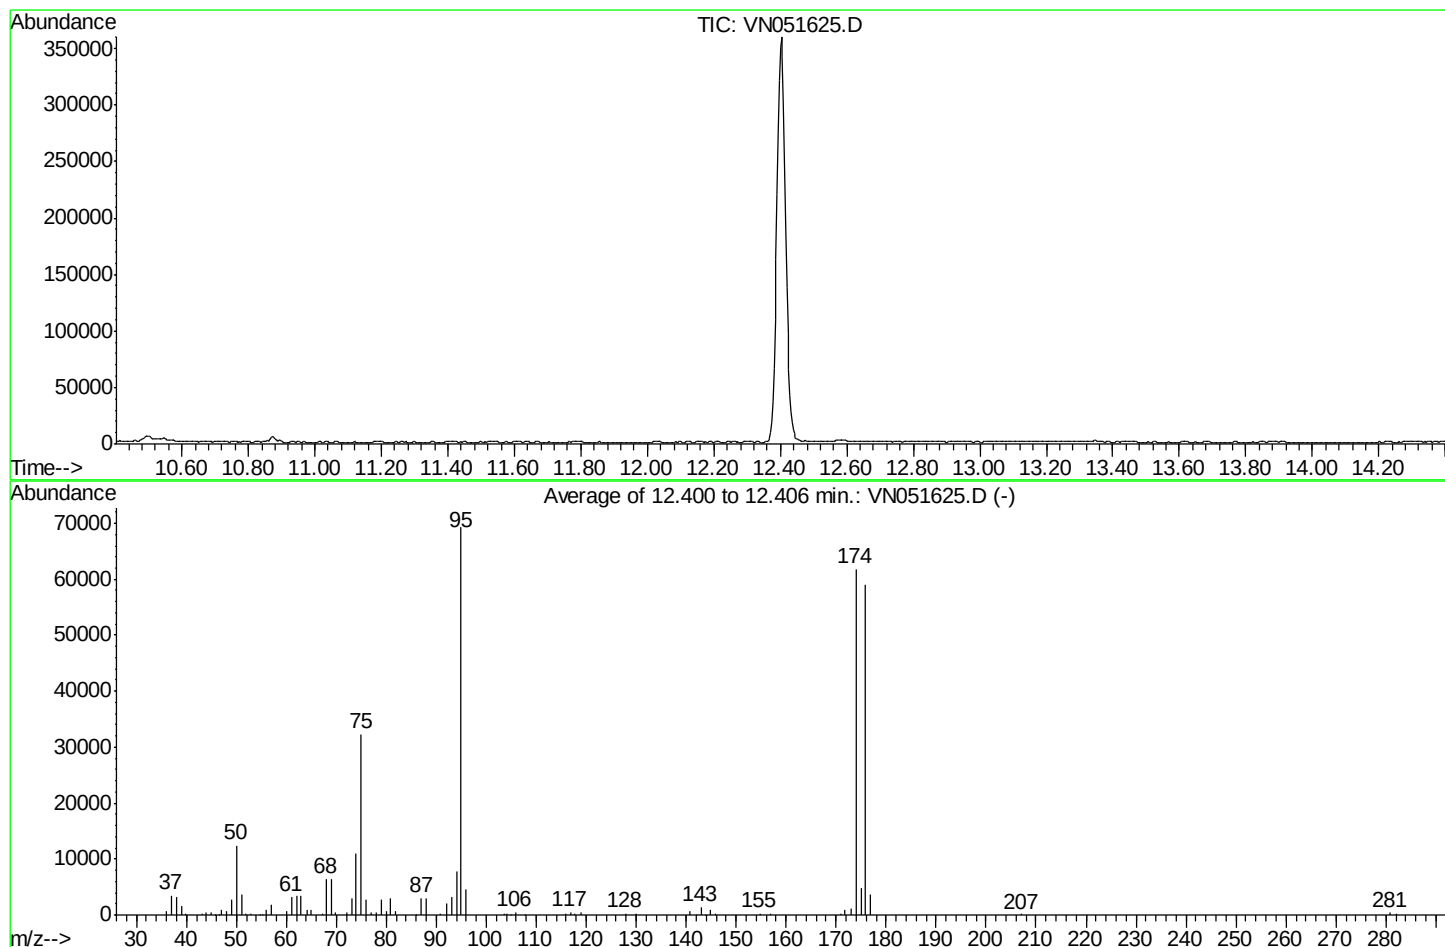

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	12416	PASS
75	95	30	60	46.7	32349	PASS
95	95	100	100	100.0	69285	PASS
96	95	5	9	6.7	4624	PASS
173	174	0.00	2	1.8	1099	PASS
174	95	50	100	89.2	61818	PASS
175	174	5	9	7.7	4762	PASS
176	174	95	101	95.4	59005	PASS
177	176	5	9	6.1	3600	PASS