

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN100120\
 Data File : VN063805.D
 Acq On : 2 Oct 2020 5:44
 Operator : JC/MD
 Sample : L4236-02
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-2

Quant Time: Oct 02 06:41:58 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 01 01:46:38 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	206884	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	387356	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	388027	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	163315	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	182312	53.34	ug/l	0.00
Spiked Amount			Recovery	=	106.68%	
35) Dibromofluoromethane	7.55	113	132278	49.21	ug/l	0.00
Spiked Amount			Recovery	=	98.42%	
50) Toluene-d8	10.06	98	490704	48.16	ug/l	0.00
Spiked Amount			Recovery	=	96.32%	
62) 4-Bromofluorobenzene	12.38	95	188492	49.21	ug/l	0.00
Spiked Amount			Recovery	=	98.42%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	2.04	50	666	0.260	ug/l #	42
4) Vinyl Chloride	2.16	62	19639	7.638	ug/l	99
6) Chloroethane	2.67	64	1144	0.745	ug/l	90
12) 1,1-Dichloroethene	3.70	96	137493	65.998	ug/l	97
16) Acetone	3.79	43	3443	3.272	ug/l #	87
17) Carbon Disulfide	4.02	76	467	0.782	ug/l #	76
24) 1,1-Dichloroethane	5.79	63	87215	19.155	ug/l	98
27) cis-1,2-Dichloroethene	6.78	96	30470	11.354	ug/l	91
31) Cyclohexane	7.62	56	6803	1.714	ug/l #	38
36) 1,1-Dichloropropene	7.63	75	19247	4.905	ug/l #	50
38) Carbon Tetrachloride	7.62	117	23725	5.391	ug/l #	15
39) Methylcyclohexane	9.05	83	872	0.223	ug/l #	76
40) Benzene	8.01	78	7042	0.628	ug/l #	86
42) 1,2-Dichloroethane	8.09	62	14475	3.025	ug/l	98
43) Isopropyl Acetate	8.10	43	18231	2.835	ug/l #	76
44) Trichloroethene	8.81	130	2564	0.873	ug/l	96
48) Methyl methacrylate	9.16	41	997	0.314	ug/l #	18
49) 1,4-Dioxane	9.17	88	27788	615.371	ug/l	97
71) Bromoform	12.37	173	777	0.333	ug/l #	1
74) N-amyl acetate	12.06	43	82	2.230	ug/l #	1
76) 1,2,3-Trichloropropane	12.38	75	111147	30.873	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.38	75	111147	88.920	ug/l #	10
86) p-Isopropyltoluene	13.42	119	1991	0.210	ug/l	87
90) Hexachloroethane	13.97	117	828	0.450	ug/l #	14


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN100120\
Data File : VN063805.D
Acq On : 2 Oct 2020 5:44
Operator : JC/MD
Sample : L4236-02
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-2

Quant Time: Oct 02 06:41:58 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 01 01:46:38 2020
Response via : Initial Calibration

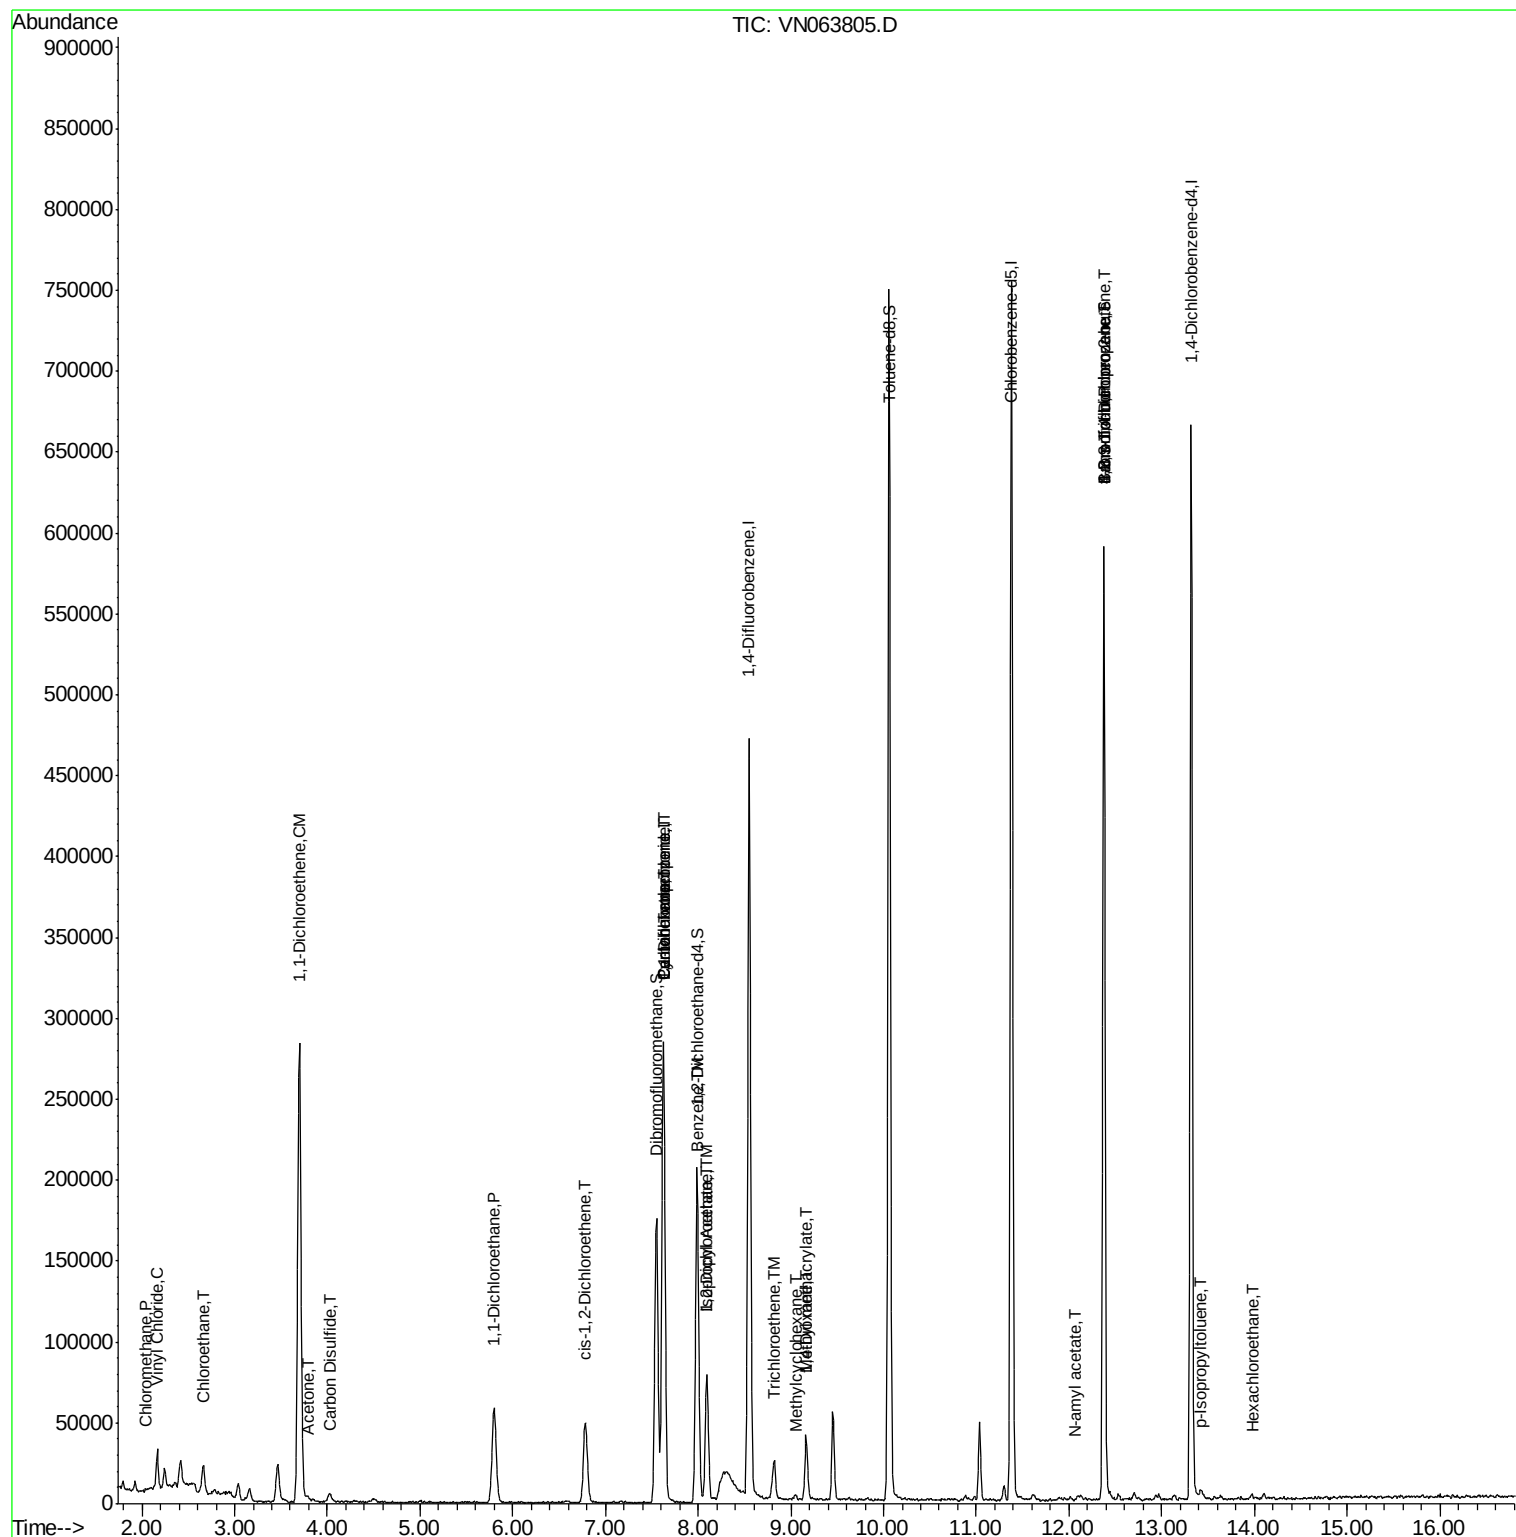

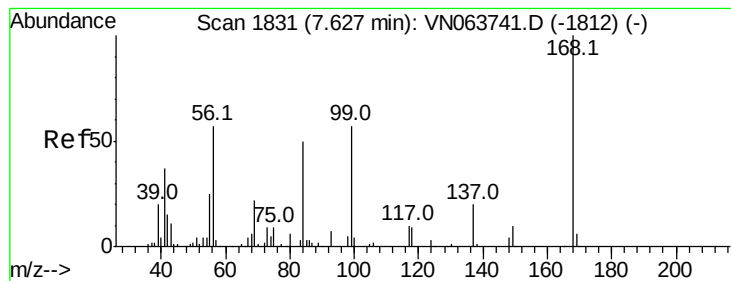

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN063805.D

Acq: 2 Oct 2020 5:44

Instrument :

MSVOA_N

ClientSampleId :


MW-2

Tot Ion:168 Resp: 206884

Ion Ratio Lower Upper




168 100

99 63.9 51.8 77.6



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

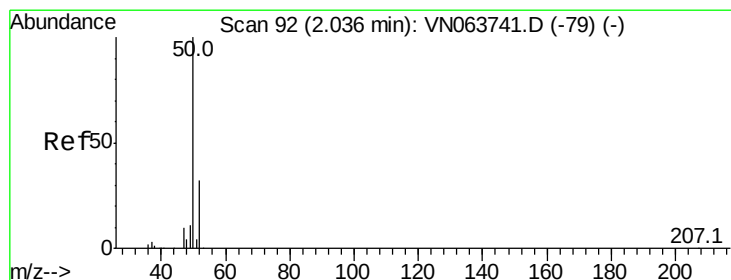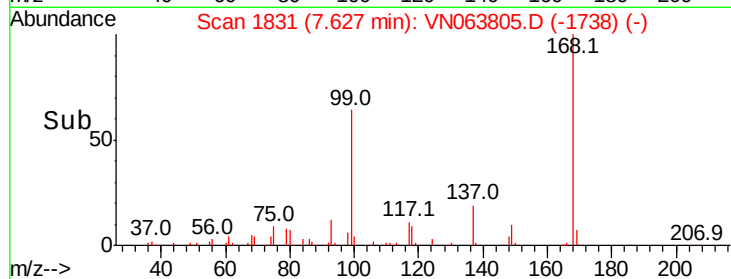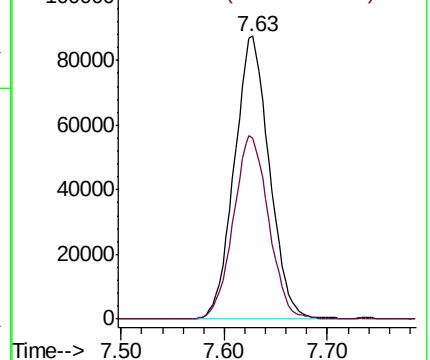

#3

Chloromethane

Concen: 0.260 ug/l

RT: 2.04 min Scan# 92

Delta R.T. 0.00 min

Lab File: VN063805.D


Acq: 2 Oct 2020 5:44

Tgt Ion: 50 Resp: 666

Ion Ratio Lower Upper



50 100


52 0.0 25.8 38.8#

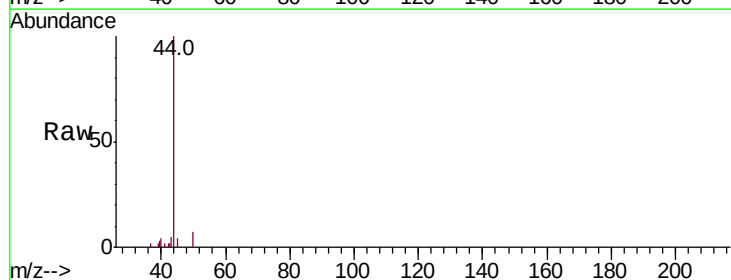

Abundance Ion 49.90 (49.60 to 50.60): VN

Ion 51.90 (51.60 to 52.60): VN

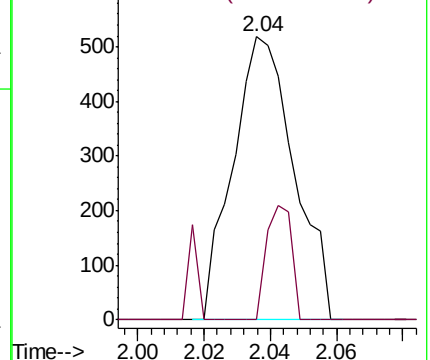

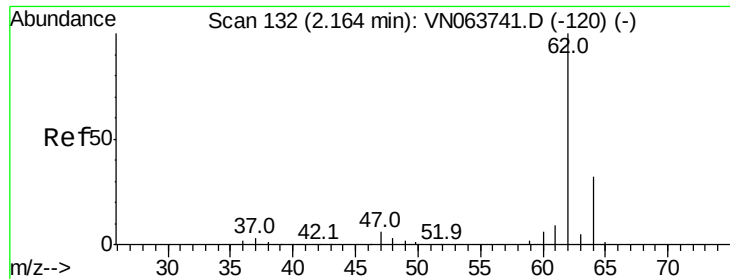

#4

Vinyl Chloride

Concen: 7.638 ug/l

RT: 2.16 min Scan# 132

Delta R.T. 0.00 min

Lab File: VN063805.D

Acq: 2 Oct 2020 5:44

Instrument :

MSVOA_N

ClientSampled :


MW-2

Tot Ion: 62 Resp: 19639

Ion Ratio Lower Upper

62 100

64 32.7 25.6 38.4

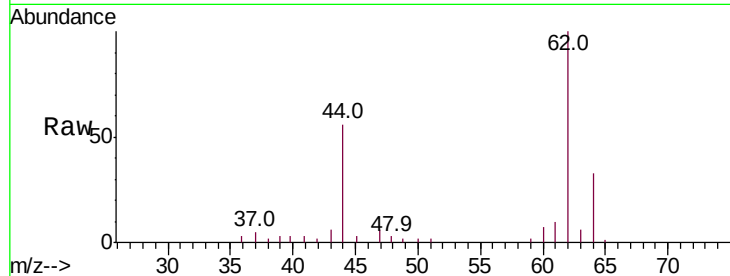

Abundance Ion 61.90 (61.60 to 62.60): VN063805.D (-120) (-)

Ion 63.90 (63.60 to 64.60): VN063805.D (-120) (-)

2.16



15000

10000

5000

0

Time--> 2.10 2.15 2.20

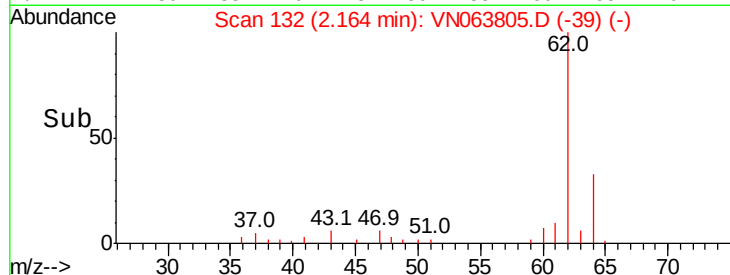

#6

Chloroethane

Concen: 0.745 ug/l

RT: 2.67 min Scan# 289

Delta R.T. -0.00 min

Lab File: VN063805.D


Acq: 2 Oct 2020 5:44

Tgt Ion: 64 Resp: 1144

Ion Ratio Lower Upper

64 100

66 25.6 25.1 37.7



Abundance Ion 63.90 (63.60 to 64.60): VN063805.D (-275) (-)

Ion 65.90 (65.60 to 66.60): VN063805.D (-275) (-)

2.67


600


400

200

0

Time--> 2.62 2.64 2.66 2.68 2.70

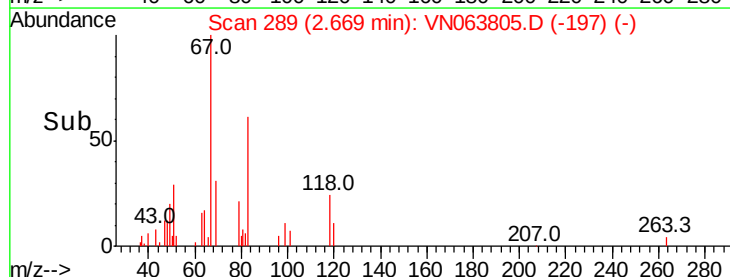


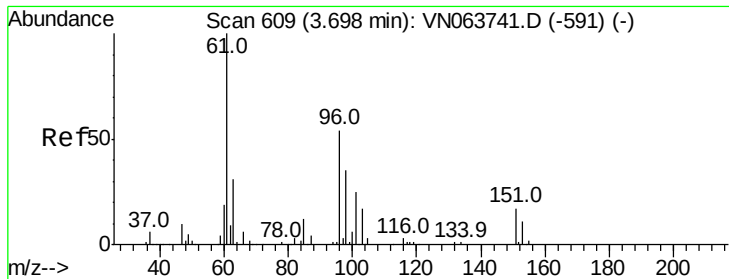




#12
 1,1-Dichloroethene
 Concen: 65.998 ug/l
 RT: 3.70 min Scan# 609
 Delta R.T. 0.00 min
 Lab File: VN063805.D
 Acq: 2 Oct 2020 5:44

Instrument :
 MSVOA_N
 ClientSampled :
 MW-2

Tot Ion: 96 Resp: 137493
 Ion Ratio Lower Upper
 96 100
 61 178.6 147.7 221.5
 98 64.0 51.9 77.9

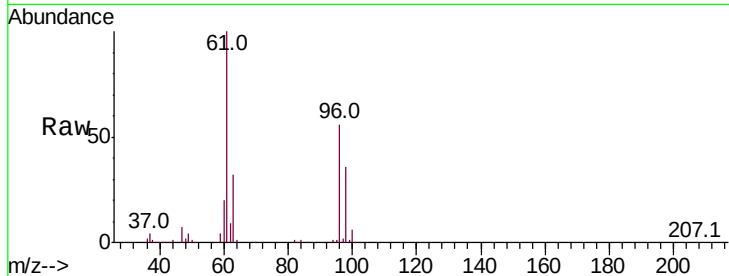


Abundance Ion 95.90 (95.60 to 96.60): VN0
 Ion 60.90 (60.60 to 61.60): VN0
 Ion 97.90 (97.60 to 98.60): VN0

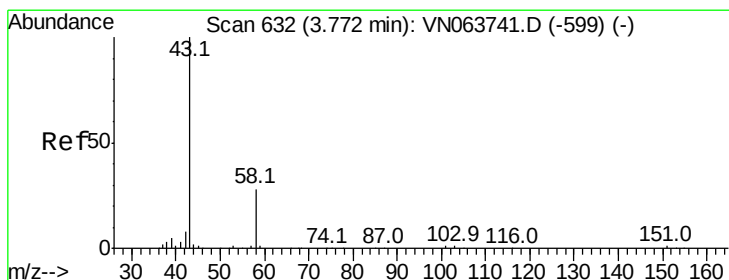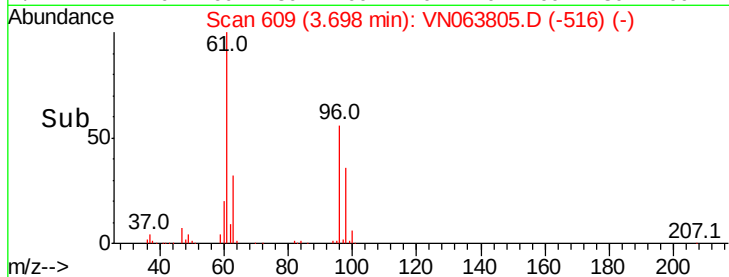
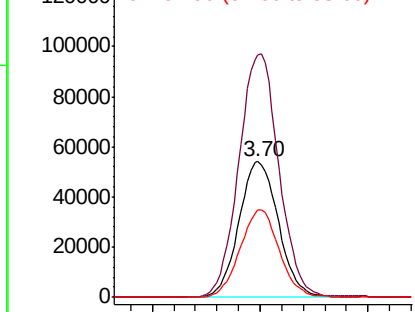



#16
 Acetone
 Concen: 3.272 ug/l
 RT: 3.79 min Scan# 637
 Delta R.T. 0.02 min
 Lab File: VN063805.D
 Acq: 2 Oct 2020 5:44

Tgt Ion: 43 Resp: 3443
 Ion Ratio Lower Upper
 43 100
 58 20.9 22.3 33.5#

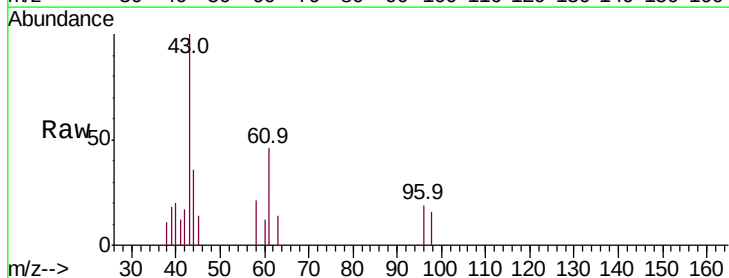

Abundance Ion 43.00 (42.70 to 43.70): VN0
 Ion 58.00 (57.70 to 58.70): VN0

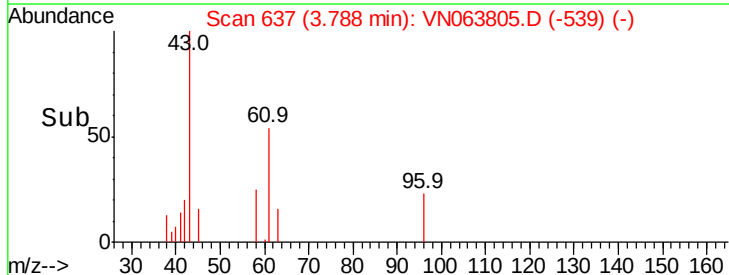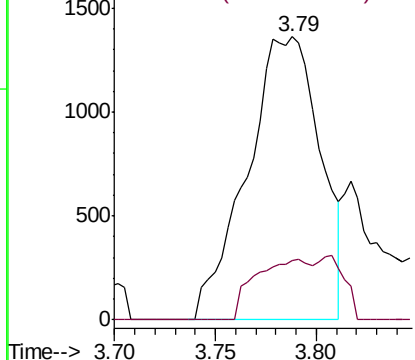



#17

Carbon Disulfide

Concen: 0.782 ug/l

RT: 4.02 min Scan# 708

Delta R.T. 0.00 min

Lab File: VN063805.D

Acq: 2 Oct 2020 5:44

Instrument :

MSVOA_N

ClientSampleId :


MW-2

Tot Ion: 76 Resp: 467

Ion Ratio Lower Upper

76 100

78 0.0 7.0 10.4#





Abundance Ion 75.90 (75.60 to 76.60): VN063741.D (-685) (-)

Ion 77.90 (77.60 to 78.60): VN063741.D (-685) (-)

4.02

4.00 4.02 4.04

Time-->



#24

1,1-Dichloroethane

Concen: 19.155 ug/l

RT: 5.79 min Scan# 1261

Delta R.T. -0.00 min

Lab File: VN063805.D

Acq: 2 Oct 2020 5:44


Tgt Ion: 63 Resp: 87215

Ion Ratio Lower Upper

63 100

98 5.7 2.7 8.1

100 4.6 1.9 5.7



Abundance Ion 62.90 (62.60 to 63.60): VN063741.D (-1237) (-)


Ion 97.90 (97.60 to 98.60): VN063741.D (-1237) (-)


Ion 99.90 (99.60 to 100.60): VN063741.D (-1237) (-)

5.79

5.70 5.79 5.88

Time-->




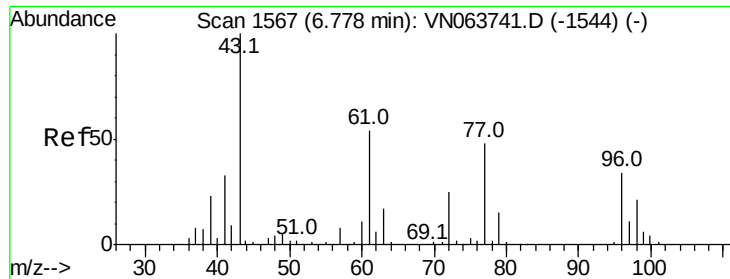




#27
 cis-1,2-Dichloroethene
 Concen: 11.354 ug/l
 RT: 6.78 min Scan# 1568
 Delta R.T. 0.00 min
 Lab File: VN063805.D
 Acq: 2 Oct 2020 5:44

Instrument :
 MSVOA_N
 ClientSampled :
 MW-2

Tot Ion: 96 Resp: 30470
 Ion Ratio Lower Upper
 96 100
 61 145.0 0.0 321.2
 98 62.5 0.0 124.4

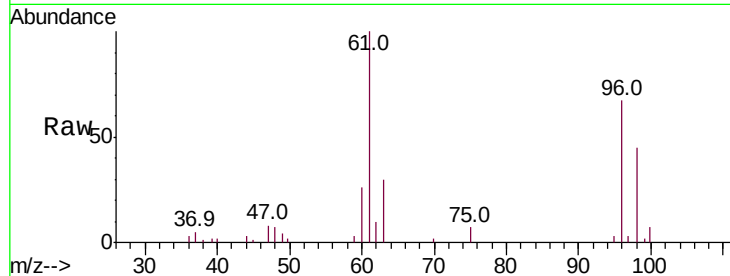


Abundance Ion 95.90 (95.60 to 96.60): VN0
 Ion 60.90 (60.60 to 61.60): VN0
 Ion 97.90 (97.60 to 98.60): VN0

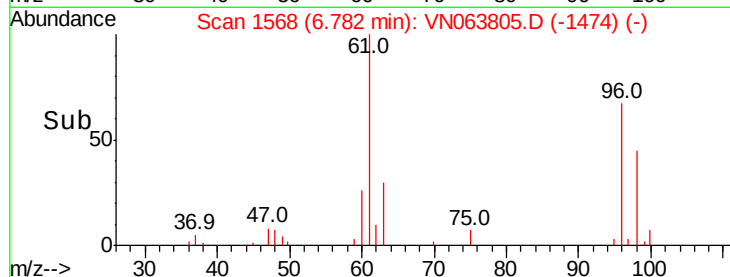
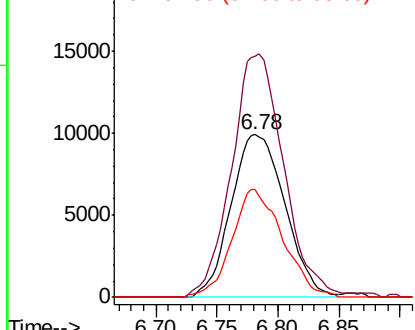



#31
 Cyclohexane
 Concen: 1.714 ug/l
 RT: 7.62 min Scan# 1829
 Delta R.T. 0.01 min
 Lab File: VN063805.D
 Acq: 2 Oct 2020 5:44

Tgt Ion: 56 Resp: 6803
 Ion Ratio Lower Upper
 56 100
 69 127.9 25.4 38.2#
 84 94.0 63.3 94.9



Abundance Ion 56.00 (55.70 to 56.70): VN0
 Ion 69.00 (68.70 to 69.70): VN0
 Ion 84.00 (83.70 to 84.70): VN0

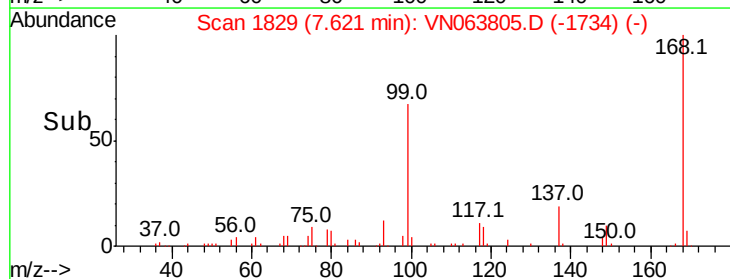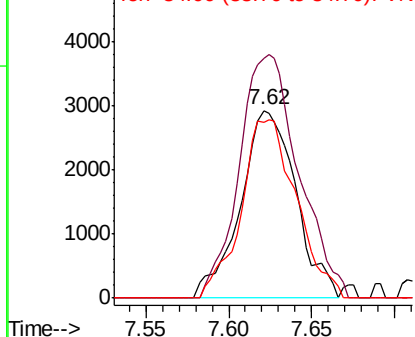

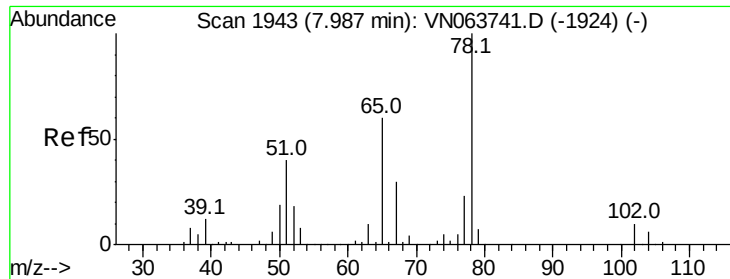

#33

1,2-Dichloroethane-d4

Concen: 53.341 ug/l

RT: 7.99 min Scan# 1943

Delta R.T. 0.00 min

Lab File: VN063805.D

Acq: 2 Oct 2020 5:44

Instrument :

MSVOA_N

ClientSampled :


MW-2

Tot Ion: 65 Resp: 182312

Ion Ratio Lower Upper

65 100

67 49.7 0.0 99.6

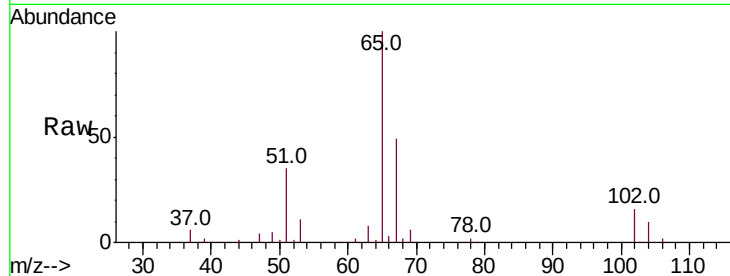

Abundance Ion 64.90 (64.60 to 65.60): VN063741.D (-1924) (-)

Ion 66.90 (66.60 to 67.60): VN063741.D (-1924) (-)

7.99

80000

60000

40000

20000



0

7.90

8.00

8.10

Time-->

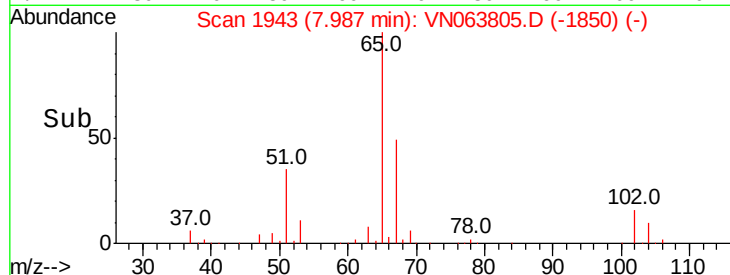

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.55 min Scan# 2118

Delta R.T. 0.00 min

Lab File: VN063805.D

Acq: 2 Oct 2020 5:44


Tgt Ion: 114 Resp: 387356

Ion Ratio Lower Upper

114 100

63 23.0 0.0 45.0

88 16.3 0.0 34.0



Abundance Ion 113.90 (113.60 to 114.60): VN063741.D (-2100) (-)

Ion 63.00 (62.70 to 63.70): VN063741.D (-2100) (-)

Ion 87.90 (87.60 to 88.60): VN063741.D (-2100) (-)

250000

200000

150000

100000

50000


0


8.50

8.60

8.70

Time-->




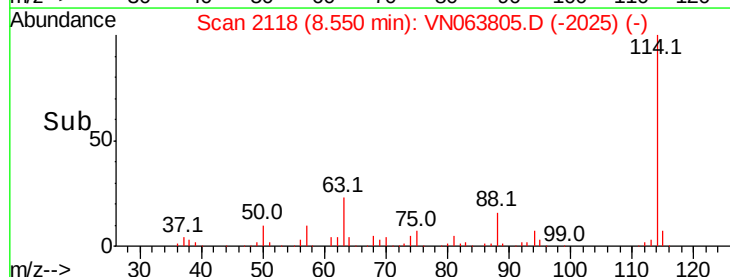




#35
 Dibromofluoromethane
 Concen: 49.215 ug/l
 RT: 7.55 min Scan# 1808
 Delta R.T. 0.00 min
 Lab File: VN063805.D
 Acq: 2 Oct 2020 5:44




Instrument :
 MSVOA_N
 ClientSampleId :
 MW-2


Tot Ion:113 Resp: 132278
 Ion Ratio Lower Upper
 113 100
 111 101.8 81.8 122.8
 192 17.8 14.2 21.2

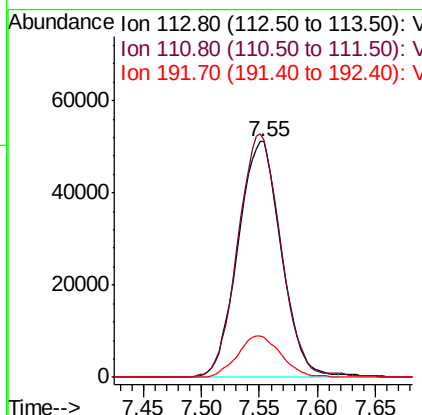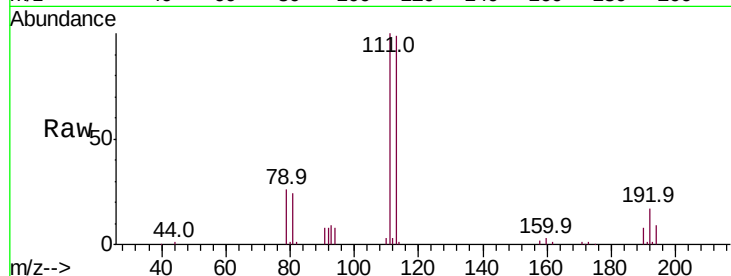

#36
 1,1-Dichloropropene
 Concen: 4.905 ug/l
 RT: 7.63 min Scan# 1832
 Delta R.T. -0.12 min
 Lab File: VN063805.D
 Acq: 2 Oct 2020 5:44

Tgt Ion: 75 Resp: 19247
 Ion Ratio Lower Upper
 75 100
 110 8.3 16.9 50.6#
 77 0.0 24.5 36.7#


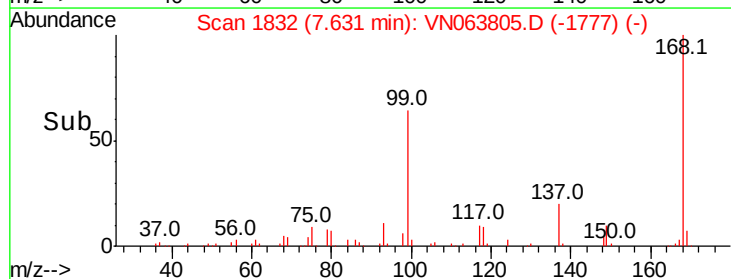
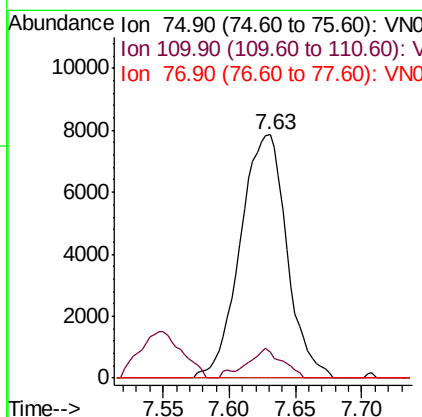



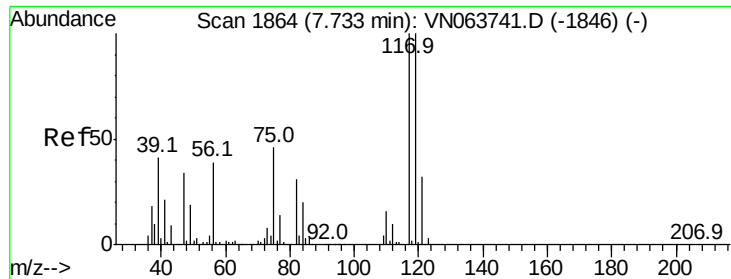

#38
Carbon Tetrachloride
Concen: 5.391 ug/l
RT: 7.62 min Scan# 1830
Delta R.T. -0.11 min
Lab File: VN063805.D
Acq: 2 Oct 2020 5:44




Instrument :
MSVOA_N
ClientSampled :
MW-2


Tot Ion:117 Resp: 23725
Ion Ratio Lower Upper
117 100
119 6.6 80.1 120.1#
121 0.0 25.7 38.5#

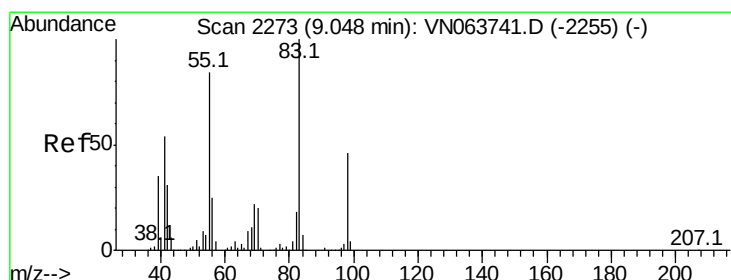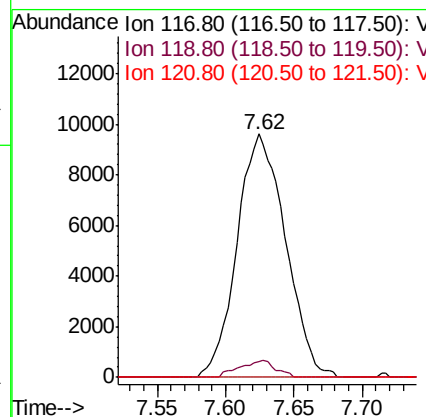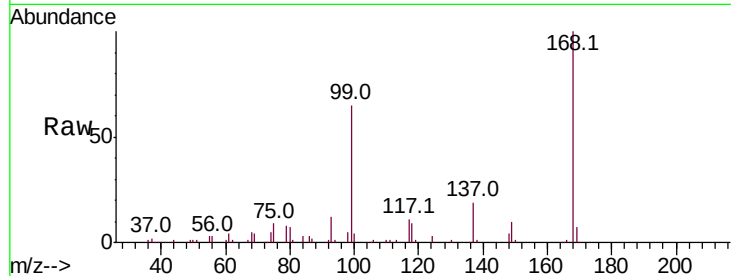

#39
Methylcyclohexane
Concen: 0.223 ug/l
RT: 9.05 min Scan# 2272
Delta R.T. -0.00 min
Lab File: VN063805.D
Acq: 2 Oct 2020 5:44

Tgt Ion: 83 Resp: 872
Ion Ratio Lower Upper
83 100
55 67.2 67.1 100.7
98 67.4 36.6 54.8#

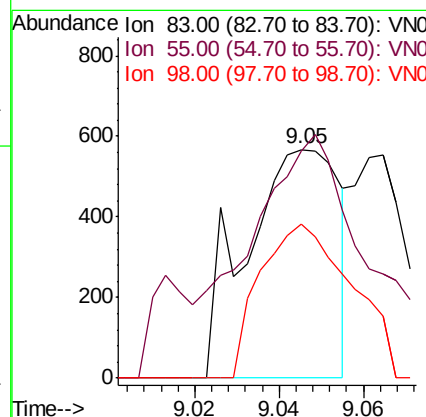



#40

Benzene

Concen: 0.628 ug/l

RT: 8.01 min Scan# 1949

Delta R.T. 0.00 min

Lab File: VN063805.D

Acq: 2 Oct 2020 5:44

Instrument :

MSVOA_N

ClientSampled :





MW-2

Tot Ion: 78 Resp: 7042

Ion Ratio Lower Upper

78 100

77 30.2 18.7 28.1#

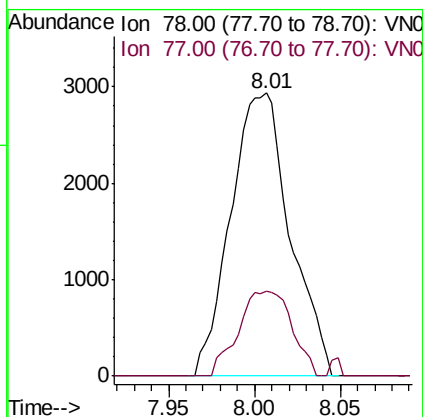

#42

1,2-Dichloroethane

Concen: 3.025 ug/l

RT: 8.09 min Scan# 1975

Delta R.T. 0.01 min

Lab File: VN063805.D




Acq: 2 Oct 2020 5:44


Tgt Ion: 62 Resp: 14475

Ion Ratio Lower Upper

62 100

98 6.9 0.0 15.0

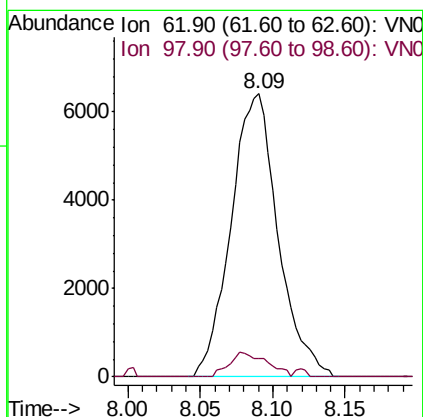

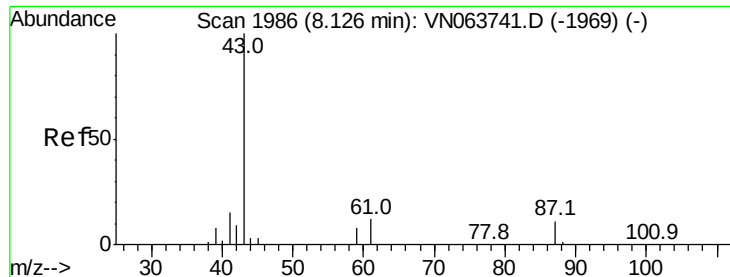

#43

Isopropyl Acetate

Concen: 2.835 ug/l

RT: 8.10 min Scan# 1977

Delta R.T. -0.03 min

Lab File: VN063805.D

Acq: 2 Oct 2020 5:44

Instrument :

MSVOA_N

ClientSampled :

MW-2


Tot Ion: 43 Resp: 18231

Ion Ratio Lower Upper

43 100

61 8.6 14.2 21.4#




87 0.0 9.0 13.6#

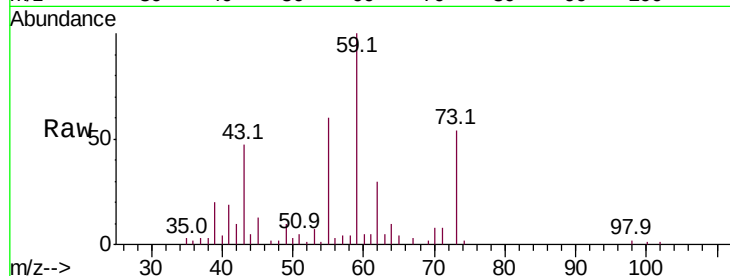

Abundance Ion 43.00 (42.70 to 43.70): VN063741.D (-1969) (-)

Ion 61.00 (60.70 to 61.70): VN063741.D (-1969) (-)

Ion 87.00 (86.70 to 87.70): VN063741.D (-1969) (-)

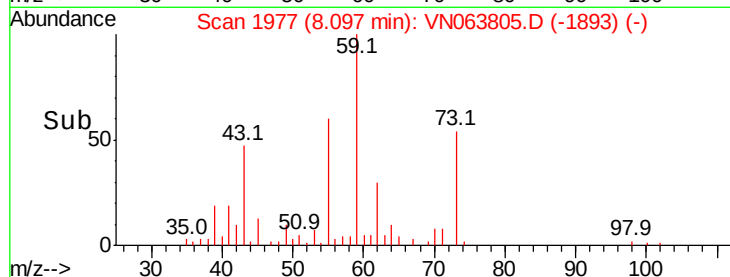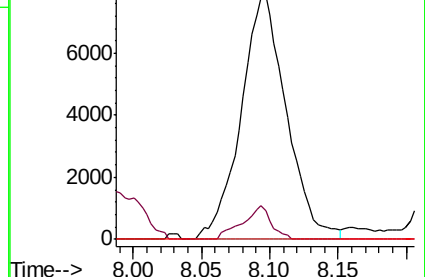

#44

Trichloroethene

Concen: 0.873 ug/l

RT: 8.81 min Scan# 2198

Delta R.T. 0.01 min

Lab File: VN063805.D


Acq: 2 Oct 2020 5:44

Tgt Ion:130 Resp: 2564

Ion Ratio Lower Upper



130 100


95 102.2 0.0 213.6



Abundance Ion 129.80 (129.50 to 130.50): VN063741.D (-2180) (-)

Ion 94.90 (94.60 to 95.60): VN063741.D (-2180) (-)



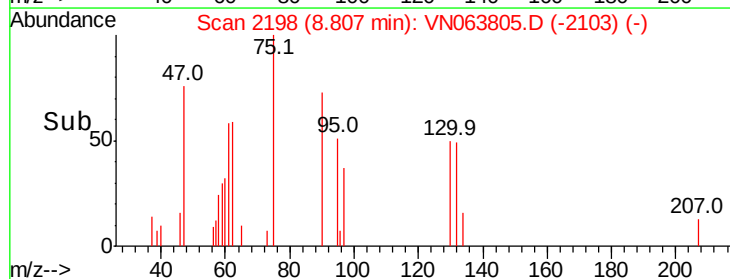
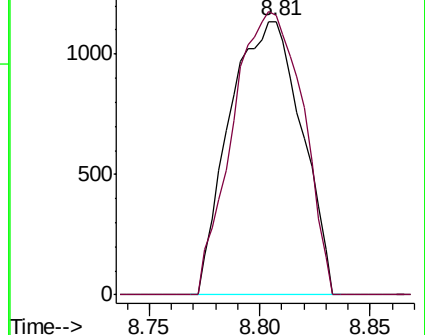


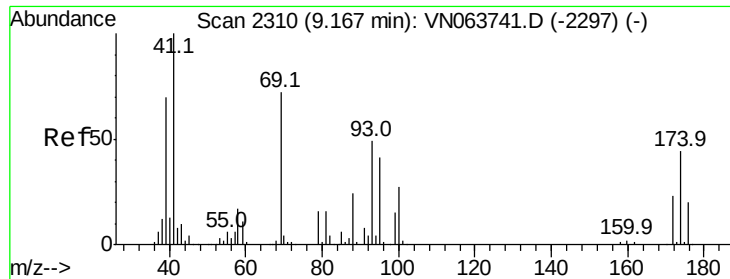

#48
Methvl methacrylate
Concen: 0.314 ug/l
RT: 9.16 min Scan# 2309
Delta R.T. -0.00 min
Lab File: VN063805.D
Acq: 2 Oct 2020 5:44




Instrument :
MSVOA_N
ClientSampled :
MW-2


Tot Ion: 41 Resp: 997
Ion Ratio Lower Upper
41 100
69 0.0 60.9 91.3#
39 9.7 57.5 86.3#

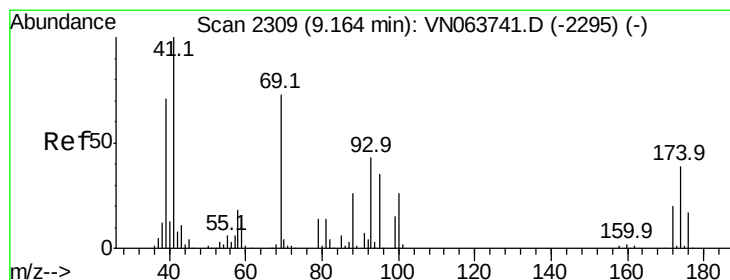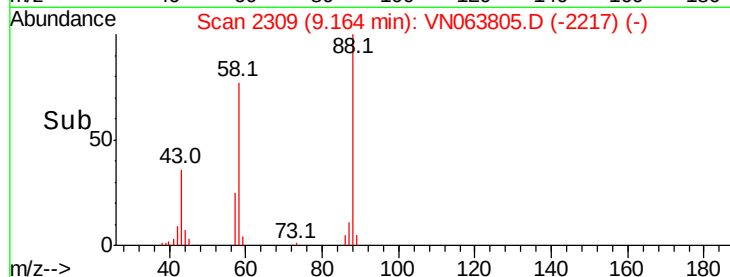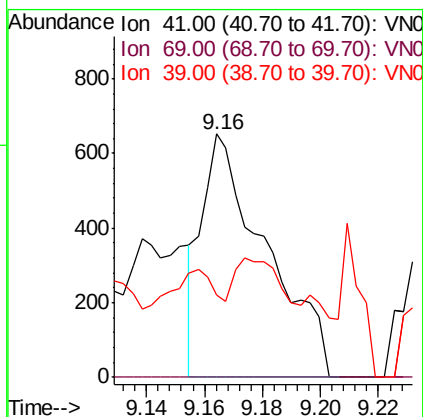

#49
1,4-Dioxane
Concen: 615.371 ug/l
RT: 9.17 min Scan# 2310
Delta R.T. 0.00 min
Lab File: VN063805.D
Acq: 2 Oct 2020 5:44

Tgt Ion: 88 Resp: 27788
Ion Ratio Lower Upper
88 100
43 39.5 33.1 49.7
58 75.5 58.9 88.3


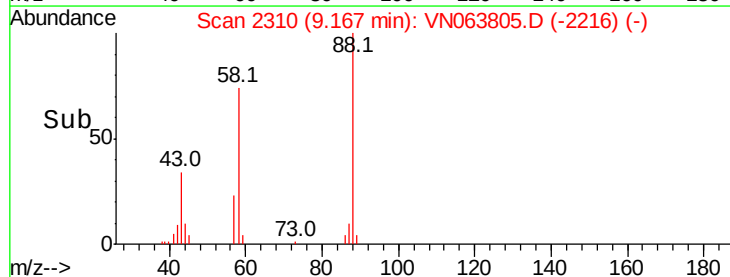
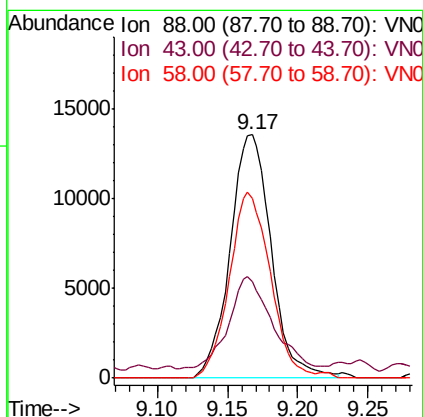



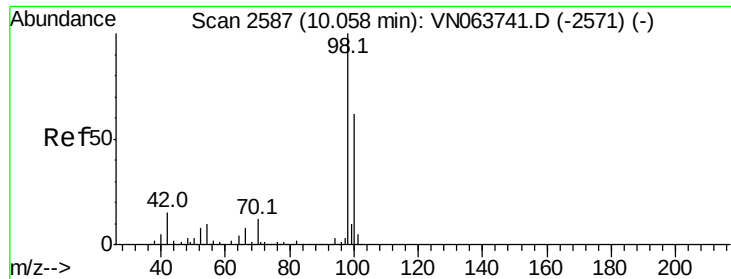

#50
Toluene-d8
Concen: 48.160 ug/l
RT: 10.06 min Scan# 2588
Delta R.T. 0.00 min
Lab File: VN063805.D
Acq: 2 Oct 2020 5:44




Instrument :
MSVOA_N
ClientSampled :
MW-2


Tot Ion: 98 Resp: 490704
Ion Ratio Lower Upper
98 100
100 63.8 49.8 74.6

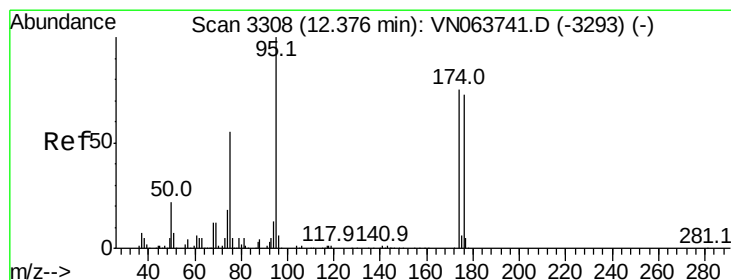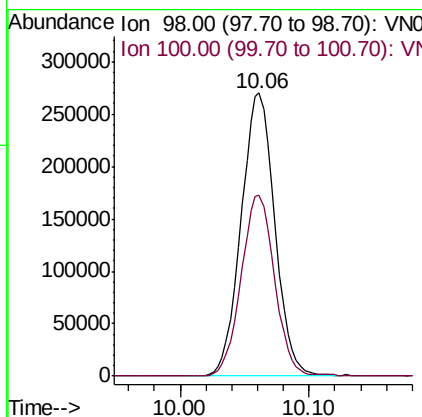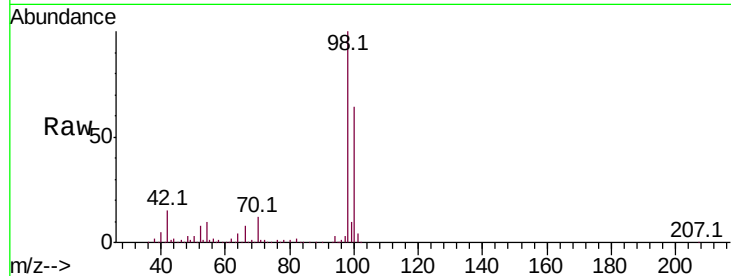

#62
4-Bromofluorobenzene
Concen: 49.212 ug/l
RT: 12.38 min Scan# 3308
Delta R.T. 0.00 min
Lab File: VN063805.D
Acq: 2 Oct 2020 5:44

Tgt Ion: 95 Resp: 188492
Ion Ratio Lower Upper
95 100
174 75.8 0.0 150.6
176 73.4 0.0 145.4



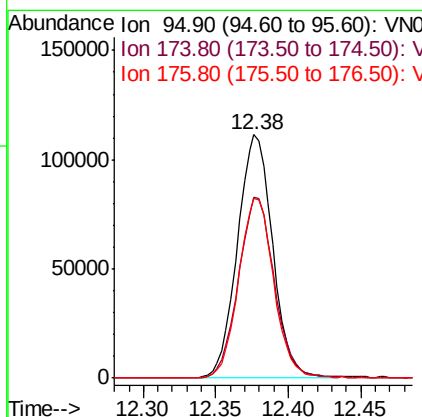



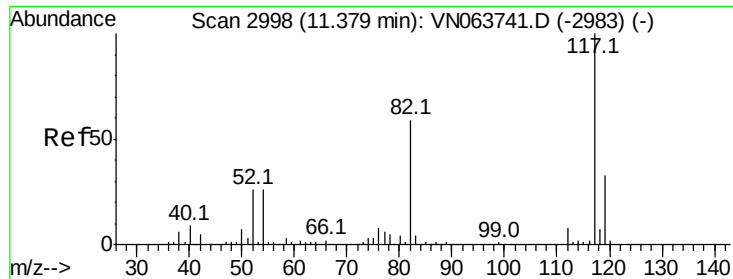

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2998
Delta R.T. 0.00 min
Lab File: VN063805.D
Acq: 2 Oct 2020 5:44




Instrument :
MSVOA_N
ClientSampleId :
MW-2


Tot Ion:117 Resp: 388027
Ion Ratio Lower Upper
117 100
82 60.7 47.4 71.2
119 32.0 26.4 39.6

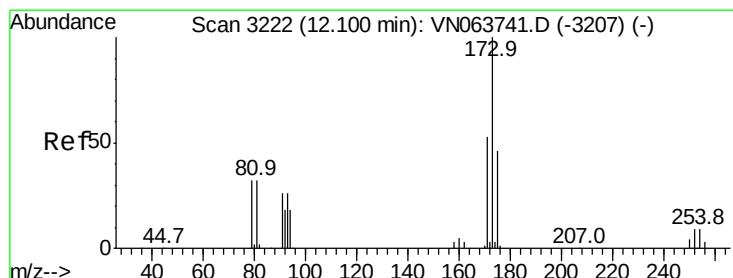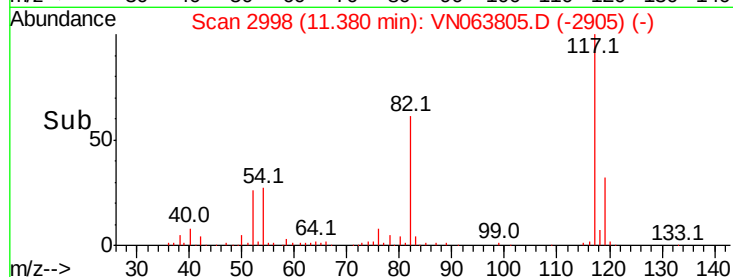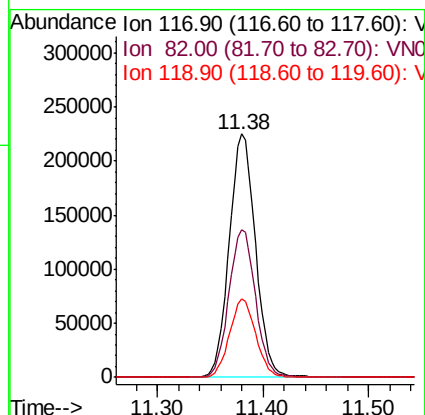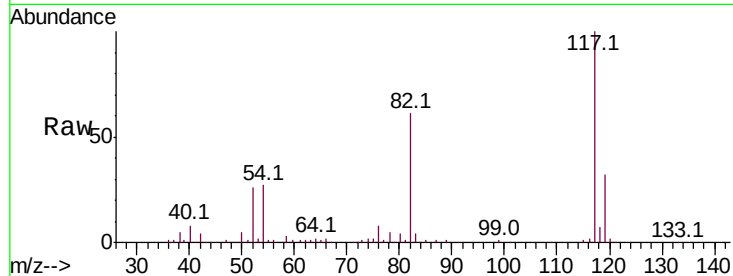

#71
Bromoform
Concen: 0.333 ug/l
RT: 12.37 min Scan# 3306
Delta R.T. 0.27 min
Lab File: VN063805.D
Acq: 2 Oct 2020 5:44

Tgt Ion:173 Resp: 777
Ion Ratio Lower Upper
173 100
175 1125.2 23.5 70.5#
254 0.0 0.0 0.0

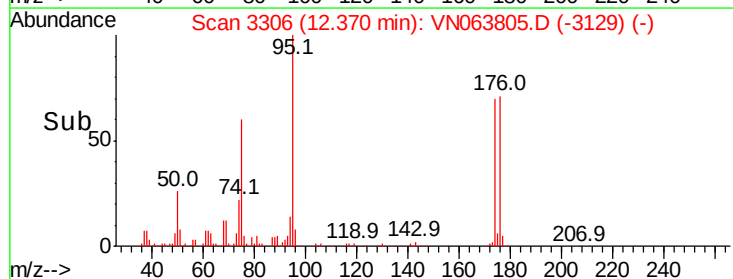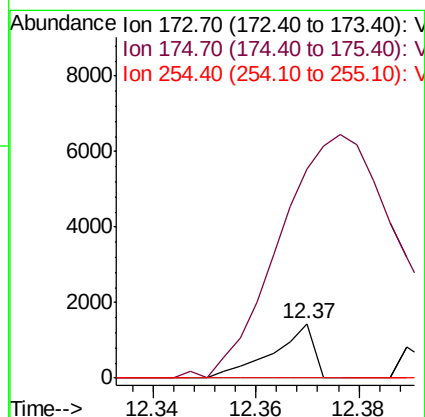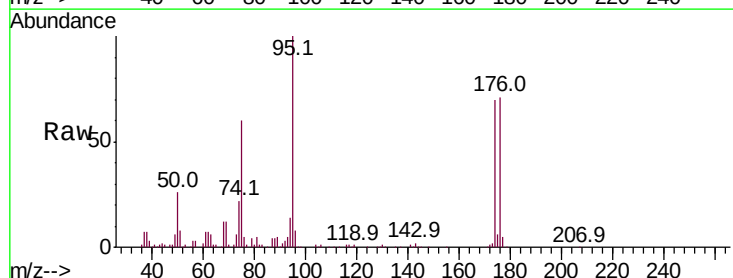







#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.32 min Scan# 3601
Delta R.T. 0.00 min
Lab File: VN063805.D
Acq: 2 Oct 2020 5:44

Instrument :
MSVOA_N
ClientSampled :
MW-2

Tot Ion:152 Resp: 163315
Ion Ratio Lower Upper
152 100
115 61.4 31.3 93.8
150 157.7 0.0 341.8




Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

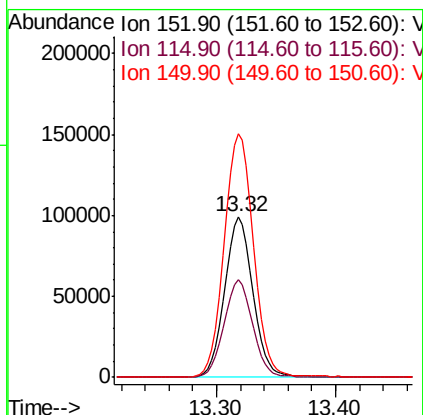




#74
N-ethyl acetate
Concen: 2.230 ug/l
RT: 12.06 min Scan# 3209
Delta R.T. 0.01 min
Lab File: VN063805.D
Acq: 2 Oct 2020 5:44

Tgt Ion: 43 Resp: 82
Ion Ratio Lower Upper
43 100
70 0.0 29.8 44.8#
55 130.5 17.9 26.9#
61 0.0 17.0 25.4#



Abundance Ion 43.00 (42.70 to 43.70): V
Ion 70.00 (69.70 to 70.70): V
Ion 55.00 (54.70 to 55.70): V
Ion 61.00 (60.70 to 61.70): V



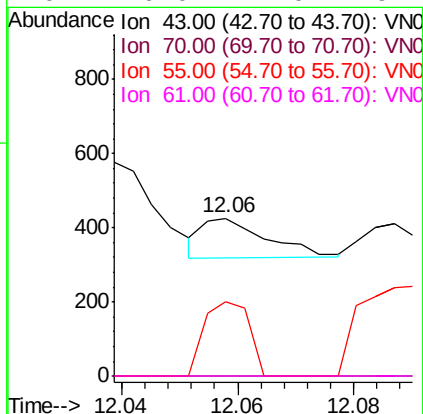





#76
 1,2,3-Trichloropropane
 Concen: 30.873 ug/l
 RT: 12.38 min Scan# 3308
 Delta R.T. -0.15 min
 Lab File: VN063805.D
 Acq: 2 Oct 2020 5:44




Instrument :
 MSVOA_N
 ClientSampled :
 MW-2


Tot Ion: 75 Resp: 111147
 Ion Ratio Lower Upper
 75 100
 77 1.5 0.0 0.0#

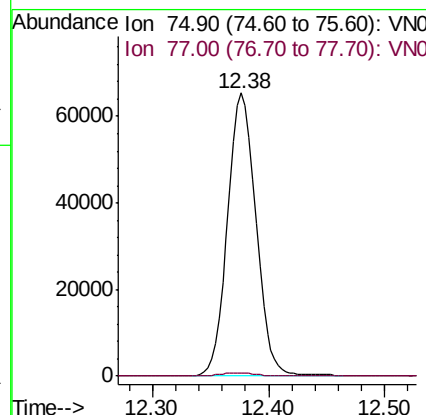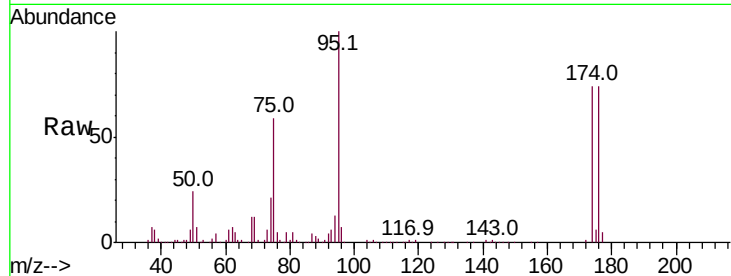

#81
 trans-1,4-Dichloro-2-butene
 Concen: 88.920 ug/l
 RT: 12.38 min Scan# 3308
 Delta R.T. 0.10 min
 Lab File: VN063805.D
 Acq: 2 Oct 2020 5:44

Tgt Ion: 75 Resp: 111147
 Ion Ratio Lower Upper
 75 100
 53 1.9 88.2 132.2#
 89 6.8 36.0 54.0#

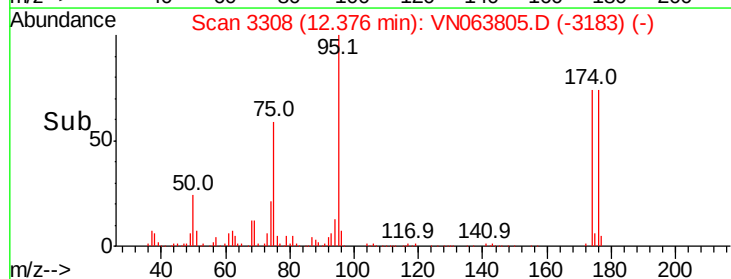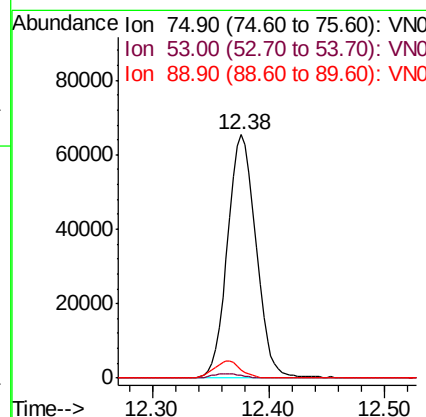


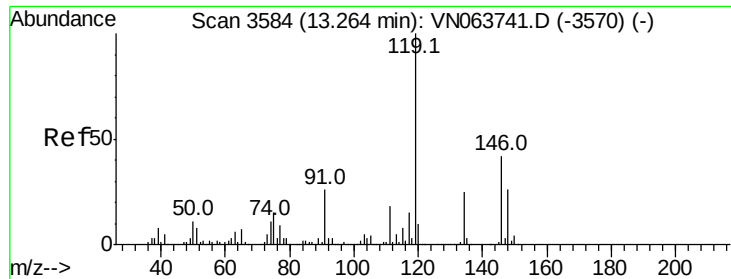




#86
 p-Isopropyltoluene
 Concen: 0.210 ug/l
 RT: 13.42 min Scan# 3632
 Delta R.T. 0.15 min
 Lab File: VN063805.D
 Acq: 2 Oct 2020 5:44

Instrument :
 MSVOA_N
 ClientSampled :
 MW-2

Tot Ion:119 Resp: 1991
 Ion Ratio Lower Upper
 119 100
 134 37.0 12.6 37.8
 91 25.0 13.4 40.2

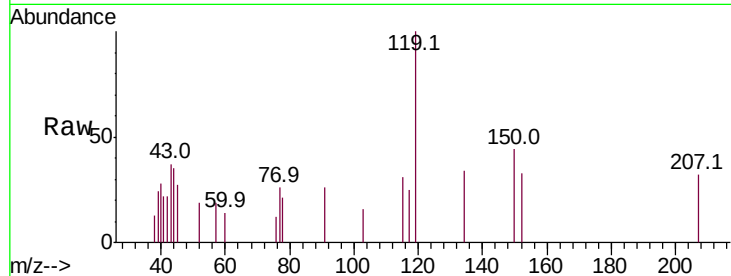


Abundance Ion 119.00 (118.70 to 119.70): V
 Ion 134.00 (133.70 to 134.70): V
 Ion 91.00 (90.70 to 91.70): V

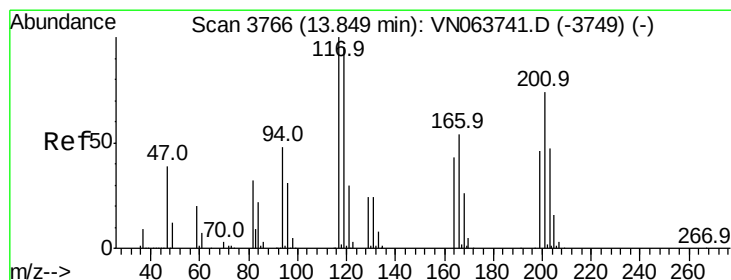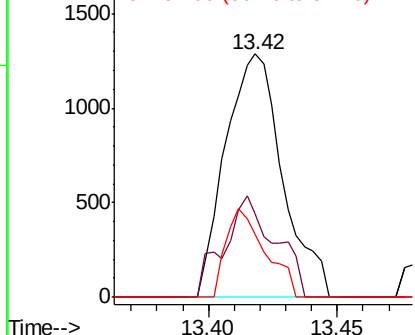

#90
 Hexachloroethane
 Concen: 0.450 ug/l
 RT: 13.97 min Scan# 3805
 Delta R.T. 0.13 min
 Lab File: VN063805.D
 Acq: 2 Oct 2020 5:44

Tgt Ion:117 Resp: 828
 Ion Ratio Lower Upper
 117 100
 201 0.0 36.0 108.0#



Abundance Ion 116.80 (116.50 to 117.50): V
 Ion 200.70 (200.40 to 201.40): V

