

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN100120\
 Data File : VN063787.D
 Acq On : 1 Oct 2020 21:21
 Operator : JC/MD
 Sample : PB132009ZHE#09
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB132009ZHE#09

Quant Time: Oct 02 03:44:40 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 01 01:46:38 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	209789	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	405204	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	420285	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	173653	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.99	65	186617	53.84	ug/l	0.00
Spiked Amount 50.000			Recovery	=	107.68%	
35) Dibromofluoromethane	7.55	113	134451	47.82	ug/l	0.00
Spiked Amount 50.000			Recovery	=	95.64%	
50) Toluene-d8	10.06	98	522055	48.98	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.96%	
62) 4-Bromofluorobenzene	12.38	95	206586	51.56	ug/l	0.00
Spiked Amount 50.000			Recovery	=	103.12%	
Target Compounds						
16) Acetone	3.78	43	22618	21.200	ug/l	94
18) Methyl Acetate	4.30	43	5049	1.823	ug/l #	76
20) Methylene Chloride	4.51	84	8049	3.385	ug/l #	92
43) Isopropyl Acetate	8.13	43	74675	11.100	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN100120\
Data File : VN063787.D
Acq On : 1 Oct 2020 21:21
Operator : JC/MD
Sample : PB132009ZHE#09
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB132009ZHE#09

Quant Time: Oct 02 03:44:40 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 01 01:46:38 2020
Response via : Initial Calibration

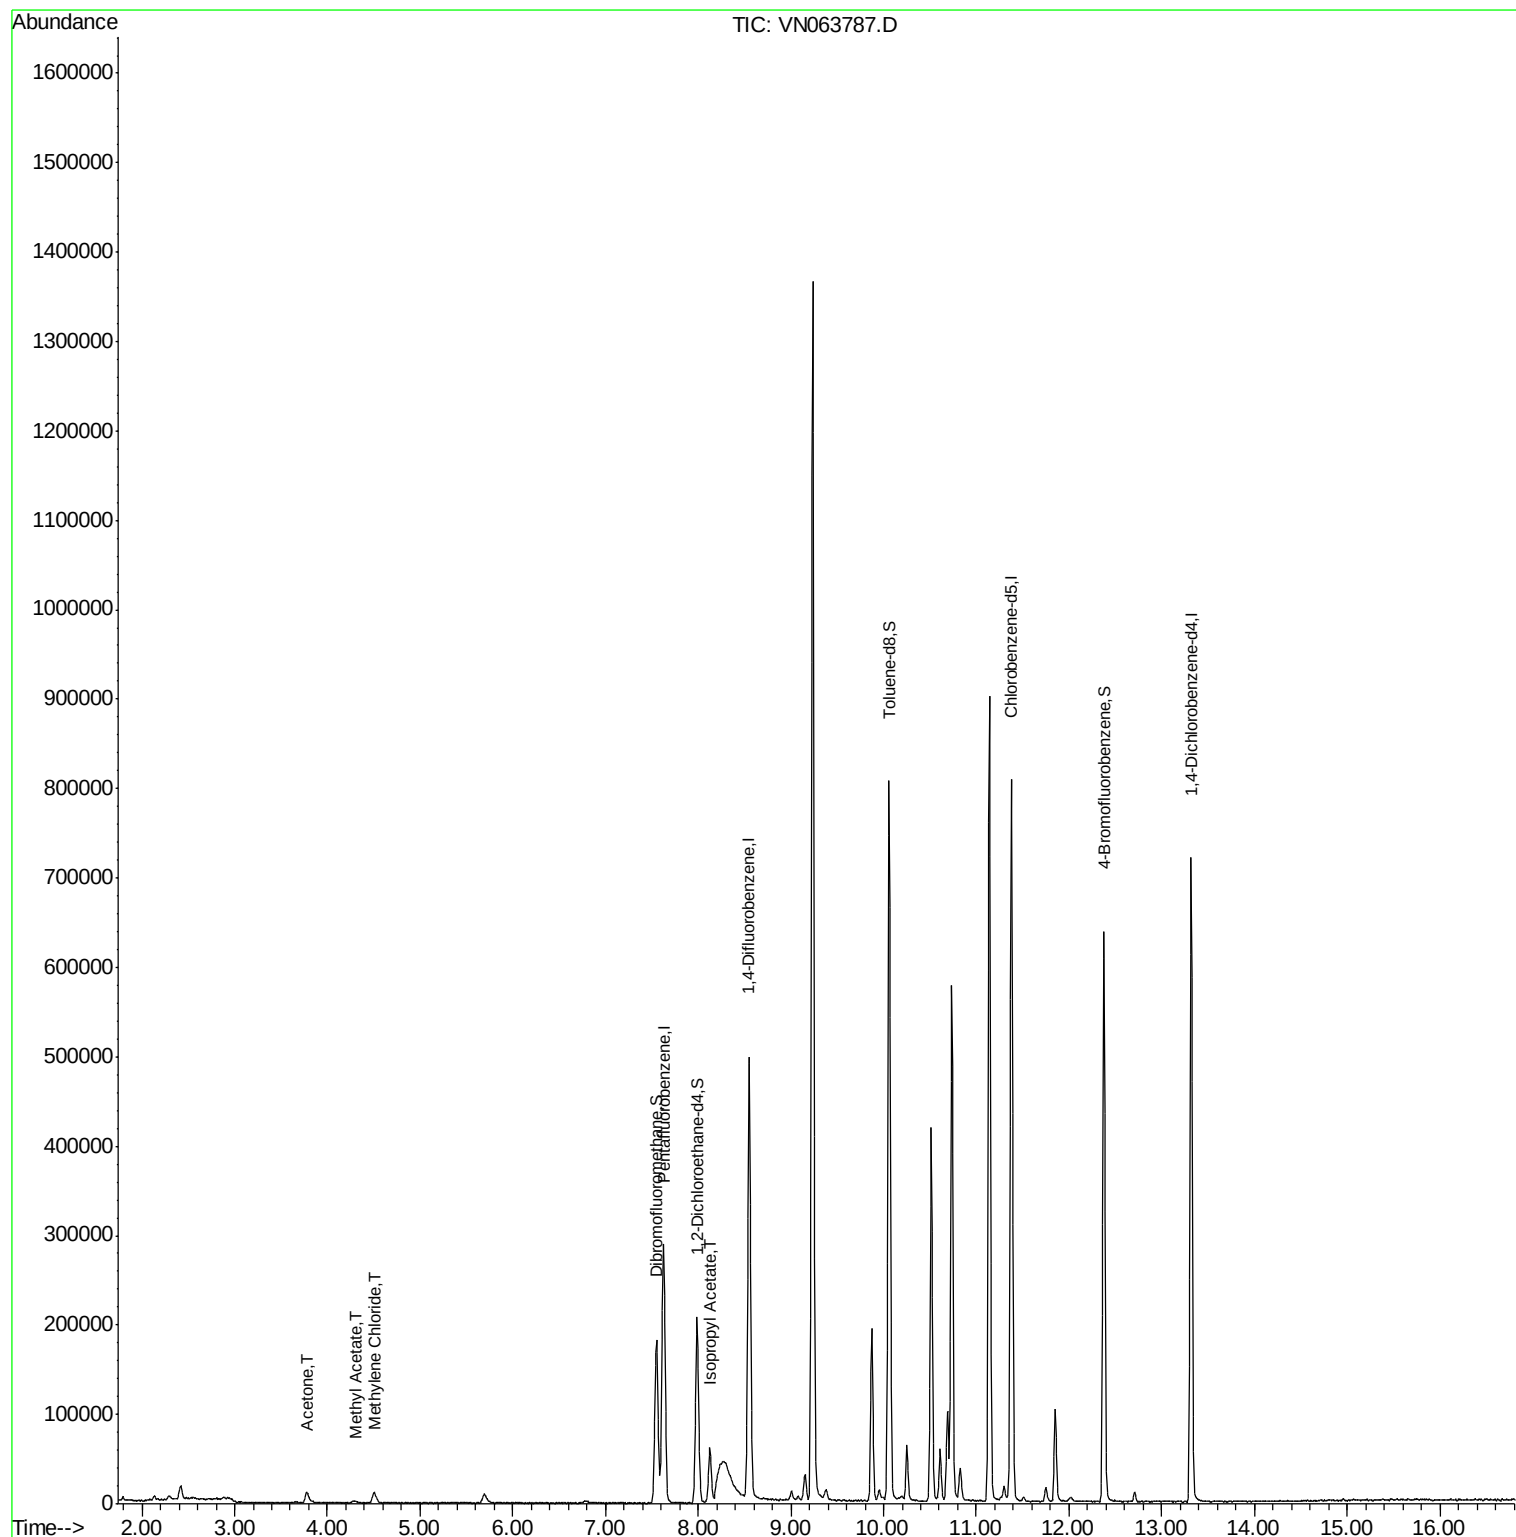

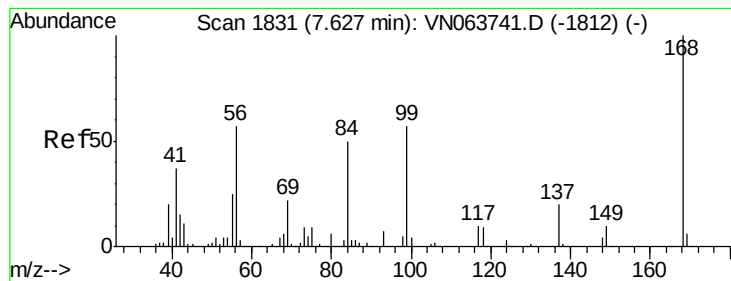

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN063787.D

Acq: 1 Oct 2020 21:21

Instrument :

MSVOA_N

ClientSampleId :


PB132009ZHE#09

Tot Ion:168 Resp: 209789

Ion Ratio Lower Upper

168 100

99 67.7 51.8 77.6

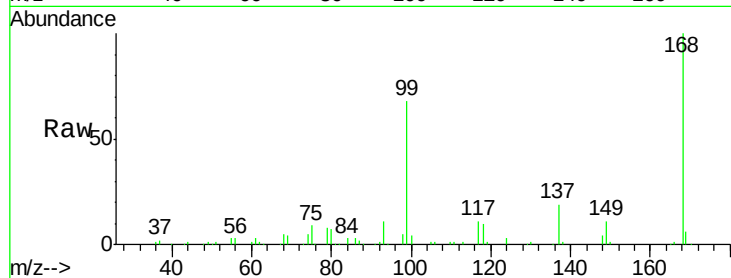

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

7.63

80000



60000

40000

20000

0

Time--> 7.50 7.60 7.70

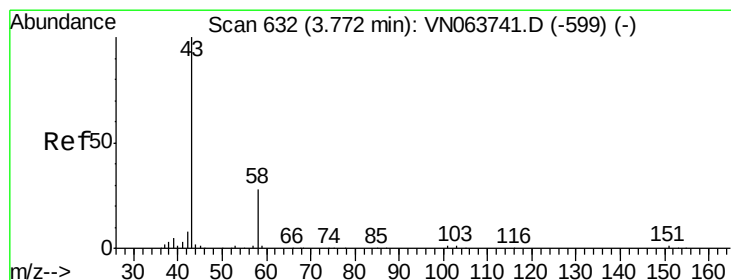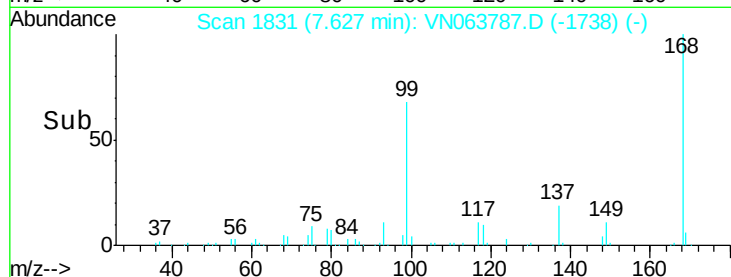

#16

Acetone

Concen: 21.200 ug/l

RT: 3.78 min Scan# 635

Delta R.T. 0.01 min

Lab File: VN063787.D


Acq: 1 Oct 2020 21:21

Tgt Ion: 43 Resp: 22618

Ion Ratio Lower Upper

43 100

58 24.9 22.3 33.5

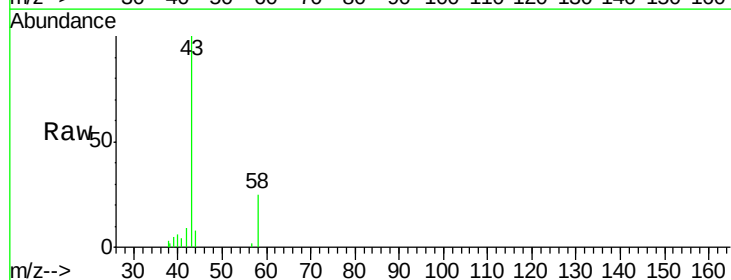

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

3.78

8000


6000


4000

2000

0

Time--> 3.70 3.75 3.80 3.85 3.90




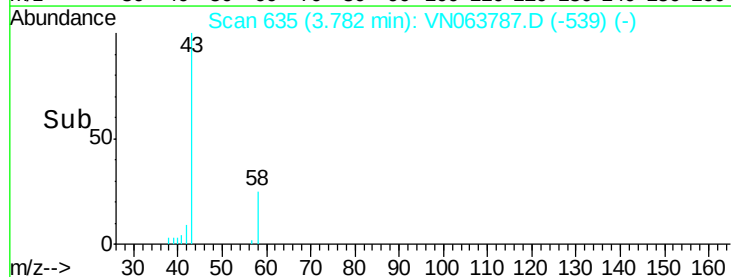


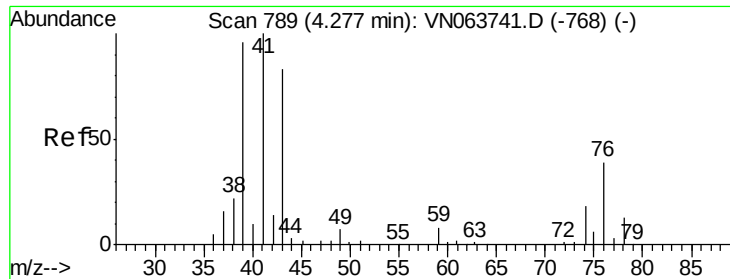

#18
Methyl Acetate
Concen: 1.823 ug/l
RT: 4.30 min Scan# 796
Delta R.T. 0.02 min
Lab File: VN063787.D
Acq: 1 Oct 2020 21:21




Instrument :
MSVOA_N
ClientSampleId :
PB132009ZHE#09


Tot Ion: 43 Resp: 5049
Ion Ratio Lower Upper
43 100
74 10.5 17.4 26.2#

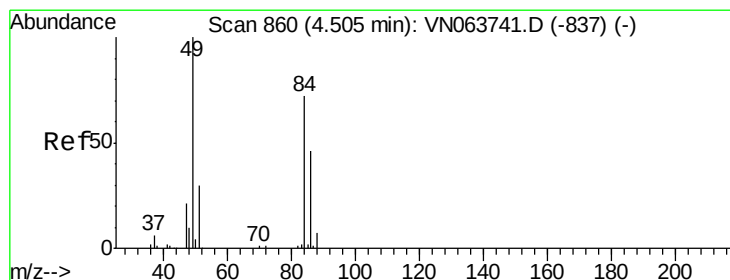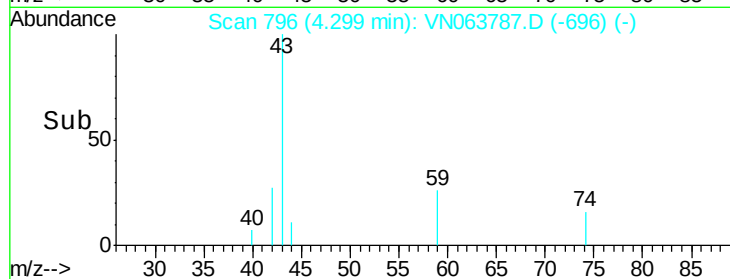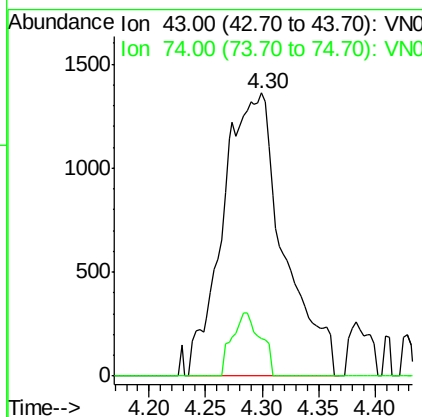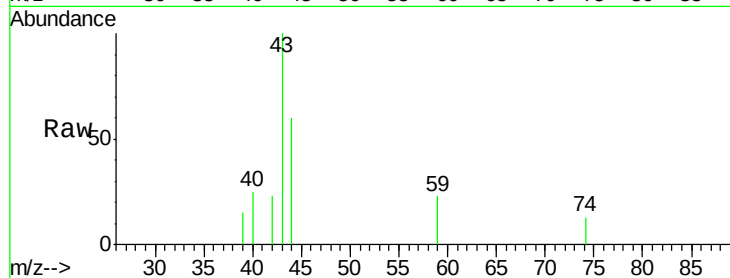

#20
Methylene Chloride
Concen: 3.385 ug/l
RT: 4.51 min Scan# 861
Delta R.T. 0.00 min
Lab File: VN063787.D
Acq: 1 Oct 2020 21:21

Tgt Ion: 84 Resp: 8049
Ion Ratio Lower Upper
84 100
49 144.9 110.4 165.6
51 51.3 33.3 49.9#
86 68.3 50.7 76.1


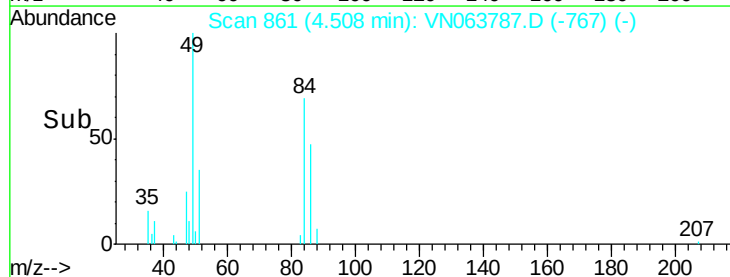
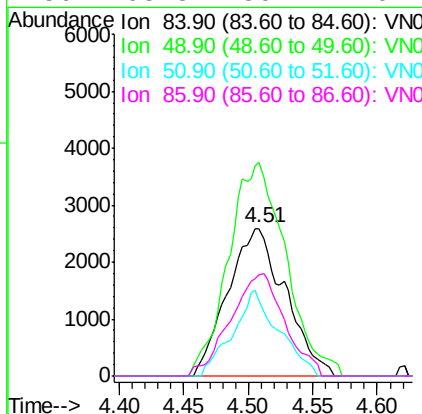
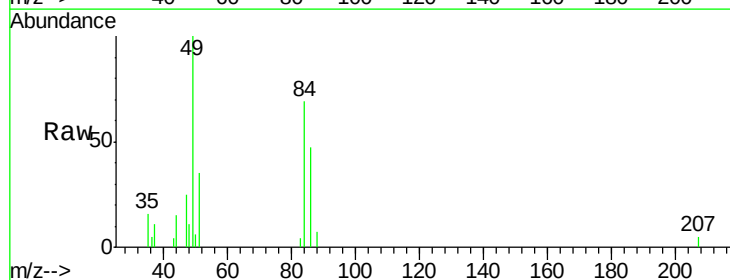


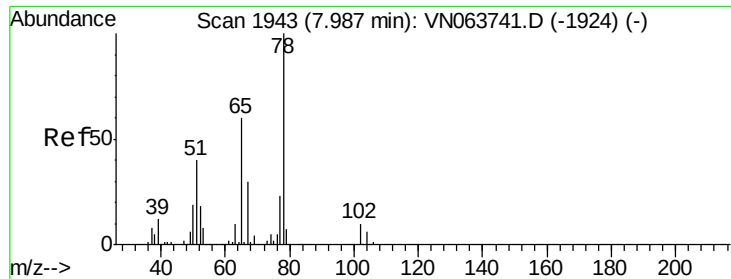

#33
 1,2-Dichloroethane-d4
 Concen: 53.844 ug/l
 RT: 7.99 min Scan# 1943
 Delta R.T. 0.00 min
 Lab File: VN063787.D
 Acq: 1 Oct 2020 21:21




Instrument :
 MSVOA_N
 ClientSampleId :
 PB132009ZHE#09


Tot Ion: 65 Resp: 186617
 Ion Ratio Lower Upper
 65 100
 67 49.2 0.0 99.6

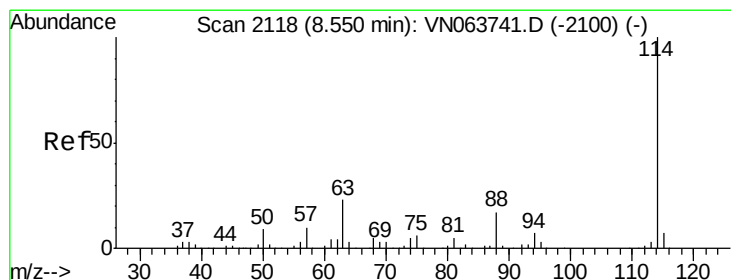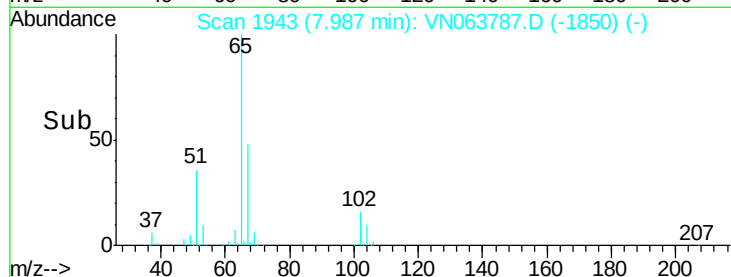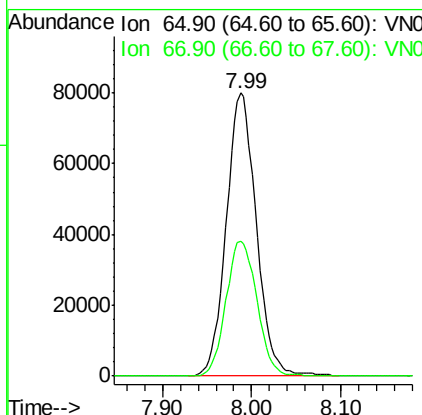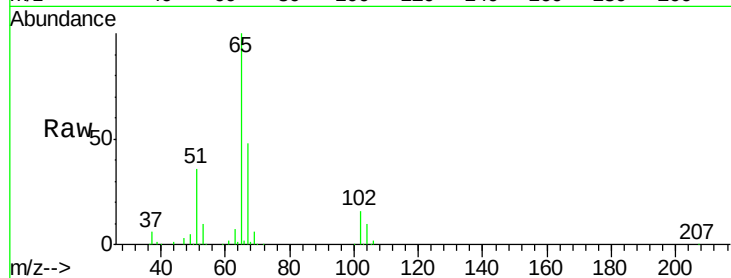

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2119
 Delta R.T. 0.00 min
 Lab File: VN063787.D
 Acq: 1 Oct 2020 21:21

Tgt Ion: 114 Resp: 405204
 Ion Ratio Lower Upper
 114 100
 63 22.2 0.0 45.0
 88 16.6 0.0 34.0

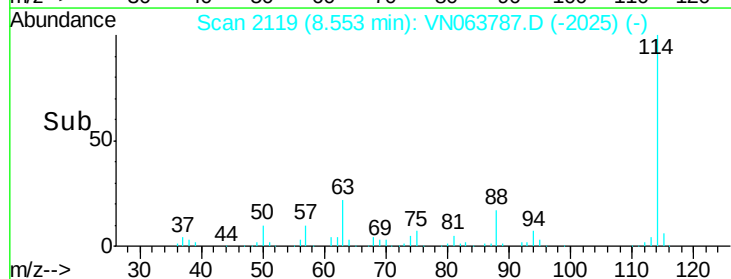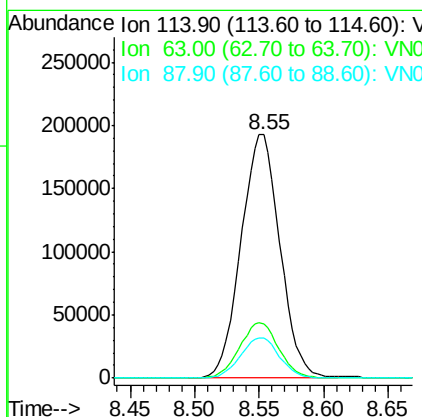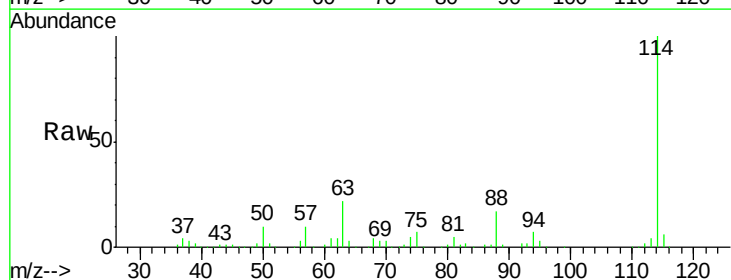


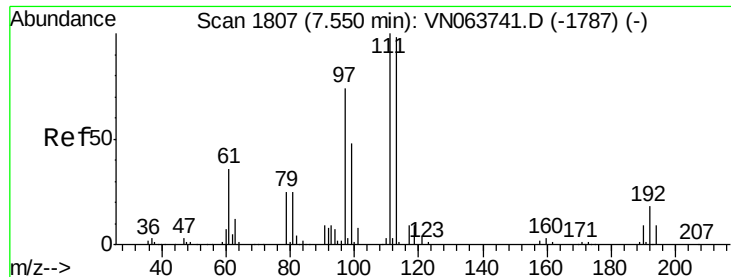




#35
 Dibromofluoromethane
 Concen: 47.820 ug/l
 RT: 7.55 min Scan# 1808
 Delta R.T. 0.00 min
 Lab File: VN063787.D
 Acq: 1 Oct 2020 21:21

Instrument :
 MSVOA_N
 ClientSampleId :
 PB132009ZHE#09

Tot Ion:113 Resp: 134451
 Ion Ratio Lower Upper
 113 100
 111 103.1 81.8 122.8
 192 17.8 14.2 21.2

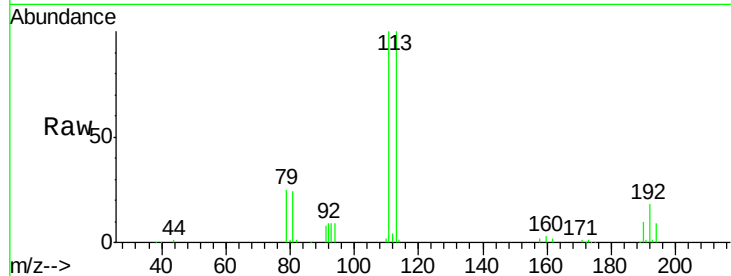


Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

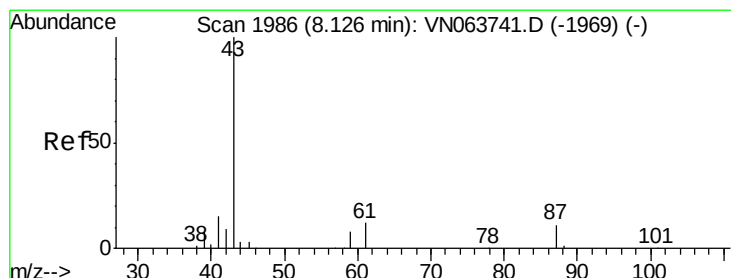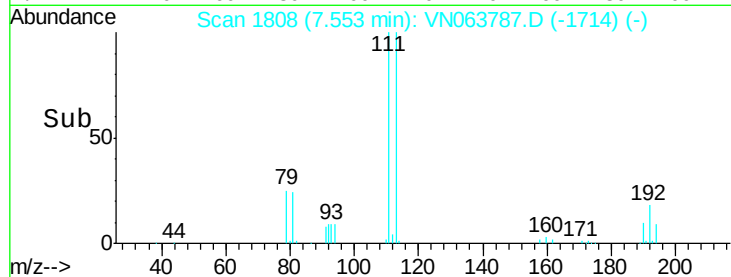
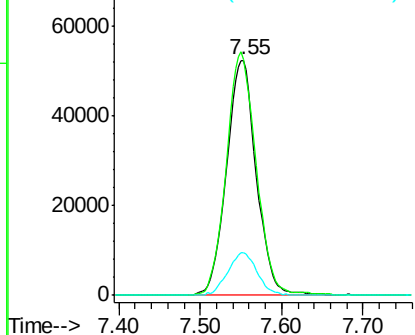



#43
 Isopropyl Acetate
 Concen: 11.100 ug/l
 RT: 8.13 min Scan# 1986
 Delta R.T. 0.00 min
 Lab File: VN063787.D
 Acq: 1 Oct 2020 21:21

Tgt Ion: 43 Resp: 74675
 Ion Ratio Lower Upper
 43 100
 61 16.7 14.2 21.4
 87 11.9 9.0 13.6

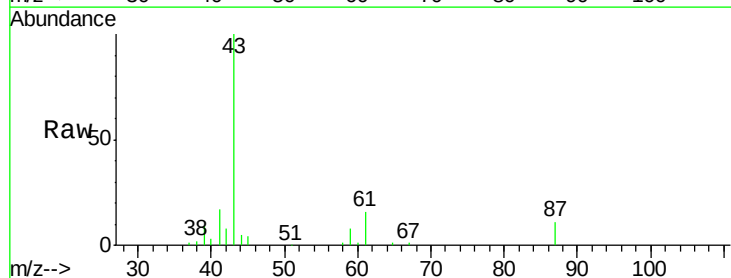

Abundance Ion 43.00 (42.70 to 43.70): V
 Ion 61.00 (60.70 to 61.70): V
 Ion 87.00 (86.70 to 87.70): V

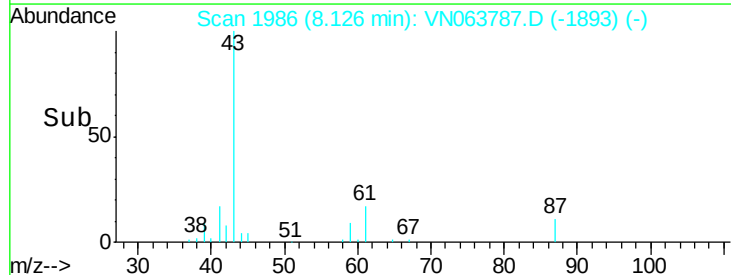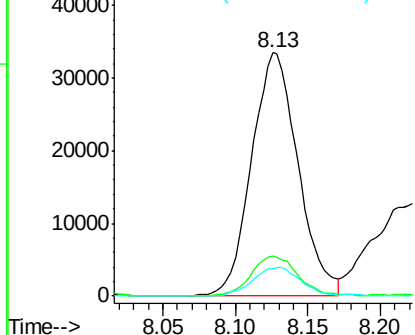

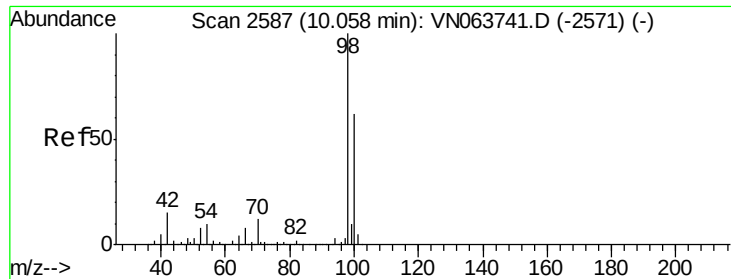

#50

Toluene-d8

Concen: 48.980 ug/l

RT: 10.06 min Scan# 2587

Delta R.T. 0.00 min

Lab File: VN063787.D

Acq: 1 Oct 2020 21:21

Instrument :

MSVOA_N

ClientSampleId :





PB132009ZHE#09

Tot Ion: 98 Resp: 522055

Ion Ratio Lower Upper

98 100

100 63.9 49.8 74.6

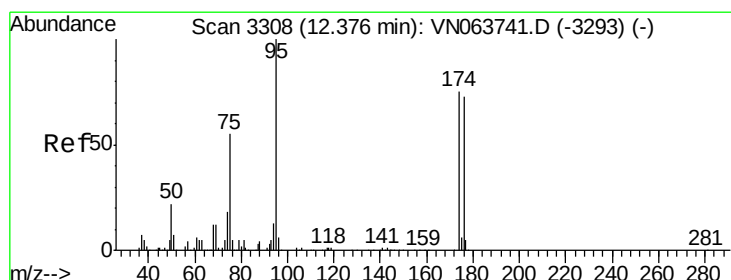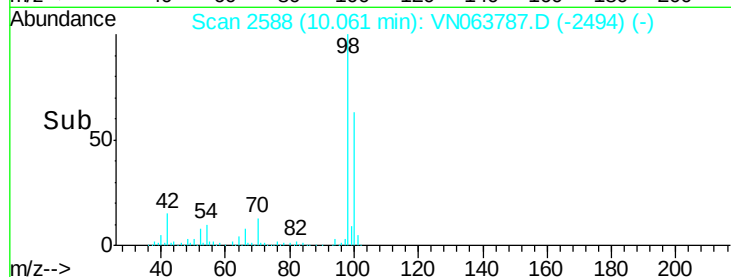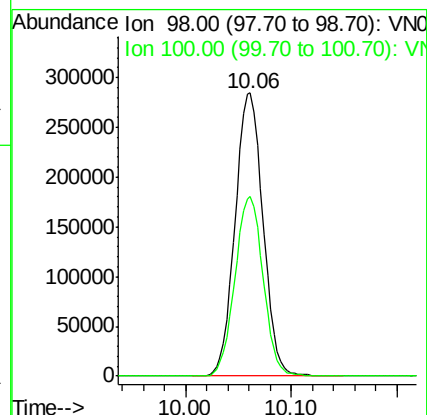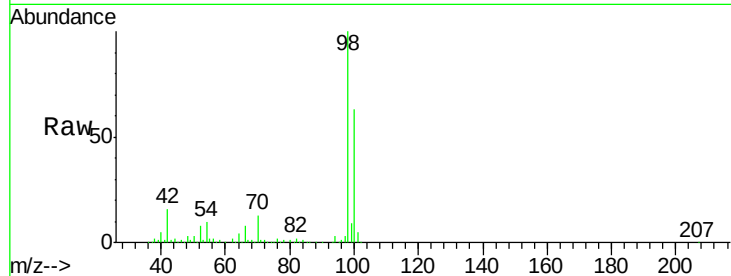

#62

4-Bromofluorobenzene

Concen: 51.561 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. 0.00 min

Lab File: VN063787.D

Acq: 1 Oct 2020 21:21




Tgt Ion: 95 Resp: 206586


Ion Ratio Lower Upper

95 100

174 74.7 0.0 150.6

176 70.9 0.0 145.4


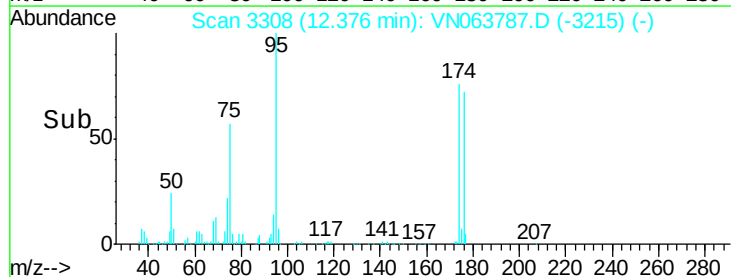
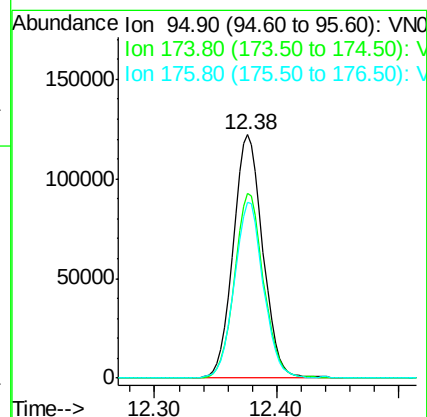
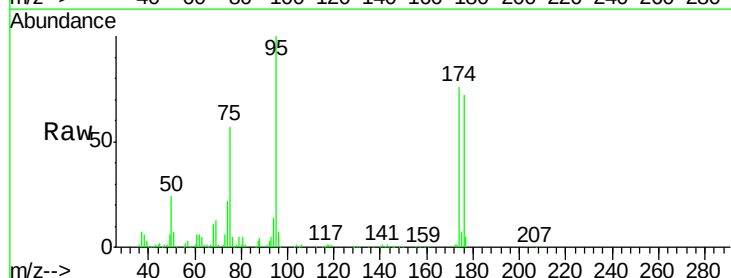


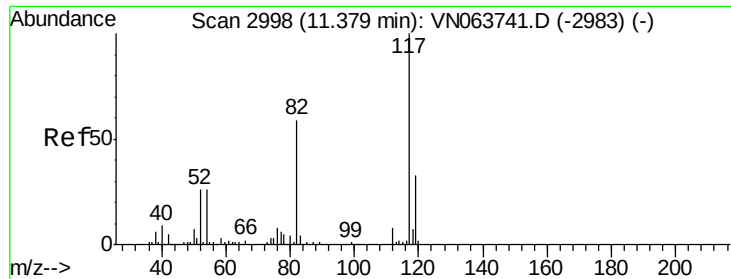

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2998
Delta R.T. 0.00 min
Lab File: VN063787.D
Acq: 1 Oct 2020 21:21

Instrument :
MSVOA_N
ClientSampleId :
PB132009ZHE#09

Tot Ion:117 Resp: 420285
Ion Ratio Lower Upper
117 100
82 61.4 47.4 71.2
119 32.4 26.4 39.6

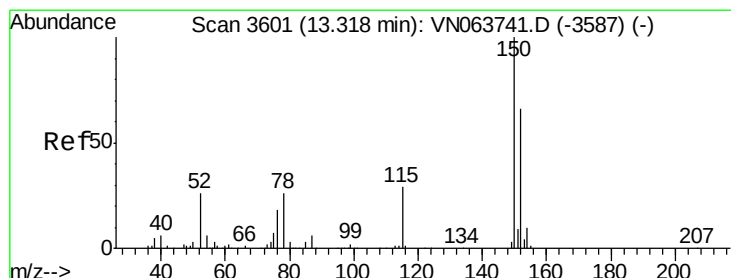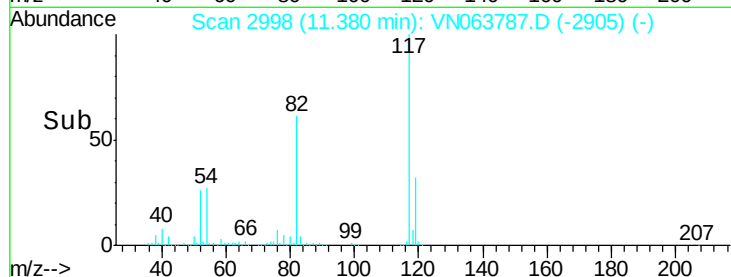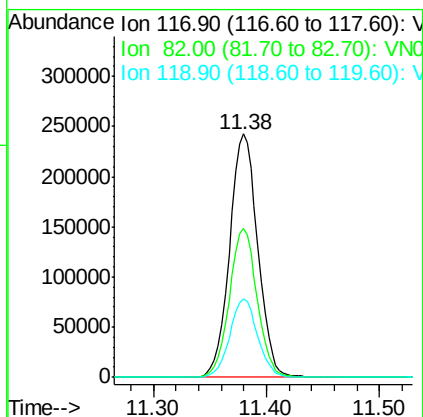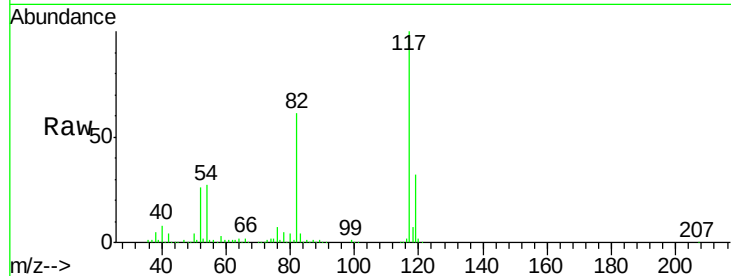

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.32 min Scan# 3601
Delta R.T. 0.00 min
Lab File: VN063787.D
Acq: 1 Oct 2020 21:21

Tgt Ion:152 Resp: 173653
Ion Ratio Lower Upper
152 100
115 63.7 31.3 93.8
150 157.2 0.0 341.8

