

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN100121\  
 Data File : VN068791.D  
 Acq On : 1 Oct 2021 18:33  
 Operator : JC/MD  
 Sample : M4040-01  
 Misc : 5.00mL/MSVOA\_N/WATER  
 ALS Vial : 17 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 SW-RR-01(2.0)

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N092921W.M

Title : SW846 8260

Signal : TIC: VN068791.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 8.021       | 2227          | 2249        | 2261         | rBV      | 382511         | 914779        | 34.59%          | 6.800%        |
| 2         | 8.088       | 2262          | 2274        | 2303         | rVB2     | 667517         | 1508314       | 57.03%          | 11.213%       |
| 3         | 8.440       | 2383          | 2405        | 2435         | rBV      | 418445         | 959261        | 36.27%          | 7.131%        |
| 4         | 8.971       | 2583          | 2603        | 2628         | rBV      | 960434         | 1994435       | 75.41%          | 14.827%       |
| 5         | 10.443      | 3130          | 3152        | 3182         | rBV      | 1437084        | 2644800       | 100.00%         | 19.661%       |
| 6         | 11.746      | 3619          | 3638        | 3663         | rBV      | 1205071        | 2143721       | 81.05%          | 15.936%       |
| 7         | 12.733      | 3986          | 4006        | 4027         | rBV      | 956876         | 1636682       | 61.88%          | 12.167%       |
| 8         | 13.675      | 4341          | 4357        | 4385         | rBV      | 953680         | 1649772       | 62.38%          | 12.264%       |




Sum of corrected areas: 13451764

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN100121\  
Data File : VN068791.D  
Acq On : 1 Oct 2021 18:33  
Operator : JC/MD  
Sample : M4040-01  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
SW-RR-01(2.0)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N092921W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

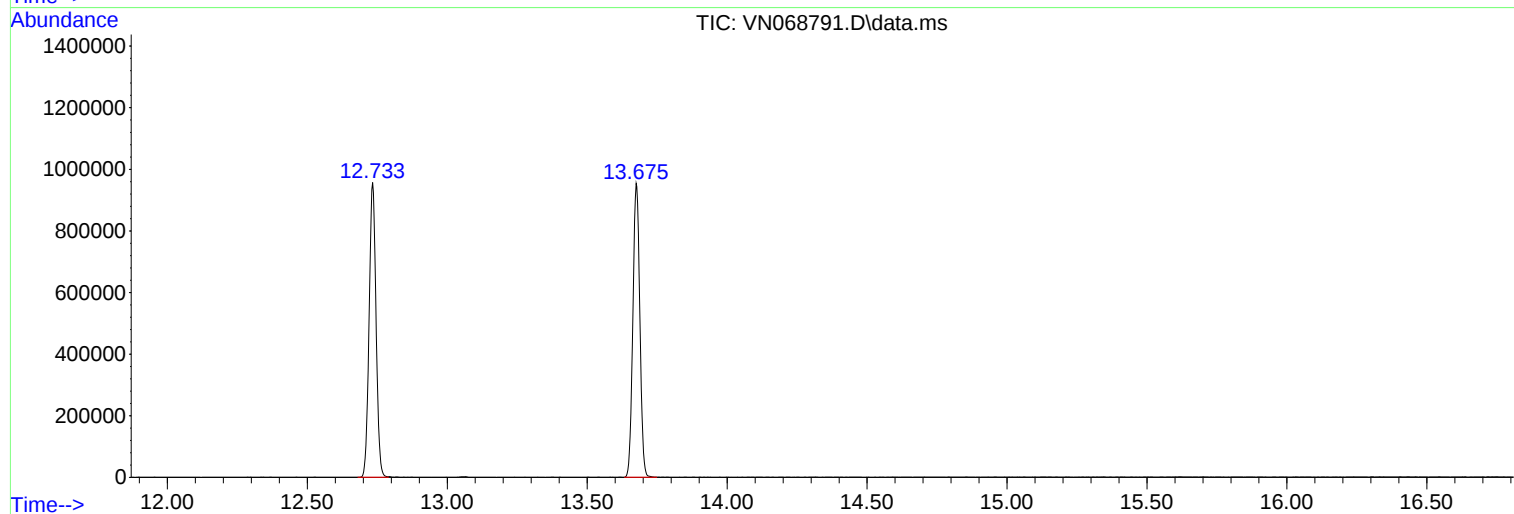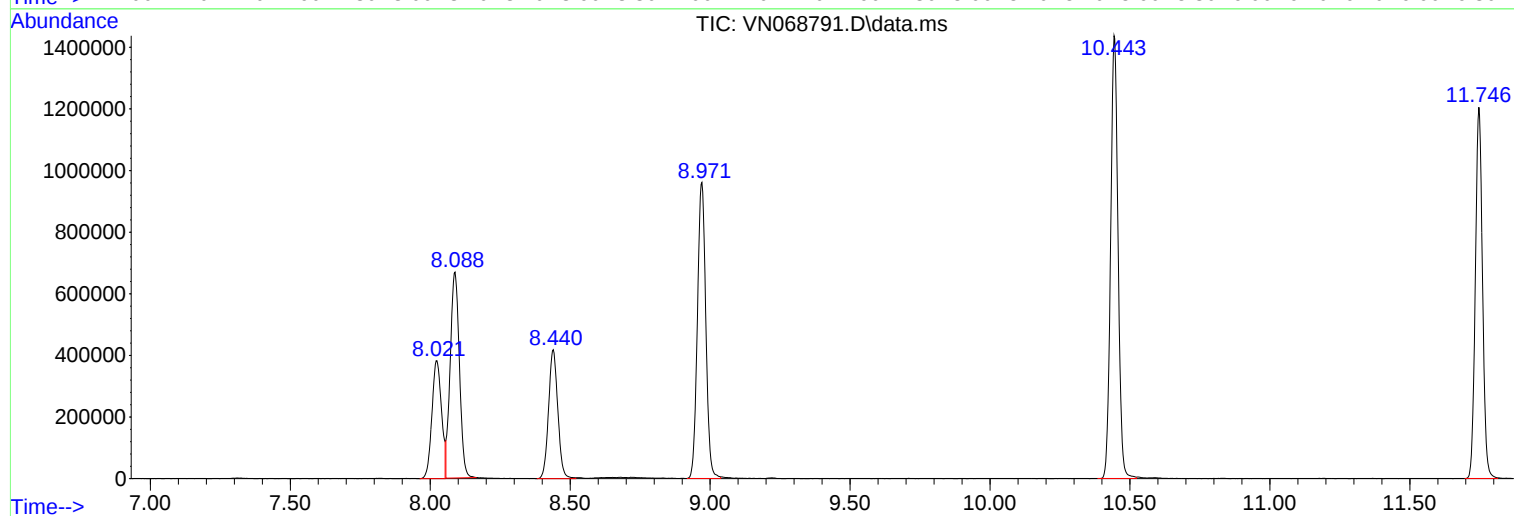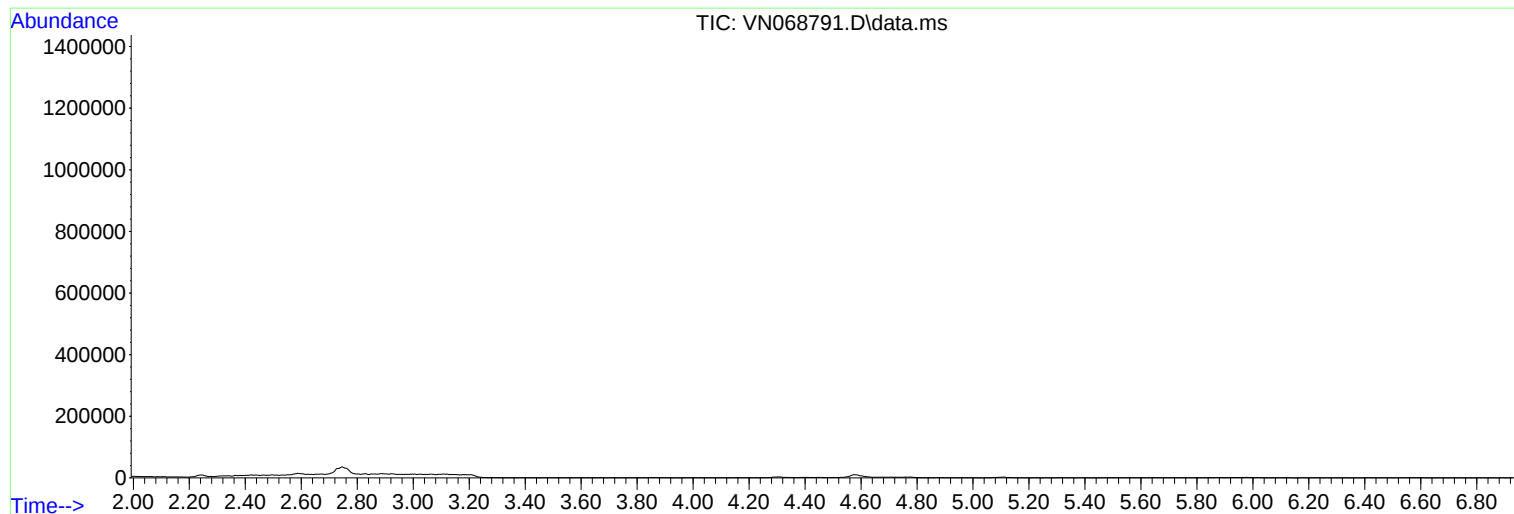

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN100121\  
Data File : VN068791.D  
Acq On : 1 Oct 2021 18:33  
Operator : JC/MD  
Sample : M4040-01  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
SW-RR-01(2.0)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N092921W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN100121\  
Data File : VN068791.D  
Acq On : 1 Oct 2021 18:33  
Operator : JC/MD  
Sample : M4040-01  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
SW-RR-01(2.0)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N092921W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |

-----