


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100121\
 Data File : VN068775.D
 Acq On : 1 Oct 2021 10:42
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N092921W.M
 Title : SW846 8260
 Last Update : Wed Sep 29 23:31:35 2021

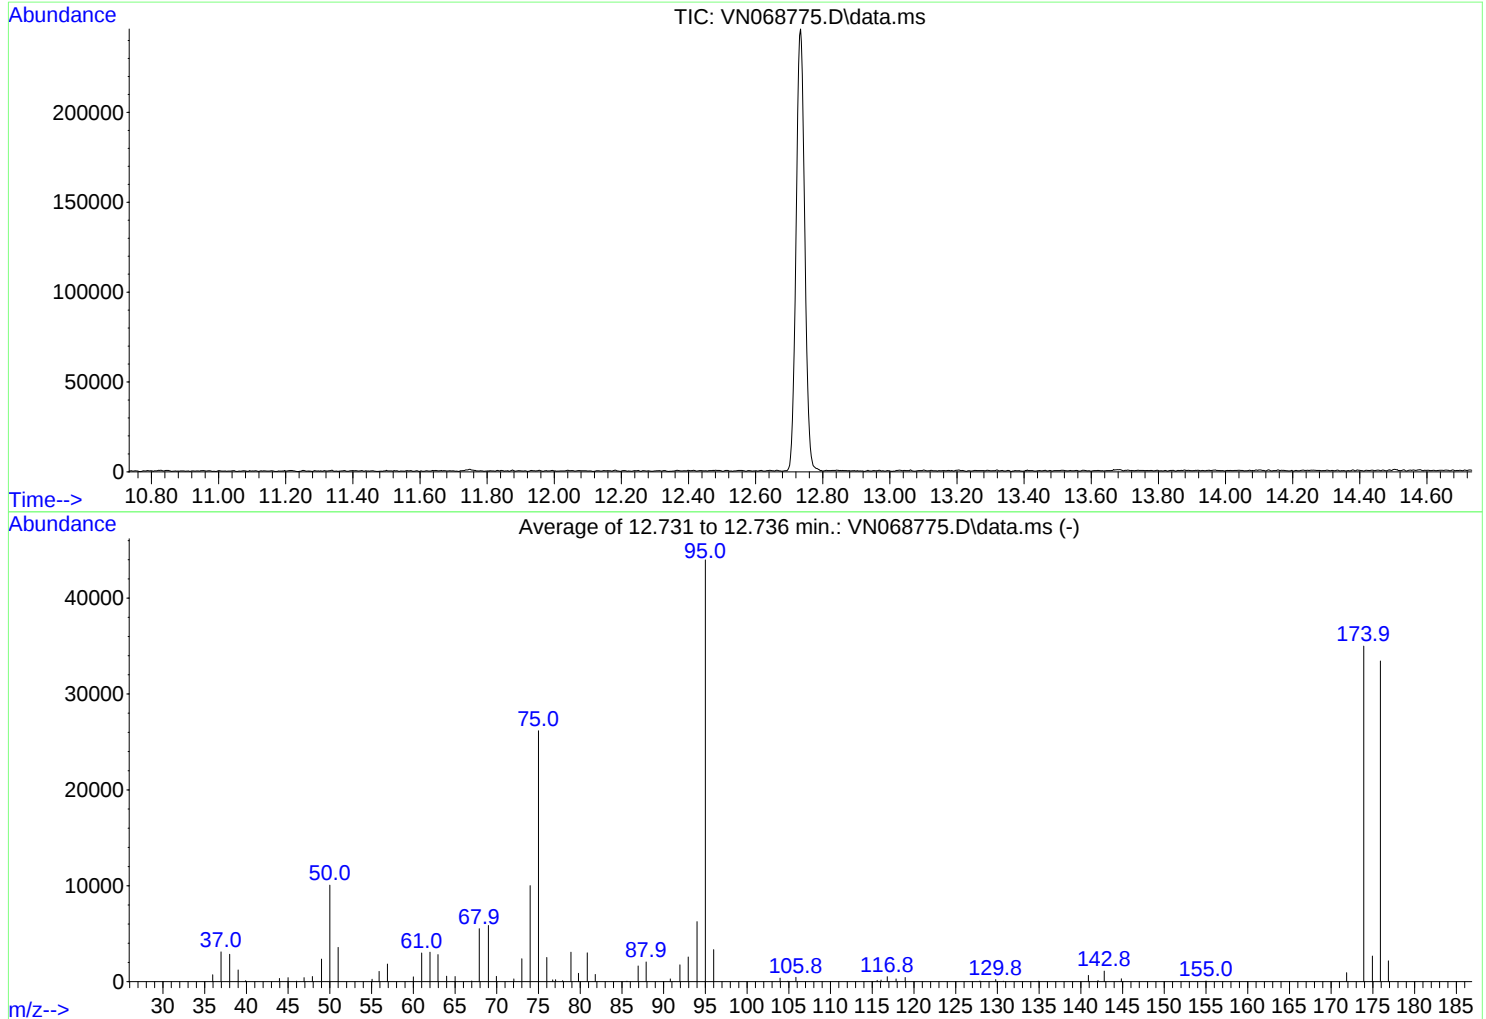

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3989

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	10065	PASS
75	95	30	60	59.5	26168	PASS
95	95	100	100	100.0	43992	PASS
96	95	5	9	7.6	3346	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	79.5	34995	PASS
175	174	5	9	7.6	2676	PASS
176	174	95	101	95.6	33451	PASS
177	176	5	9	6.5	2172	PASS