
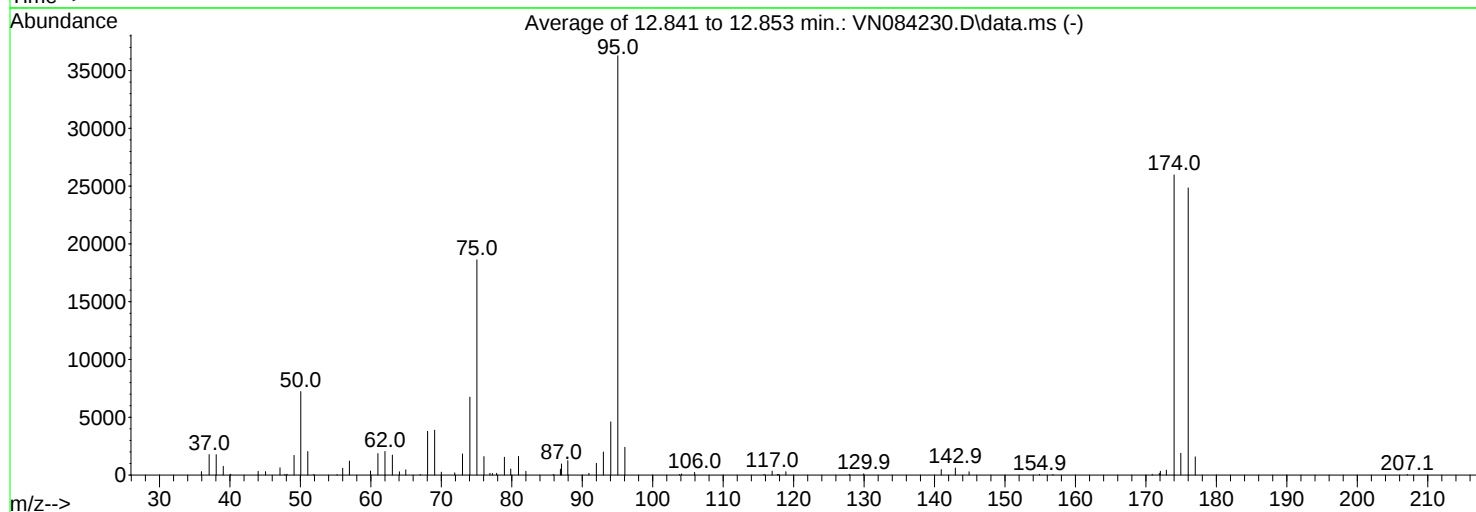


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100124\
Data File : VN084230.D
Acq On : 01 Oct 2024 10:57
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N093024W.M
Title : SW846 8260
Last Update : Tue Oct 01 07:11:01 2024

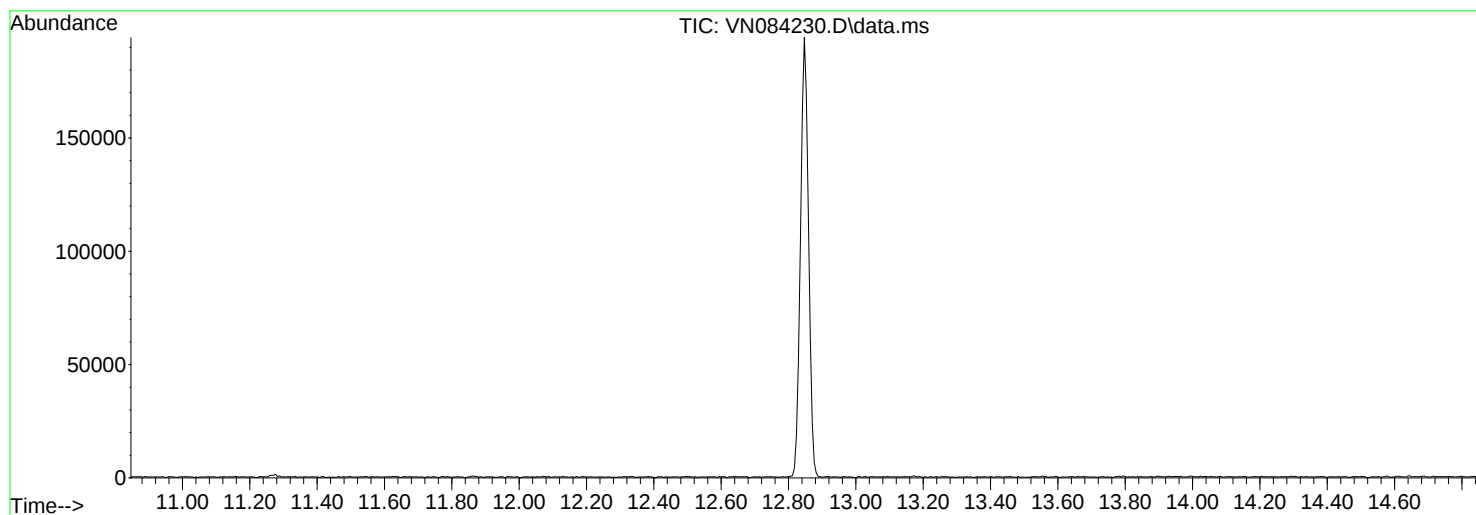

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	7226	PASS
75	95	30	60	51.3	18624	PASS
95	95	100	100	100.0	36280	PASS
96	95	5	9	6.6	2410	PASS
173	174	0.00	2	1.6	427	PASS
174	95	50	100	71.6	25971	PASS
175	174	5	9	7.3	1889	PASS
176	174	95	101	95.7	24848	PASS
177	176	5	9	6.4	1578	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	299	50.05	7226	64.95	453	77.25	141
37.05	1778	51.05	2036	67.00	65	77.85	157
38.05	1767	51.90	53	68.05	3786	78.95	1545
39.05	760	55.20	51	69.05	3882	79.85	529
40.10	76	56.00	597	70.00	259	80.95	1615
44.00	331	56.95	1219	71.90	200	82.00	335
45.05	299	59.95	352	73.00	1833	85.90	55
47.10	627	61.00	1863	74.05	6744	86.90	517
47.80	72	62.00	2044	75.05	18624	87.05	964
48.10	81	63.05	1730	76.05	1604	87.95	1254
49.10	1708	64.05	287	76.90	159	90.95	158

Average of 12.841 to 12.853 min.: VN084230.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.00	1017	117.90	59	172.05	333		
93.00	1995	118.90	292	172.90	427		
94.05	4603	127.90	61	174.00	25971		
95.05	36280	129.95	115	174.95	1889		
96.05	2410	140.95	480	176.00	24848		
103.80	50	142.95	612	177.00	1578		
104.10	99	144.90	290	207.10	53		
105.95	228	154.90	54				
115.80	69	156.80	50				
116.95	344	170.90	70				
117.70	56	171.90	154				