


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100125\
Data File : VN088000.D
Acq On : 01 Oct 2025 08:32
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N092325W.M
Title : SW846 8260
Last Update : Wed Sep 24 05:05:30 2025

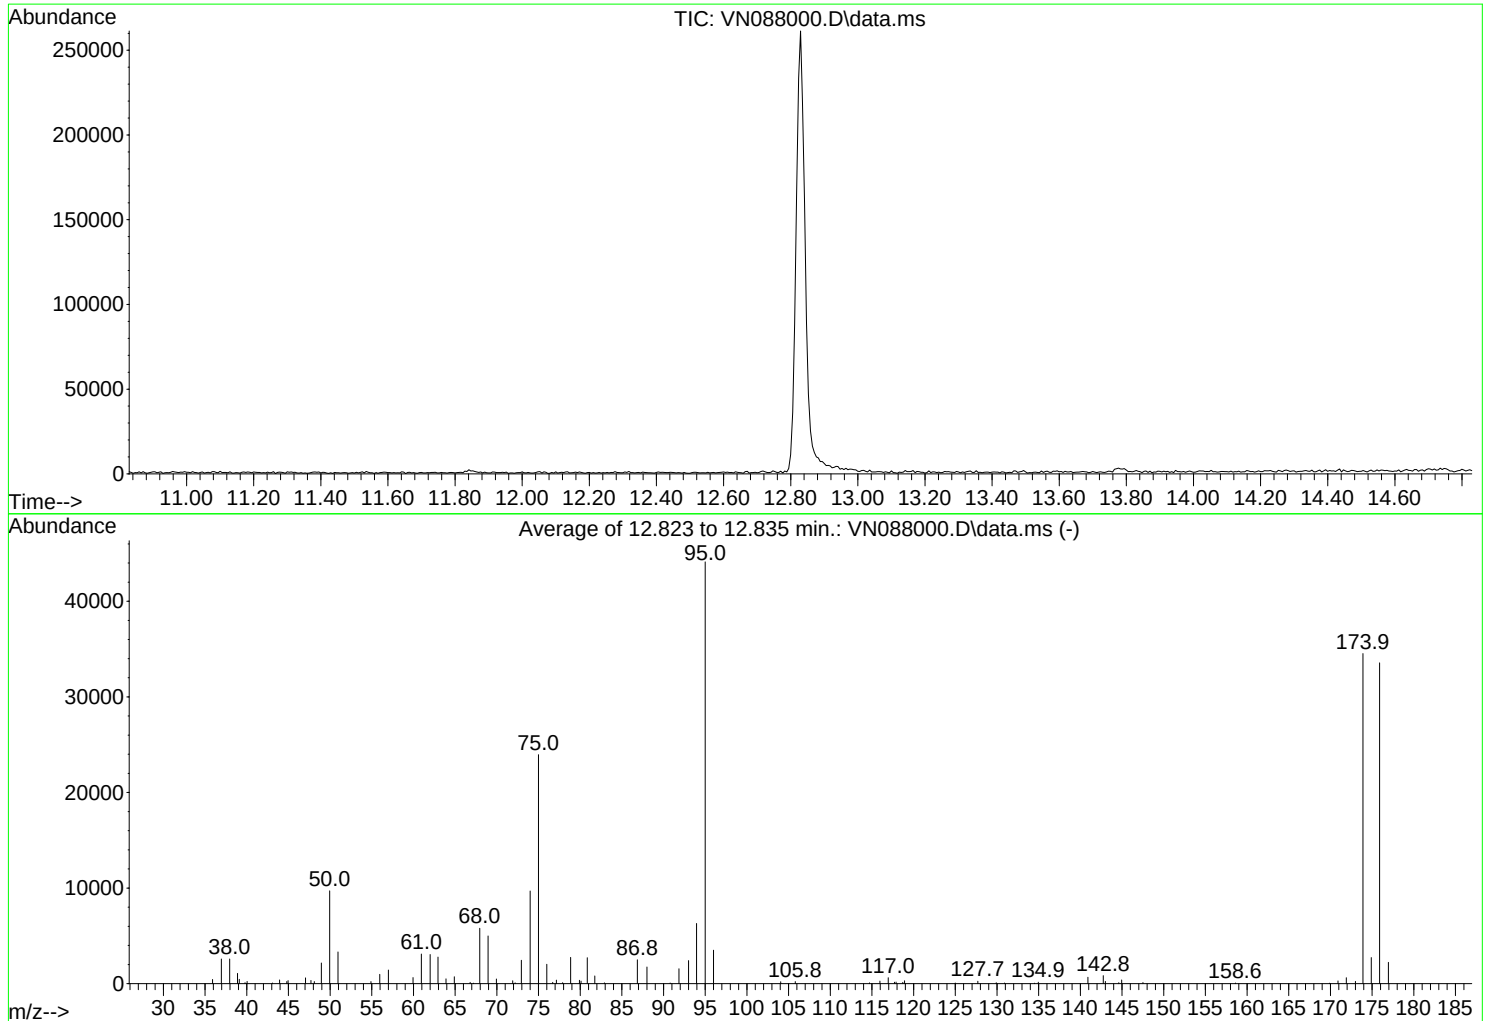

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1838

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.0	9715	PASS
75	95	30	60	54.3	23963	PASS
95	95	100	100	100.0	44128	PASS
96	95	5	9	7.9	3507	PASS
173	174	0.00	2	0.7	241	PASS
174	95	50	100	78.3	34539	PASS
175	174	5	9	7.9	2727	PASS
176	174	95	101	97.2	33557	PASS
177	176	5	9	6.6	2227	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	439	47.05	605	62.00	3050	72.95	244
36.95	2572	47.70	329	62.95	2774	74.00	970
37.95	2574	48.10	216	63.90	505	75.00	2396
38.90	1067	48.95	2152	64.90	720	76.00	202
39.10	452	49.95	9715	66.80	129	76.70	136
39.80	94	50.95	3316	67.20	57	77.15	371
40.05	237	54.90	222	67.95	5798	77.90	94
43.10	65	55.95	970	68.95	4995	78.85	2755
43.95	381	57.00	1424	69.95	478	79.90	344
44.80	223	59.95	637	71.90	295	80.10	271
44.95	327	60.95	3094	72.20	85	80.85	2708

Average of 12.823 to 12.835 min.: VN088000.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.75	803	105.80	221	130.90	70	170.90	285
82.90	90	114.70	92	134.50	52	171.90	619
86.85	2496	115.95	264	134.95	146	173.00	241
88.00	1743	116.95	612	140.90	668	173.90	34539
90.80	62	117.70	155	142.75	839	174.90	2727
91.85	1553	117.90	167	143.00	242	175.90	33557
93.00	2406	118.70	130	144.60	109	176.95	2227
93.95	6297	118.90	299	144.95	387		
95.00	44128	125.00	73	147.50	118		
96.00	3507	127.70	252	158.60	61		
104.05	197	129.90	99	169.90	50		

Instrument :

MSVOA_N

ClientSampleId :

BFB