


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN100219\
Data File : VN058474.D
Acq On : 2 Oct 2019 14:55
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092719W.M
Title : SW846 8260
Last Update : Mon Sep 30 08:07:38 2019

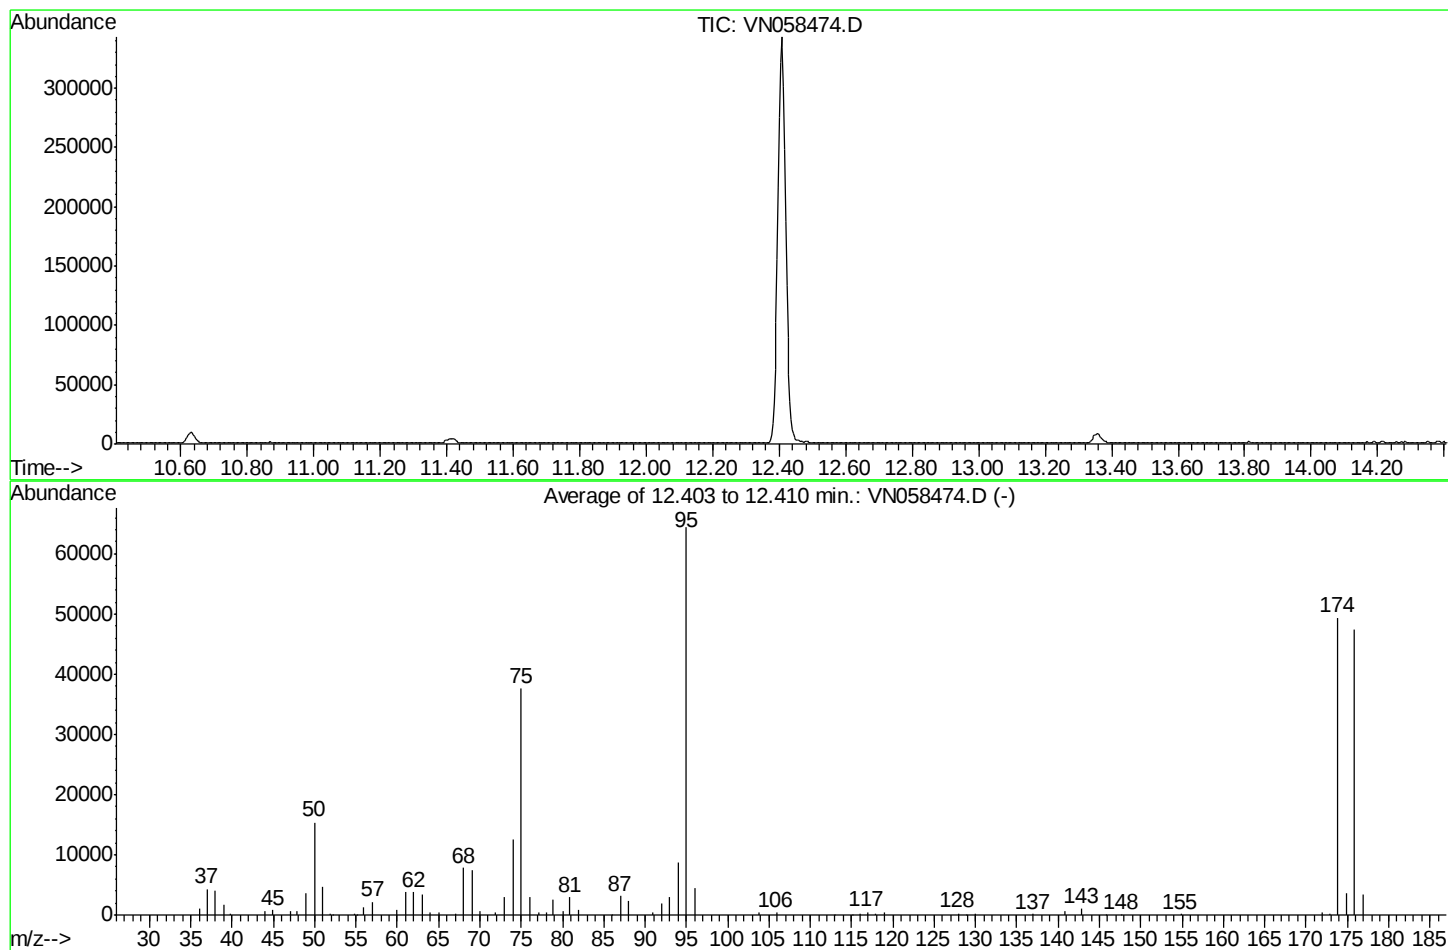

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.9	15403	PASS
75	95	30	60	58.4	37613	PASS
95	95	100	100	100.0	64410	PASS
96	95	5	9	7.1	4576	PASS
173	174	0.00	2	0.3	172	PASS
174	95	50	100	76.7	49413	PASS
175	174	5	9	7.1	3526	PASS
176	174	95	101	95.8	47360	PASS
177	176	5	9	7.0	3333	PASS