

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN100220\
 Data File : VN063820.D
 Acq On : 2 Oct 2020 14:45
 Operator : JC/MD
 Sample : L4183-05DL 5X
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 32676DL

Quant Time: Oct 05 04:15:11 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 01 01:46:38 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	218530	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	416556	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	419463	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	180702	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	184977	51.24	ug/l	0.00
Spiked Amount			Recovery	=	102.48%	
35) Dibromofluoromethane	7.55	113	130242	45.06	ug/l	0.00
Spiked Amount			Recovery	=	90.12%	
50) Toluene-d8	10.06	98	505990	46.18	ug/l	0.00
Spiked Amount			Recovery	=	92.36%	
62) 4-Bromofluorobenzene	12.38	95	212875	51.68	ug/l	0.00
Spiked Amount			Recovery	=	103.36%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
5) Bromomethane	2.54	94	369	0.216	ug/l	93
11) Tert butyl alcohol	4.73	59	140	0.351	ug/l #	71
13) Acrolein	3.57	56	238	0.973	ug/l #	59
16) Acetone	3.78	43	156032	140.398	ug/l	98
17) Carbon Disulfide	4.02	76	916	0.852	ug/l #	76
18) Methyl Acetate	4.29	43	1321	0.458	ug/l #	54
25) 2-Butanone	6.79	43	14973	9.503	ug/l	95
29) Tetrahydrofuran	7.16	42	212	0.201	ug/l #	48
31) Cyclohexane	7.63	56	6407	1.529	ug/l #	19
36) 1,1-Dichloropropene	7.62	75	20493	4.856	ug/l #	45
37) Ethyl Acetate	6.79	43	14973	3.571	ug/l #	70
38) Carbon Tetrachloride	7.62	117	23384	4.941	ug/l #	15
40) Benzene	8.00	78	8170	0.678	ug/l	93
41) Methacrylonitrile	7.15	41	520	0.279	ug/l #	29
52) Toluene	10.13	92	6623	0.888	ug/l	95
57) 1,3-Dichloropropane	10.78	76	1421	0.281	ug/l #	43
59) 2-Hexanone	10.78	43	159381	52.865	ug/l #	42
67) Ethyl Benzene	11.49	91	50861	3.248	ug/l	97
68) m/p-Xylenes	11.59	106	70197	12.030	ug/l	95
69) o-Xylene	11.92	106	23527	4.314	ug/l	98
70) Styrene	11.93	104	1964	0.212	ug/l #	1
74) N-amyl acetate	12.03	43	728	2.329	ug/l #	57
76) 1,2,3-Trichloropropane	12.38	75	121769	30.569	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.38	75	121769	88.044	ug/l #	6
84) 1,2,4-Trimethylbenzene	13.01	105	2217	0.201	ug/l	96
95) Naphthalene	15.10	128	28949	4.779	ug/l	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN100220\
Data File : VN063820.D
Acq On : 2 Oct 2020 14:45
Operator : JC/MD
Sample : L4183-05DL 5X
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
32676DL

Quant Time: Oct 05 04:15:11 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 01 01:46:38 2020
Response via : Initial Calibration

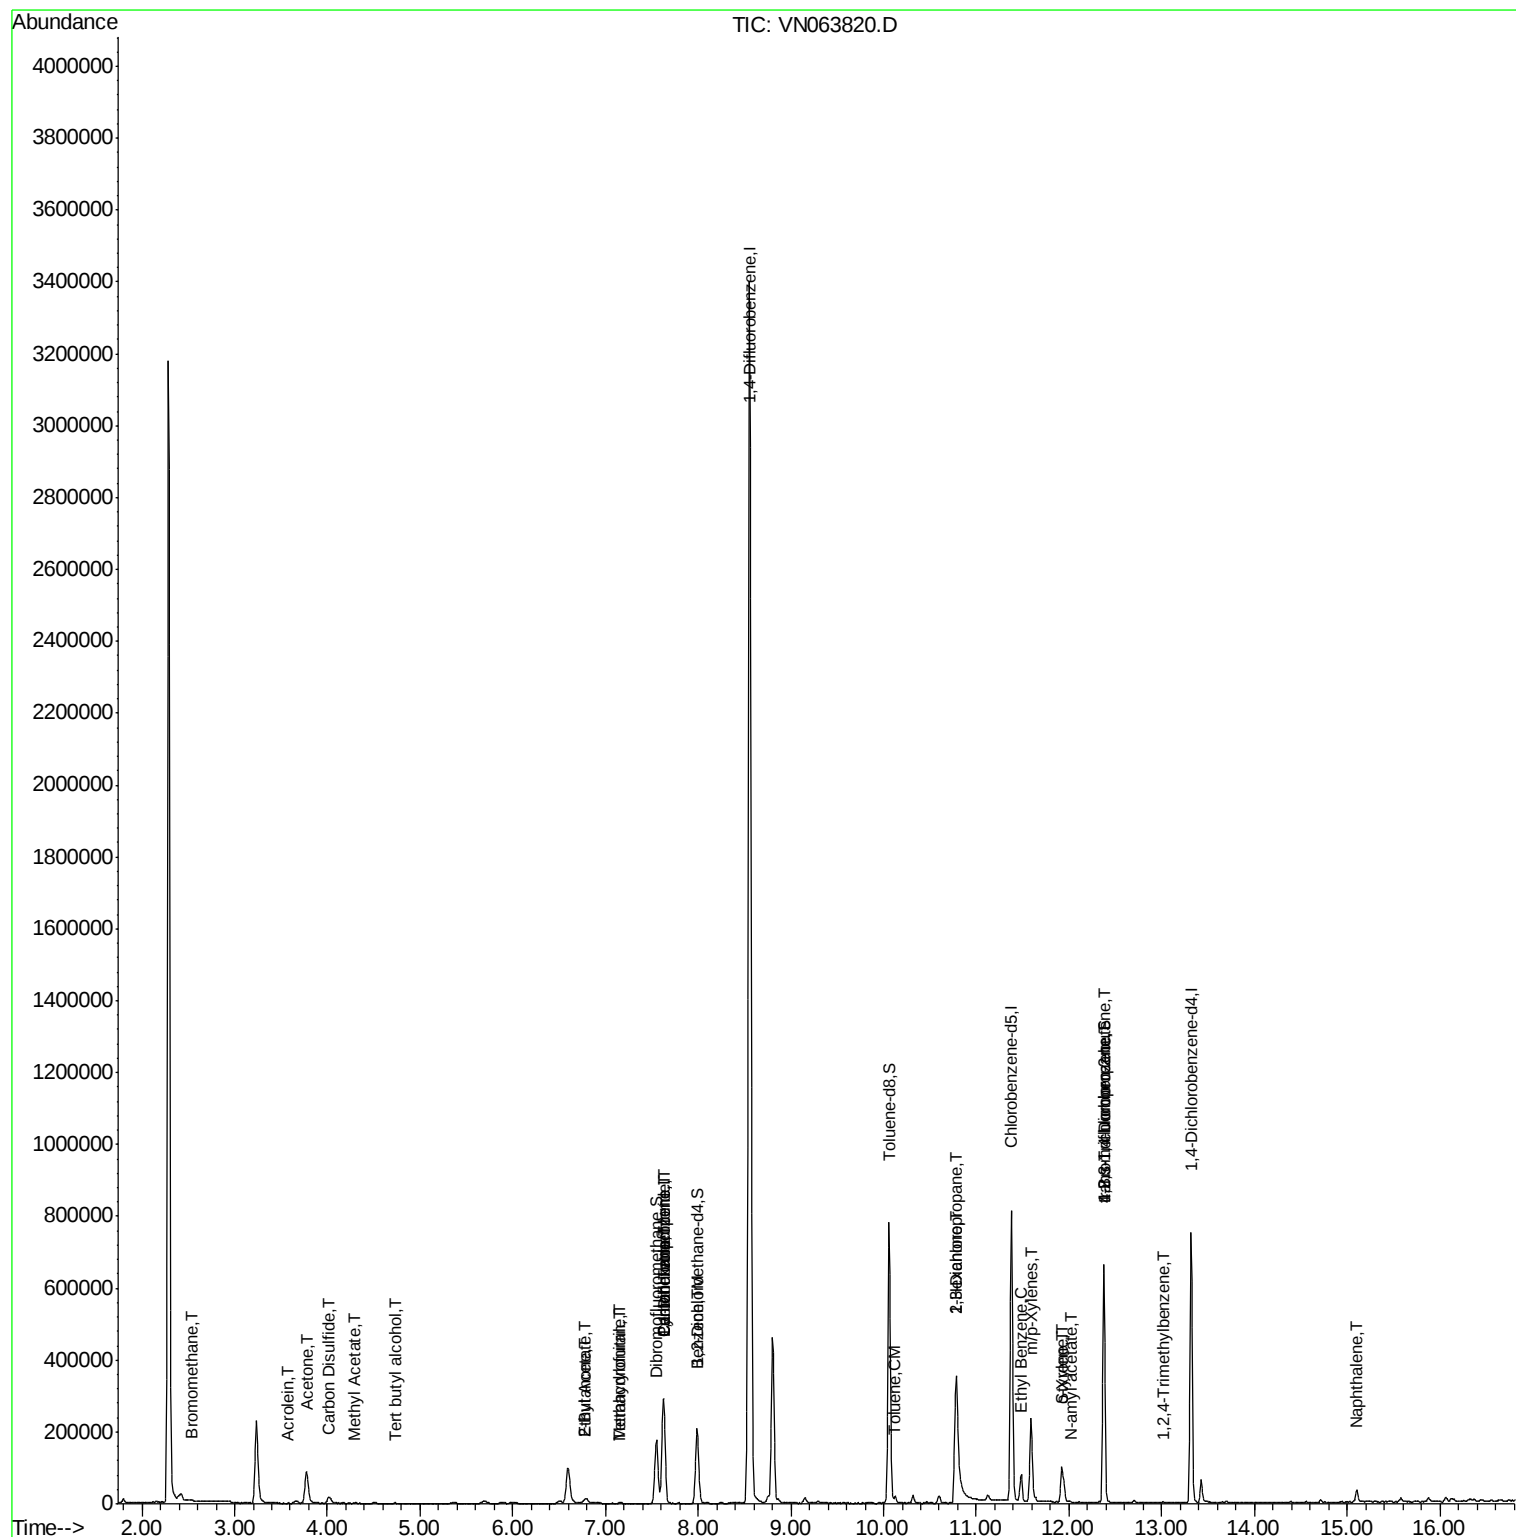



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN063820.D

Acq: 2 Oct 2020 14:45

Instrument :

MSVOA_N

ClientSampleId :


32676DL

Tot Ion:168 Resp: 218530

Ion Ratio Lower Upper

168 100

99 66.9 51.8 77.6



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.63

100000

80000



60000

40000

20000

0

Time--> 7.50 7.60 7.70



#5

Bromomethane

Concen: 0.216 ug/l

RT: 2.54 min Scan# 249

Delta R.T. 0.01 min

Lab File: VN063820.D


Acq: 2 Oct 2020 14:45

Tgt Ion: 94 Resp: 369

Ion Ratio Lower Upper

94 100

96 84.8 73.3 109.9



Abundance Ion 93.90 (93.60 to 94.60): VN

Ion 95.90 (95.60 to 96.60): VN

2.54


300


200

100

0

Time--> 2.52 2.54 2.56







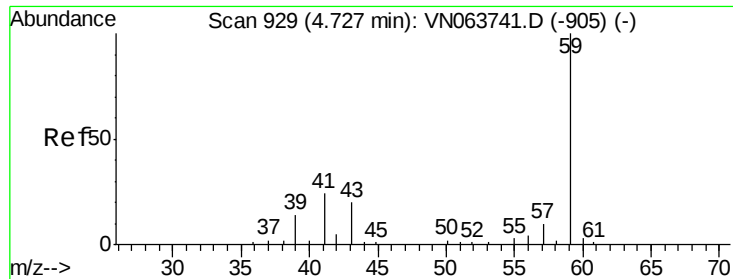

#11
Tert butyl alcohol
Concen: 0.351 ug/l
RT: 4.73 min Scan# 930
Delta R.T. 0.00 min
Lab File: VN063820.D
Acq: 2 Oct 2020 14:45




Instrument :
MSVOA_N
ClientSampleID :
32676DL


Tot Ion: 59 Resp: 140
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#

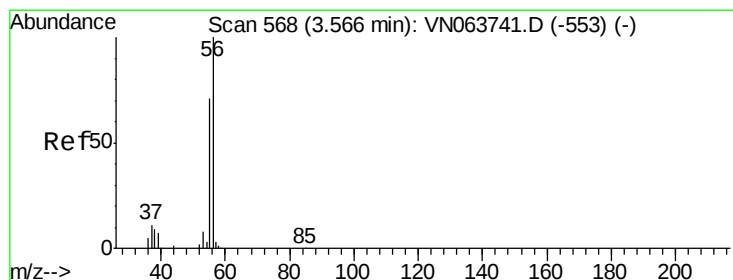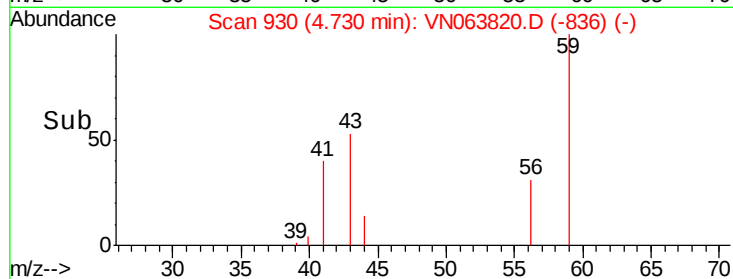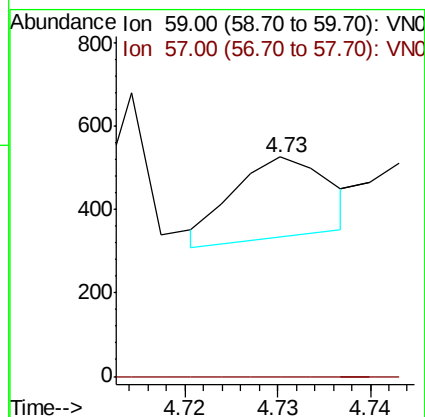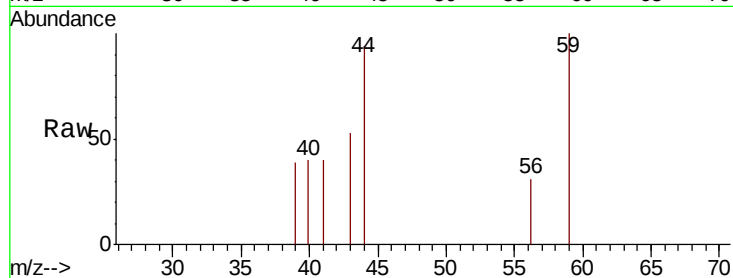

#13
Acrolein
Concen: 0.973 ug/l
RT: 3.57 min Scan# 570
Delta R.T. 0.01 min
Lab File: VN063820.D
Acq: 2 Oct 2020 14:45

Tgt Ion: 56 Resp: 238
Ion Ratio Lower Upper
56 100
55 105.0 56.9 85.3#

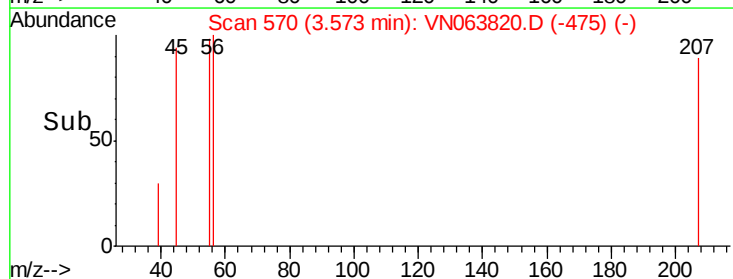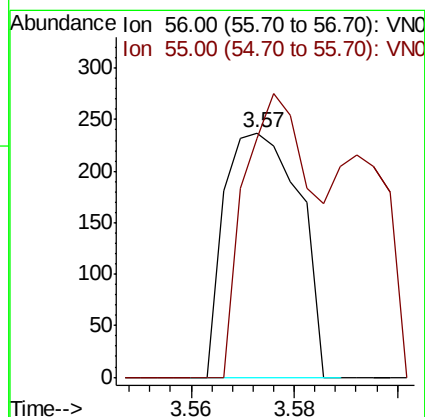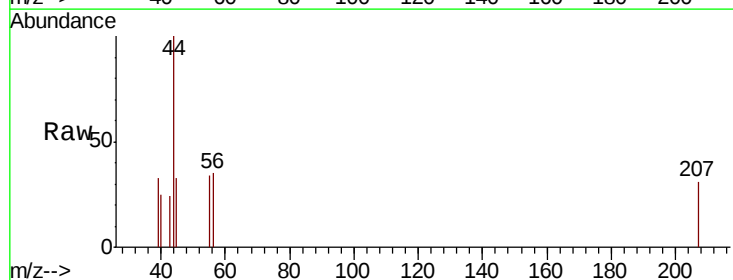



#16

Acetone

Concen: 140.398 ug/l

RT: 3.78 min Scan# 633

Delta R.T. 0.00 min

Lab File: VN063820.D

Acq: 2 Oct 2020 14:45

Instrument :

MSVOA_N

ClientSampled :


32676DL

Tot Ion: 43 Resp: 156032




Ion Ratio Lower Upper

43 100

58 28.9 22.3 33.5



Abundance Ion 43.00 (42.70 to 43.70): VN063741.D (-599) (-)

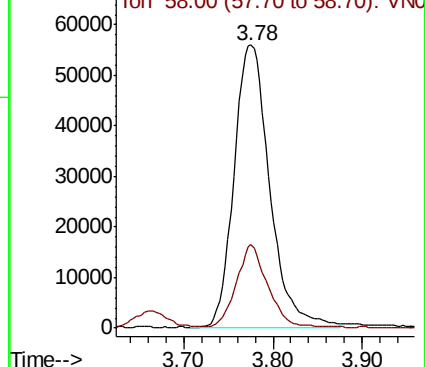

#17

Carbon Disulfide

Concen: 0.852 ug/l

RT: 4.02 min Scan# 708

Delta R.T. 0.00 min

Lab File: VN063820.D


Acq: 2 Oct 2020 14:45

Tgt Ion: 76 Resp: 916



Ion Ratio Lower Upper


76 100

78 0.0 7.0 10.4#



Abundance Ion 75.90 (75.60 to 76.60): VN063741.D (-685) (-)



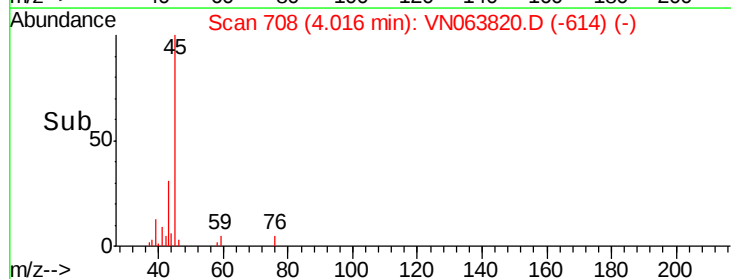
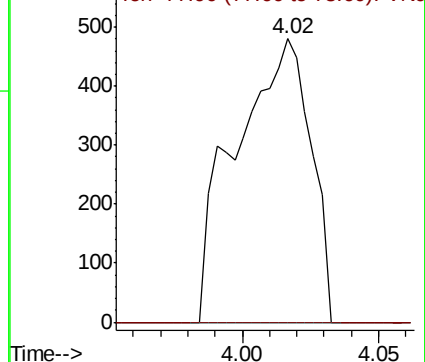


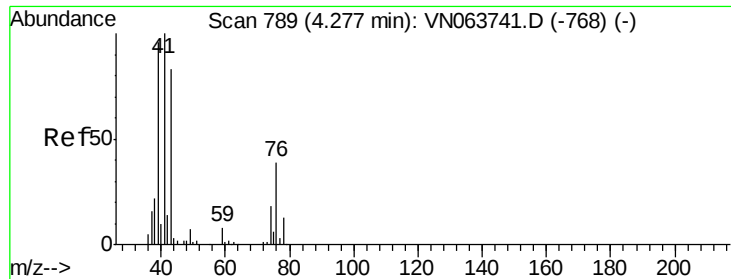

#18
Methyl Acetate
Concen: 0.458 ug/l
RT: 4.29 min Scan# 794
Delta R.T. 0.02 min
Lab File: VN063820.D
Acq: 2 Oct 2020 14:45




Instrument :
MSVOA_N
ClientSampleId :
32676DL


Tot Ion: 43 Resp: 1321
Ion Ratio Lower Upper
43 100
74 0.0 17.4 26.2#

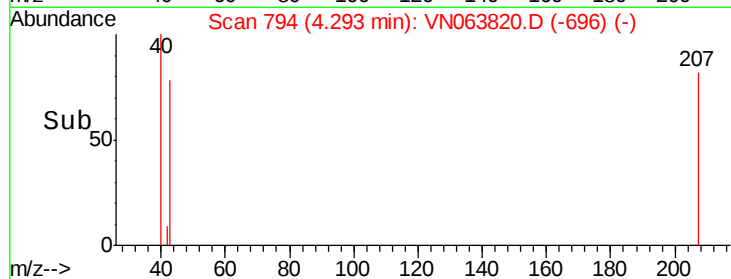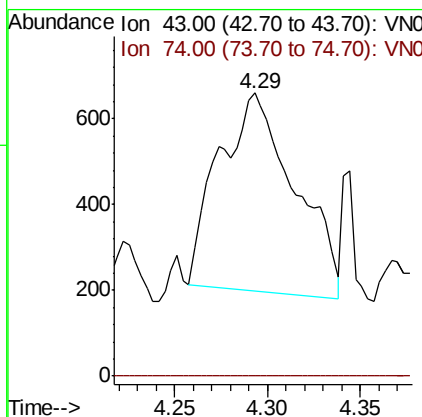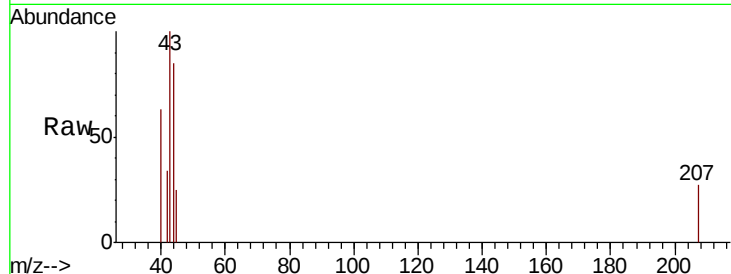

#25
2-Butanone
Concen: 9.503 ug/l
RT: 6.79 min Scan# 1571
Delta R.T. 0.01 min
Lab File: VN063820.D
Acq: 2 Oct 2020 14:45

Tgt Ion: 43 Resp: 14973
Ion Ratio Lower Upper
43 100
72 26.6 19.3 28.9



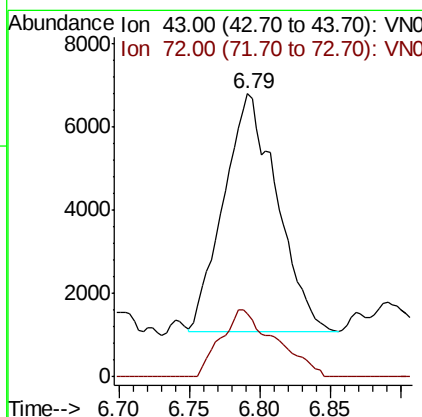



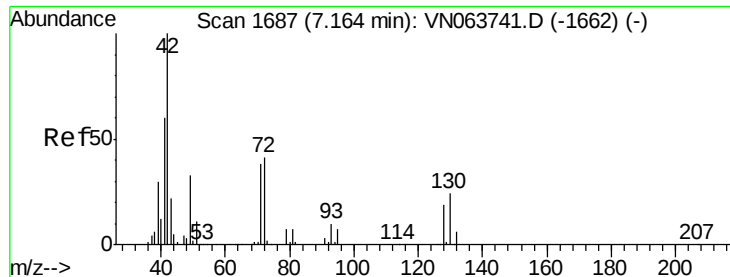

#29
Tetrahydrofuran
Concen: 0.201 ug/l
RT: 7.16 min Scan# 1686
Delta R.T. -0.00 min
Lab File: VN063820.D
Acq: 2 Oct 2020 14:45




Instrument :
MSVOA_N
ClientSampleId :
32676DL


Tot Ion: 42 Resp: 212
Ion Ratio Lower Upper
42 100
72 0.0 32.8 49.2#
71 16.0 30.6 45.8#

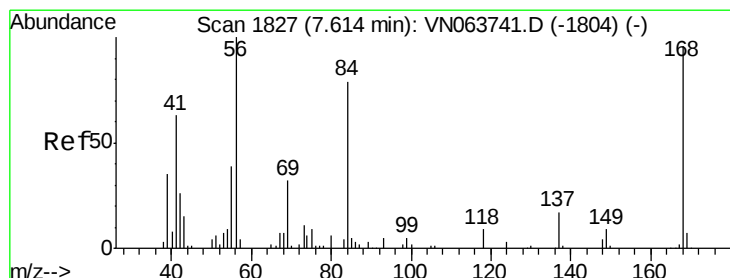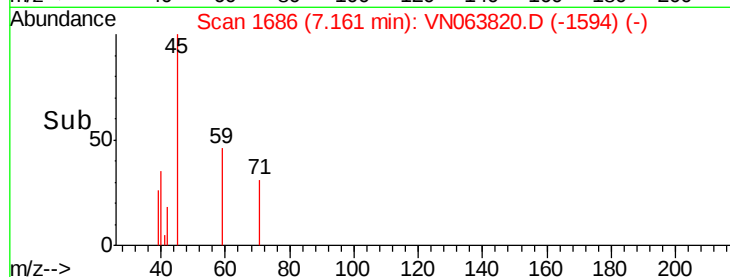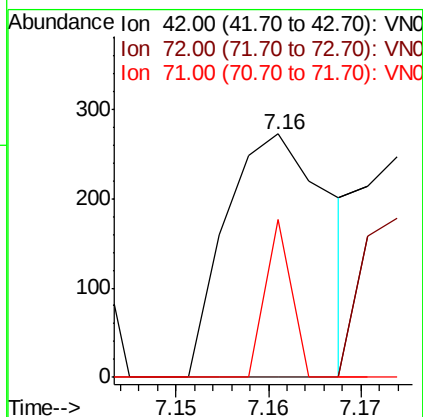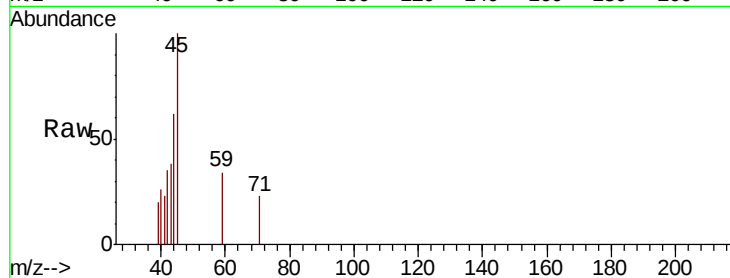

#31
Cyclohexane
Concen: 1.529 ug/l
RT: 7.63 min Scan# 1831
Delta R.T. 0.01 min
Lab File: VN063820.D
Acq: 2 Oct 2020 14:45

Tgt Ion: 56 Resp: 6407
Ion Ratio Lower Upper
56 100
69 158.1 25.4 38.2#
84 98.5 63.3 94.9#


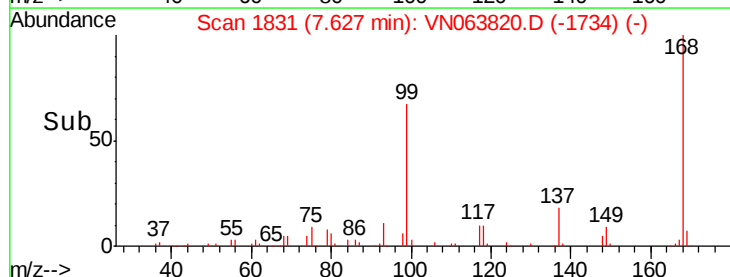
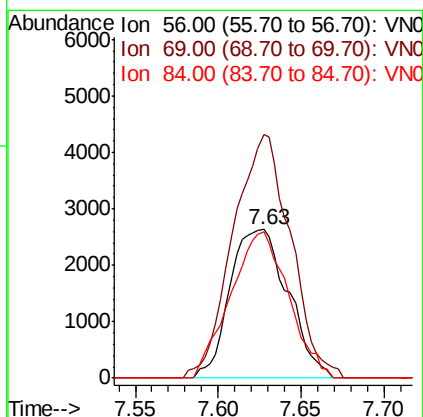
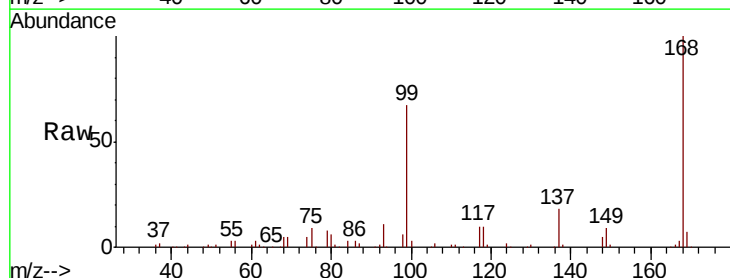


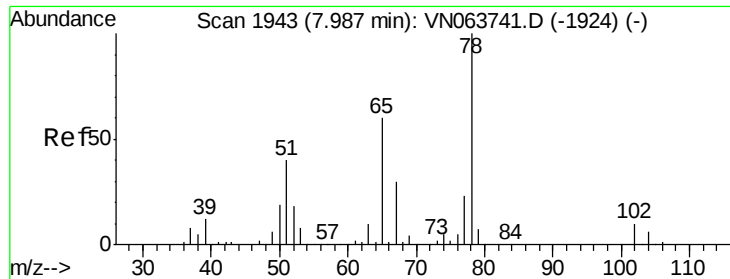

#33
 1,2-Dichloroethane-d4
 Concen: 51.236 ug/l
 RT: 7.99 min Scan# 1943
 Delta R.T. 0.00 min
 Lab File: VN063820.D
 Acq: 2 Oct 2020 14:45




Instrument :
 MSVOA_N
 ClientSampleId :
 32676DL


Tot Ion: 65 Resp: 184977
 Ion Ratio Lower Upper
 65 100
 67 48.6 0.0 99.6

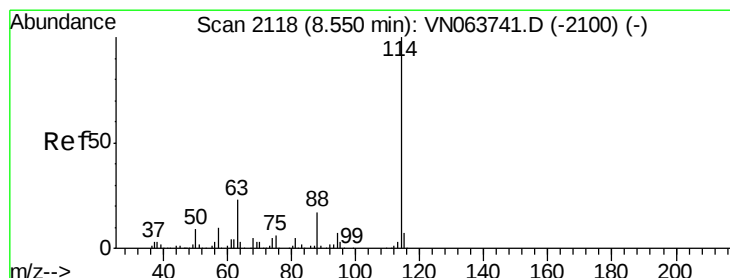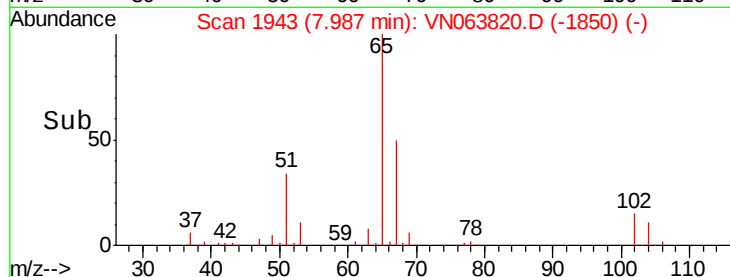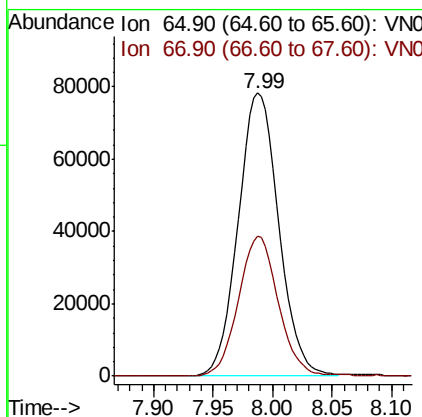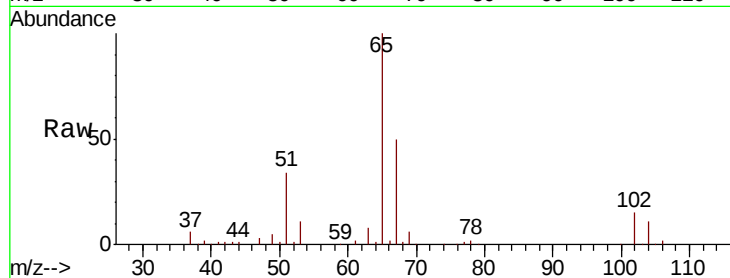

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2118
 Delta R.T. 0.00 min
 Lab File: VN063820.D
 Acq: 2 Oct 2020 14:45

Tgt Ion: 114 Resp: 416556
 Ion Ratio Lower Upper
 114 100
 63 22.5 0.0 45.0
 88 28.8 0.0 34.0


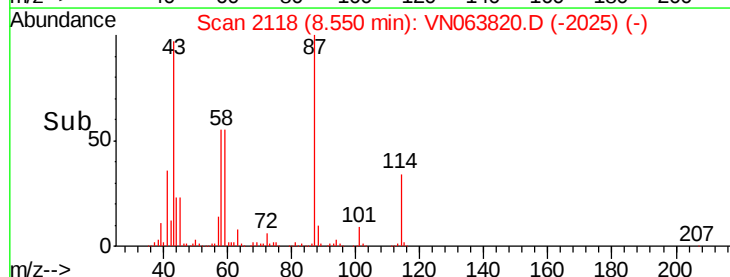
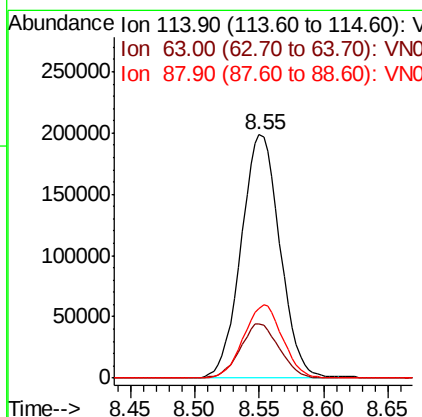
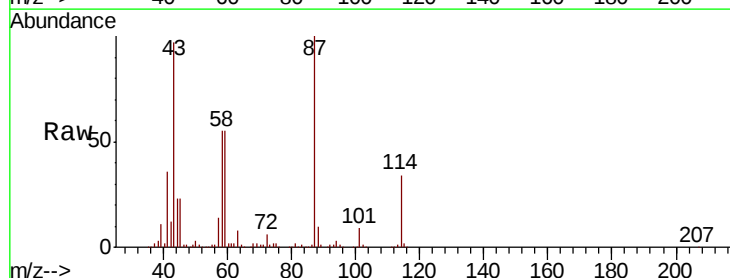




#35
 Dibromofluoromethane
 Concen: 45.060 ug/l
 RT: 7.55 min Scan# 1807
 Delta R.T. 0.00 min
 Lab File: VN063820.D
 Acq: 2 Oct 2020 14:45




Instrument :
 MSVOA_N
 ClientSampleId :
 32676DL


Tot Ion:113 Resp: 130242
 Ion Ratio Lower Upper
 113 100
 111 102.9 81.8 122.8
 192 18.3 14.2 21.2

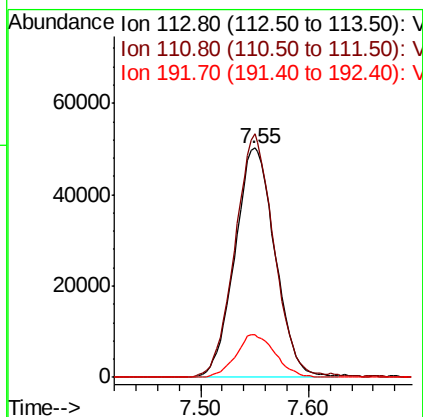

#36
 1,1-Dichloropropene
 Concen: 4.856 ug/l
 RT: 7.62 min Scan# 1830
 Delta R.T. -0.13 min
 Lab File: VN063820.D
 Acq: 2 Oct 2020 14:45

Tgt Ion: 75 Resp: 20493
 Ion Ratio Lower Upper
 75 100
 110 3.1 16.9 50.6#
 77 0.0 24.5 36.7#

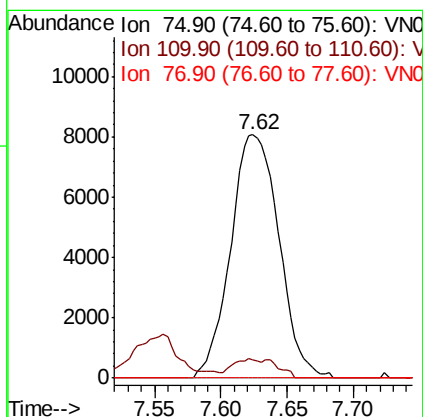

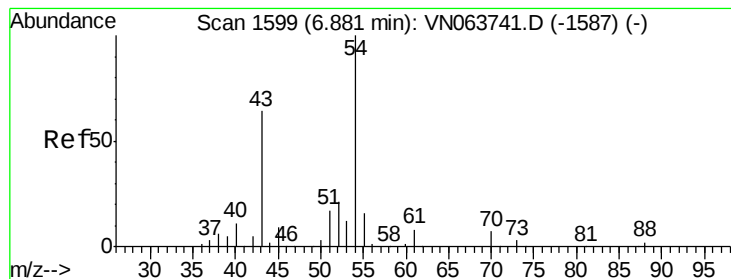

#37

Ethyl Acetate

Concen: 3.571 ug/l

RT: 6.79 min Scan# 1571

Delta R.T. -0.09 min

Lab File: VN063820.D

Acq: 2 Oct 2020 14:45

Instrument :

MSVOA_N

ClientSampleID :

32676DL


Tot Ion: 43 Resp: 14973

Ion Ratio Lower Upper

43 100

61 0.0 10.4 15.6#




70 0.0 7.3 10.9#



Abundance Ion 43.00 (42.70 to 43.70): VN063820.D (-1506) (-)

Ion 60.90 (60.60 to 61.60): VN063820.D (-1506) (-)

Ion 70.00 (69.70 to 70.70): VN063820.D (-1506) (-)

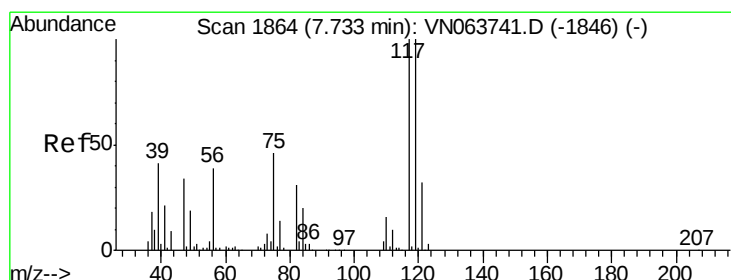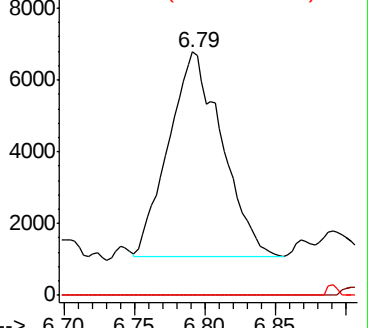

#38

Carbon Tetrachloride

Concen: 4.941 ug/l

RT: 7.62 min Scan# 1829

Delta R.T. -0.11 min

Lab File: VN063820.D

Acq: 2 Oct 2020 14:45


Tgt Ion: 117 Resp: 23384

Ion Ratio Lower Upper

117 100

119 6.8 80.1 120.1#



121 0.0 25.7 38.5#




Abundance Ion 116.80 (116.50 to 117.50): VN063820.D (-1771) (-)

Ion 118.80 (118.50 to 119.50): VN063820.D (-1771) (-)

Ion 120.80 (120.50 to 121.50): VN063820.D (-1771) (-)

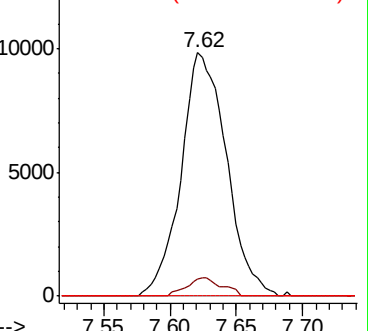

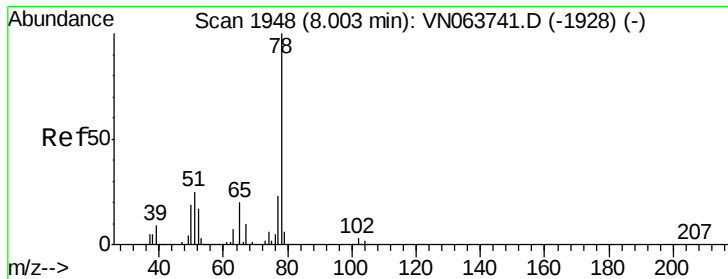

#40

Benzene

Concen: 0.678 ug/l

RT: 8.00 min Scan# 1948

Delta R.T. 0.00 min

Lab File: VN063820.D

Acq: 2 Oct 2020 14:45

Instrument :

MSVOA_N

ClientSampleId :


32676DL

Tot Ion: 78 Resp: 8170




Ion Ratio Lower Upper

78 100

77 20.1 18.7 28.1

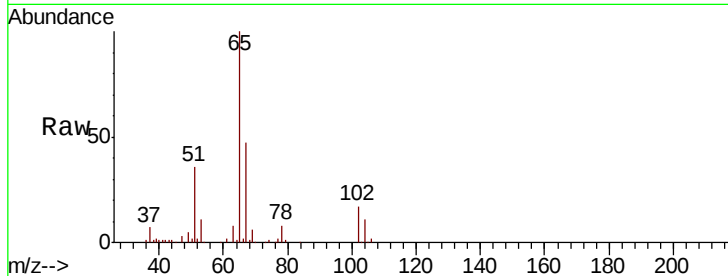

Abundance Ion 78.00 (77.70 to 78.70): VN063741.D (-1928) (-)

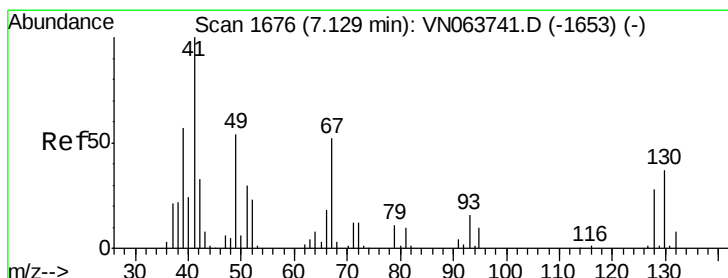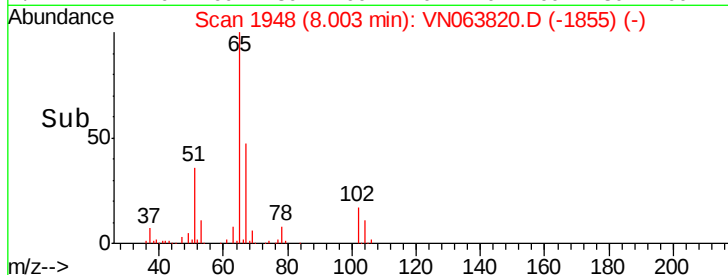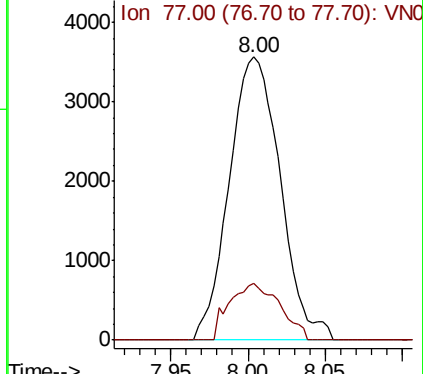

#41

Methacrylonitrile

Concen: 0.279 ug/l

RT: 7.15 min Scan# 1683

Delta R.T. 0.02 min

Lab File: VN063820.D

Acq: 2 Oct 2020 14:45

Tgt Ion: 41 Resp: 520


Ion Ratio Lower Upper

41 100



39 11.5 42.5 63.7#


67 0.0 57.4 86.2#

52 0.0 26.9 40.3#

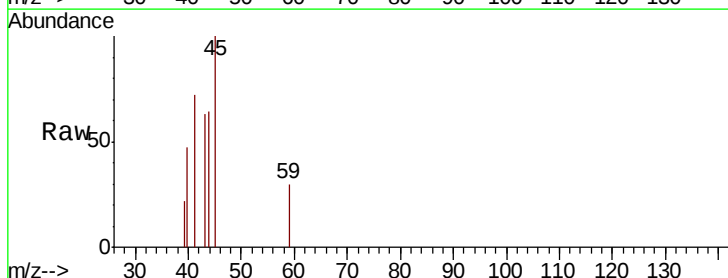

Abundance Ion 41.00 (40.70 to 41.70): VN063741.D (-1653) (-)

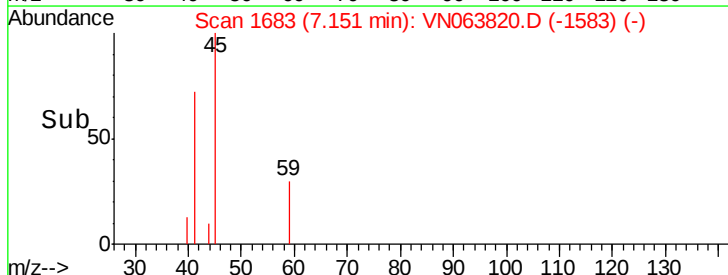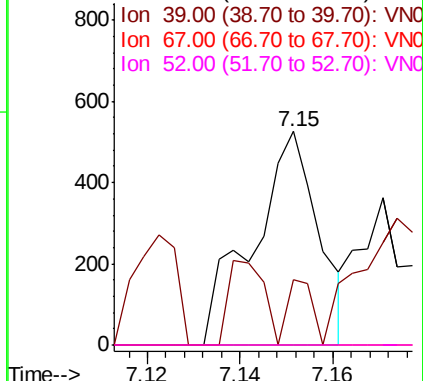

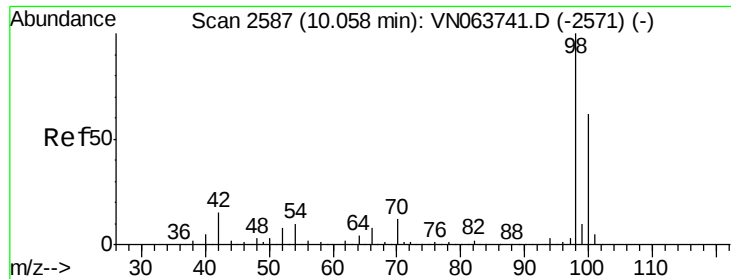

#50

Toluene-d8

Concen: 46.179 ug/l

RT: 10.06 min Scan# 2587

Delta R.T. 0.00 min

Lab File: VN063820.D

Acq: 2 Oct 2020 14:45

Instrument :

MSVOA_N

ClientSampled :


32676DL

Tot Ion: 98 Resp: 505990

Ion Ratio Lower Upper

98 100

100 64.0 49.8 74.6



Abundance Ion 98.00 (97.70 to 98.70): VN063741.D (-2571) (-)

Ion 100.00 (99.70 to 100.70): VN063741.D (-2571) (-)

10.06

250000

200000



150000

100000

50000

0

Time-->



#52

Toluene

Concen: 0.888 ug/l

RT: 10.13 min Scan# 2608

Delta R.T. 0.00 min

Lab File: VN063820.D


Acq: 2 Oct 2020 14:45

Tgt Ion: 92 Resp: 6623

Ion Ratio Lower Upper

92 100

91 169.3 140.6 210.8



Abundance Ion 92.00 (91.70 to 92.70): VN063741.D (-2592) (-)

Ion 91.00 (90.70 to 91.70): VN063741.D (-2592) (-)


6000


4000

2000

0

Time-->







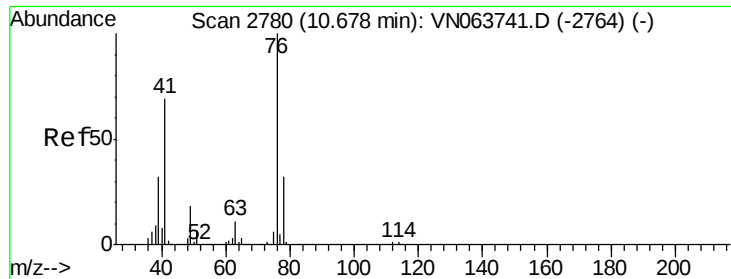

#57
 1,3-Dichloropropane
 Concen: 0.281 ug/l
 RT: 10.78 min Scan# 2813
 Delta R.T. 0.11 min
 Lab File: VN063820.D
 Acq: 2 Oct 2020 14:45




Instrument :
 MSVOA_N
 ClientSampled :
 32676DL


Tot Ion: 76 Resp: 1421
 Ion Ratio Lower Upper
 76 100
 78 0.0 25.2 37.8#

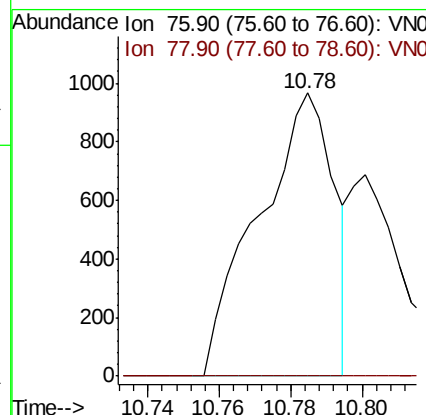

#59
 2-Hexanone
 Concen: 52.865 ug/l
 RT: 10.78 min Scan# 2813
 Delta R.T. 0.06 min
 Lab File: VN063820.D
 Acq: 2 Oct 2020 14:45

Tgt Ion: 43 Resp: 159381
 Ion Ratio Lower Upper
 43 100
 58 9.7 24.6 73.8#


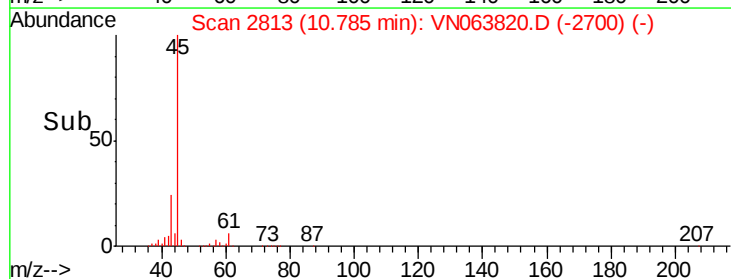
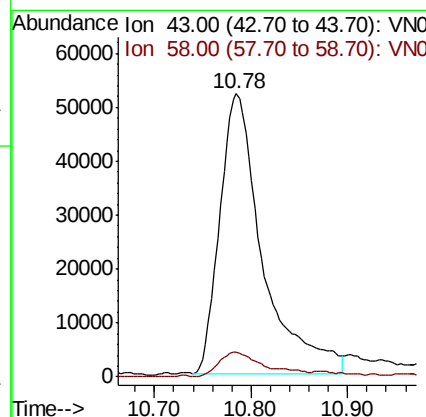



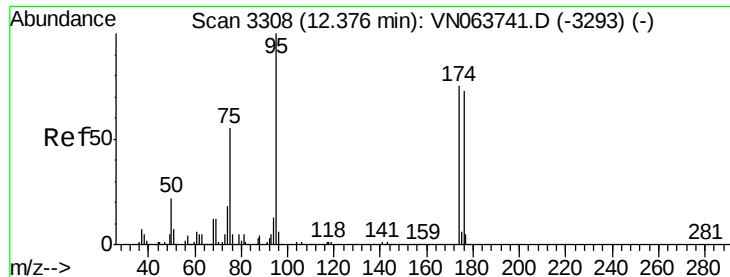

#62
4-Bromofluorobenzene
Concen: 51.683 ug/l
RT: 12.38 min Scan# 3308
Delta R.T. 0.00 min
Lab File: VN063820.D
Acq: 2 Oct 2020 14:45




Instrument :
MSVOA_N
ClientSampleId :
32676DL


Tot Ion: 95 Resp: 212875
Ion Ratio Lower Upper
95 100
174 75.2 0.0 150.6
176 71.6 0.0 145.4

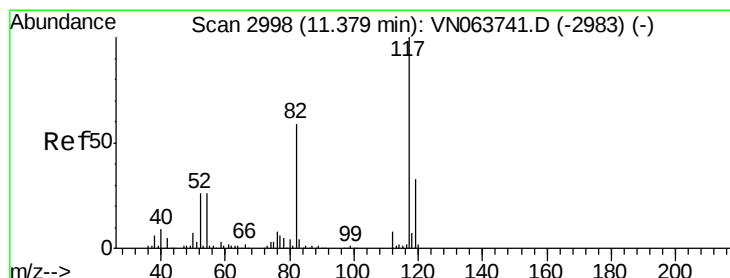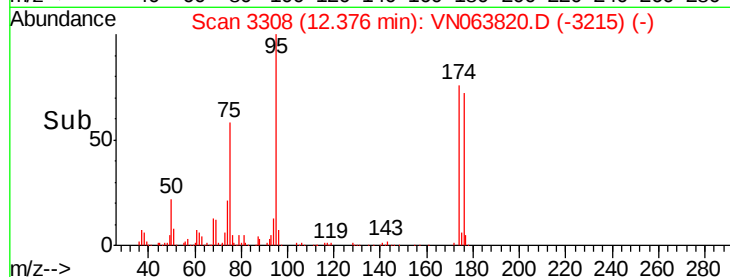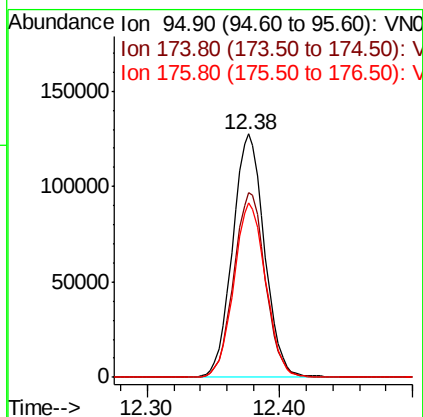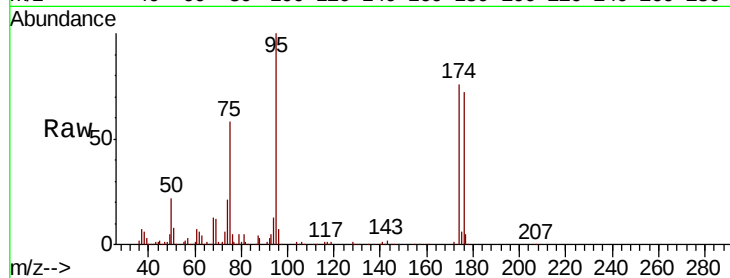

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2998
Delta R.T. 0.00 min
Lab File: VN063820.D
Acq: 2 Oct 2020 14:45

Tgt Ion: 117 Resp: 419463
Ion Ratio Lower Upper
117 100
82 59.8 47.4 71.2
119 31.9 26.4 39.6


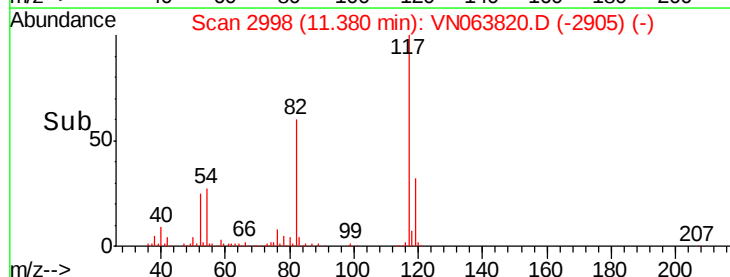
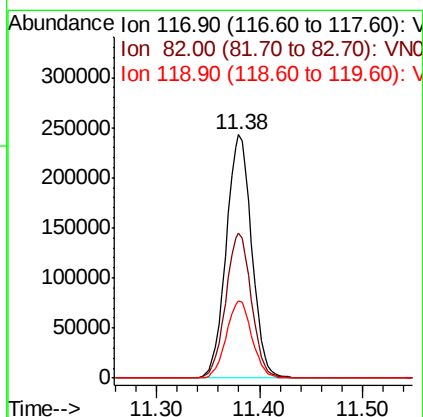
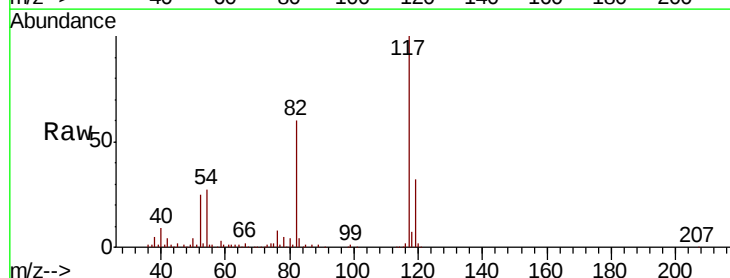


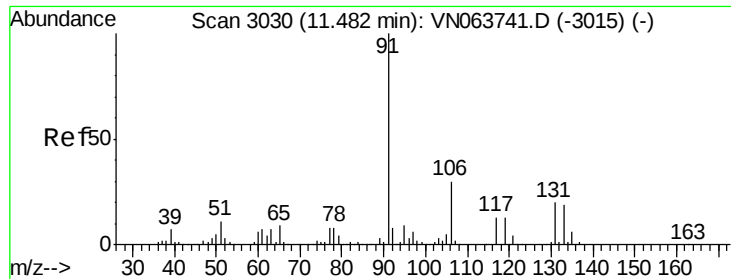

#67
Ethyl Benzene
Concen: 3.248 ug/l
RT: 11.49 min Scan# 3031
Delta R.T. 0.00 min
Lab File: VN063820.D
Acq: 2 Oct 2020 14:45




Instrument :
MSVOA_N
ClientSampleID :
32676DL


Tot Ion: 91 Resp: 50861
Ion Ratio Lower Upper
91 100
106 31.7 24.2 36.2

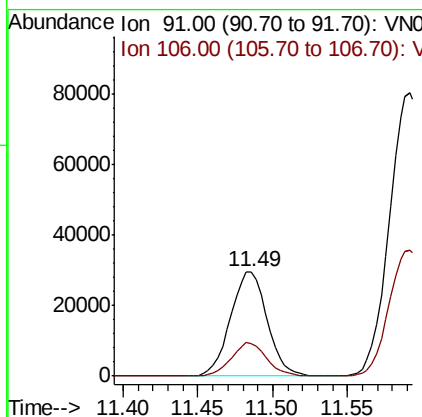

#68
m/p-Xylenes
Concen: 12.030 ug/l
RT: 11.59 min Scan# 3064
Delta R.T. -0.00 min
Lab File: VN063820.D
Acq: 2 Oct 2020 14:45

Tgt Ion: 106 Resp: 70197
Ion Ratio Lower Upper
106 100
91 217.9 168.0 252.0



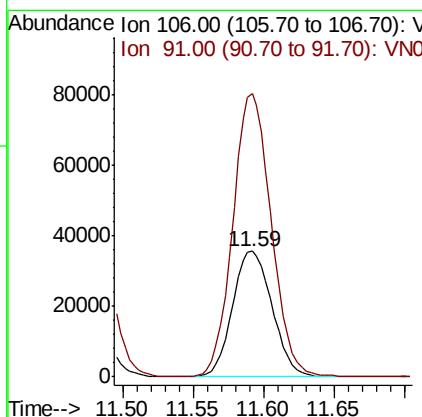





#69
o-Xylene
Concen: 4.314 ug/l
RT: 11.92 min Scan# 3166
Delta R.T. 0.00 min
Lab File: VN063820.D
Acq: 2 Oct 2020 14:45




Instrument :
MSVOA_N
ClientSampled :
32676DL


Tot Ion:106 Resp: 23527
Ion Ratio Lower Upper
106 100
91 228.8 112.7 338.0

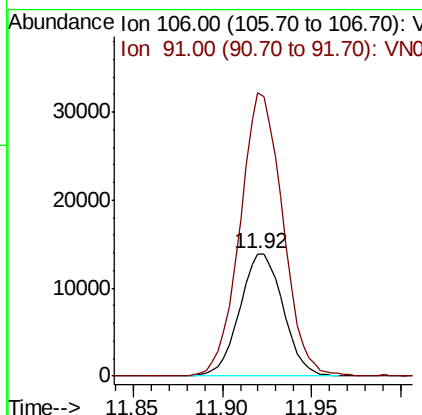

#70
Styrene
Concen: 0.212 ug/l
RT: 11.93 min Scan# 3169
Delta R.T. -0.01 min
Lab File: VN063820.D
Acq: 2 Oct 2020 14:45

Tgt Ion:104 Resp: 1964
Ion Ratio Lower Upper
104 100
78 220.4 44.1 66.1#
103 186.8 44.3 66.5#

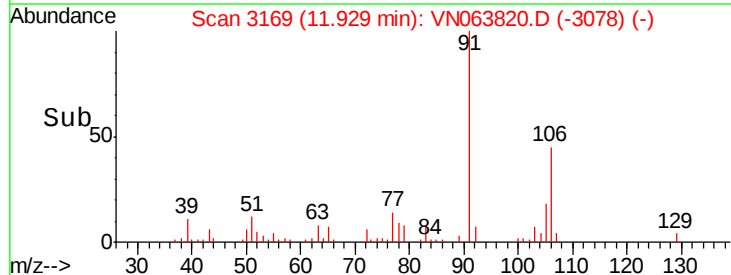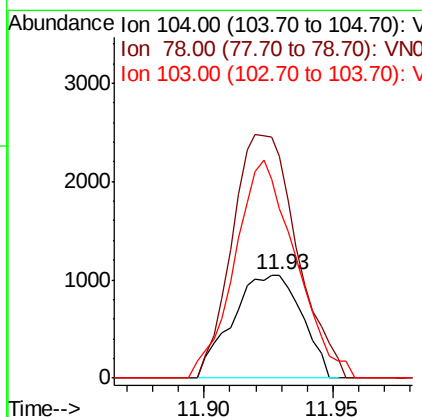



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3601

Delta R.T. 0.00 min

Lab File: VN063820.D

Acq: 2 Oct 2020 14:45

Instrument :

MSVOA_N

ClientSampleId :

32676DL


Tot Ion:152 Resp: 180702

Ion Ratio Lower Upper

152 100

115 63.5 31.3 93.8

150 158.9 0.0 341.8






Abundance

Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

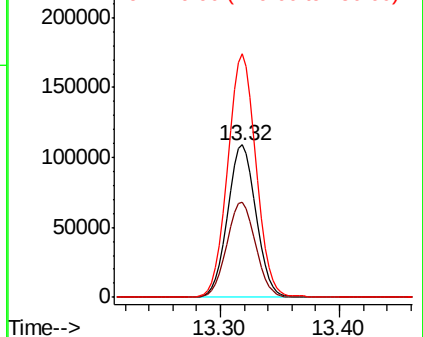

#74

N-ethyl acetate

Concen: 2.329 ug/l

RT: 12.03 min Scan# 3201

Delta R.T. -0.01 min

Lab File: VN063820.D

Acq: 2 Oct 2020 14:45

Tgt Ion: 43 Resp: 728


Ion Ratio Lower Upper

43 100

70 0.0 29.8 44.8#

55 0.0 17.9 26.9#

61 23.6 17.0 25.4





Abundance


Ion 43.00 (42.70 to 43.70): V

Ion 70.00 (69.70 to 70.70): V

Ion 55.00 (54.70 to 55.70): V

Ion 61.00 (60.70 to 61.70): V

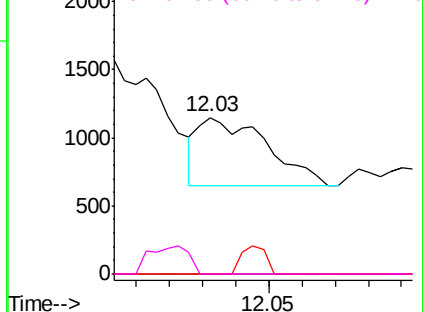



#76

1,2,3-Trichloropropane

Concen: 30.569 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. -0.15 min

Lab File: VN063820.D

Acq: 2 Oct 2020 14:45

Instrument :

MSVOA_N

ClientSampleId :


32676DL

Tot Ion: 75 Resp: 121769

Ion Ratio Lower Upper




75 100

77 1.0 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 77.00 (76.70 to 77.70): VN0

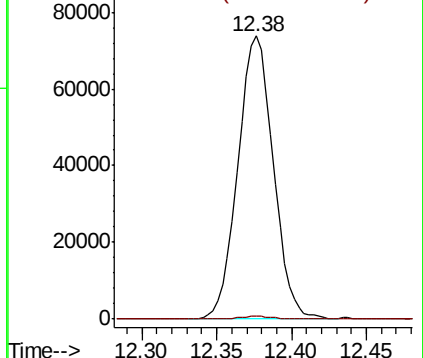

#81

trans-1,4-Dichloro-2-butene

Concen: 88.044 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. 0.10 min

Lab File: VN063820.D

Acq: 2 Oct 2020 14:45


Tgt Ion: 75 Resp: 121769

Ion Ratio Lower Upper

75 100

53 0.0 88.2 132.2#



89 0.0 36.0 54.0#




Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 53.00 (52.70 to 53.70): VN0

Ion 88.90 (88.60 to 89.60): VN0




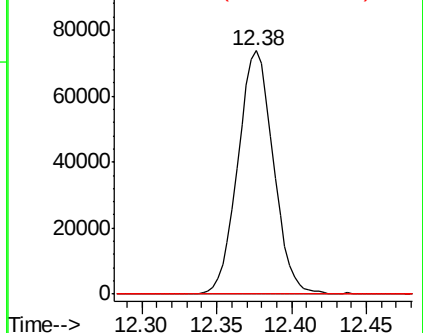


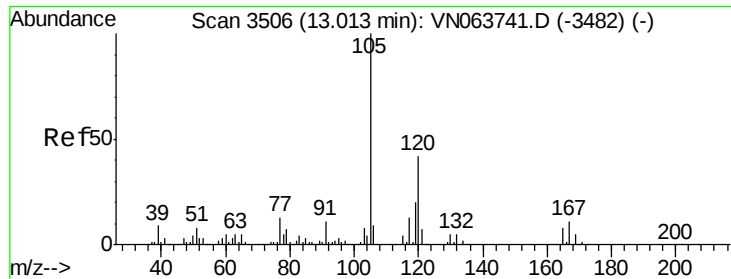

#84
 1,2,4-Trimethylbenzene
 Concen: 0.201 ug/l
 RT: 13.01 min Scan# 3506
 Delta R.T. 0.00 min
 Lab File: VN063820.D
 Acq: 2 Oct 2020 14:45

Instrument :
 MSVOA_N
 ClientSampleId :
 32676DL

Tot Ion:105 Resp: 2217
 Ion Ratio Lower Upper
 105 100
 120 39.4 20.9 62.7

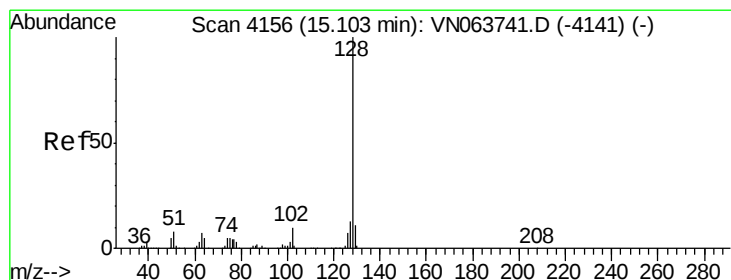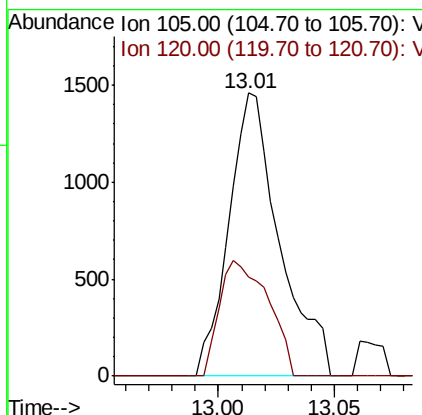

#95
 Naphthalene
 Concen: 4.779 ug/l
 RT: 15.10 min Scan# 4156
 Delta R.T. 0.00 min
 Lab File: VN063820.D
 Acq: 2 Oct 2020 14:45

Tgt Ion:128 Resp: 28949
 Ion Ratio Lower Upper
 128 100
 127 14.0 10.5 15.7
 129 11.8 8.7 13.1

