

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN100220\
 Data File : VN063824.D
 Acq On : 2 Oct 2020 16:20
 Operator : JC/MD
 Sample : PB132030ZHE#03
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB132030ZHE#03


Quant Time: Oct 05 04:16:21 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 01 01:46:38 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	212395	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	396662	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	416355	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	168630	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	184807	52.67	ug/l	0.00
Spiked Amount			Recovery	=	105.34%	
35) Dibromofluoromethane	7.55	113	129990	47.23	ug/l	0.00
Spiked Amount			Recovery	=	94.46%	
50) Toluene-d8	10.06	98	515835	49.44	ug/l	0.00
Spiked Amount			Recovery	=	98.88%	
62) 4-Bromofluorobenzene	12.38	95	207710	52.96	ug/l	0.00
Spiked Amount			Recovery	=	105.92%	

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Tert butyl alcohol	4.72	59	1275	3.291	ug/l #	94
13) Acrolein	3.69	56	59	0.248	ug/l #	14
16) Acetone	3.78	43	19124	17.705	ug/l	96
17) Carbon Disulfide	4.01	76	82	0.715	ug/l #	76
18) Methyl Acetate	4.28	43	2034	0.725	ug/l #	60
20) Methylene Chloride	4.50	84	20445	8.345	ug/l	88
25) 2-Butanone	6.79	43	15330	10.010	ug/l	99
29) Tetrahydrofuran	7.17	42	2228	2.169	ug/l #	59
31) Cyclohexane	7.63	56	6508	1.598	ug/l #	41
36) 1,1-Dichloropropene	7.62	75	19135	4.762	ug/l #	53
37) Ethyl Acetate	6.79	43	15330	3.840	ug/l #	71
38) Carbon Tetrachloride	7.63	117	22648	5.026	ug/l #	15
41) Methacrylonitrile	7.18	41	1296	0.730	ug/l #	25
43) Isopropyl Acetate	8.13	43	67659	10.274	ug/l	97
45) 1,2-Dichloropropane	9.23	63	1174	0.379	ug/l #	44
48) Methyl methacrylate	9.15	41	5946	1.827	ug/l #	12
49) 1,4-Dioxane	9.24	88	65	1.406	ug/l #	1
51) 4-Methyl-2-Pentanone	9.95	43	8821	2.282	ug/l	92
54) cis-1,3-Dichloropropene	9.87	75	26614	5.387	ug/l #	67
56) Ethyl methacrylate	10.52	69	1926	0.477	ug/l #	1
57) 1,3-Dichloropropane	10.74	76	4523	0.939	ug/l #	43
59) 2-Hexanone	10.74	43	77135	26.868	ug/l #	59
74) N-amyl acetate	12.01	43	5896	3.202	ug/l #	49
76) 1,2,3-Trichloropropane	12.38	75	116338	31.297	ug/l #	100
80) 1,3,5-Trimethylbenzene	12.71	105	2714	0.263	ug/l	98
81) trans-1,4-Dichloro-2-buten	12.38	75	116338	90.139	ug/l #	6

(#) = qualifier out of range (m) = manual integration (+) = signals summed

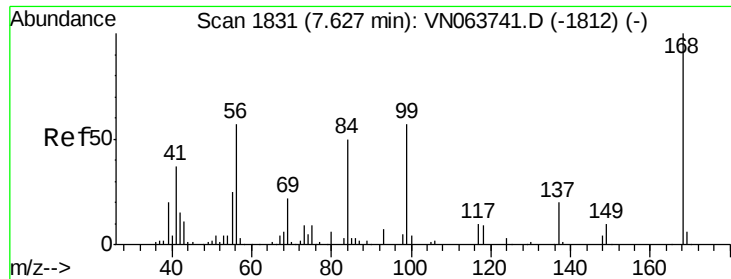

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN063824.D

Acq: 2 Oct 2020 16:20

Instrument :

MSVOA_N

ClientSampleId :


PB132030ZHE#03

Tot Ion:168 Resp: 212395

Ion Ratio Lower Upper




168 100

99 68.4 51.8 77.6

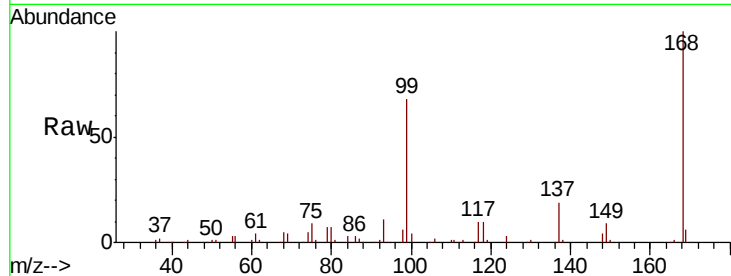

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

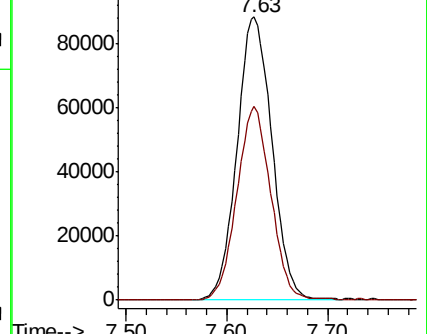

#11

Tert butyl alcohol

Concen: 3.291 ug/l

RT: 4.72 min Scan# 928

Delta R.T. -0.00 min

Lab File: VN063824.D


Acq: 2 Oct 2020 16:20

Tgt Ion: 59 Resp: 1275

Ion Ratio Lower Upper



59 100


57 13.1 8.7 13.1#



Abundance Ion 59.00 (58.70 to 59.70): VN0

Ion 57.00 (56.70 to 57.70): VN0

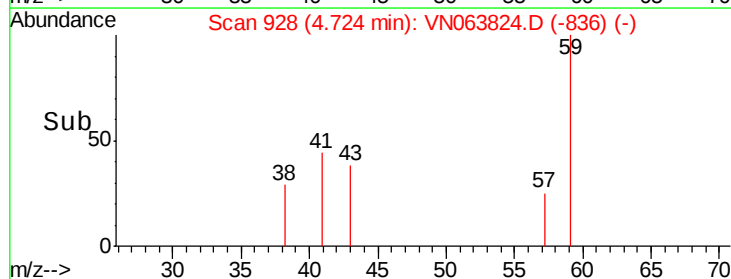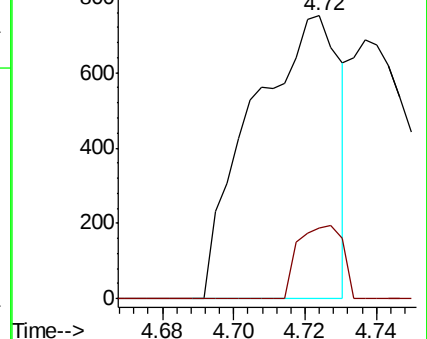



#13

Acrolein

Concen: 0.248 ug/l

RT: 3.69 min Scan# 606

Delta R.T. 0.12 min

Lab File: VN063824.D

Acq: 2 Oct 2020 16:20

Instrument :

MSVOA_N

ClientSampleId :


PB132030ZHE#03

Tot Ion: 56 Resp: 59

Ion Ratio Lower Upper

56 100

55 0.0 56.9 85.3#



Abundance Ion 56.00 (55.70 to 56.70): VN0

Ion 55.00 (54.70 to 55.70): VN0

3.69



150

100

50

0

Time-->



#16

Acetone

Concen: 17.705 ug/l

RT: 3.78 min Scan# 634

Delta R.T. 0.01 min

Lab File: VN063824.D


Acq: 2 Oct 2020 16:20

Tgt Ion: 43 Resp: 19124

Ion Ratio Lower Upper

43 100

58 29.8 22.3 33.5



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

3.78

8000


6000


4000

2000

0

Time-->







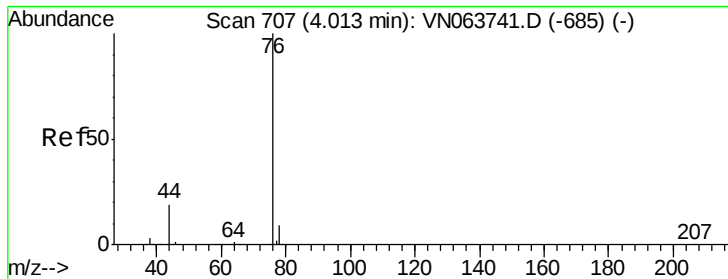

#17
Carbon Disulfide
Concen: 0.715 ug/l
RT: 4.01 min Scan# 705
Delta R.T. -0.01 min
Lab File: VN063824.D
Acq: 2 Oct 2020 16:20




Instrument :
MSVOA_N
ClientSampleId :
PB132030ZHE#03


Tot Ion: 76 Resp: 82
Ion Ratio Lower Upper
76 100
78 0.0 7.0 10.4#

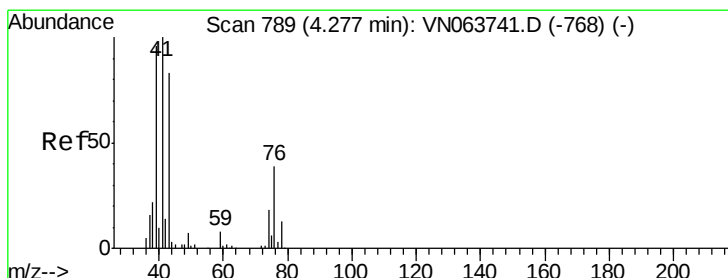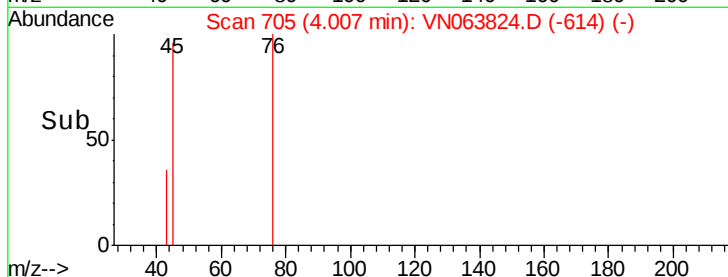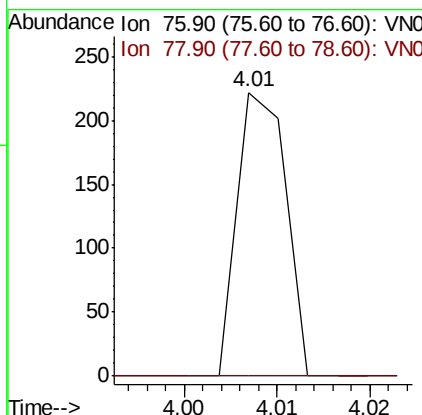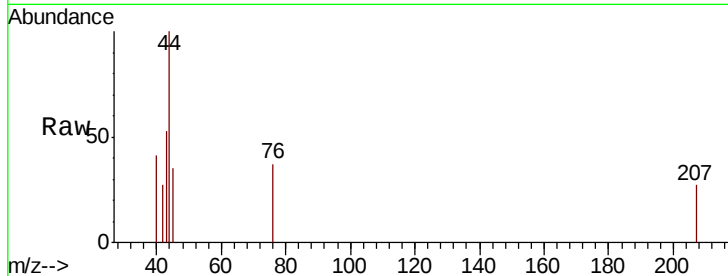

#18
Methyl Acetate
Concen: 0.725 ug/l
RT: 4.28 min Scan# 791
Delta R.T. 0.01 min
Lab File: VN063824.D
Acq: 2 Oct 2020 16:20

Tgt Ion: 43 Resp: 2034
Ion Ratio Lower Upper
43 100
74 2.9 17.4 26.2#


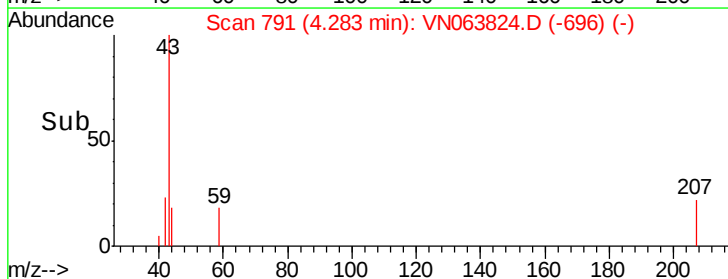
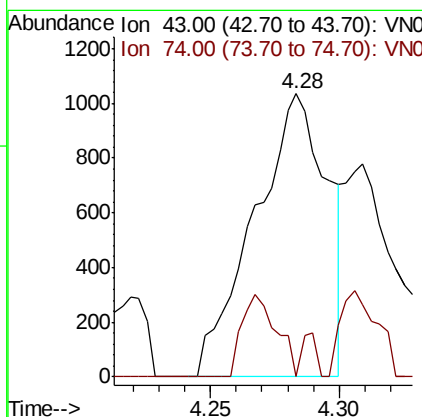
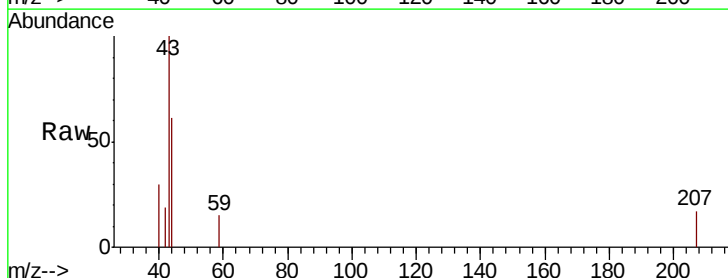


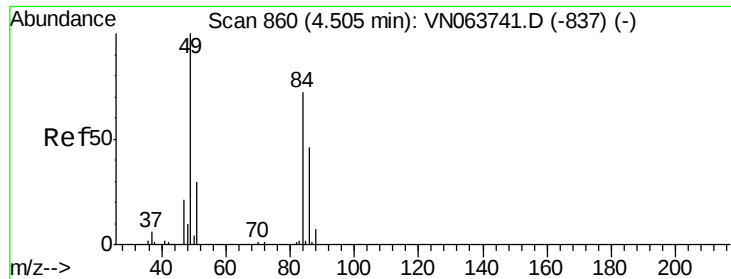

#20
Methvlene Chloride
Concen: 8.345 ug/l
RT: 4.50 min Scan# 858
Delta R.T. -0.01 min
Lab File: VN063824.D
Acq: 2 Oct 2020 16:20




Instrument :
MSVOA_N
ClientSampleId :
PB132030ZHE#03


Tot Ion:	84	Resp:	20445
Ion	Ratio	Lower	Upper
84	100		
49	157.0	110.4	165.6
51	39.1	33.3	49.9
86	71.4	50.7	76.1

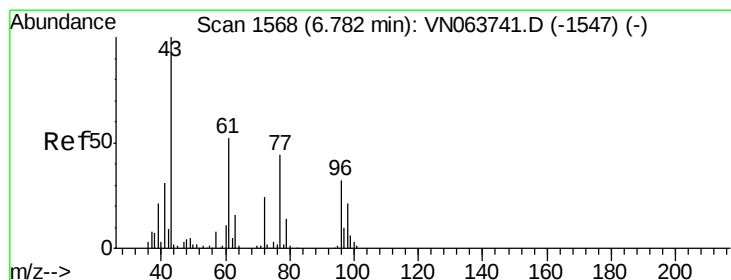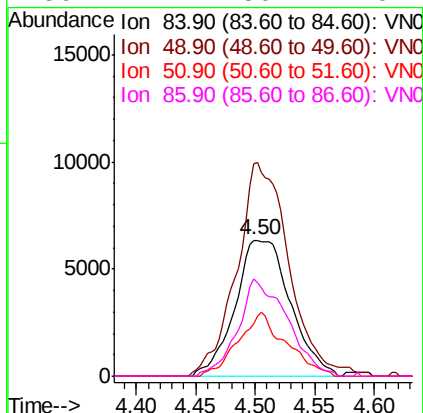

#25
2-Butanone
Concen: 10.010 ug/l
RT: 6.79 min Scan# 1571
Delta R.T. 0.01 min
Lab File: VN063824.D
Acq: 2 Oct 2020 16:20

Tgt Ion:	43	Resp:	15330
Ion	Ratio	Lower	Upper
43	100		
72	24.6	19.3	28.9

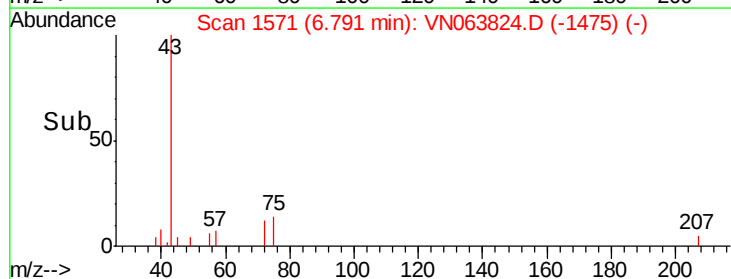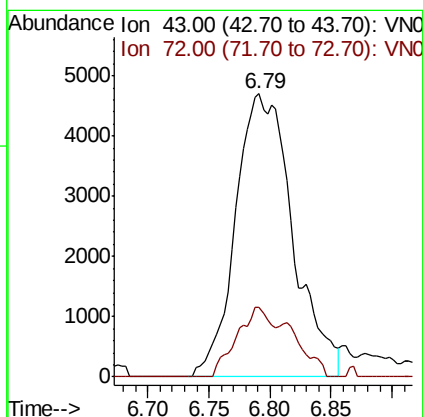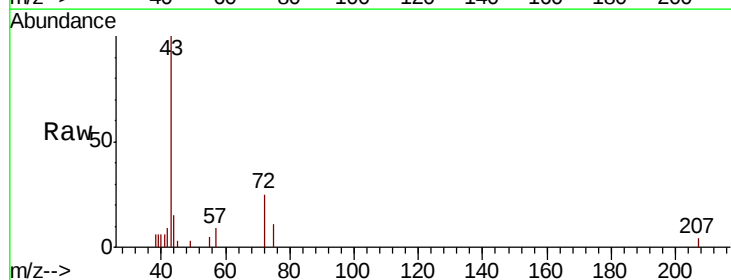

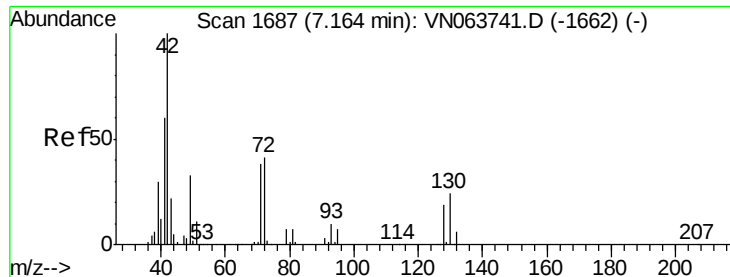

#29

Tetrahydrofuran

Concen: 2.169 ug/l

RT: 7.17 min Scan# 1689

Delta R.T. 0.01 min

Lab File: VN063824.D

Acq: 2 Oct 2020 16:20

Instrument :

MSVOA_N

ClientSampleId :

PB132030ZHE#03





Tot Ion: 42 Resp: 2228

Ion Ratio Lower Upper

42 100

72 12.3 32.8 49.2#

71 16.5 30.6 45.8#

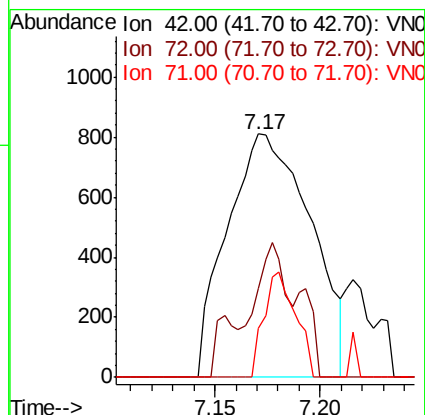

#31

Cyclohexane

Concen: 1.598 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.01 min

Lab File: VN063824.D

Acq: 2 Oct 2020 16:20




Tgt Ion: 56 Resp: 6508


Ion Ratio Lower Upper

56 100

69 140.2 25.4 38.2#

84 82.5 63.3 94.9


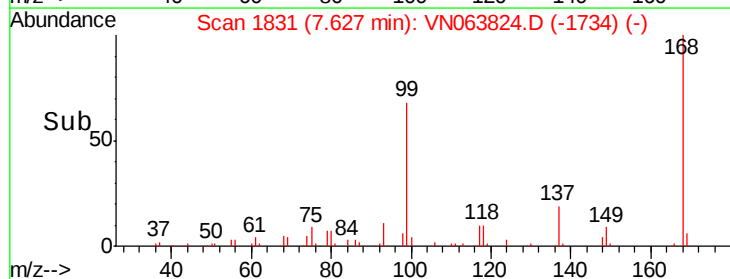
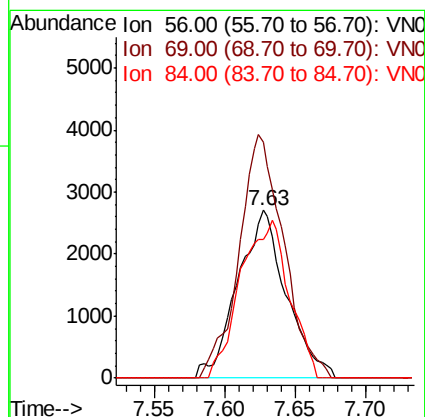



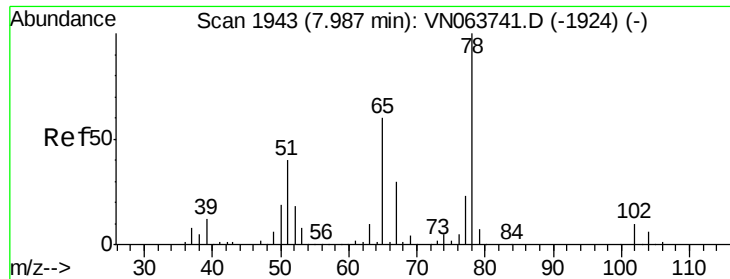

#33
 1,2-Dichloroethane-d4
 Concen: 52.668 ug/l
 RT: 7.99 min Scan# 1943
 Delta R.T. 0.00 min
 Lab File: VN063824.D
 Acq: 2 Oct 2020 16:20




Instrument :
 MSVOA_N
 ClientSampleId :
 PB132030ZHE#03


Tot Ion: 65 Resp: 184807
 Ion Ratio Lower Upper
 65 100
 67 50.4 0.0 99.6

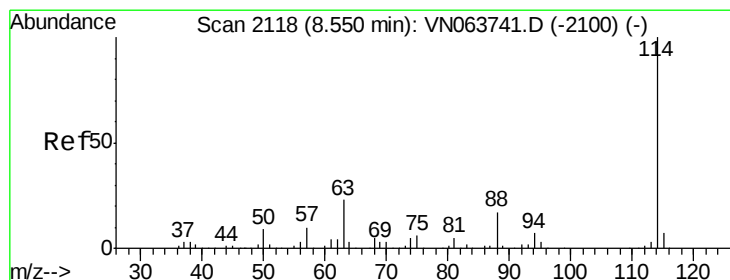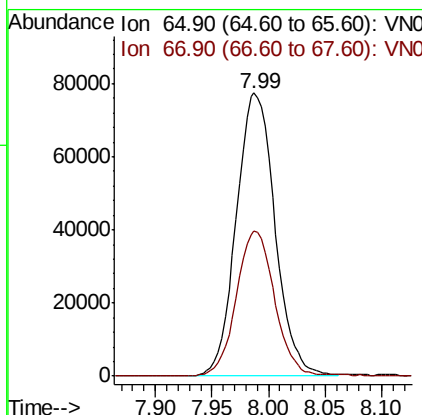

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2118
 Delta R.T. 0.00 min
 Lab File: VN063824.D
 Acq: 2 Oct 2020 16:20

Tgt Ion: 114 Resp: 396662
 Ion Ratio Lower Upper
 114 100
 63 22.7 0.0 45.0
 88 16.4 0.0 34.0



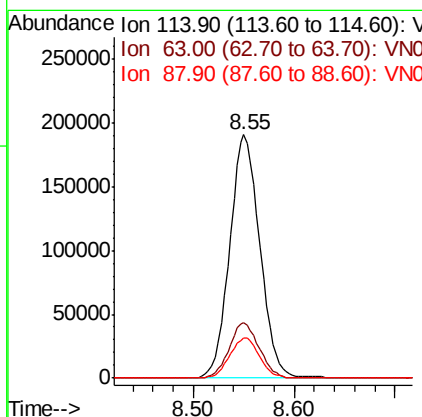





#35
Dibromofluoromethane
Concen: 47.229 ug/l
RT: 7.55 min Scan# 1808
Delta R.T. 0.00 min
Lab File: VN063824.D
Acq: 2 Oct 2020 16:20




Instrument :
MSVOA_N
ClientSampleId :
PB132030ZHE#03


Tot Ion:113 Resp: 129990
Ion Ratio Lower Upper
113 100
111 103.3 81.8 122.8
192 18.2 14.2 21.2

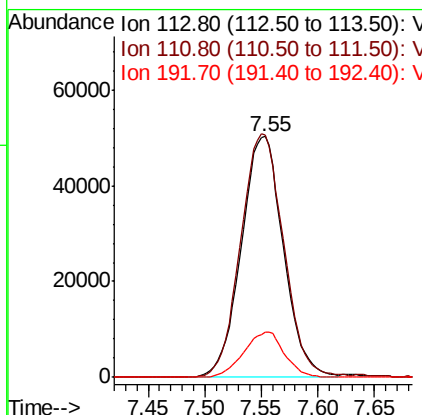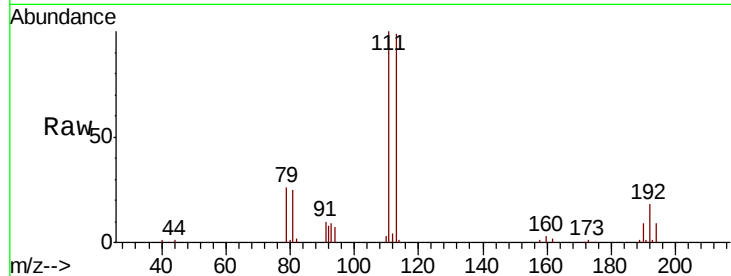

#36
1,1-Dichloropropene
Concen: 4.762 ug/l
RT: 7.62 min Scan# 1830
Delta R.T. -0.13 min
Lab File: VN063824.D
Acq: 2 Oct 2020 16:20

Tgt Ion: 75 Resp: 19135
Ion Ratio Lower Upper
75 100
110 12.1 16.9 50.6#
77 0.0 24.5 36.7#



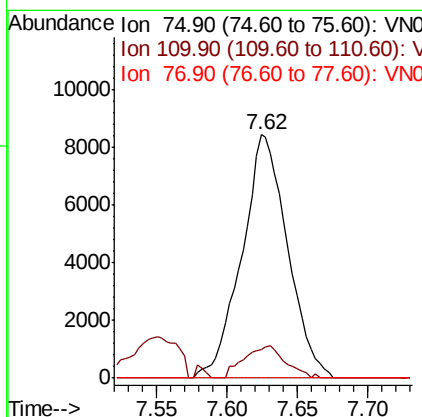
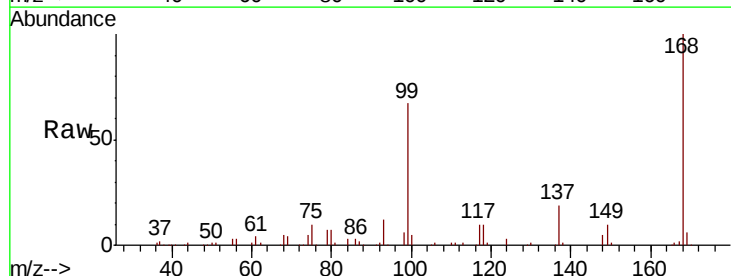


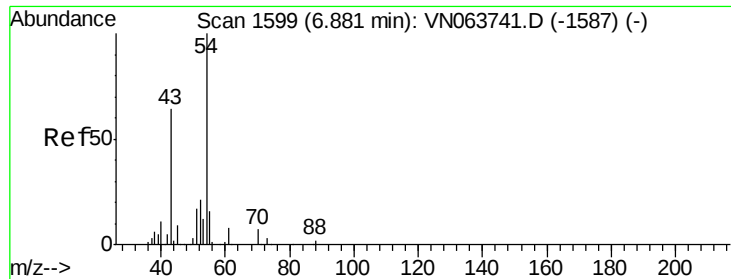

#37
Ethyl Acetate
Concen: 3.840 ug/l
RT: 6.79 min Scan# 1571
Delta R.T. -0.09 min
Lab File: VN063824.D
Acq: 2 Oct 2020 16:20




Instrument :
MSVOA_N
ClientSampleId :
PB132030ZHE#03


Tot Ion: 43 Resp: 15330
Ion Ratio Lower Upper
43 100
61 0.0 10.4 15.6#
70 0.2 7.3 10.9#

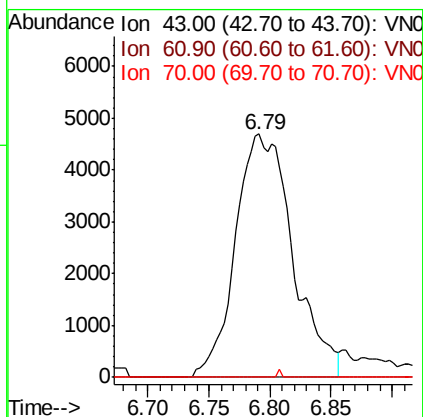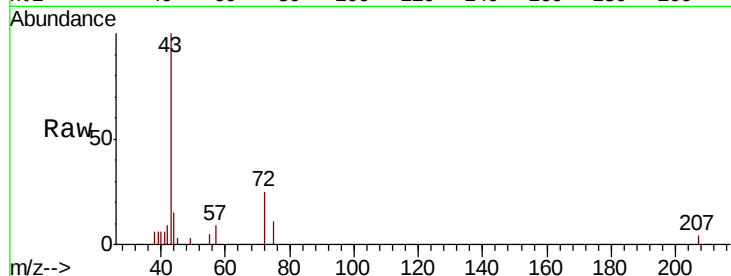

#38
Carbon Tetrachloride
Concen: 5.026 ug/l
RT: 7.63 min Scan# 1832
Delta R.T. -0.10 min
Lab File: VN063824.D
Acq: 2 Oct 2020 16:20

Tgt Ion: 117 Resp: 22648
Ion Ratio Lower Upper
117 100
119 6.2 80.1 120.1#
121 0.0 25.7 38.5#

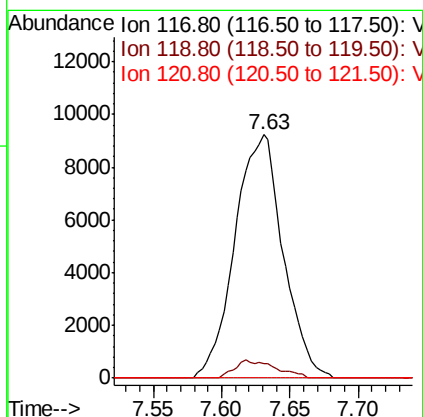



#41

Methacrylonitrile

Concen: 0.730 ug/l

RT: 7.18 min Scan# 1691

Delta R.T. 0.05 min

Lab File: VN063824.D

Acq: 2 Oct 2020 16:20

Instrument :

MSVOA_N

ClientSampleId :

PB132030ZHE#03

Tot Ion: 41 Resp: 1296





Ion Ratio Lower Upper

41 100

39 102.4 42.5 63.7#

67 0.0 57.4 86.2#

52 0.0 26.9 40.3#

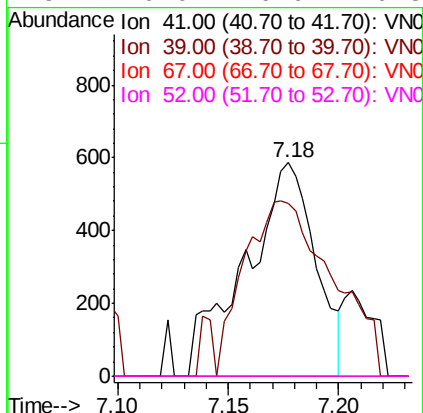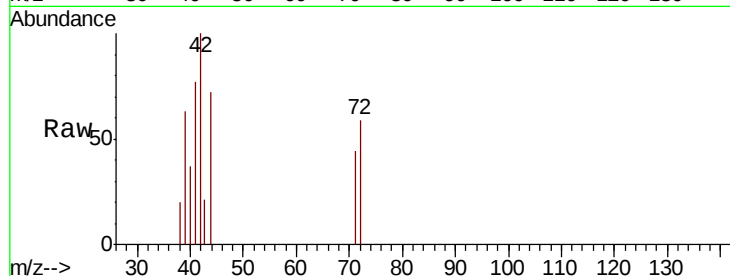

#43

Isopropyl Acetate

Concen: 10.274 ug/l

RT: 8.13 min Scan# 1986

Delta R.T. 0.00 min

Lab File: VN063824.D

Acq: 2 Oct 2020 16:20




Tgt Ion: 43 Resp: 67659


Ion Ratio Lower Upper

43 100

61 16.1 14.2 21.4

87 12.1 9.0 13.6

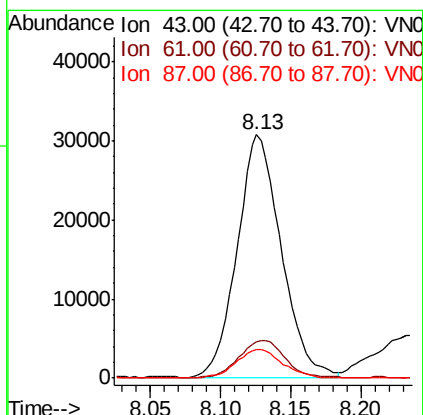

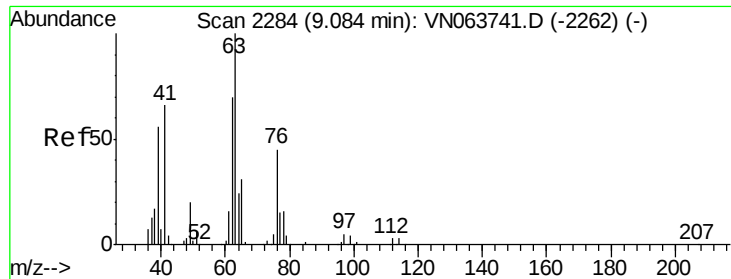

#45

1,2-Dichloropropane

Concen: 0.379 ug/l

RT: 9.23 min Scan# 2330

Delta R.T. 0.15 min

Lab File: VN063824.D

Acq: 2 Oct 2020 16:20

Instrument :

MSVOA_N

ClientSampleId :


PB132030ZHE#03

Tot Ion: 63 Resp: 1174

Ion Ratio Lower Upper

63 100

65 0.0 24.7 37.1#

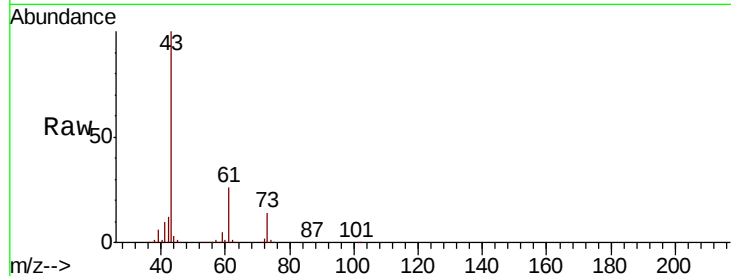

Abundance Ion 62.90 (62.60 to 63.60): VN0

Ion 64.90 (64.60 to 65.60): VN0

9.23

800

600

400



200

0

9.20

9.25

Time-->



#48

Methyl methacrylate

Concen: 1.827 ug/l

RT: 9.15 min Scan# 2305

Delta R.T. -0.02 min

Lab File: VN063824.D

Acq: 2 Oct 2020 16:20


Tgt Ion: 41 Resp: 5946

Ion Ratio Lower Upper

41 100

69 0.0 60.9 91.3#

39 0.0 57.5 86.3#



Abundance Ion 41.00 (40.70 to 41.70): VN0

Ion 69.00 (68.70 to 69.70): VN0

Ion 39.00 (38.70 to 39.70): VN0

60000

50000

40000

30000

20000

10000


0


9.10

9.15

9.20

Time-->



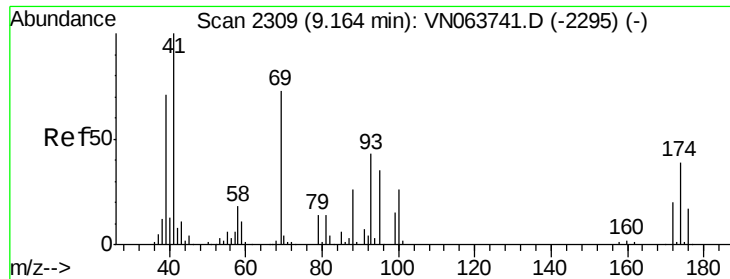

#49

1,4-Dioxane

Concen: 1.406 ug/l

RT: 9.24 min Scan# 2332

Delta R.T. 0.07 min

Lab File: VN063824.D

Acq: 2 Oct 2020 16:20

Instrument :

MSVOA_N

ClientSampleId :

PB132030ZHE#03


Tot Ion: 88 Resp: 65

Ion Ratio Lower Upper

88 100

43 1757981.5 33.1 49.7#




58 8481.5 58.9 88.3#



Abundance Ion 88.00 (87.70 to 88.70): VN0

Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

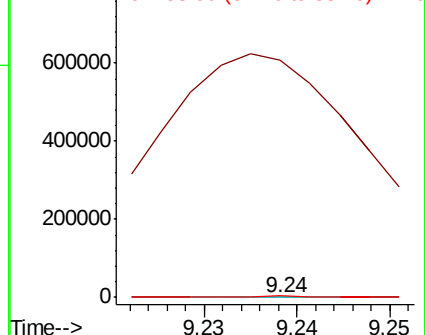

#50

Toluene-d8

Concen: 49.439 ug/l

RT: 10.06 min Scan# 2588

Delta R.T. 0.00 min

Lab File: VN063824.D


Acq: 2 Oct 2020 16:20

Tgt Ion: 98 Resp: 515835

Ion Ratio Lower Upper



98 100


100 63.3 49.8 74.6



Abundance Ion 98.00 (97.70 to 98.70): VN0

Ion 100.00 (99.70 to 100.70): VN0

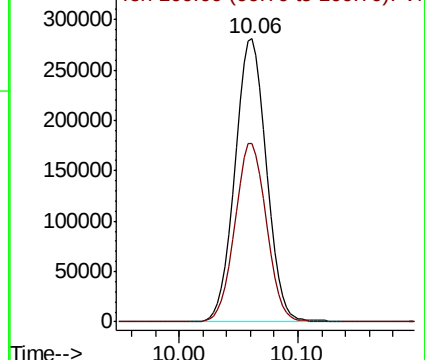



#51

4-Methyl-2-Pentanone

Concen: 2.282 ug/l

RT: 9.95 min Scan# 2553

Delta R.T. -0.00 min

Lab File: VN063824.D

Acq: 2 Oct 2020 16:20

Instrument :

MSVOA_N

ClientSampleId :


PB132030ZHE#03

Tot Ion: 43 Resp: 8821

Ion Ratio Lower Upper

43 100

58 31.1 28.4 42.6

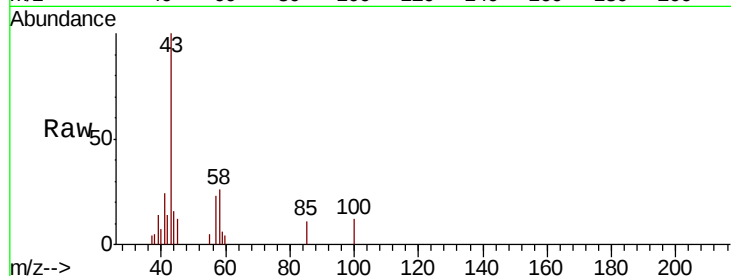

Abundance Ion 43.00 (42.70 to 43.70): VN063741.D (-2537) (-)

Ion 58.00 (57.70 to 58.70): VN063741.D (-2537) (-)

20000

15000



10000

5000

0

9.90 9.95 10.00

Time-->



#54

cis-1,3-Dichloropropene

Concen: 5.387 ug/l

RT: 9.87 min Scan# 2530

Delta R.T. 0.07 min

Lab File: VN063824.D

Acq: 2 Oct 2020 16:20


Tgt Ion: 75 Resp: 26614

Ion Ratio Lower Upper

75 100

77 0.0 24.6 36.8#

39 45.6 49.7 74.5#



Abundance Ion 74.90 (74.60 to 75.60): VN063741.D (-2493) (-)

Ion 76.90 (76.60 to 77.60): VN063741.D (-2493) (-)

Ion 39.00 (38.70 to 39.70): VN063741.D (-2493) (-)

20000

15000


10000


5000

0

9.80 9.85 9.90 9.95

Time-->



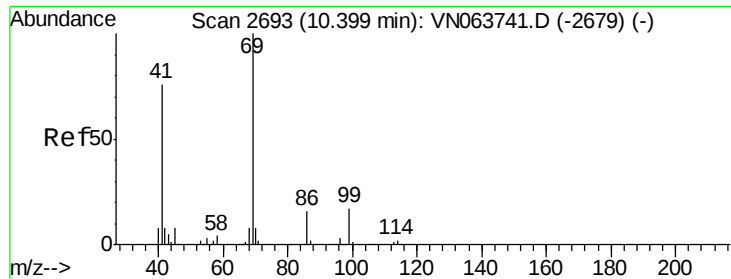

#56

Ethyl methacrylate

Concen: 0.477 ug/l

RT: 10.52 min Scan# 2730

Delta R.T. 0.12 min

Lab File: VN063824.D

Acq: 2 Oct 2020 16:20

Instrument :

MSVOA_N

ClientSampleId :

PB132030ZHE#03





Tot Ion: 69 Resp: 1926

Ion Ratio Lower Upper

69 100

41 3815.2 61.1 91.7#

39 1894.8 42.2 63.4#

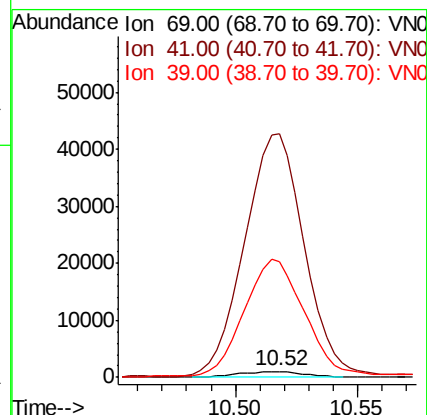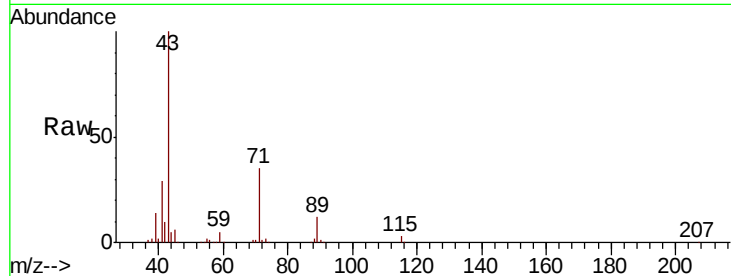

#57

1,3-Dichloropropane

Concen: 0.939 ug/l

RT: 10.74 min Scan# 2798

Delta R.T. 0.06 min

Lab File: VN063824.D




Acq: 2 Oct 2020 16:20


Tgt Ion: 76 Resp: 4523

Ion Ratio Lower Upper

76 100

78 0.0 25.2 37.8#


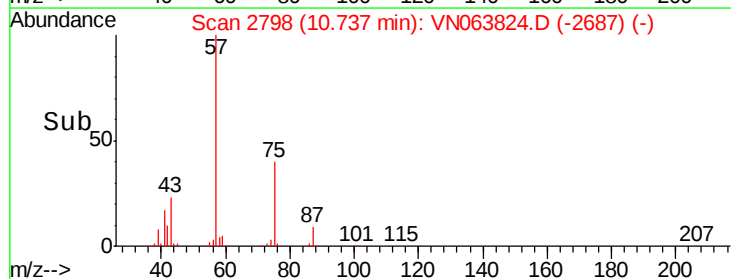
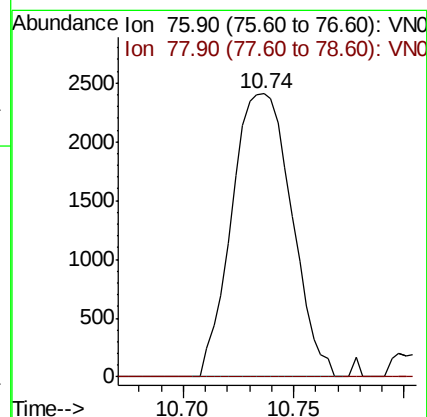





#59
2-Hexanone
Concen: 26.868 ug/l
RT: 10.74 min Scan# 2798
Delta R.T. 0.02 min
Lab File: VN063824.D
Acq: 2 Oct 2020 16:20




Instrument :
MSVOA_N
ClientSampleId :
PB132030ZHE#03


Tot Ion: 43 Resp: 77135
Ion Ratio Lower Upper
43 100
58 21.0 24.6 73.8#

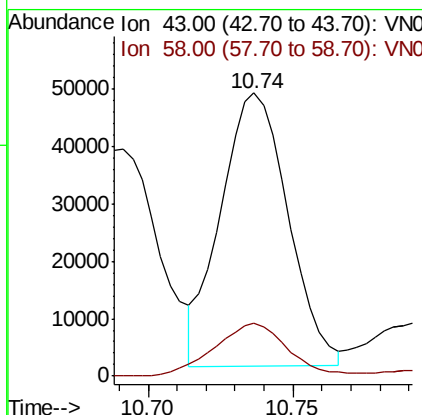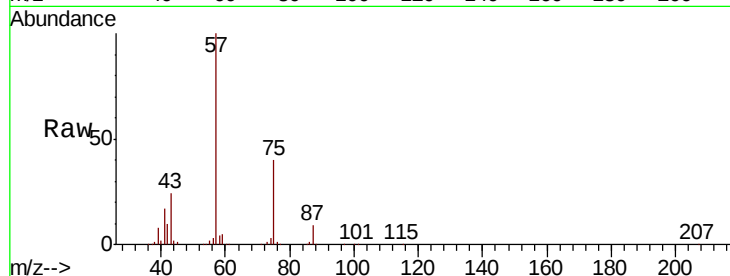

#62
4-Bromofluorobenzene
Concen: 52.958 ug/l
RT: 12.38 min Scan# 3308
Delta R.T. 0.00 min
Lab File: VN063824.D
Acq: 2 Oct 2020 16:20

Tgt Ion: 95 Resp: 207710
Ion Ratio Lower Upper
95 100
174 75.1 0.0 150.6
176 72.0 0.0 145.4

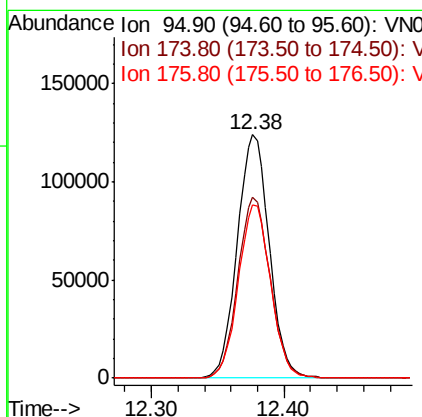


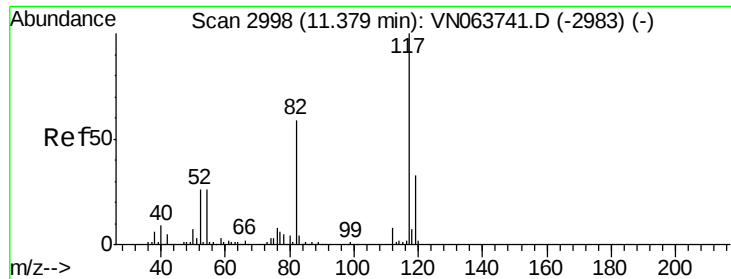




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2998
Delta R.T. 0.00 min
Lab File: VN063824.D
Acq: 2 Oct 2020 16:20

Instrument :
MSVOA_N
ClientSampleId :
PB132030ZHE#03

Tot Ion:117 Resp: 416355
Ion Ratio Lower Upper
117 100
82 61.3 47.4 71.2
119 32.1 26.4 39.6

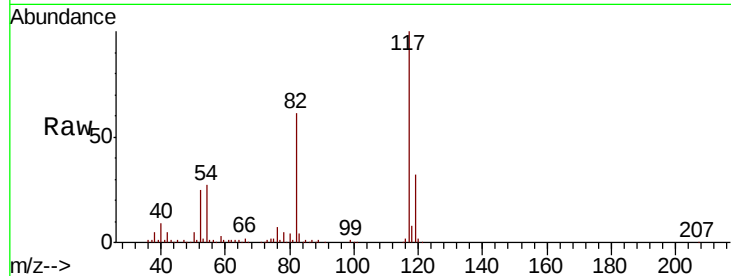


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

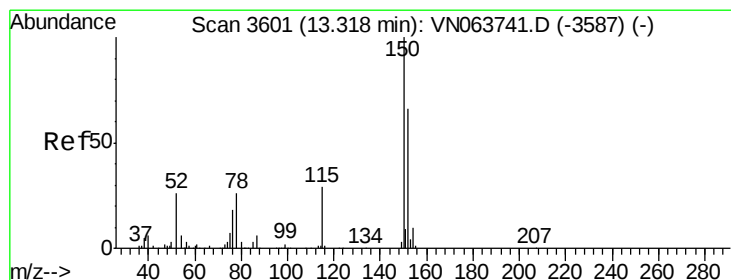
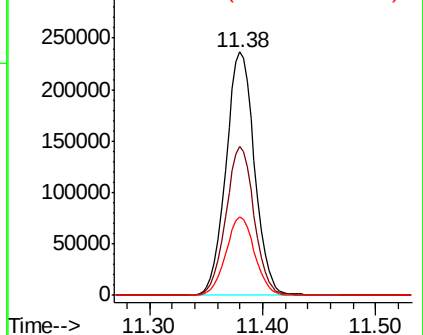



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.32 min Scan# 3601
Delta R.T. 0.00 min
Lab File: VN063824.D
Acq: 2 Oct 2020 16:20

Tgt Ion:152 Resp: 168630
Ion Ratio Lower Upper
152 100
115 65.2 31.3 93.8
150 158.2 0.0 341.8



Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

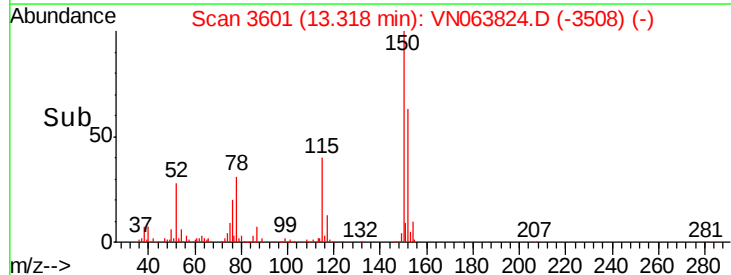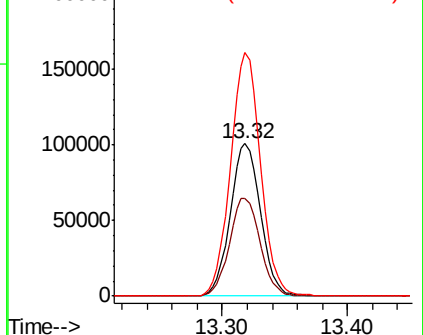



#74

N-amvl acetate

Concen: 3.202 ug/l

RT: 12.01 min Scan# 3194

Delta R.T. -0.03 min

Lab File: VN063824.D

Acq: 2 Oct 2020 16:20

Instrument :

MSVOA_N

ClientSampleId :

PB132030ZHE#03

Tot Ion: 43 Resp: 5896


Ion Ratio Lower Upper

43 100

70 0.0 29.8 44.8#

55 5.1 17.9 26.9#

61 0.0 17.0 25.4#



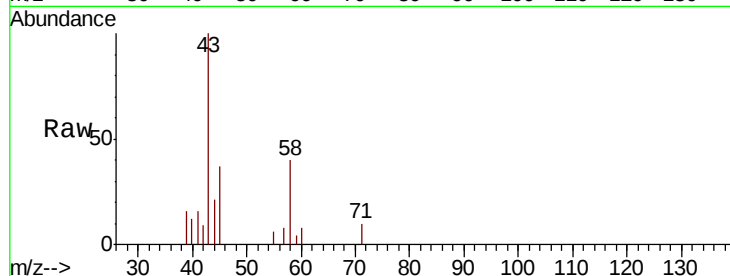


Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 70.00 (69.70 to 70.70): VN0

Ion 55.00 (54.70 to 55.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

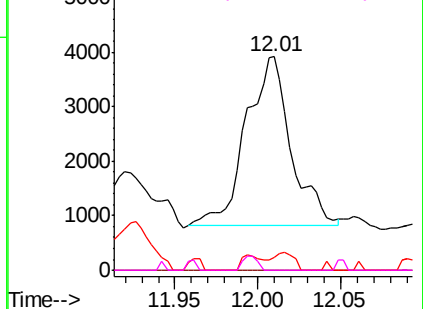

#76

1,2,3-Trichloropropane

Concen: 31.297 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. -0.15 min

Lab File: VN063824.D


Acq: 2 Oct 2020 16:20

Tgt Ion: 75 Resp: 116338

Ion Ratio Lower Upper



75 100


77 1.1 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 77.00 (76.70 to 77.70): VN0




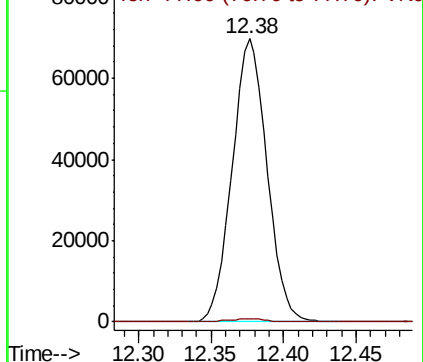




#80
 1,3,5-Trimethylbenzene
 Concen: 0.263 ug/l
 RT: 12.71 min Scan# 3413
 Delta R.T. 0.01 min
 Lab File: VN063824.D
 Acq: 2 Oct 2020 16:20

Instrument :
 MSVOA_N
 ClientSampleId :
 PB132030ZHE#03

Tot Ion:105 Resp: 2714
 Ion Ratio Lower Upper
 105 100
 120 45.0 23.3 69.9

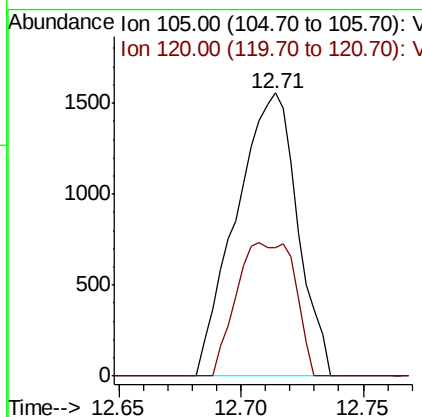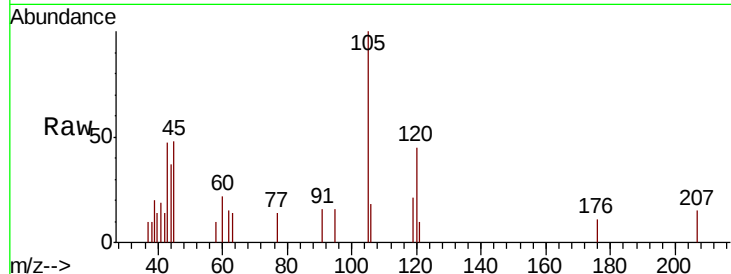

#81
 trans-1,4-Dichloro-2-butene
 Concen: 90.139 ug/l
 RT: 12.38 min Scan# 3308
 Delta R.T. 0.10 min
 Lab File: VN063824.D
 Acq: 2 Oct 2020 16:20

Tgt Ion: 75 Resp: 116338
 Ion Ratio Lower Upper
 75 100
 53 0.2 88.2 132.2#
 89 0.0 36.0 54.0#

