

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN100220\
 Data File : VN063825.D
 Acq On : 2 Oct 2020 16:44
 Operator : JC/MD
 Sample : PB132030ZHE#04
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB132030ZHE#04

Quant Time: Oct 05 04:16:39 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 01 01:46:38 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	211691	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	398044	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	419540	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	172680	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	184653	52.80	ug/l	0.00
Spiked Amount			Recovery	=	105.60%	
35) Dibromofluoromethane	7.55	113	133109	48.19	ug/l	0.00
Spiked Amount			Recovery	=	96.38%	
50) Toluene-d8	10.06	98	515421	49.23	ug/l	0.00
Spiked Amount			Recovery	=	98.46%	
62) 4-Bromofluorobenzene	12.38	95	205591	52.24	ug/l	0.00
Spiked Amount			Recovery	=	104.48%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Tert butyl alcohol	4.72	59	1817	4.706	ug/l #	76
16) Acetone	3.78	43	19016	17.663	ug/l #	88
17) Carbon Disulfide	4.00	76	198	0.734	ug/l #	76
18) Methyl Acetate	4.28	43	3157	1.129	ug/l #	59
20) Methylene Chloride	4.51	84	20012	8.198	ug/l	93
25) 2-Butanone	6.79	43	16107	10.553	ug/l	91
29) Tetrahydrofuran	7.15	42	701	0.685	ug/l #	59
31) Cyclohexane	7.63	56	6162	1.518	ug/l #	26
36) 1,1-Dichloropropene	7.63	75	18988	4.709	ug/l #	51
37) Ethyl Acetate	6.79	43	16107	4.020	ug/l #	70
38) Carbon Tetrachloride	7.62	117	23924	5.291	ug/l #	16
41) Methacrylonitrile	7.15	41	386	0.217	ug/l #	1
43) Isopropyl Acetate	8.13	43	67459	10.208	ug/l	99
45) 1,2-Dichloropropane	9.24	63	1183	0.380	ug/l #	44
48) Methyl methacrylate	9.14	41	6018	1.843	ug/l #	36
51) 4-Methyl-2-Pentanone	9.96	43	7468	1.926	ug/l #	84
54) cis-1,3-Dichloropropene	9.87	75	24279	4.897	ug/l #	73
56) Ethyl methacrylate	10.52	69	1814	0.448	ug/l #	1
57) 1,3-Dichloropropane	10.74	76	4491	0.929	ug/l #	43
59) 2-Hexanone	10.74	43	79592	27.627	ug/l #	57
74) N-amyl acetate	12.00	43	5528	3.118	ug/l #	50
76) 1,2,3-Trichloropropane	12.38	75	118250	31.065	ug/l #	100
80) 1,3,5-Trimethylbenzene	12.71	105	2601	0.246	ug/l	89
81) trans-1,4-Dichloro-2-buten	12.38	75	118250	89.472	ug/l #	6
95) Naphthalene	15.11	128	104	1.935	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN100220\
Data File : VN063825.D
Acq On : 2 Oct 2020 16:44
Operator : JC/MD
Sample : PB132030ZHE#04
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB132030ZHE#04

Quant Time: Oct 05 04:16:39 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 01 01:46:38 2020
Response via : Initial Calibration

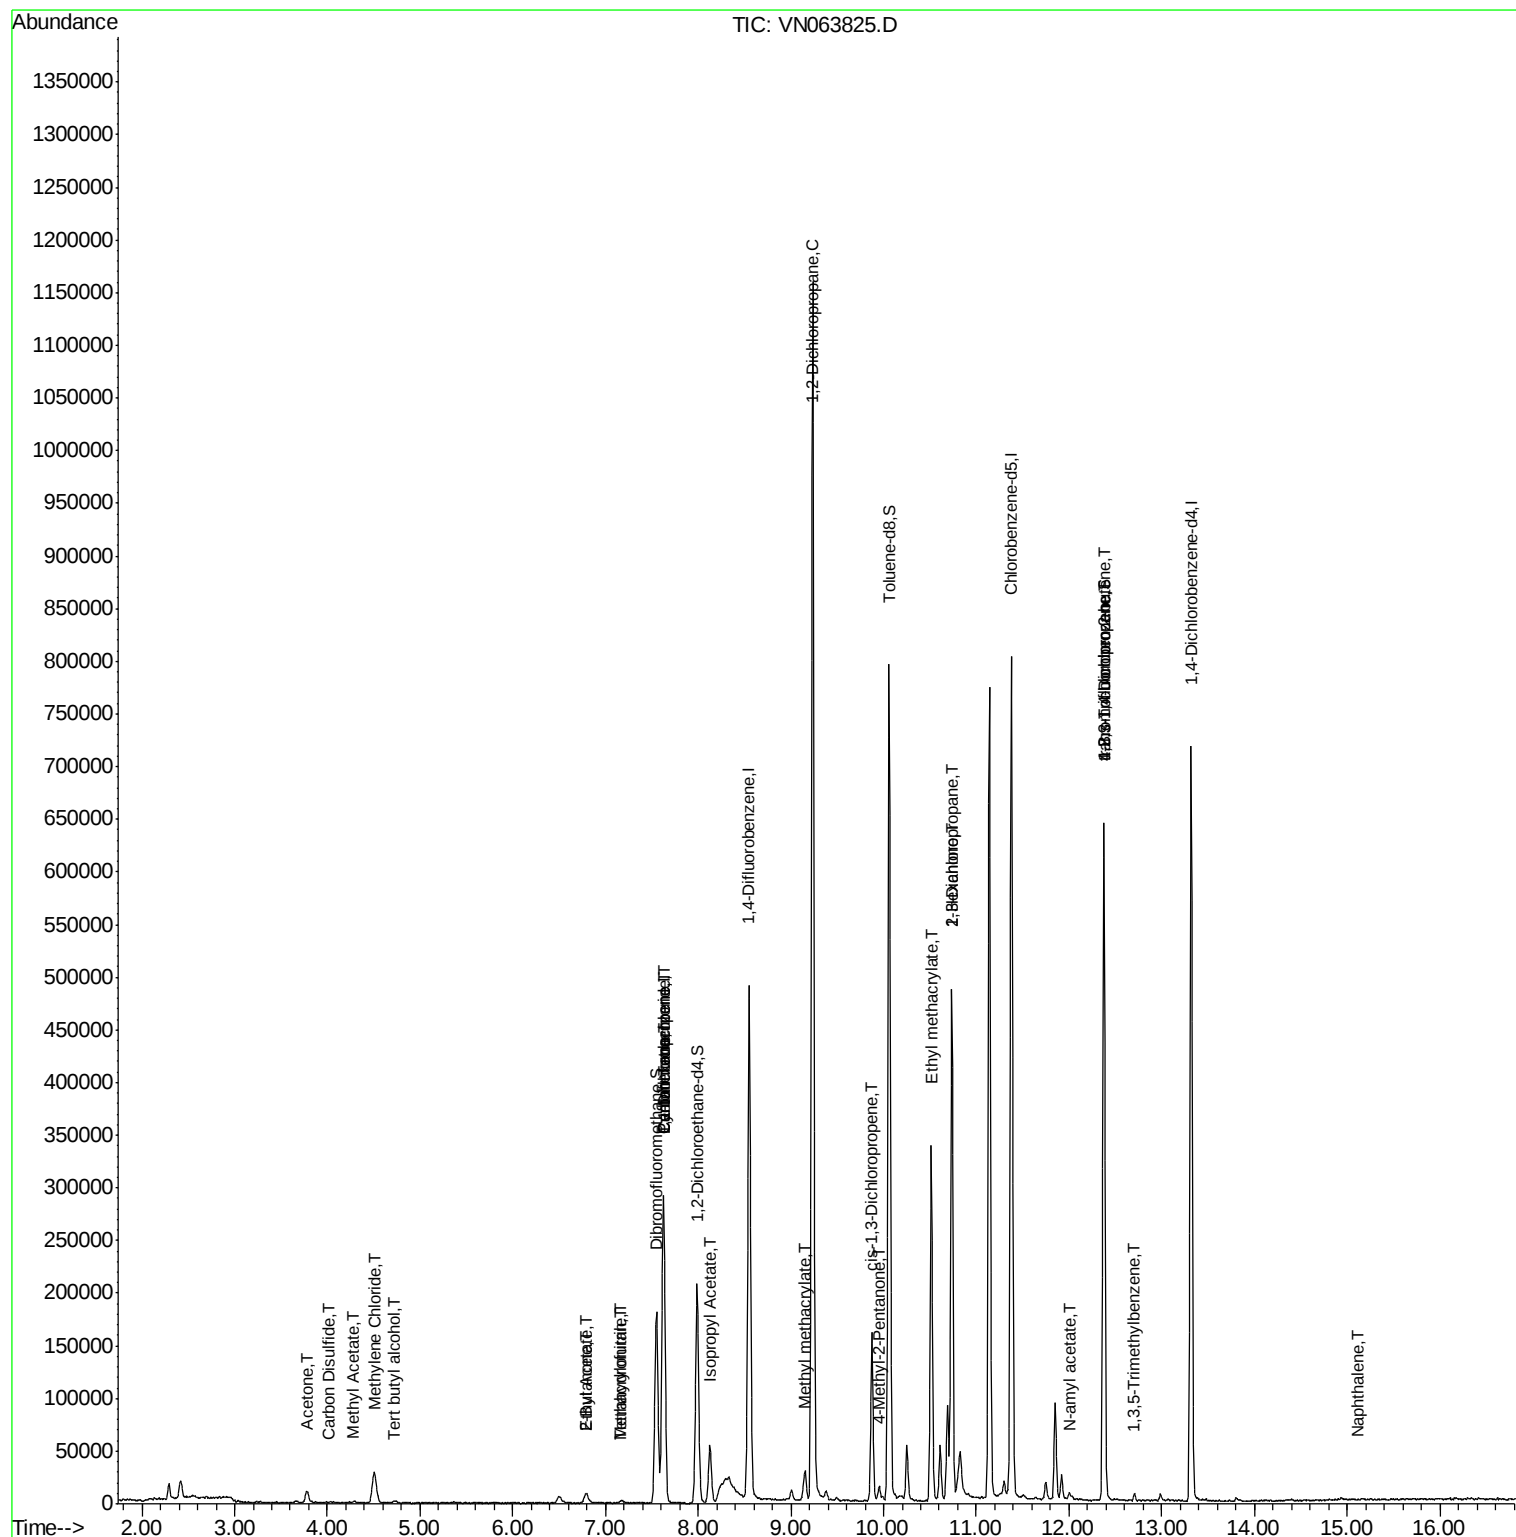

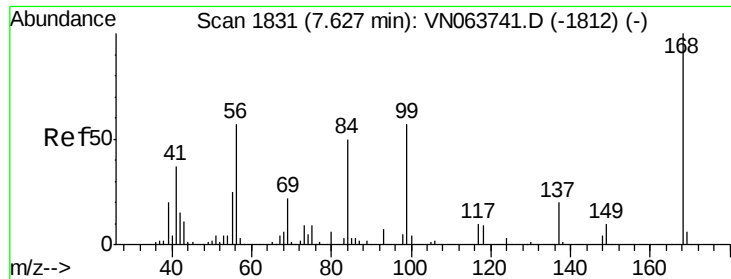

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN063825.D

Acq: 2 Oct 2020 16:44

Instrument :

MSVOA_N

ClientSampleId :


PB132030ZHE#04

Tot Ion:168 Resp: 211691




Ion Ratio Lower Upper

168 100

99 64.8 51.8 77.6



Abundance Ion 167.90 (167.60 to 168.60): VN063825.D (-1738) (-)

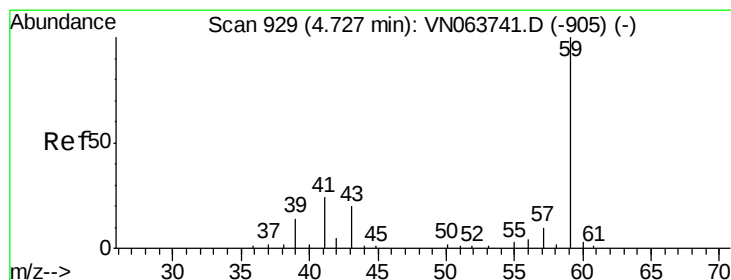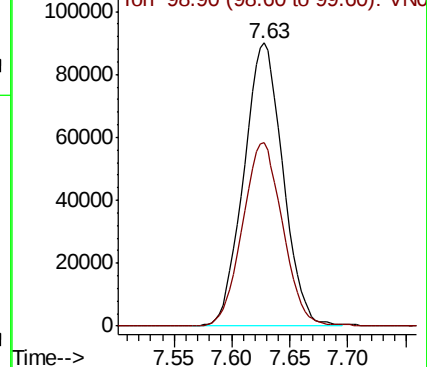

#11

Tert butyl alcohol

Concen: 4.706 ug/l

RT: 4.72 min Scan# 927

Delta R.T. -0.01 min

Lab File: VN063825.D


Acq: 2 Oct 2020 16:44

Tgt Ion: 59 Resp: 1817



Ion Ratio Lower Upper


59 100

57 1.9 8.7 13.1#



Abundance Ion 59.00 (58.70 to 59.70): VN063825.D (-836) (-)

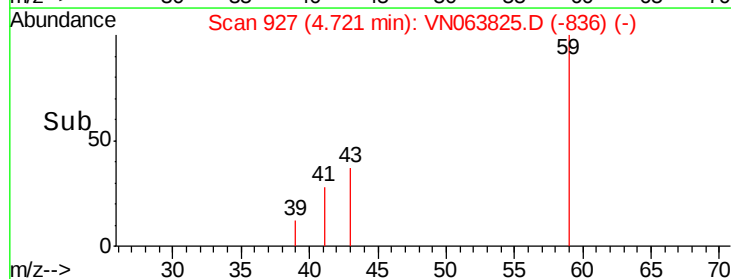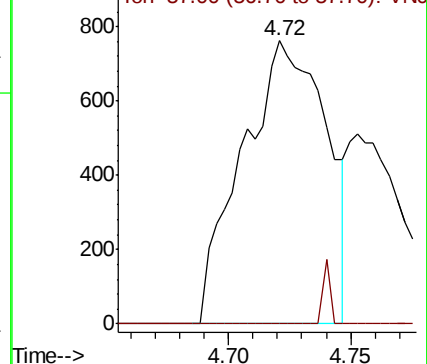

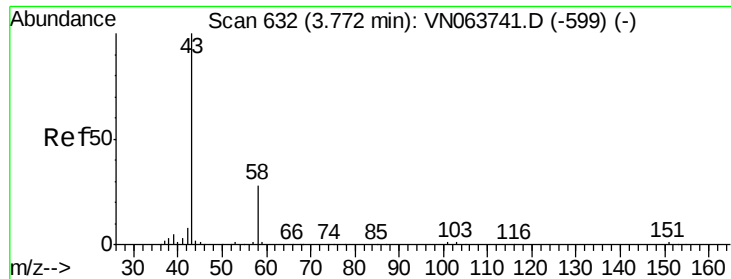

#16

Acetone

Concen: 17.663 ug/l

RT: 3.78 min Scan# 633

Delta R.T. 0.00 min

Lab File: VN063825.D

Acq: 2 Oct 2020 16:44

Instrument :

MSVOA_N

ClientSampleId :





PB132030ZHE#04

Tot Ion: 43 Resp: 19016

Ion Ratio Lower Upper

43 100

58 21.7 22.3 33.5#

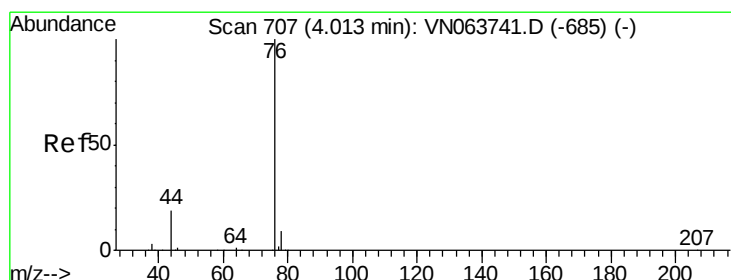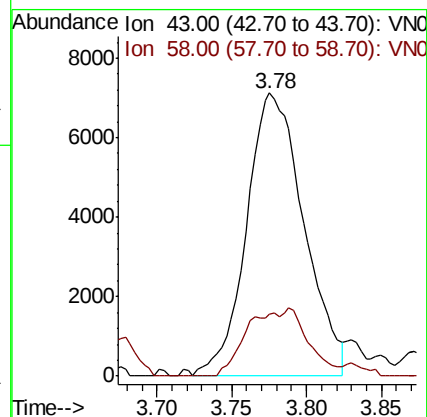

#17

Carbon Disulfide

Concen: 0.734 ug/l

RT: 4.00 min Scan# 703

Delta R.T. -0.01 min

Lab File: VN063825.D




Acq: 2 Oct 2020 16:44


Tgt Ion: 76 Resp: 198

Ion Ratio Lower Upper

76 100

78 0.0 7.0 10.4#



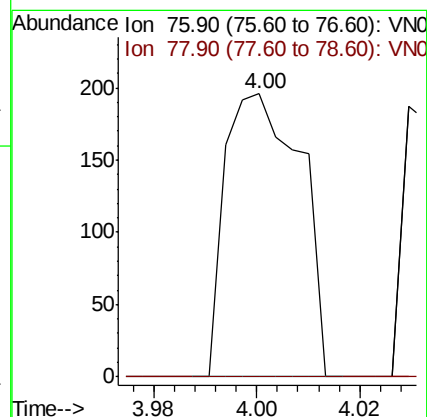





#18
Methyl Acetate
Concen: 1.129 ug/l
RT: 4.28 min Scan# 790
Delta R.T. 0.00 min
Lab File: VN063825.D
Acq: 2 Oct 2020 16:44




Instrument :
MSVOA_N
ClientSampleId :
PB132030ZHE#04


Tot Ion: 43 Resp: 3157
Ion Ratio Lower Upper
43 100
74 2.2 17.4 26.2#

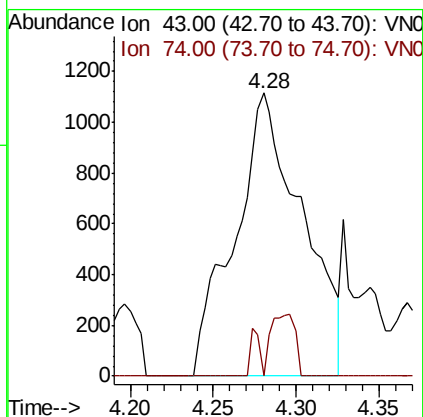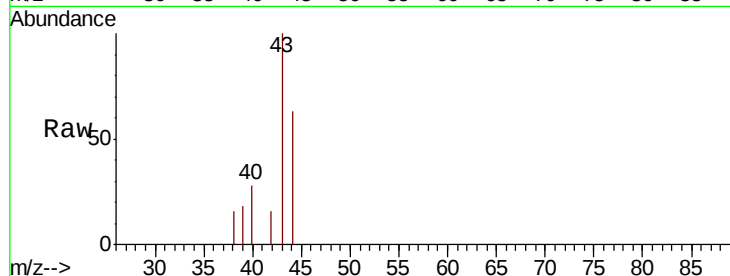

#20
Methylene Chloride
Concen: 8.198 ug/l
RT: 4.51 min Scan# 861
Delta R.T. 0.00 min
Lab File: VN063825.D
Acq: 2 Oct 2020 16:44

Tgt Ion: 84 Resp: 20012
Ion Ratio Lower Upper
84 100
49 144.3 110.4 165.6
51 38.5 33.3 49.9
86 71.7 50.7 76.1

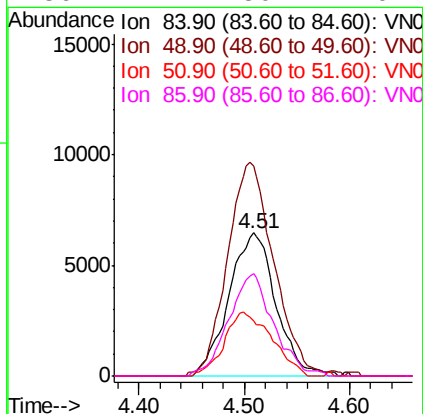

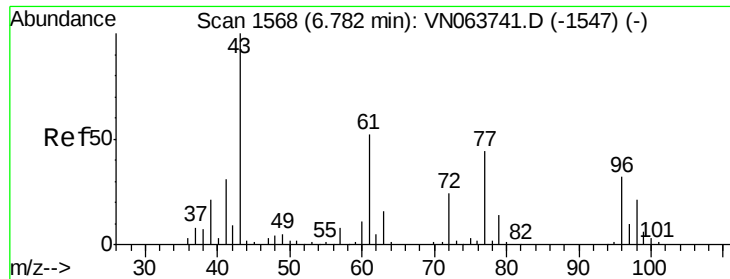

#25

2-Butanone

Concen: 10.553 ug/l

RT: 6.79 min Scan# 1572

Delta R.T. 0.01 min

Lab File: VN063825.D

Acq: 2 Oct 2020 16:44

Instrument :

MSVOA_N

ClientSampleId :


PB132030ZHE#04

Tot Ion: 43 Resp: 16107

Ion Ratio Lower Upper

43 100

72 19.8 19.3 28.9

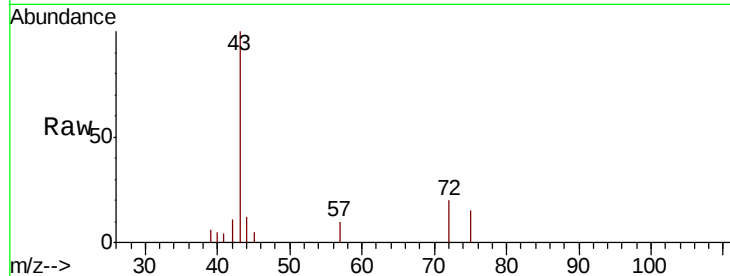

Abundance Ion 43.00 (42.70 to 43.70): VN063741.D (-1547) (-)

Ion 72.00 (71.70 to 72.70): VN063741.D (-1547) (-)

6.79

6000

5000

4000

3000



2000

1000

0

6.70 6.75 6.80 6.85

Time-->

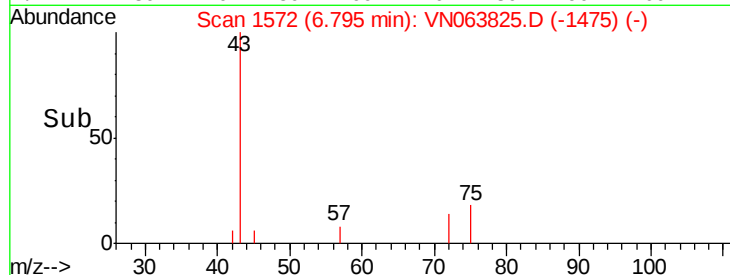

#29

Tetrahydrofuran

Concen: 0.685 ug/l

RT: 7.15 min Scan# 1684

Delta R.T. -0.01 min

Lab File: VN063825.D

Acq: 2 Oct 2020 16:44


Tgt Ion: 42 Resp: 701

Ion Ratio Lower Upper

42 100

72 15.4 32.8 49.2#

71 62.6 30.6 45.8#



Abundance Ion 42.00 (41.70 to 42.70): VN063741.D (-1662) (-)

Ion 72.00 (71.70 to 72.70): VN063741.D (-1662) (-)

Ion 71.00 (70.70 to 71.70): VN063741.D (-1662) (-)

1200

1000

800

600


400


200

0

7.12 7.14 7.16

Time-->




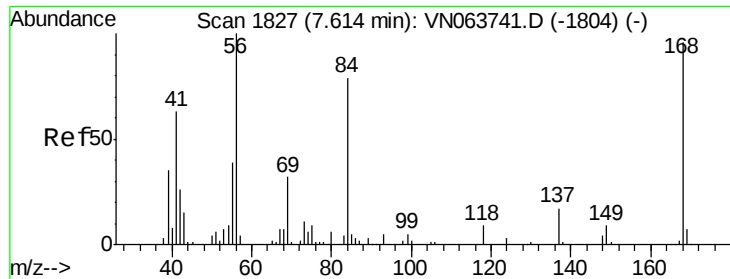




#31
Cyclohexane
Concen: 1.518 ug/l
RT: 7.63 min Scan# 1831
Delta R.T. 0.01 min
Lab File: VN063825.D
Acq: 2 Oct 2020 16:44

Instrument :
MSVOA_N
ClientSampleId :
PB132030ZHE#04

Tot Ion: 56 Resp: 6162
Ion Ratio Lower Upper
56 100
69 157.3 25.4 38.2#
84 90.6 63.3 94.9

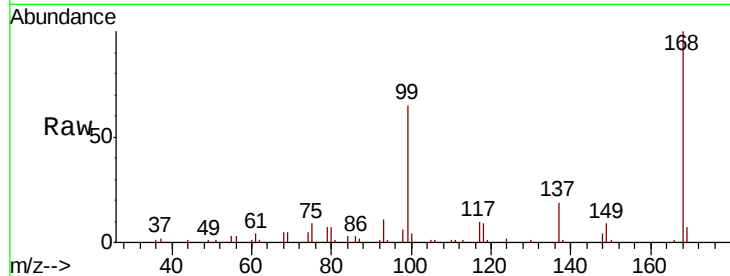


Abundance Ion 56.00 (55.70 to 56.70): VN0
Ion 69.00 (68.70 to 69.70): VN0
Ion 84.00 (83.70 to 84.70): VN0


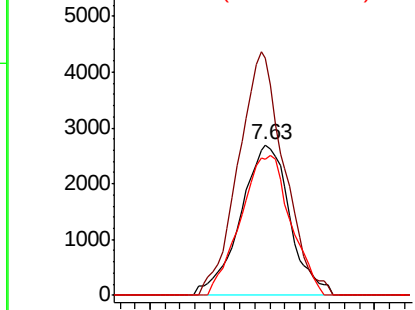



#33
1,2-Dichloroethane-d4
Concen: 52.799 ug/l
RT: 7.99 min Scan# 1943
Delta R.T. 0.00 min
Lab File: VN063825.D
Acq: 2 Oct 2020 16:44

Tgt Ion: 65 Resp: 184653
Ion Ratio Lower Upper
65 100
67 50.2 0.0 99.6



Abundance Ion 64.90 (64.60 to 65.60): VN0
Ion 66.90 (66.60 to 67.60): VN0

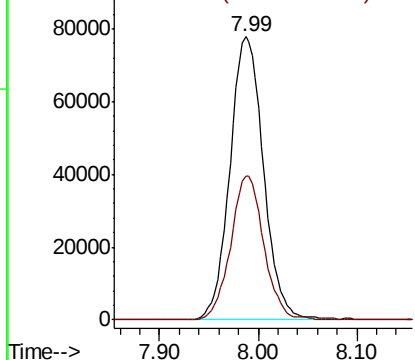


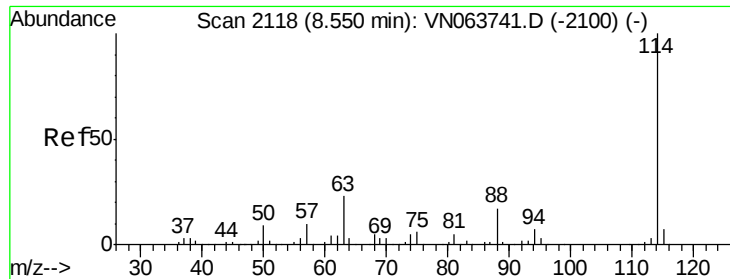




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2118
 Delta R.T. 0.00 min
 Lab File: VN063825.D
 Acq: 2 Oct 2020 16:44

Instrument :
 MSVOA_N
 ClientSampleId :
 PB132030ZHE#04

Tot Ion:114 Resp: 398044
 Ion Ratio Lower Upper
 114 100
 63 23.0 0.0 45.0
 88 16.4 0.0 34.0

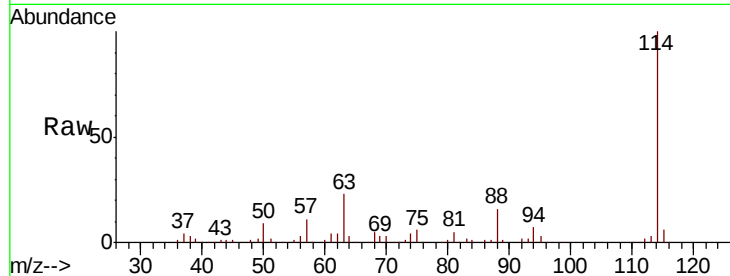


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VN
 Ion 87.90 (87.60 to 88.60): VN

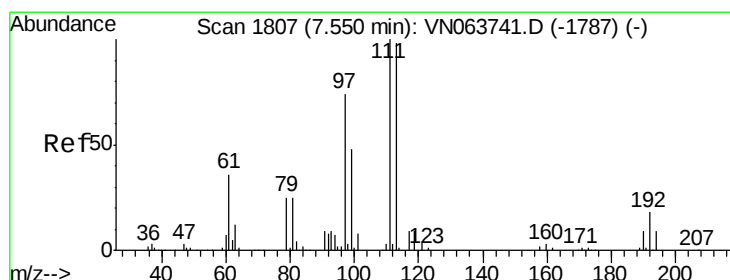
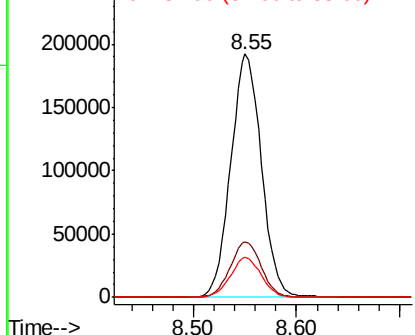



#35
 Dibromofluoromethane
 Concen: 48.194 ug/l
 RT: 7.55 min Scan# 1807
 Delta R.T. 0.00 min
 Lab File: VN063825.D
 Acq: 2 Oct 2020 16:44

Tgt Ion:113 Resp: 133109
 Ion Ratio Lower Upper
 113 100
 111 101.2 81.8 122.8
 192 18.2 14.2 21.2



Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V




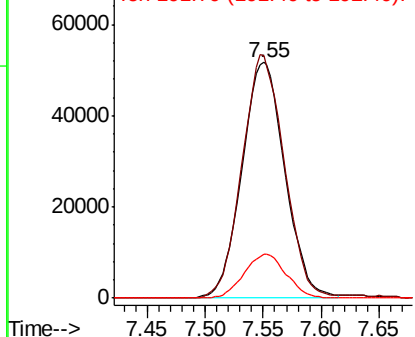


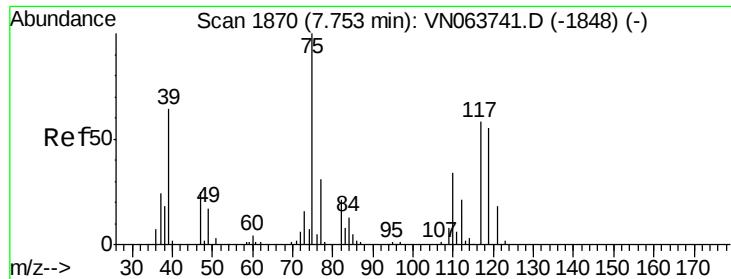

#36
 1,1-Dichloropropene
 Concen: 4.709 ug/l
 RT: 7.63 min Scan# 1831
 Delta R.T. -0.13 min
 Lab File: VN063825.D
 Acq: 2 Oct 2020 16:44




Instrument :
 MSVOA_N
 ClientSampleId :
 PB132030ZHE#04


Tot Ion: 75 Resp: 18988
 Ion Ratio Lower Upper
 75 100
 110 9.5 16.9 50.6#
 77 0.0 24.5 36.7#

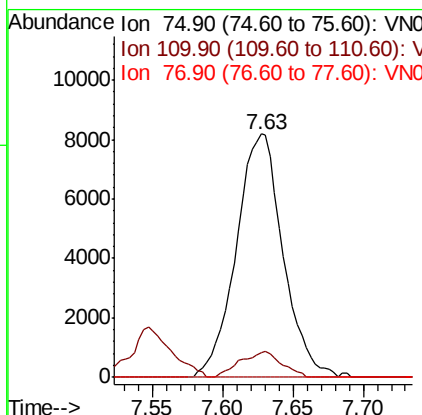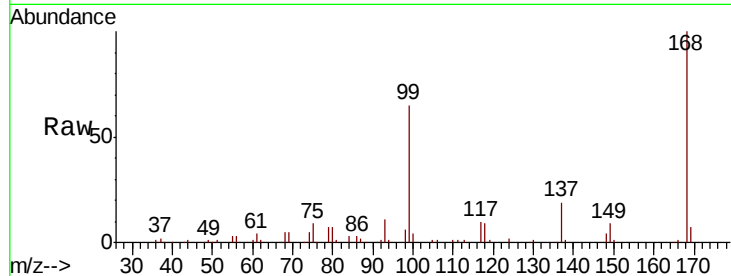

#37
 Ethyl Acetate
 Concen: 4.020 ug/l
 RT: 6.79 min Scan# 1572
 Delta R.T. -0.09 min
 Lab File: VN063825.D
 Acq: 2 Oct 2020 16:44

Tgt Ion: 43 Resp: 16107
 Ion Ratio Lower Upper
 43 100
 61 0.0 10.4 15.6#
 70 0.0 7.3 10.9#

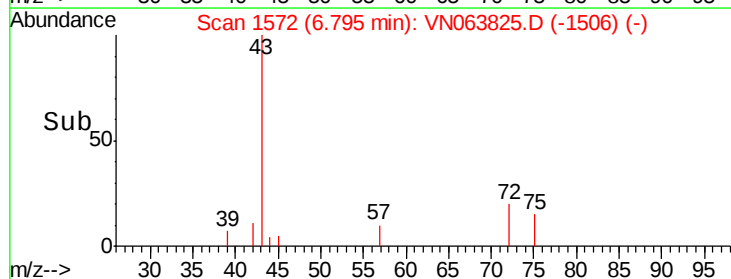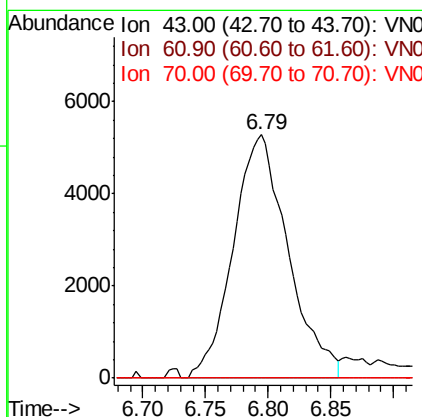

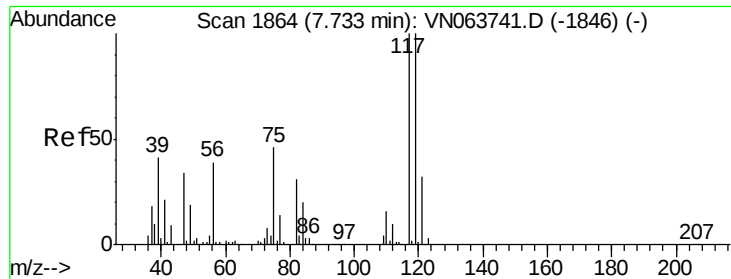

#38

Carbon Tetrachloride

Concen: 5.291 ug/l

RT: 7.62 min Scan# 1830

Delta R.T. -0.11 min

Lab File: VN063825.D

Acq: 2 Oct 2020 16:44

Instrument :

MSVOA_N

ClientSampleId :

PB132030ZHE#04


Tot Ion:117 Resp: 23924

Ion Ratio Lower Upper

117 100

119 8.1 80.1 120.1#




121 0.0 25.7 38.5#

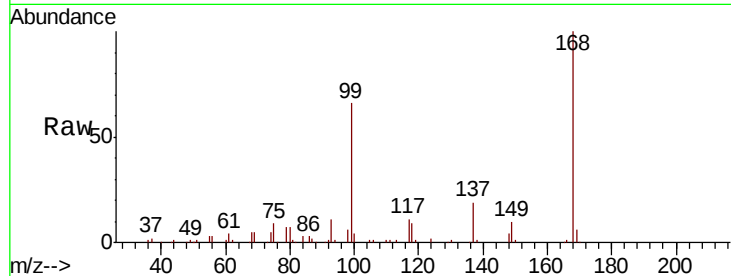

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

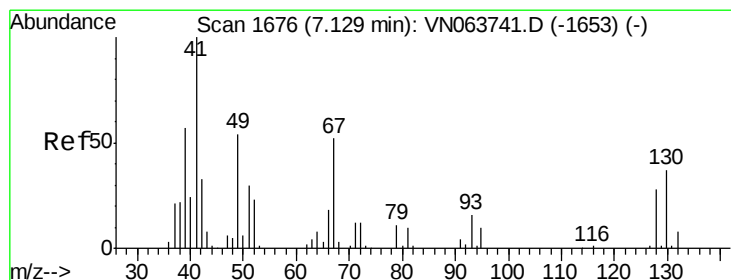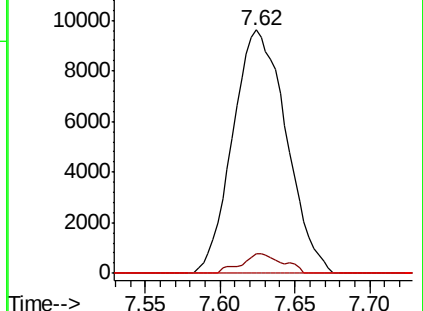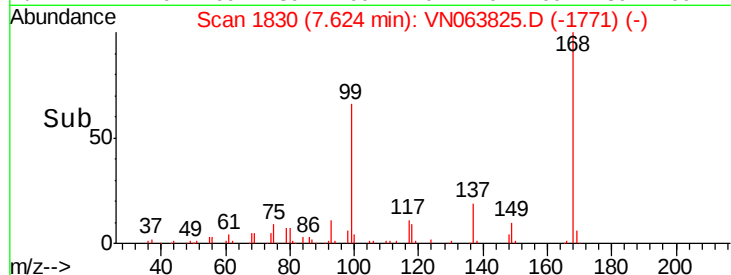

#41

Methacrylonitrile

Concen: 0.217 ug/l

RT: 7.15 min Scan# 1684

Delta R.T. 0.03 min

Lab File: VN063825.D

Acq: 2 Oct 2020 16:44

Tgt Ion: 41 Resp: 386


Ion Ratio Lower Upper

41 100

39 231.3 42.5 63.7#

67 0.0 57.4 86.2#

52 0.0 26.9 40.3#






Abundance Ion 41.00 (40.70 to 41.70): V

Ion 39.00 (38.70 to 39.70): V

Ion 67.00 (66.70 to 67.70): V

Ion 52.00 (51.70 to 52.70): V

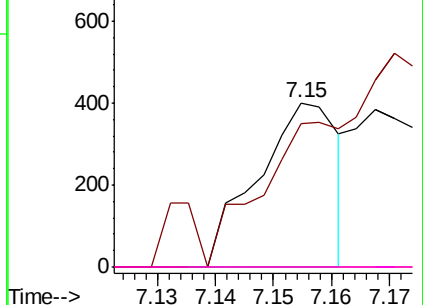



#43

Isopropyl Acetate

Concen: 10.208 ug/l

RT: 8.13 min Scan# 1986

Delta R.T. 0.00 min

Lab File: VN063825.D

Acq: 2 Oct 2020 16:44

Instrument :

MSVOA_N

ClientSampleId :

PB132030ZHE#04


Tot Ion: 43 Resp: 67459

Ion Ratio Lower Upper

43 100

61 17.4 14.2 21.4




87 11.5 9.0 13.6

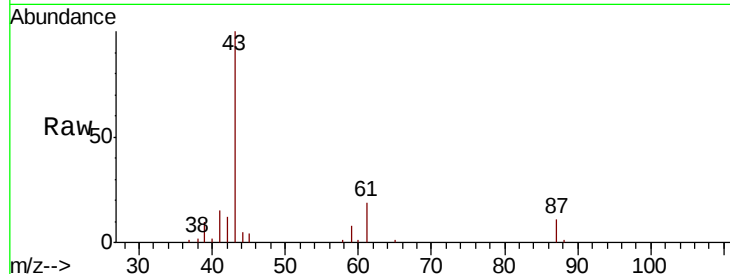

Abundance Ion 43.00 (42.70 to 43.70): VN063825.D (-1986) (-)

Ion 61.00 (60.70 to 61.70): VN063825.D (-1986) (-)

Ion 87.00 (86.70 to 87.70): VN063825.D (-1986) (-)

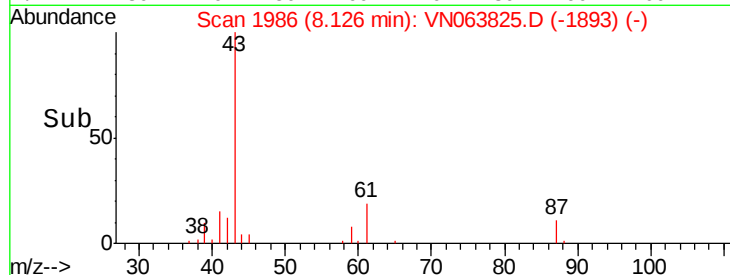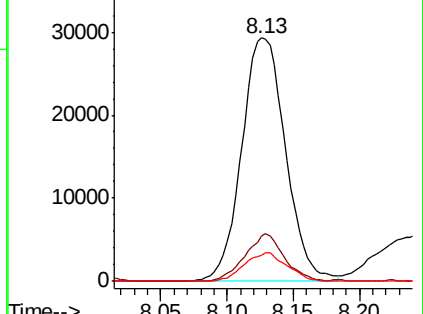

#45

1,2-Dichloropropane

Concen: 0.380 ug/l

RT: 9.24 min Scan# 2332

Delta R.T. 0.15 min

Lab File: VN063825.D


Acq: 2 Oct 2020 16:44

Tgt Ion: 63 Resp: 1183

Ion Ratio Lower Upper



63 100


65 0.0 24.7 37.1#

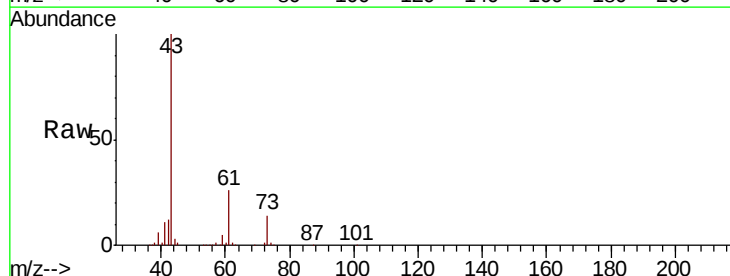

Abundance Ion 62.90 (62.60 to 63.60): VN063825.D (-2191) (-)

Ion 64.90 (64.60 to 65.60): VN063825.D (-2191) (-)

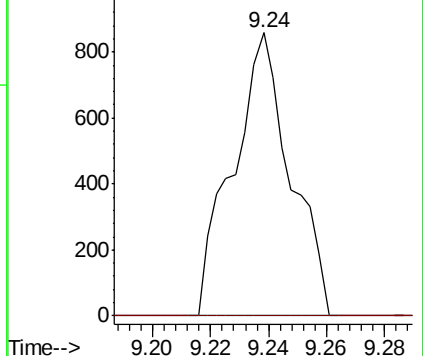


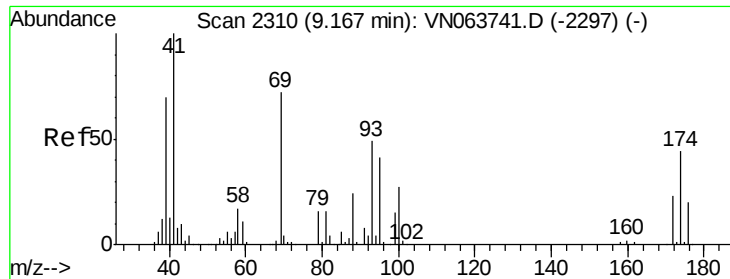




#48
Methvl methacrylate
Concen: 1.843 ug/l
RT: 9.14 min Scan# 2303
Delta R.T. -0.02 min
Lab File: VN063825.D
Acq: 2 Oct 2020 16:44

Instrument :
MSVOA_N
ClientSampleId :
PB132030ZHE#04

Tot Ion: 41 Resp: 6018
Ion Ratio Lower Upper
41 100
69 0.0 60.9 91.3#
39 40.8 57.5 86.3#




Abundance Ion 41.00 (40.70 to 41.70): VN0
Ion 69.00 (68.70 to 69.70): VN0
Ion 39.00 (38.70 to 39.70): VN0


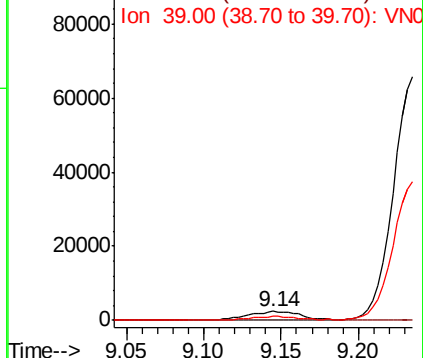



#50
Toluene-d8
Concen: 49.227 ug/l
RT: 10.06 min Scan# 2588
Delta R.T. 0.00 min
Lab File: VN063825.D
Acq: 2 Oct 2020 16:44

Tgt Ion: 98 Resp: 515421
Ion Ratio Lower Upper
98 100
100 63.4 49.8 74.6



Abundance Ion 98.00 (97.70 to 98.70): VN0
Ion 100.00 (99.70 to 100.70): VN0




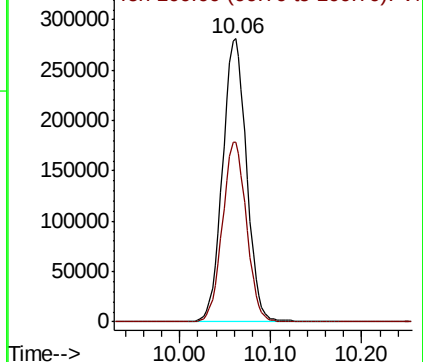




#51
4-Methyl-2-Pentanone
Concen: 1.926 ug/l
RT: 9.96 min Scan# 2555
Delta R.T. 0.00 min
Lab File: VN063825.D
Acq: 2 Oct 2020 16:44




Instrument :
MSVOA_N
ClientSampleId :
PB132030ZHE#04


Tot Ion: 43 Resp: 7468
Ion Ratio Lower Upper
43 100
58 44.7 28.4 42.6#

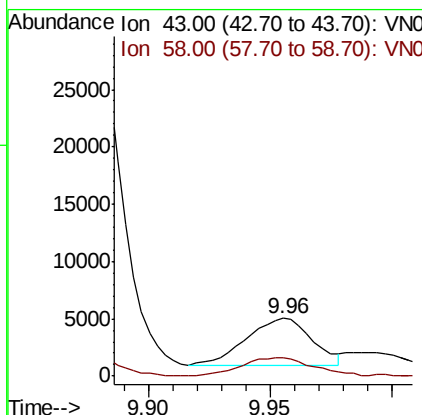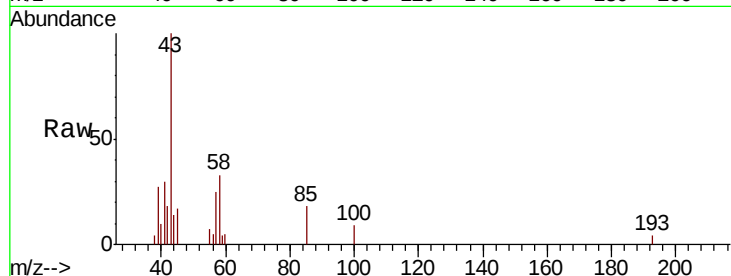

#54
cis-1,3-Dichloropropene
Concen: 4.897 ug/l
RT: 9.87 min Scan# 2529
Delta R.T. 0.06 min
Lab File: VN063825.D
Acq: 2 Oct 2020 16:44

Tgt Ion: 75 Resp: 24279
Ion Ratio Lower Upper
75 100
77 0.0 24.6 36.8#
39 51.9 49.7 74.5

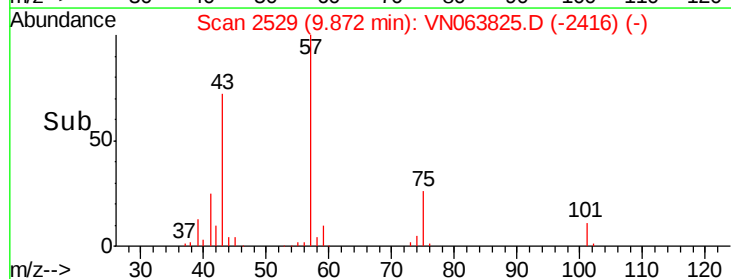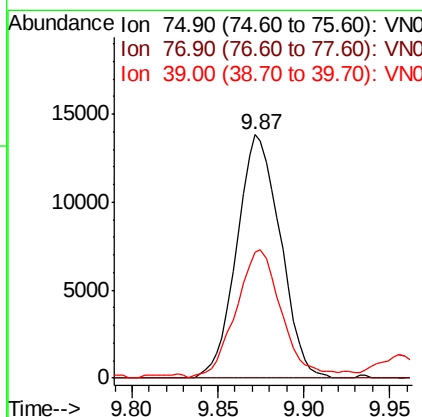

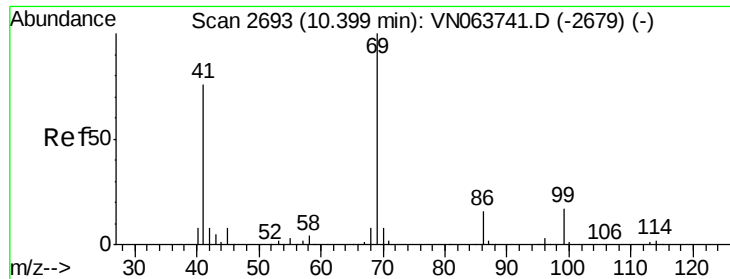

#56

Ethyl methacrylate

Concen: 0.448 ug/l

RT: 10.52 min Scan# 2730

Delta R.T. 0.12 min

Lab File: VN063825.D

Acq: 2 Oct 2020 16:44

Instrument :

MSVOA_N

ClientSampleId :

PB132030ZHE#04


Tot Ion: 69 Resp: 1814

Ion Ratio Lower Upper

69 100

41 4122.9 61.1 91.7#




39 1894.4 42.2 63.4#

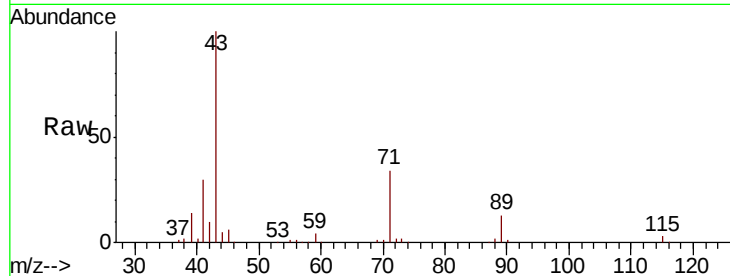

Abundance Ion 69.00 (68.70 to 69.70): VN063825.D (-2600) (-)

Ion 41.00 (40.70 to 41.70): VN063825.D (-2600) (-)

Ion 39.00 (38.70 to 39.70): VN063825.D (-2600) (-)

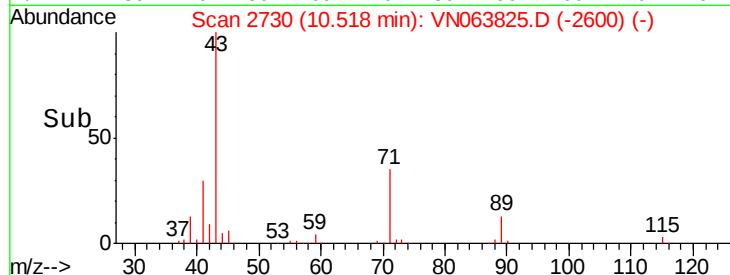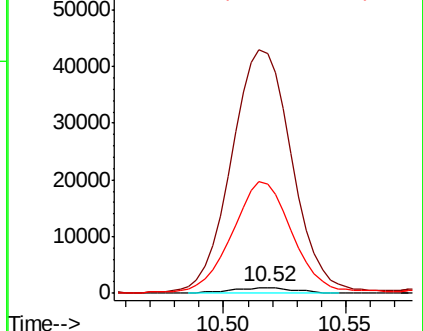

#57

1,3-Dichloropropane

Concen: 0.929 ug/l

RT: 10.74 min Scan# 2799

Delta R.T. 0.06 min

Lab File: VN063825.D


Acq: 2 Oct 2020 16:44

Tgt Ion: 76 Resp: 4491

Ion Ratio Lower Upper



76 100


78 0.0 25.2 37.8#



Abundance Ion 75.90 (75.60 to 76.60): VN063825.D (-2687) (-)

Ion 77.90 (77.60 to 78.60): VN063825.D (-2687) (-)




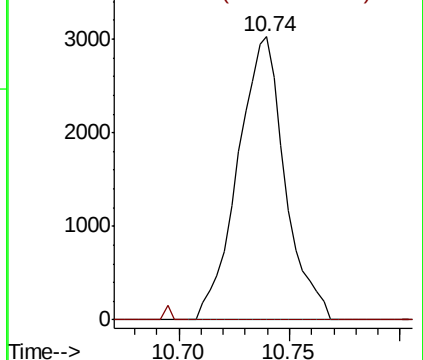




#59
2-Hexanone
Concen: 27.627 ug/l
RT: 10.74 min Scan# 2798
Delta R.T. 0.02 min
Lab File: VN063825.D
Acq: 2 Oct 2020 16:44




Instrument :
MSVOA_N
ClientSampleId :
PB132030ZHE#04


Tot Ion: 43 Resp: 79592
Ion Ratio Lower Upper
43 100
58 20.1 24.6 73.8#

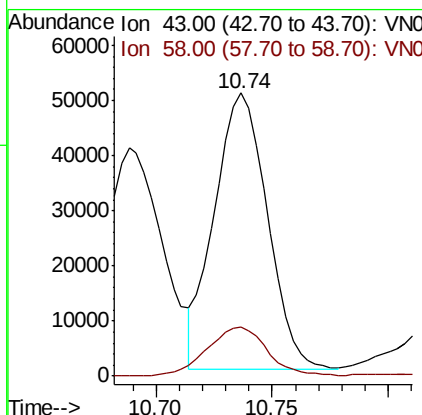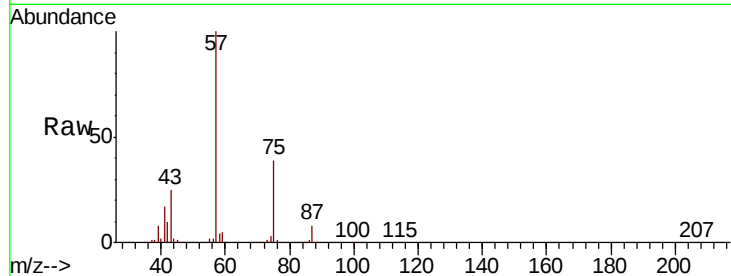

#62
4-Bromofluorobenzene
Concen: 52.235 ug/l
RT: 12.38 min Scan# 3308
Delta R.T. 0.00 min
Lab File: VN063825.D
Acq: 2 Oct 2020 16:44

Tgt Ion: 95 Resp: 205591
Ion Ratio Lower Upper
95 100
174 75.8 0.0 150.6
176 72.7 0.0 145.4

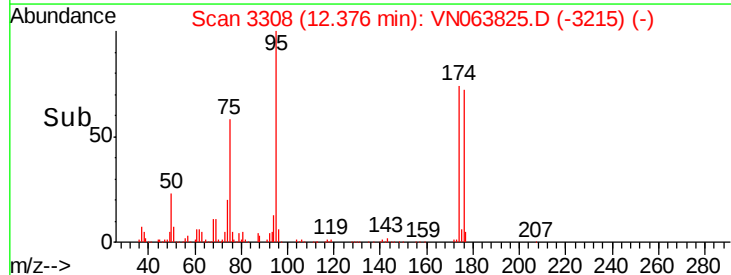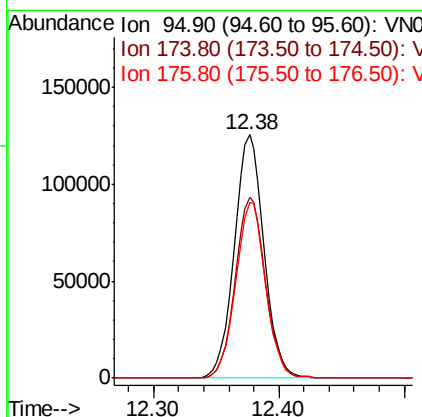


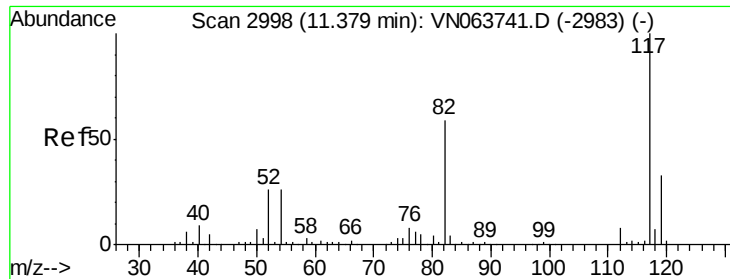




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2998
Delta R.T. 0.00 min
Lab File: VN063825.D
Acq: 2 Oct 2020 16:44

Instrument :
MSVOA_N
ClientSampleId :
PB132030ZHE#04

Tot Ion:117 Resp: 419540
Ion Ratio Lower Upper
117 100
82 57.9 47.4 71.2
119 31.8 26.4 39.6

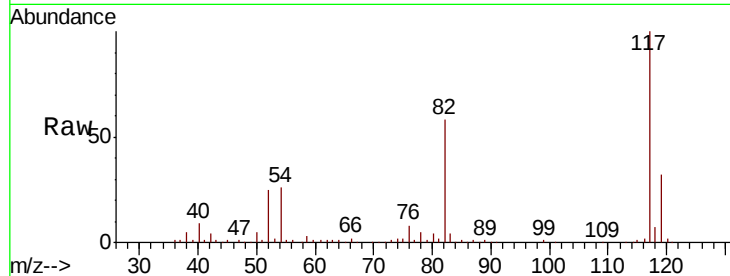


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

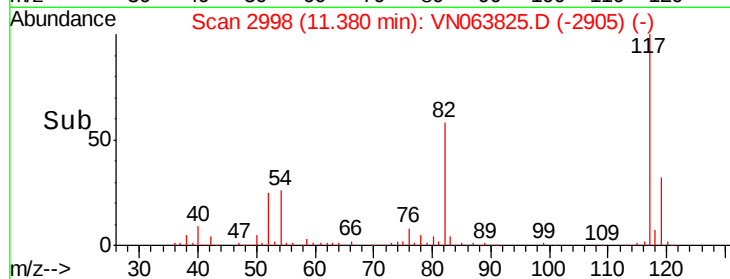
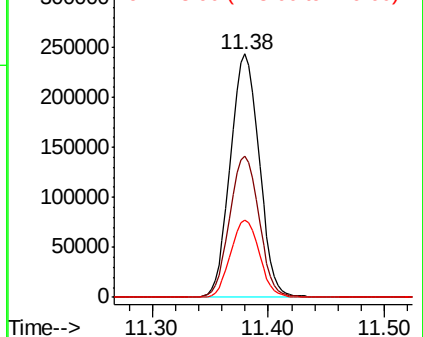



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.32 min Scan# 3601
Delta R.T. 0.00 min
Lab File: VN063825.D
Acq: 2 Oct 2020 16:44

Tgt Ion:152 Resp: 172680
Ion Ratio Lower Upper
152 100
115 61.2 31.3 93.8
150 156.4 0.0 341.8



Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

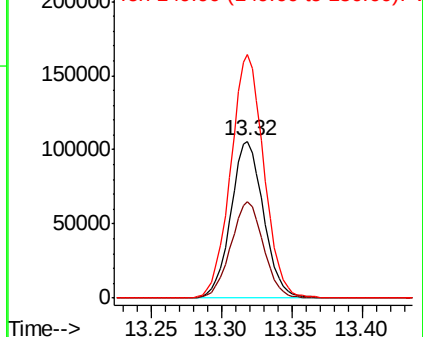



#74

N-amyl acetate

Concen: 3.118 ug/l

RT: 12.00 min Scan# 3192

Delta R.T. -0.04 min

Lab File: VN063825.D

Acq: 2 Oct 2020 16:44

Instrument :

MSVOA_N

ClientSampleId :

PB132030ZHE#04

Tot Ion: 43 Resp: 5528





Ion Ratio Lower Upper

43 100

70 0.0 29.8 44.8#

55 5.7 17.9 26.9#

61 0.0 17.0 25.4#

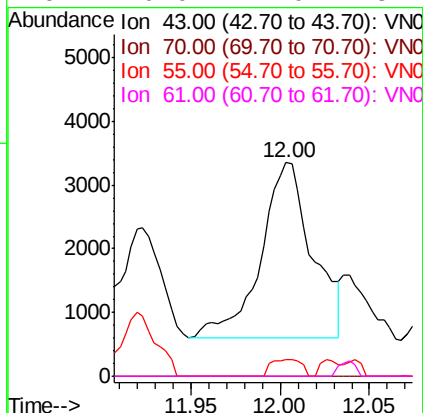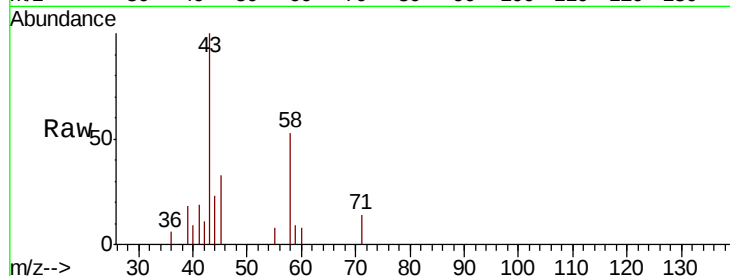

#76

1,2,3-Trichloropropane

Concen: 31.065 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. -0.15 min

Lab File: VN063825.D




Acq: 2 Oct 2020 16:44


Tgt Ion: 75 Resp: 118250

Ion Ratio Lower Upper

75 100

77 1.0 0.0 0.0#


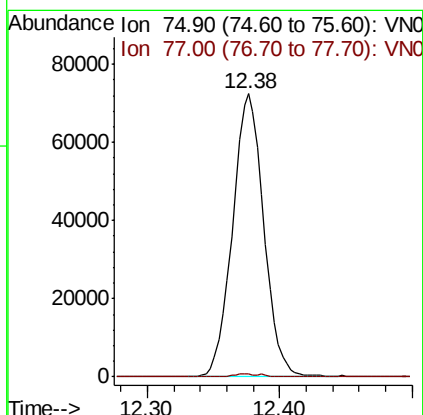






#80
 1,3,5-Trimethylbenzene
 Concen: 0.246 ug/l
 RT: 12.71 min Scan# 3412
 Delta R.T. 0.00 min
 Lab File: VN063825.D
 Acq: 2 Oct 2020 16:44




Instrument :
 MSVOA_N
 ClientSampleId :
 PB132030ZHE#04


Tot Ion:105 Resp: 2601
 Ion Ratio Lower Upper
 105 100
 120 53.8 23.3 69.9

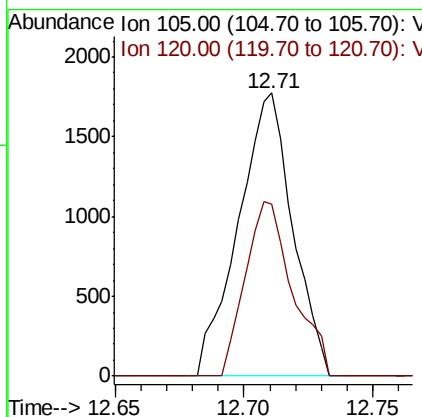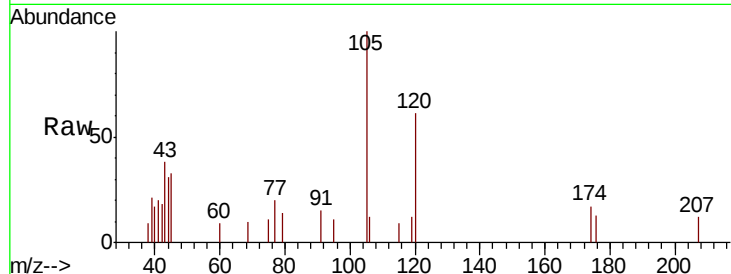

#81
 trans-1,4-Dichloro-2-butene
 Concen: 89.472 ug/l
 RT: 12.38 min Scan# 3308
 Delta R.T. 0.10 min
 Lab File: VN063825.D
 Acq: 2 Oct 2020 16:44

Tgt Ion: 75 Resp: 118250
 Ion Ratio Lower Upper
 75 100
 53 0.1 88.2 132.2#
 89 0.0 36.0 54.0#

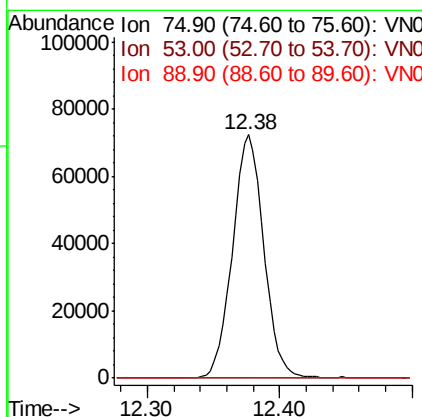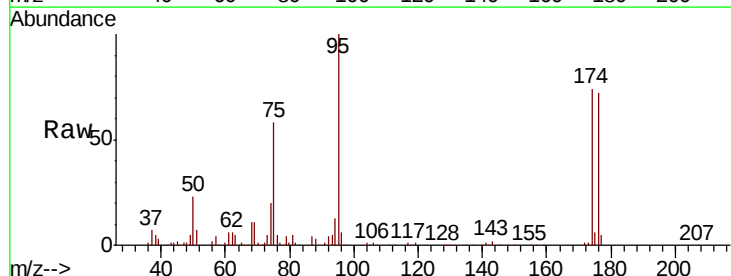

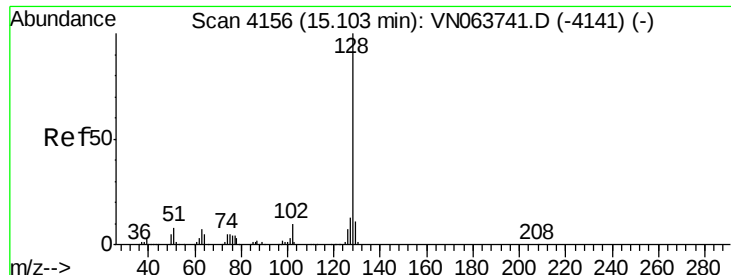

#95

Naphthalene

Concen: 1.935 ug/l

RT: 15.11 min Scan# 4159

Delta R.T. 0.01 min

Lab File: VN063825.D

Acq: 2 Oct 2020 16:44

Instrument :

MSVOA_N

ClientSampleId :

PB132030ZHE#04


Tot Ion:128 Resp: 104

Ion Ratio Lower Upper

128 100

127 0.0 10.5 15.7#

129 0.0 8.7 13.1#



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

