
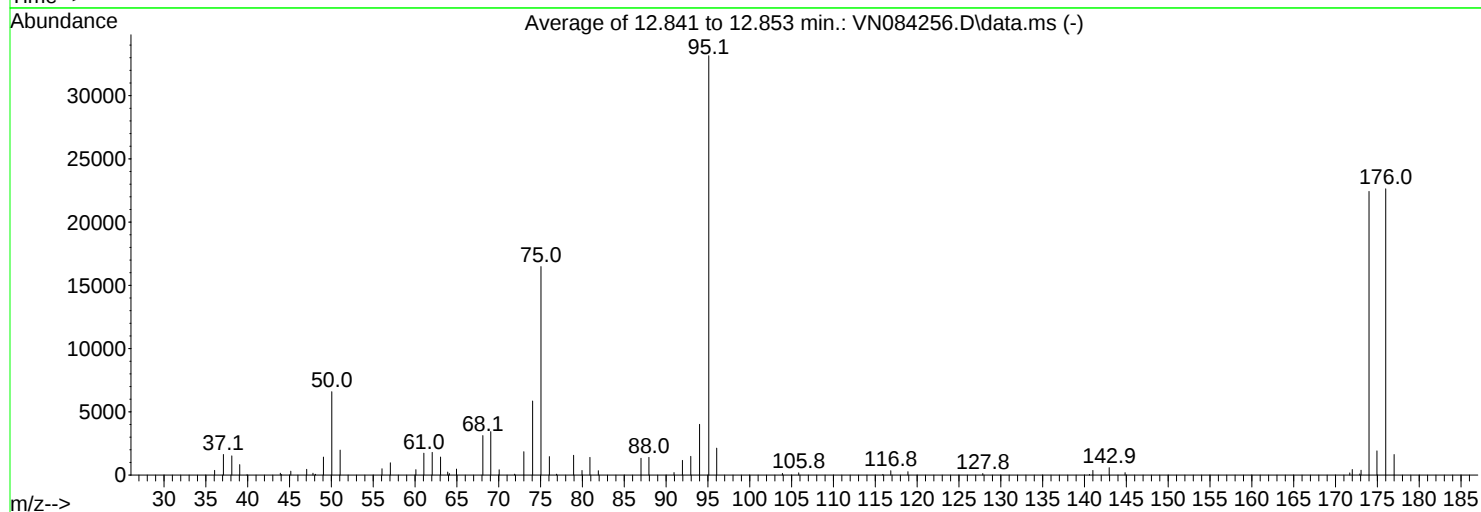


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100224\
Data File : VN084256.D
Acq On : 02 Oct 2024 10:42
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N093024W.M
Title : SW846 8260
Last Update : Tue Oct 01 07:11:01 2024

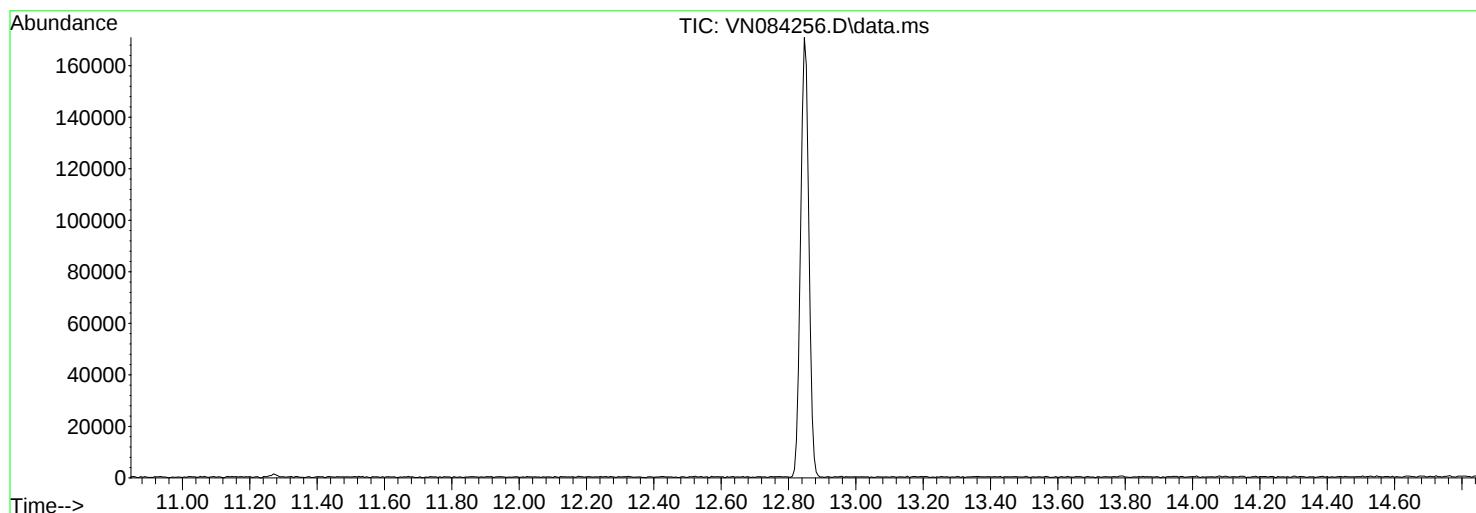

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	6592	PASS
75	95	30	60	49.7	16487	PASS
95	95	100	100	100.0	33157	PASS
96	95	5	9	6.4	2130	PASS
173	174	0.00	2	1.7	385	PASS
174	95	50	100	67.6	22427	PASS
175	174	5	9	8.5	1912	PASS
176	174	95	101	100.9	22635	PASS
177	176	5	9	7.2	1627	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	372	49.05	1424	64.95	476	79.95	364
37.10	1631	50.05	6592	68.10	3123	80.90	1402
38.10	1521	51.05	1975	69.05	3436	81.90	342
39.05	828	56.05	502	70.05	420	87.00	1329
39.90	13	57.05	972	71.90	75	87.95	1401
43.90	148	60.10	431	73.00	1848	90.95	202
44.05	41	61.05	1732	74.05	5859	91.95	1163
45.15	307	62.05	1795	75.05	16487	92.95	1483
47.05	454	63.05	1427	76.05	1462	94.00	4011
47.80	149	63.90	239	76.90	73	95.10	33157
48.10	67	64.10	116	78.95	1564	96.05	2130

Average of 12.841 to 12.853 min.: VN084256.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
103.90	133	172.00	442				
105.85	181	172.90	89				
115.90	53	173.05	385				
116.85	347	174.00	22427				
118.90	271	174.95	1912				
127.85	123	176.00	22635				
140.60	51	177.00	1627				
141.00	370						
142.95	584						
144.85	193						
171.70	173						

Instrument :

MSVOA_N

ClientSampleId :

BFB