
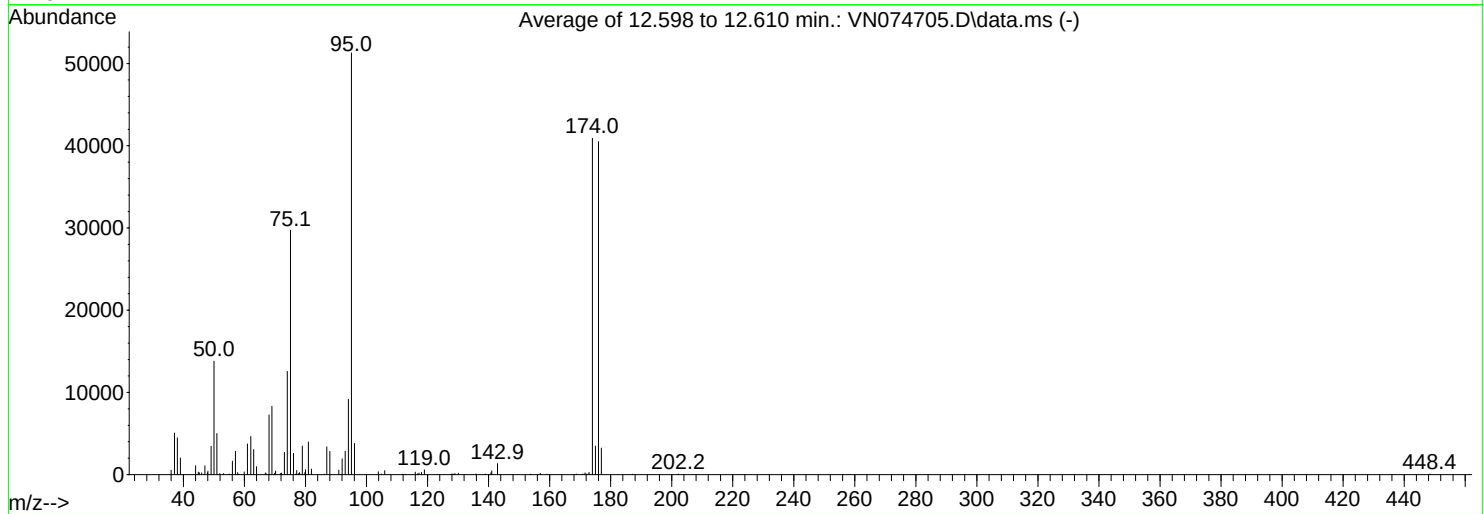


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100322\
Data File : VN074705.D
Acq On : 03 Oct 2022 12:31
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100322W.M
Title : SW846 8260
Last Update : Tue Oct 04 05:54:56 2022

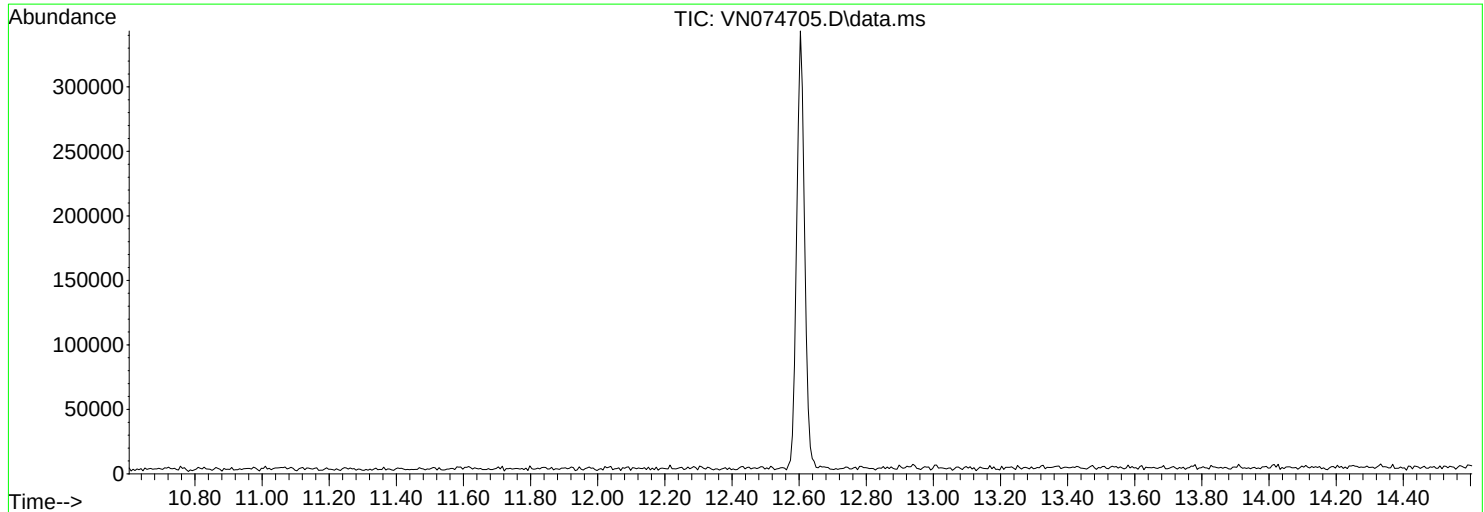

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	26.9	13797	PASS
75	95	30	60	57.9	29709	PASS
95	95	100	100	100.0	51299	PASS
96	95	5	9	7.4	3793	PASS
173	174	0.00	2	0.7	278	PASS
174	95	50	100	79.8	40912	PASS
175	174	5	9	8.5	3489	PASS
176	174	95	101	99.0	40491	PASS
177	176	5	9	8.0	3227	PASS