
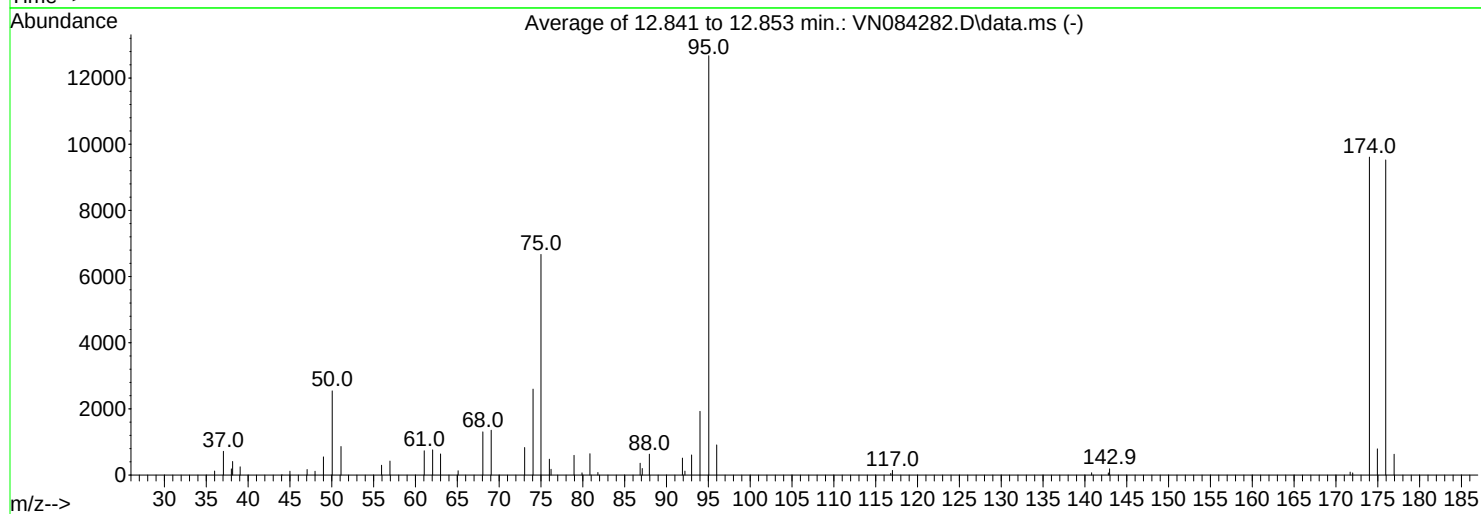


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100324\
Data File : VN084282.D
Acq On : 03 Oct 2024 08:20
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N093024W.M
Title : SW846 8260
Last Update : Tue Oct 01 07:11:01 2024

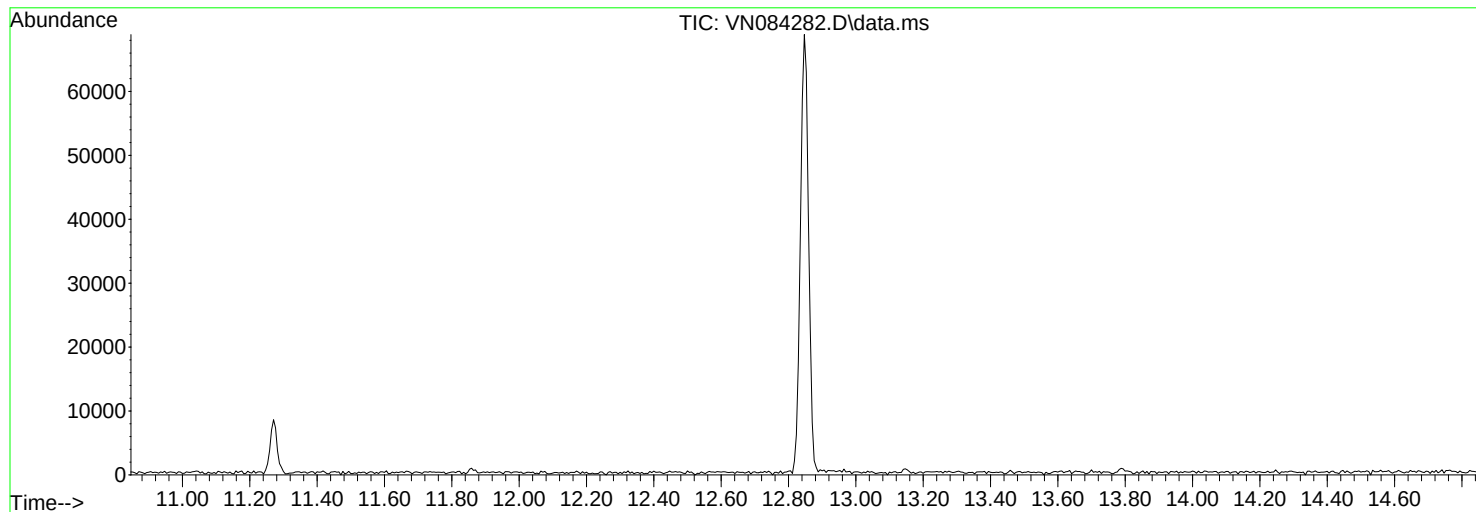

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	2545	PASS
75	95	30	60	52.6	6669	PASS
95	95	100	100	100.0	12674	PASS
96	95	5	9	7.2	911	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	75.8	9610	PASS
175	174	5	9	8.2	792	PASS
176	174	95	101	99.1	9524	PASS
177	176	5	9	6.6	630	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	122	51.10	863	75.00	6669	92.20	121
37.05	718	55.95	297	76.00	480	93.00	608
38.00	187	56.95	423	76.20	176	94.00	1927
38.15	410	61.05	734	78.95	596	95.05	12674
39.05	250	62.05	761	79.90	67	96.00	911
44.05	8	63.00	639	80.85	646	116.80	50
45.00	118	65.10	130	81.80	79	117.00	142
47.05	168	68.05	1306	86.85	358	140.80	69
48.00	116	69.05	1355	87.10	199	142.80	65
49.00	550	73.05	833	87.95	633	142.95	188
50.05	2545	74.05	2599	91.90	513	171.70	90

Average of 12.841 to 12.853 min.: VN084282.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
172.00	65						
174.00	9610						
174.95	792						
175.95	9524						
176.95	630						

Instrument :

MSVOA_N

ClientSampleId :

BFB