



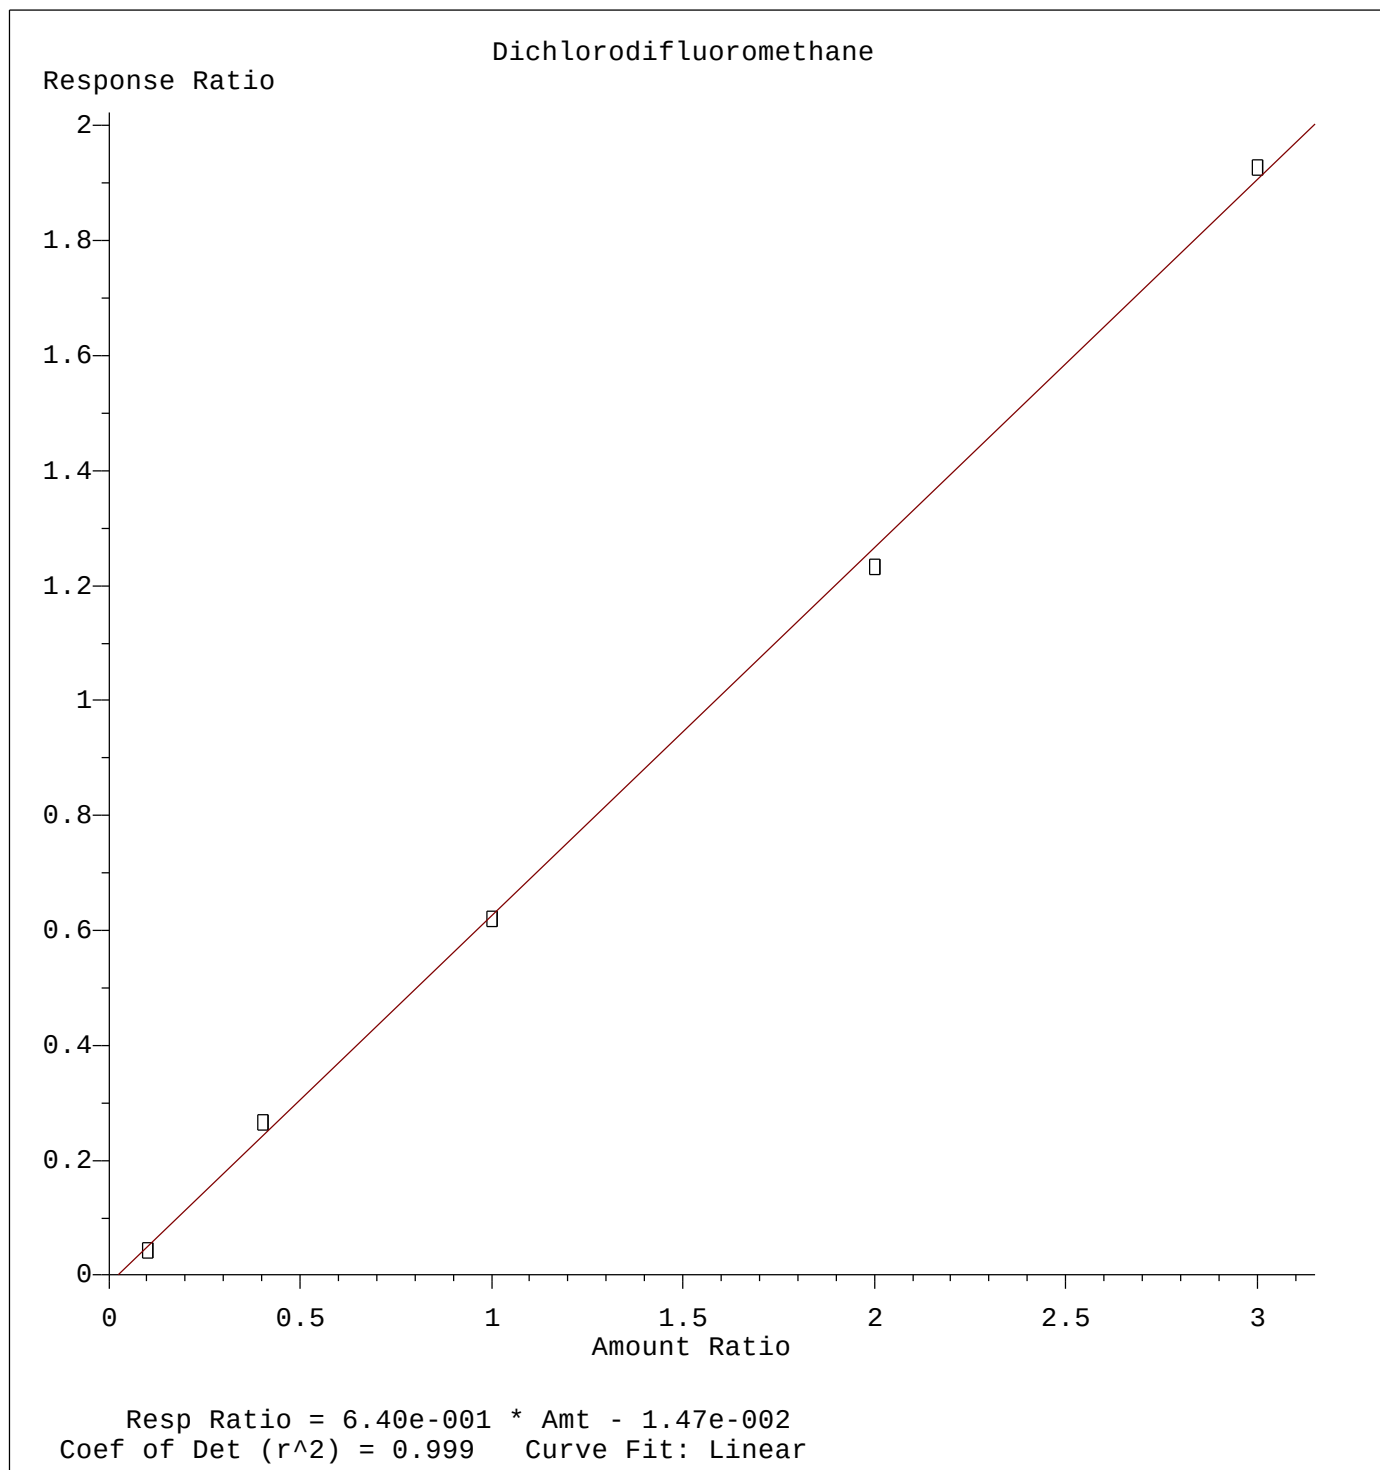

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N100418W.M
Calibration Table Last Updated: Mon Oct 08 13:43:30 2018

1,2,3-Trichloropropane

Response Ratio

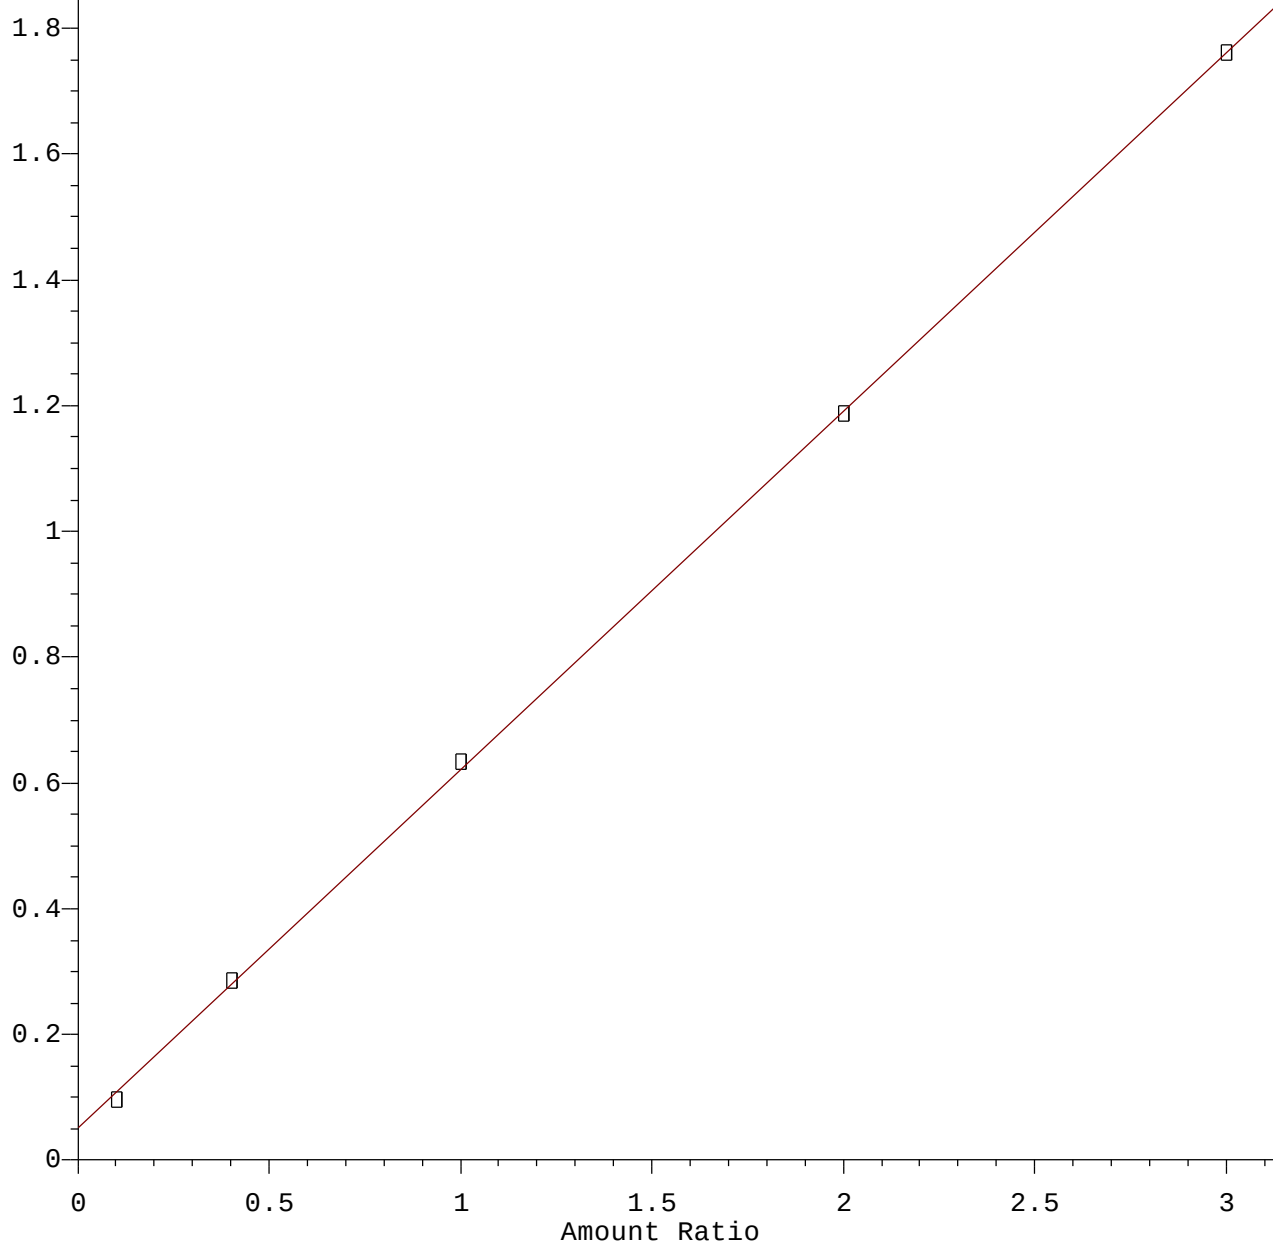


Resp Ratio = $5.70 \times 10^{-1} \times \text{Amt} + 5.10 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N100418W.M
Calibration Table Last Updated: Mon Oct 08 13:43:30 2018


1,1,2,2-Tetrachloroethane

Response Ratio

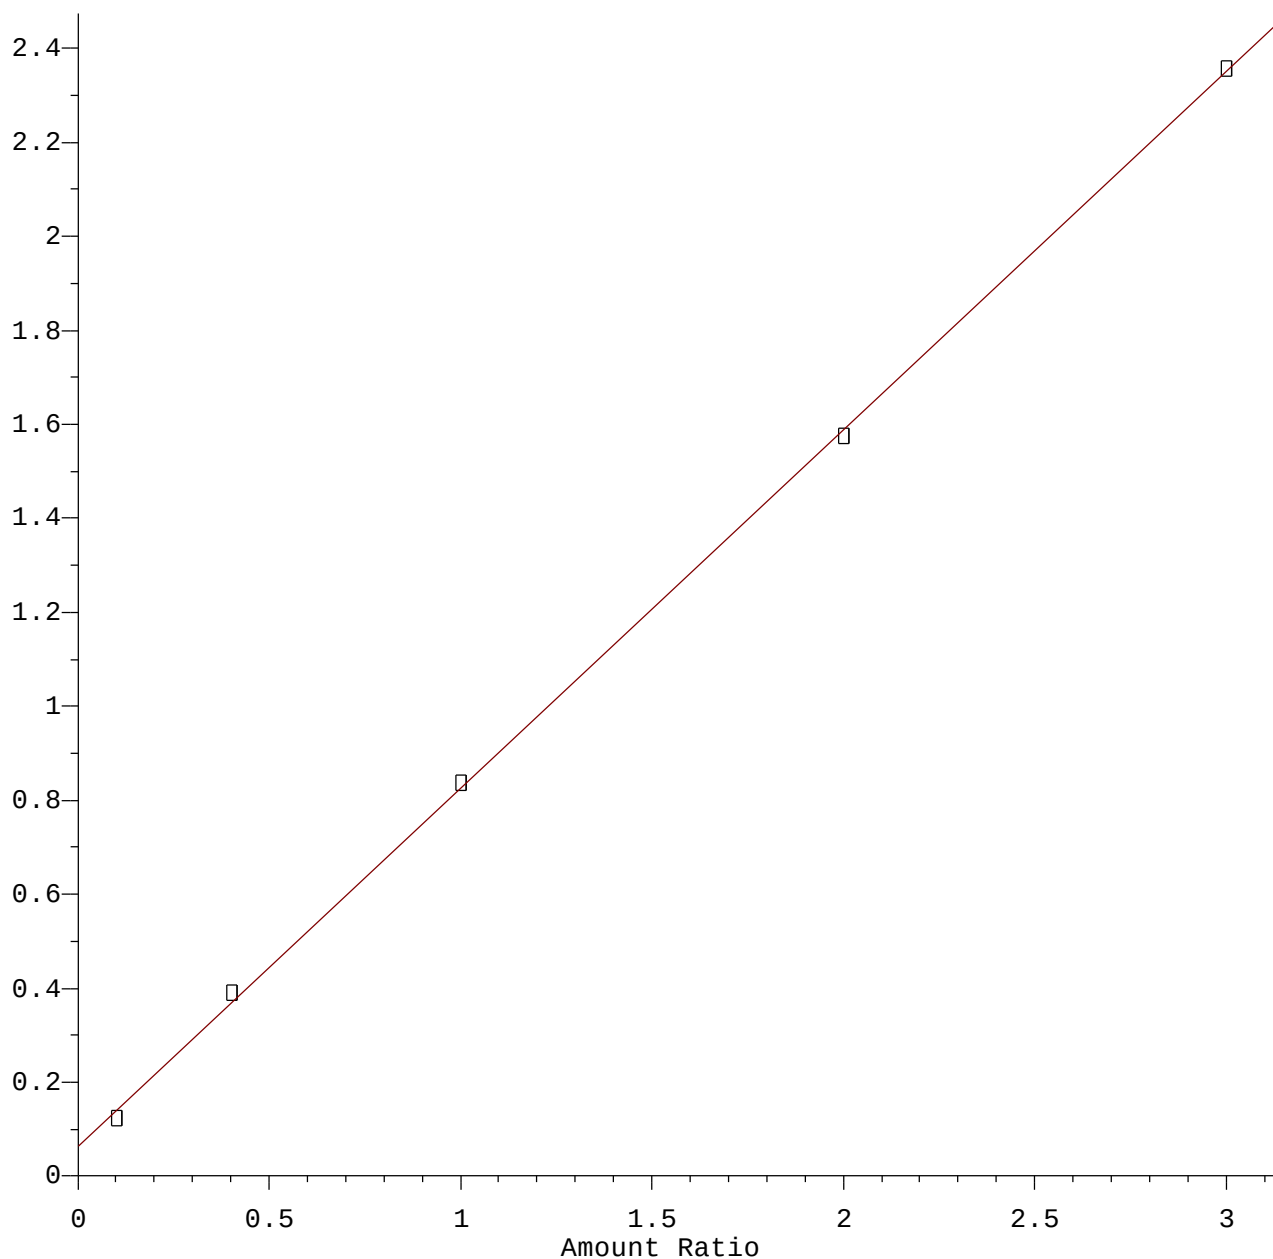


Resp Ratio = $7.62 \times 10^{-1} \times \text{Amt} + 6.40 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N100418W.M
Calibration Table Last Updated: Mon Oct 08 13:43:30 2018

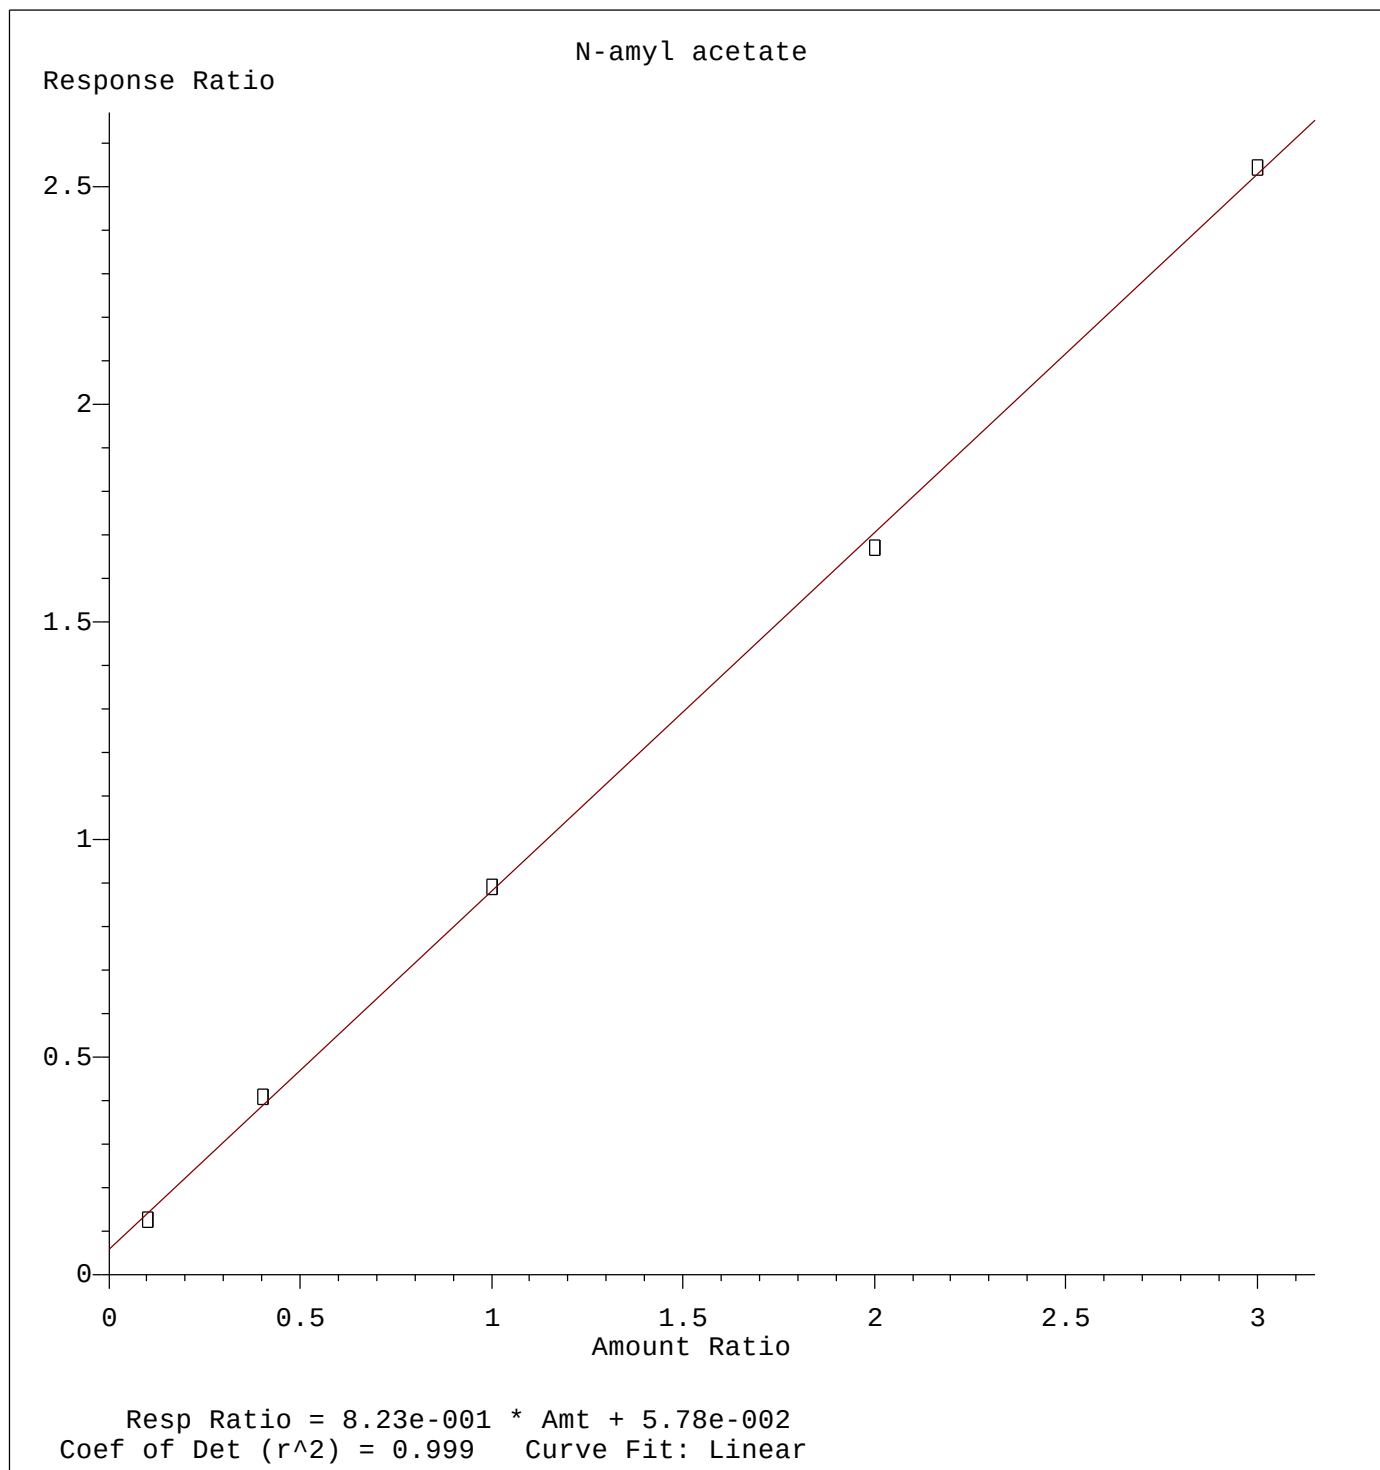


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N100418W.M
Calibration Table Last Updated: Mon Oct 08 13:43:30 2018

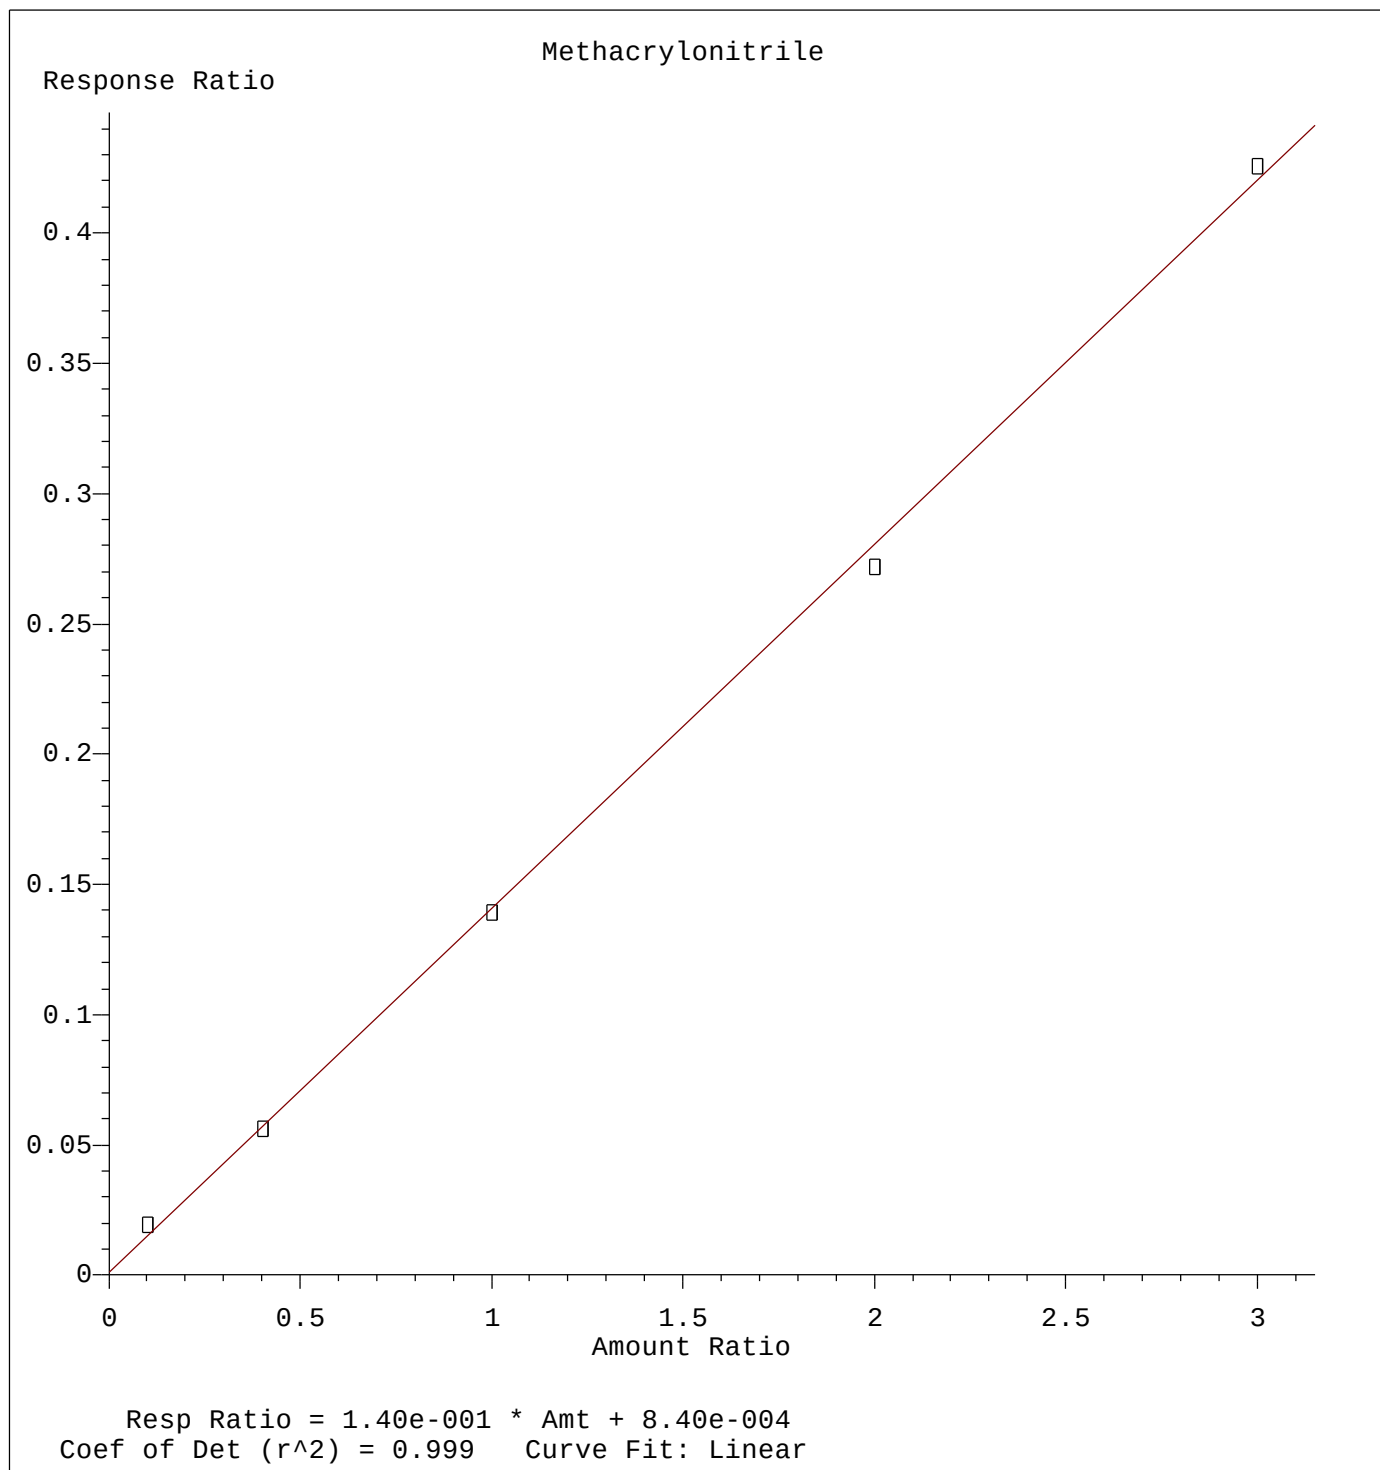

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N100418W.M
Calibration Table Last Updated: Mon Oct 08 13:43:30 2018

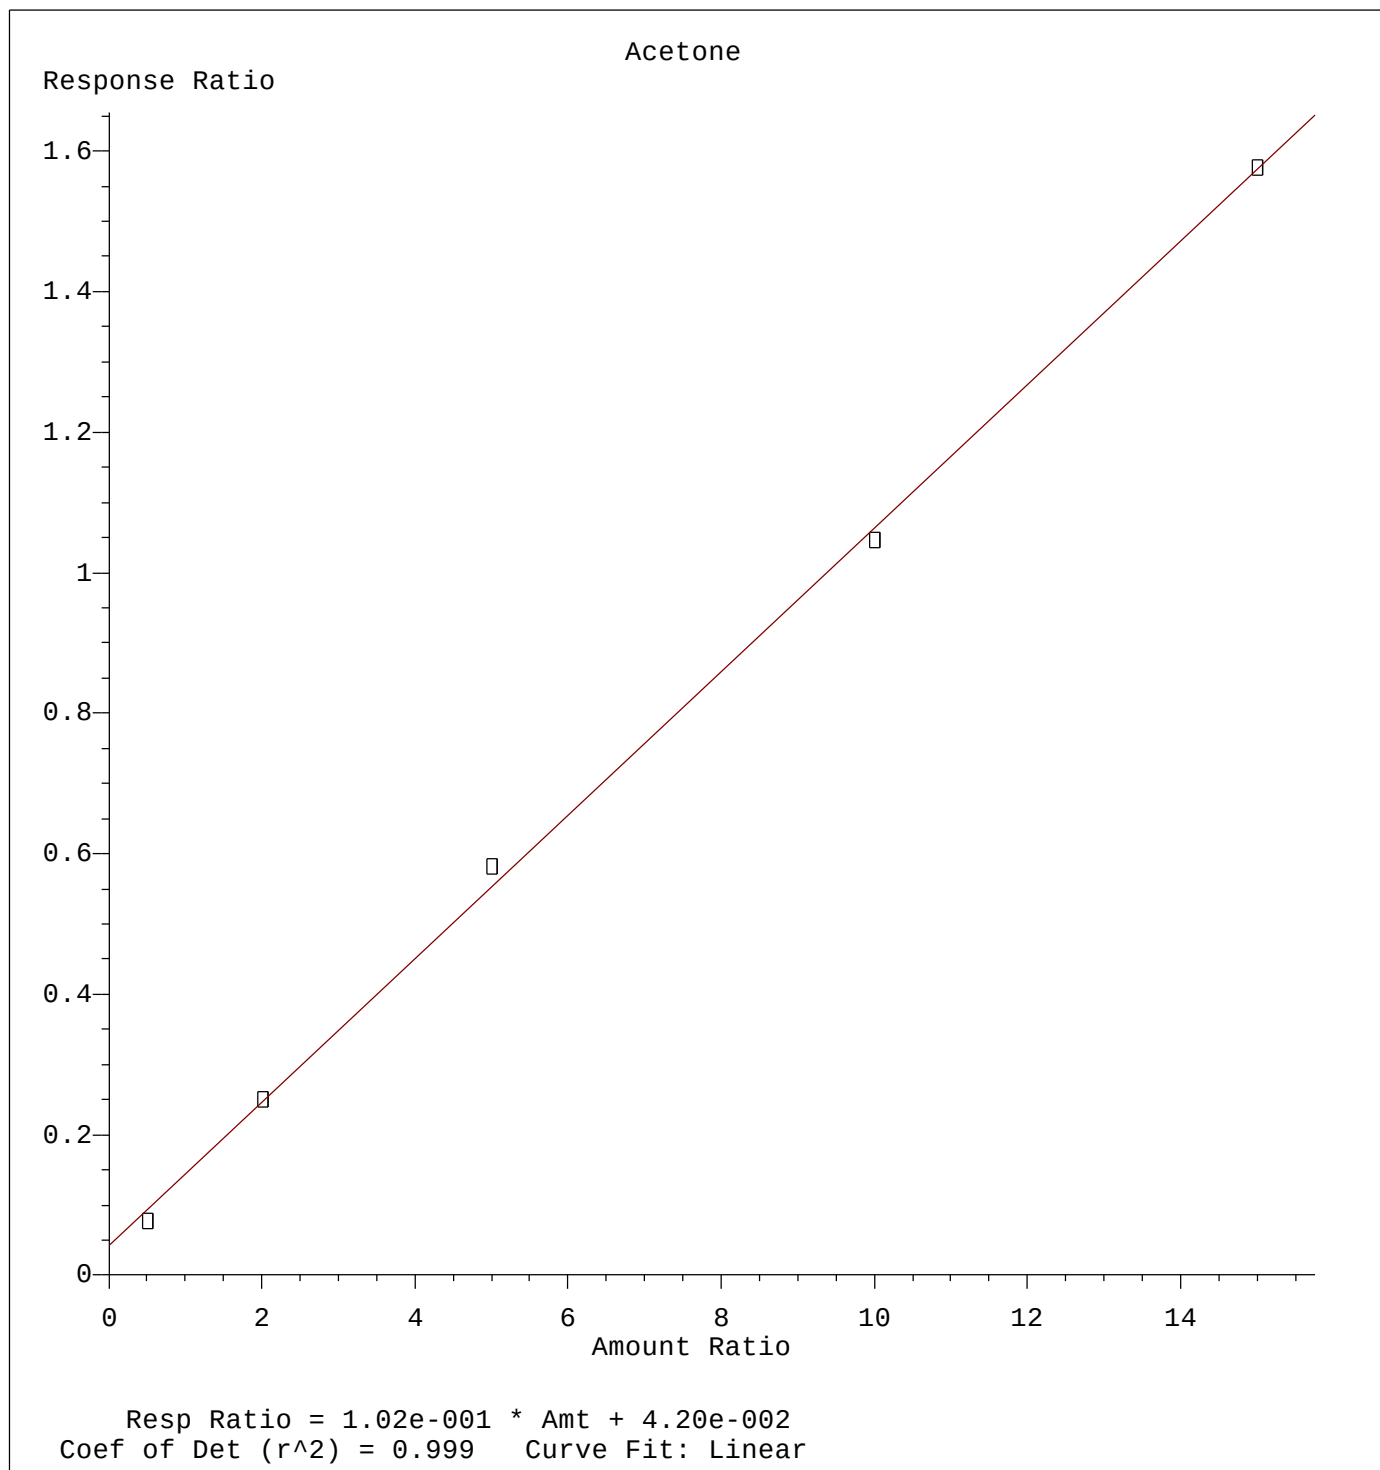


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N100418W.M
Calibration Table Last Updated: Mon Oct 08 13:43:30 2018

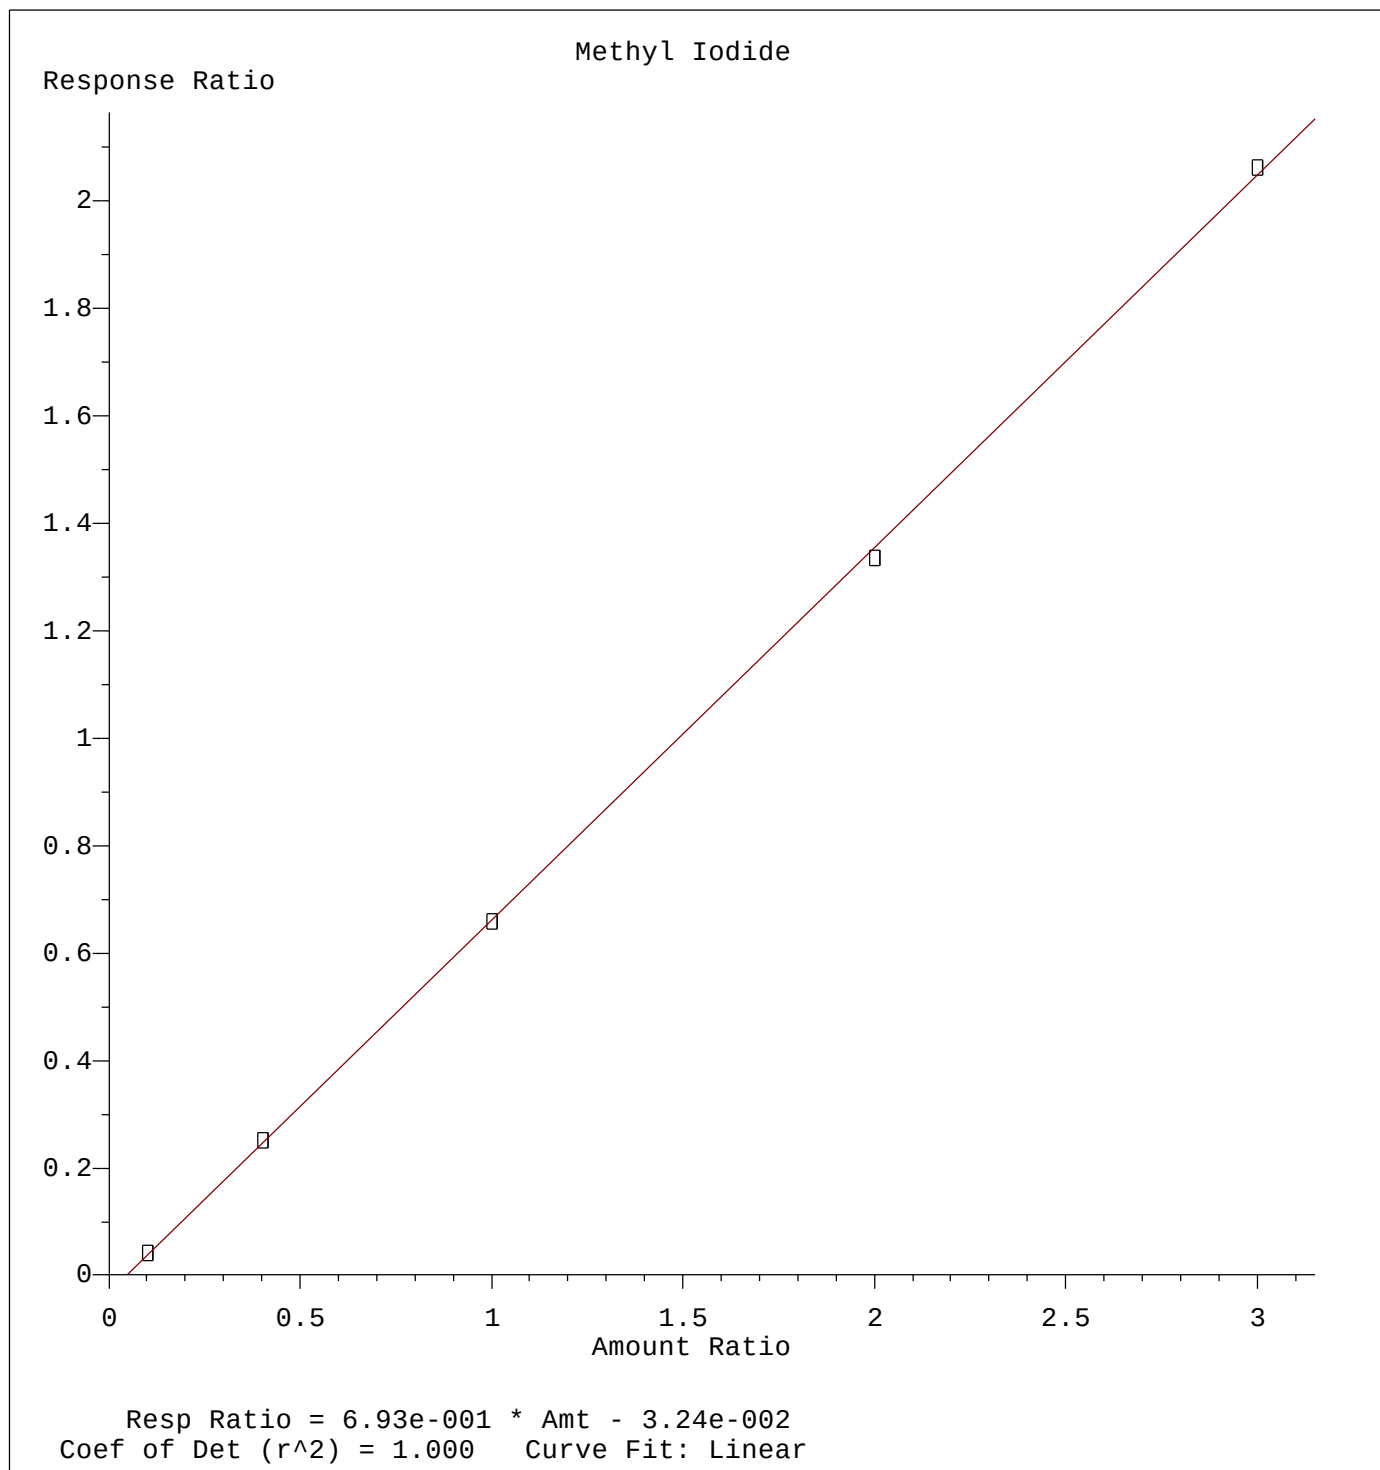

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N100418W.M
Calibration Table Last Updated: Mon Oct 08 13:43:30 2018

Trichlorofluoromethane

Response Ratio

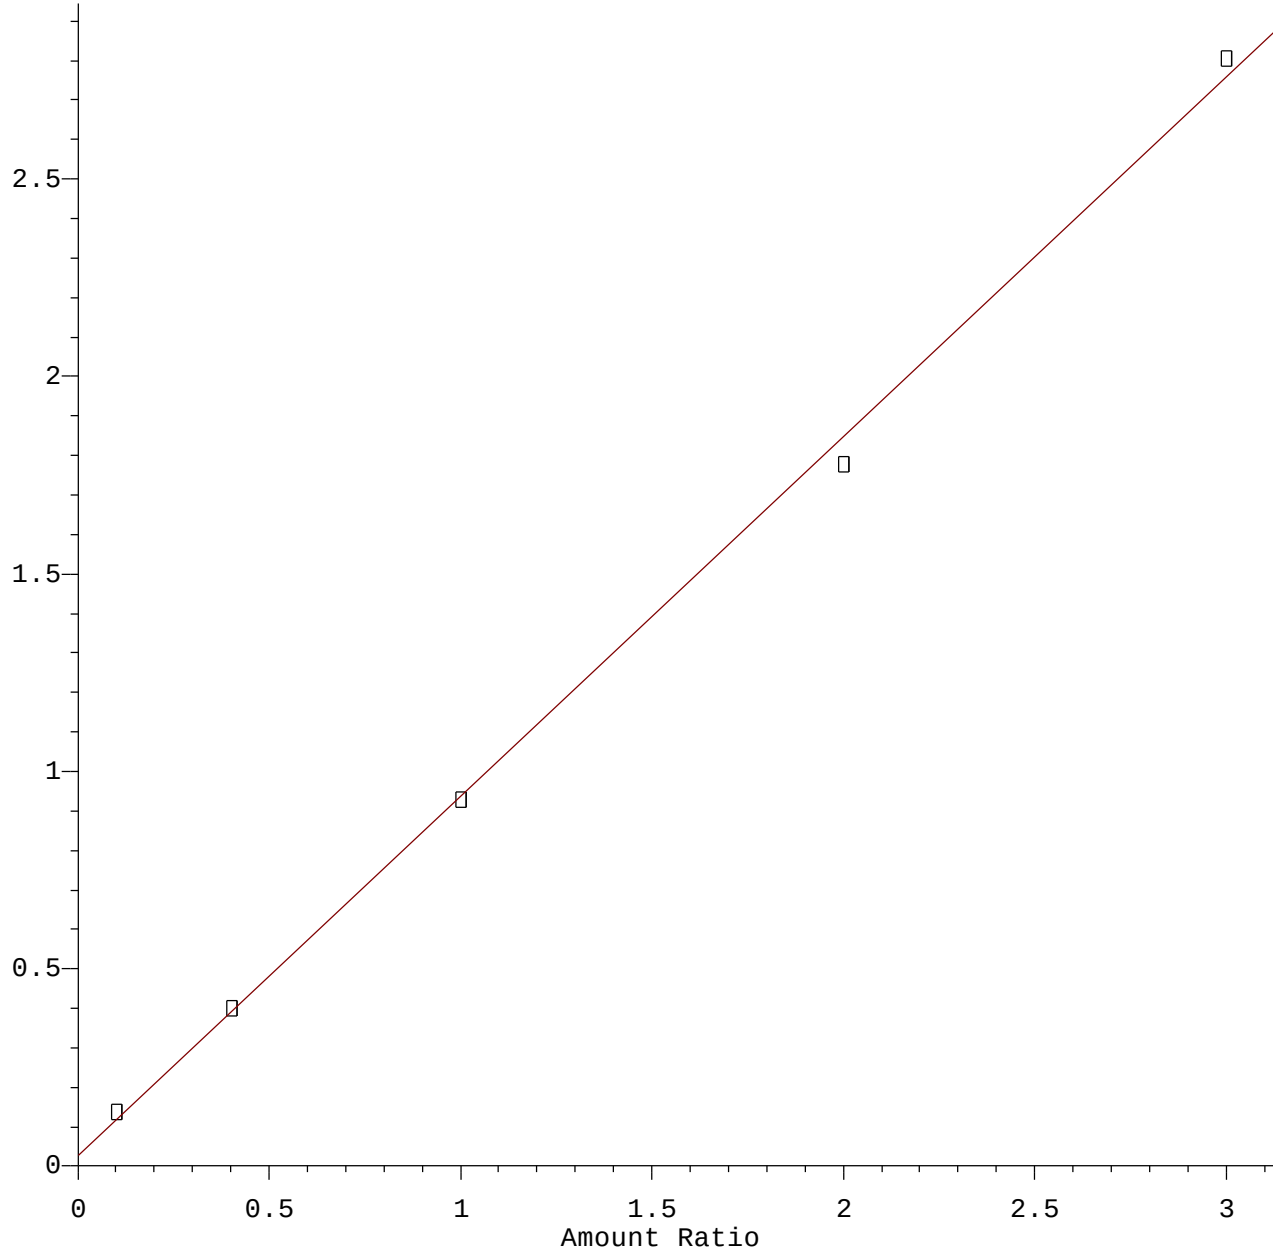

Resp Ratio = $9.10 \times 10^{-1} \times \text{Amt} + 2.53 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N100418W.M
Calibration Table Last Updated: Mon Oct 08 13:43:30 2018